

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052223\
 Data File : PS023076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2023 21:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 21:47:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.483	6.857	782.2E6	300.9E6	514.238	536.182
Target Compounds							
1) T	Dalapon	2.588	0.000	924718	0	<MDL	N.D. #
3) T	4-Nitroph...	6.317	0.000	6201295	0	5.890	N.D. #
5) T	DICAMBA	6.695f	7.026	690247	517435	<MDL	<MDL #
6) T	MCP	6.754	0.000	676230	0	<MDL	N.D. #
8) T	DICHLORPROP	7.266	7.664	1454113	6973487	<MDL	11.268 #
9) T	2,4-D	7.406	7.879f	9727633	1240031	4.203	1.733 #
10) T	Pentachlo...	7.679	0.000	1112807	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.216	0.000	3178622	0	<MDL	N.D. #
12) T	2,4,5-T	8.480	9.145f	3527152	1403528	<MDL	<MDL #
13) T	2,4-DB	8.979	0.000	14575538	0	6.213	N.D. #
14) T	DINOSEB	10.066	0.000	812516	0	<MDL	N.D. #
15) T	Picloram	9.892	10.901	24120365	3282217	1.407	<MDL #
16) T	DCPA	10.336	10.901	2428687	3282217	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052223\
Data File : PS023076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2023 21:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 21:47:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

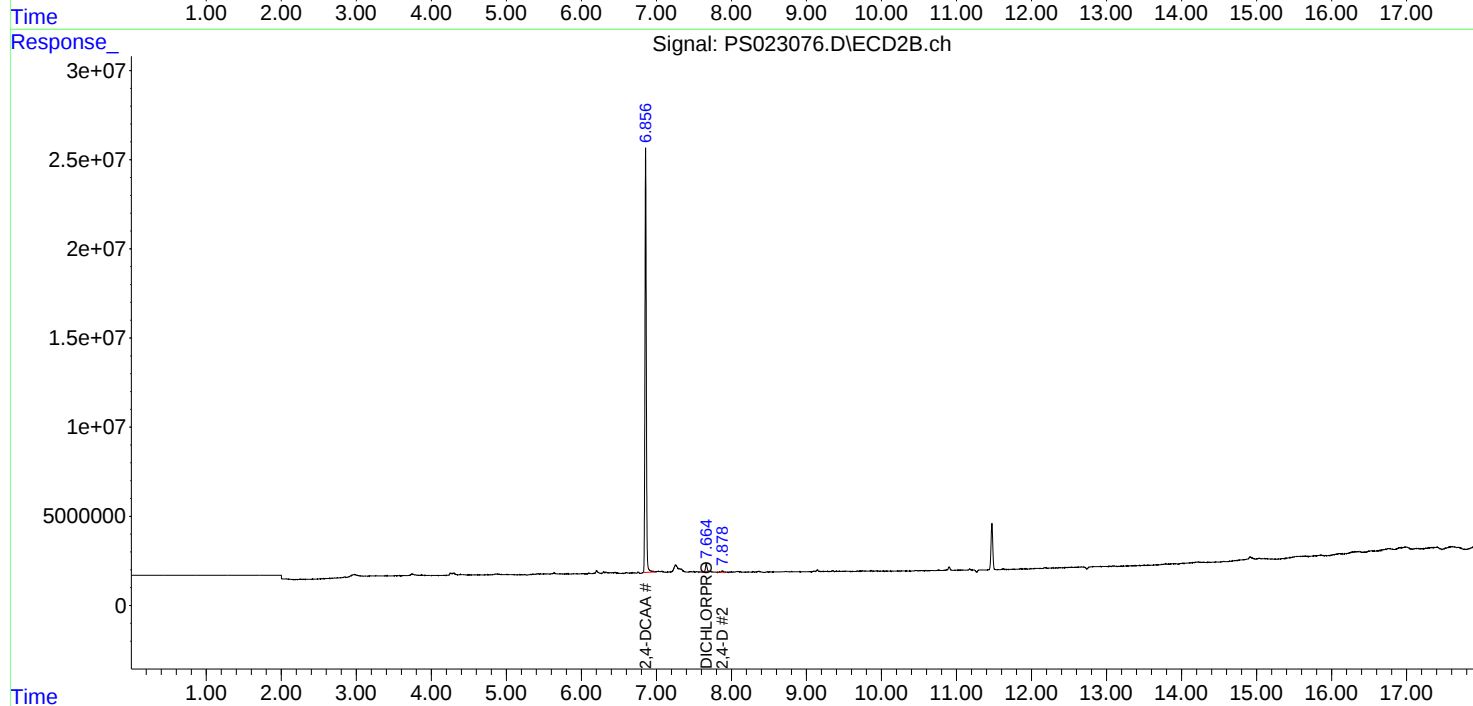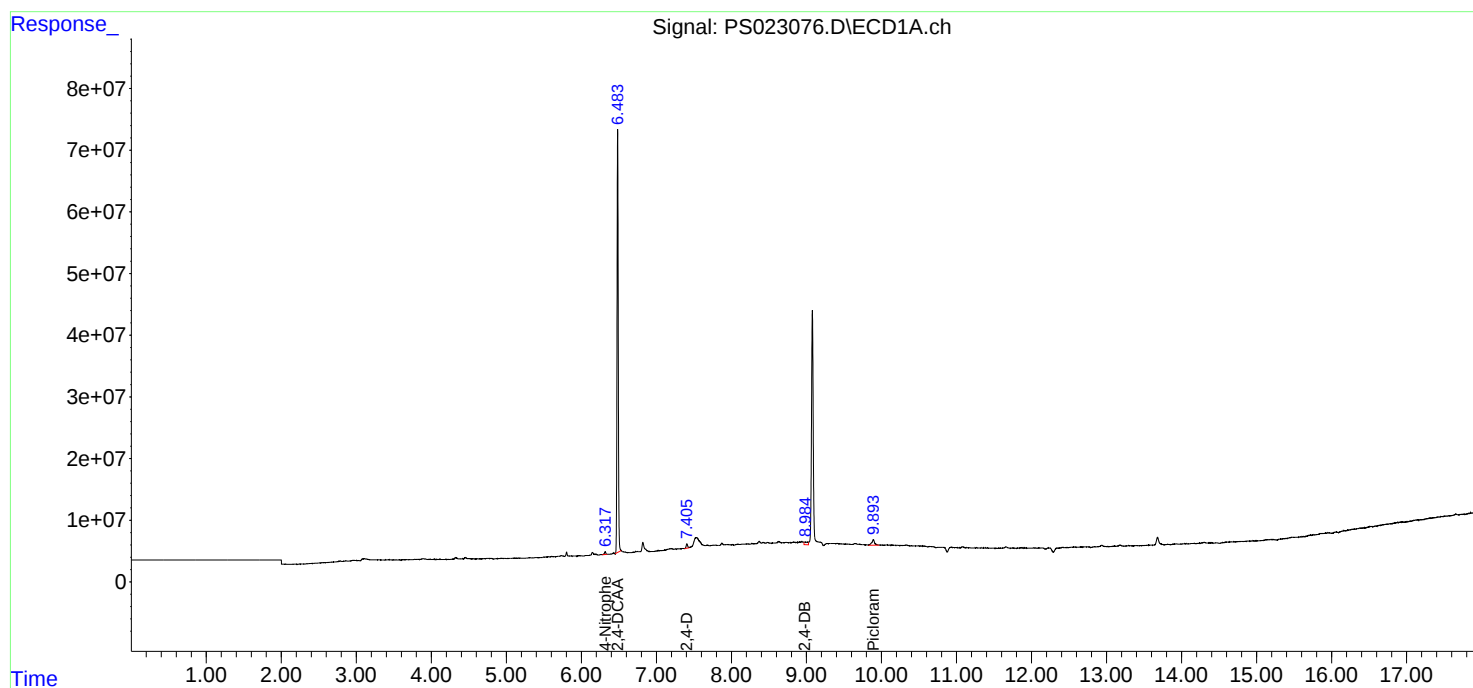


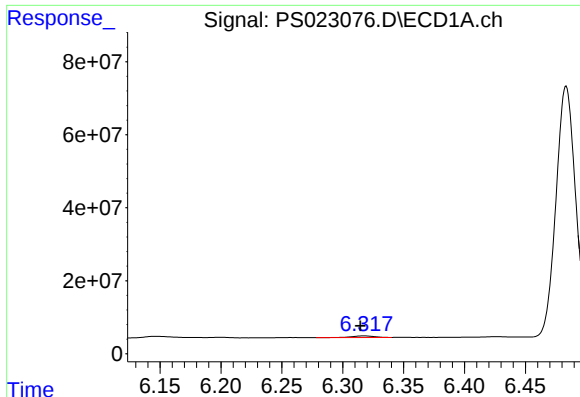

#3 4-Nitrophenol


R.T.: 6.317 min
Delta R.T.: 0.003 min
Response: 6201295
Conc: 5.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

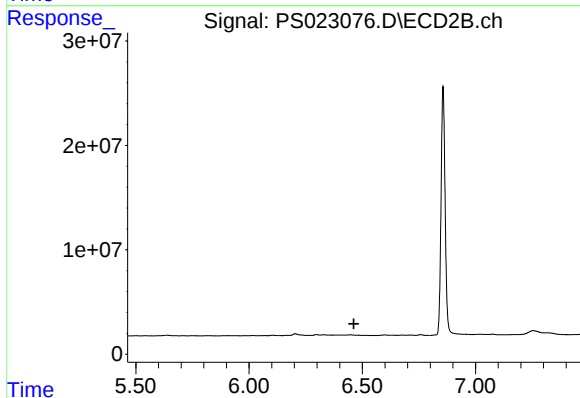


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

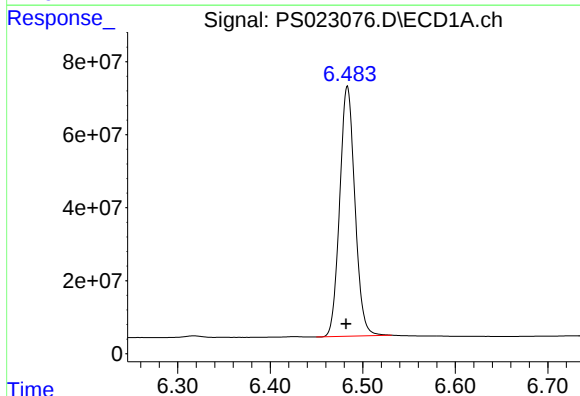


#4 2,4-DCAA

R.T.: 6.483 min
Delta R.T.: 0.001 min
Response: 782153744
Conc: 514.24 ng/ml

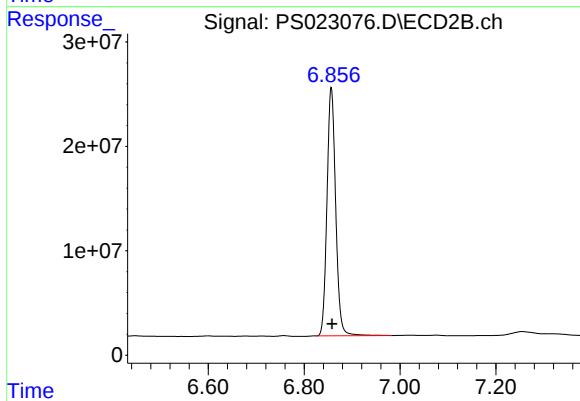

#4 2,4-DCAA


R.T.: 6.857 min
Delta R.T.: -0.001 min
Response: 300859786
Conc: 536.18 ng/ml

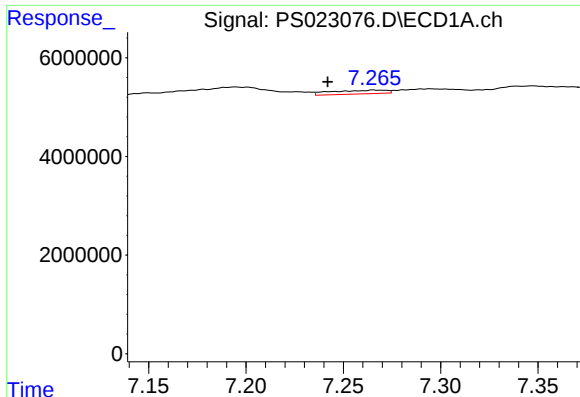

#8 DICHLORPROP


R.T.: 7.266 min
Delta R.T.: 0.024 min
Response: 1454113
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

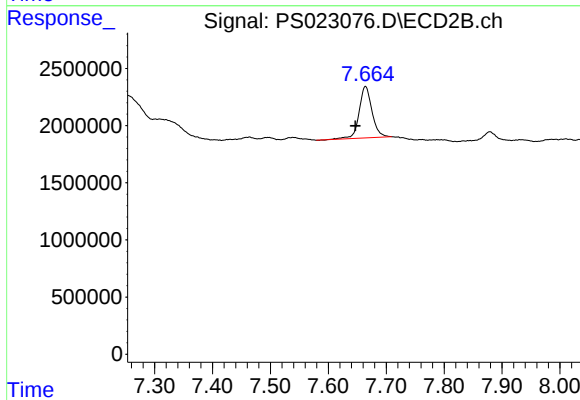


#8 DICHLORPROP

R.T.: 7.664 min
Delta R.T.: 0.017 min
Response: 6973487
Conc: 11.27 ng/ml

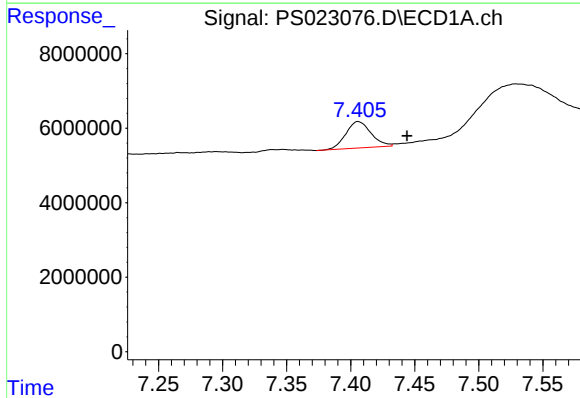


#9 2,4-D

R.T.: 7.406 min
Delta R.T.: -0.038 min
Response: 9727633
Conc: 4.20 ng/ml

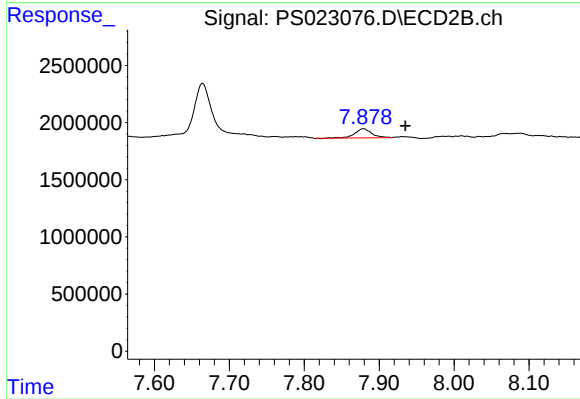

#9 2,4-D


R.T.: 7.879 min
Delta R.T.: -0.056 min
Response: 1240031
Conc: 1.73 ng/ml

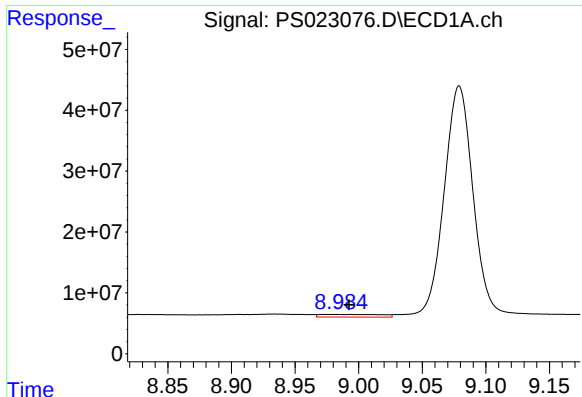

#13 2,4-DB


R.T.: 8.979 min
Delta R.T.: -0.014 min
Response: 14575538
Conc: 6.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

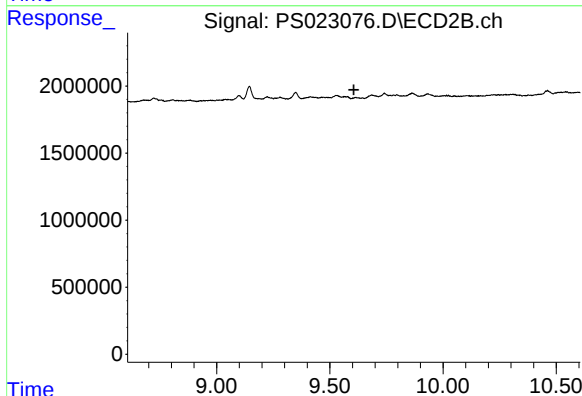


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

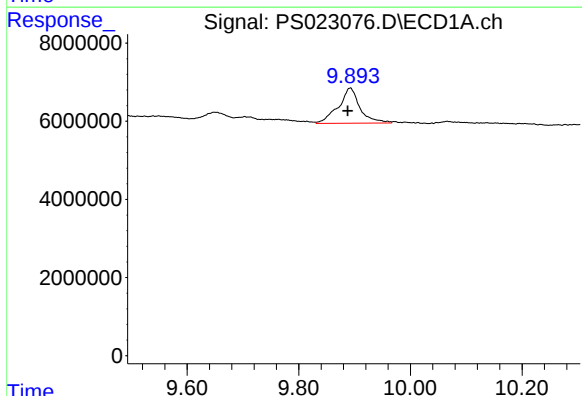

#15 Picloram

R.T.: 9.892 min
Delta R.T.: 0.004 min
Response: 24120365
Conc: 1.41 ng/ml

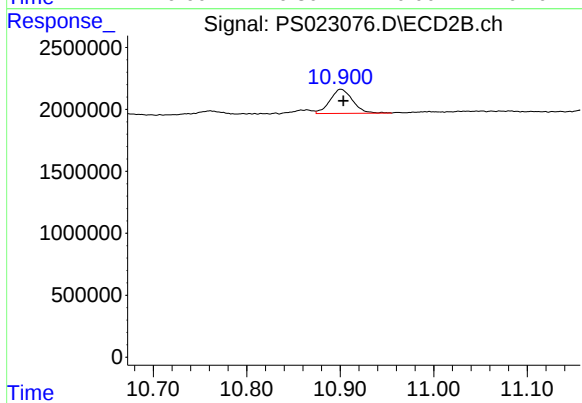

#15 Picloram

R.T.: 10.901 min
Delta R.T.: -0.003 min
Response: 3282217
Conc: N.D.