

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052322\
 Data File : PS019497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2022 01:37
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 03:12:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.238	0.000	1266433	0	<MDL	N.D.	#
Target Compounds								
2) T	3,5-DICHL...	6.465	0.000	555451	0	<MDL	N.D.	#
3) T	4-Nitroph...	7.012	6.404	4421643	240836	4.563	<MDL	#
5) T	DICAMBA	7.434	7.024f	1088842	493666	<MDL	<MDL	#
6) T	MCP	7.587	7.057	588906	103962	<MDL	<MDL	#
7) T	MCPA	7.733	0.000	1158754	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.138	7.647f	272153	1705750	<MDL	1.990	#
9) T	2,4-D	8.354	7.936f	70917	1745043	<MDL	1.747	#
10) T	Pentachlo...	8.680	8.309	6262624	688874	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.212	8.674	1897330	495284	<MDL	<MDL	#
12) T	2,4,5-T	9.459	9.081	28252786	3271725	1.336	<MDL	#
13) T	2,4-DB	10.011	9.579	582594	886726	<MDL	1.560	#
14) T	DINOSEB	11.187	9.880	27388290	1157548	1.659	<MDL	#
15) T	Picloram	10.996	10.807f	585.2E6	8343859	20.020	1.395	#
16) T	DCPA	11.461	10.807	3925756	8343859	<MDL	1.421	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052322\
Data File : PS019497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2022 01:37
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 03:12:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

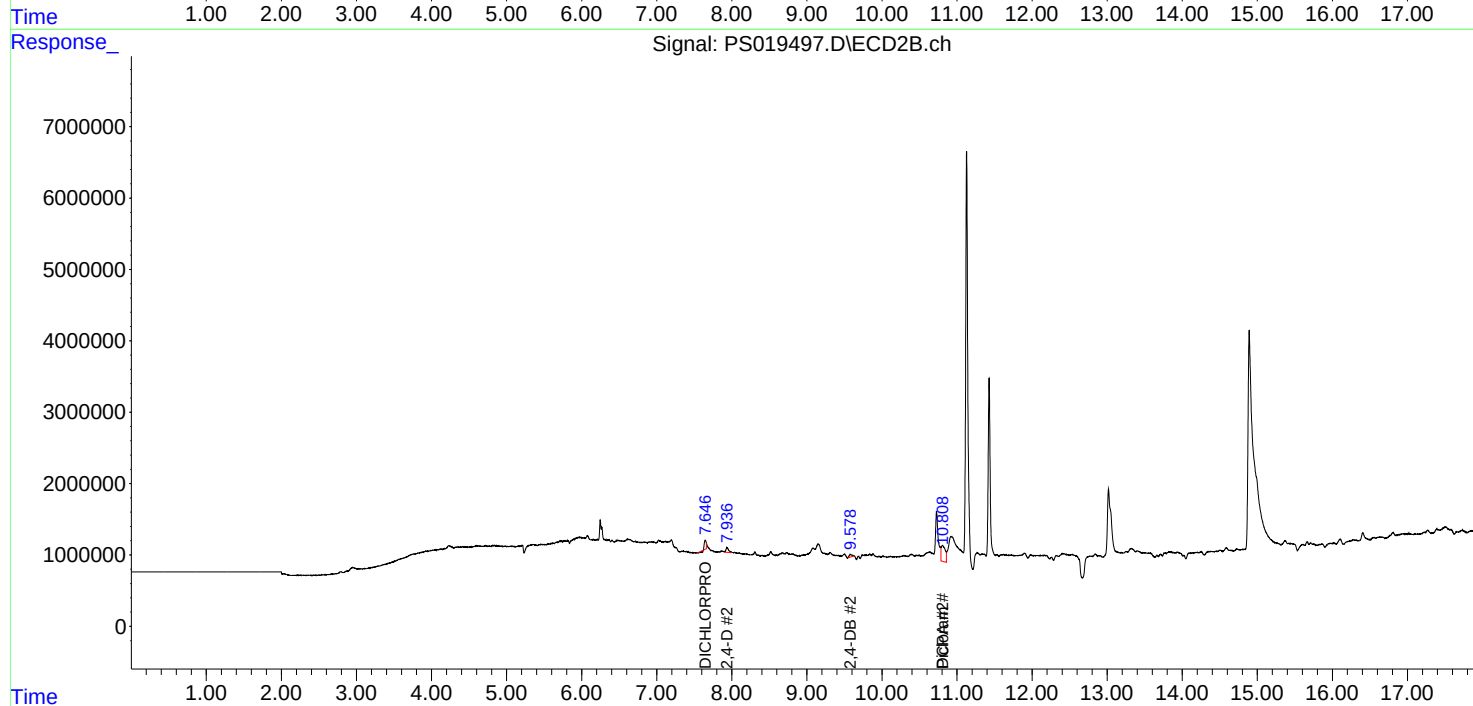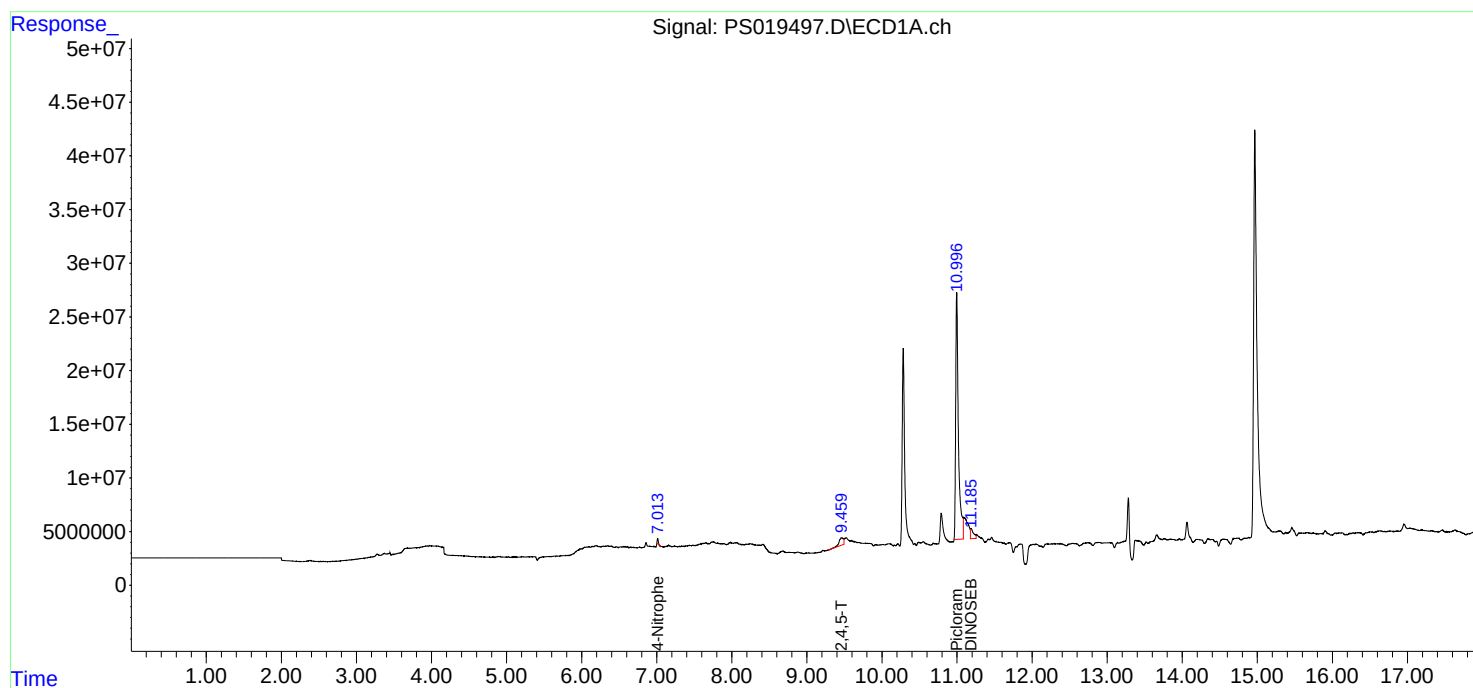


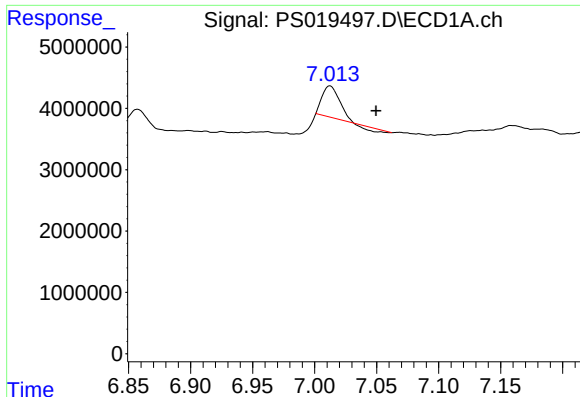

#3 4-Nitrophenol


R.T.: 7.012 min
Delta R.T.: -0.037 min
Response: 4421643
Conc: 4.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

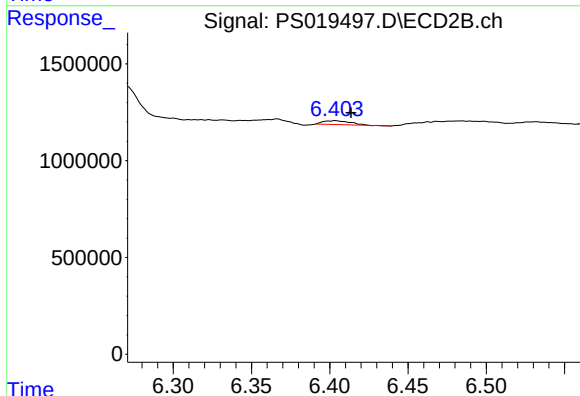


#3 4-Nitrophenol

R.T.: 6.404 min
Delta R.T.: -0.010 min
Response: 240836
Conc: N.D.

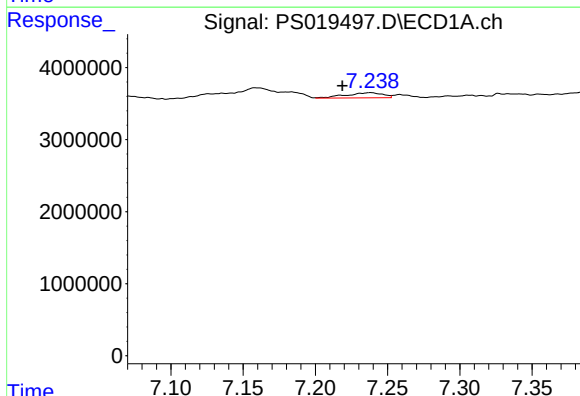


#4 2,4-DCAA

R.T.: 7.238 min
Delta R.T.: 0.019 min
Response: 1266433
Conc: N.D.

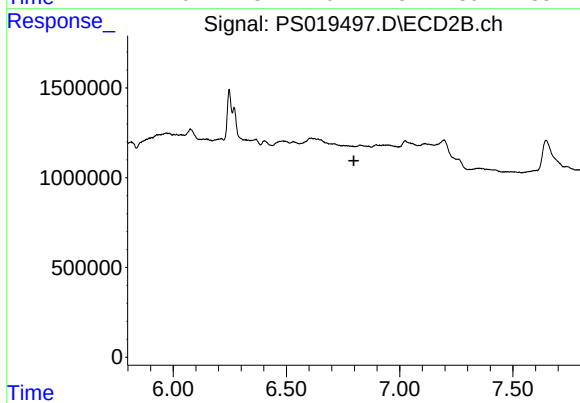

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.798 min
Response: 0
Conc: N.D.

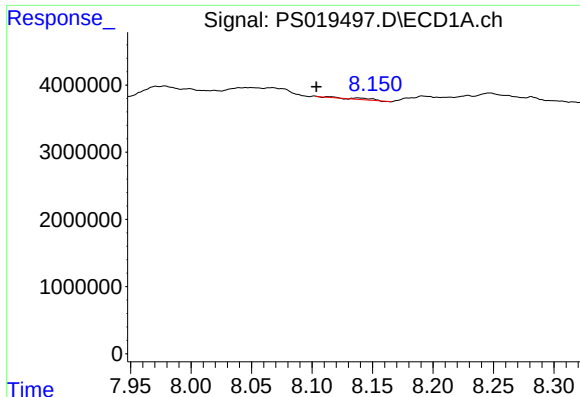

#8 DICHLORPROP


R.T.: 8.138 min
Delta R.T.: 0.034 min
Response: 272153
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

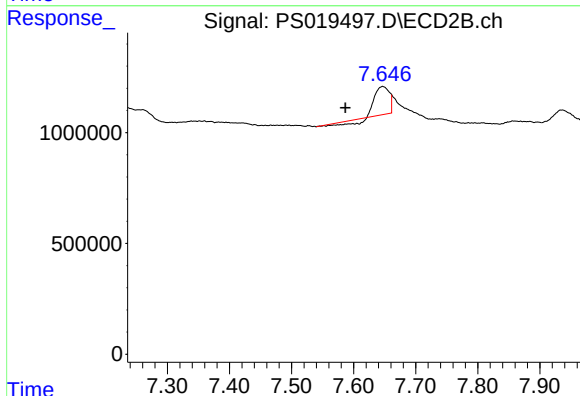


#8 DICHLORPROP

R.T.: 7.647 min
Delta R.T.: 0.060 min
Response: 1705750
Conc: 1.99 ng/ml

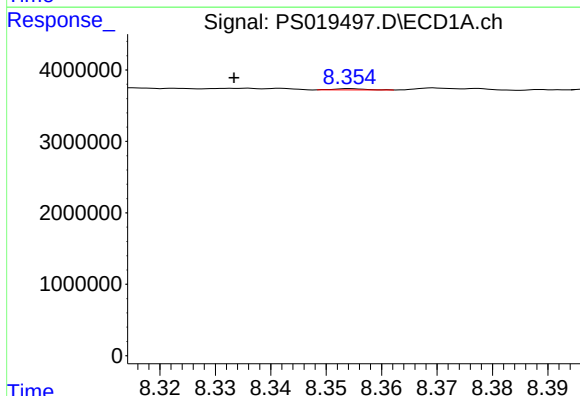


#9 2,4-D

R.T.: 8.354 min
Delta R.T.: 0.021 min
Response: 70917
Conc: N.D.

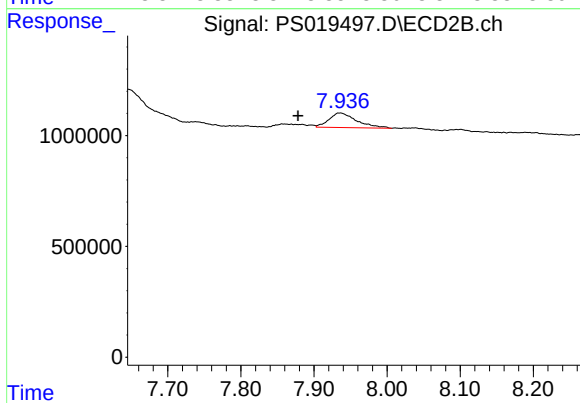

#9 2,4-D


R.T.: 7.936 min
Delta R.T.: 0.058 min
Response: 1745043
Conc: 1.75 ng/ml

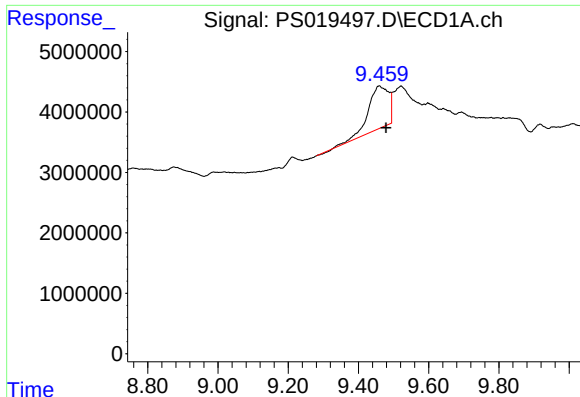

#12 2,4,5-T


R.T.: 9.459 min
Delta R.T.: -0.019 min
Response: 28252786
Conc: 1.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

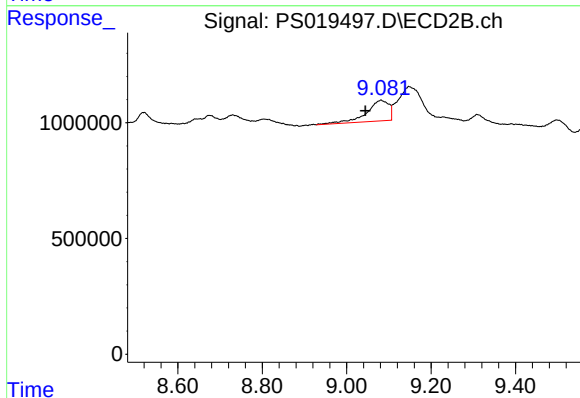


#12 2,4,5-T

R.T.: 9.081 min
Delta R.T.: 0.037 min
Response: 3271725
Conc: N.D.

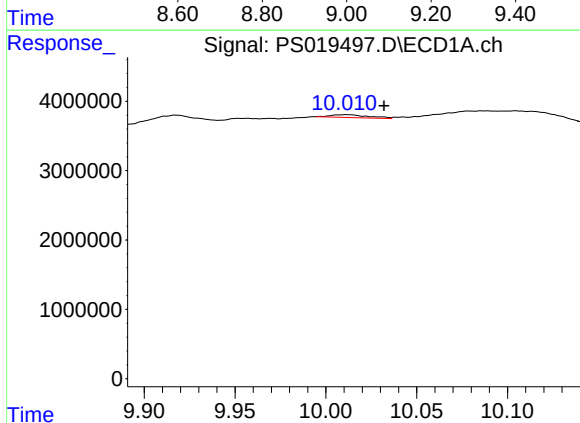


#13 2,4-DB

R.T.: 10.011 min
Delta R.T.: -0.021 min
Response: 582594
Conc: N.D.

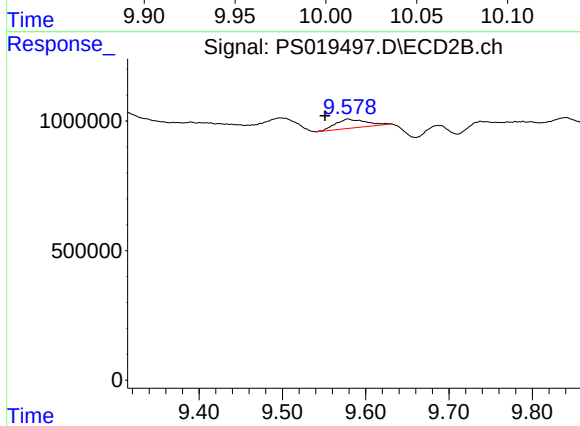

#13 2,4-DB


R.T.: 9.579 min
Delta R.T.: 0.027 min
Response: 886726
Conc: 1.56 ng/ml

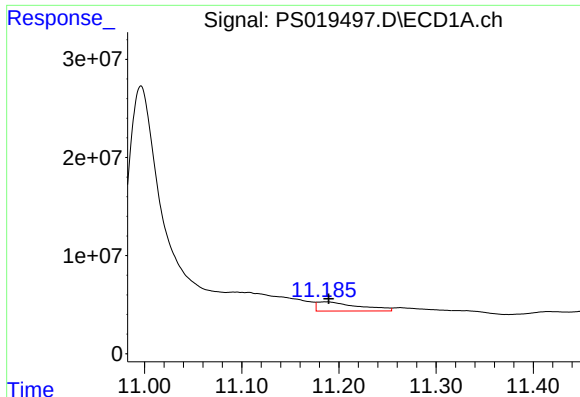

#14 DINOSEB


R.T.: 11.187 min
Delta R.T.: -0.003 min
Response: 27388290
Conc: 1.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

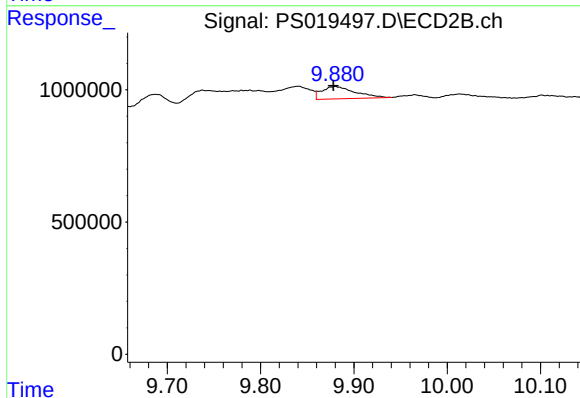


#14 DINOSEB

R.T.: 9.880 min
Delta R.T.: 0.002 min
Response: 1157548
Conc: N.D.

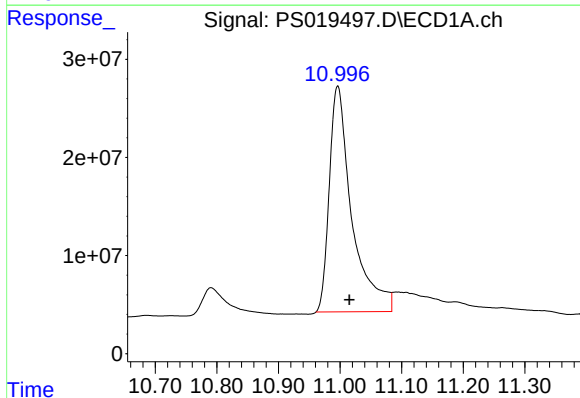


#15 Picloram

R.T.: 10.996 min
Delta R.T.: -0.019 min
Response: 585173637
Conc: 20.02 ng/ml

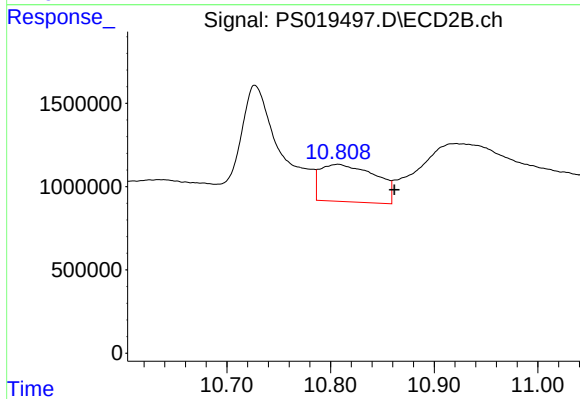

#15 Picloram


R.T.: 10.807 min
Delta R.T.: -0.054 min
Response: 8343859
Conc: 1.40 ng/ml

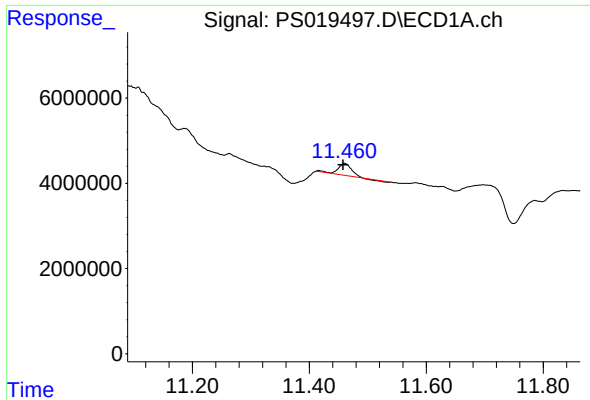

#16 DCPA

R.T.: 11.461 min
Delta R.T.: 0.003 min
Response: 3925756
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

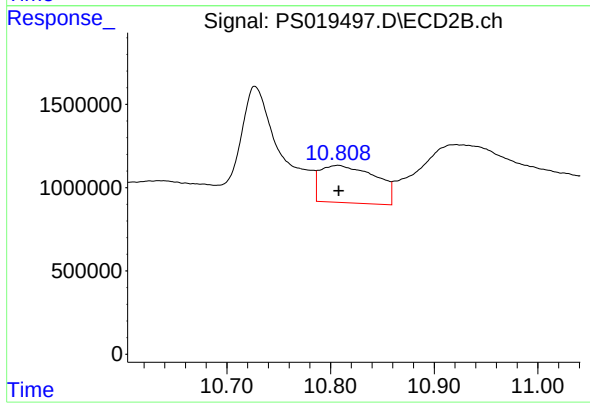

#16 DCPA

R.T.: 10.807 min
Delta R.T.: 0.000 min
Response: 8343859
Conc: 1.42 ng/ml