

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052323\
 Data File : PS023097.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 May 2023 16:06
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 23 21:17:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.486	6.859	793.6E6	301.8E6	521.746	537.923
Target Compounds							
1) T	Dalapon	2.582	0.000	1505250	0	<MDL	N.D. #
3) T	4-Nitroph...	6.321	0.000	3986348	0	3.787	N.D. #
7) T	MCPA	0.000	7.310	0	5317499	N.D.	2.008
8) T	DICHLORPROP	7.249	7.667	509639	3288048	<MDL	5.313 #
9) T	2,4-D	7.409	0.000	10696525	0	4.622	N.D. #
10) T	Pentachlo...	7.683	0.000	1150773	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.220	0.000	9276054	0	<MDL	N.D. #
12) T	2,4,5-T	8.486	9.148f	4023235	1464242	<MDL	<MDL #
13) T	2,4-DB	8.991	0.000	7691390	0	3.278	N.D. #
14) T	DINOSEB	10.070	0.000	509060	0	<MDL	N.D. #
15) T	Picloram	9.900	10.907	24270780	2650567	1.415	<MDL #
16) T	DCPA	10.339	10.907f	2544320	2650567	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052323\
Data File : PS023097.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 May 2023 16:06
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 23 21:17:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

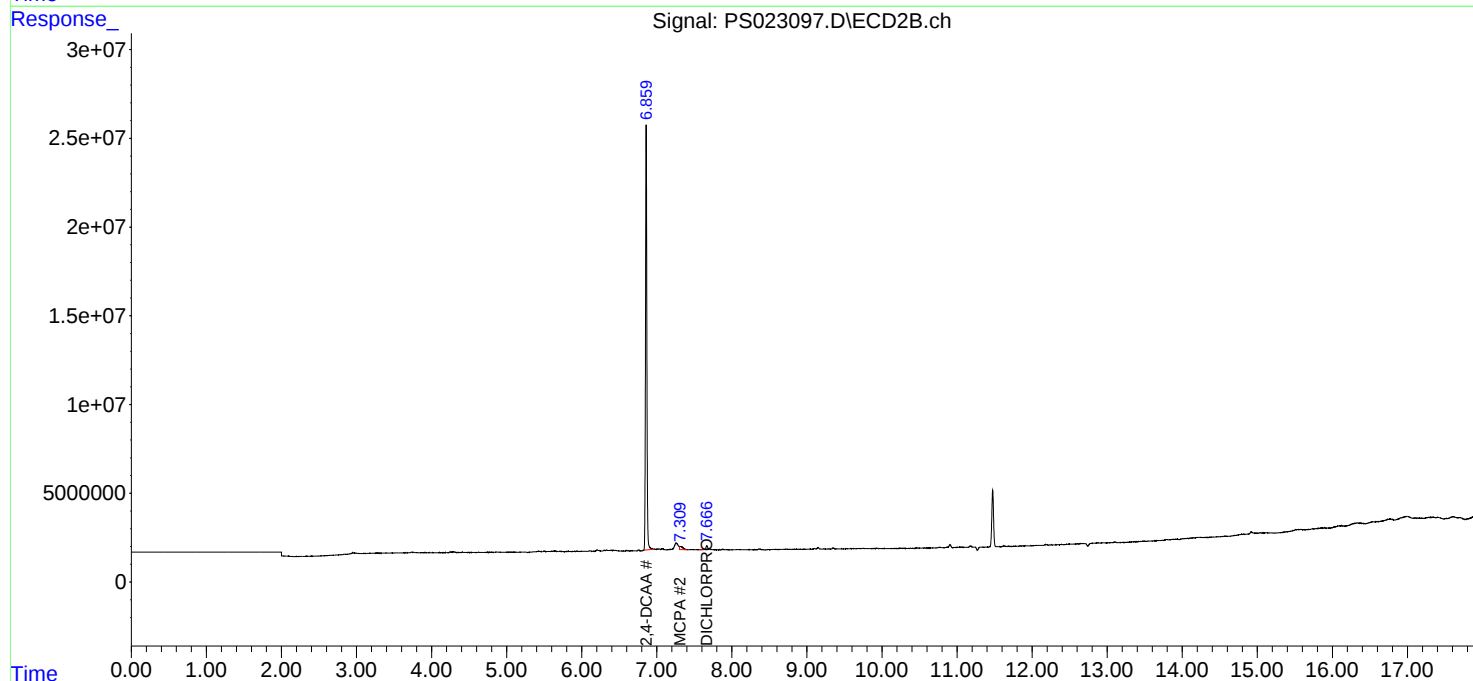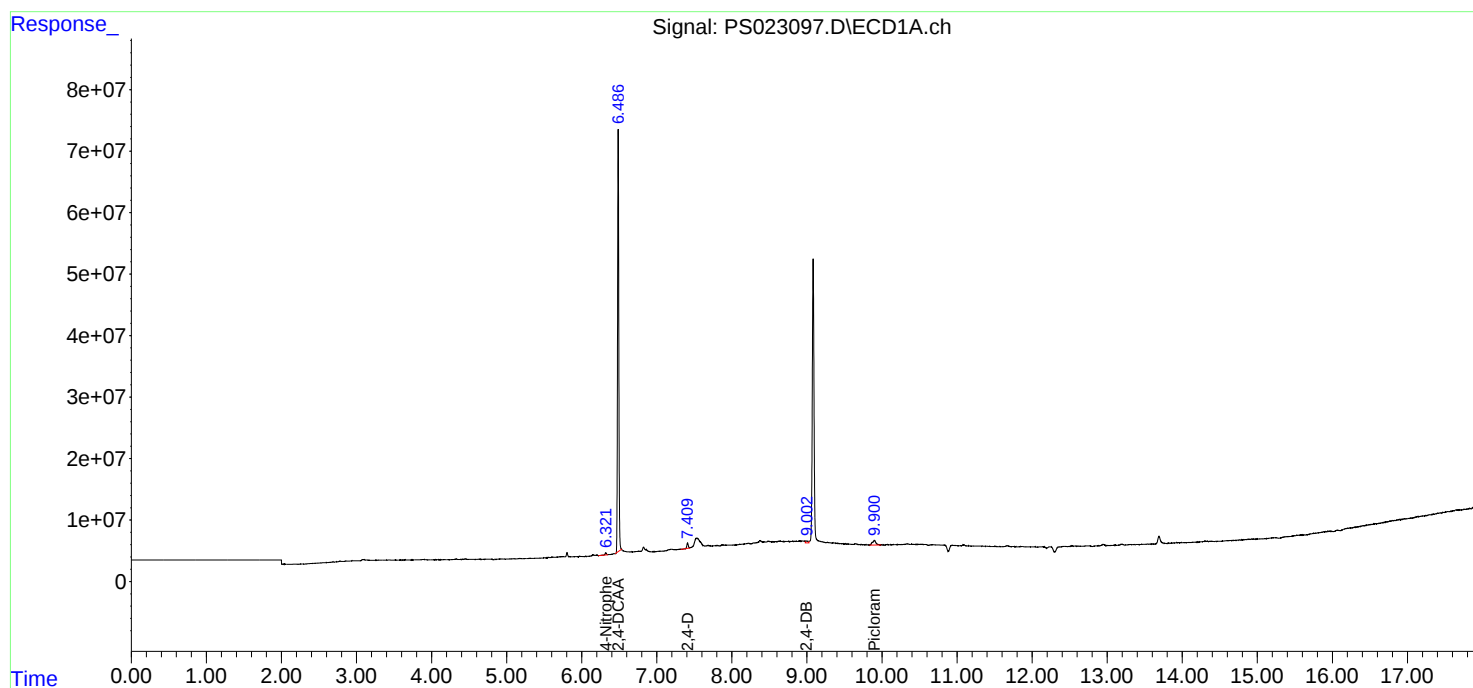


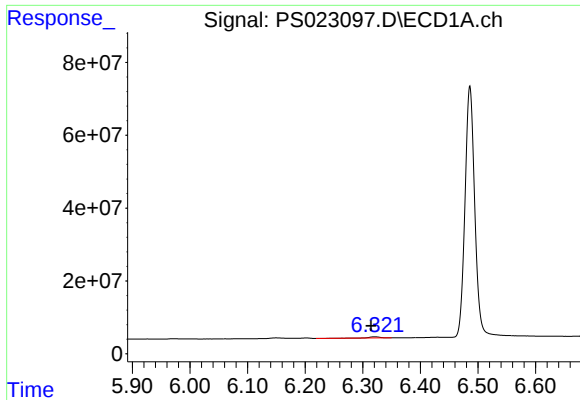

#3 4-Nitrophenol


R.T.: 6.321 min
Delta R.T.: 0.006 min
Response: 3986348
Conc: 3.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

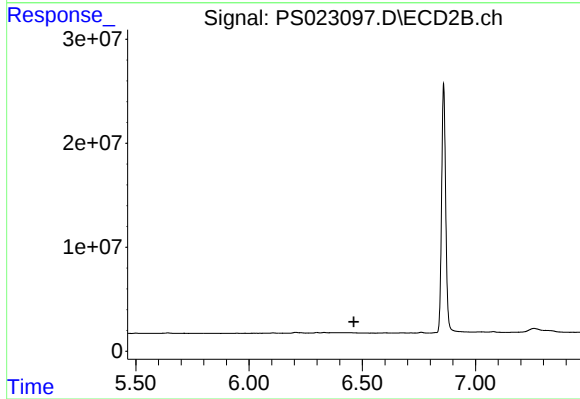


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

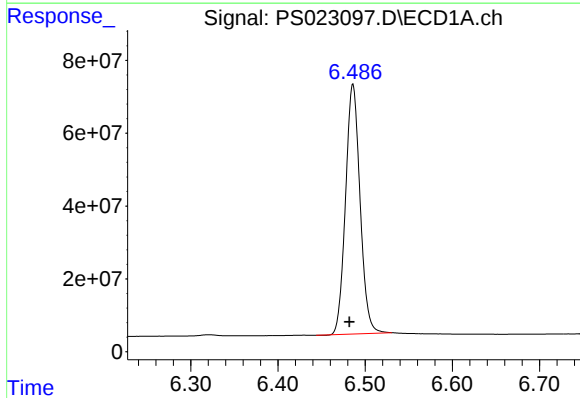


#4 2,4-DCAA

R.T.: 6.486 min
Delta R.T.: 0.004 min
Response: 793572680
Conc: 521.75 ng/ml

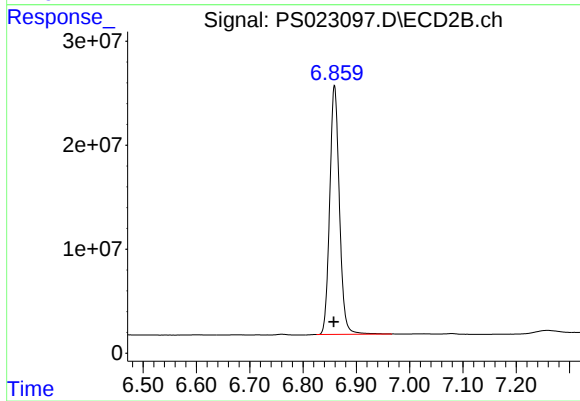

#4 2,4-DCAA


R.T.: 6.859 min
Delta R.T.: 0.001 min
Response: 301836877
Conc: 537.92 ng/ml

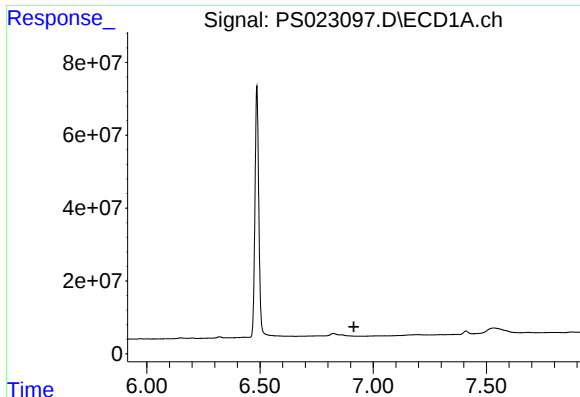

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.915 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

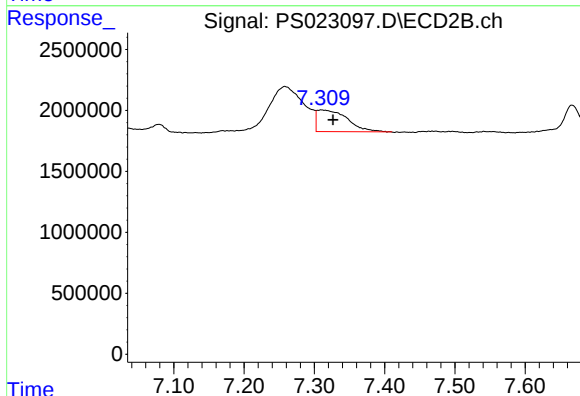


#7 MCPA

R.T.: 7.310 min
Delta R.T.: -0.017 min
Response: 5317499
Conc: 2.01 ug/ml

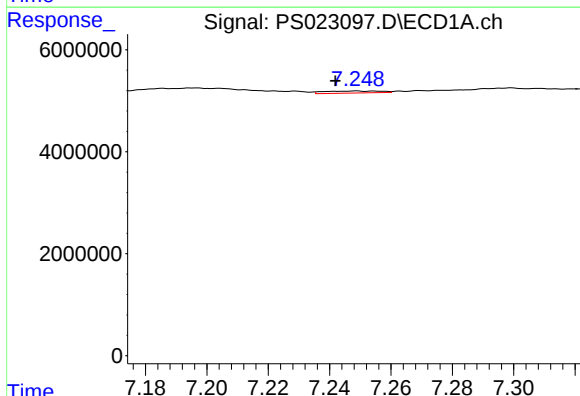


#8 DICHLORPROP

R.T.: 7.249 min
Delta R.T.: 0.007 min
Response: 509639
Conc: N.D.

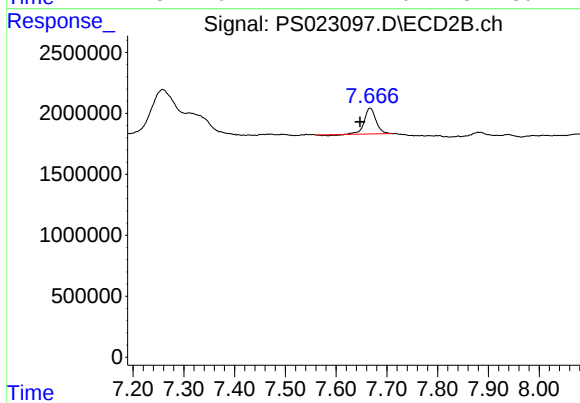

#8 DICHLORPROP


R.T.: 7.667 min
Delta R.T.: 0.020 min
Response: 3288048
Conc: 5.31 ng/ml

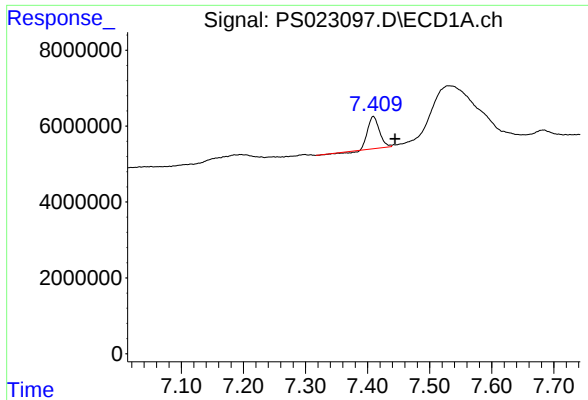

#9 2,4-D


R.T.: 7.409 min
Delta R.T.: -0.035 min
Response: 10696525
Conc: 4.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

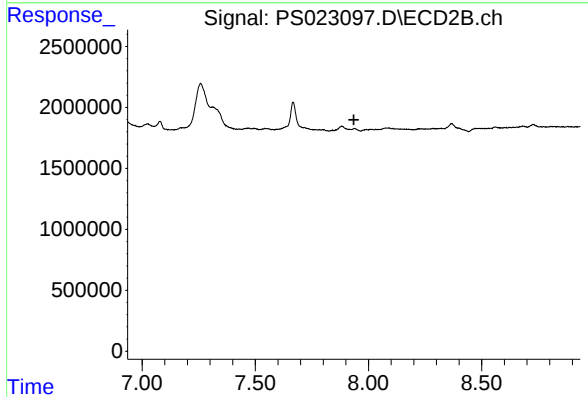


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.935 min
Response: 0
Conc: N.D.

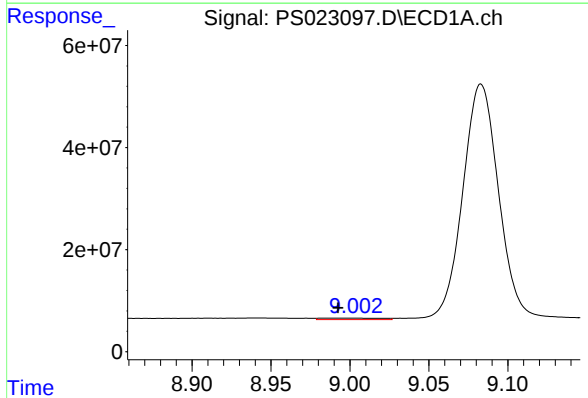


#13 2,4-DB

R.T.: 8.991 min
Delta R.T.: -0.001 min
Response: 7691390
Conc: 3.28 ng/ml

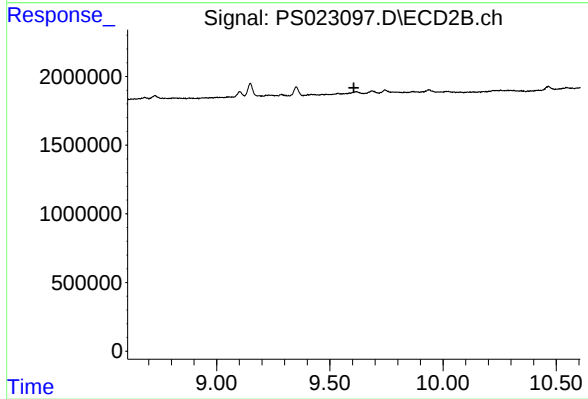

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

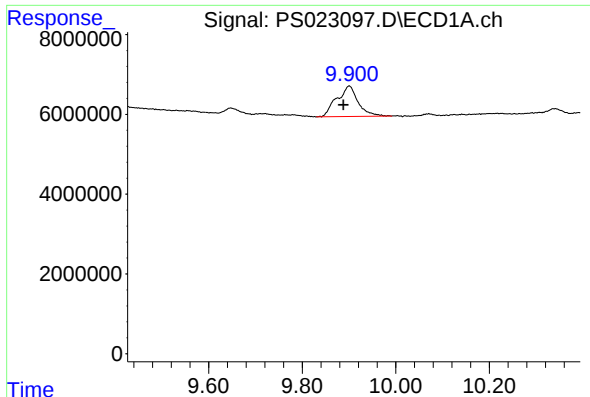

#15 Picloram

R.T.: 9.900 min
Delta R.T.: 0.013 min
Response: 24270780
Conc: 1.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

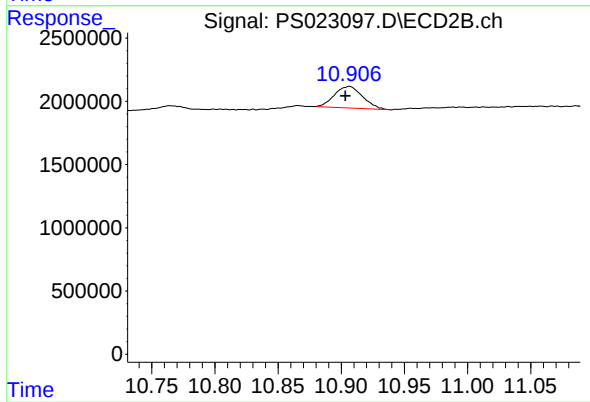

#15 Picloram

R.T.: 10.907 min
Delta R.T.: 0.003 min
Response: 2650567
Conc: N.D.