

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052421\
 Data File : PS015062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2021 14:56
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 24 17:47:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5) T	DICAMBA	7.341	0.000	4921657	0	<MDL	N.D. #
6) T	MCPP	7.559f	0.000	686687	0	<MDL	N.D. #
7) T	MCPA	7.616	0.000	5891055	0	<MDL	N.D. #
10) T	Pentachlo...	8.562	8.392	9333687	3744350	<MDL	<MDL #
11) T	2,4,5-TP ...	9.108	0.000	7570764	0	<MDL	N.D. #
12) T	2,4,5-T	9.403	9.147	14444043	3935961	1.579	1.475
14) T	DINSEB	11.087	0.000	10496542	0	1.464	N.D. #
15) T	Picloram	10.932	10.968	134.1E6	51941677	11.042	13.035
16) T	DCPA	11.351	10.892	12524218	5101893	<MDL	1.197 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052421\
Data File : PS015062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2021 14:56
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 24 17:47:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

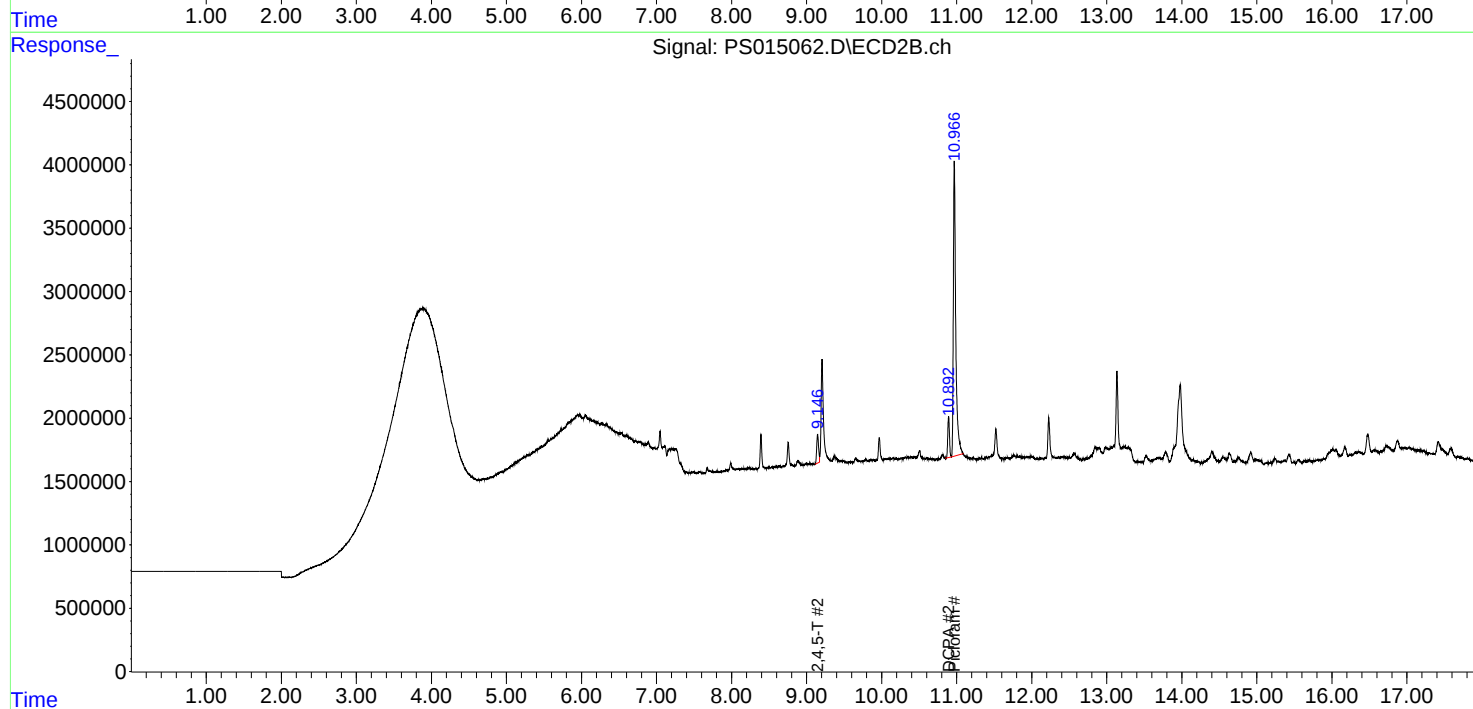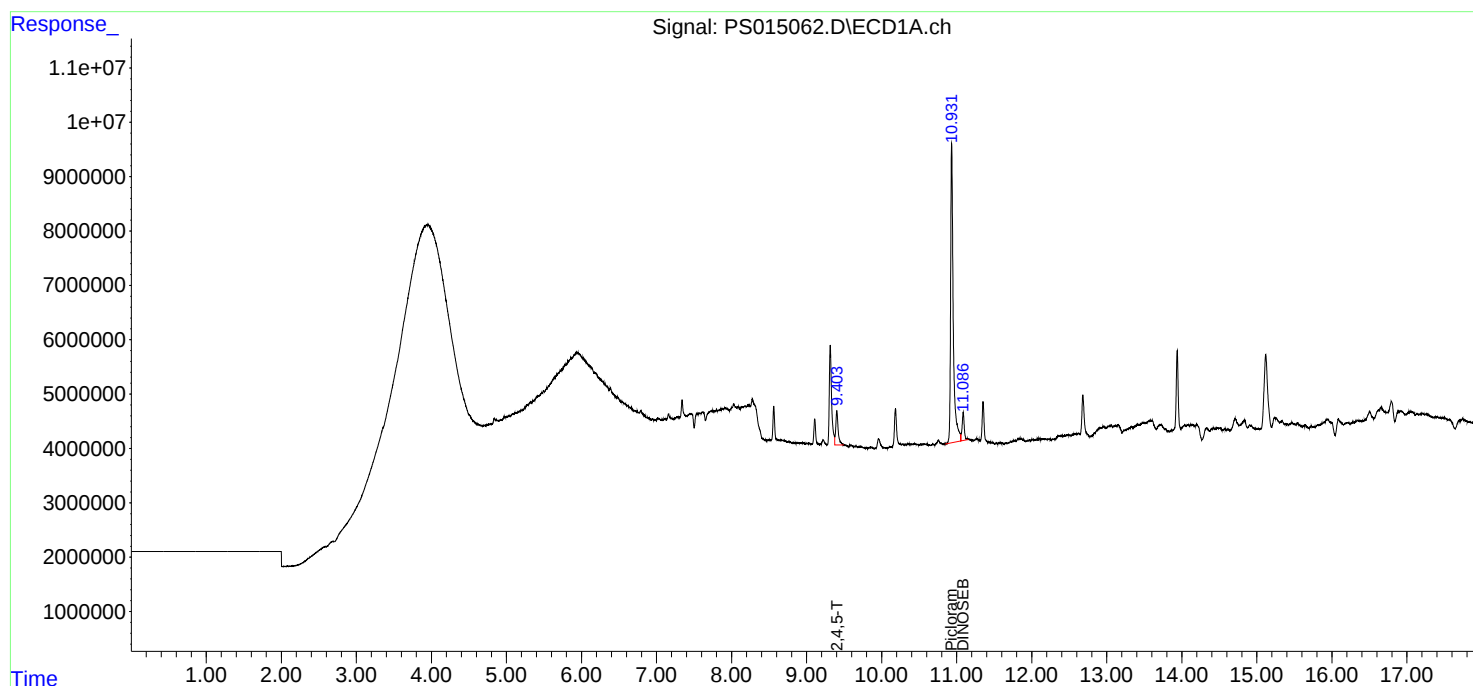


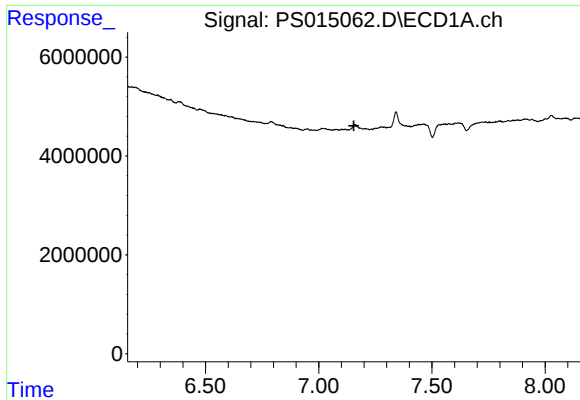

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.156 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

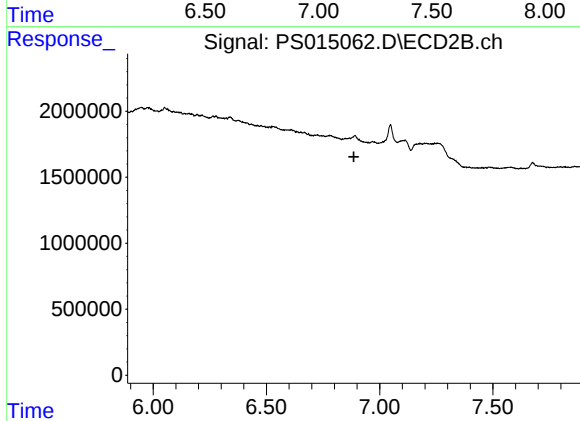


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

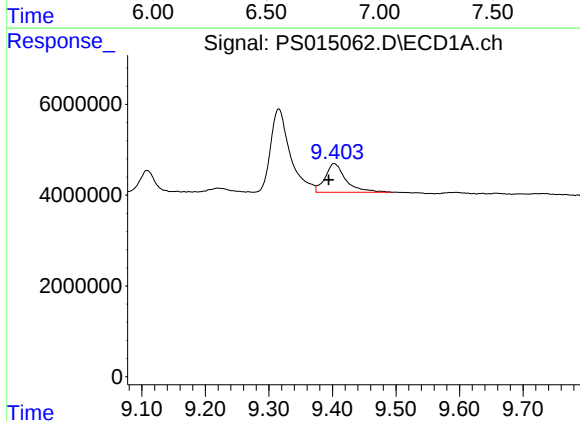


#12 2,4,5-T

R.T.: 9.403 min
Delta R.T.: 0.009 min
Response: 14444043
Conc: 1.58 ng/ml

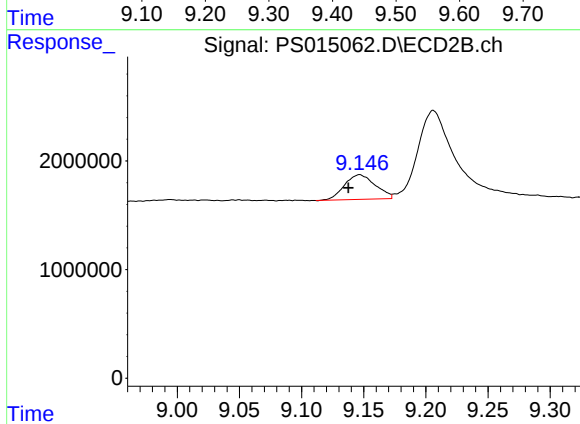

#12 2,4,5-T


R.T.: 9.147 min
Delta R.T.: 0.009 min
Response: 3935961
Conc: 1.47 ng/ml

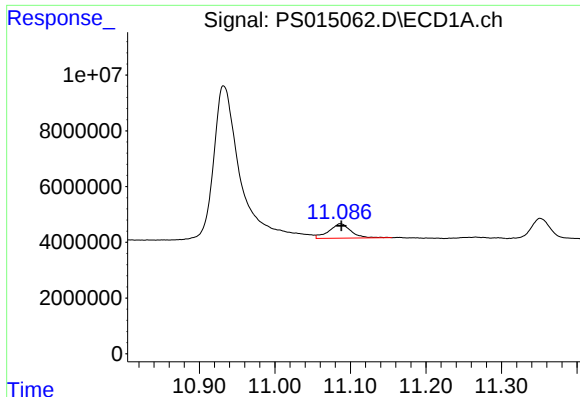

#14 DINoseb


R.T.: 11.087 min
Delta R.T.: -0.001 min
Response: 10496542
Conc: 1.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

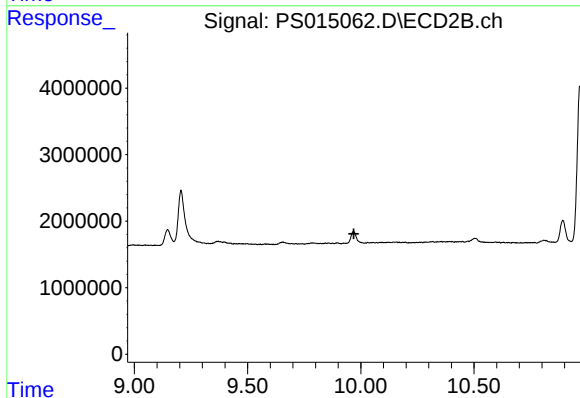


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.970 min
Response: 0
Conc: N.D.

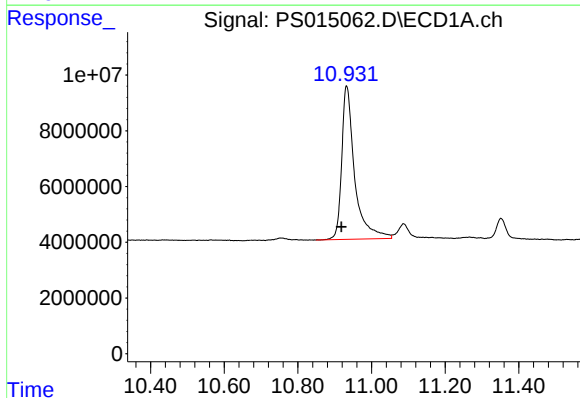


#15 Picloram

R.T.: 10.932 min
Delta R.T.: 0.013 min
Response: 134134688
Conc: 11.04 ng/ml

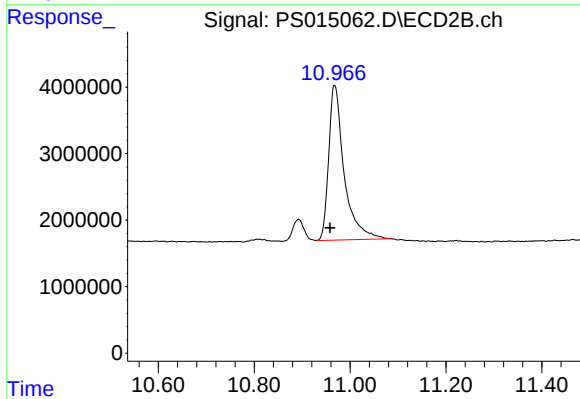

#15 Picloram


R.T.: 10.968 min
Delta R.T.: 0.009 min
Response: 51941677
Conc: 13.04 ng/ml

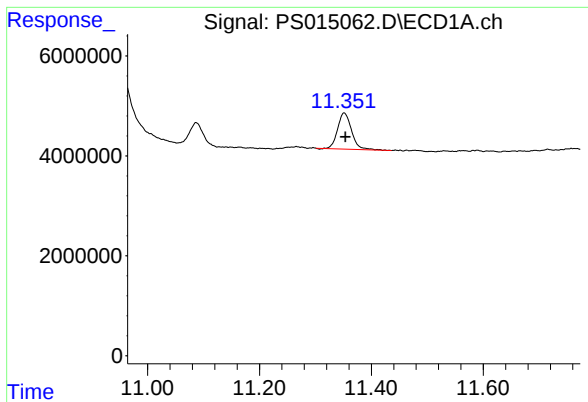

#16 DCPA

R.T.: 11.351 min
Delta R.T.: -0.002 min
Response: 12524218
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

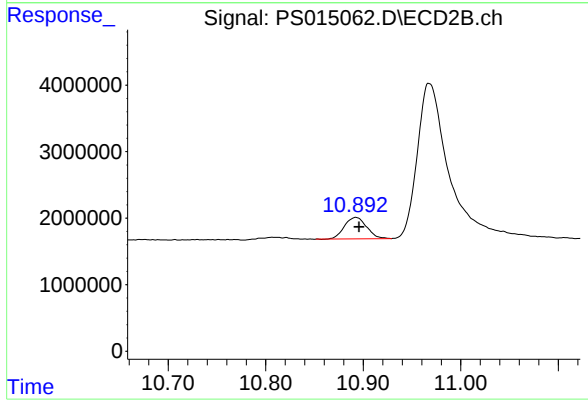

#16 DCPA

R.T.: 10.892 min
Delta R.T.: -0.003 min
Response: 5101893
Conc: 1.20 ng/ml