

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052422\
 Data File : PS019510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2022 21:57
 Operator : AJ\MA
 Sample : HSTDICC1500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 01:58:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 01:57:58 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.198	6.782	3524.8E6	1172.6E6	1489.276	1518.065
Target Compounds							
1) T	Dalapon	3.016	2.529	6791.4E6	1369.4E6	1363.765	1376.777
2) T	3,5-DICHL...	6.412	5.962	4194.1E6	1638.7E6	1366.280	1385.837
3) T	4-Nitroph...	7.027	6.398	1531.9E6	588.8E6	1429.898	1375.924
5) T	DICAMBA	7.388	6.947	12560.4E6	4638.0E6	1365.891	1383.334
6) T	MCPD	7.564	7.052	1124.8E6	397.1E6	144.427	143.989
7) T	MCPA	7.714	7.266	1548.2E6	547.1E6	141.055	141.449
8) T	DICHLORPROP	8.079	7.566	3451.5E6	1240.7E6	1388.440	1416.788
9) T	2,4-D	8.307	7.857	4074.6E6	1501.7E6	1409.889	1413.838
10) T	Pentachlo...	8.615	8.284	40143.6E6	14093.8E6	1285.987	1317.353
11) T	2,4,5-TP ...	9.164	8.644	20314.5E6	6710.6E6	1371.749	1381.052
12) T	2,4,5-T	9.449	9.021	23924.6E6	6409.2E6	1358.951	1390.503
13) T	2,4-DB	10.000	9.525	5912.2E6	913.3E6	1442.948	1454.815
14) T	DINOSEB	11.156	9.852	19849.8E6	4863.6E6	1360.253	1390.062
15) T	Picloram	10.977	10.830	39630.3E6	8862.6E6	1381.419	1398.609
16) T	DCPA	11.423	10.781	30271.8E6	8106.7E6	1362.404	1382.377



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052422\
Data File : PS019510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2022 21:57
Operator : AJ\MA
Sample : HSTDICC1500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 01:58:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 01:57:58 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

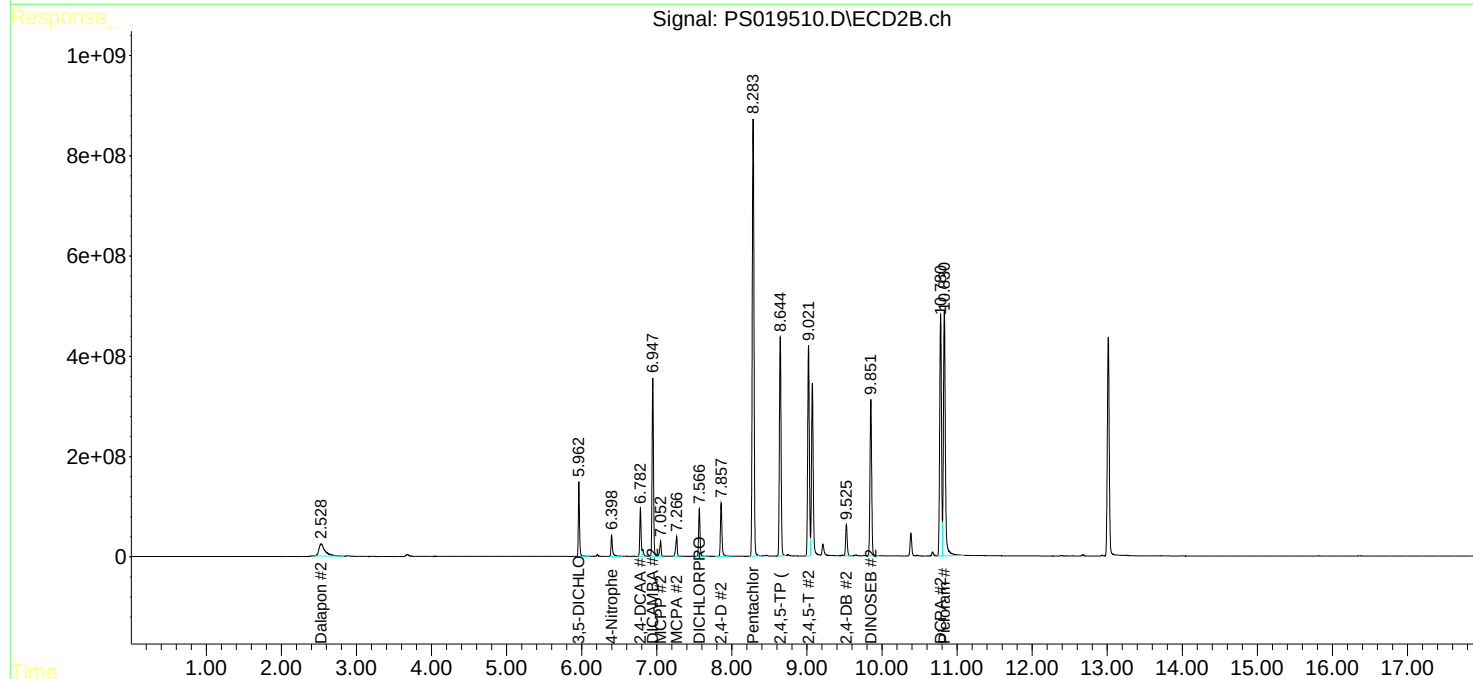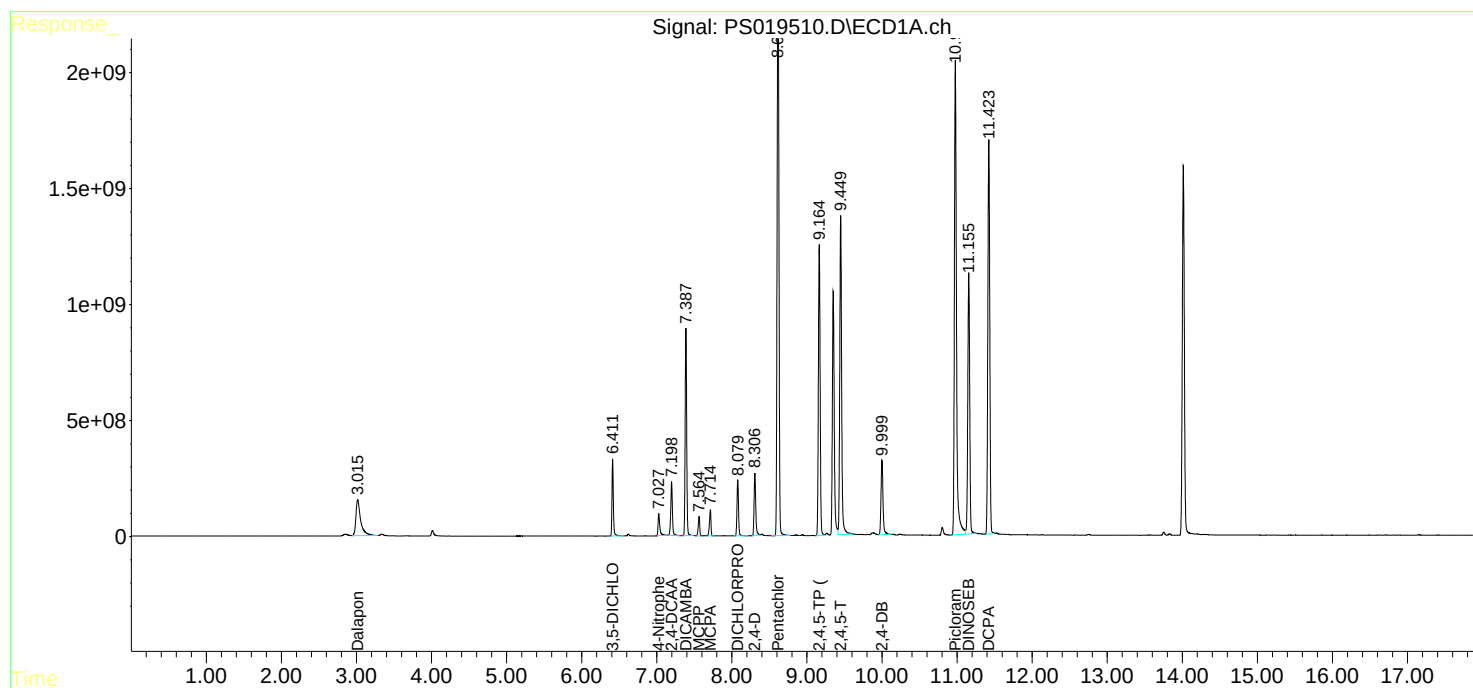


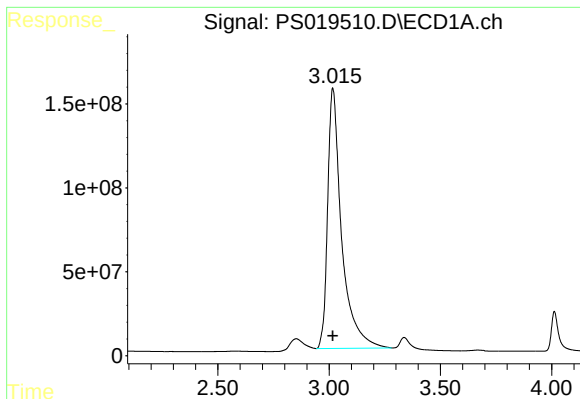

#1 Dalapon


R.T.: 3.016 min
Delta R.T.: 0.000 min
Response: 6791390796
Conc: 1363.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

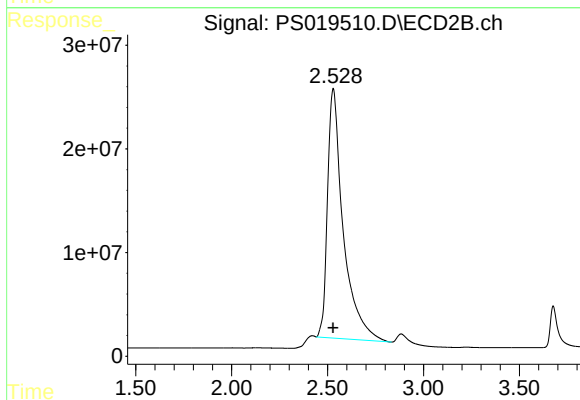


#1 Dalapon

R.T.: 2.529 min
Delta R.T.: 0.000 min
Response: 1369390542
Conc: 1376.78 ng/ml

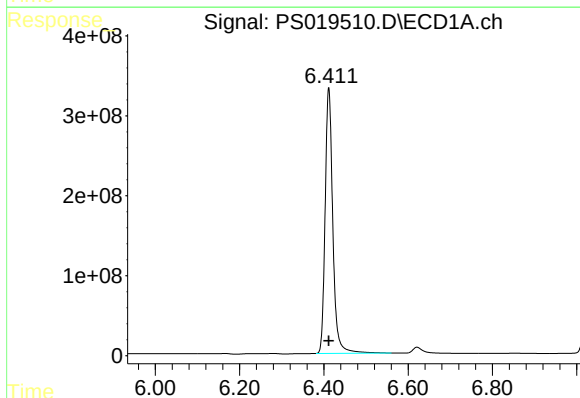


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 4194131836
Conc: 1366.28 ng/ml

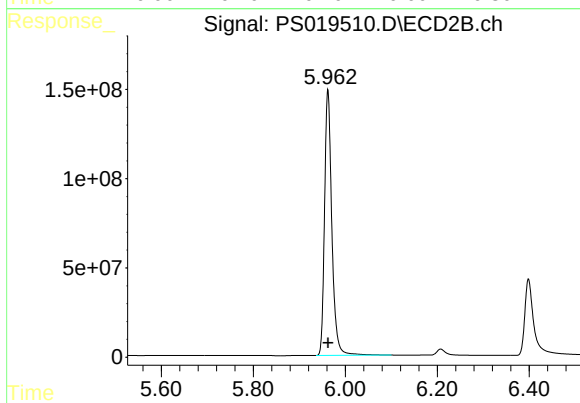

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.962 min
Delta R.T.: 0.000 min
Response: 1638679190
Conc: 1385.84 ng/ml

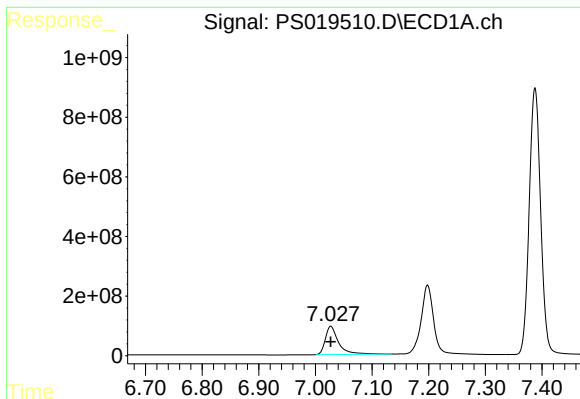

#3 4-Nitrophenol


R.T.: 7.027 min
Delta R.T.: 0.000 min
Response: 1531912487
Conc: 1429.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

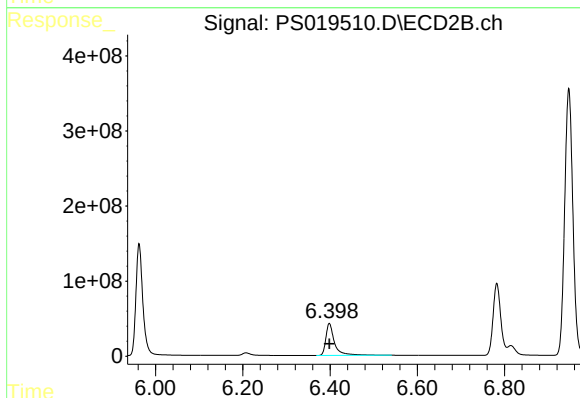


#3 4-Nitrophenol

R.T.: 6.398 min
Delta R.T.: 0.000 min
Response: 588758858
Conc: 1375.92 ng/ml

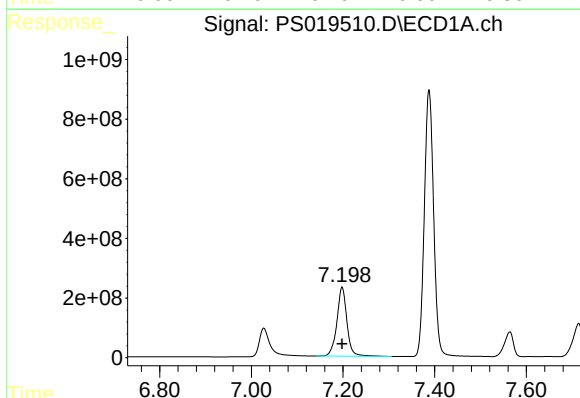


#4 2,4-DCAA

R.T.: 7.198 min
Delta R.T.: 0.000 min
Response: 3524762542
Conc: 1489.28 ng/ml

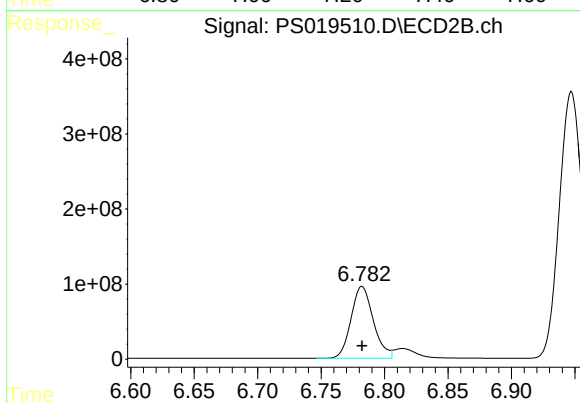

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: 0.000 min
Response: 1172580900
Conc: 1518.07 ng/ml

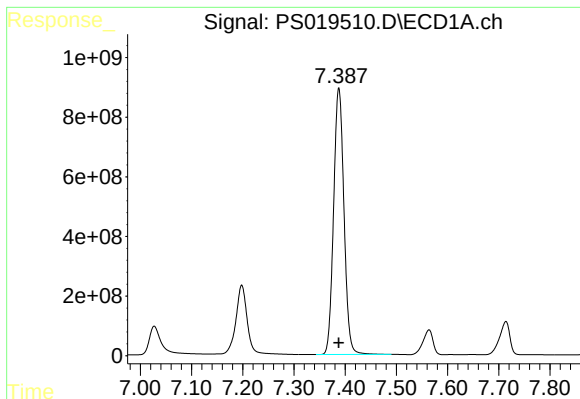

#5 DICAMBA


R.T.: 7.388 min
Delta R.T.: 0.000 min
Response: 12560351368
Conc: 1365.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

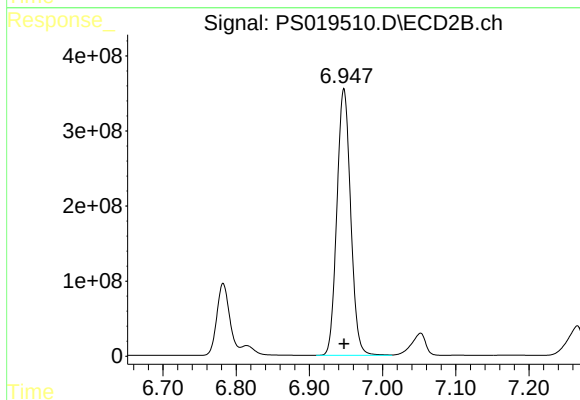


#5 DICAMBA

R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 4637979679
Conc: 1383.33 ng/ml

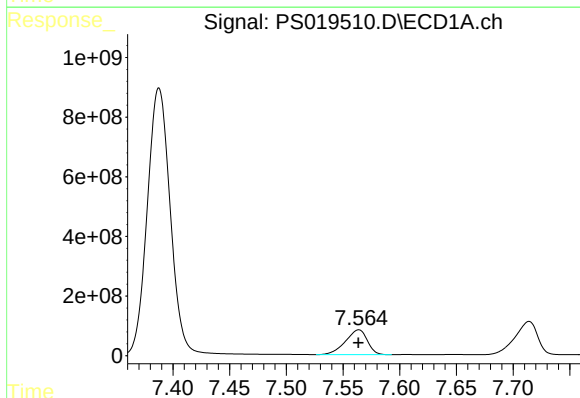


#6 MCP

R.T.: 7.564 min
Delta R.T.: 0.000 min
Response: 1124752852
Conc: 144.43 ug/ml

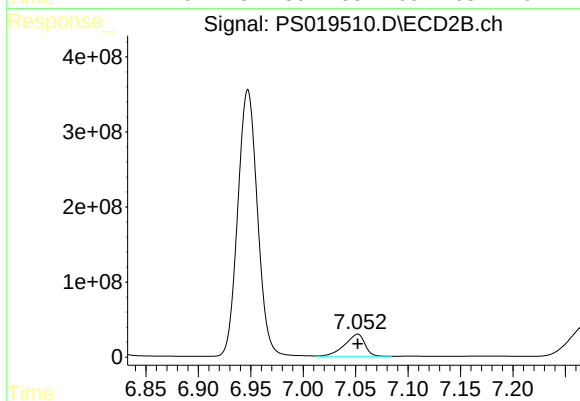

#6 MCP


R.T.: 7.052 min
Delta R.T.: 0.000 min
Response: 397062633
Conc: 143.99 ug/ml

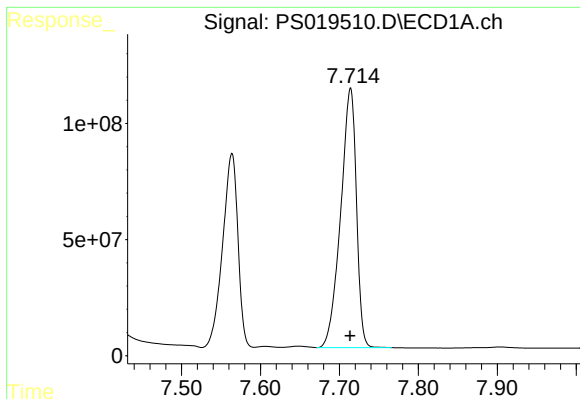

#7 MCPA


R.T.: 7.714 min
Delta R.T.: 0.000 min
Response: 1548217975
Conc: 141.05 ug/ml

Instrument :
ECD_S
ClientSampleId :

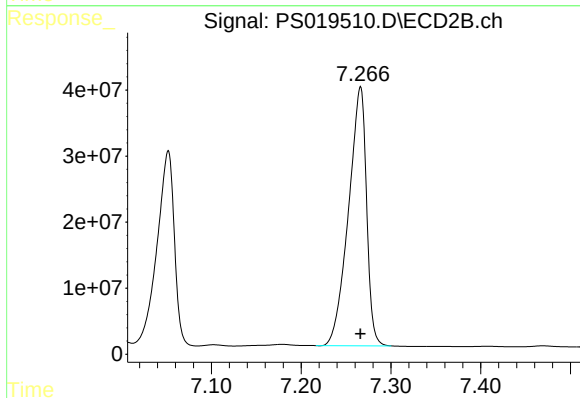


#7 MCPA

R.T.: 7.266 min
Delta R.T.: 0.000 min
Response: 547060199
Conc: 141.45 ug/ml

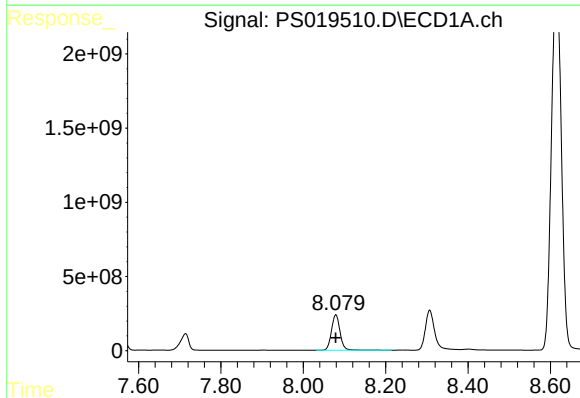


#8 DICHLORPROP

R.T.: 8.079 min
Delta R.T.: 0.000 min
Response: 3451546980
Conc: 1388.44 ng/ml

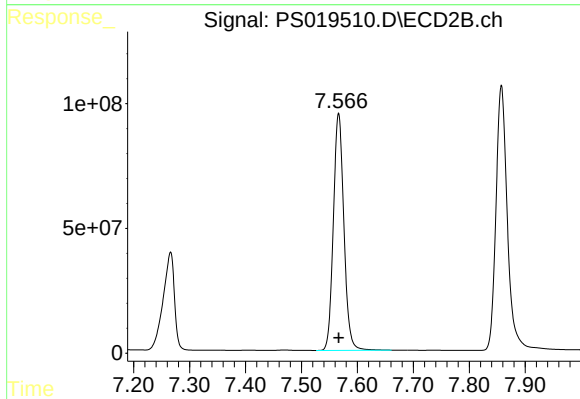

#8 DICHLORPROP


R.T.: 7.566 min
Delta R.T.: 0.000 min
Response: 1240684625
Conc: 1416.79 ng/ml

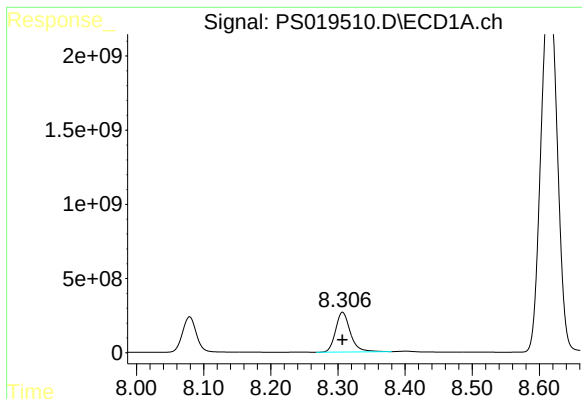

#9 2,4-D


R.T.: 8.307 min
Delta R.T.: 0.000 min
Response: 4074595551
Conc: 1409.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

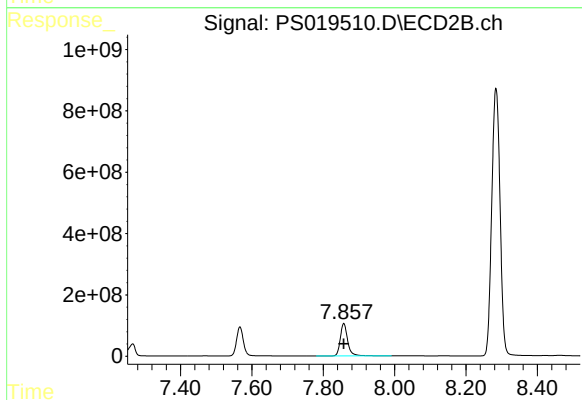


#9 2,4-D

R.T.: 7.857 min
Delta R.T.: 0.000 min
Response: 1501685144
Conc: 1413.84 ng/ml

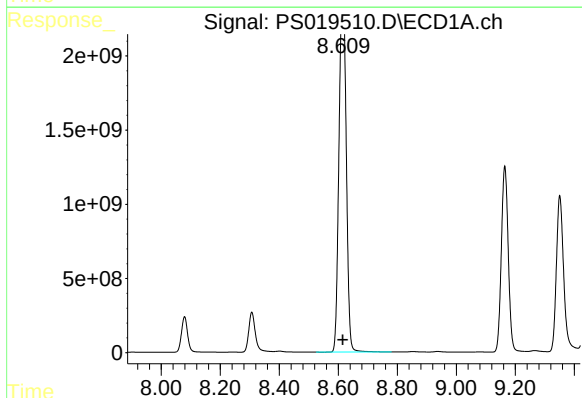


#10 Pentachlorophenol

R.T.: 8.615 min
Delta R.T.: 0.000 min
Response: 40143639784
Conc: 1285.99 ng/ml

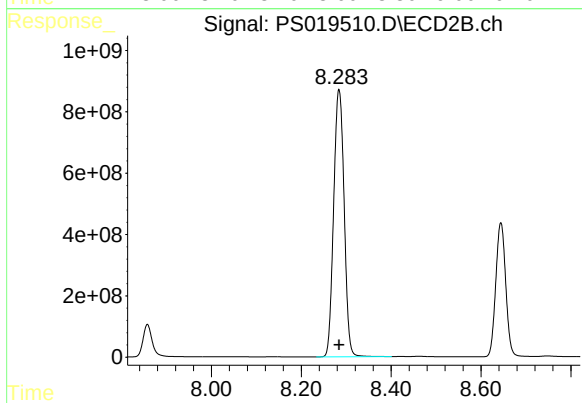

#10 Pentachlorophenol


R.T.: 8.284 min
Delta R.T.: 0.000 min
Response: 14093762487
Conc: 1317.35 ng/ml

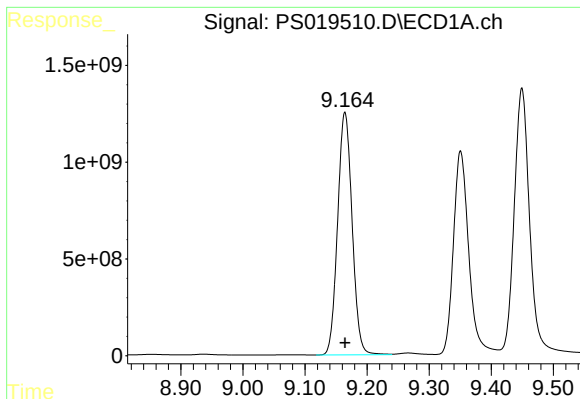

#11 2,4,5-TP (SILVEX)


R.T.: 9.164 min
Delta R.T.: 0.000 min
Response: 20314465795
Conc: 1371.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

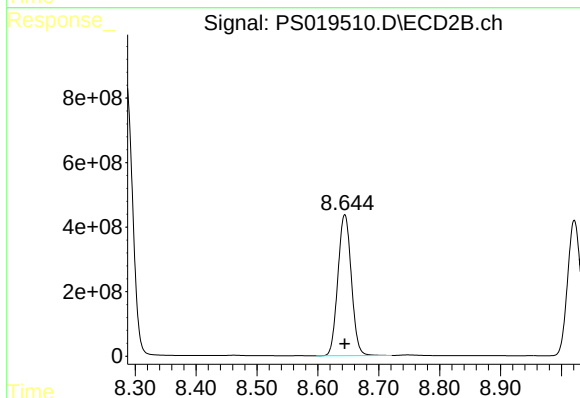


#11 2,4,5-TP (SILVEX)

R.T.: 8.644 min
Delta R.T.: 0.000 min
Response: 6710567662
Conc: 1381.05 ng/ml

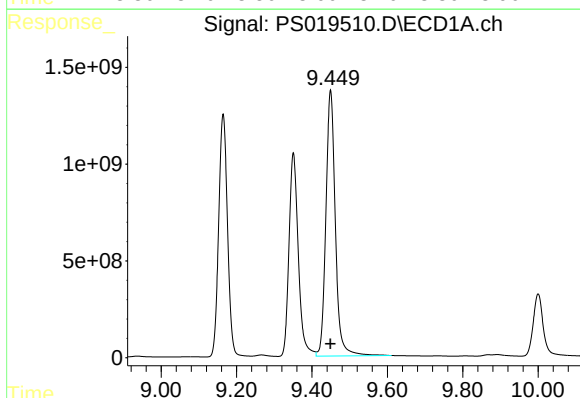


#12 2,4,5-T

R.T.: 9.449 min
Delta R.T.: 0.000 min
Response: 23924643217
Conc: 1358.95 ng/ml

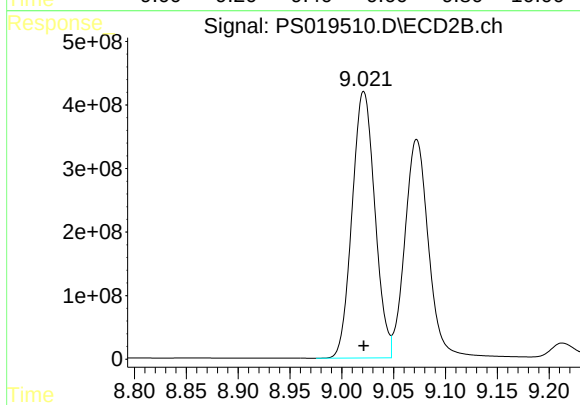

#12 2,4,5-T


R.T.: 9.021 min
Delta R.T.: 0.000 min
Response: 6409159523
Conc: 1390.50 ng/ml

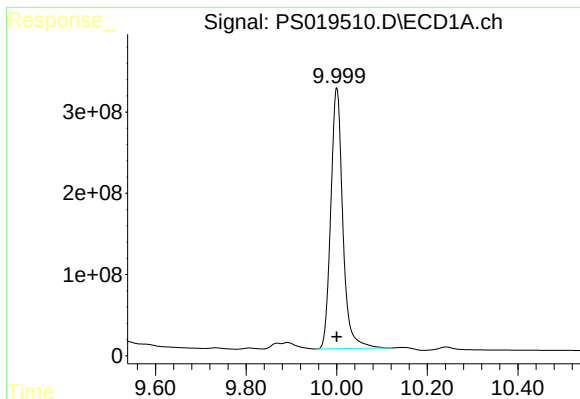

#13 2,4-DB


R.T.: 10.000 min
Delta R.T.: 0.000 min
Response: 5912179325
Conc: 1442.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

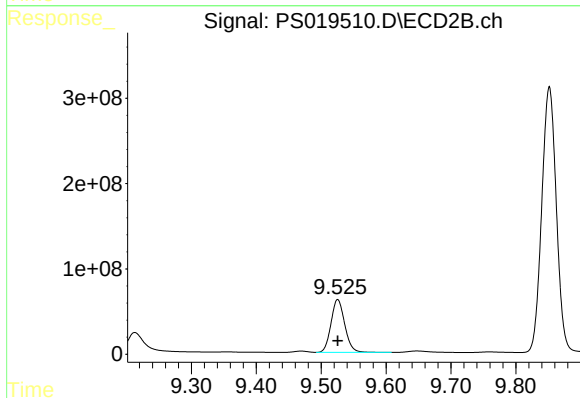


#13 2,4-DB

R.T.: 9.525 min
Delta R.T.: 0.000 min
Response: 913319890
Conc: 1454.81 ng/ml

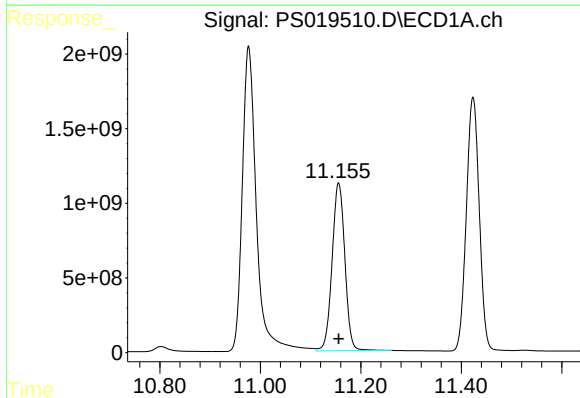


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: 0.000 min
Response: 19849794540
Conc: 1360.25 ng/ml

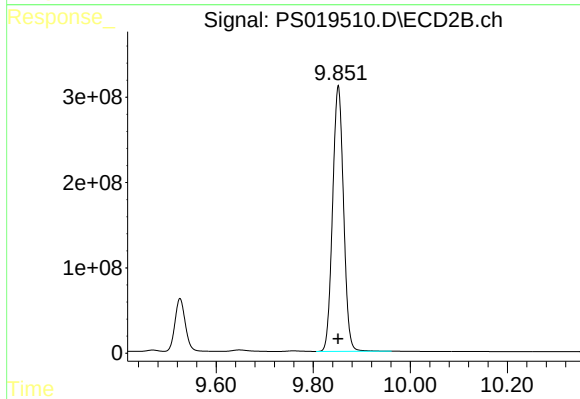

#14 DINOSEB


R.T.: 9.852 min
Delta R.T.: 0.000 min
Response: 4863618333
Conc: 1390.06 ng/ml

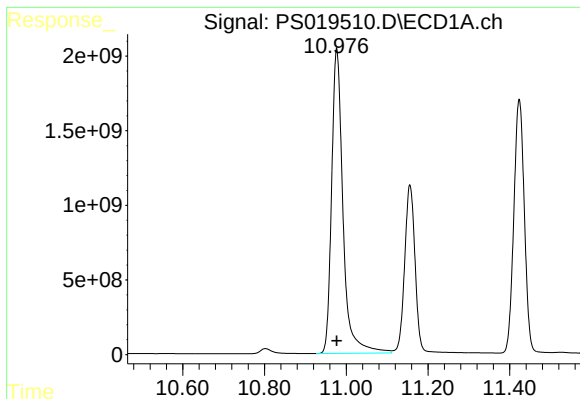

#15 Picloram


R.T.: 10.977 min
Delta R.T.: 0.000 min
Response: 39630263962
Conc: 1381.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

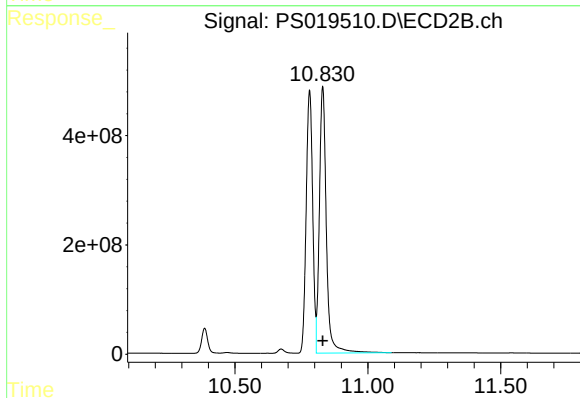


#15 Picloram

R.T.: 10.830 min
Delta R.T.: 0.000 min
Response: 8862567307
Conc: 1398.61 ng/ml

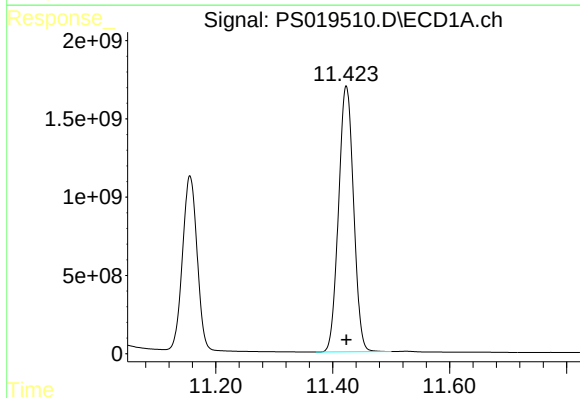

#16 DCPA

R.T.: 11.423 min
Delta R.T.: 0.000 min
Response: 30271773452
Conc: 1362.40 ng/ml

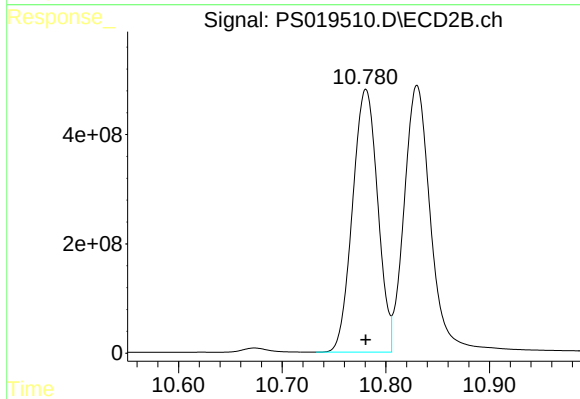

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 8106729535
Conc: 1382.38 ng/ml