

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052423\
 Data File : PS023100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 May 2023 09:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:15:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.487	6.859	796.5E6	299.4E6	523.692	533.612
Target Compounds							
1) T	Dalapon	2.573	0.000	765149	0	<MDL	N.D. #
3) T	4-Nitroph...	6.320	0.000	6717198	0	6.380	N.D. #
5) T	DICAMBA	0.000	7.078f	0	853679	N.D.	<MDL
6) T	MCP	6.758	7.078	112201	853679	<MDL	<MDL #
7) T	MCPA	6.862f	7.333	-4347073	3469213	N.D.	1.310
8) T	DICHLORPROP	7.199f	7.668	6696954	3274356	3.573	5.291 #
9) T	2,4-D	7.410	0.000	16597243	0	7.172	N.D. #
10) T	Pentachlo...	7.681	0.000	664546	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.220	0.000	3066824	0	<MDL	N.D. #
12) T	2,4,5-T	8.488	9.149f	2452960	1668983	<MDL	<MDL #
13) T	2,4-DB	8.999	0.000	2183537	0	<MDL	N.D. #
14) T	DINOSEB	10.075	0.000	875621	0	<MDL	N.D. #
15) T	Picloram	9.901	10.906	41285741	6007003	2.408	1.410 #
16) T	DCPA	10.341	10.906f	2163858	6007003	<MDL	1.608 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052423\
Data File : PS023100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 May 2023 09:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:15:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

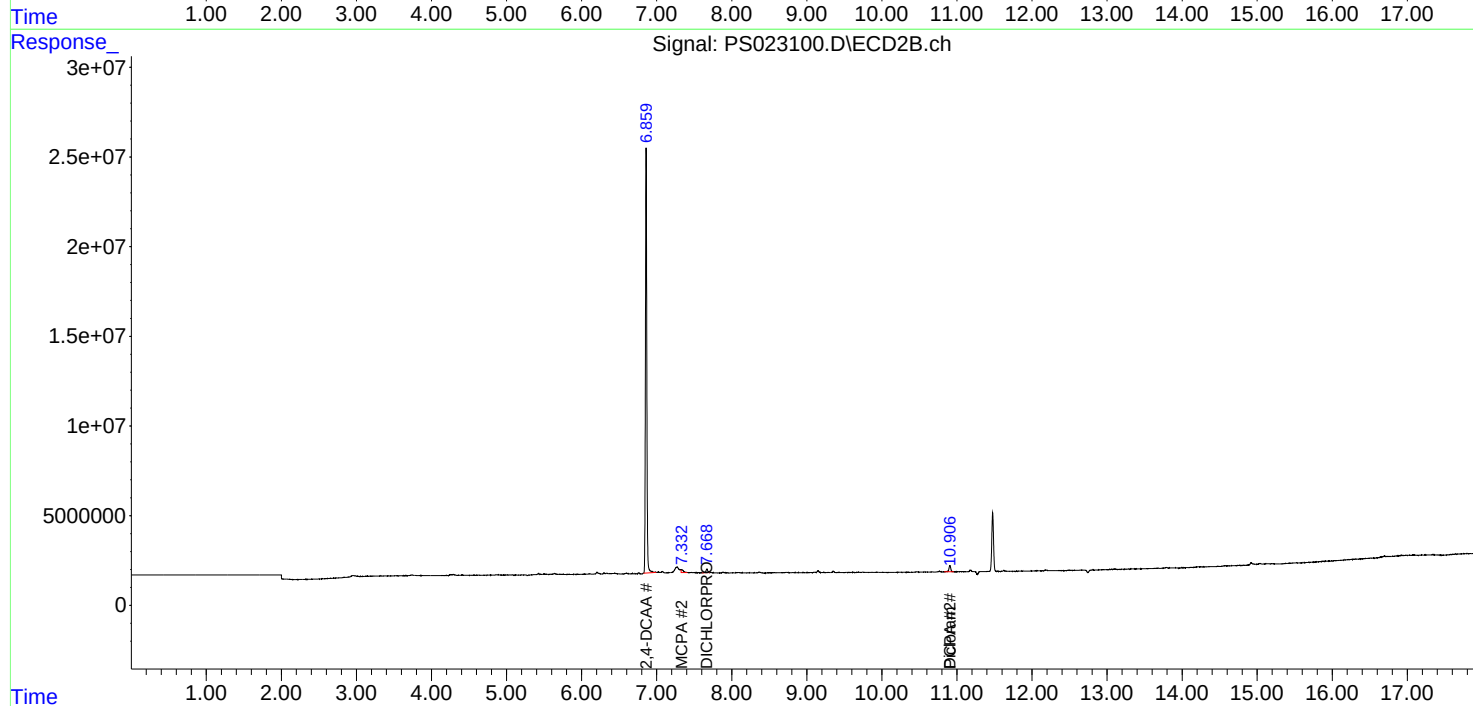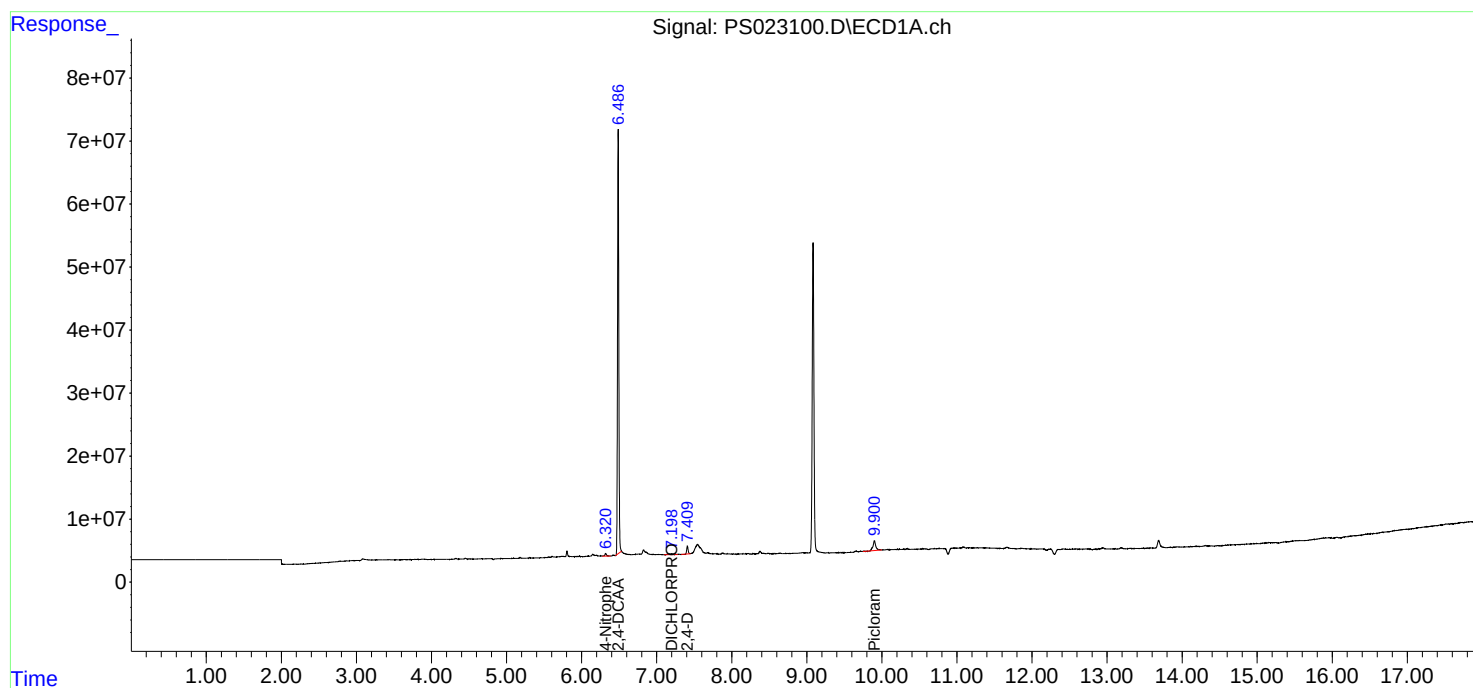


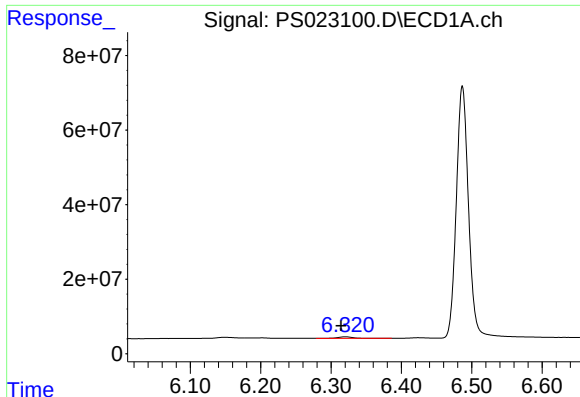

#3 4-Nitrophenol


R.T.: 6.320 min
Delta R.T.: 0.006 min
Response: 6717198
Conc: 6.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

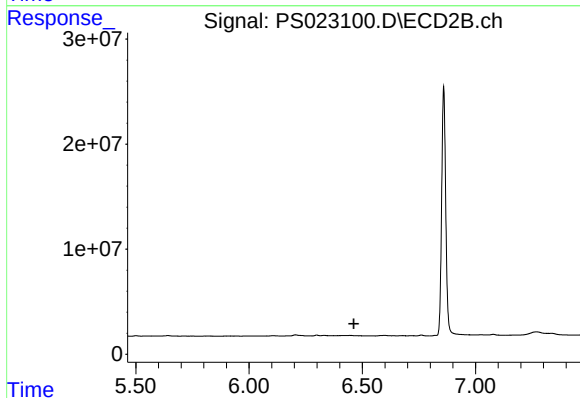


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

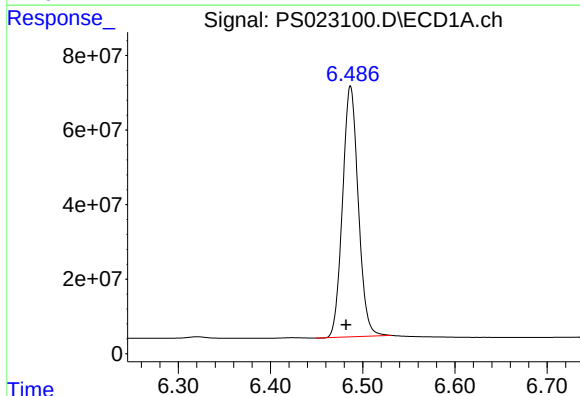


#4 2,4-DCAA

R.T.: 6.487 min
Delta R.T.: 0.005 min
Response: 796533324
Conc: 523.69 ng/ml

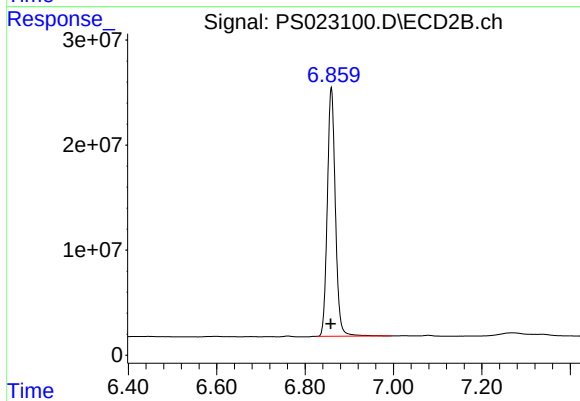

#4 2,4-DCAA


R.T.: 6.859 min
Delta R.T.: 0.001 min
Response: 299417614
Conc: 533.61 ng/ml

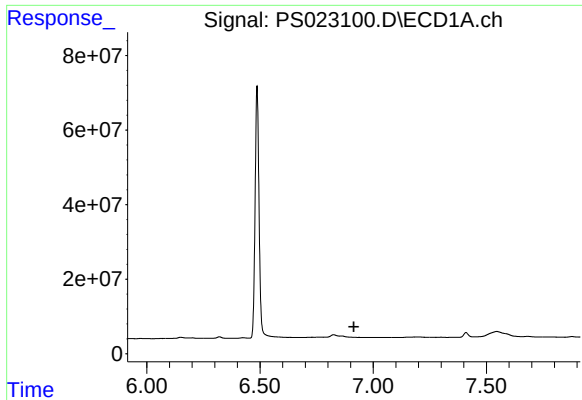

#7 MCPA


R.T.: 6.862 min
Delta R.T.: -0.053 min
Response: -4347073
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

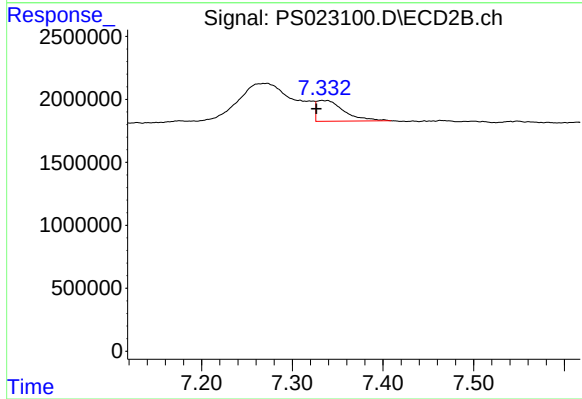


#7 MCPA

R.T.: 7.333 min
Delta R.T.: 0.006 min
Response: 3469213
Conc: 1.31 ug/ml

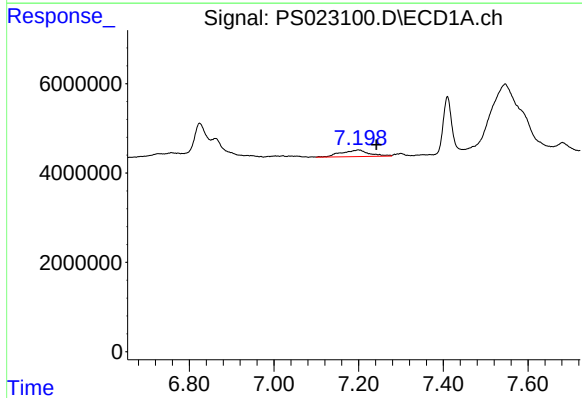


#8 DICHLORPROP

R.T.: 7.199 min
Delta R.T.: -0.043 min
Response: 6696954
Conc: 3.57 ng/ml

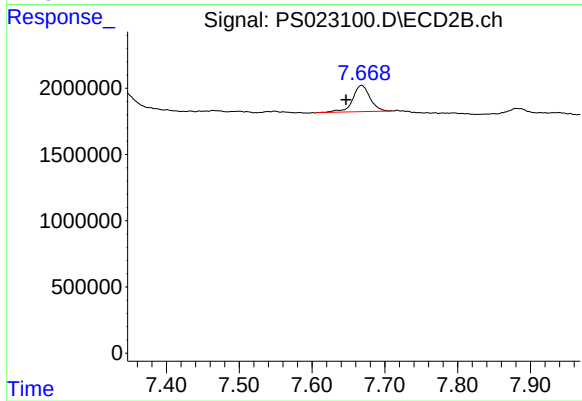

#8 DICHLORPROP


R.T.: 7.668 min
Delta R.T.: 0.021 min
Response: 3274356
Conc: 5.29 ng/ml

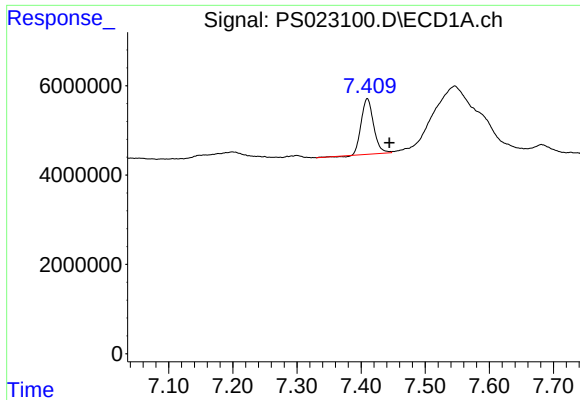

#9 2,4-D


R.T.: 7.410 min
Delta R.T.: -0.034 min
Response: 16597243
Conc: 7.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

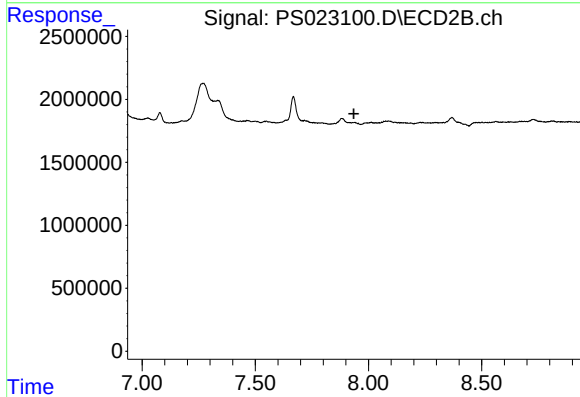


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.935 min
Response: 0
Conc: N.D.

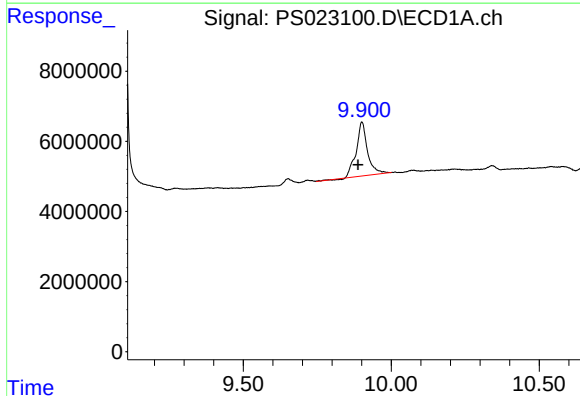


#15 Picloram

R.T.: 9.901 min
Delta R.T.: 0.013 min
Response: 41285741
Conc: 2.41 ng/ml

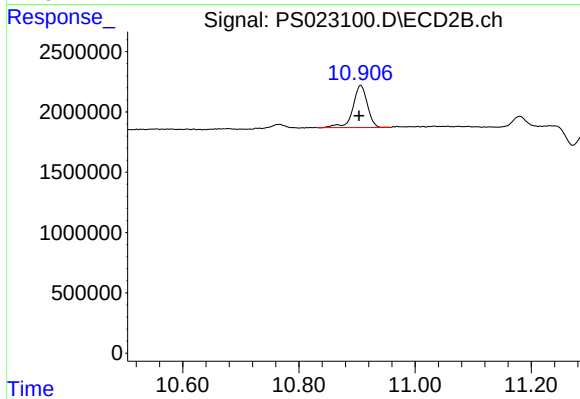

#15 Picloram


R.T.: 10.906 min
Delta R.T.: 0.003 min
Response: 6007003
Conc: 1.41 ng/ml

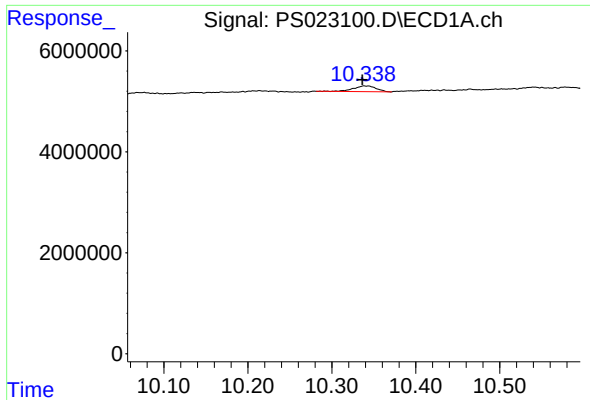

#16 DCPA

R.T.: 10.341 min
Delta R.T.: 0.004 min
Response: 2163858
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

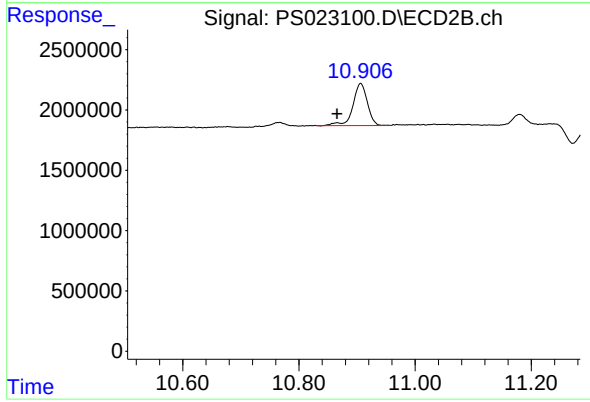

#16 DCPA

R.T.: 10.906 min
Delta R.T.: 0.041 min
Response: 6007003
Conc: 1.61 ng/ml