

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052423\
 Data File : PS023118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2023 00:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 25 05:43:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.485	6.859	782.9E6	300.9E6	514.761	536.166
Target Compounds							
1) T	Dalapon	2.581	0.000	2179124	0	1.348	N.D. #
2) T	3,5-DICHL...	5.893f	0.000	167173	0	<MDL	N.D. #
3) T	4-Nitroph...	6.318	0.000	6732279	0	6.395	N.D. #
5) T	DICAMBA	6.697f	7.025	796220	671746	<MDL	<MDL #
6) T	MCP	6.753	7.078	311062	1061523	<MDL	<MDL #
7) T	MCPA	6.938	7.308	-188928	5735987	N.D.	2.166
8) T	DICHLORPROP	7.197f	7.666	10992741	6804840	5.866	10.996 #
9) T	2,4-D	7.408	7.879f	19962265	1080247	8.626	1.510 #
10) T	Pentachlo...	7.679	0.000	1473427	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.215	0.000	4163151	0	<MDL	N.D. #
12) T	2,4,5-T	8.482	9.145f	3544335	1341604	<MDL	<MDL #
13) T	2,4-DB	8.937f	0.000	37779178	0	16.104	N.D. #
14) T	DINOSEB	10.066	0.000	498904	0	<MDL	N.D. #
15) T	Picloram	9.894	10.903	29148994	4079399	1.700	<MDL #
16) T	DCPA	10.337	10.903	2329763	4079399	<MDL	1.092 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052423\
Data File : PS023118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2023 00:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 25 05:43:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

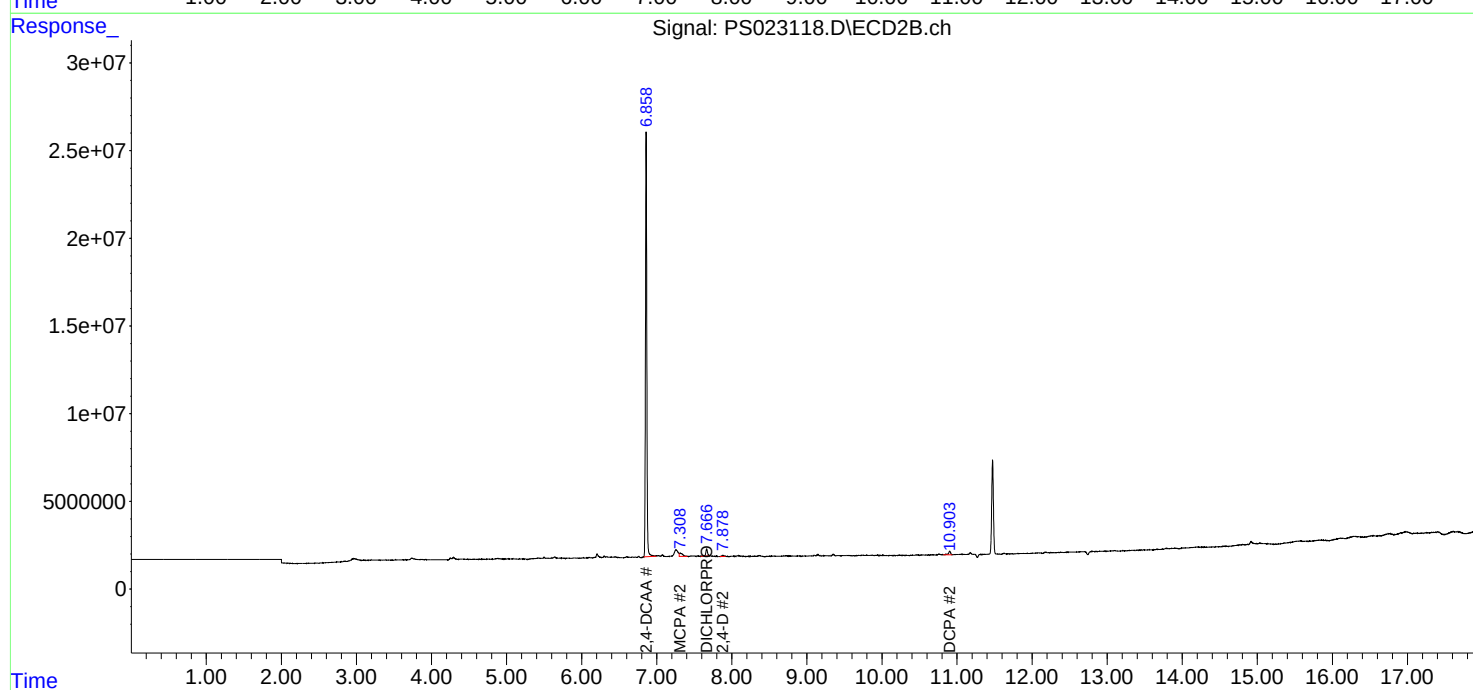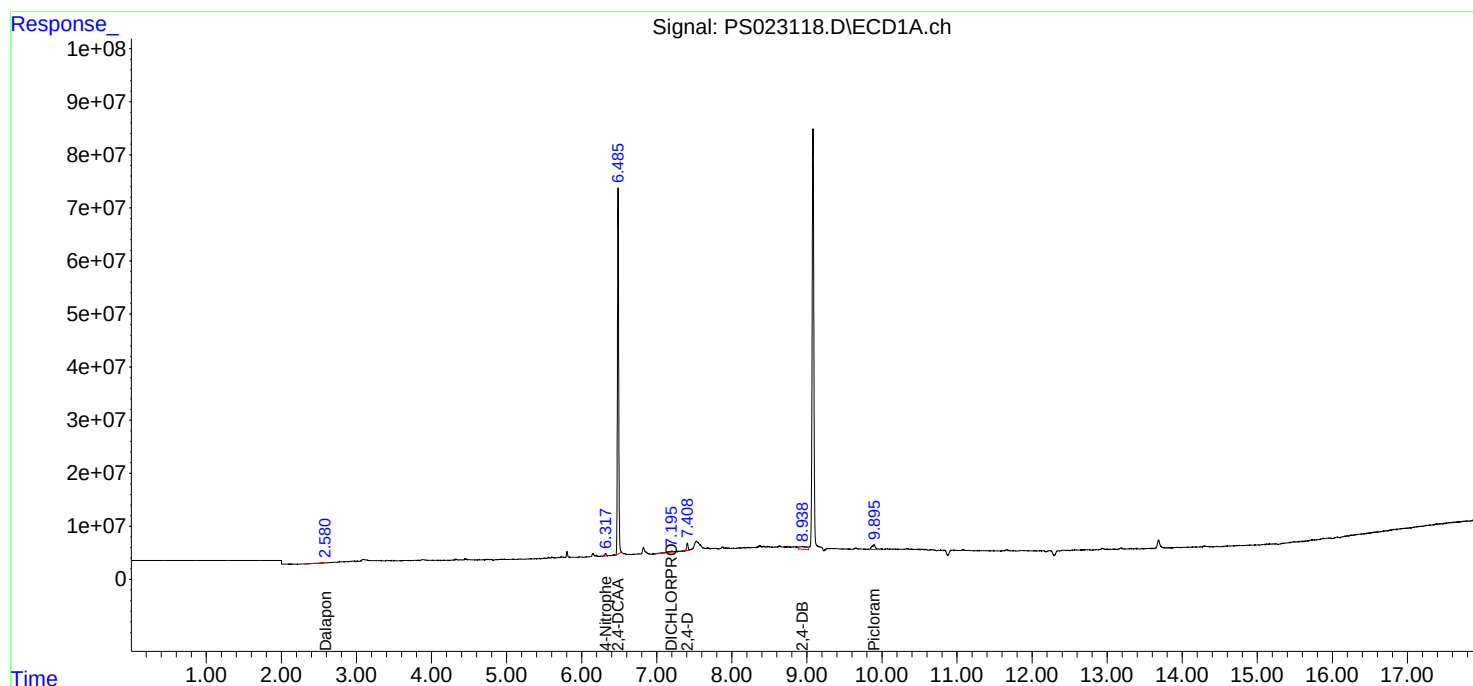


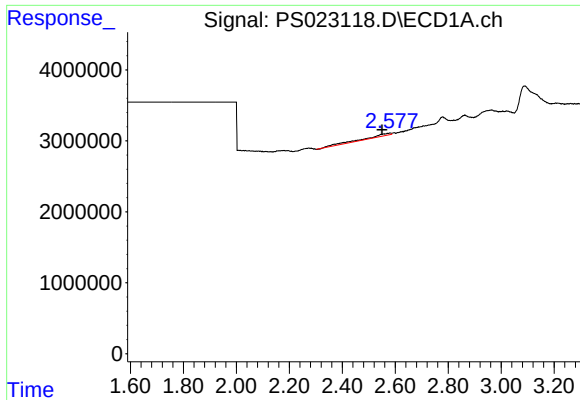

#1 Dalapon


R.T.: 2.581 min
Delta R.T.: 0.030 min
Response: 2179124
Conc: 1.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

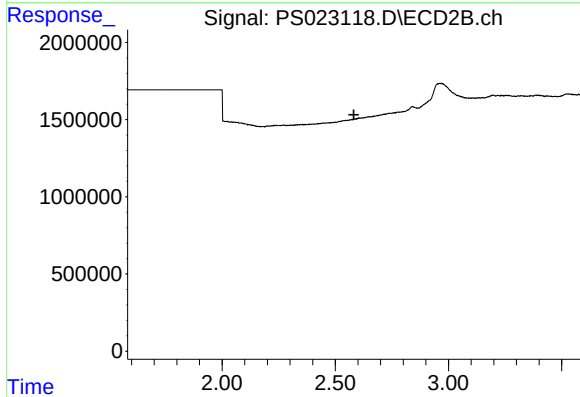


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.582 min
Response: 0
Conc: N.D.

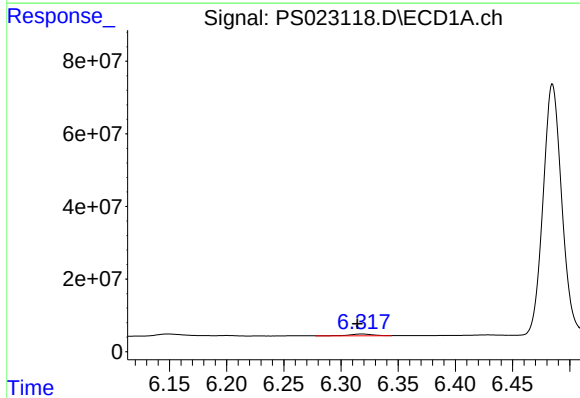


#3 4-Nitrophenol

R.T.: 6.318 min
Delta R.T.: 0.004 min
Response: 6732279
Conc: 6.39 ng/ml

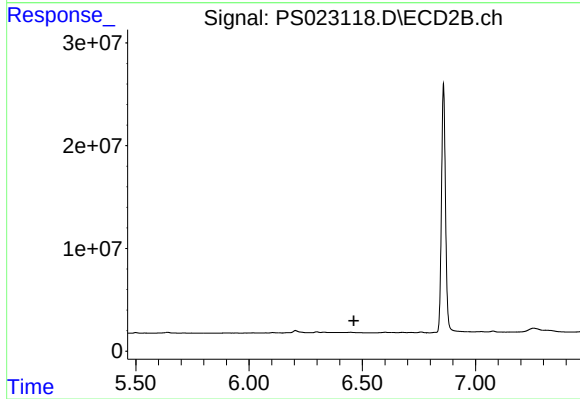

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

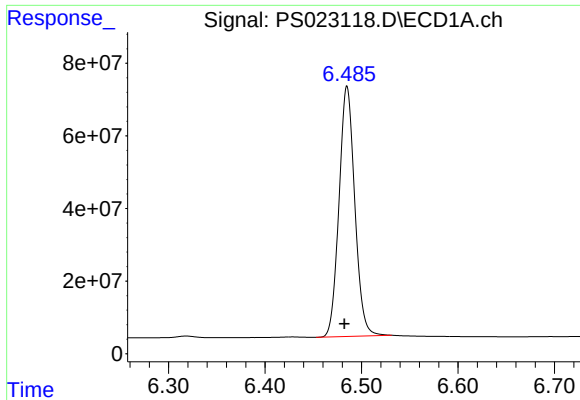

#4 2,4-DCAA


R.T.: 6.485 min
Delta R.T.: 0.003 min
Response: 782948627
Conc: 514.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

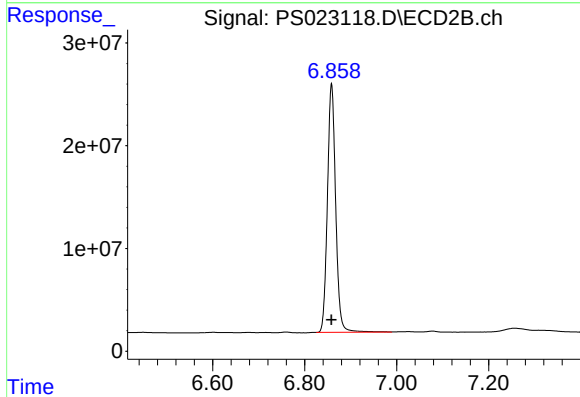


#4 2,4-DCAA

R.T.: 6.859 min
Delta R.T.: 0.000 min
Response: 300851224
Conc: 536.17 ng/ml

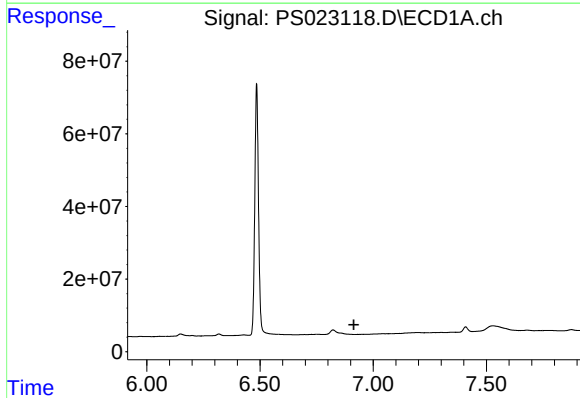


#7 MCPA

R.T.: 6.938 min
Delta R.T.: 0.023 min
Response: -188928
Conc: N.D.

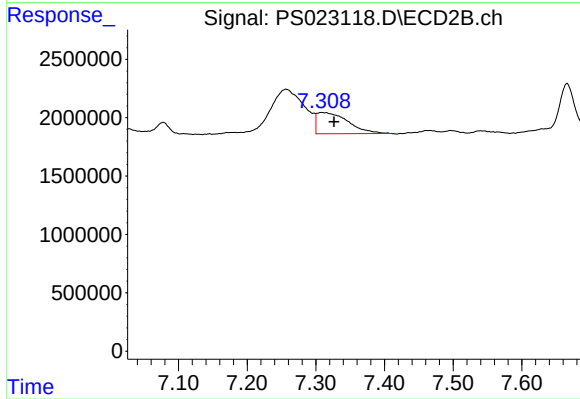

#7 MCPA


R.T.: 7.308 min
Delta R.T.: -0.018 min
Response: 5735987
Conc: 2.17 ug/ml

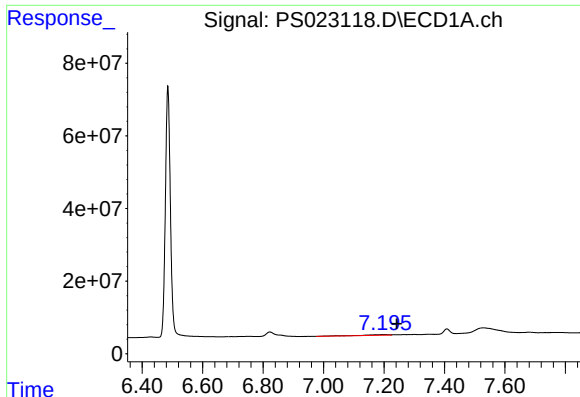

#8 DICHLORPROP


R.T.: 7.197 min
Delta R.T.: -0.045 min
Response: 10992741
Conc: 5.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

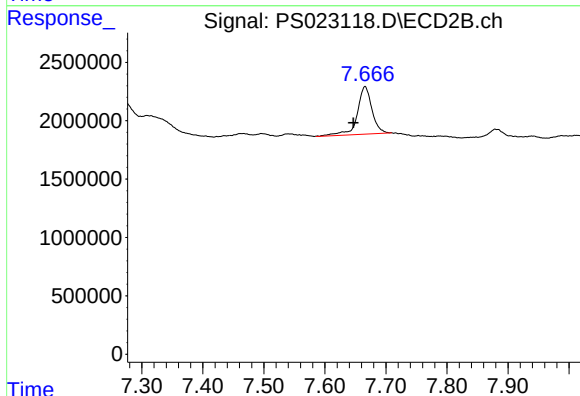


#8 DICHLORPROP

R.T.: 7.666 min
Delta R.T.: 0.019 min
Response: 6804840
Conc: 11.00 ng/ml

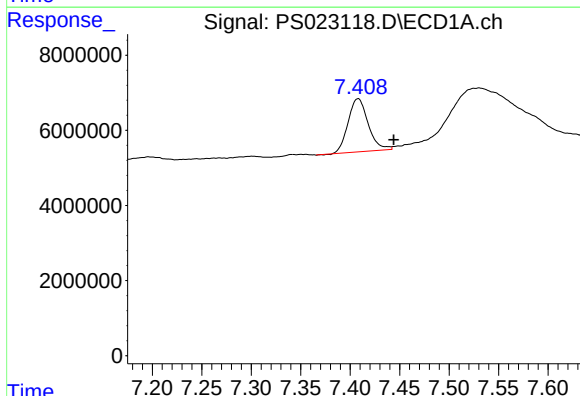


#9 2,4-D

R.T.: 7.408 min
Delta R.T.: -0.036 min
Response: 19962265
Conc: 8.63 ng/ml

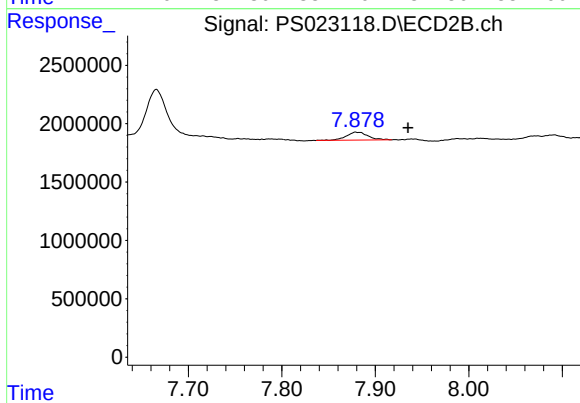

#9 2,4-D


R.T.: 7.879 min
Delta R.T.: -0.056 min
Response: 1080247
Conc: 1.51 ng/ml

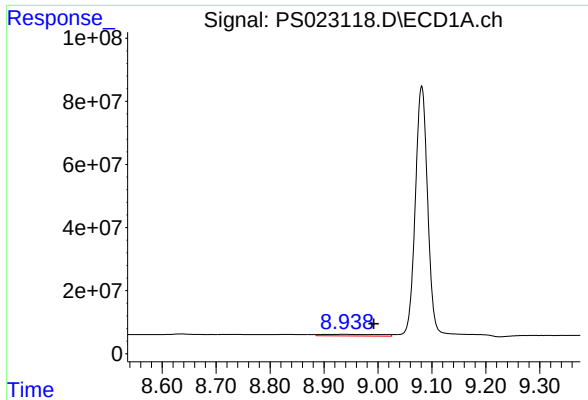

#13 2,4-DB


R.T.: 8.937 min
Delta R.T.: -0.055 min
Response: 37779178
Conc: 16.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

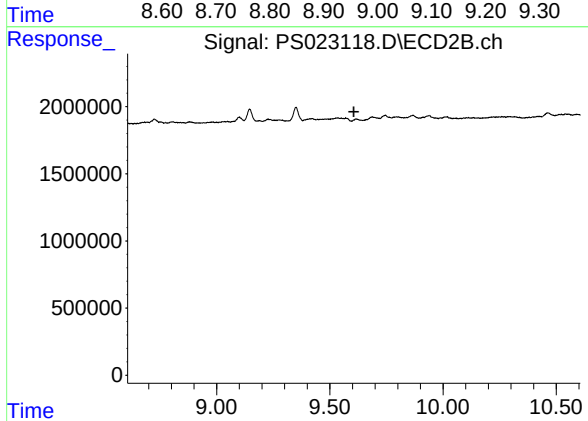


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

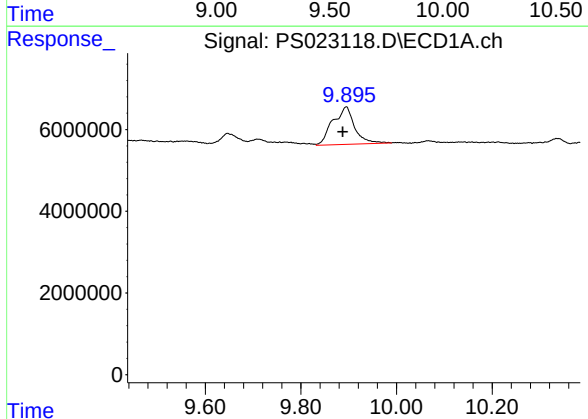


#15 Picloram

R.T.: 9.894 min
Delta R.T.: 0.007 min
Response: 29148994
Conc: 1.70 ng/ml

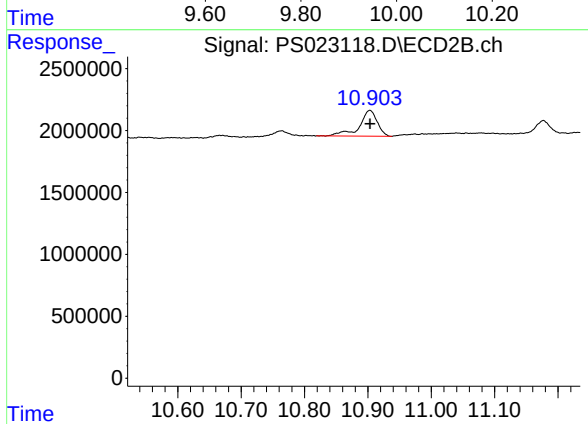

#15 Picloram


R.T.: 10.903 min
Delta R.T.: 0.000 min
Response: 4079399
Conc: N.D.

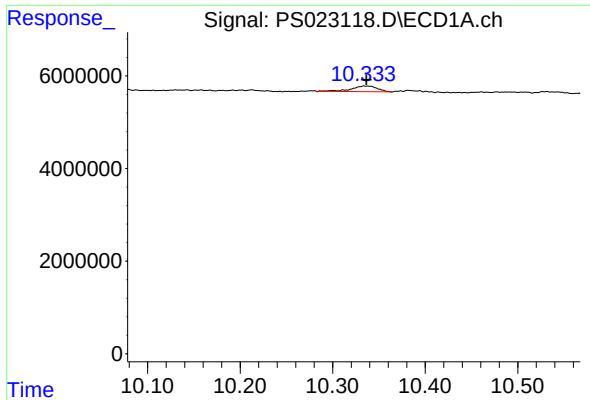

#16 DCPA

R.T.: 10.337 min
Delta R.T.: 0.000 min
Response: 2329763
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

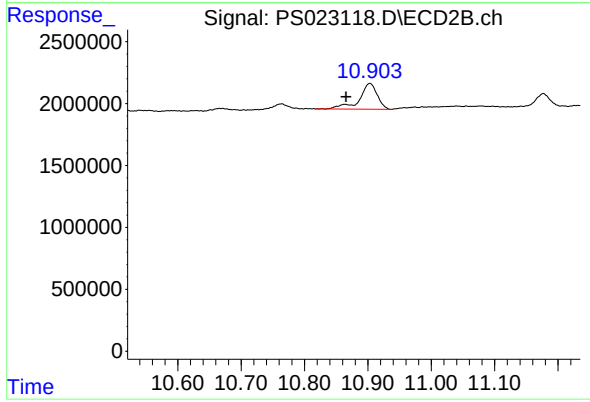

#16 DCPA

R.T.: 10.903 min
Delta R.T.: 0.037 min
Response: 4079399
Conc: 1.09 ng/ml