

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 08:37
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:51:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
Target Compounds							
2) T	3,5-DICHL...	4.938	0.000	3041.8E6	0	1763.779	N.D. #
3) T	4-Nitroph...	5.396	0.000	35884096	0	57.552	N.D. #
5) T	DICAMBA	0.000	5.436	0	2387.0E6	N.D.	646.155
6) T	MCP	5.966	0.000	17462441	0	4.195	N.D. #
8) T	DICHLORPROP	0.000	5.972	0	30245657	N.D.	32.080
9) T	2,4-D	6.614	0.000	3386.3E6	0	2475.536	N.D. #
10) T	Pentachlo...	6.876	0.000	19257400	0	1.097	N.D. #
12) T	2,4,5-T	0.000	7.389	0	62833772	N.D.	14.099
15) T	Picloram	9.114	9.097	1277.6E6	178.4E6	122.610	23.916 #
16) T	DCPA	0.000	9.097	0	178.4E6	N.D.	27.543



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 08:37
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:51:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

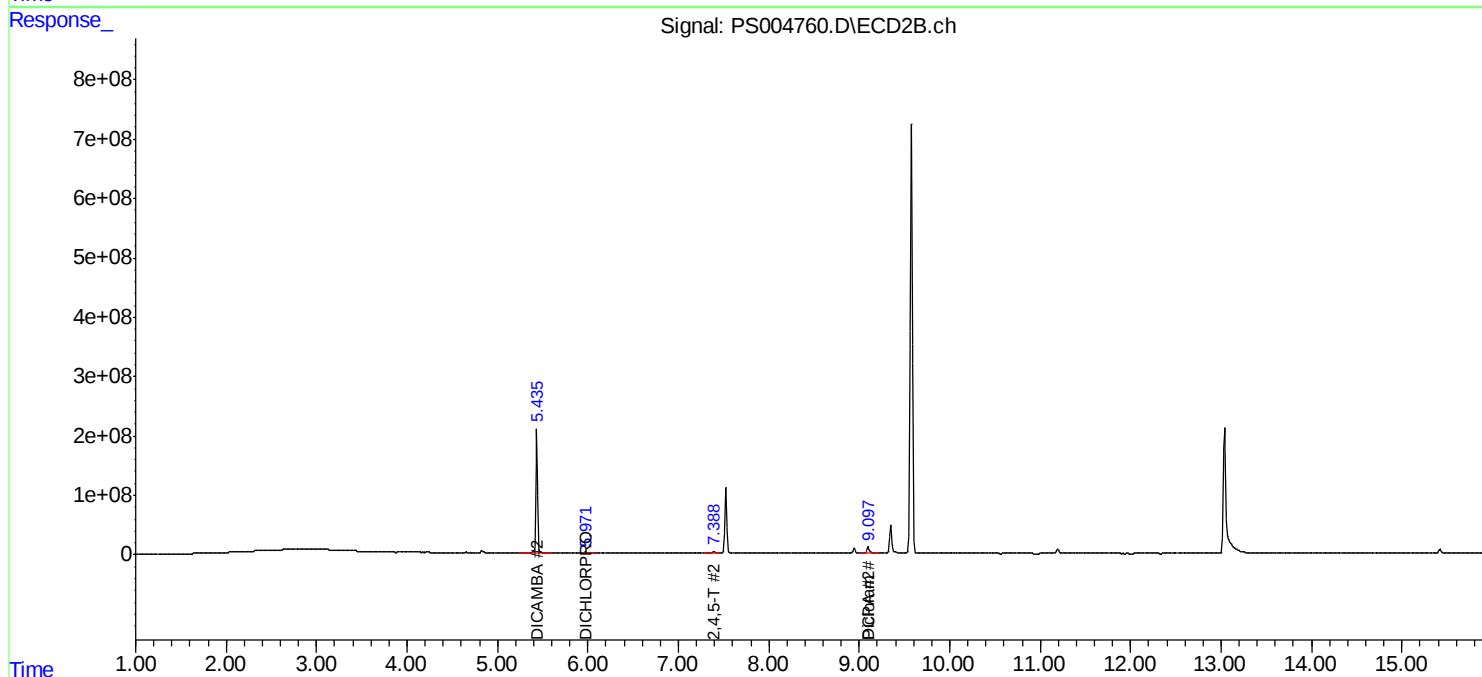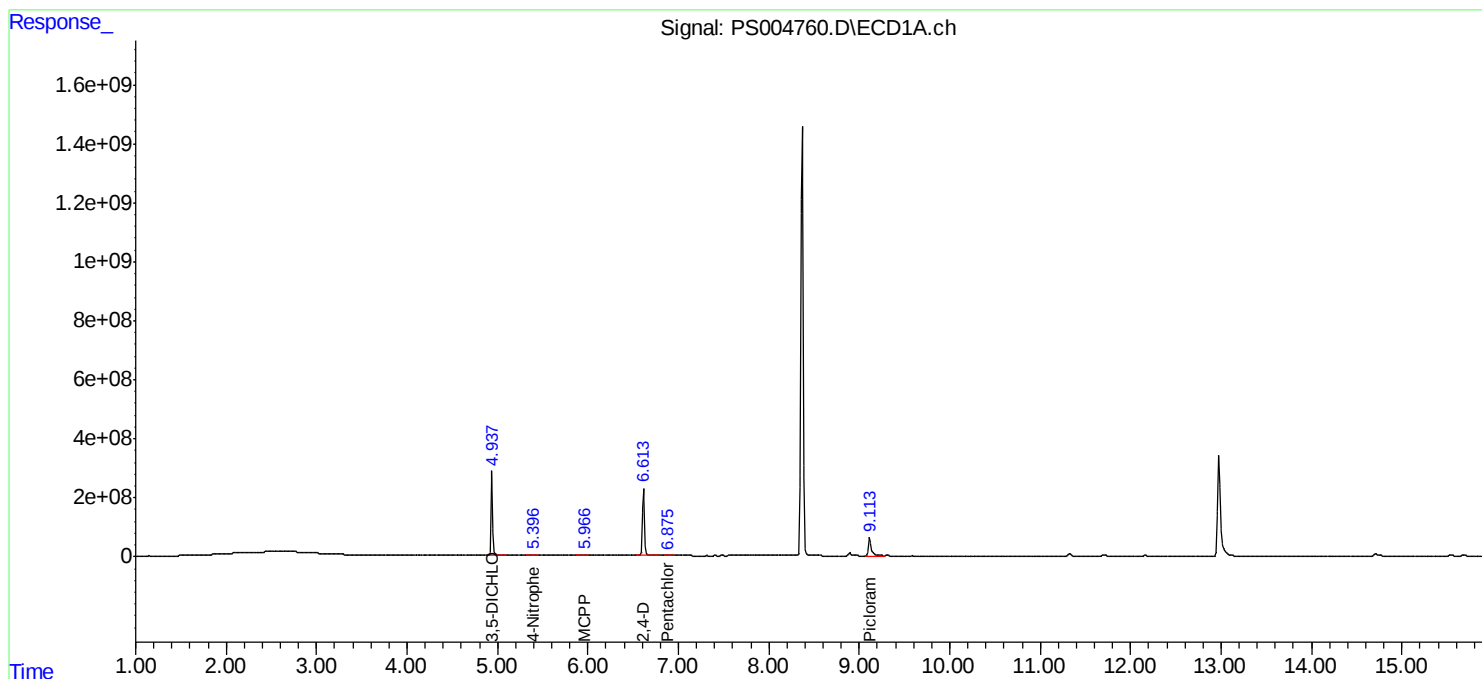


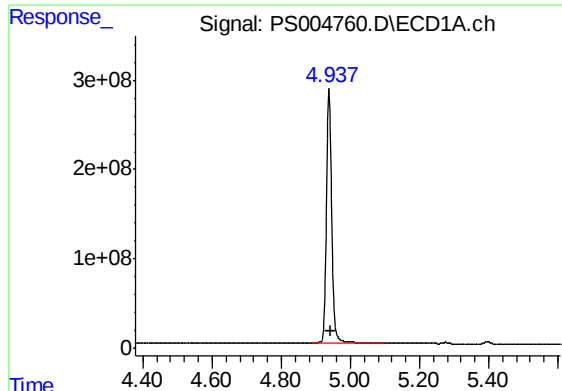

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.938 min
Delta R.T.: -0.004 min
Response: 3041763027
Conc: 1763.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

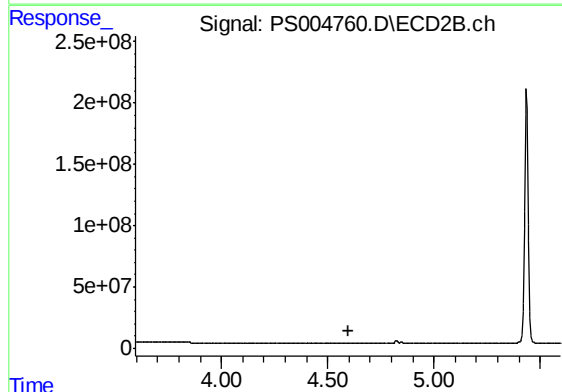


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

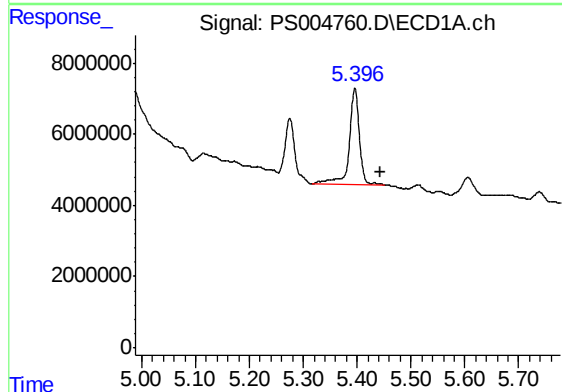


#3 4-Nitrophenol

R.T.: 5.396 min
Delta R.T.: -0.047 min
Response: 35884096
Conc: 57.55 ng/ml

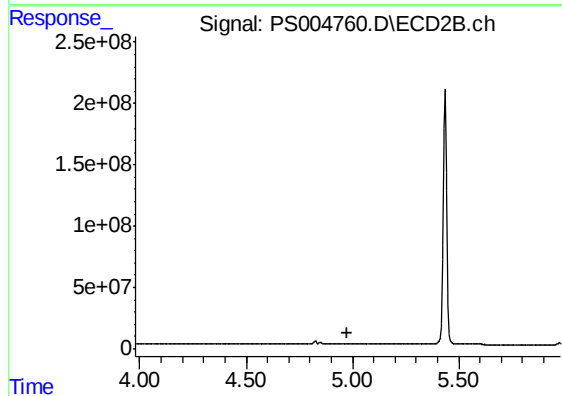

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

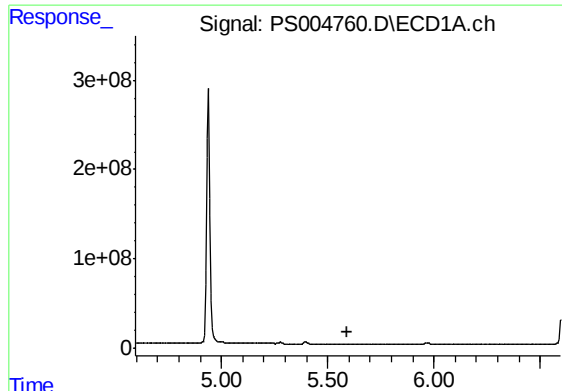

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

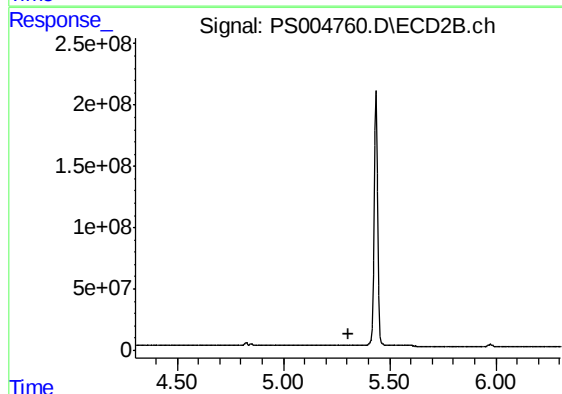


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.304 min
Response: 0
Conc: N.D.

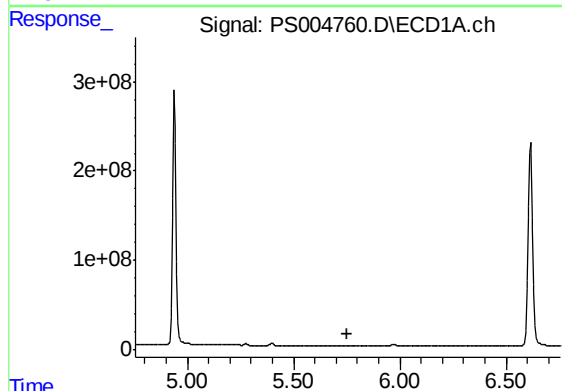


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

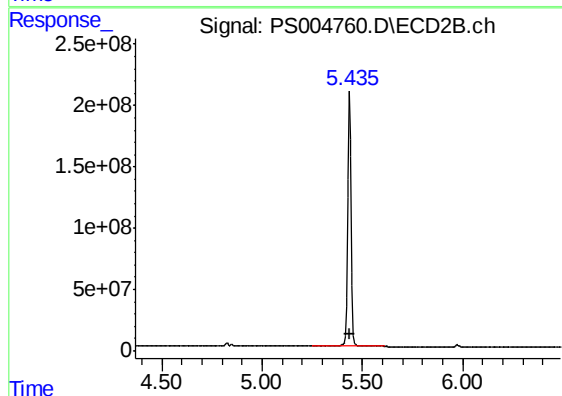

#5 DICAMBA


R.T.: 5.436 min
Delta R.T.: -0.002 min
Response: 2387046103
Conc: 646.16 ng/ml

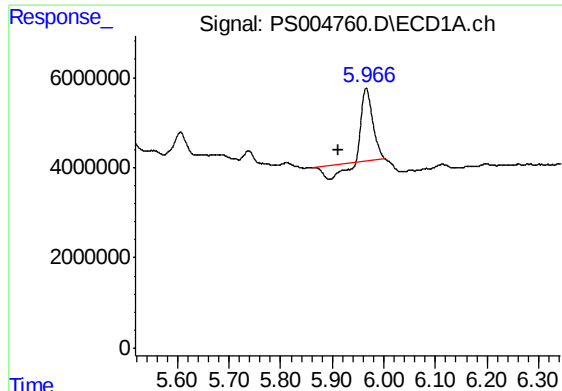

#6 MCP


R.T.: 5.966 min
Delta R.T.: 0.054 min
Response: 17462441
Conc: 4.19 ug/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

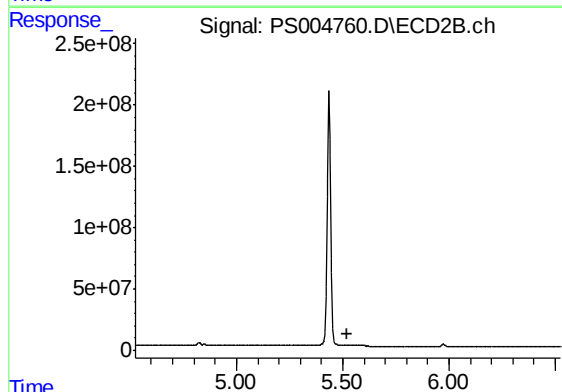


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

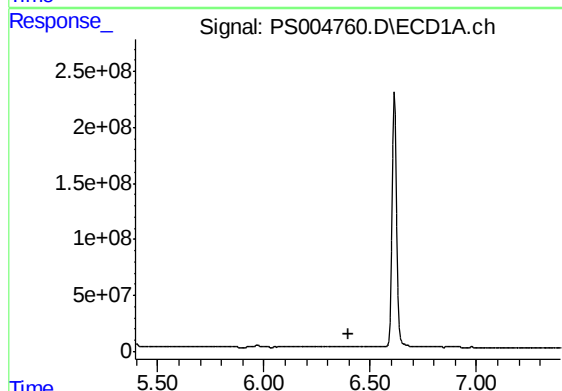


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

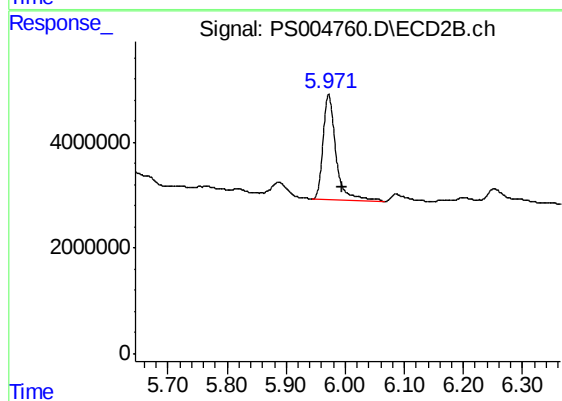

#8 DICHLORPROP


R.T.: 5.972 min
Delta R.T.: -0.022 min
Response: 30245657
Conc: 32.08 ng/ml

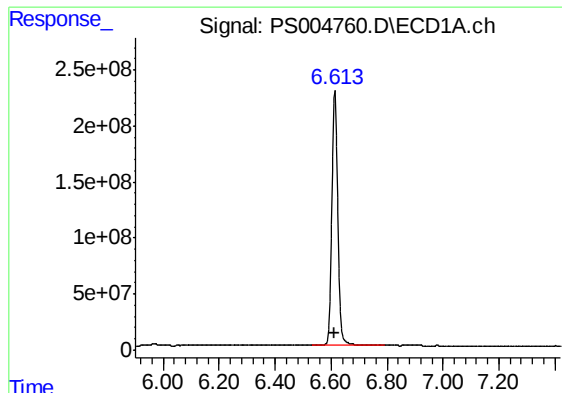

#9 2,4-D


R.T.: 6.614 min
Delta R.T.: 0.002 min
Response: 3386307263
Conc: 2475.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

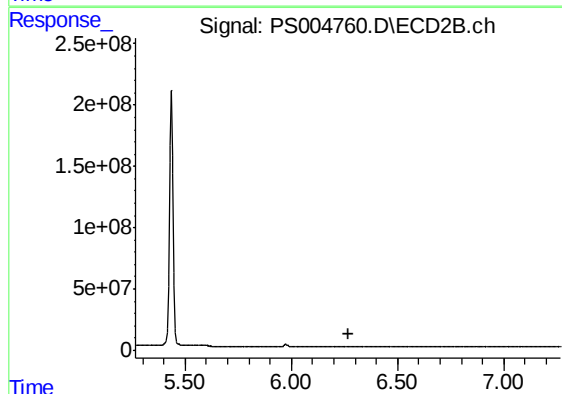


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

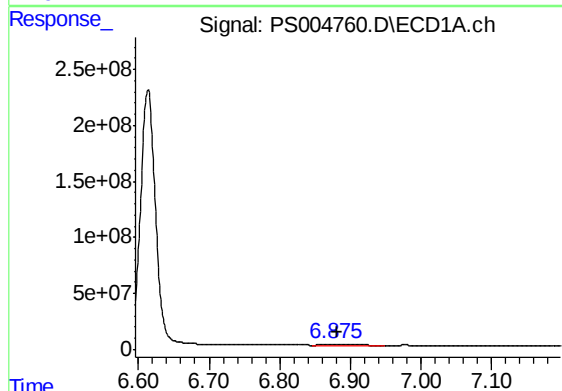


#10 Pentachlorophenol

R.T.: 6.876 min
Delta R.T.: -0.006 min
Response: 19257400
Conc: 1.10 ng/ml

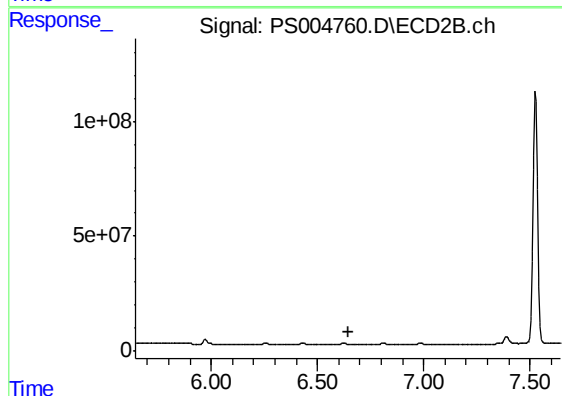

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 6.644 min
Response: 0
Conc: N.D.

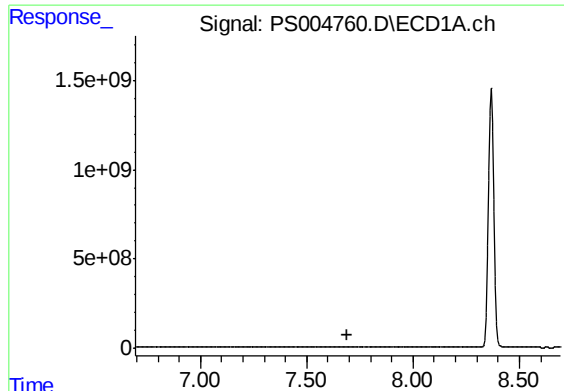

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

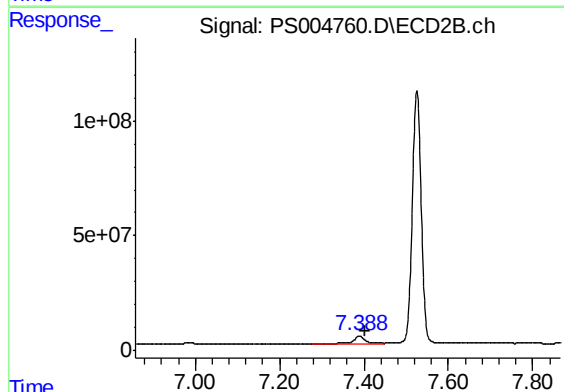


#12 2,4,5-T

R.T.: 7.389 min
Delta R.T.: -0.015 min
Response: 62833772
Conc: 14.10 ng/ml

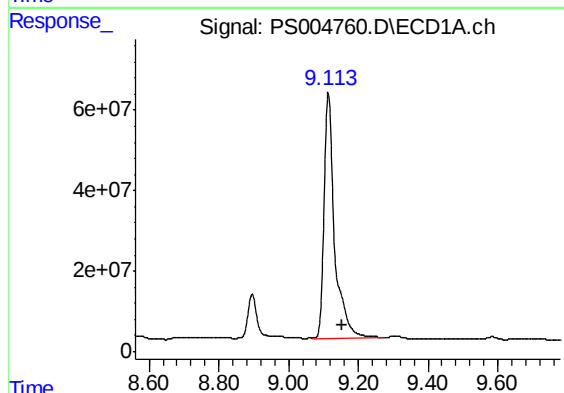


#15 Picloram

R.T.: 9.114 min
Delta R.T.: -0.041 min
Response: 1277593631
Conc: 122.61 ng/ml

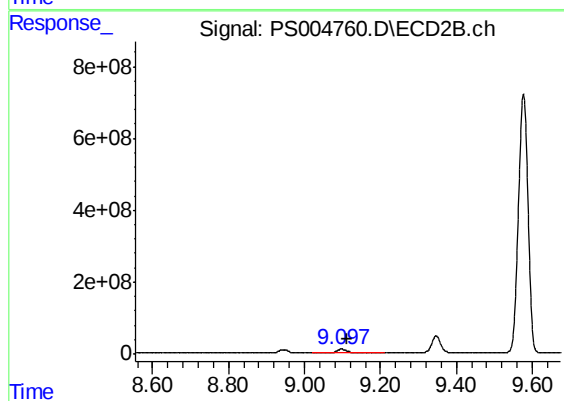

#15 Picloram


R.T.: 9.097 min
Delta R.T.: -0.016 min
Response: 178428215
Conc: 23.92 ng/ml

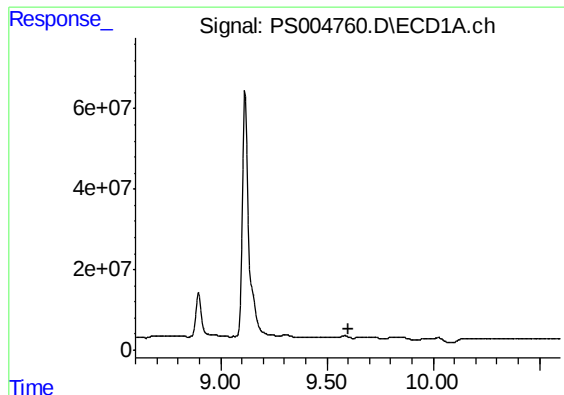

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

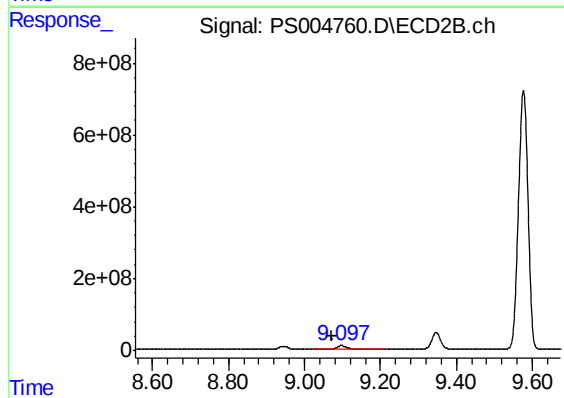

#16 DCPA

R.T.: 9.097 min
Delta R.T.: 0.025 min
Response: 178428215
Conc: 27.54 ng/ml