

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 08:59
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:51:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.285	754.5E6	532.2E6	538.244	551.574
Target Compounds							
2) T	3,5-DICHL...	4.942	0.000	57858626	0	33.550	N.D. #
5) T	DICAMBA	0.000	5.440	0	53536619	N.D.	14.492
9) T	2,4-D	6.618	0.000	121.3E6	0	88.681	N.D. #
12) T	2,4,5-T	0.000	7.398	0	34379695	N.D.	7.714
15) T	Picloram	9.156	9.103	143.2E6	116.1E6	13.739	15.564
16) T	DCPA	0.000	9.103	0	116.1E6	N.D.	17.925



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 08:59
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:51:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

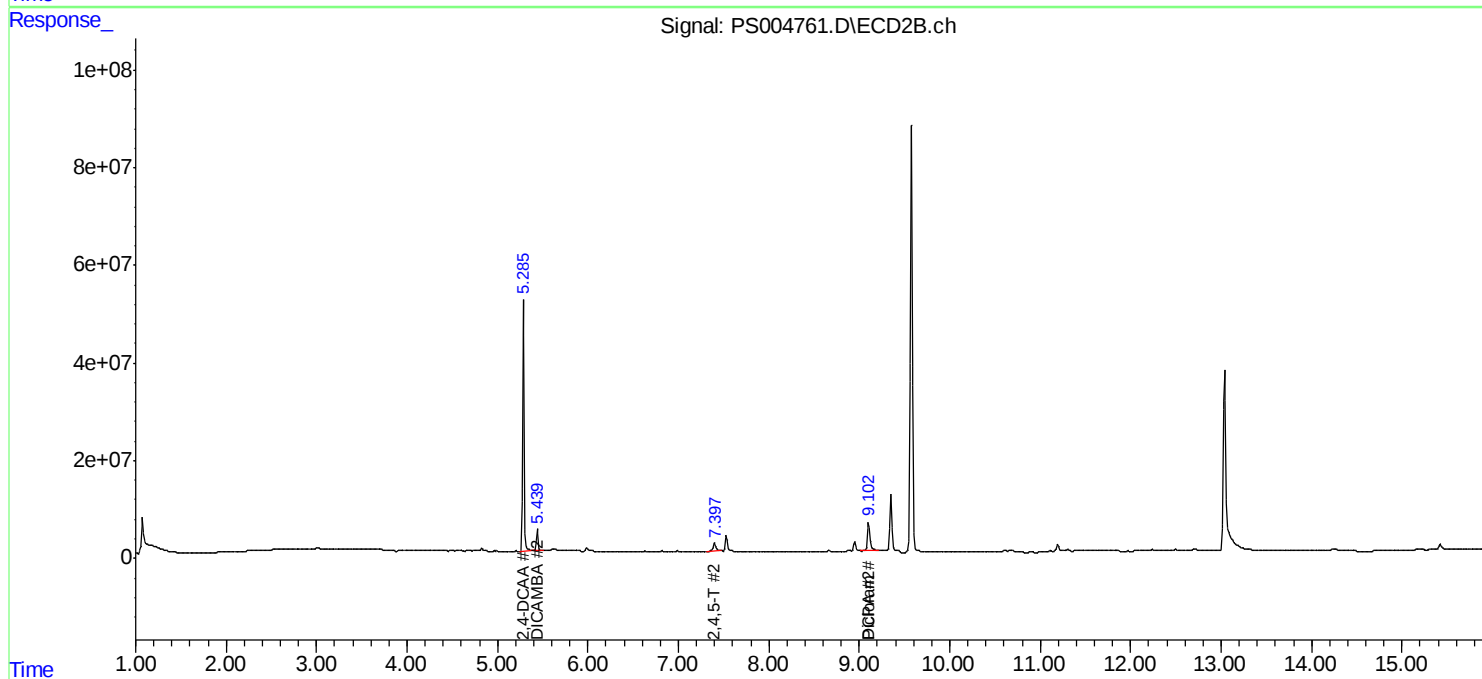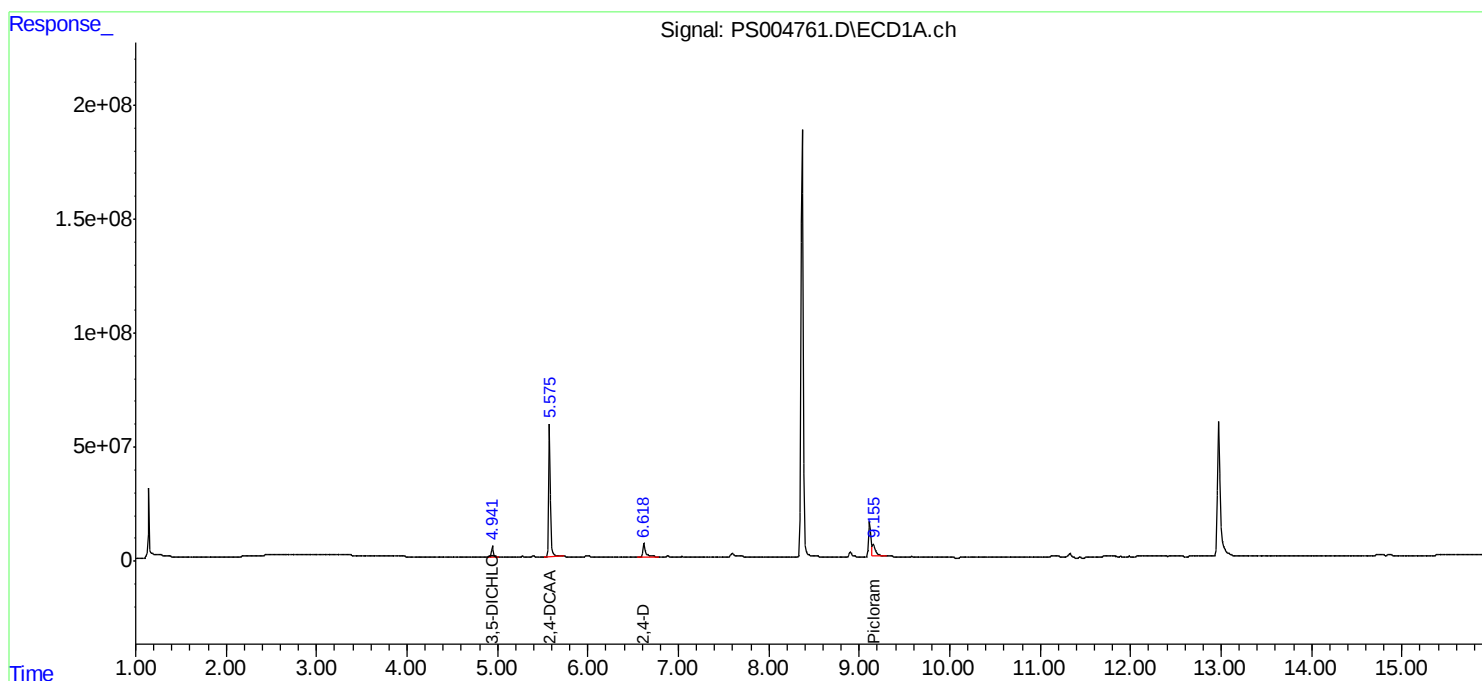


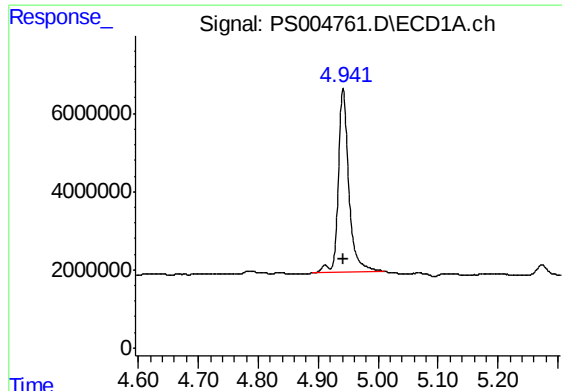

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 57858626
Conc: 33.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

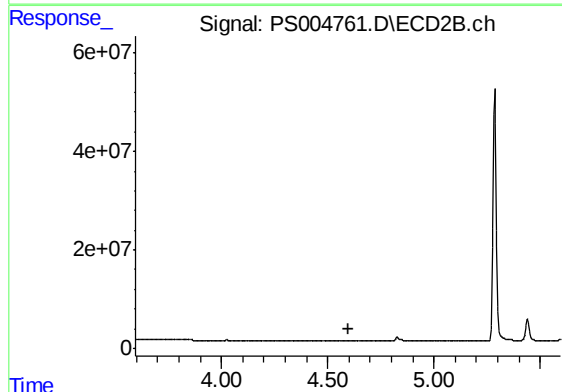


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

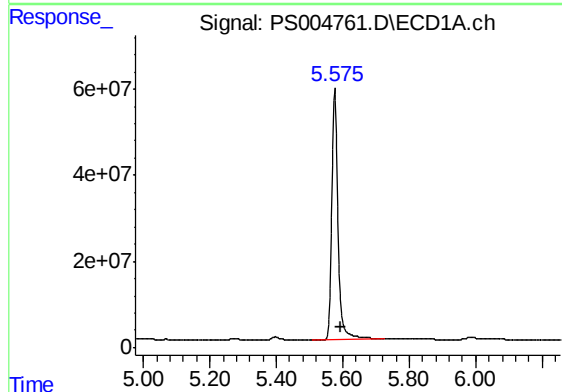


#4 2,4-DCAA

R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 754486937
Conc: 538.24 ng/ml

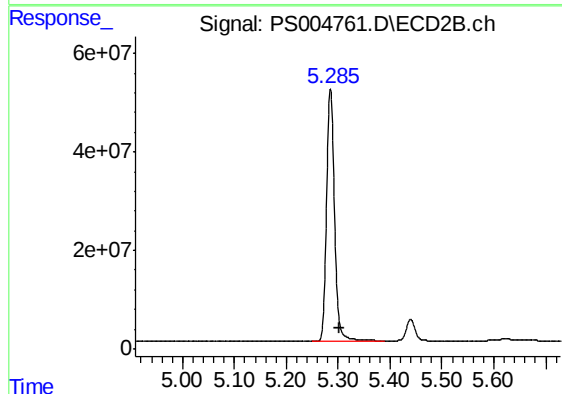

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: -0.019 min
Response: 532178176
Conc: 551.57 ng/ml

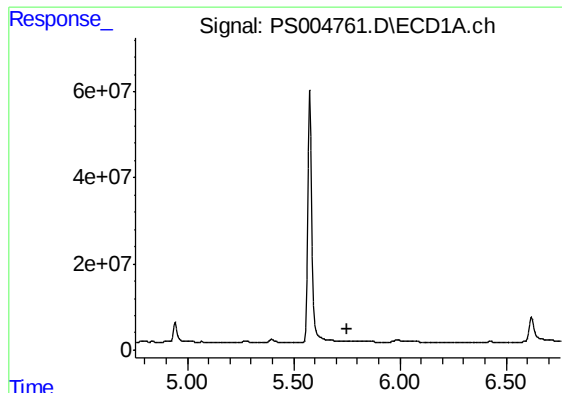

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

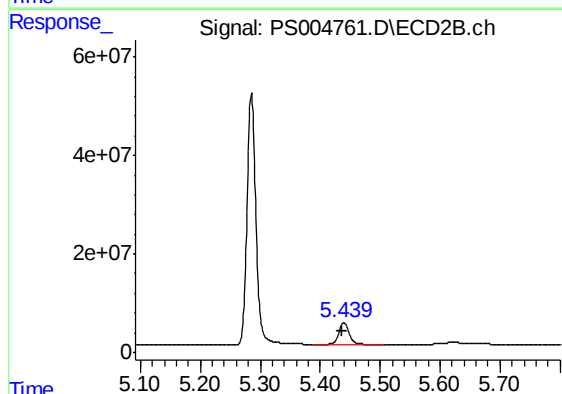


#5 DICAMBA

R.T.: 5.440 min
Delta R.T.: 0.002 min
Response: 53536619
Conc: 14.49 ng/ml

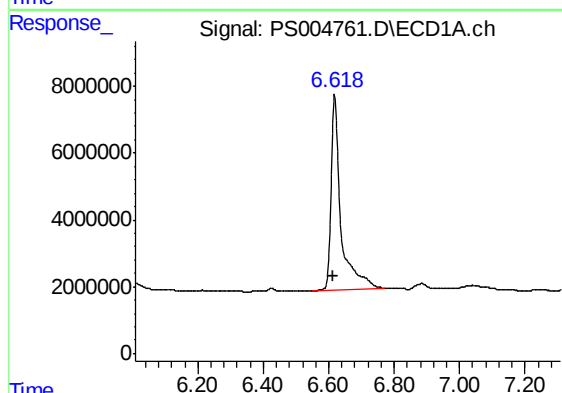


#9 2,4-D

R.T.: 6.618 min
Delta R.T.: 0.006 min
Response: 121307897
Conc: 88.68 ng/ml

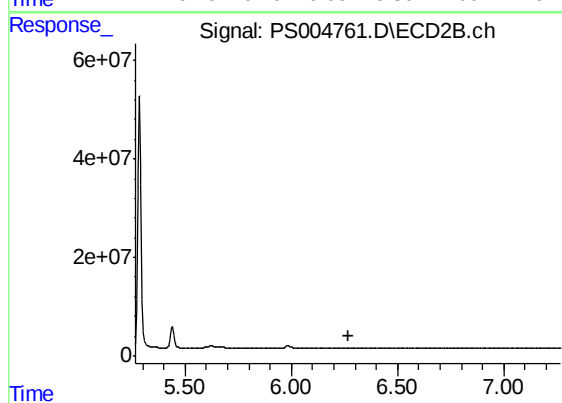

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

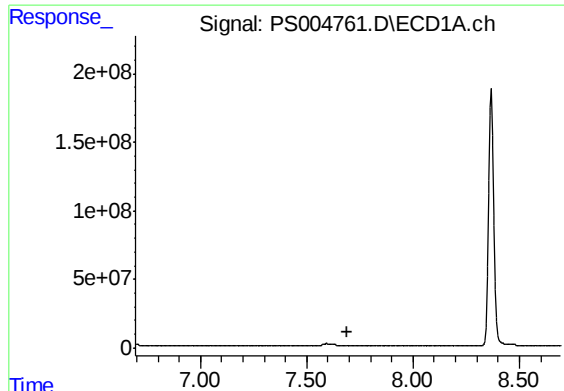

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

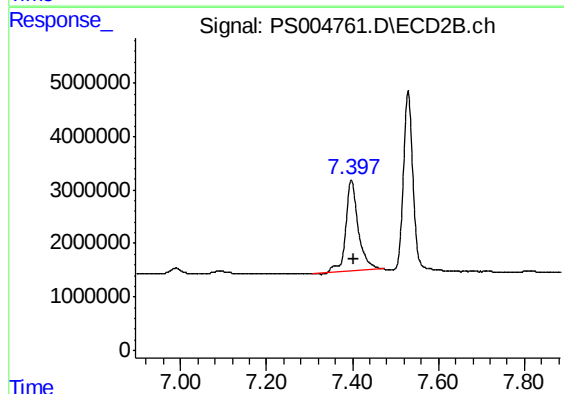


#12 2,4,5-T

R.T.: 7.398 min
Delta R.T.: -0.006 min
Response: 34379695
Conc: 7.71 ng/ml

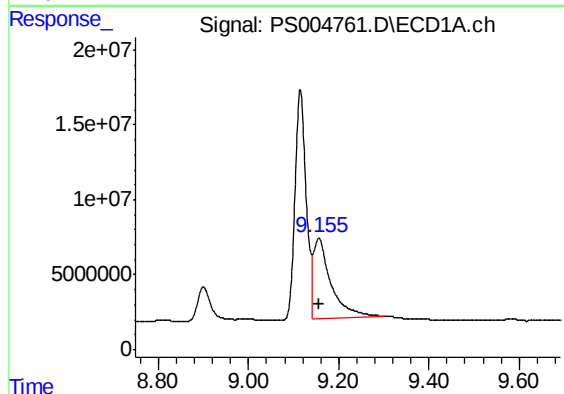


#15 Picloram

R.T.: 9.156 min
Delta R.T.: 0.000 min
Response: 143162360
Conc: 13.74 ng/ml

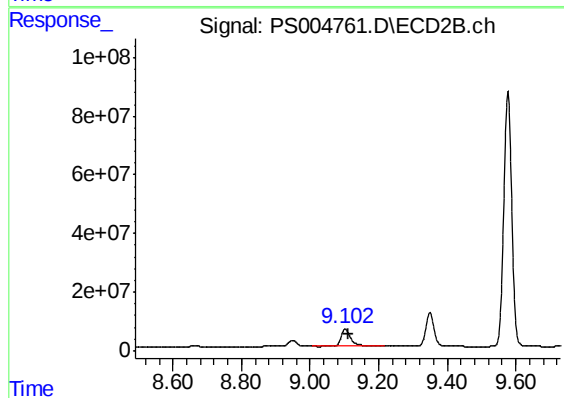

#15 Picloram


R.T.: 9.103 min
Delta R.T.: -0.010 min
Response: 116118301
Conc: 15.56 ng/ml

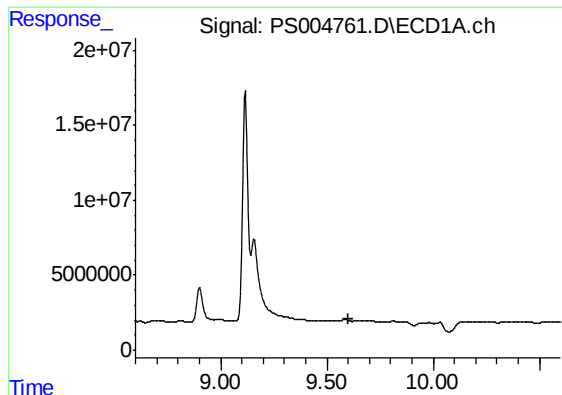

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.599 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

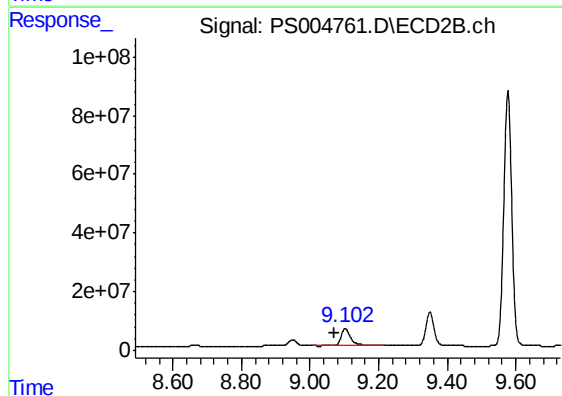

#16 DCPA

R.T.: 9.103 min
Delta R.T.: 0.030 min
Response: 116118301
Conc: 17.92 ng/ml