

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 11:54
 Operator : SM\AJ
 Sample : K2643-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-03-052319-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:52:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.286	666.4E6	476.6E6	475.371	493.949
Target Compounds							
1) T	Dalapon	2.077	0.000	42673759	0	25.743	N.D. #
2) T	3,5-DICHL...	4.995	4.604	11416065	319.2E6	6.620	259.036 #
3) T	4-Nitroph...	5.490	4.950	34533242	23022830	55.386	48.580
5) T	DICAMBA	5.715	5.393	14851785	20475522	2.797	5.543 #
6) T	MCPD	5.930	5.592	13338067	19248355	3.204	7.025 #
7) T	MCPA	0.000	5.764	0	80766143	N.D.	19.739
8) T	DICHLORPROP	0.000	5.976	0	17750708	N.D.	18.827
9) T	2,4-D	6.661	0.000	20452816	0	14.952	N.D. #
10) T	Pentachlo...	6.940	0.000	13948705	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	6.941	0	205.6E6	N.D.	39.962



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 11:54
Operator : SM\AJ
Sample : K2643-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OR-03-052319-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:52:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

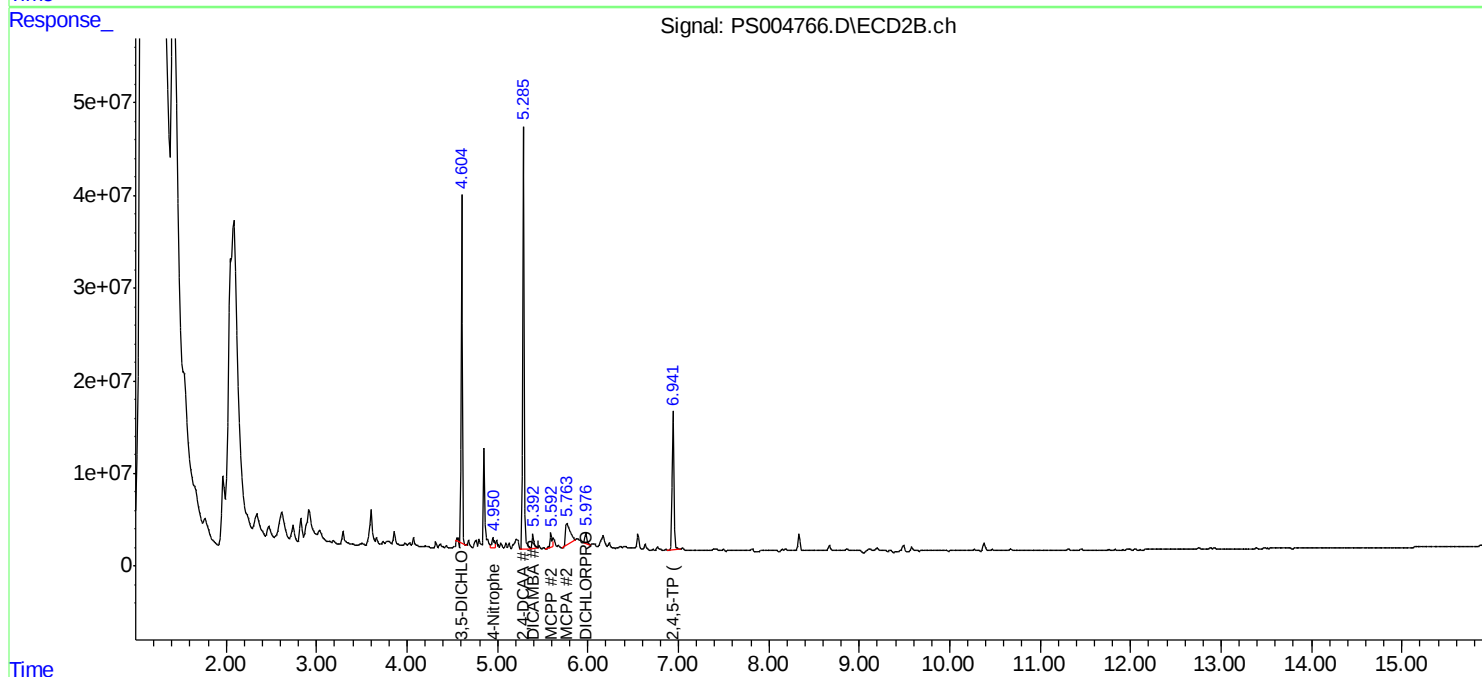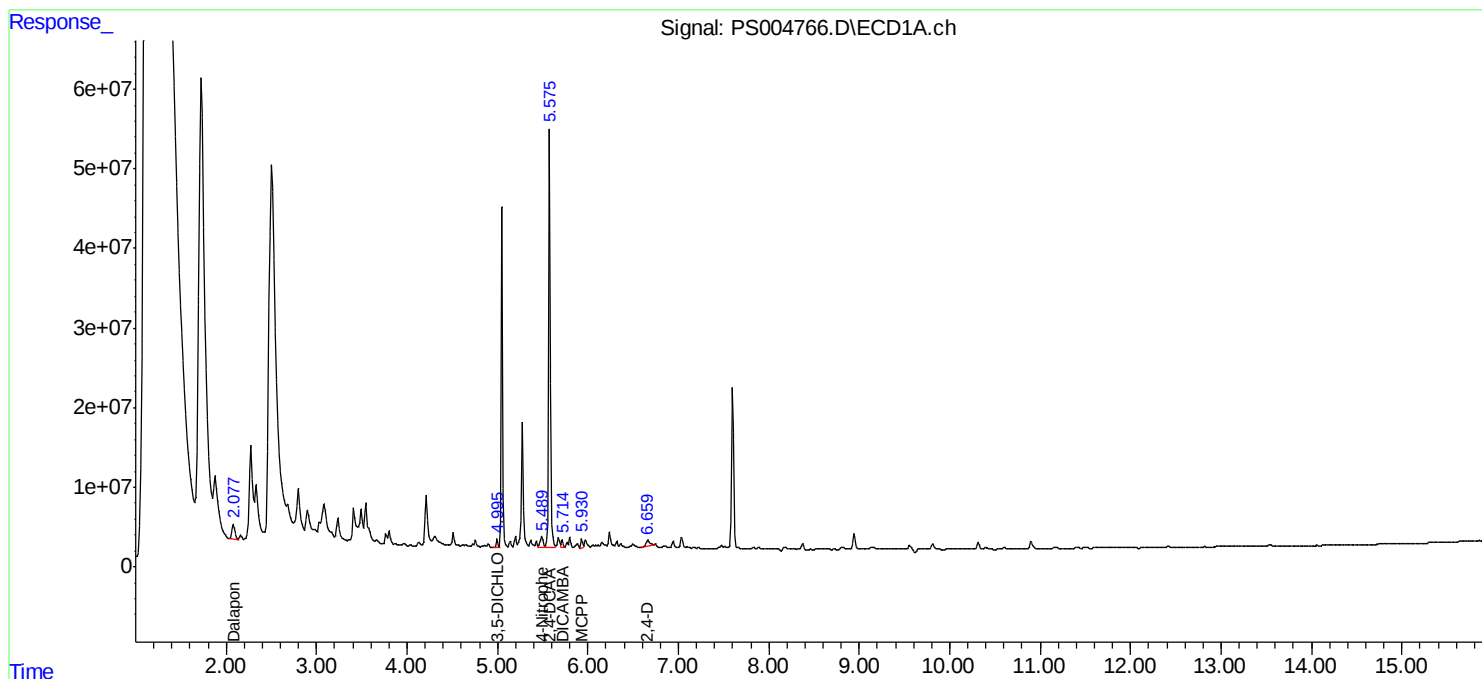


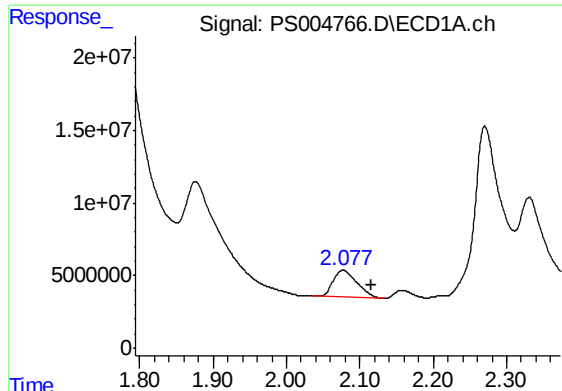

#1 Dalapon


R.T.: 2.077 min
Delta R.T.: -0.039 min
Response: 42673759
Conc: 25.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-03-052319-A

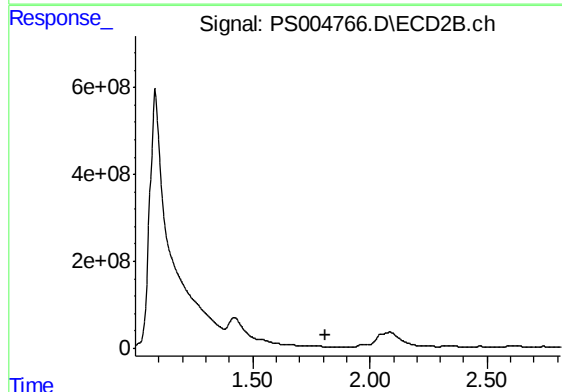


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

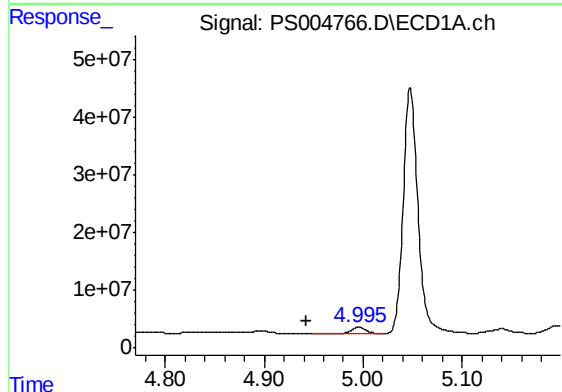


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.995 min
Delta R.T.: 0.053 min
Response: 11416065
Conc: 6.62 ng/ml

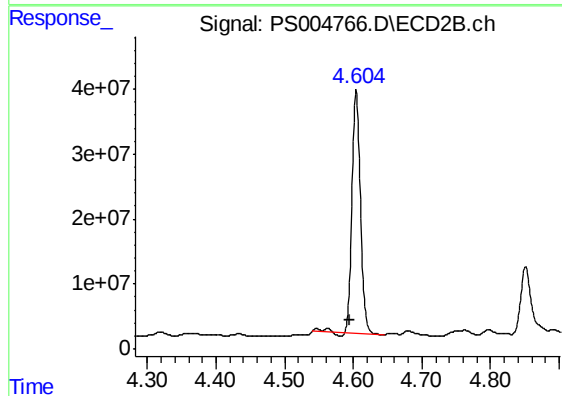

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.604 min
Delta R.T.: 0.009 min
Response: 319165042
Conc: 259.04 ng/ml

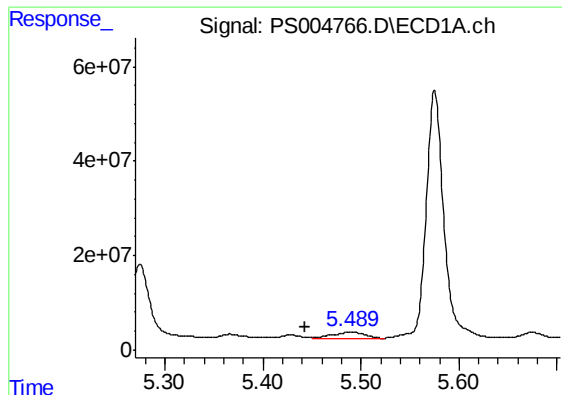

#3 4-Nitrophenol


R.T.: 5.490 min
Delta R.T.: 0.047 min
Response: 34533242
Conc: 55.39 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-03-052319-A

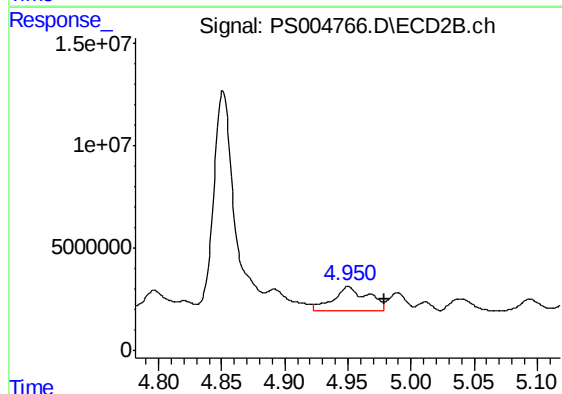


#3 4-Nitrophenol

R.T.: 4.950 min
Delta R.T.: -0.028 min
Response: 23022830
Conc: 48.58 ng/ml

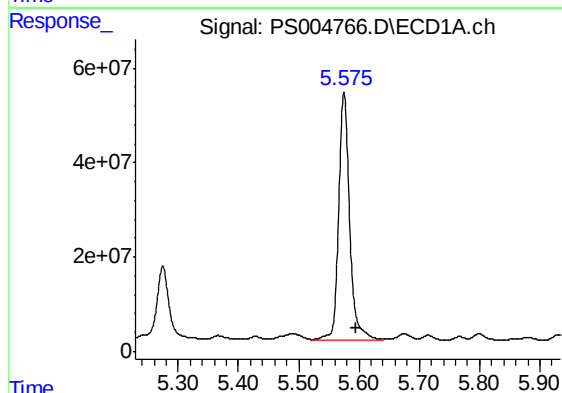


#4 2,4-DCAA

R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 666353531
Conc: 475.37 ng/ml

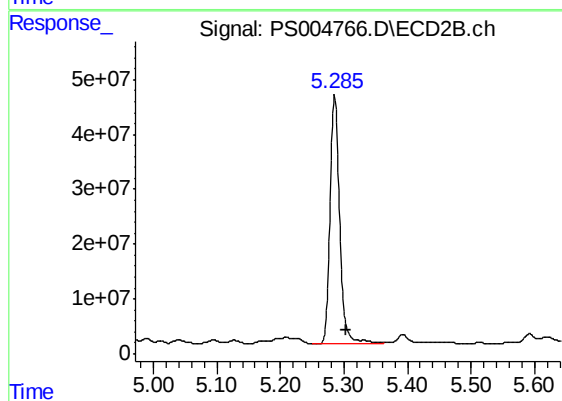

#4 2,4-DCAA


R.T.: 5.286 min
Delta R.T.: -0.018 min
Response: 476580095
Conc: 493.95 ng/ml

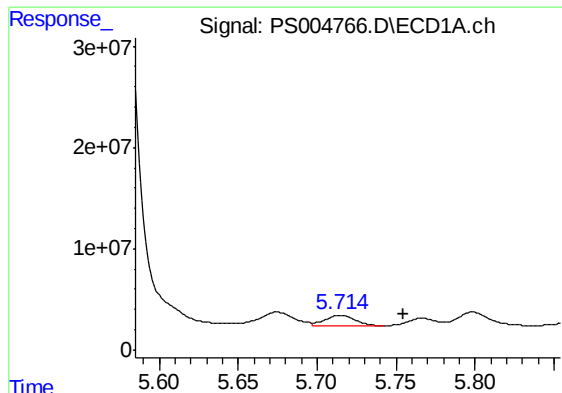

#5 DICAMBA


R.T.: 5.715 min
Delta R.T.: -0.040 min
Response: 14851785
Conc: 2.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-03-052319-A

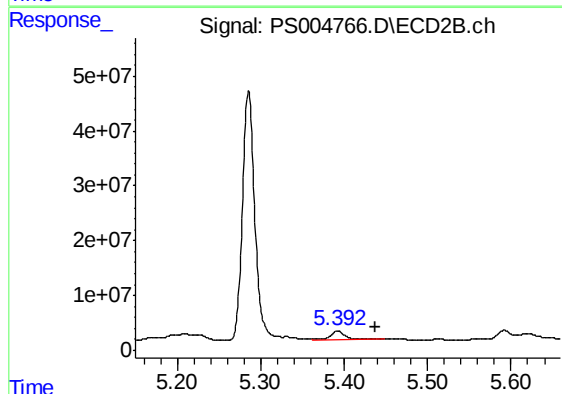


#5 DICAMBA

R.T.: 5.393 min
Delta R.T.: -0.045 min
Response: 20475522
Conc: 5.54 ng/ml

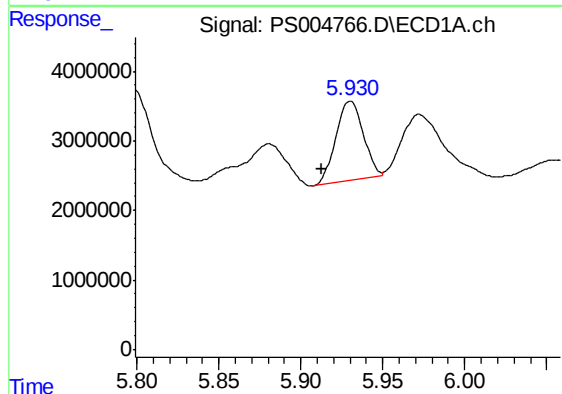


#6 MCPP

R.T.: 5.930 min
Delta R.T.: 0.018 min
Response: 13338067
Conc: 3.20 ug/ml

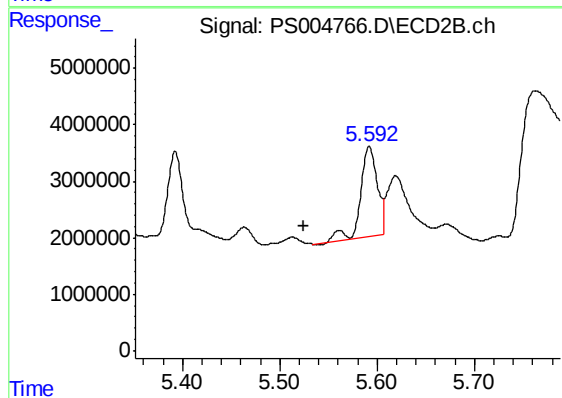

#6 MCPP


R.T.: 5.592 min
Delta R.T.: 0.068 min
Response: 19248355
Conc: 7.02 ug/ml

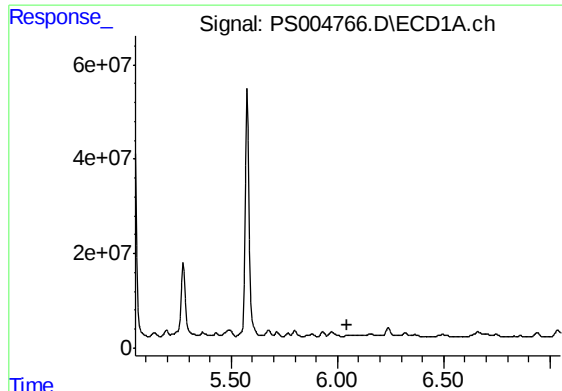

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
OR-03-052319-A

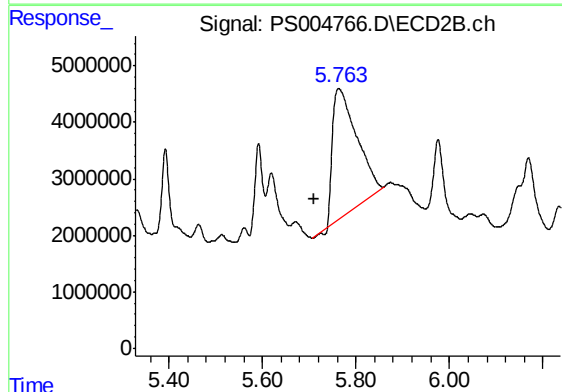


#7 MCPA

R.T.: 5.764 min
Delta R.T.: 0.054 min
Response: 80766143
Conc: 19.74 ug/ml

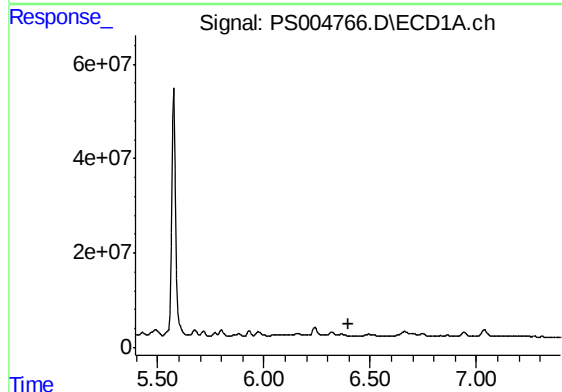


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

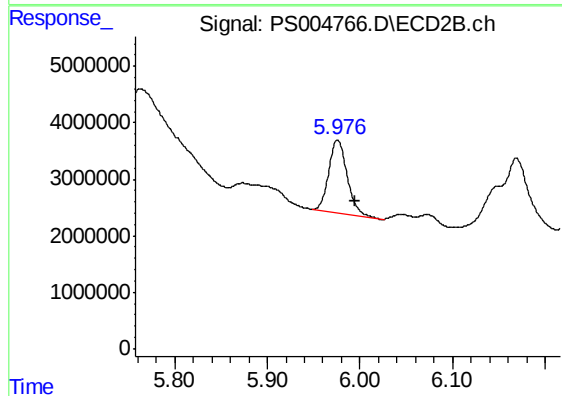

#8 DICHLORPROP


R.T.: 5.976 min
Delta R.T.: -0.018 min
Response: 17750708
Conc: 18.83 ng/ml

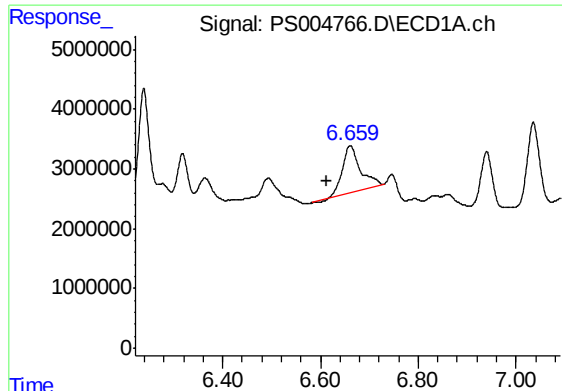

#9 2,4-D


R.T.: 6.661 min
Delta R.T.: 0.049 min
Response: 20452816
Conc: 14.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-03-052319-A

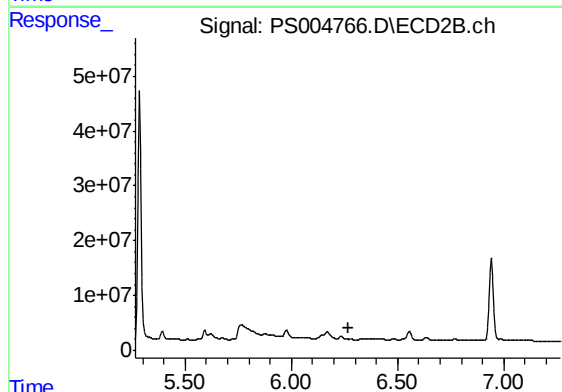


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

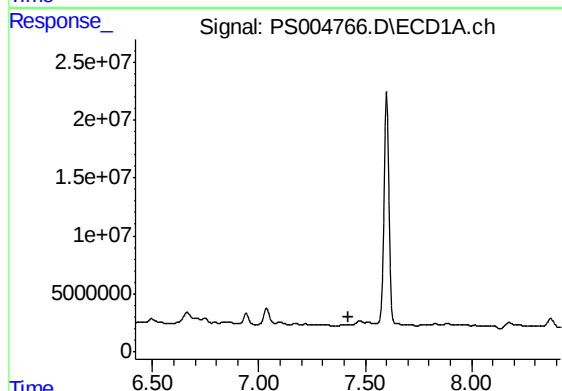

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

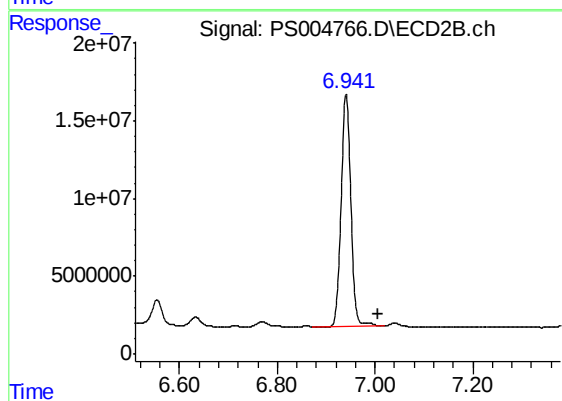

#11 2,4,5-TP (SILVEX)

R.T.: 6.941 min
Delta R.T.: -0.065 min
Response: 205619477
Conc: 39.96 ng/ml