

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 13:00
 Operator : SM\AJ
 Sample : K3023-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SSSI-0523-S-TCLP-11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:53:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.593	5.303	699.7E6	477.7E6	499.176	495.148
Target Compounds							
1) T	Dalapon	2.094	1.783	46006622	-8351391	27.754	N.D. #
2) T	3,5-DICHL...	0.000	4.580	0	17883822	N.D.	14.515
3) T	4-Nitroph...	5.446	4.967	15765916	28601713	25.286	60.351 #
5) T	DICAMBA	5.733	5.410	20792987	24517511	3.916	6.637 #
6) T	MCPD	5.948	0.000	19192016	0	4.610	N.D. #
7) T	MCPA	6.044	5.763	46150360	326.0E6	7.968	79.665 #
8) T	DICHLORPROP	0.000	5.992	0	23681575	N.D.	25.118
9) T	2,4-D	6.679	0.000	21211565	0	15.507	N.D. #
10) T	Pentachlo...	0.000	6.648	0	13802626	N.D.	1.124
11) T	2,4,5-TP ...	0.000	6.959	0	303.3E6	N.D.	58.953



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 13:00
Operator : SM\AJ
Sample : K3023-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:53:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

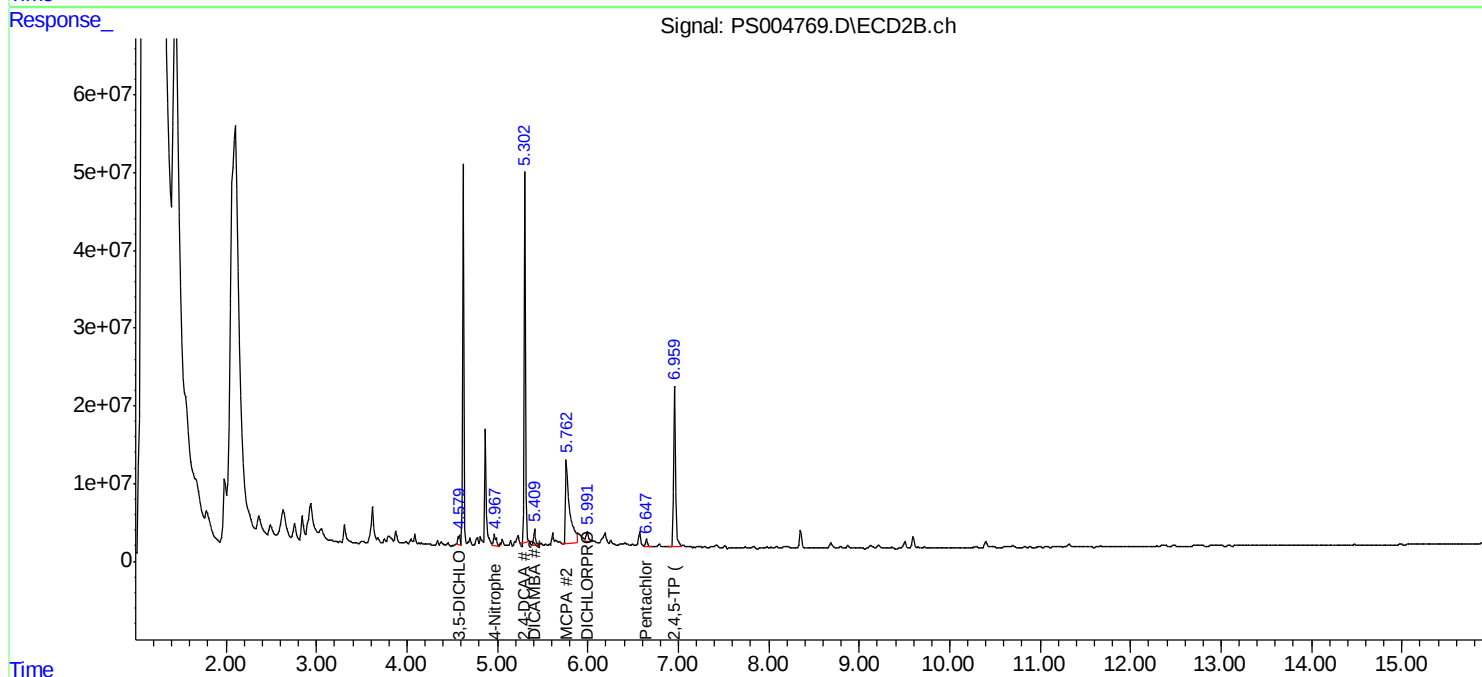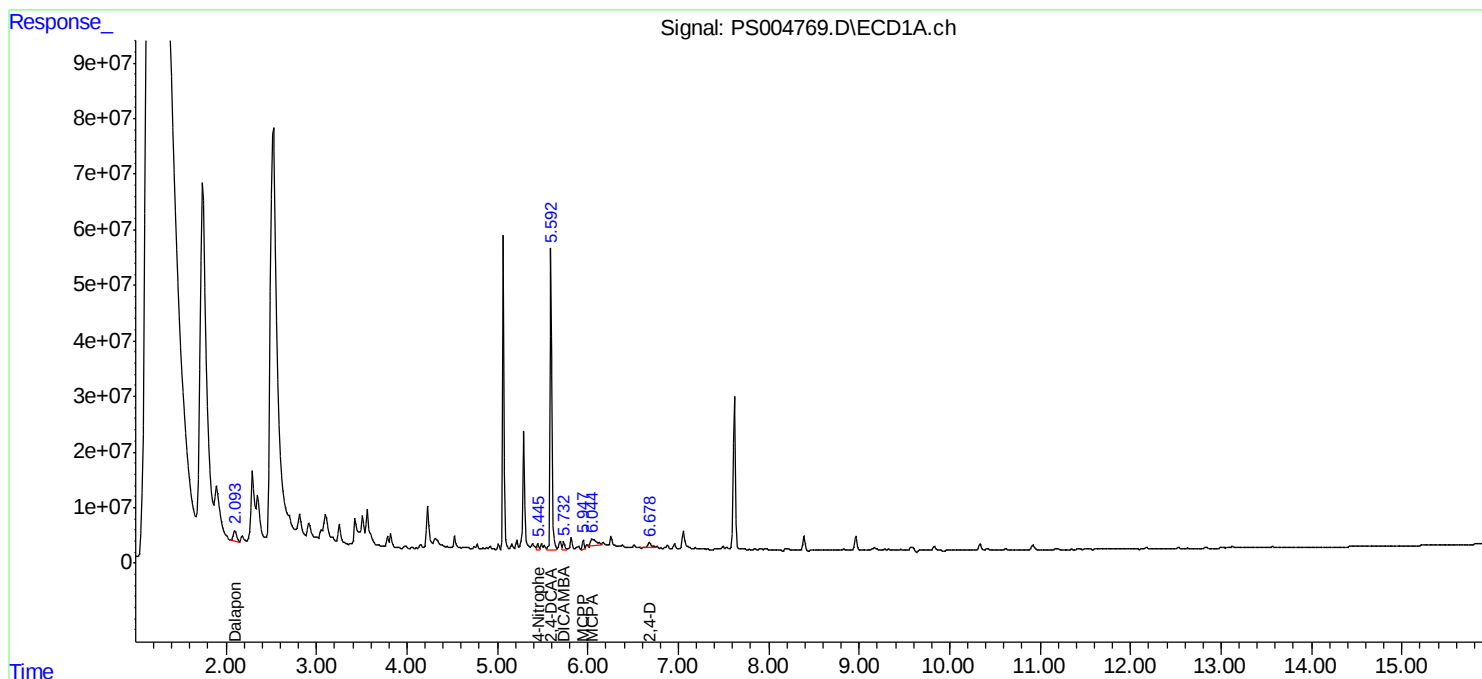


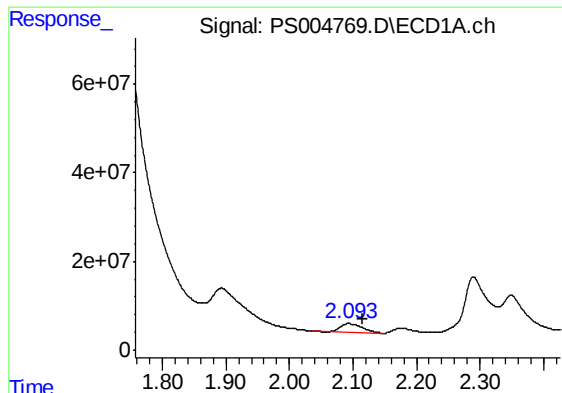

#1 Dalapon


R.T.: 2.094 min
Delta R.T.: -0.022 min
Response: 46006622
Conc: 27.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

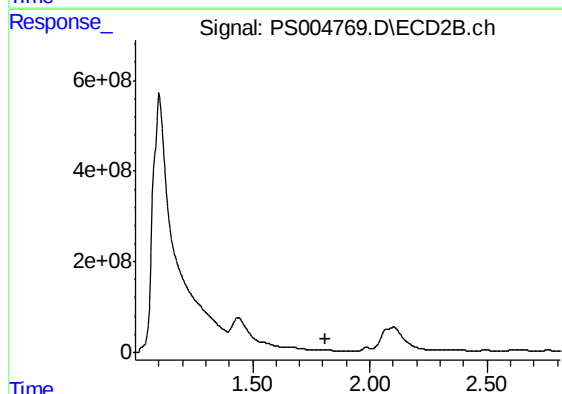


#1 Dalapon

R.T.: 1.783 min
Delta R.T.: -0.030 min
Response: -8351391
Conc: N.D.

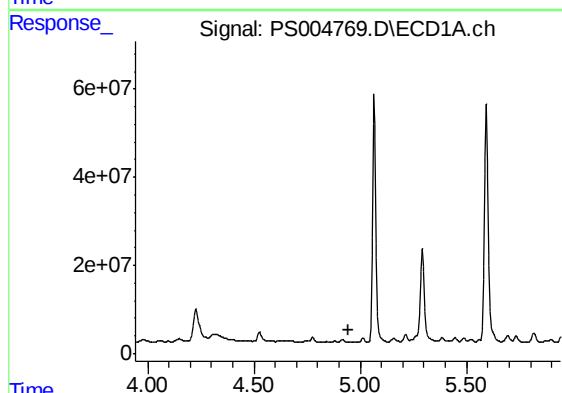


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

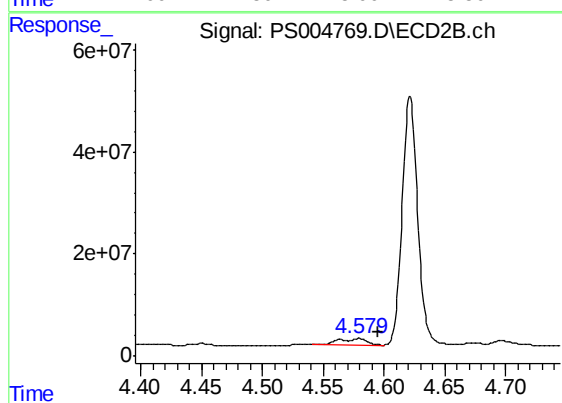

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.580 min
Delta R.T.: -0.016 min
Response: 17883822
Conc: 14.51 ng/ml

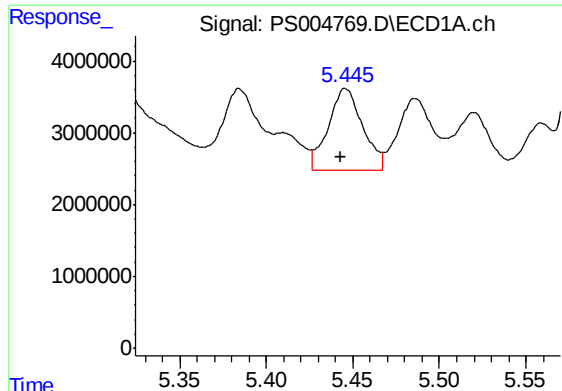

#3 4-Nitrophenol


R.T.: 5.446 min
Delta R.T.: 0.003 min
Response: 15765916
Conc: 25.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

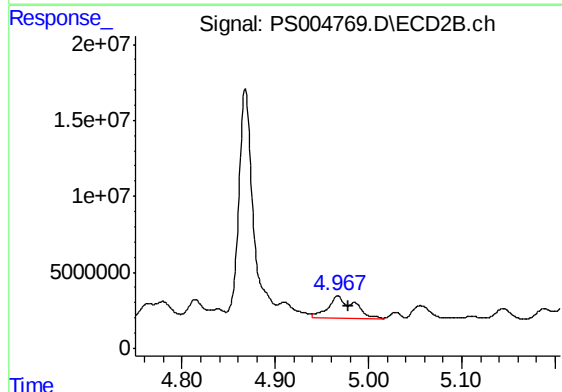


#3 4-Nitrophenol

R.T.: 4.967 min
Delta R.T.: -0.011 min
Response: 28601713
Conc: 60.35 ng/ml

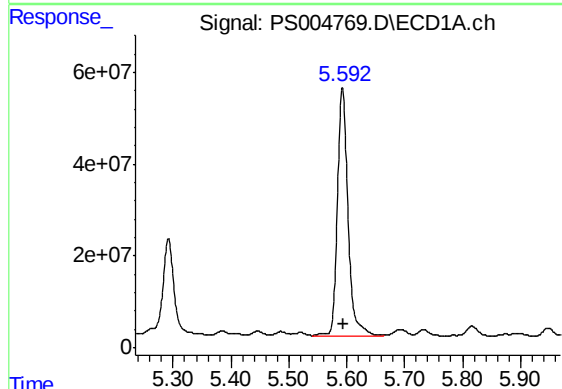


#4 2,4-DCAA

R.T.: 5.593 min
Delta R.T.: -0.002 min
Response: 699722960
Conc: 499.18 ng/ml

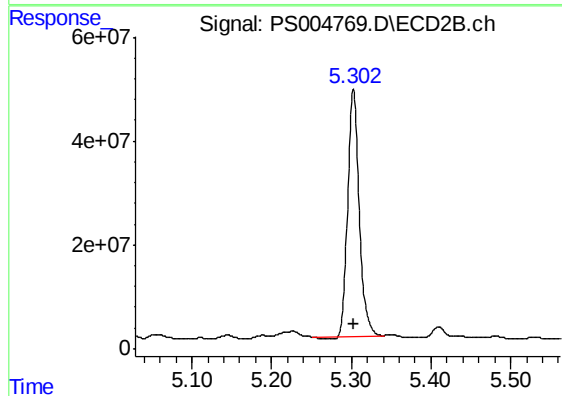

#4 2,4-DCAA


R.T.: 5.303 min
Delta R.T.: -0.001 min
Response: 477736766
Conc: 495.15 ng/ml

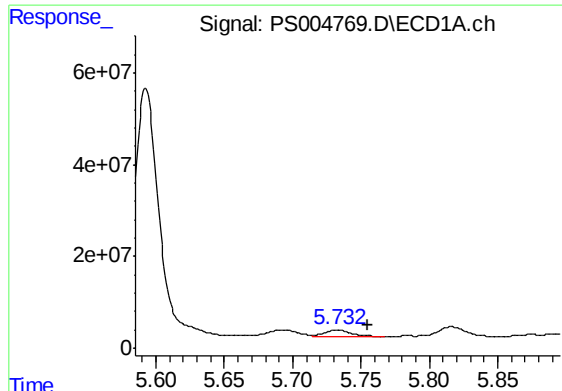

#5 DICAMBA


R.T.: 5.733 min
Delta R.T.: -0.022 min
Response: 20792987
Conc: 3.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

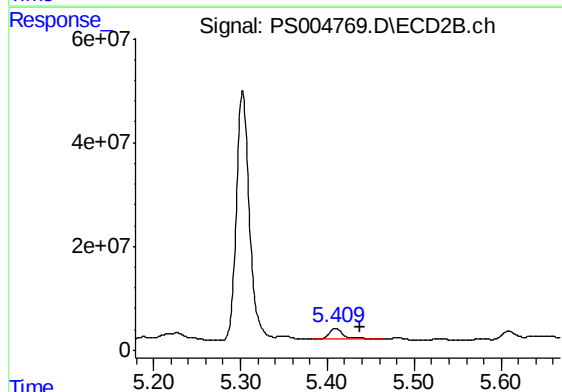


#5 DICAMBA

R.T.: 5.410 min
Delta R.T.: -0.028 min
Response: 24517511
Conc: 6.64 ng/ml

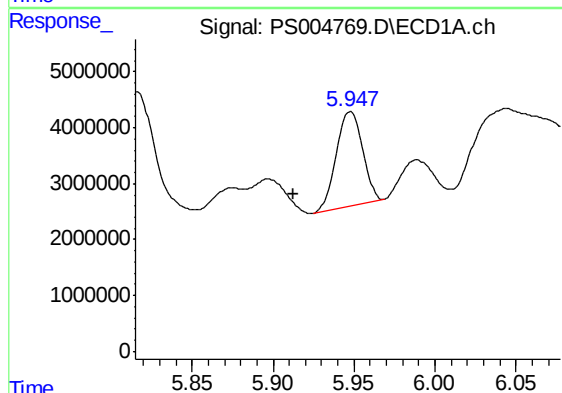


#6 MCPP

R.T.: 5.948 min
Delta R.T.: 0.035 min
Response: 19192016
Conc: 4.61 ug/ml

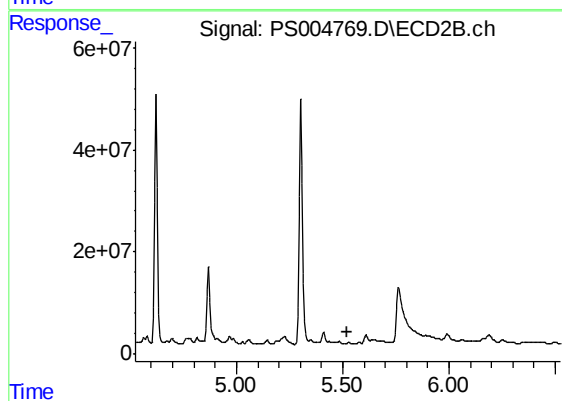

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

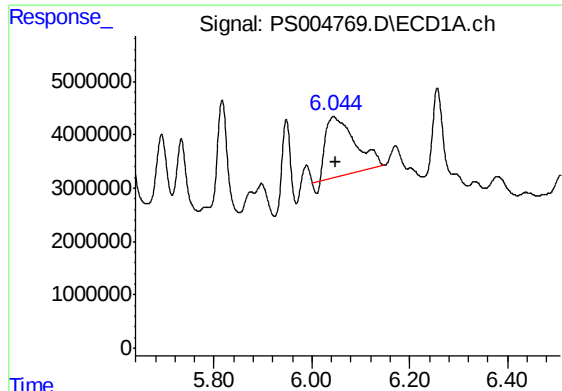

#7 MCPA


R.T.: 6.044 min
Delta R.T.: -0.005 min
Response: 46150360
Conc: 7.97 ug/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

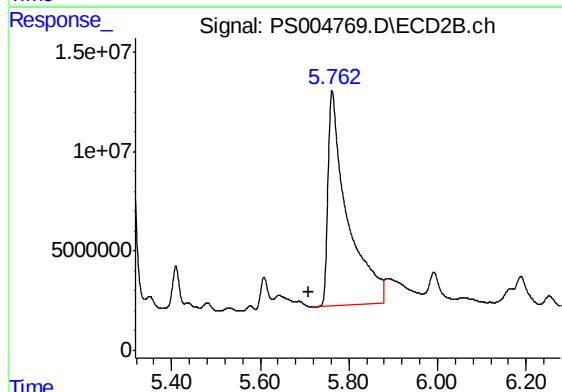


#7 MCPA

R.T.: 5.763 min
Delta R.T.: 0.054 min
Response: 325961598
Conc: 79.67 ug/ml

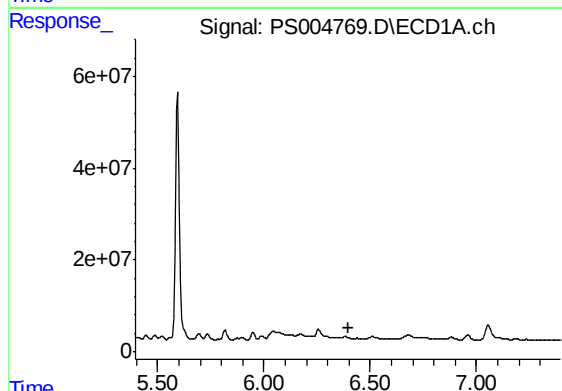


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

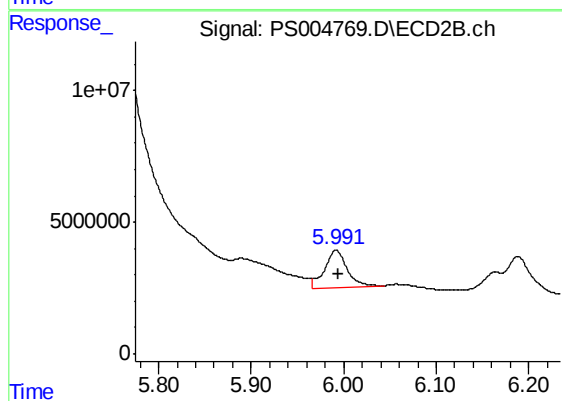

#8 DICHLORPROP


R.T.: 5.992 min
Delta R.T.: -0.002 min
Response: 23681575
Conc: 25.12 ng/ml

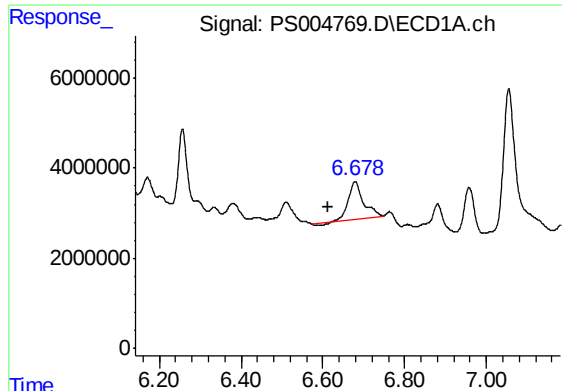

#9 2,4-D


R.T.: 6.679 min
Delta R.T.: 0.067 min
Response: 21211565
Conc: 15.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

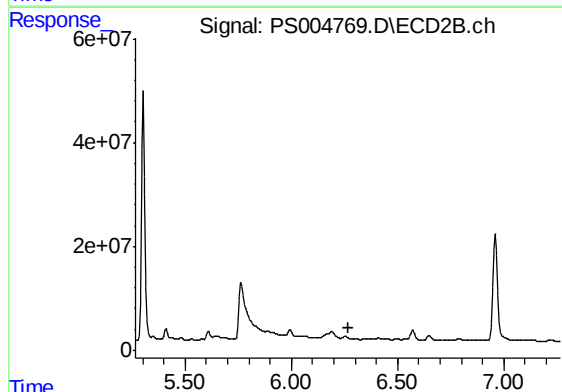


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

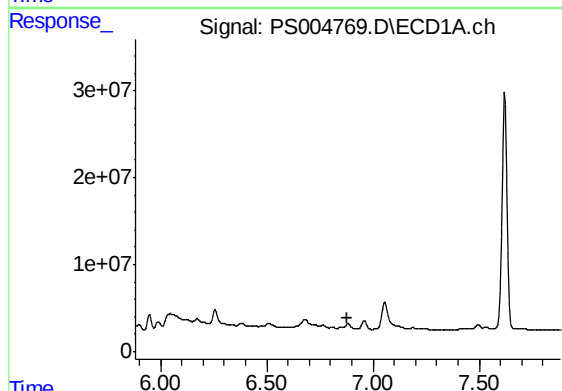


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.882 min
Response: 0
Conc: N.D.

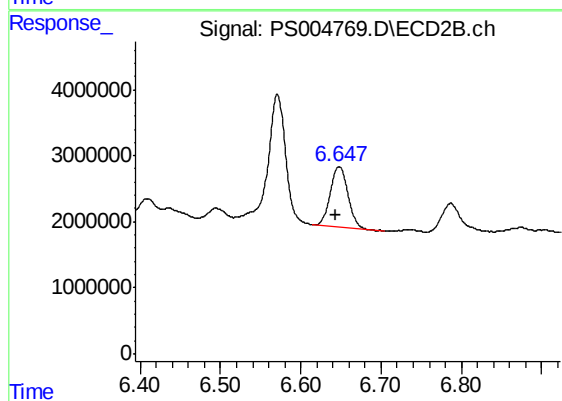

#10 Pentachlorophenol


R.T.: 6.648 min
Delta R.T.: 0.004 min
Response: 13802626
Conc: 1.12 ng/ml

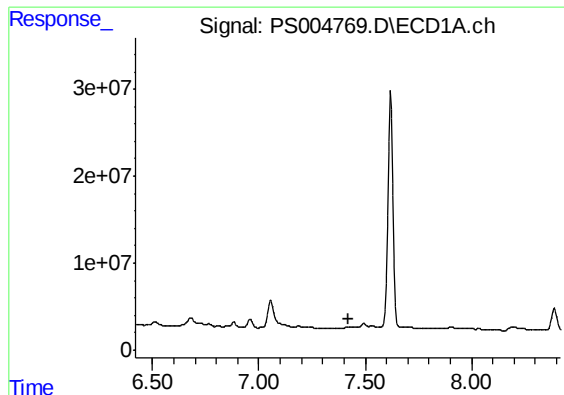

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

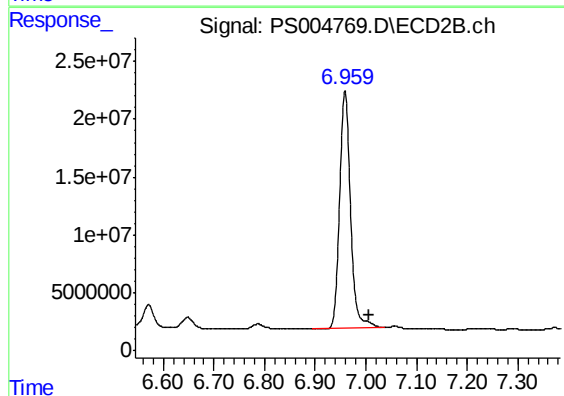

#11 2,4,5-TP (SILVEX)

R.T.: 6.959 min
Delta R.T.: -0.047 min
Response: 303333653
Conc: 58.95 ng/ml