

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004771.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 13:44
 Operator : SM\AJ
 Sample : K3026-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-5-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:53:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.590	5.285	579.5E6	417.1E6	413.425	432.271
Target Compounds							
1) T	Dalapon	2.093	0.000	36393866	0	21.955	N.D. #
2) T	3,5-DICHL...	5.011	4.604	13594771	333.7E6	7.883	270.819 #
3) T	4-Nitroph...	5.382	4.950	20743424	24088546	33.269	50.828 #
5) T	DICAMBA	5.730	5.392	16144360	16419430	3.041	4.445 #
6) T	MCP	5.946	5.592	16490592	11682451	3.961	4.264
7) T	MCPA	0.000	5.751	0	230.2E6	N.D.	56.260
8) T	DICHLORPROP	0.000	5.975	0	16331292	N.D.	17.322
9) T	2,4-D	6.676	0.000	22300316	0	16.302	N.D. #
11) T	2,4,5-TP ...	0.000	6.941	0	190.5E6	N.D.	37.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004771.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 13:44
Operator : SM\AJ
Sample : K3026-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-5-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:53:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

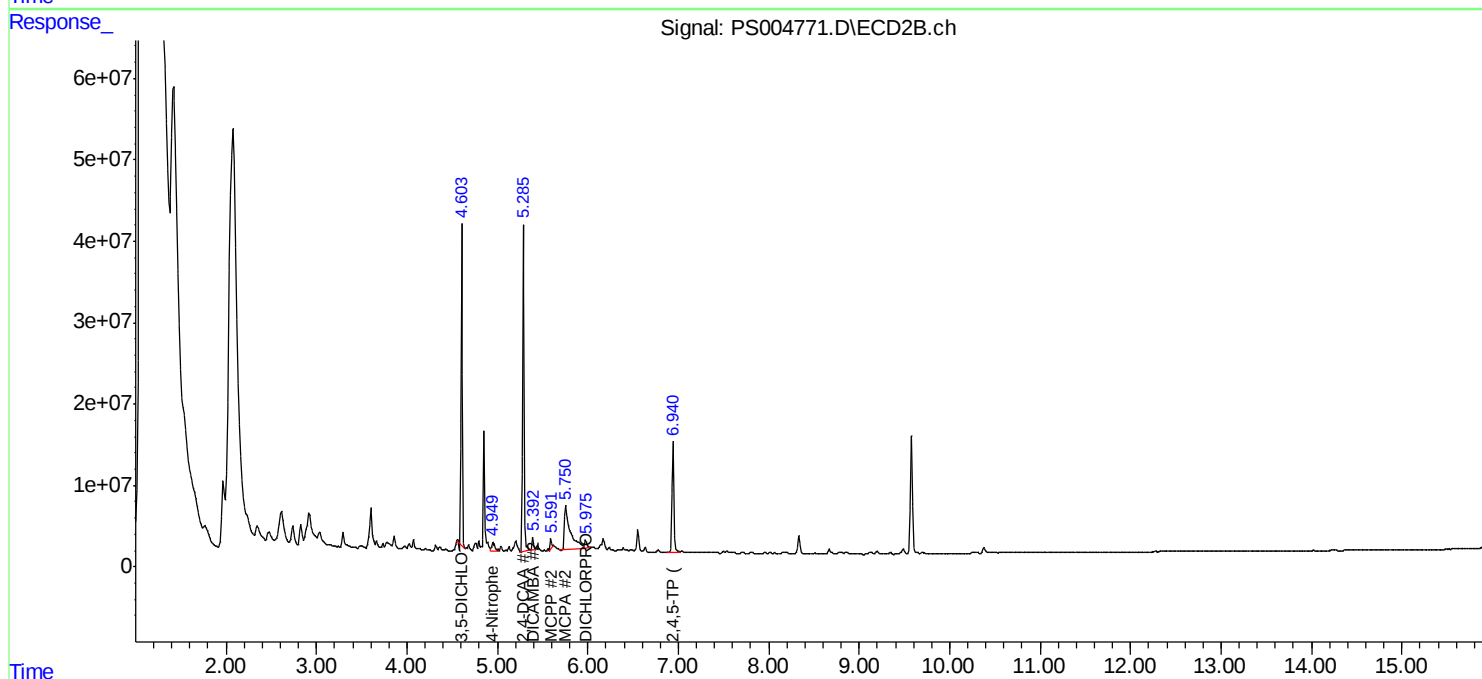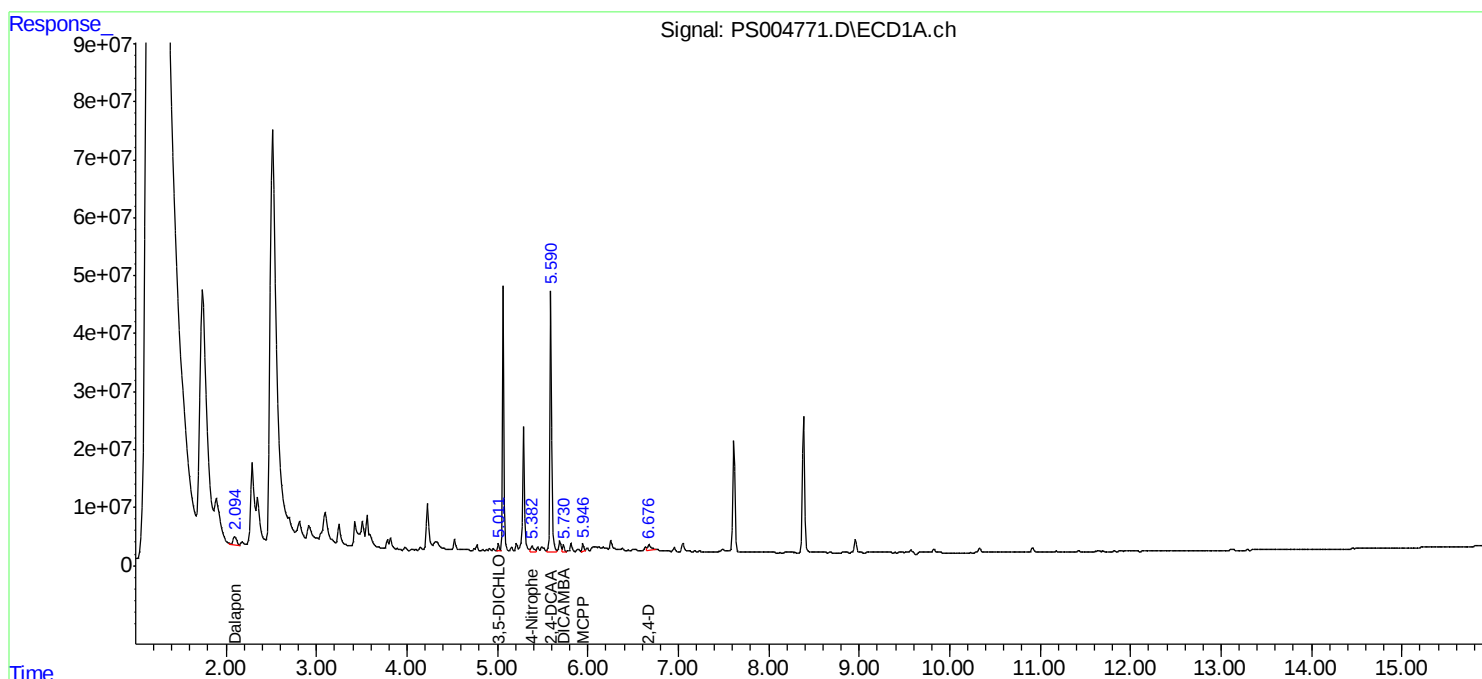


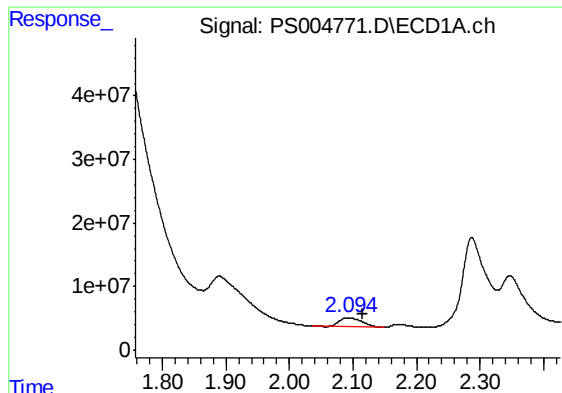

#1 Dalapon


R.T.: 2.093 min
Delta R.T.: -0.023 min
Response: 36393866
Conc: 21.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-S

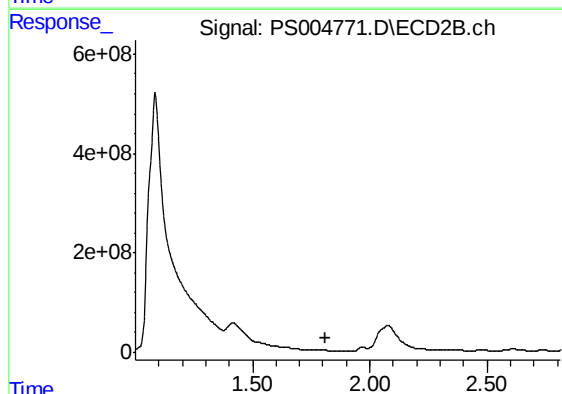


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

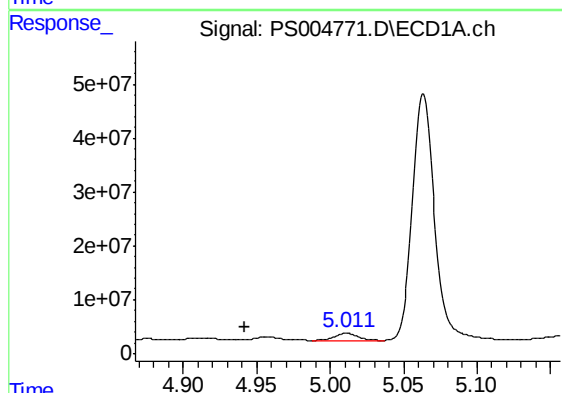


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.011 min
Delta R.T.: 0.069 min
Response: 13594771
Conc: 7.88 ng/ml

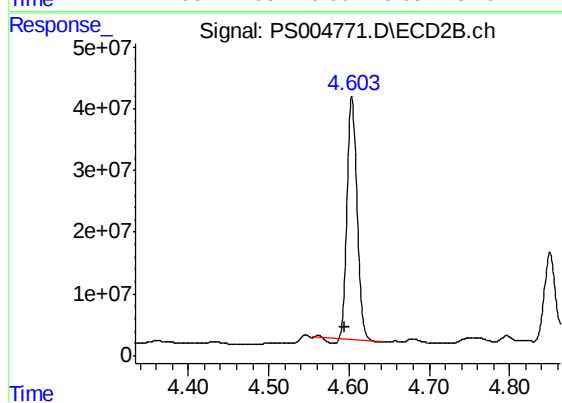

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.604 min
Delta R.T.: 0.008 min
Response: 333683349
Conc: 270.82 ng/ml

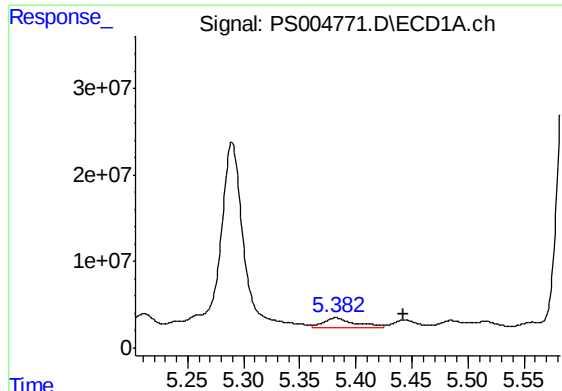

#3 4-Nitrophenol


R.T.: 5.382 min
Delta R.T.: -0.060 min
Response: 20743424
Conc: 33.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-S

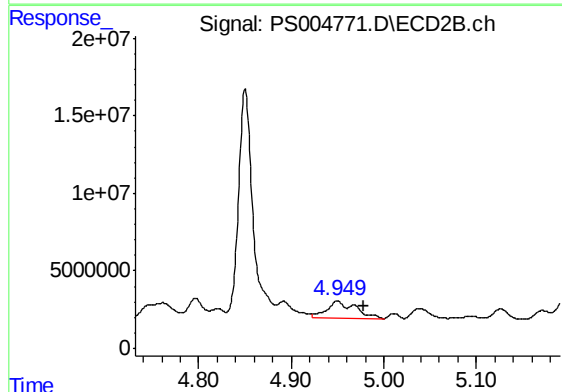


#3 4-Nitrophenol

R.T.: 4.950 min
Delta R.T.: -0.029 min
Response: 24088546
Conc: 50.83 ng/ml

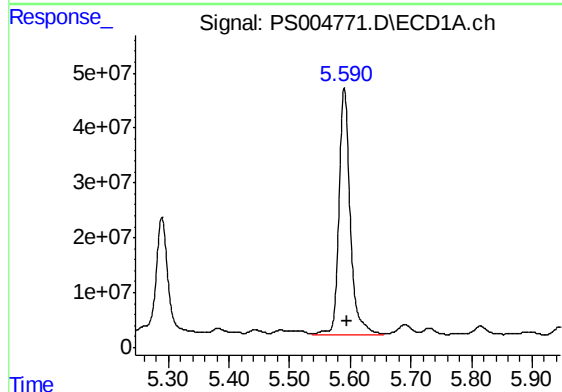


#4 2,4-DCAA

R.T.: 5.590 min
Delta R.T.: -0.005 min
Response: 579520932
Conc: 413.42 ng/ml

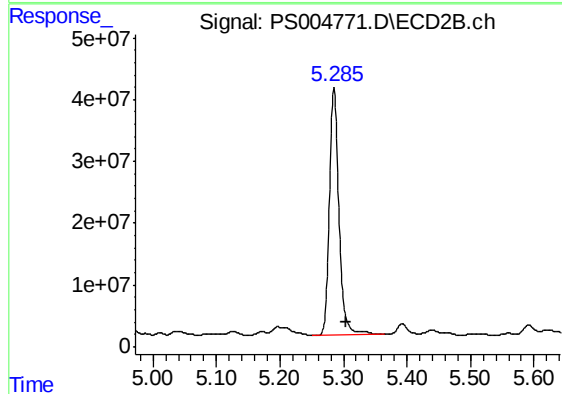

#4 2,4-DCAA


R.T.: 5.285 min
Delta R.T.: -0.018 min
Response: 417070938
Conc: 432.27 ng/ml

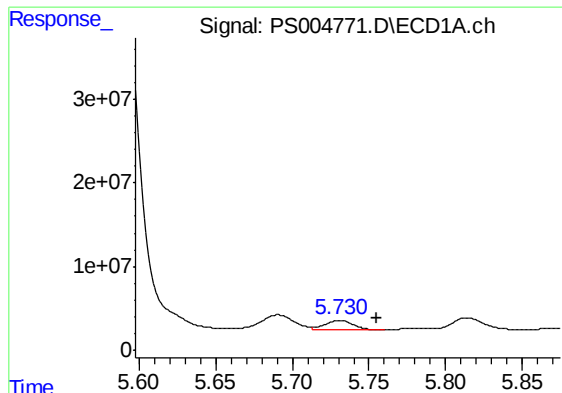

#5 DICAMBA


R.T.: 5.730 min
Delta R.T.: -0.025 min
Response: 16144360
Conc: 3.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-S

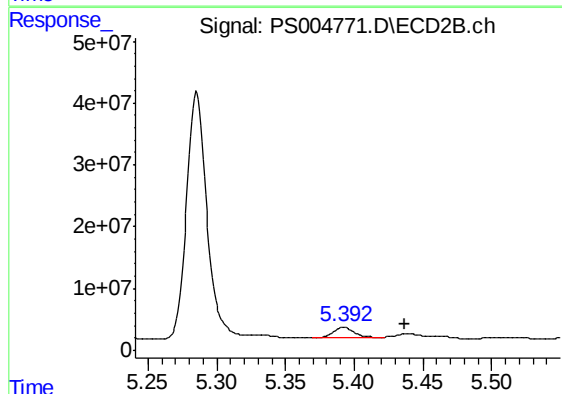


#5 DICAMBA

R.T.: 5.392 min
Delta R.T.: -0.045 min
Response: 16419430
Conc: 4.44 ng/ml

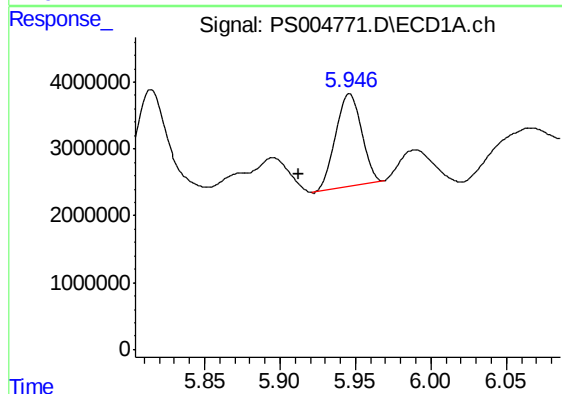


#6 MCPP

R.T.: 5.946 min
Delta R.T.: 0.033 min
Response: 16490592
Conc: 3.96 ug/ml

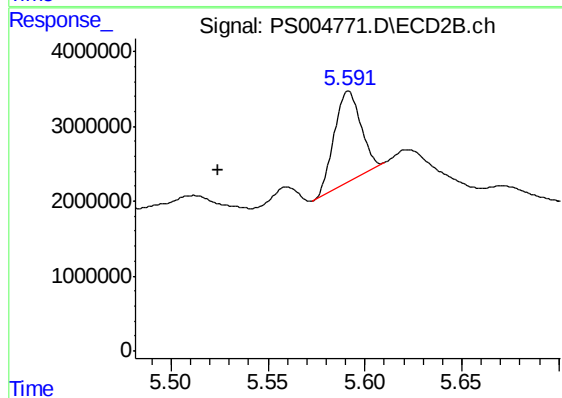

#6 MCPP


R.T.: 5.592 min
Delta R.T.: 0.067 min
Response: 11682451
Conc: 4.26 ug/ml

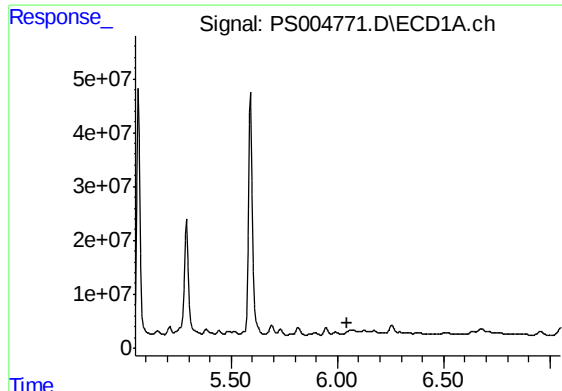

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5-S

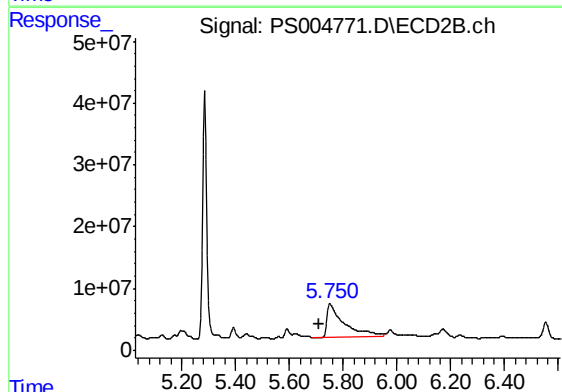


#7 MCPA

R.T.: 5.751 min
Delta R.T.: 0.042 min
Response: 230194440
Conc: 56.26 ug/ml

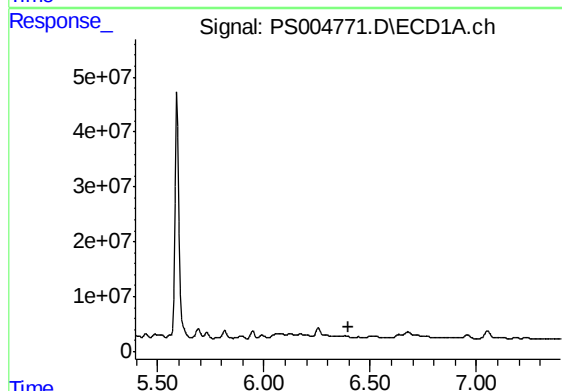


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

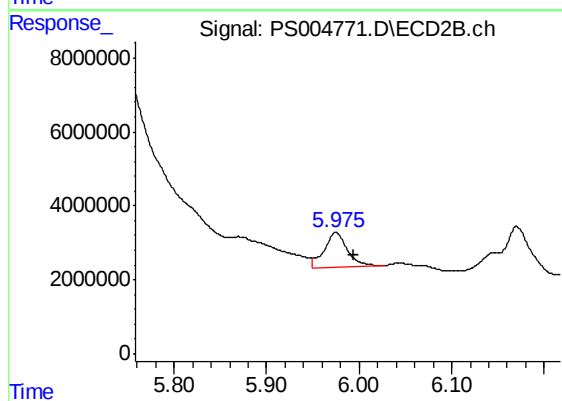

#8 DICHLORPROP


R.T.: 5.975 min
Delta R.T.: -0.019 min
Response: 16331292
Conc: 17.32 ng/ml

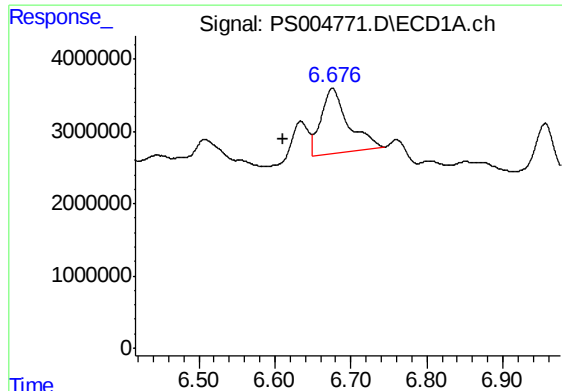

#9 2,4-D


R.T.: 6.676 min
Delta R.T.: 0.064 min
Response: 22300316
Conc: 16.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-S

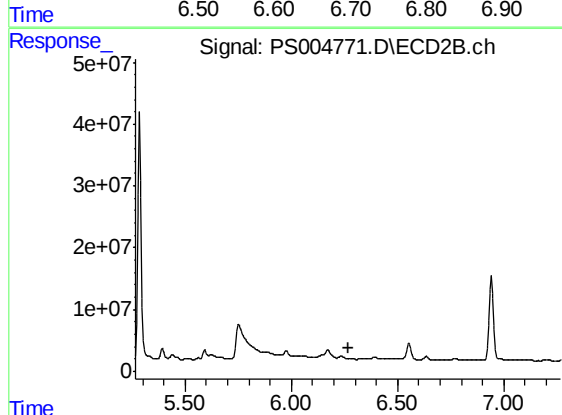


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

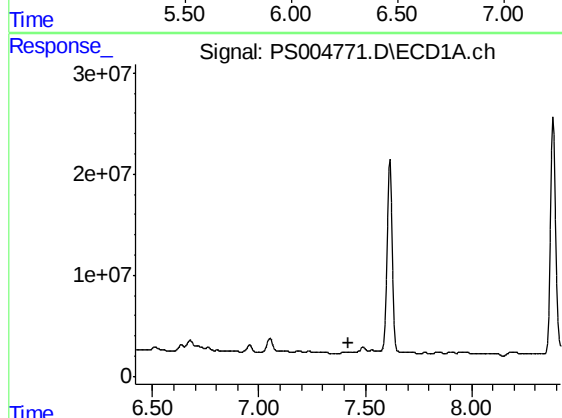

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

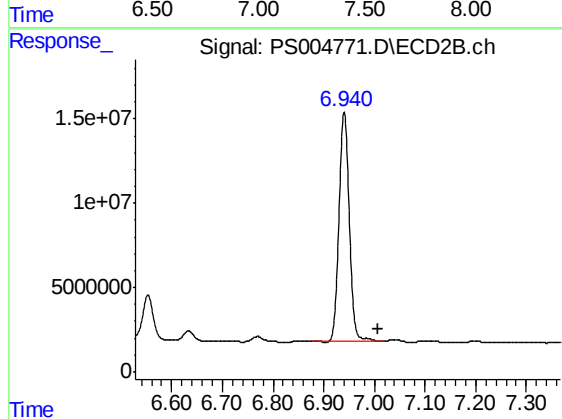

#11 2,4,5-TP (SILVEX)

R.T.: 6.941 min
Delta R.T.: -0.066 min
Response: 190453433
Conc: 37.01 ng/ml