

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 14:06
 Operator : SM\AJ
 Sample : K3026-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-5-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:53:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.574	5.284	561.5E6	402.4E6	400.568	417.030
Target Compounds							
1) T	Dalapon	2.075	0.000	33352105	0	20.120	N.D. #
2) T	3,5-DICHL...	0.000	4.603	0	305.6E6	N.D.	248.062
3) T	4-Nitroph...	5.467	4.949	18572245	23371016	29.787	49.314 #
5) T	DICAMBA	5.798	5.391	21975774	12781702	4.139	3.460
6) T	MCPD	5.930	5.590	12597353	8377762	3.026	3.058
7) T	MCPA	0.000	5.765	0	128.5E6	N.D.	31.397
8) T	DICHLORPROP	0.000	5.974	0	13997853	N.D.	14.847
9) T	2,4-D	6.616	0.000	11356992	0	8.302	N.D. #
11) T	2,4,5-TP ...	0.000	6.939	0	183.7E6	N.D.	35.705



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 14:06
Operator : SM\AJ
Sample : K3026-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-5-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:53:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

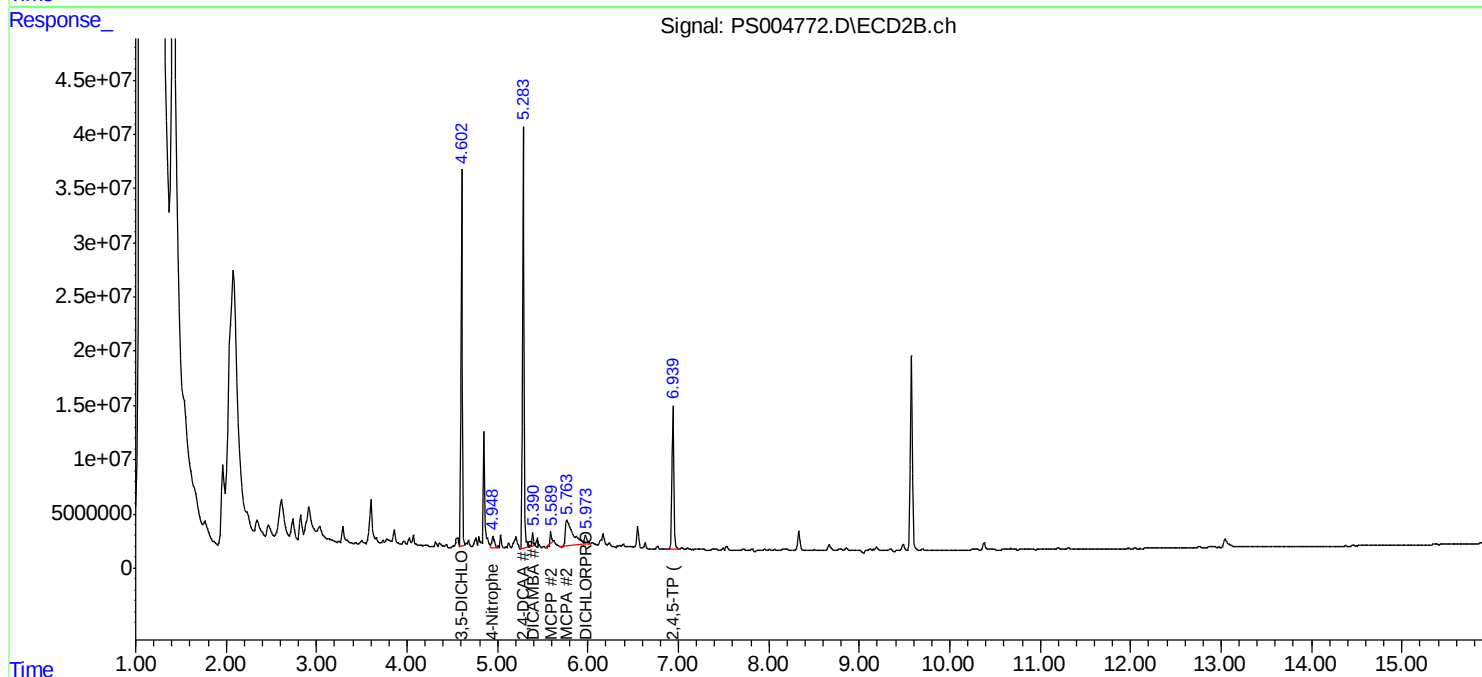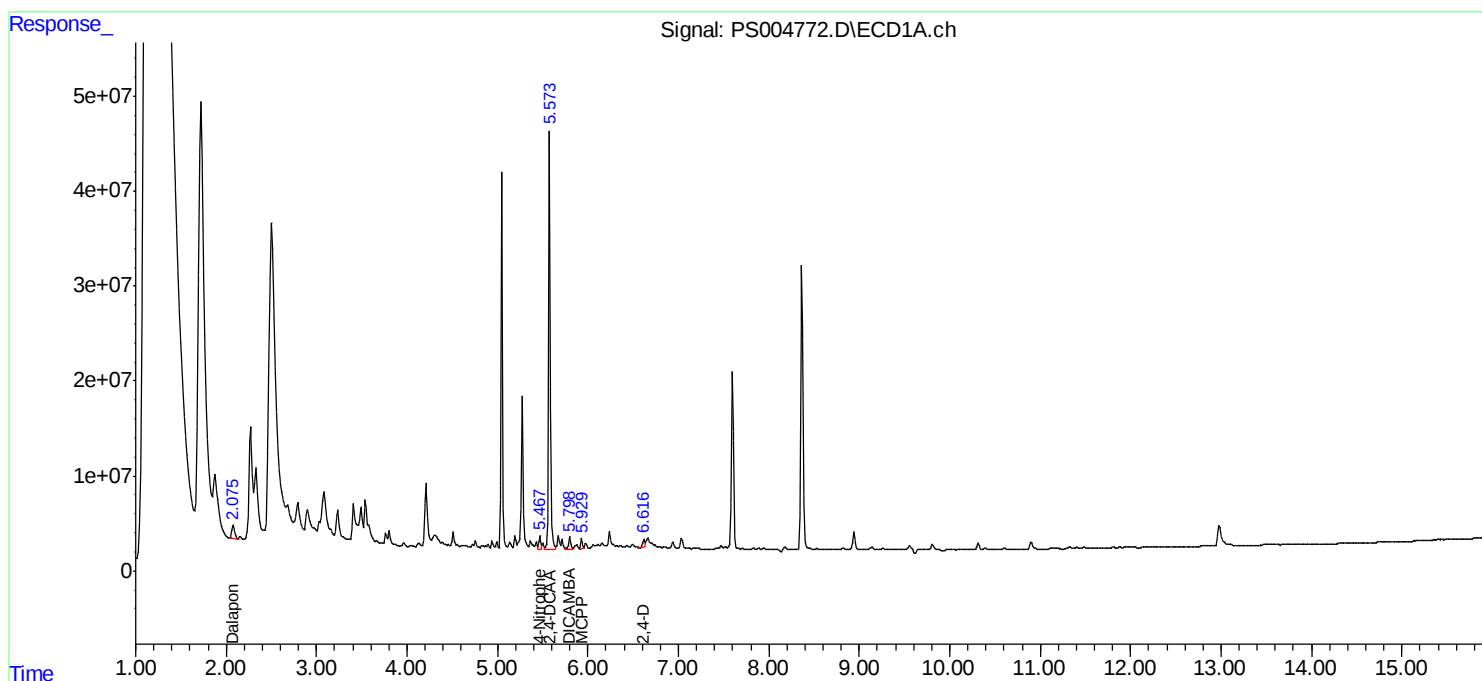


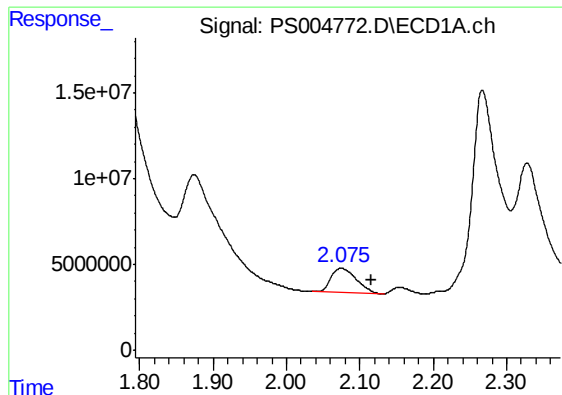

#1 Dalapon


R.T.: 2.075 min
Delta R.T.: -0.041 min
Response: 33352105
Conc: 20.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-D

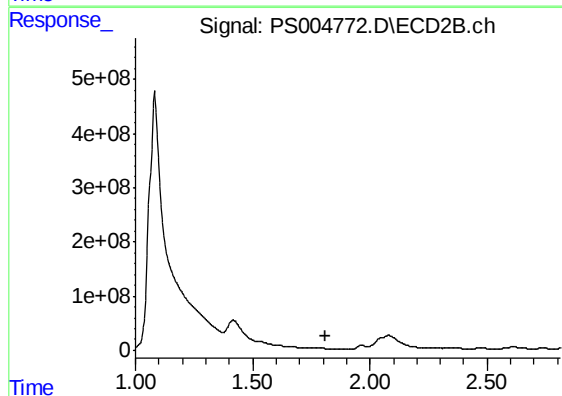


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

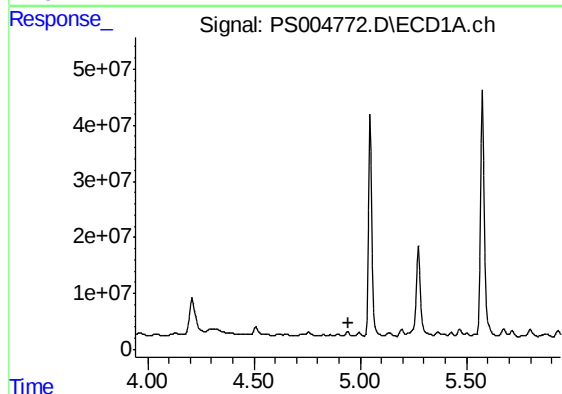


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

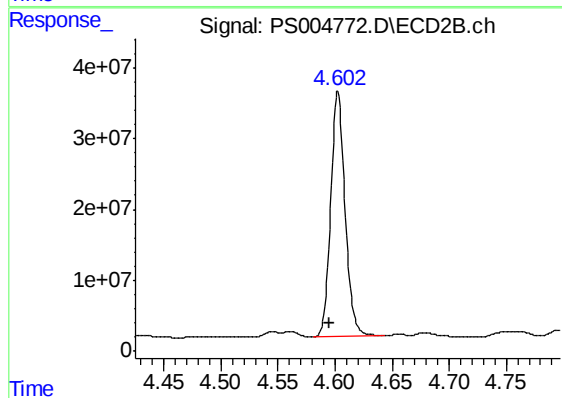

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.007 min
Response: 305644621
Conc: 248.06 ng/ml

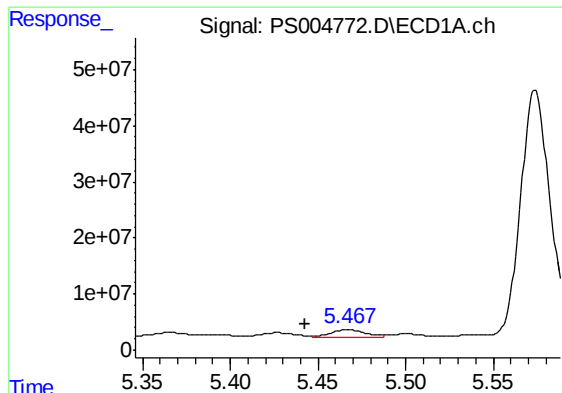

#3 4-Nitrophenol


R.T.: 5.467 min
Delta R.T.: 0.024 min
Response: 18572245
Conc: 29.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-D

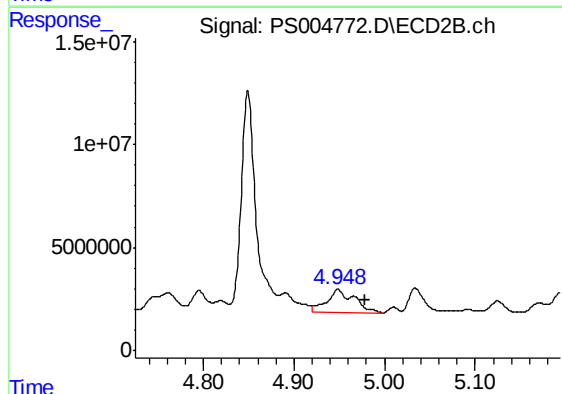


#3 4-Nitrophenol

R.T.: 4.949 min
Delta R.T.: -0.030 min
Response: 23371016
Conc: 49.31 ng/ml

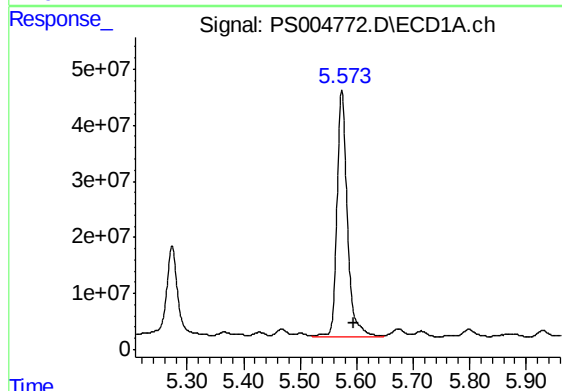


#4 2,4-DCAA

R.T.: 5.574 min
Delta R.T.: -0.021 min
Response: 561498181
Conc: 400.57 ng/ml

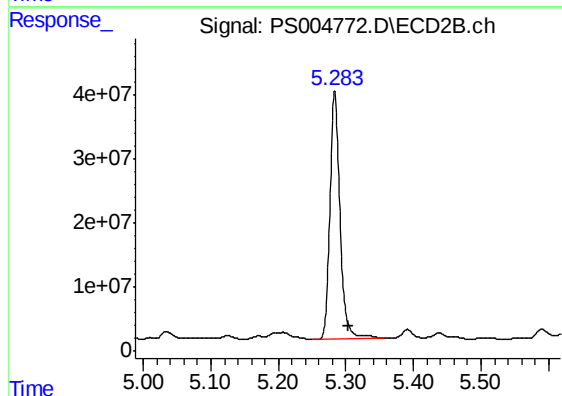

#4 2,4-DCAA


R.T.: 5.284 min
Delta R.T.: -0.020 min
Response: 402365070
Conc: 417.03 ng/ml

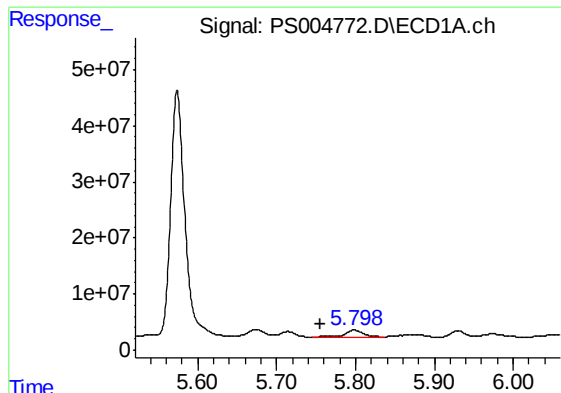

#5 DICAMBA


R.T.: 5.798 min
Delta R.T.: 0.043 min
Response: 21975774
Conc: 4.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-D

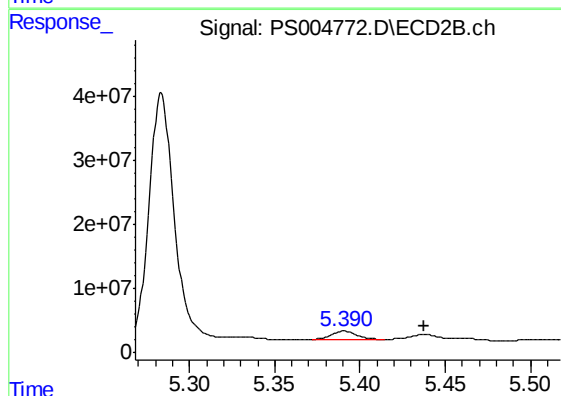


#5 DICAMBA

R.T.: 5.391 min
Delta R.T.: -0.047 min
Response: 12781702
Conc: 3.46 ng/ml

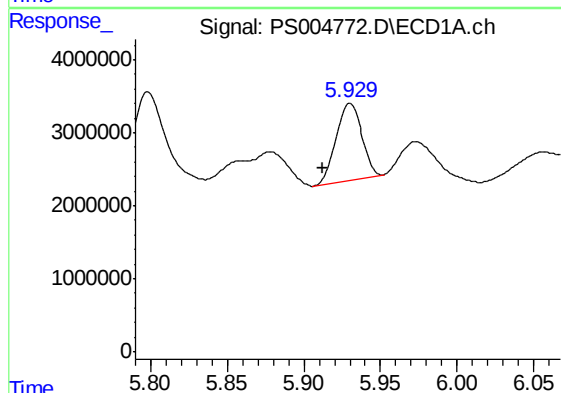


#6 MCPP

R.T.: 5.930 min
Delta R.T.: 0.017 min
Response: 12597353
Conc: 3.03 ug/ml

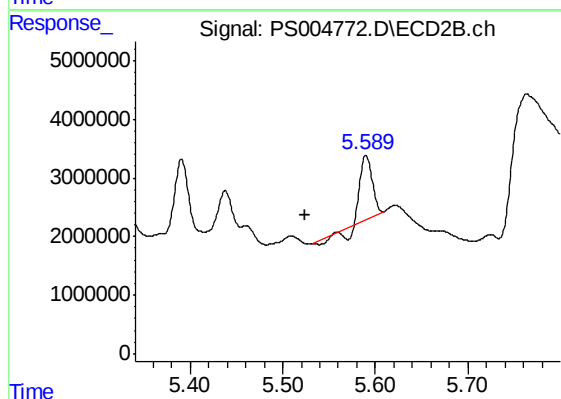

#6 MCPP


R.T.: 5.590 min
Delta R.T.: 0.066 min
Response: 8377762
Conc: 3.06 ug/ml

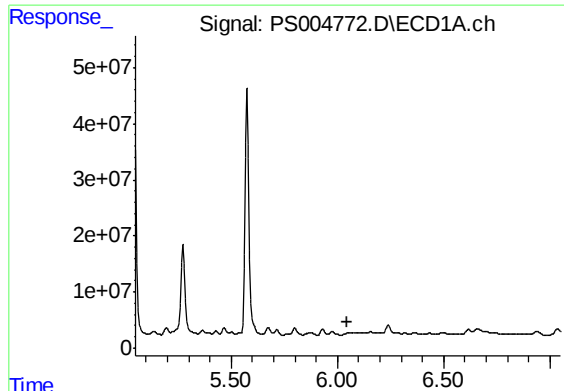

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5-D

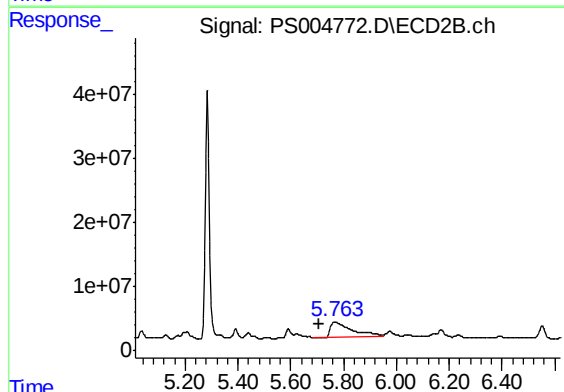


#7 MCPA

R.T.: 5.765 min
Delta R.T.: 0.055 min
Response: 128467500
Conc: 31.40 ug/ml

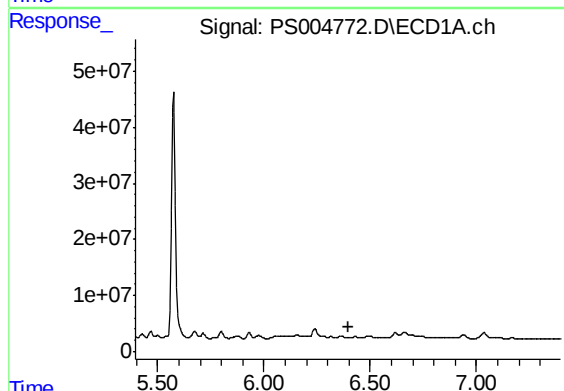


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

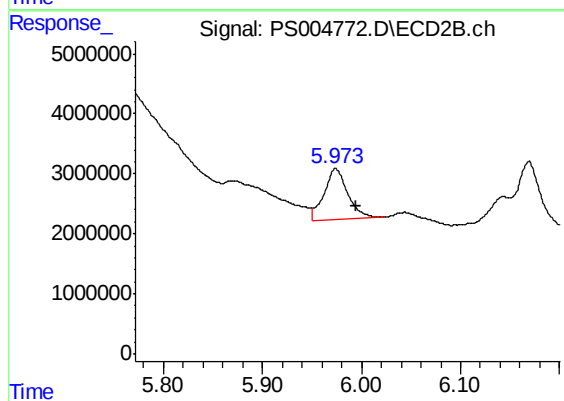

#8 DICHLORPROP


R.T.: 5.974 min
Delta R.T.: -0.020 min
Response: 13997853
Conc: 14.85 ng/ml

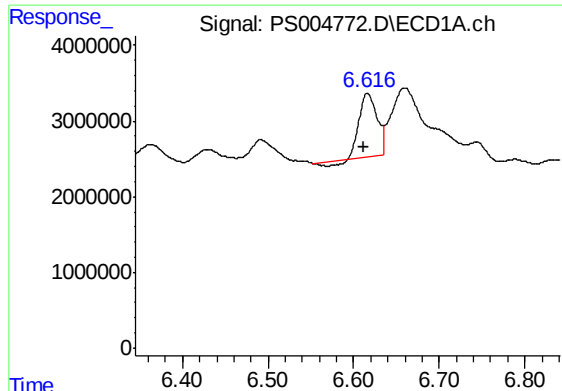

#9 2,4-D


R.T.: 6.616 min
Delta R.T.: 0.005 min
Response: 11356992
Conc: 8.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5-D

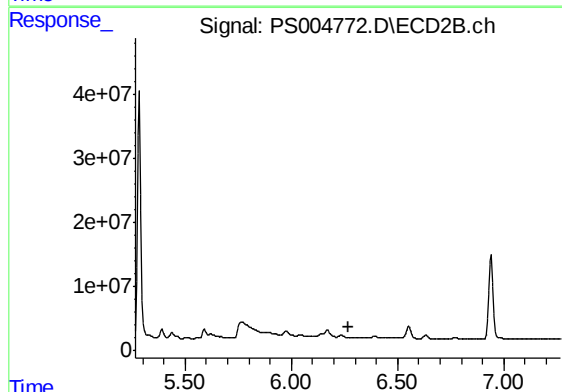


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

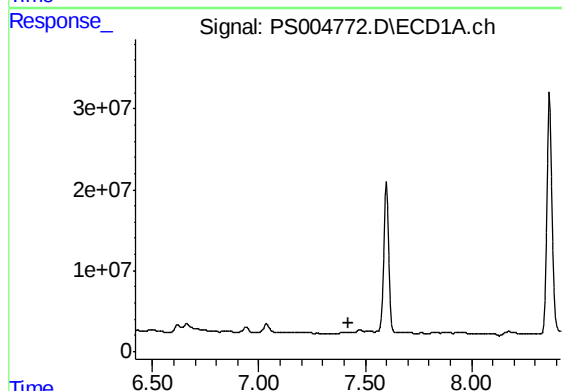

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

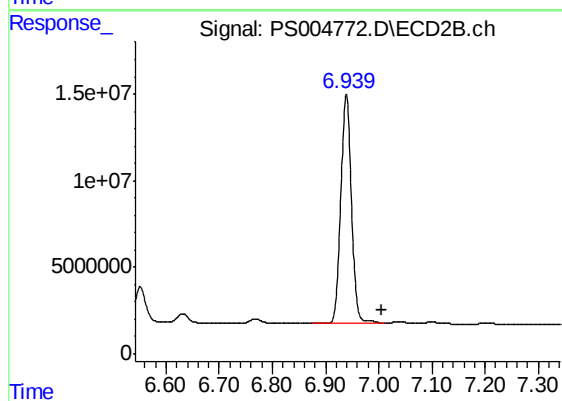

#11 2,4,5-TP (SILVEX)

R.T.: 6.939 min
Delta R.T.: -0.067 min
Response: 183713401
Conc: 35.70 ng/ml