

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004773.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 14:28
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:54:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.580	5.290	651.7E6	464.9E6	464.922	481.850
Target Compounds							
2) T	3,5-DICHL...	4.948	0.000	31012993	0	17.983	N.D. #
5) T	DICAMBA	0.000	5.445	0	29204614	N.D.	7.905
9) T	2,4-D	6.625	0.000	124.9E6	0	91.296	N.D. #
15) T	Picloram	9.120	0.000	254.6E6	0	24.430	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004773.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 14:28
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:54:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

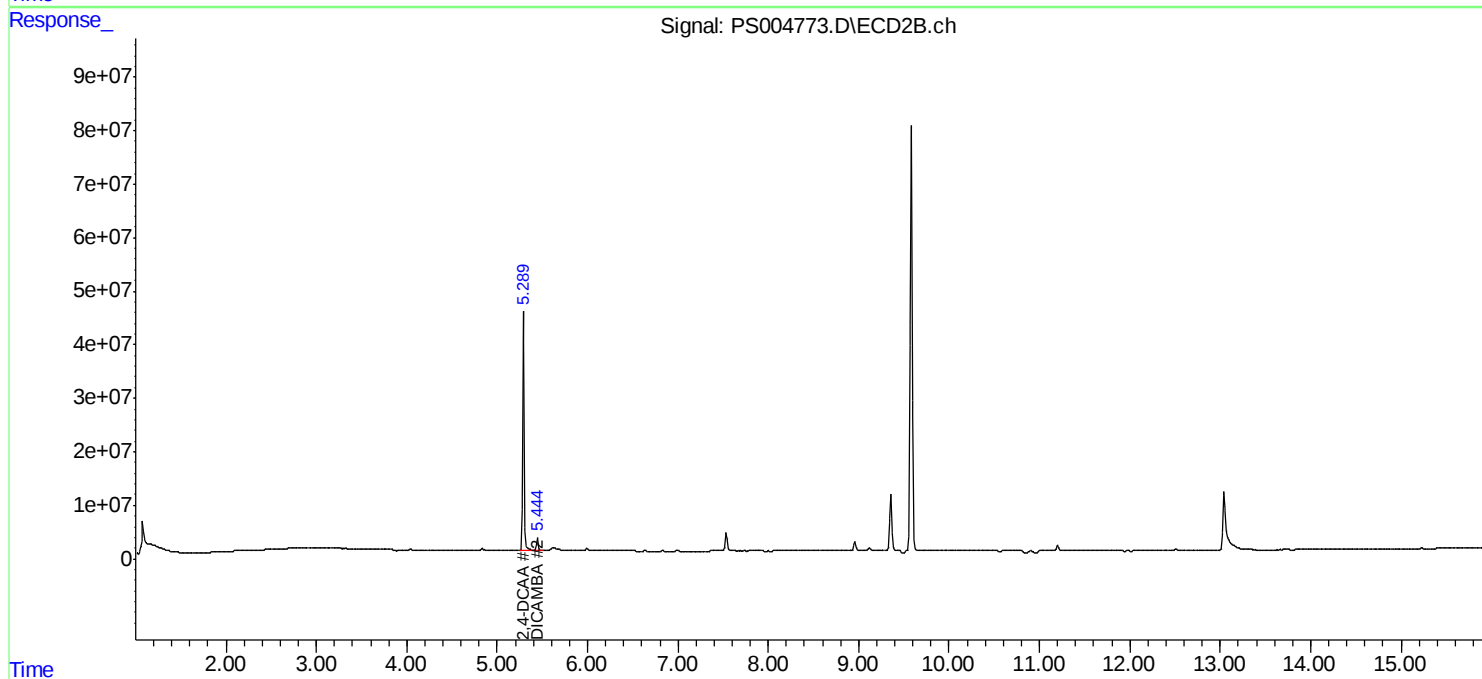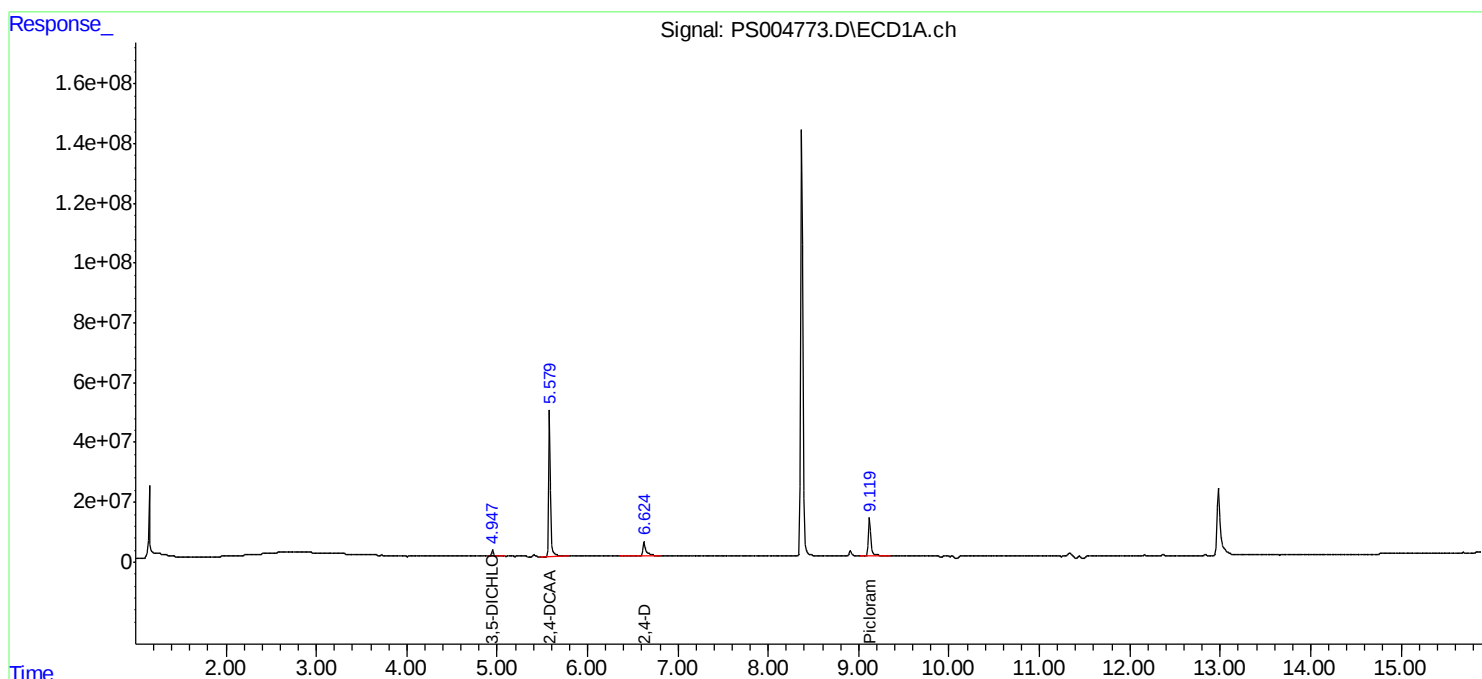


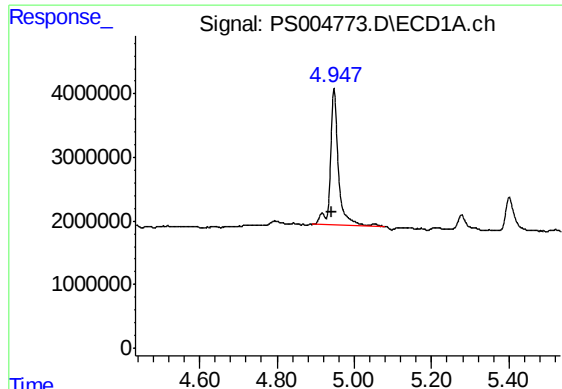

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.948 min
Delta R.T.: 0.006 min
Response: 31012993
Conc: 17.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

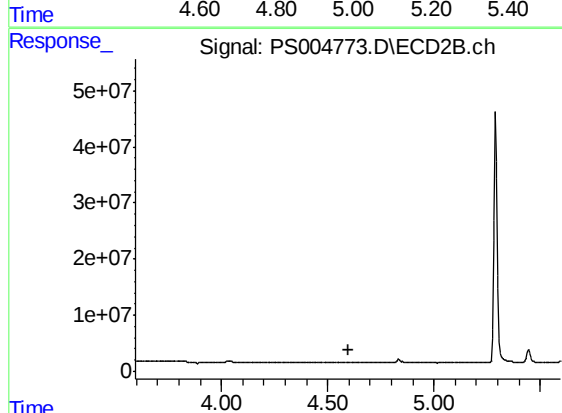


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

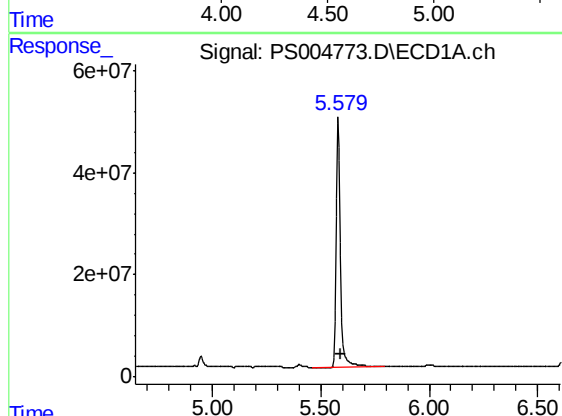


#4 2,4-DCAA

R.T.: 5.580 min
Delta R.T.: -0.015 min
Response: 651706965
Conc: 464.92 ng/ml

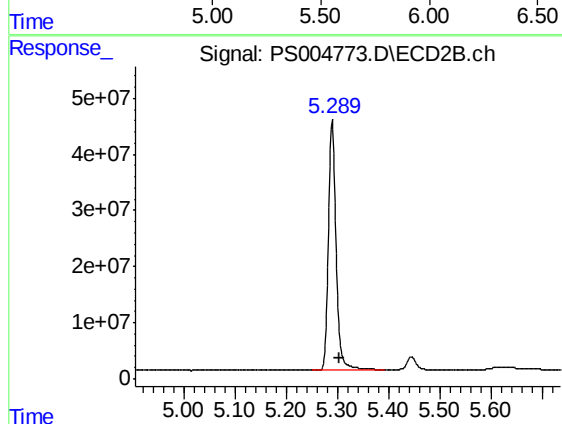

#4 2,4-DCAA


R.T.: 5.290 min
Delta R.T.: -0.014 min
Response: 464906112
Conc: 481.85 ng/ml

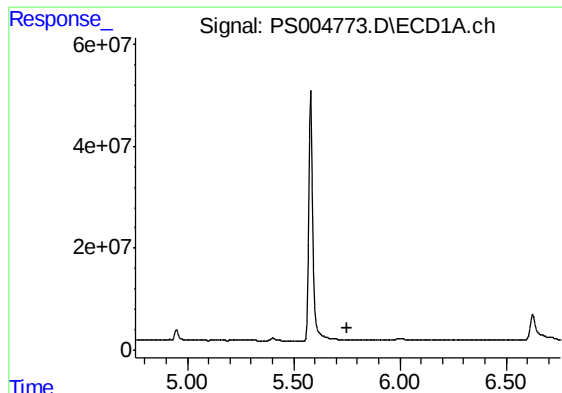

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

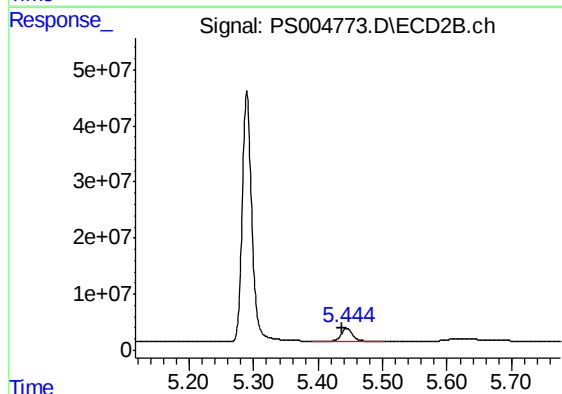


#5 DICAMBA

R.T.: 5.445 min
Delta R.T.: 0.007 min
Response: 29204614
Conc: 7.91 ng/ml

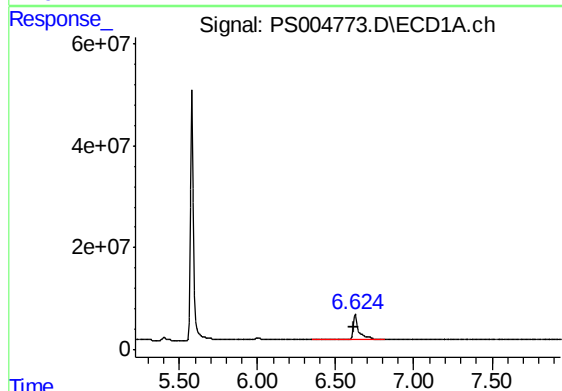


#9 2,4-D

R.T.: 6.625 min
Delta R.T.: 0.013 min
Response: 124885273
Conc: 91.30 ng/ml

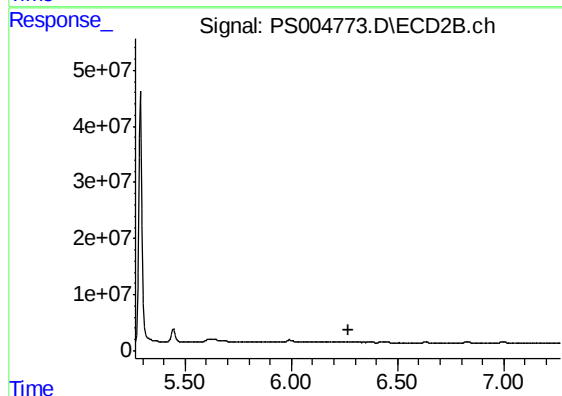

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

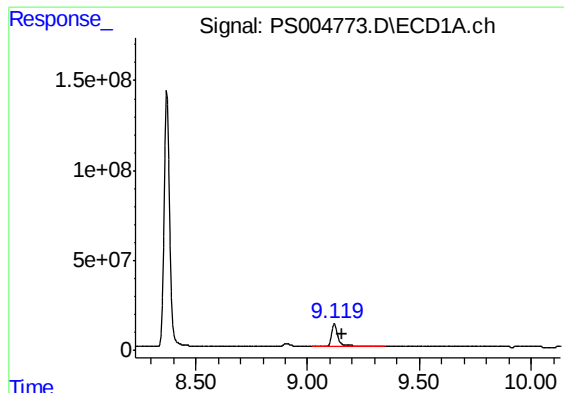

#15 Picloram

R.T.: 9.120 min
Delta R.T.: -0.036 min
Response: 254559061
Conc: 24.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

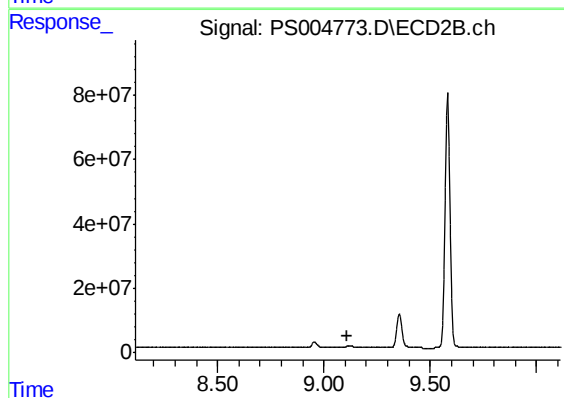

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.113 min
Response: 0
Conc: N.D.