

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 15:33
 Operator : SM\AJ
 Sample : K3026-16
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-3-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:54:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.577	5.282	569.4E6	422.1E6	406.232	437.432
Target Compounds							
1) T	Dalapon	2.078	0.000	41627089	0	25.112	N.D. #
2) T	3,5-DICHL...	0.000	4.600	0	339.5E6	N.D.	275.501
3) T	4-Nitroph...	0.000	4.946	0	24601509	N.D.	51.911
5) T	DICAMBA	5.718	5.435	17234189	18225914	3.246	4.934 #
6) T	MCPD	5.932	5.588	14958185	8086093	3.593	2.951
7) T	MCPA	6.037	5.743	61129110	277.2E6	10.554	67.737 #
8) T	DICHLORPROP	0.000	5.971	0	20103190	N.D.	21.322
9) T	2,4-D	6.619	0.000	14792366	0	10.814	N.D. #
11) T	2,4,5-TP ...	7.390	6.937	14444834	188.0E6	1.972	36.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 15:33
Operator : SM\AJ
Sample : K3026-16
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:54:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

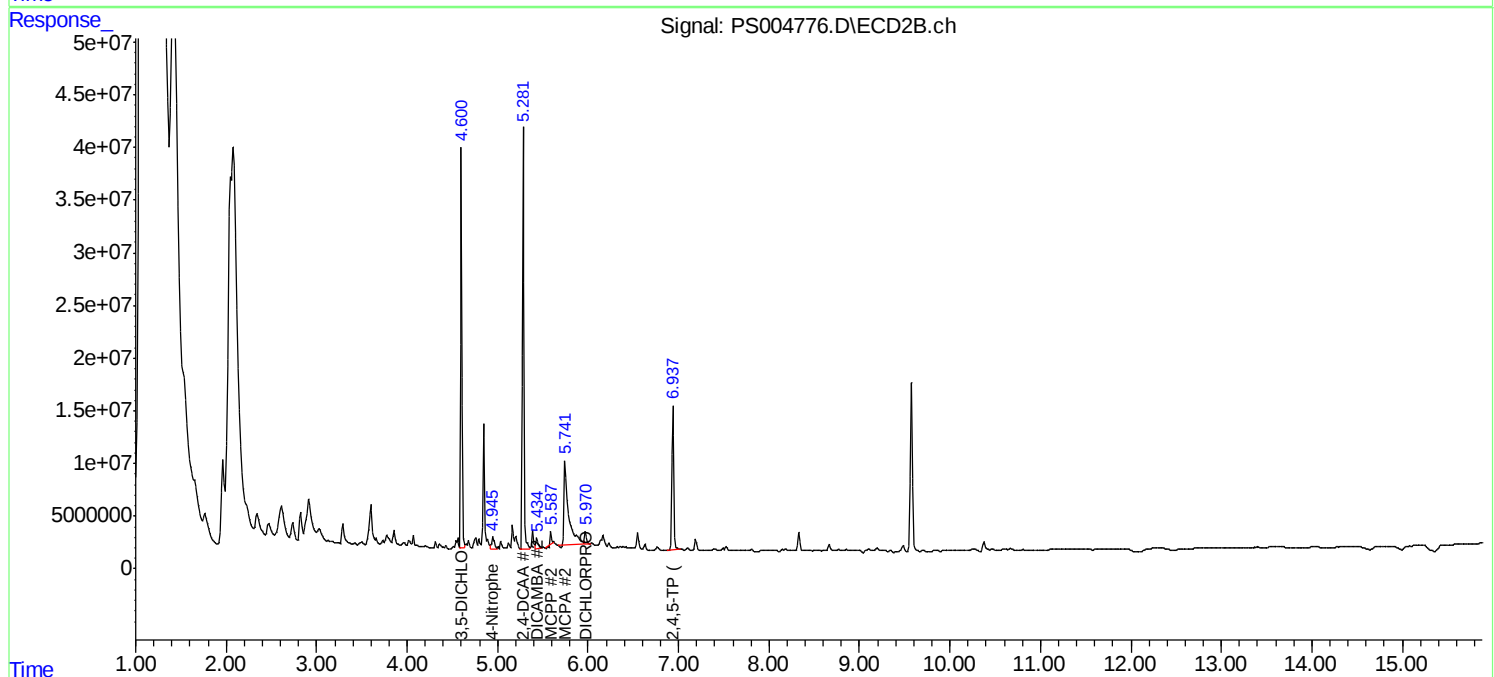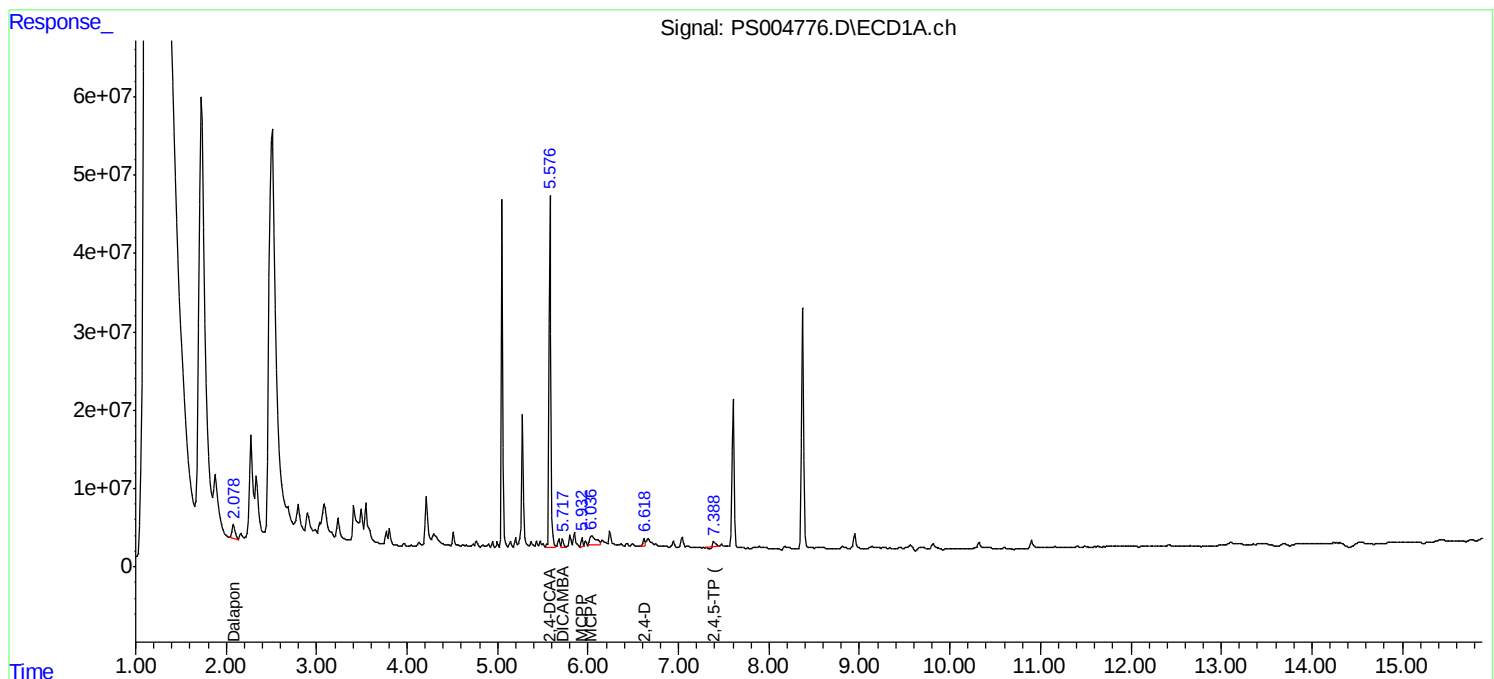


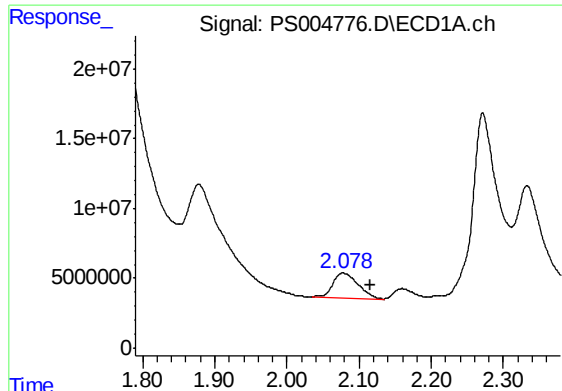

#1 Dalapon


R.T.: 2.078 min
Delta R.T.: -0.038 min
Response: 41627089
Conc: 25.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-S

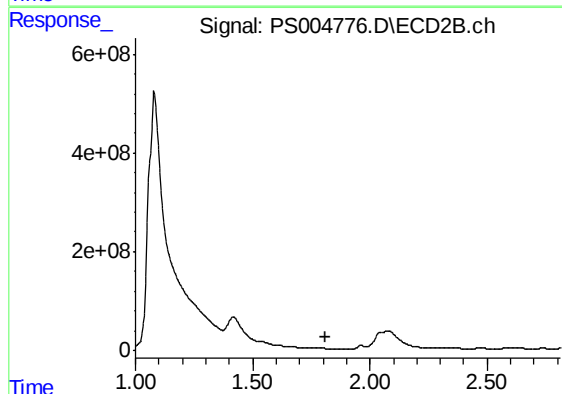


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

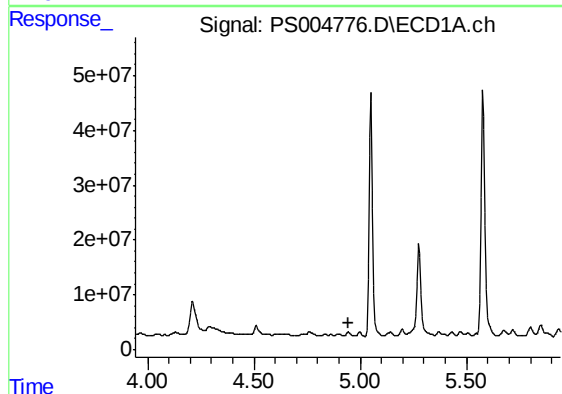


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

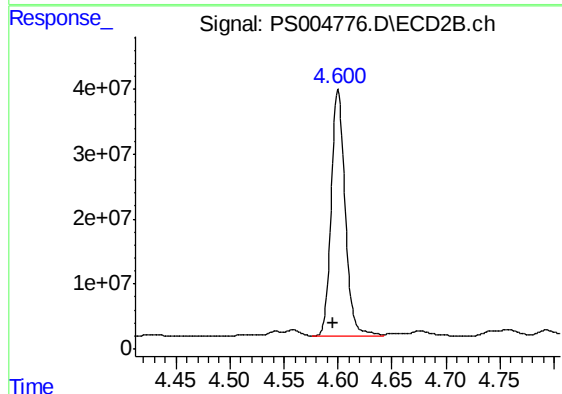

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.600 min
Delta R.T.: 0.005 min
Response: 339453088
Conc: 275.50 ng/ml

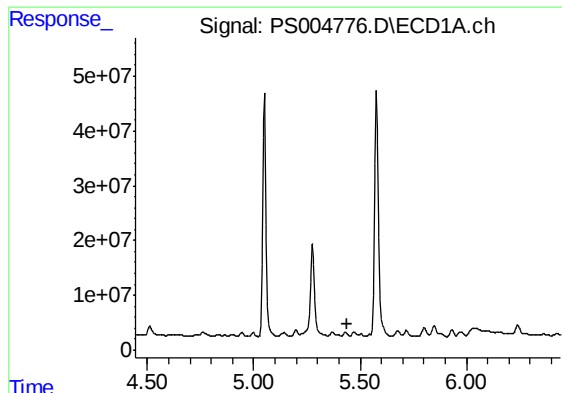

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.443 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-3-S

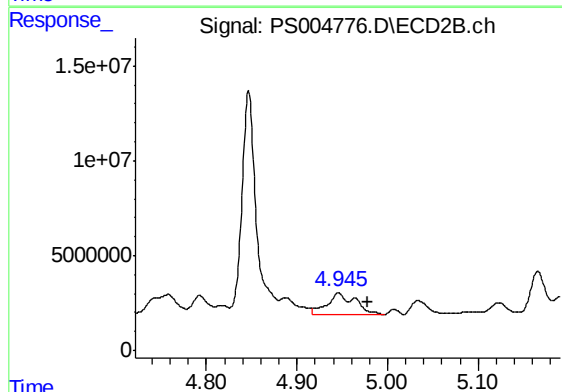


#3 4-Nitrophenol

R.T.: 4.946 min
Delta R.T.: -0.033 min
Response: 24601509
Conc: 51.91 ng/ml

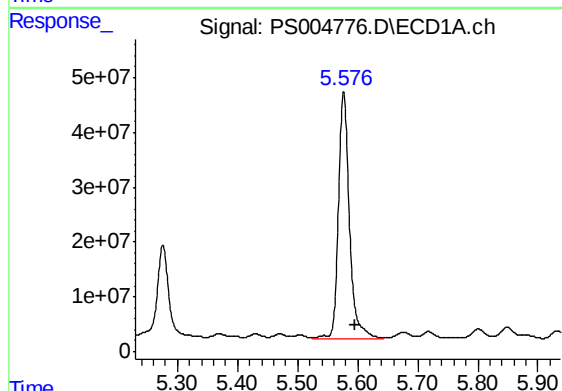


#4 2,4-DCAA

R.T.: 5.577 min
Delta R.T.: -0.018 min
Response: 569438450
Conc: 406.23 ng/ml

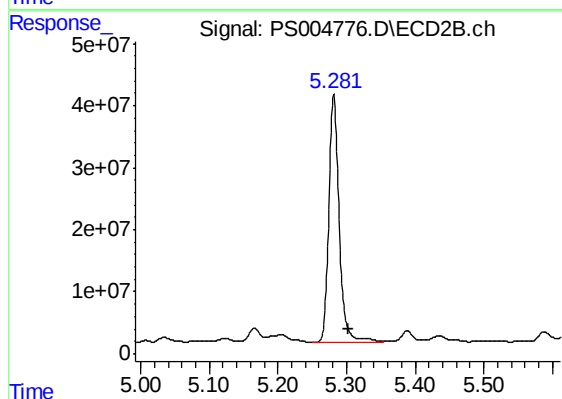

#4 2,4-DCAA


R.T.: 5.282 min
Delta R.T.: -0.022 min
Response: 422050498
Conc: 437.43 ng/ml

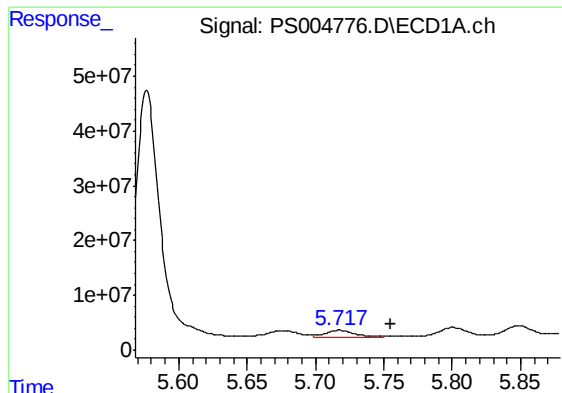

#5 DICAMBA


R.T.: 5.718 min
Delta R.T.: -0.037 min
Response: 17234189
Conc: 3.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-S

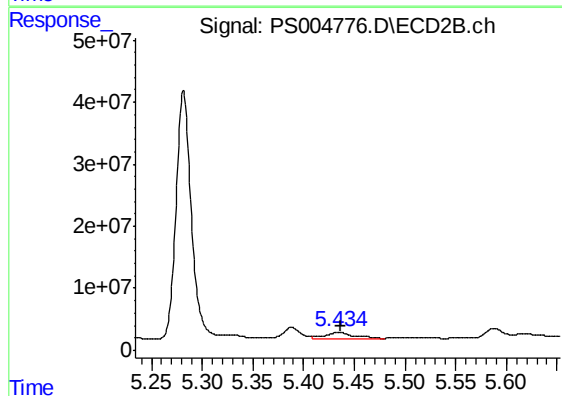


#5 DICAMBA

R.T.: 5.435 min
Delta R.T.: -0.003 min
Response: 18225914
Conc: 4.93 ng/ml

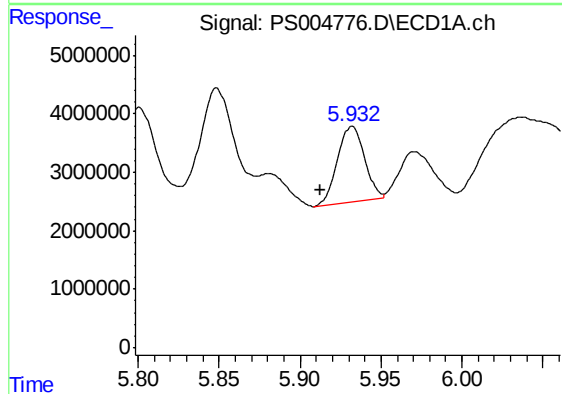


#6 MCP

R.T.: 5.932 min
Delta R.T.: 0.019 min
Response: 14958185
Conc: 3.59 ug/ml

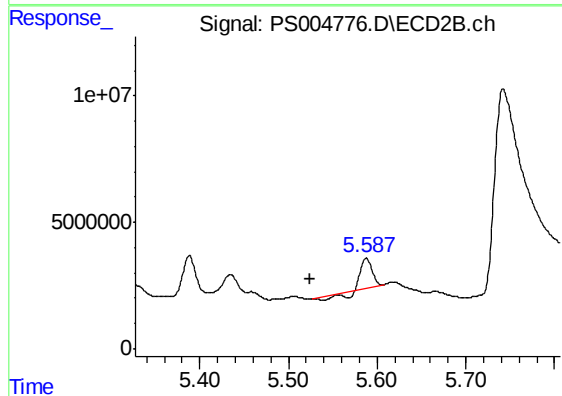

#6 MCP


R.T.: 5.588 min
Delta R.T.: 0.064 min
Response: 8086093
Conc: 2.95 ug/ml

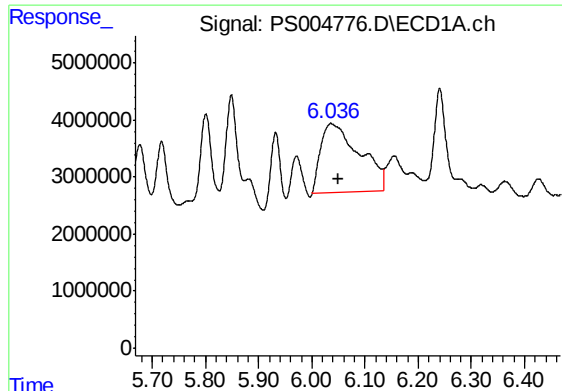

#7 MCPA


R.T.: 6.037 min
Delta R.T.: -0.013 min
Response: 61129110
Conc: 10.55 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-S

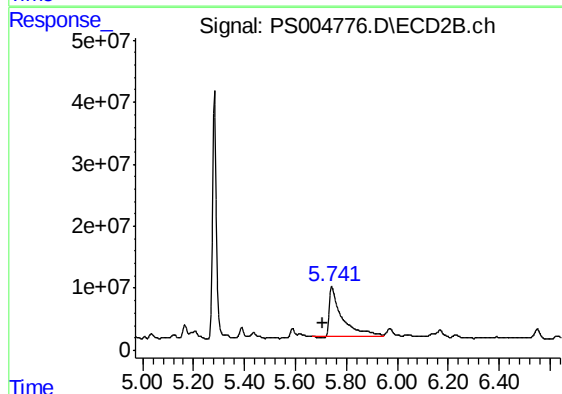


#7 MCPA

R.T.: 5.743 min
Delta R.T.: 0.034 min
Response: 277156988
Conc: 67.74 ug/ml

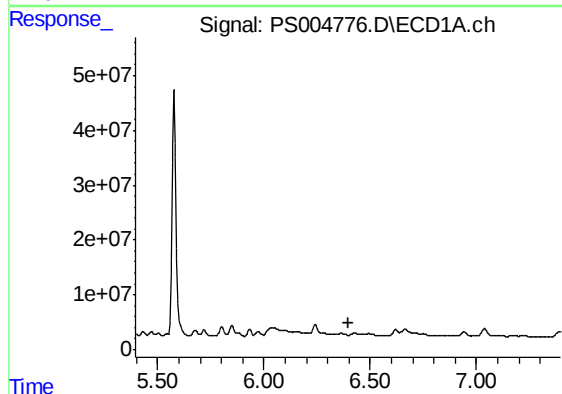


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

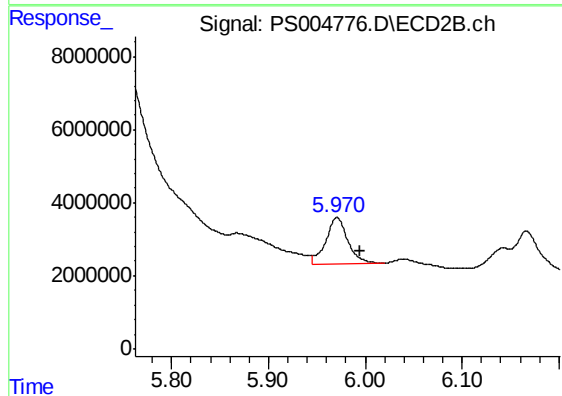

#8 DICHLORPROP


R.T.: 5.971 min
Delta R.T.: -0.023 min
Response: 20103190
Conc: 21.32 ng/ml

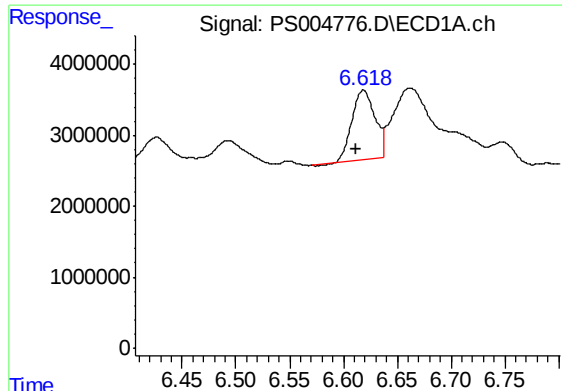

#9 2,4-D


R.T.: 6.619 min
Delta R.T.: 0.007 min
Response: 14792366
Conc: 10.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3-S

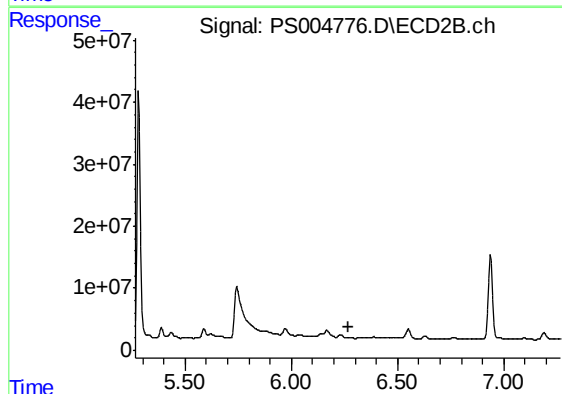


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

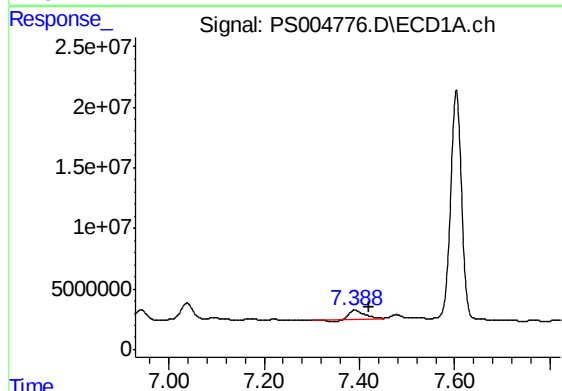

#11 2,4,5-TP (SILVEX)

R.T.: 7.390 min
Delta R.T.: -0.029 min
Response: 14444834
Conc: 1.97 ng/ml

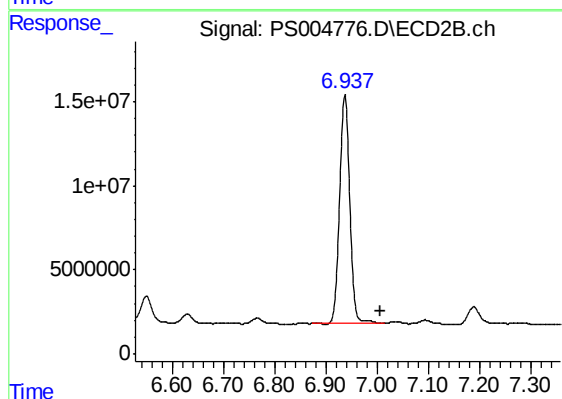

#11 2,4,5-TP (SILVEX)

R.T.: 6.937 min
Delta R.T.: -0.069 min
Response: 188045110
Conc: 36.55 ng/ml