

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 19:13
 Operator : SM\AJ
 Sample : K2993-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-6_1.5-2.0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:57:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.596	5.306	390.5E6	226.9E6	278.584	235.185
Target Compounds							
2) T	3,5-DICHL...	0.000	4.568	0	9942249	N.D.	8.069
3) T	4-Nitroph...	5.399	0.000	41910913	0	67.218	N.D. #
5) T	DICAMBA	5.735	5.412	17822043	16050367	3.357	4.345 #
6) T	MCP	5.951	0.000	12585799	0	3.023	N.D. #
7) T	MCPA	6.089	5.699	19255917	23662266	3.324	5.783 #
10) T	Pentachlo...	0.000	6.575	0	47434249	N.D.	3.861
11) T	2,4,5-TP ...	0.000	6.962	0	59988324	N.D.	11.659
13) T	2,4-DB	8.243	7.867	336.5E6	315.6E6	348.313	482.831 #
14) T	DINOSEB	0.000	8.171	0	117.5E6	N.D.	30.564



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 19:13
Operator : SM\AJ
Sample : K2993-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SB-6_1.5-2.0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:57:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

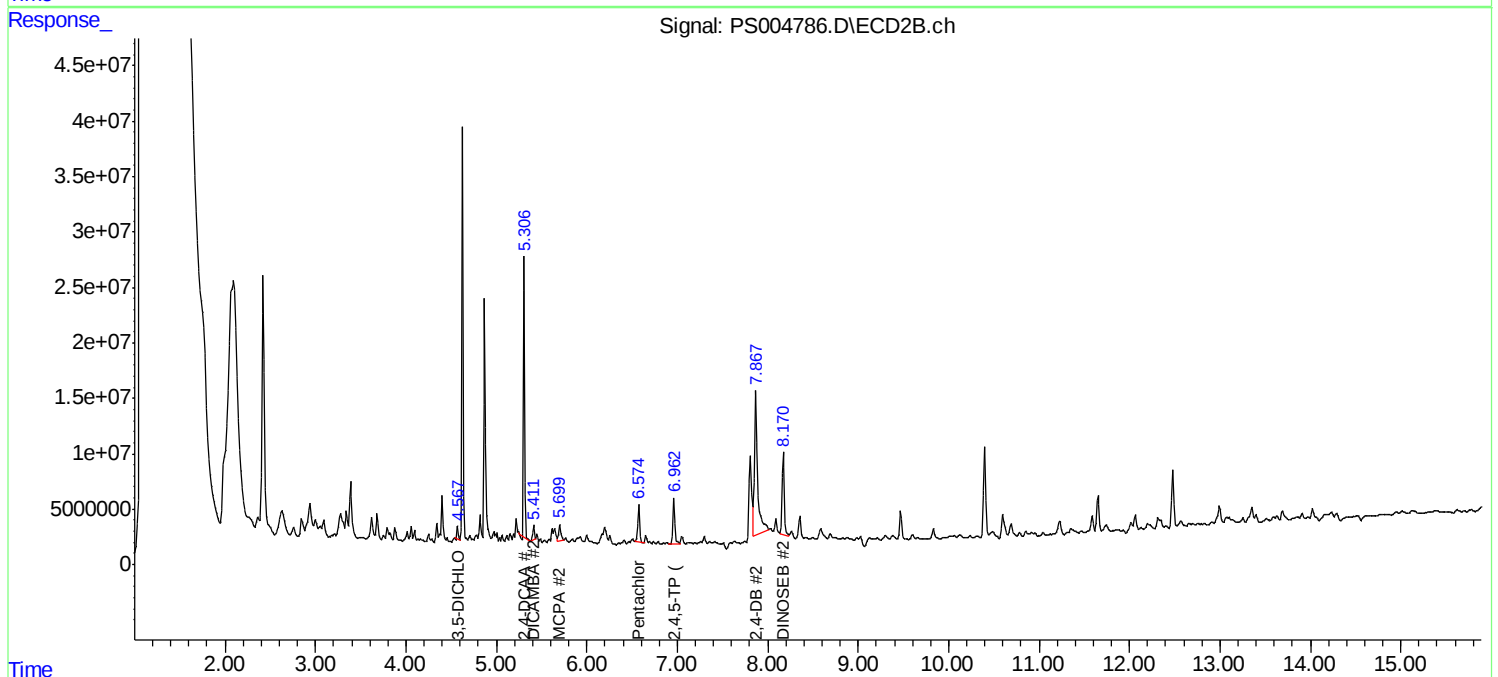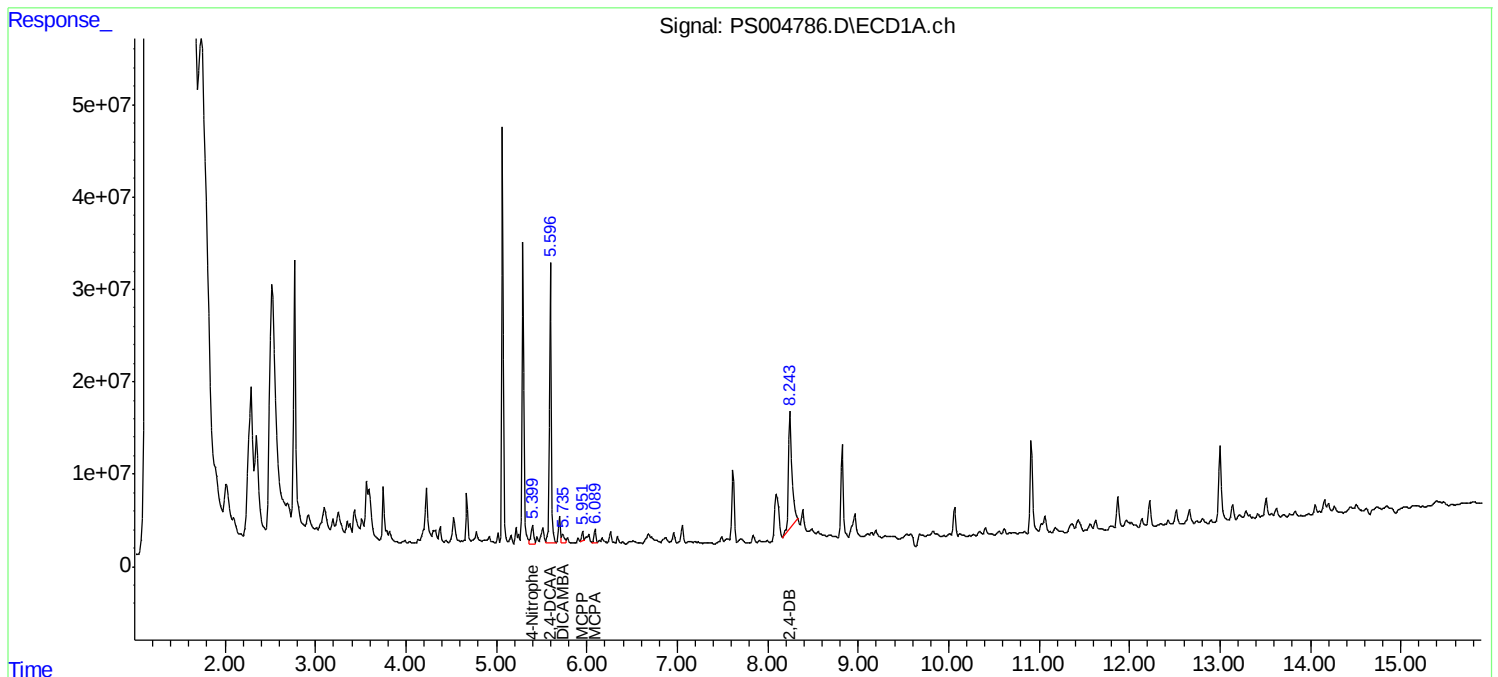


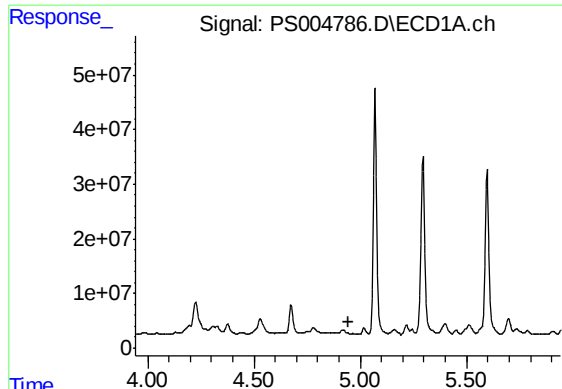

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-6_1.5-2.0

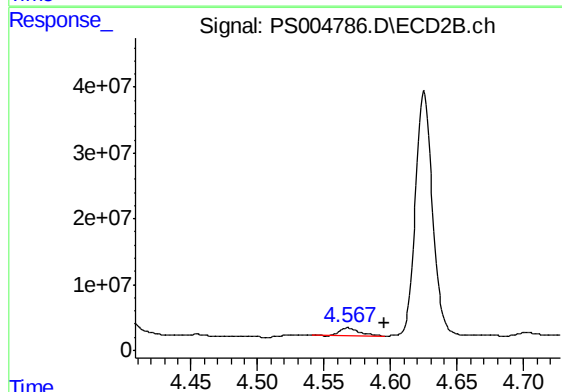


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.568 min
Delta R.T.: -0.027 min
Response: 9942249
Conc: 8.07 ng/ml

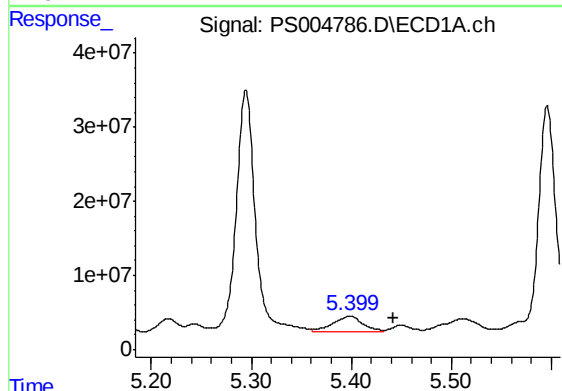


#3 4-Nitrophenol

R.T.: 5.399 min
Delta R.T.: -0.044 min
Response: 41910913
Conc: 67.22 ng/ml

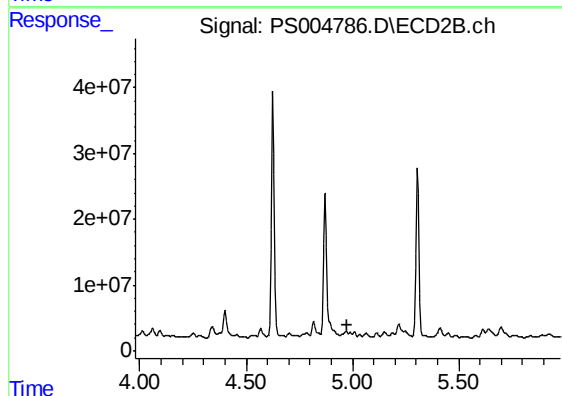

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

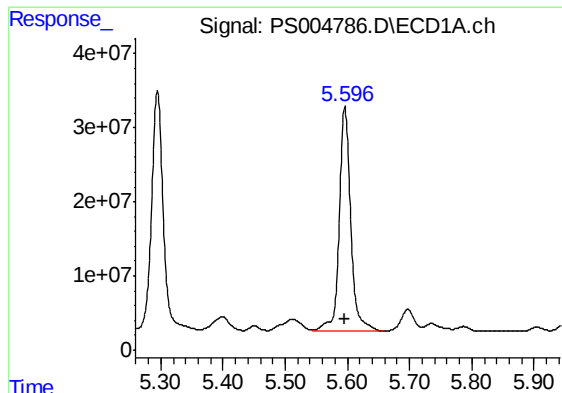

#4 2,4-DCAA


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 390506570
Conc: 278.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6_1.5-2.0

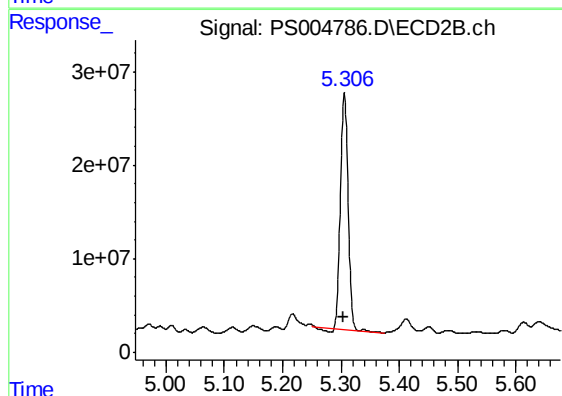


#4 2,4-DCAA

R.T.: 5.306 min
Delta R.T.: 0.002 min
Response: 226914724
Conc: 235.18 ng/ml

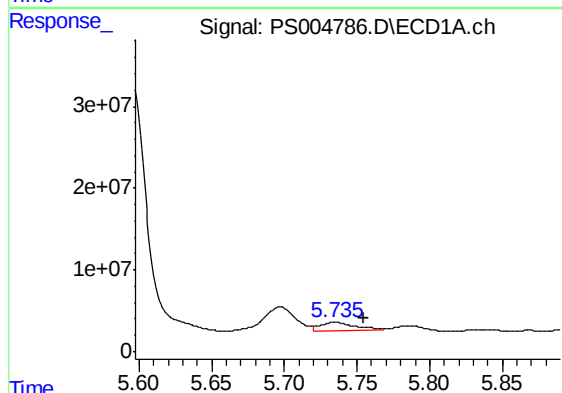


#5 DICAMBA

R.T.: 5.735 min
Delta R.T.: -0.020 min
Response: 17822043
Conc: 3.36 ng/ml

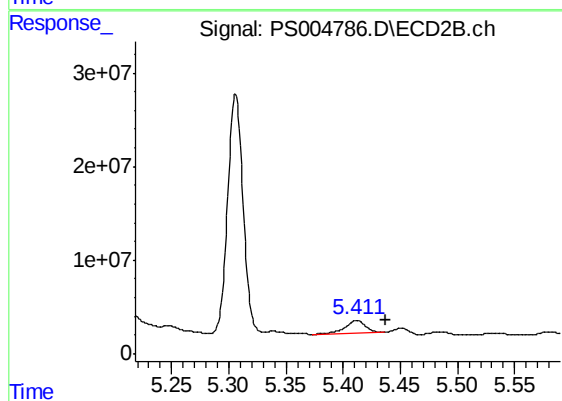

#5 DICAMBA


R.T.: 5.412 min
Delta R.T.: -0.025 min
Response: 16050367
Conc: 4.34 ng/ml

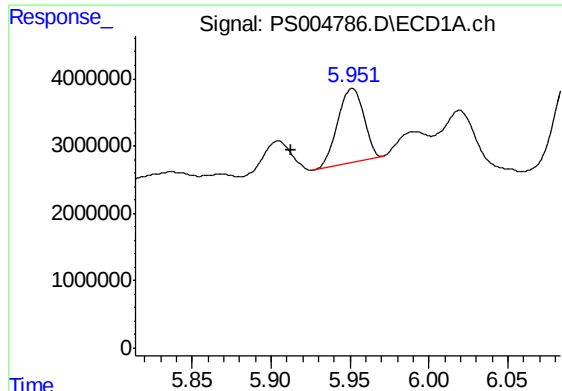

#6 MCPP


R.T.: 5.951 min
Delta R.T.: 0.039 min
Response: 12585799
Conc: 3.02 ug/ml

Instrument :
ECD_S
ClientSampleId :
SB-6_1.5-2.0

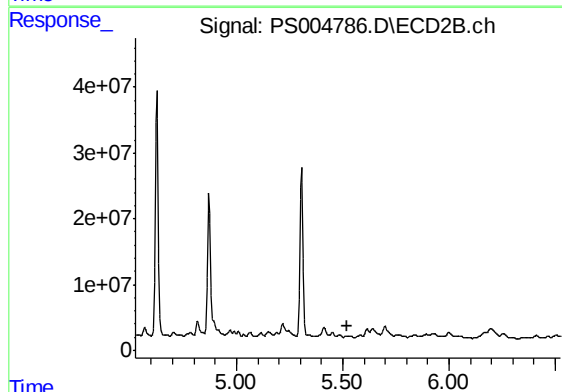


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 5.524 min
Response: 0
Conc: N.D.

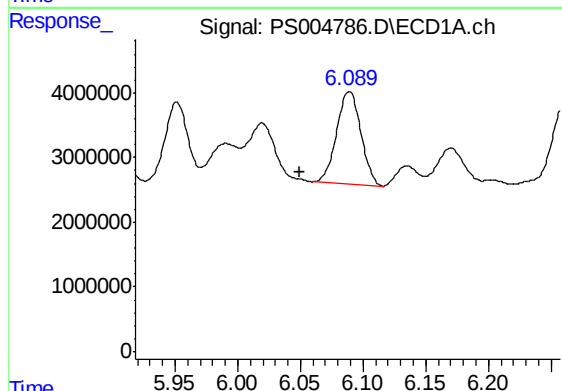


#7 MCPA

R.T.: 6.089 min
Delta R.T.: 0.040 min
Response: 19255917
Conc: 3.32 ug/ml

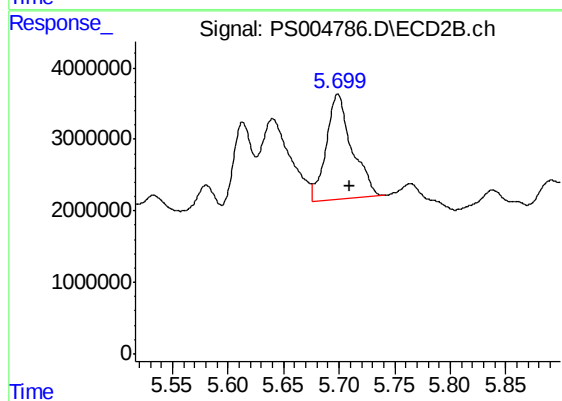

#7 MCPA


R.T.: 5.699 min
Delta R.T.: -0.010 min
Response: 23662266
Conc: 5.78 ug/ml

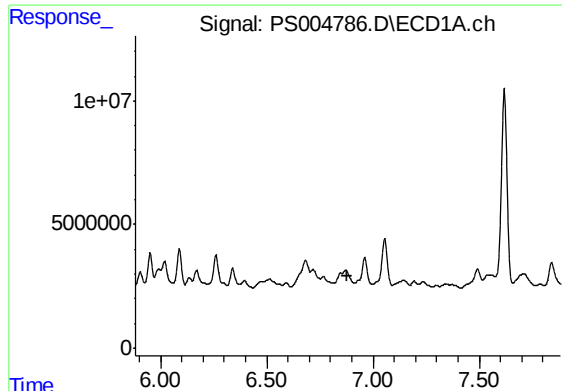

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.882 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-6_1.5-2.0

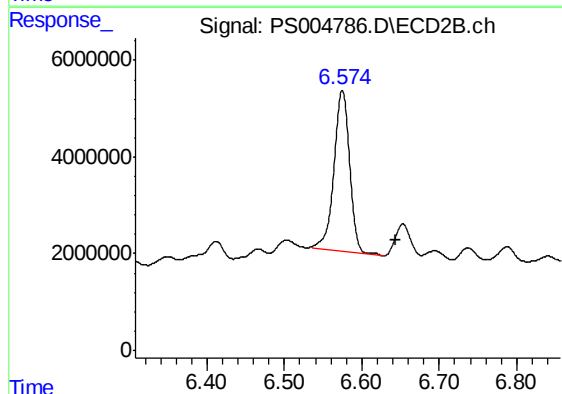


#10 Pentachlorophenol

R.T.: 6.575 min
Delta R.T.: -0.069 min
Response: 47434249
Conc: 3.86 ng/ml

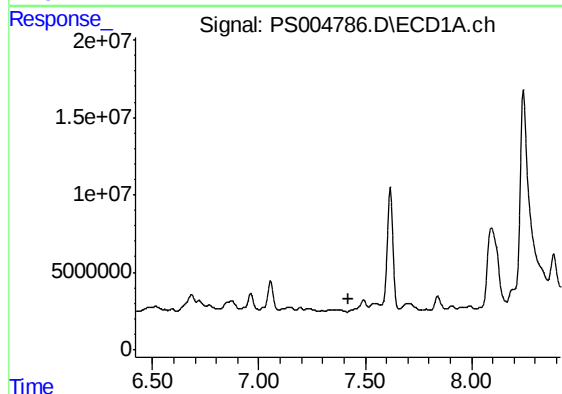


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

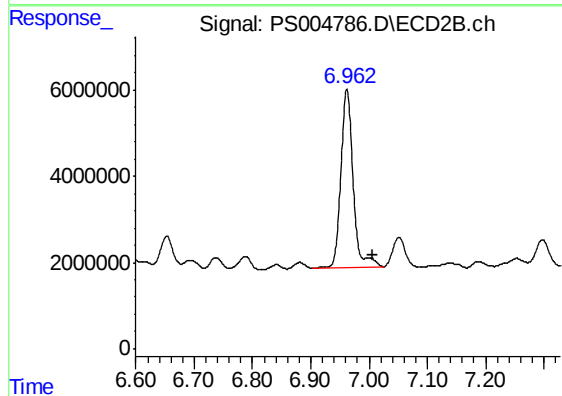

#11 2,4,5-TP (SILVEX)


R.T.: 6.962 min
Delta R.T.: -0.044 min
Response: 59988324
Conc: 11.66 ng/ml

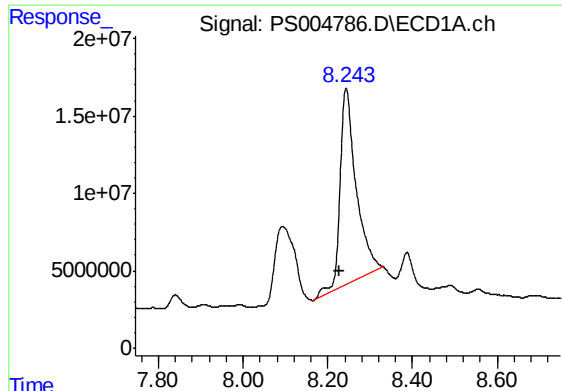

#13 2,4-DB


R.T.: 8.243 min
Delta R.T.: 0.017 min
Response: 336457221
Conc: 348.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6_1.5-2.0

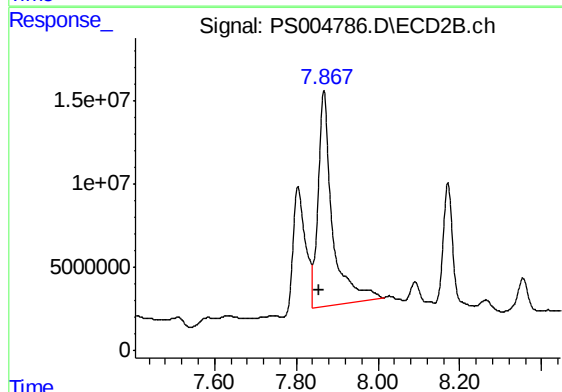


#13 2,4-DB

R.T.: 7.867 min
Delta R.T.: 0.011 min
Response: 315587692
Conc: 482.83 ng/ml

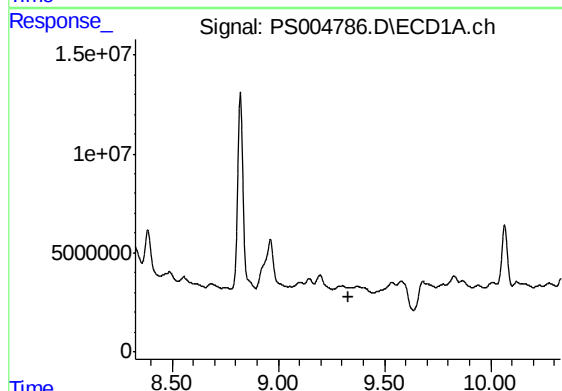

#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.328 min
Response: 0
Conc: N.D.

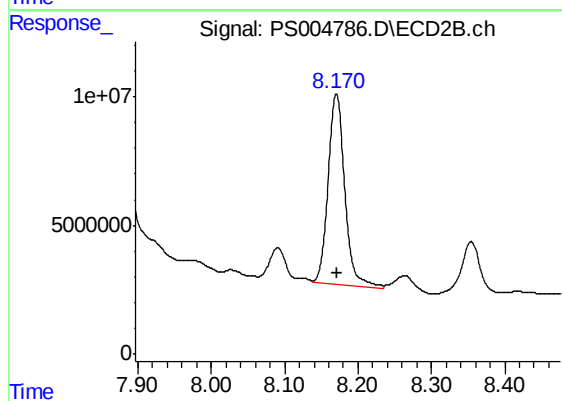

#14 DINOSEB

R.T.: 8.171 min
Delta R.T.: 0.000 min
Response: 117490686
Conc: 30.56 ng/ml