

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2019 00:42
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 01:00:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.583	5.293	666.4E6	477.6E6	475.436	495.054
Target Compounds							
2) T	3,5-DICHL...	4.951	0.000	33383842	0	19.358	N.D. #
5) T	DICAMBA	0.000	5.448	0	35987162	N.D.	9.741
9) T	2,4-D	6.627	0.000	116.0E6	0	84.802	N.D. #
15) T	Picloram	9.122	0.000	259.2E6	0	24.871	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2019 00:42
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 01:00:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

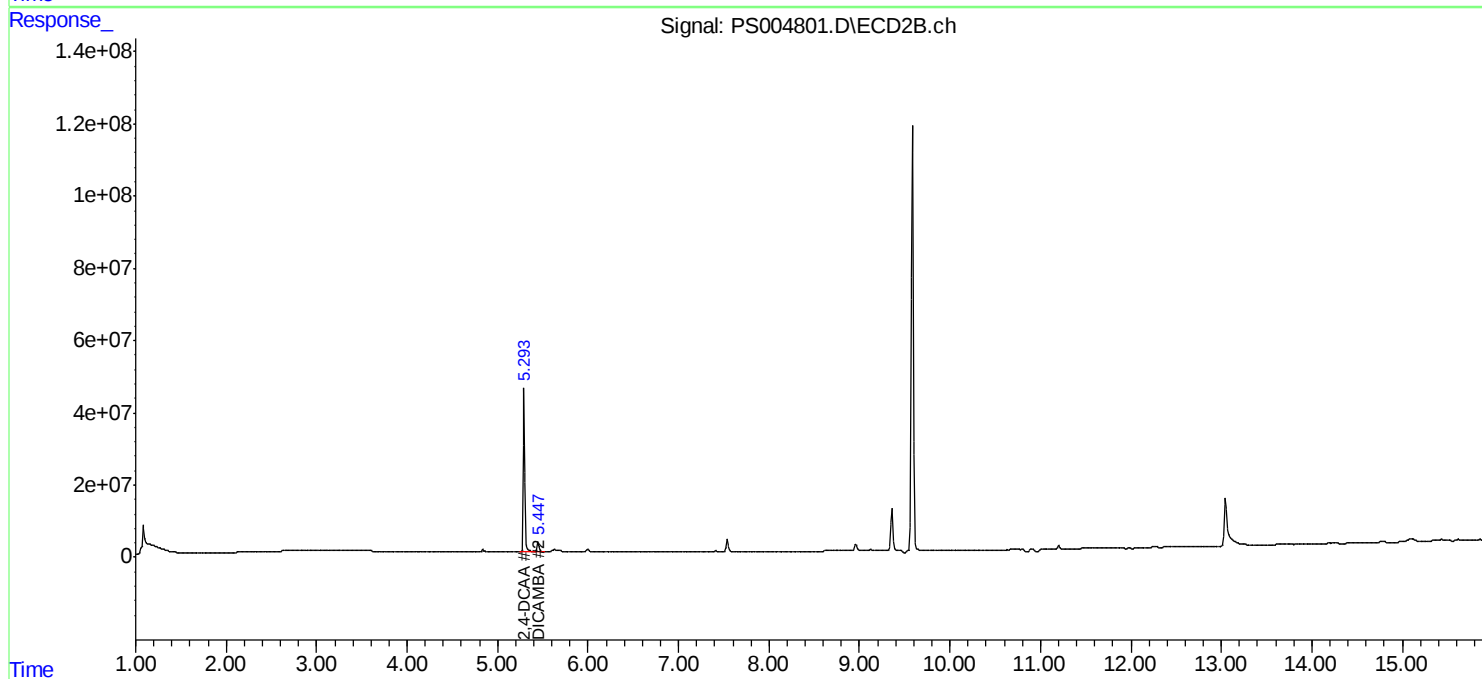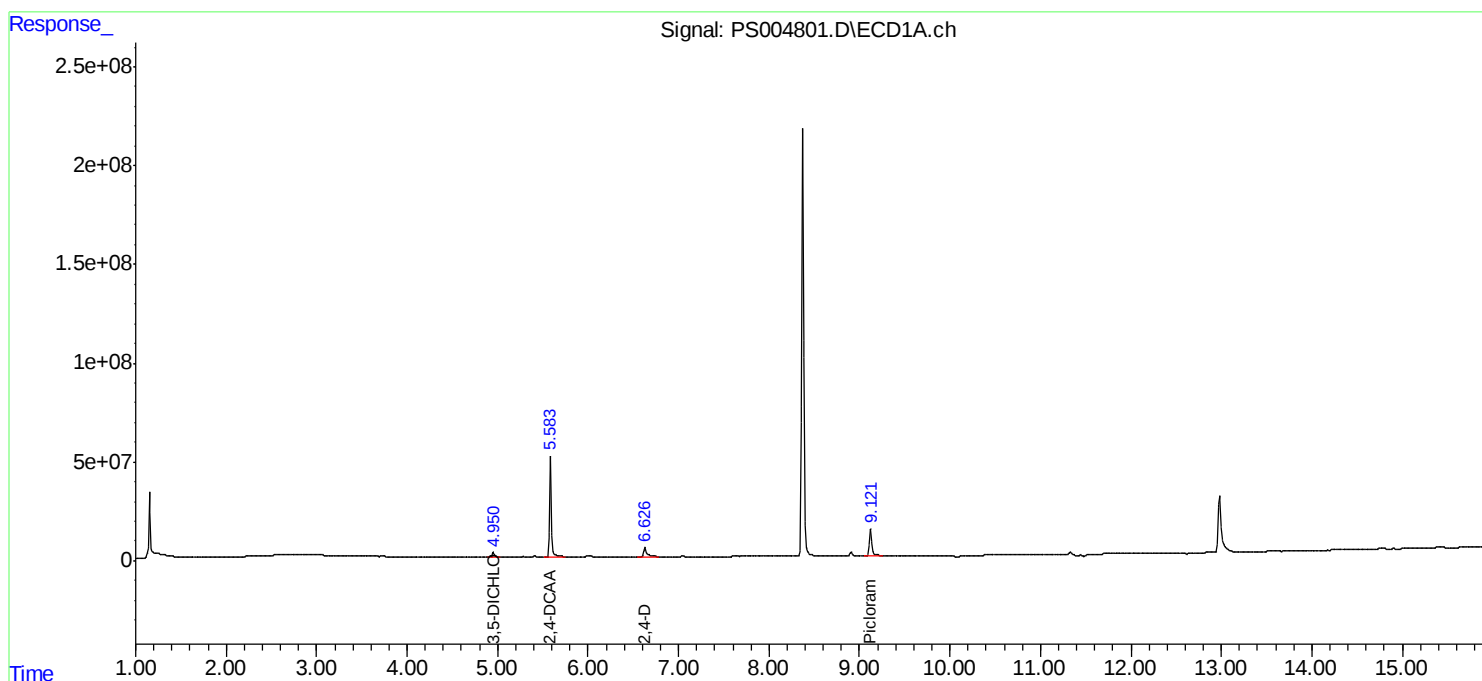


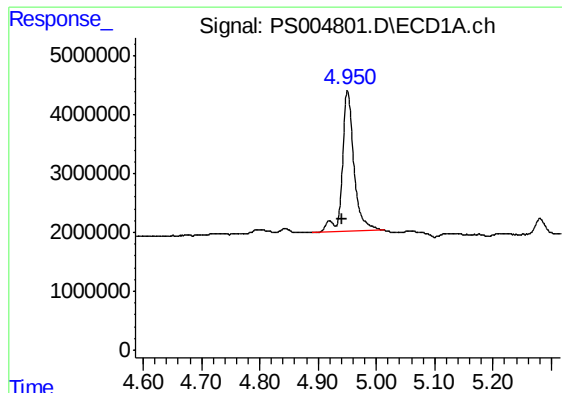

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.951 min
Delta R.T.: 0.009 min
Response: 33383842
Conc: 19.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

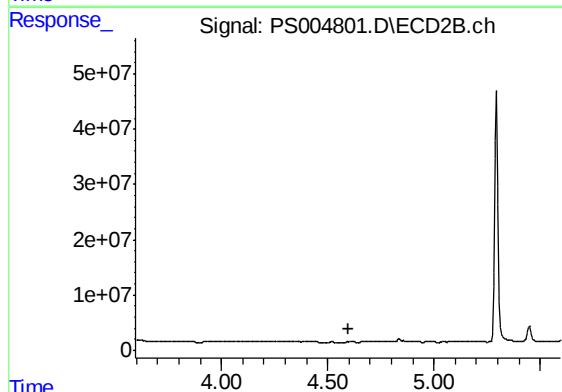


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.596 min
Response: 0
Conc: N.D.

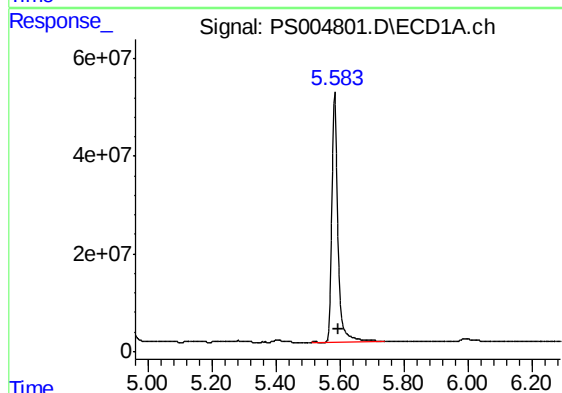


#4 2,4-DCAA

R.T.: 5.583 min
Delta R.T.: -0.012 min
Response: 666445902
Conc: 475.44 ng/ml

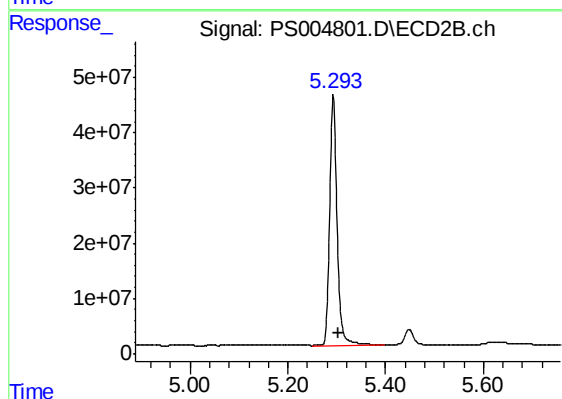

#4 2,4-DCAA


R.T.: 5.293 min
Delta R.T.: -0.011 min
Response: 477645763
Conc: 495.05 ng/ml

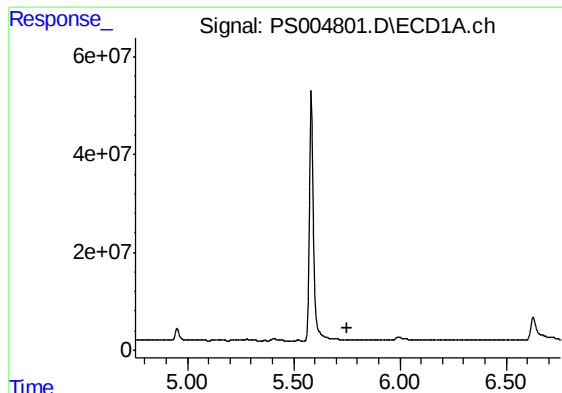

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 5.755 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

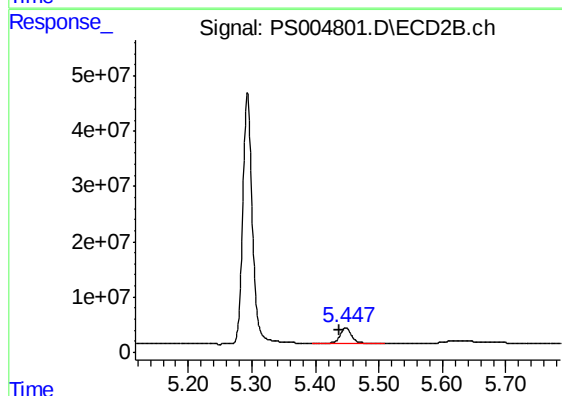


#5 DICAMBA

R.T.: 5.448 min
Delta R.T.: 0.011 min
Response: 35987162
Conc: 9.74 ng/ml

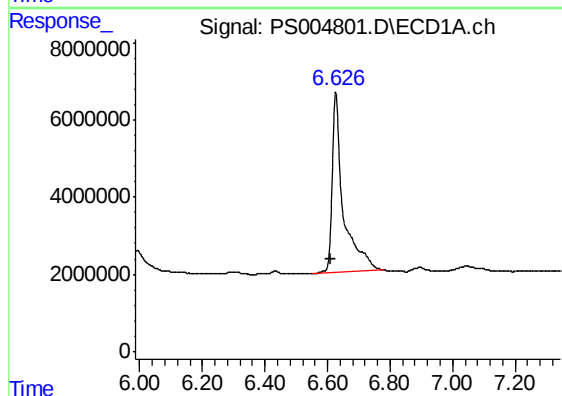


#9 2,4-D

R.T.: 6.627 min
Delta R.T.: 0.015 min
Response: 116001248
Conc: 84.80 ng/ml

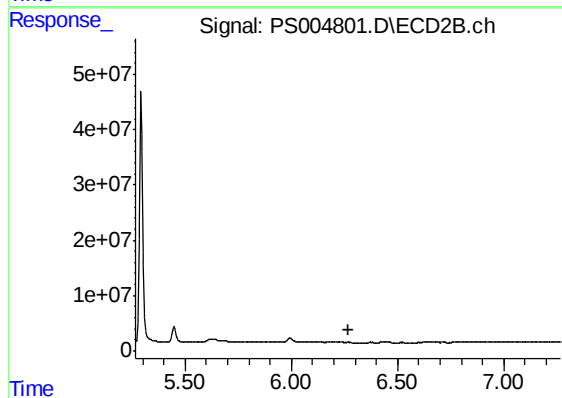

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

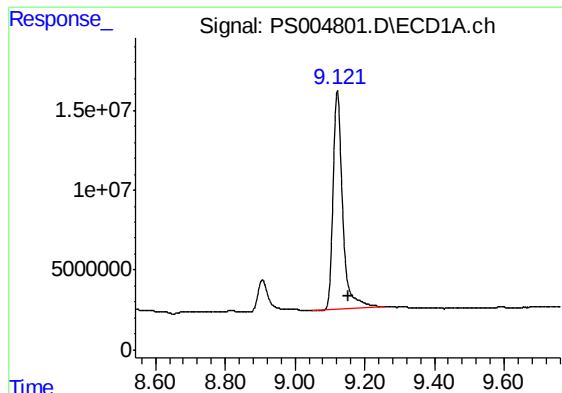

#15 Picloram

R.T.: 9.122 min
Delta R.T.: -0.034 min
Response: 259160893
Conc: 24.87 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

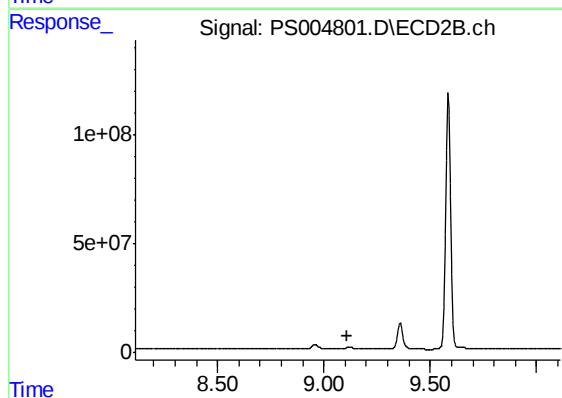

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.113 min
Response: 0
Conc: N.D.