

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
 Data File : PS004769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2019 13:00
 Operator : SM\AJ
 Sample : K3023-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SSSI-0523-S-TCLP-11

Manual Integrations
 APPROVED

Ankita
 5/28/2019 11:02:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:53:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.593	5.302	699.7E6	502.1E6	499.176	520.366m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052519\
Data File : PS004769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2019 13:00
Operator : SM\AJ
Sample : K3023-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11


Manual Integrations
APPROVED

Ankita
5/28/2019 11:02:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:53:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

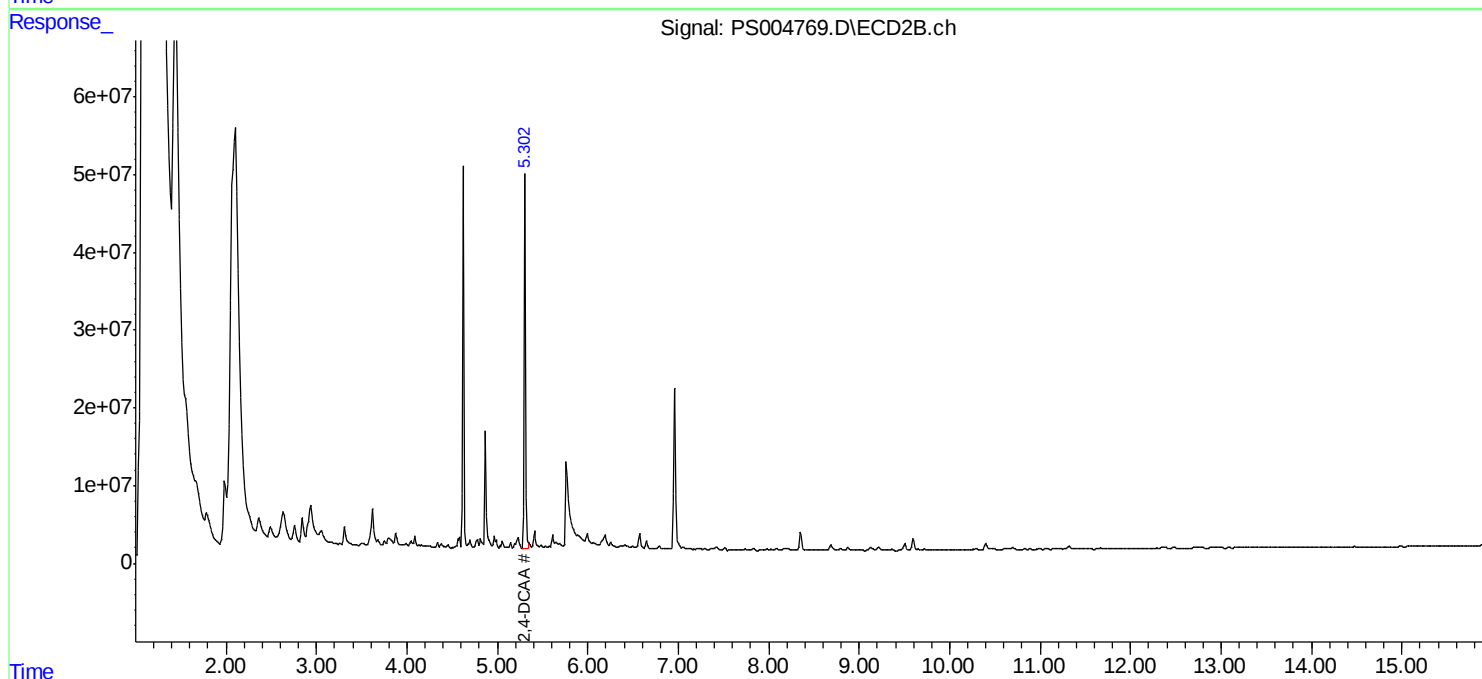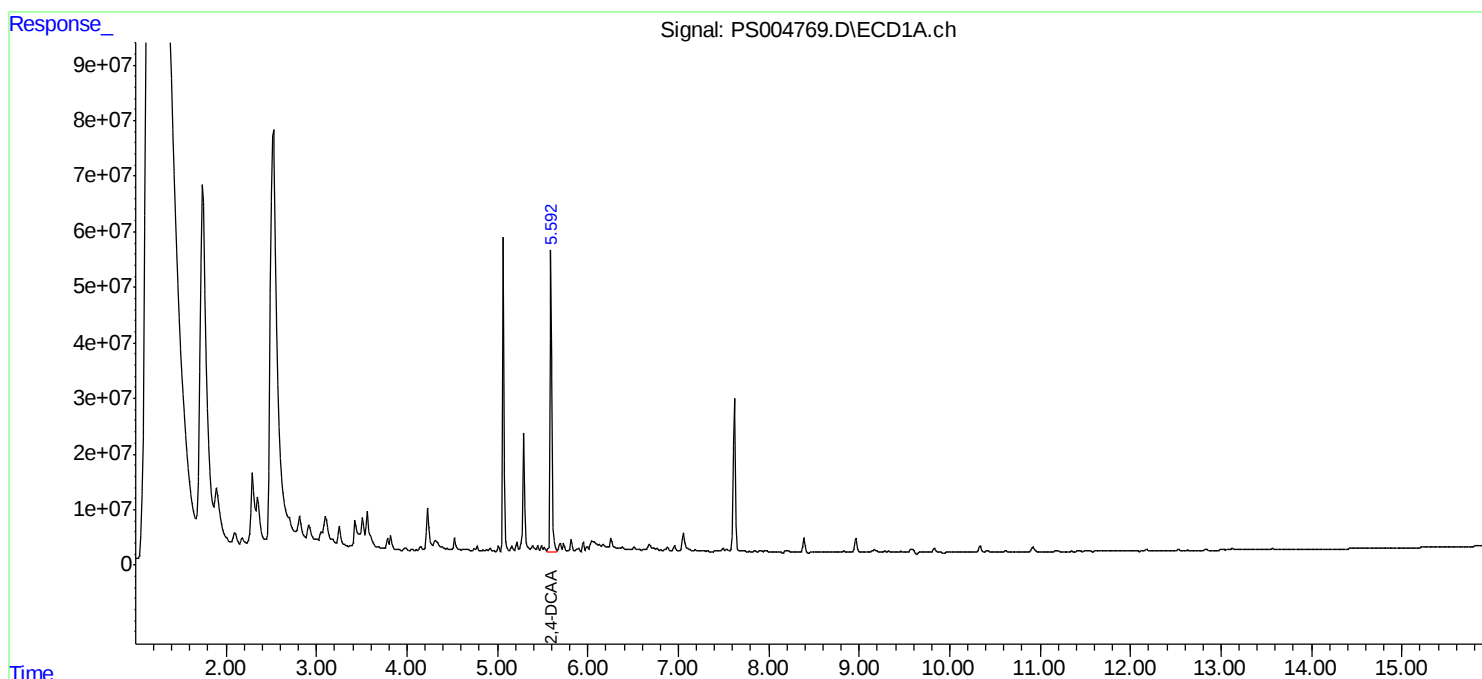

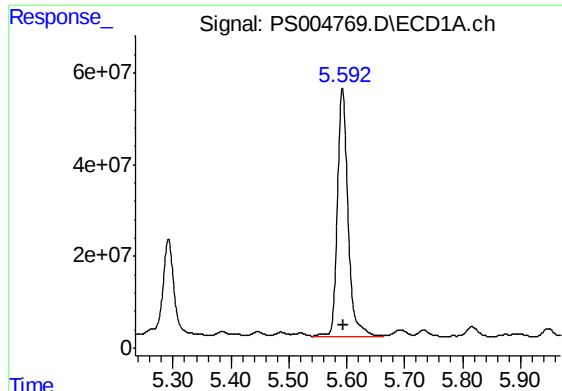


#4 2,4-DCAA

R.T.: 5.593 min
Delta R.T.: -0.002 min
Response: 699722960
Conc: 499.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
SSSI-0523-S-TCLP-11

Manual Integrations
APPROVED

Ankita
5/28/2019 11:02:18 AM

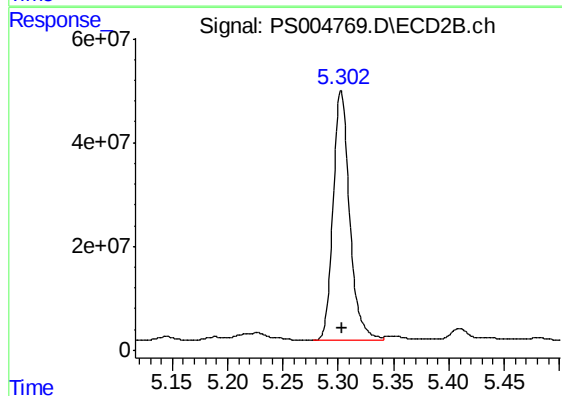

#4 2,4-DCAA

R.T.: 5.302 min
Delta R.T.: -0.002 min
Response: 502067777
Conc: 520.37 ng/ml m