

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052522\
 Data File : PS019517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 May 2022 14:14
 Operator : AJ\MA
 Sample : I,BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 00:07:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.782	1027.3E6	387.3E6	428.184	499.769
Target Compounds							
7) T	MCPA	7.654f	0.000	2826150	0	<MDL	N.D. #
8) T	DICHLORPROP	8.078	7.609	509393	1746249	<MDL	1.977 #
10) T	Pentachlo...	8.617	8.284	5153505	3385982	<MDL	<MDL #
12) T	2,4,5-T	9.470	9.033	13056785	2893640	<MDL	<MDL #
13) T	2,4-DB	10.037	0.000	17203250	0	4.252	N.D. #
14) T	DINOSEB	11.143	9.863	3805420	214003	<MDL	<MDL #
15) T	Picloram	10.965	10.857	10185289	10083426	<MDL	1.568 #
16) T	DCPA	11.436	0.000	1498444	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052522\
Data File : PS019517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 May 2022 14:14
Operator : AJ\MA
Sample : I,BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 00:07:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

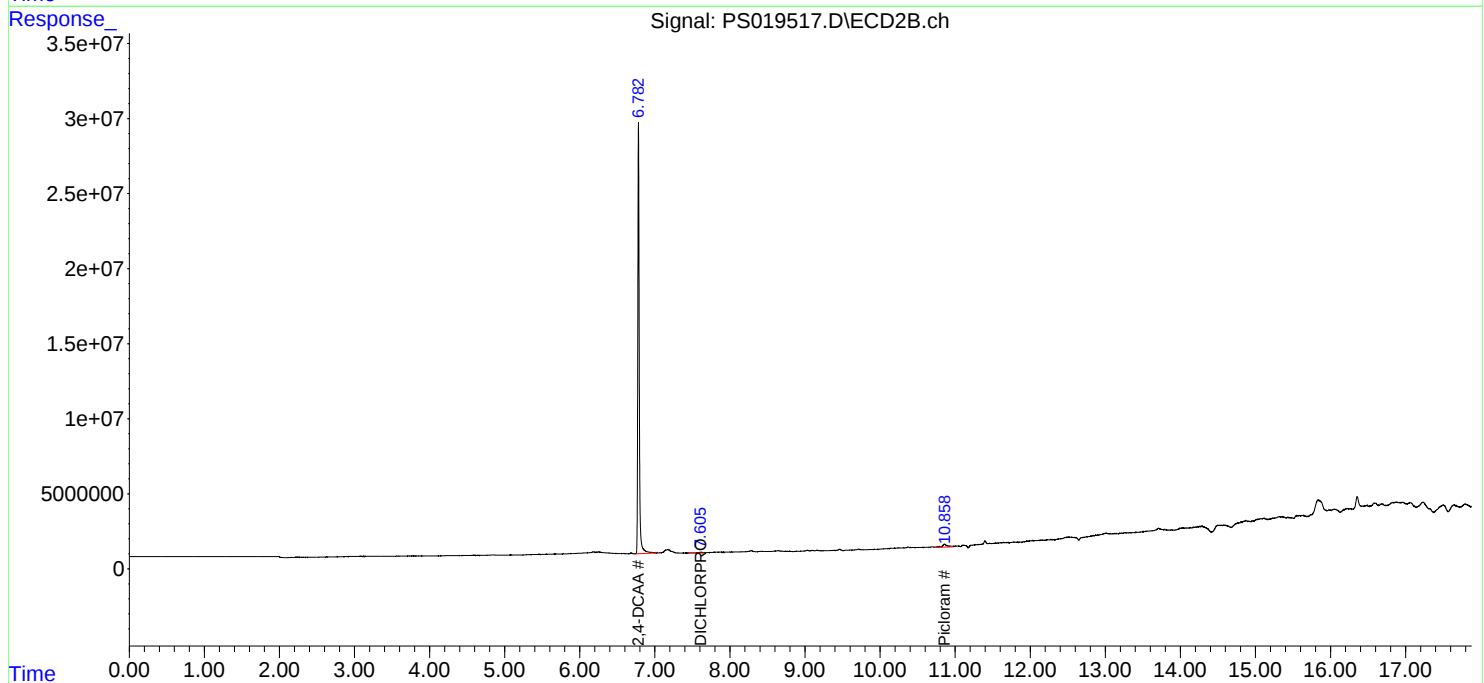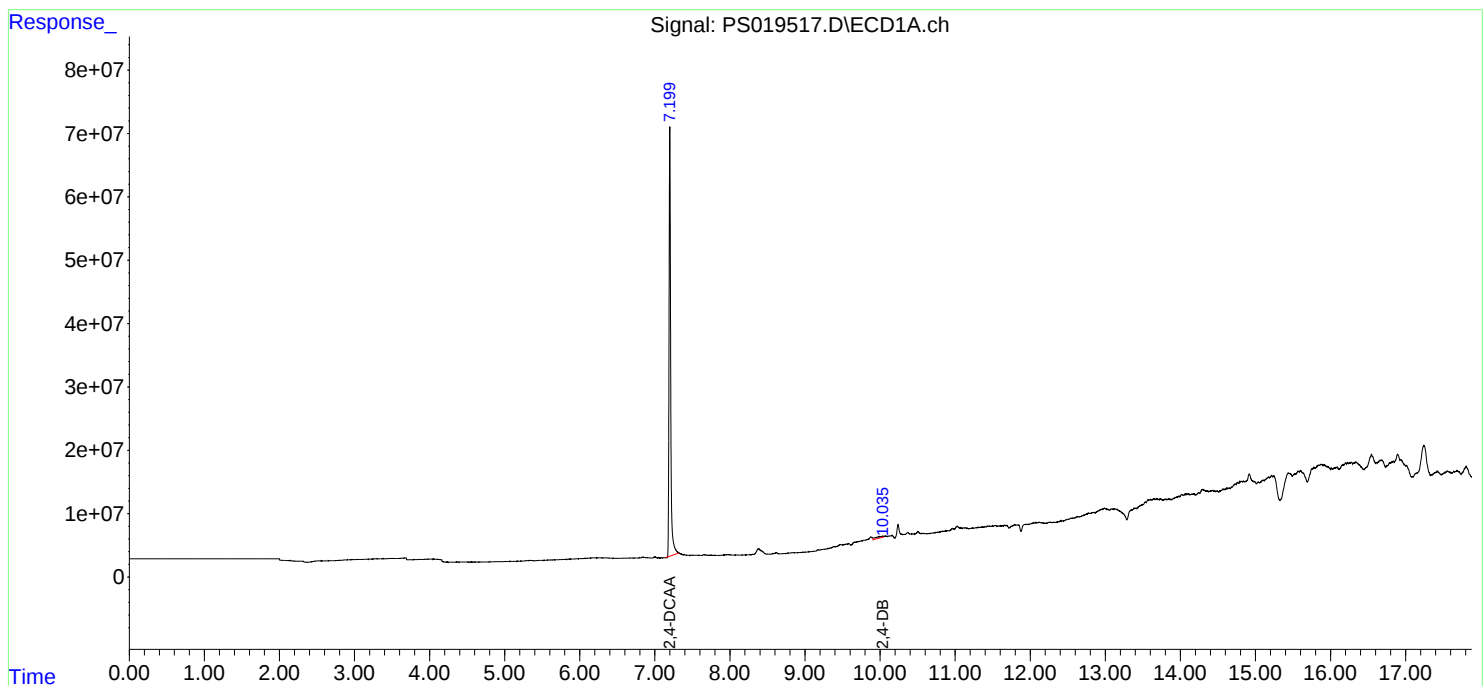


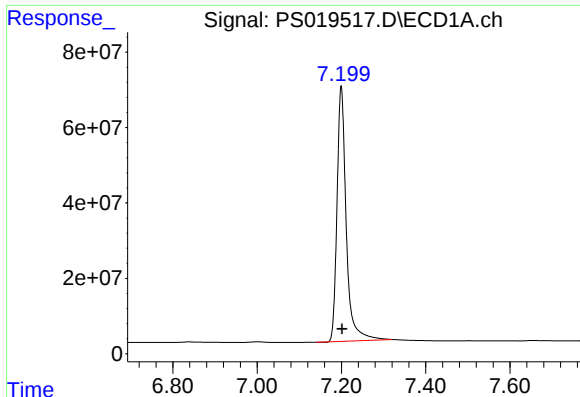

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1027285533
Conc: 428.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

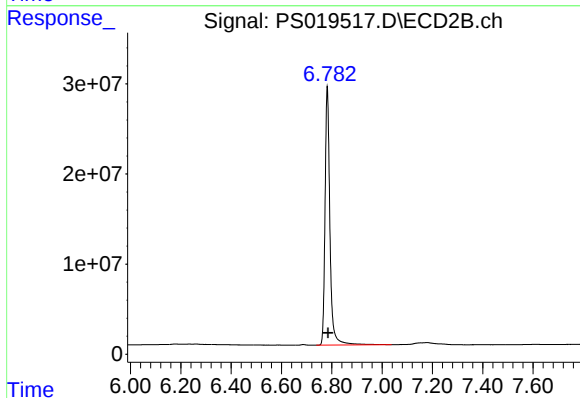


#4 2,4-DCAA

R.T.: 6.782 min
Delta R.T.: -0.002 min
Response: 387256078
Conc: 499.77 ng/ml

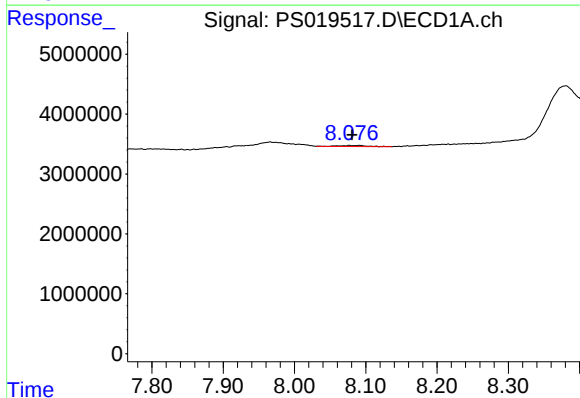


#8 DICHLORPROP

R.T.: 8.078 min
Delta R.T.: -0.003 min
Response: 509393
Conc: N.D.

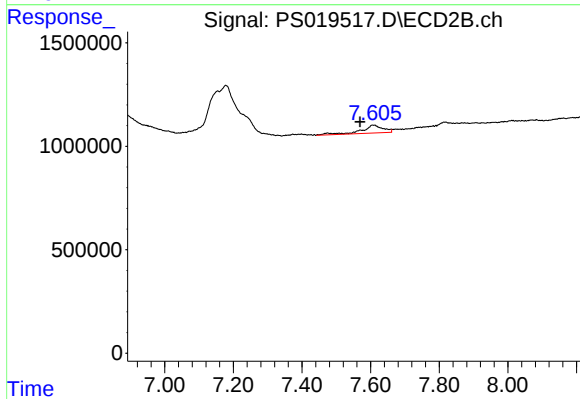

#8 DICHLORPROP


R.T.: 7.609 min
Delta R.T.: 0.040 min
Response: 1746249
Conc: 1.98 ng/ml

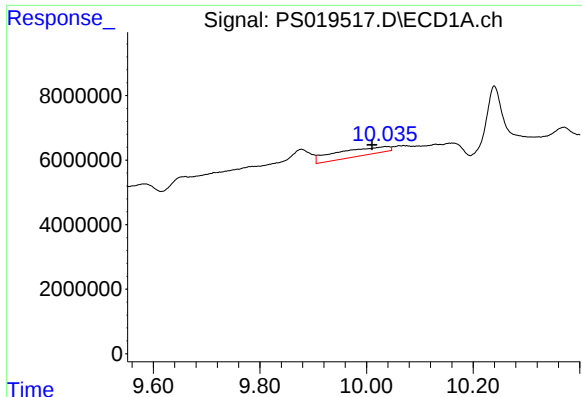

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: 0.027 min
Response: 17203250
Conc: 4.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

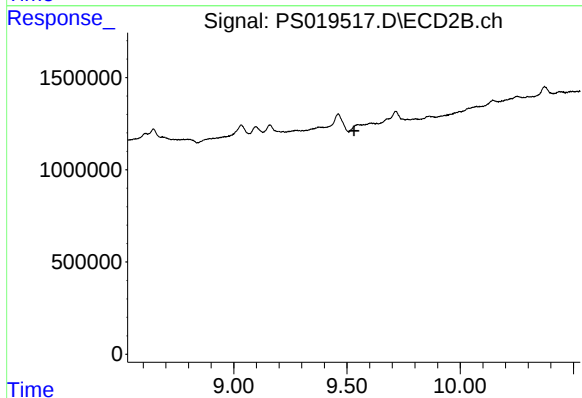


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.531 min
Response: 0
Conc: N.D.

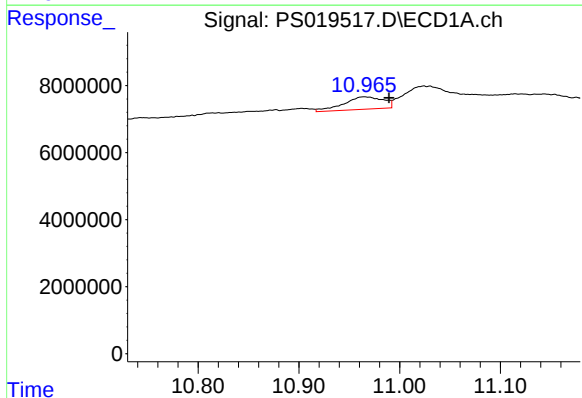

#15 Picloram

R.T.: 10.965 min
Delta R.T.: -0.024 min
Response: 10185289
Conc: N.D.

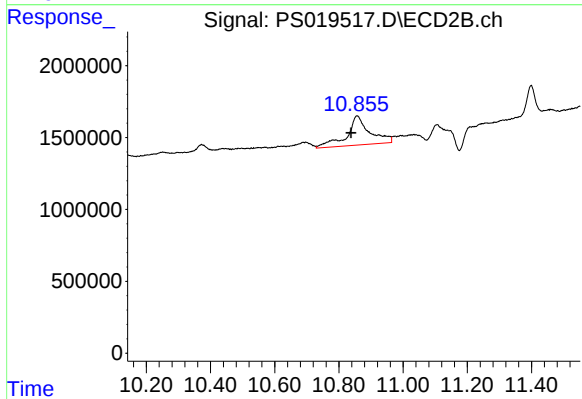

#15 Picloram

R.T.: 10.857 min
Delta R.T.: 0.020 min
Response: 10083426
Conc: 1.57 ng/ml