

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
 Data File : PS019519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 09:20
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 16:15:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.134f	0.000	462622	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	3.052	0.000	1905172	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.453	0.000	116790	0	<MDL	N.D. #
3) T	4-Nitroph...	6.988f	0.000	1022376	0	1.042	N.D. #
5) T	DICAMBA	0.000	7.008f	0	207822	N.D.	<MDL
6) T	MCPD	0.000	7.008	0	207822	N.D.	<MDL
7) T	MCPA	7.752f	0.000	1715602	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.630f	0	381384	N.D.	<MDL
9) T	2,4-D	0.000	7.826	0	40671	N.D.	<MDL
10) T	Pentachlo...	8.620	0.000	179069	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.617	0	120259	N.D.	<MDL
13) T	2,4-DB	0.000	9.565	0	360910	N.D.	<MDL
15) T	Picloram	10.966	10.812	29358086	69065	<MDL	<MDL #
16) T	DCPA	11.426	10.787	2113469	571866	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
Data File : PS019519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 09:20
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 16:15:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

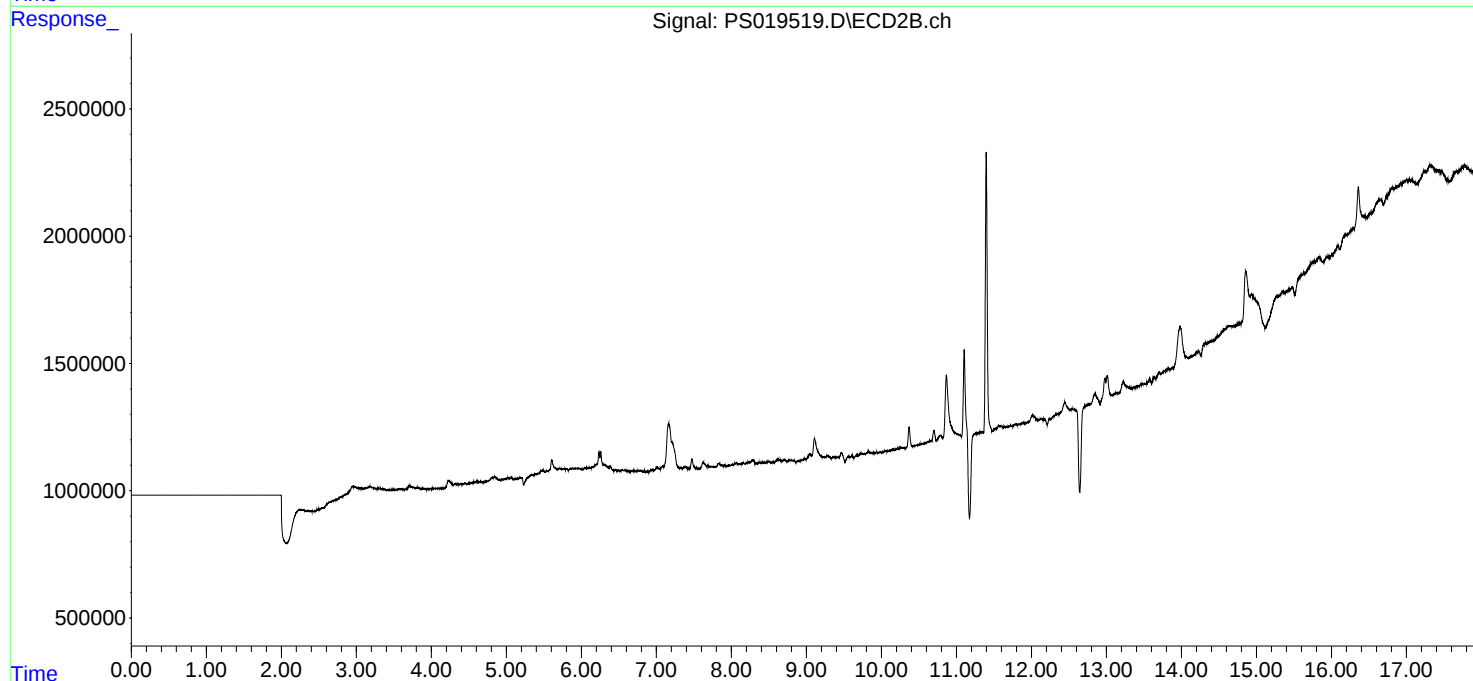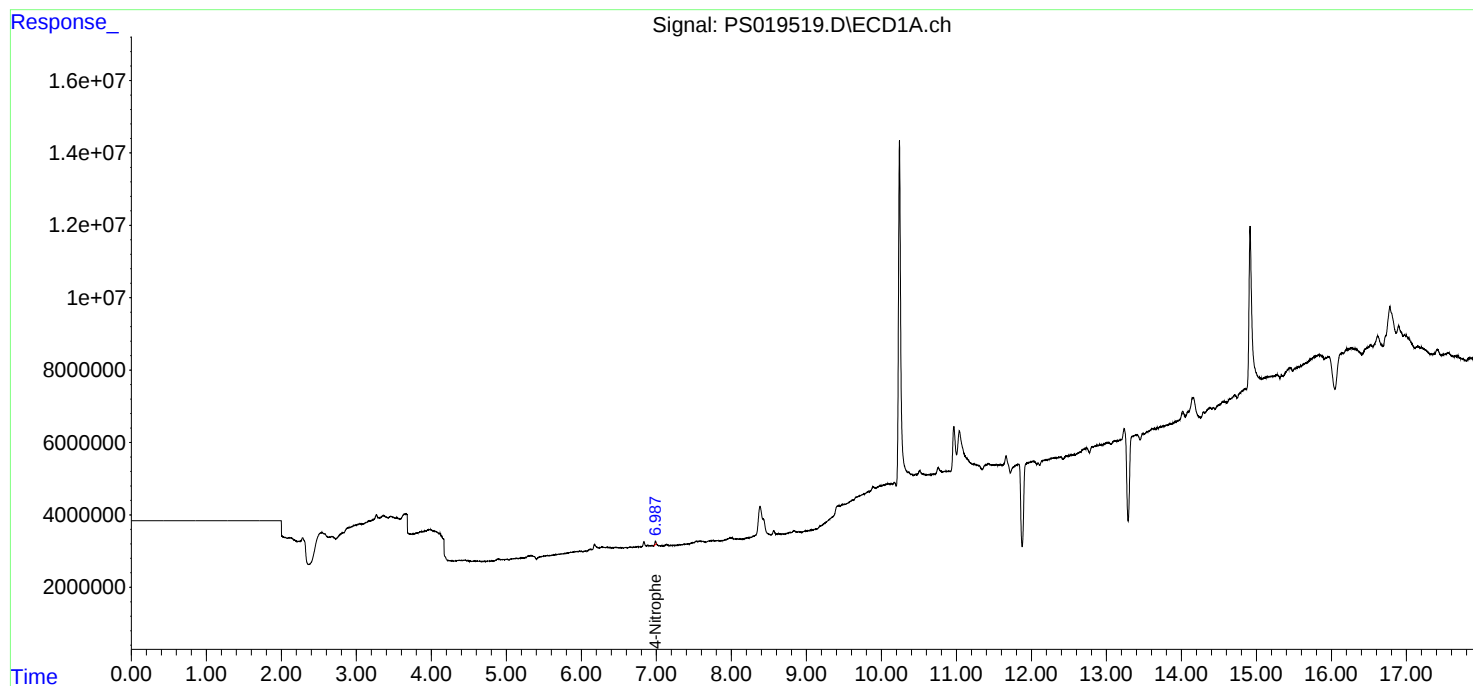


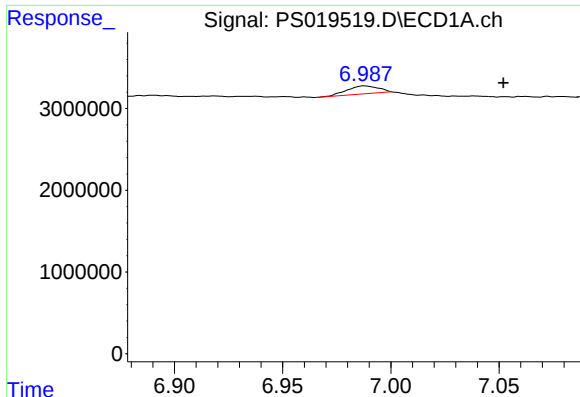

#3 4-Nitrophenol


R.T.: 6.988 min
Delta R.T.: -0.064 min
Response: 1022376
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

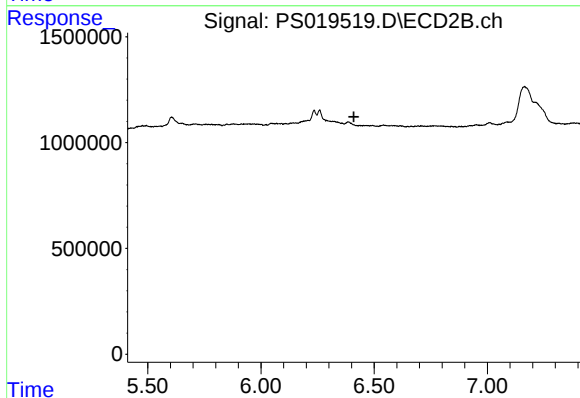


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

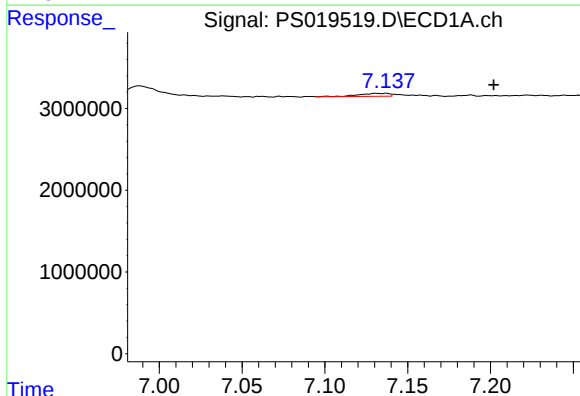

#4 2,4-DCAA

R.T.: 7.134 min
Delta R.T.: -0.068 min
Response: 462622
Conc: N.D.

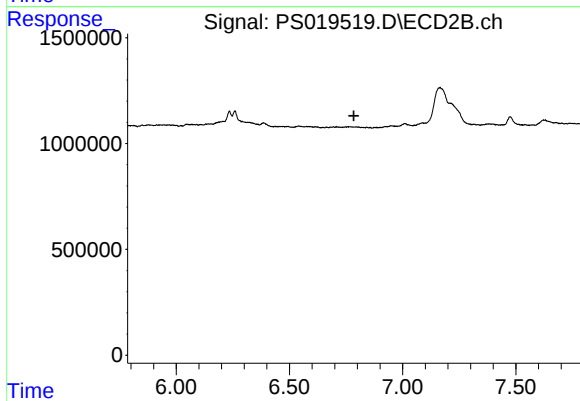

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.