

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
 Data File : PS019520.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 09:44
 Operator : AJ\MA
 Sample : I,BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 16:15:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.199	6.782	1030.2E6	397.3E6	429.417	512.683
Target Compounds							
1) T	Dalapon	3.046	2.560	613197	151432	<MDL	<MDL #
2) T	3,5-DICHL...	6.359f	0.000	645256	0	<MDL	N.D. #
6) T	MCP	0.000	7.083f	0	250331	N.D.	<MDL
7) T	MCPA	7.658f	7.180f	1491492	3963797	<MDL	1.032 #
8) T	DICHLORPROP	0.000	7.628f	0	714298	N.D.	<MDL
10) T	Pentachlo...	8.623	8.285	493118	1730494	<MDL	<MDL #
11) T	2,4,5-TP ...	9.128	0.000	3461896	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	9.058	0	274807	N.D.	<MDL
13) T	2,4-DB	10.043	9.471f	5885705	802338	1.455	1.298
15) T	Picloram	10.970	10.873	16693550	6241521	<MDL	<MDL #
16) T	DCPA	11.425	10.783	1370580	686806	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
Data File : PS019520.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 09:44
Operator : AJ\MA
Sample : I,BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 16:15:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

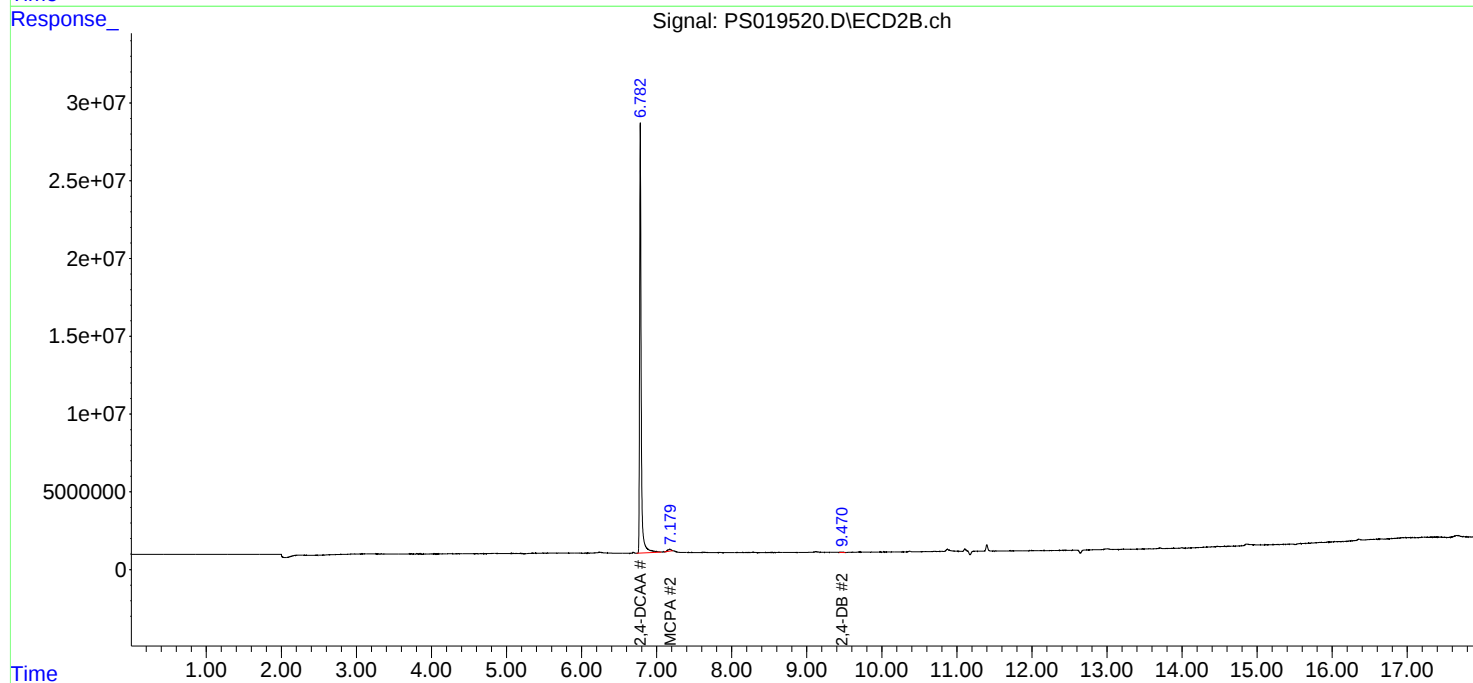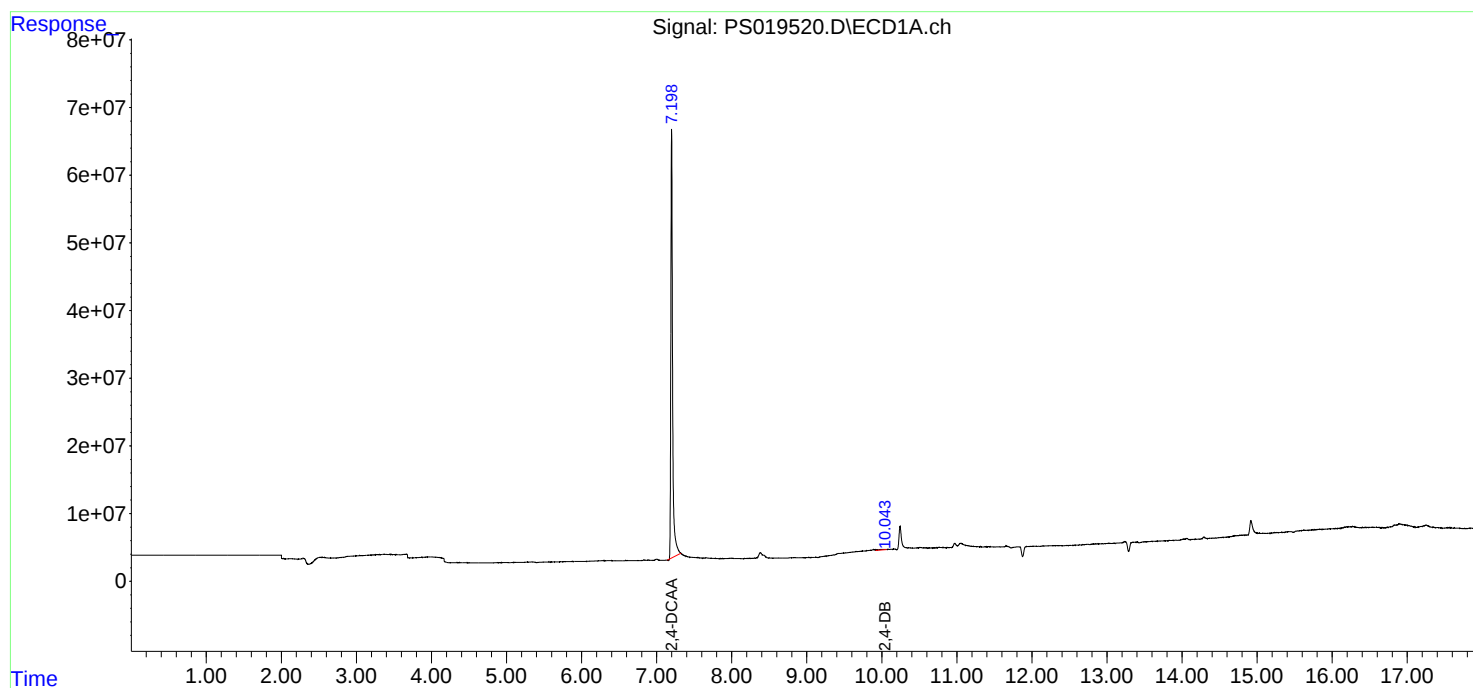


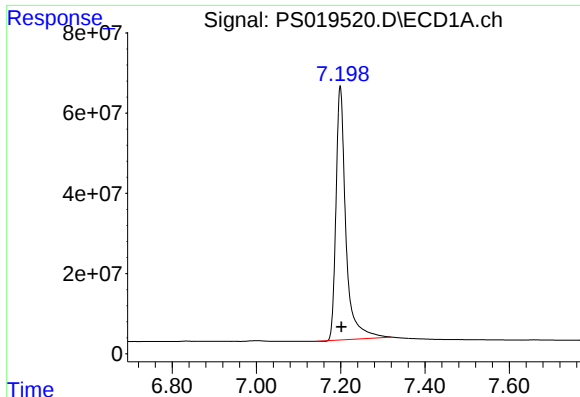

#4 2,4-DCAA


R.T.: 7.199 min
Delta R.T.: -0.003 min
Response: 1030242835
Conc: 429.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

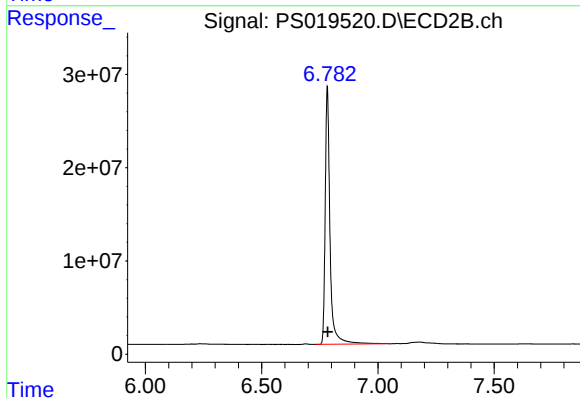


#4 2,4-DCAA

R.T.: 6.782 min
Delta R.T.: -0.002 min
Response: 397262603
Conc: 512.68 ng/ml

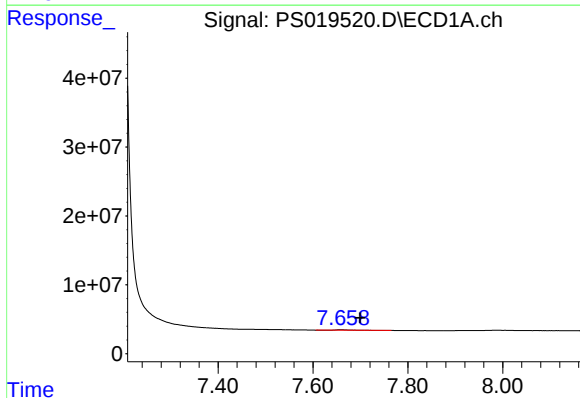


#7 MCPA

R.T.: 7.658 min
Delta R.T.: -0.041 min
Response: 1491492
Conc: N.D.

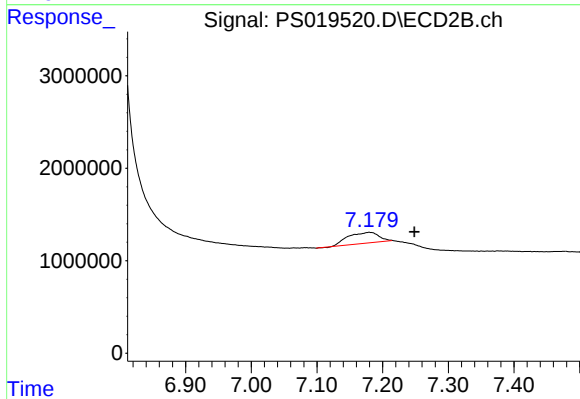

#7 MCPA


R.T.: 7.180 min
Delta R.T.: -0.069 min
Response: 3963797
Conc: 1.03 ug/ml

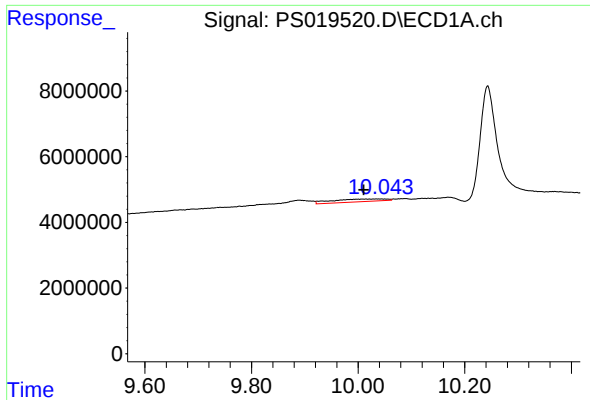

#13 2,4-DB

R.T.: 10.043 min
Delta R.T.: 0.033 min
Response: 5885705
Conc: 1.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

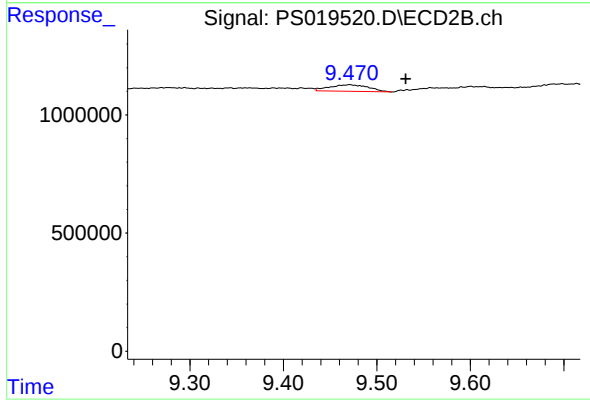

#13 2,4-DB

R.T.: 9.471 min
Delta R.T.: -0.060 min
Response: 802338
Conc: 1.30 ng/ml