

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
 Data File : PS019526.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 14:40
 Operator : AJ\MA
 Sample : PB145041BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:49:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.192	0.000	203744	0	<MDL	N.D.	#
Target Compounds								
2) T	3,5-DICHL...	6.432	5.978	968937	133378	<MDL	<MDL	#
3) T	4-Nitroph...	6.989f	6.381	1805603	2159960	1.840	5.046	#
5) T	DICAMBA	7.425	6.953	319098	107745	<MDL	<MDL	#
7) T	MCPA	7.690	0.000	400.4E6	0	37.059	N.D.	#
8) T	DICHLORPROP	8.109	7.596	402032	5301361	<MDL	6.001	#
10) T	Pentachlo...	8.624	8.280	662666	452064	<MDL	<MDL	#
11) T	2,4,5-TP ...	0.000	8.680	0	1374951	N.D.	<MDL	#
12) T	2,4,5-T	9.470	9.029	12583577	590775	<MDL	<MDL	#
13) T	2,4-DB	10.010	9.557	6793809	1756164	1.679	2.842	#
14) T	DINOSEB	11.125	9.852	40506058	429539	2.619	<MDL	#
15) T	Picloram	11.004	10.844	22066977	7161766	<MDL	1.113	#
16) T	DCPA	11.390	10.784	399209	5069430	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
Data File : PS019526.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 14:40
Operator : AJ\MA
Sample : PB145041BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:49:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

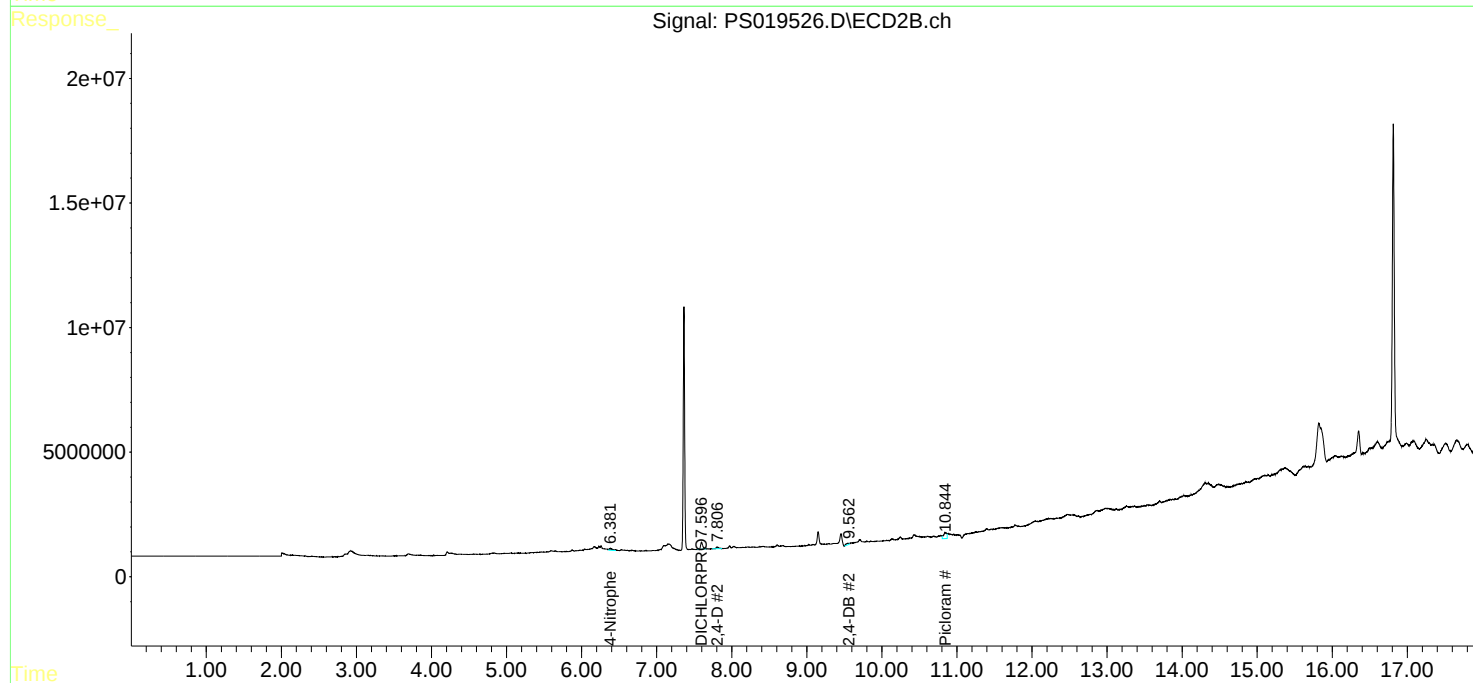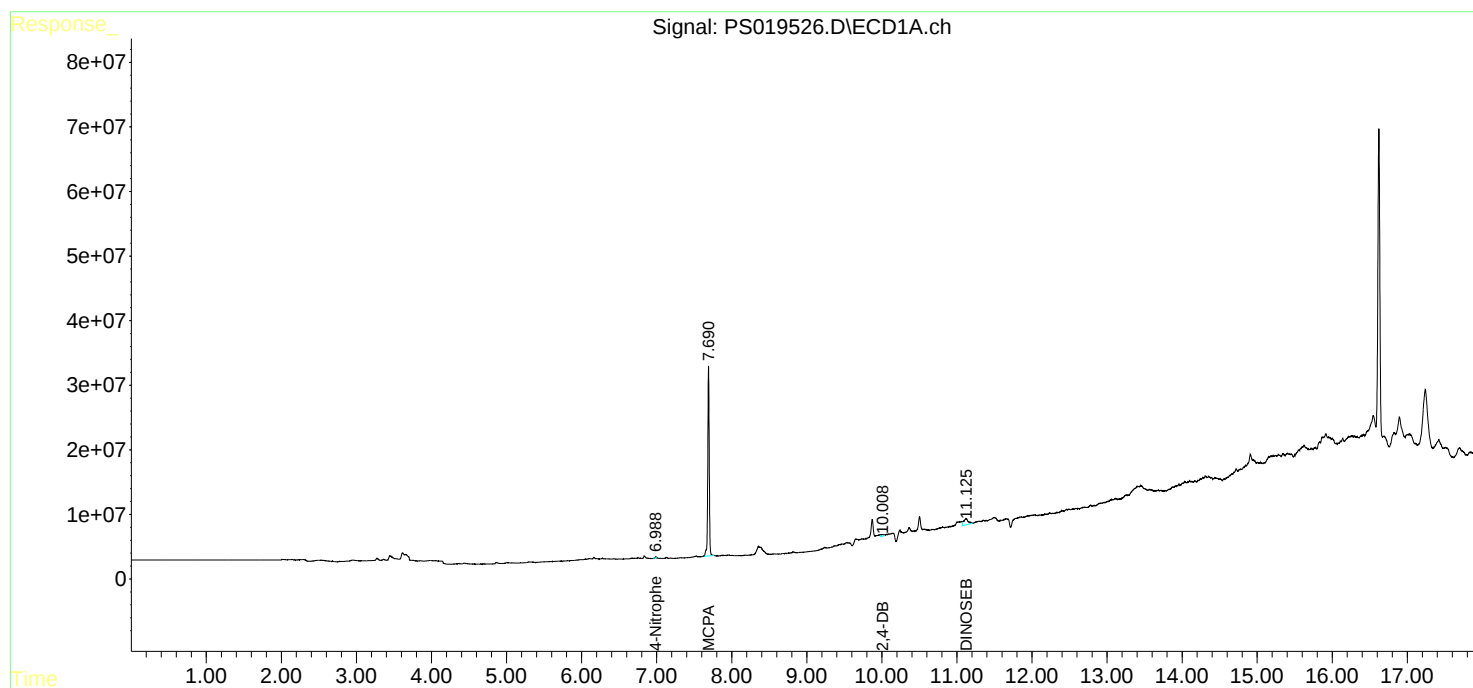


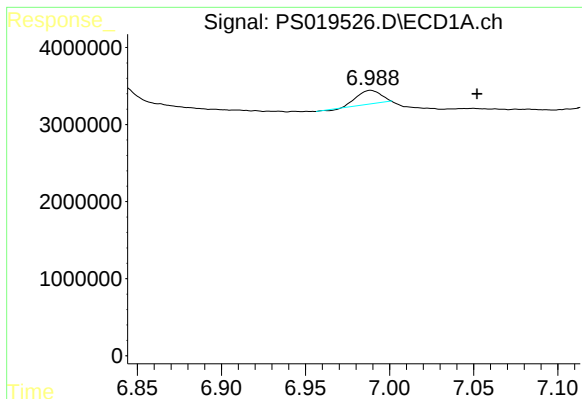

#3 4-Nitrophenol


R.T.: 6.989 min
Delta R.T.: -0.063 min
Response: 1805603
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

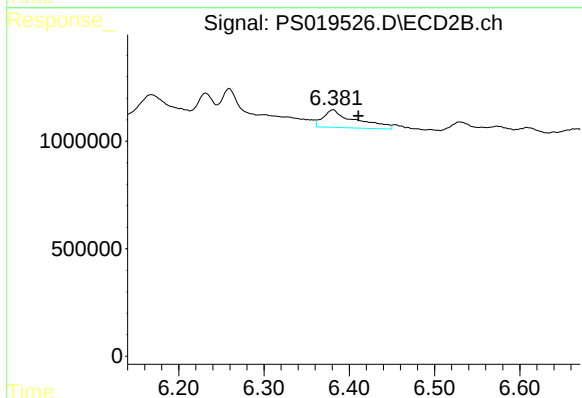


#3 4-Nitrophenol

R.T.: 6.381 min
Delta R.T.: -0.030 min
Response: 2159960
Conc: 5.05 ng/ml

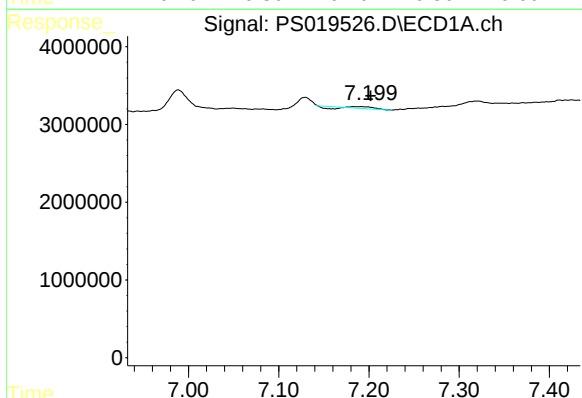


#4 2,4-DCAA

R.T.: 7.192 min
Delta R.T.: -0.010 min
Response: 203744
Conc: N.D.

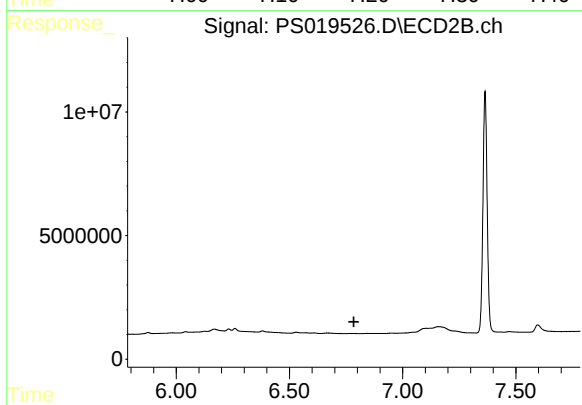

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

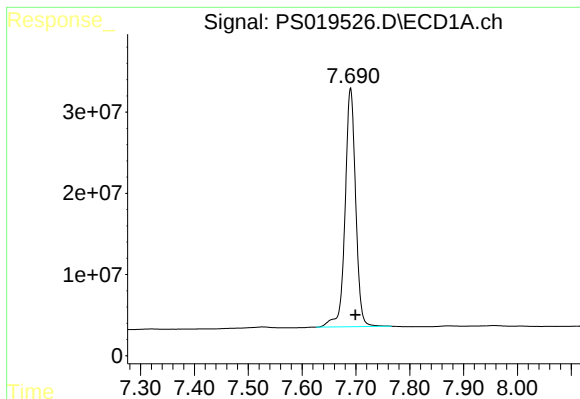

#7 MCPA


R.T.: 7.690 min
Delta R.T.: -0.009 min
Response: 400387739
Conc: 37.06 ug/ml

Instrument :
ECD_S
ClientSampleId :

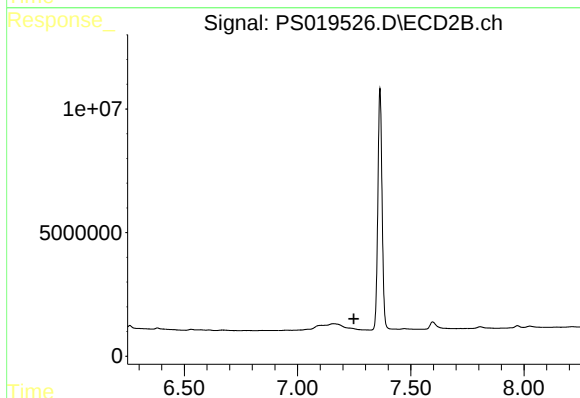


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

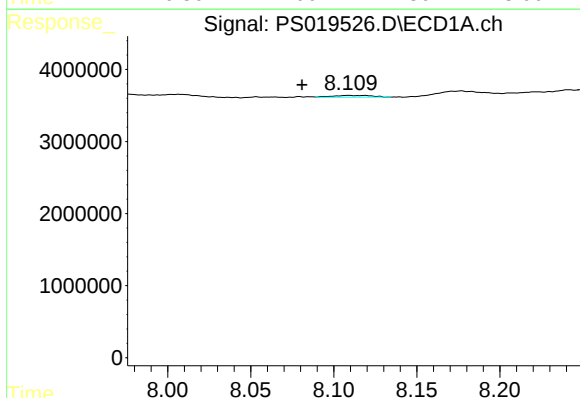


#8 DICHLORPROP

R.T.: 8.109 min
Delta R.T.: 0.028 min
Response: 402032
Conc: N.D.

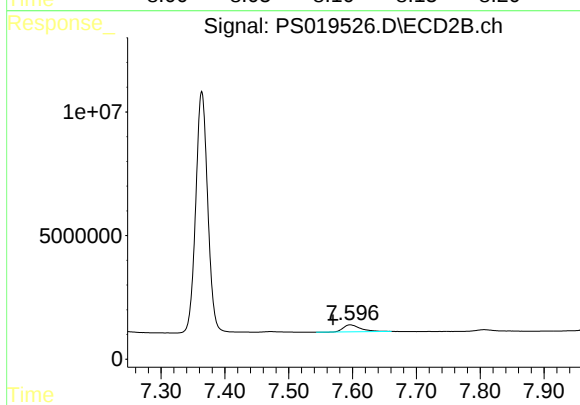

#8 DICHLORPROP


R.T.: 7.596 min
Delta R.T.: 0.027 min
Response: 5301361
Conc: 6.00 ng/ml

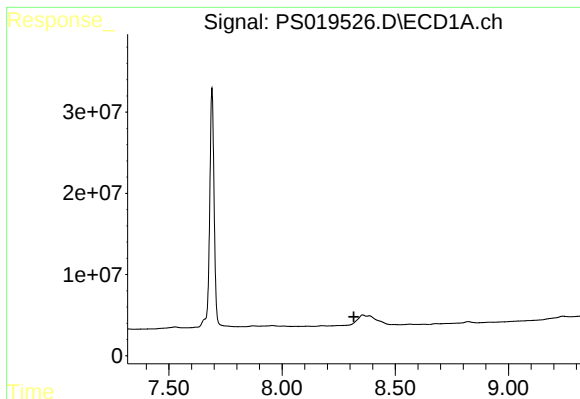

#9 2,4-D


R.T.: 8.355 min
Delta R.T.: 0.038 min
Response: -21797896
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

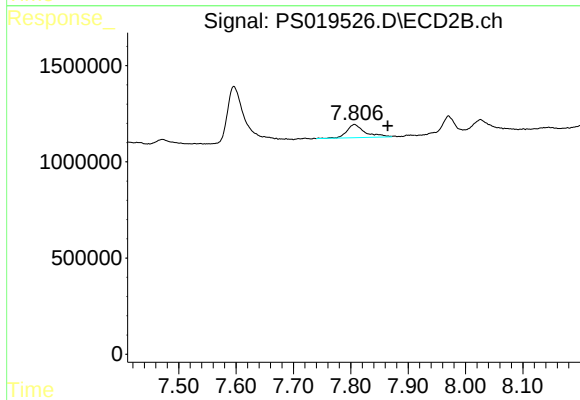


#9 2,4-D

R.T.: 7.806 min
Delta R.T.: -0.058 min
Response: 1501220
Conc: 1.41 ng/ml

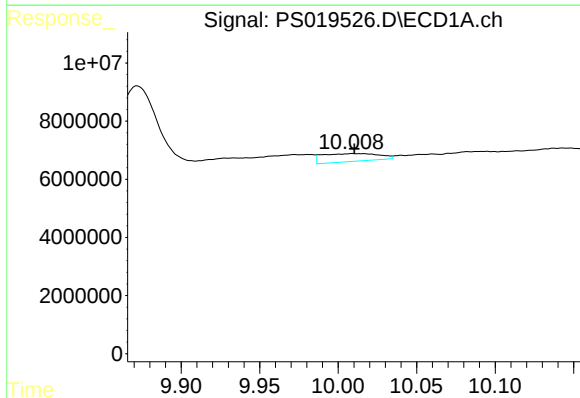


#13 2,4-DB

R.T.: 10.010 min
Delta R.T.: 0.000 min
Response: 6793809
Conc: 1.68 ng/ml

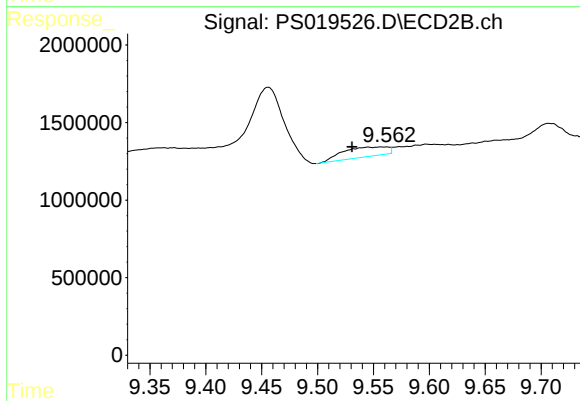

#13 2,4-DB


R.T.: 9.557 min
Delta R.T.: 0.026 min
Response: 1756164
Conc: 2.84 ng/ml

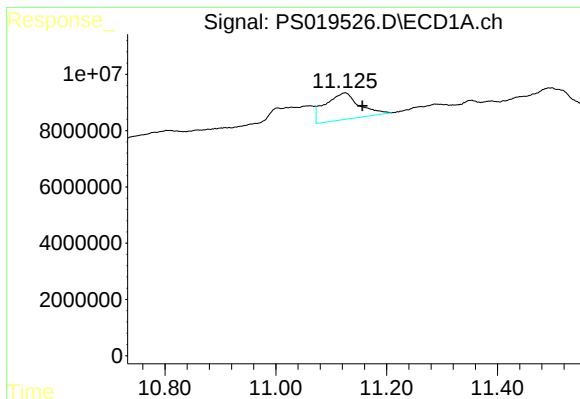

#14 DINoseb


R.T.: 11.125 min
Delta R.T.: -0.031 min
Response: 40506058
Conc: 2.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

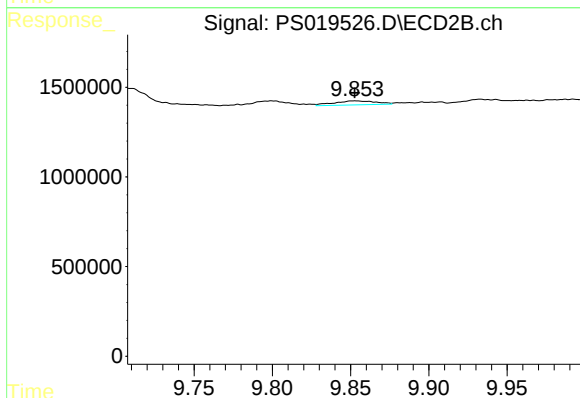


#14 DINoseb

R.T.: 9.852 min
Delta R.T.: 0.000 min
Response: 429539
Conc: N.D.

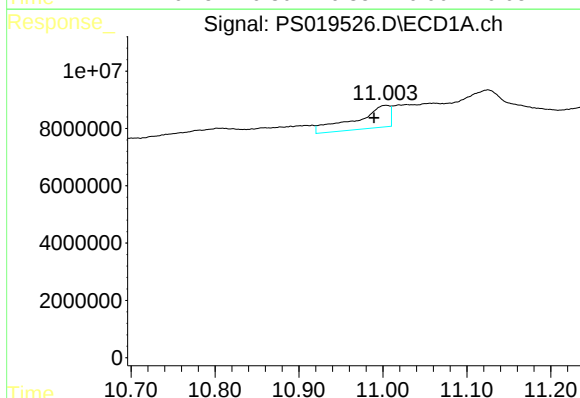

#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.014 min
Response: 22066977
Conc: N.D.

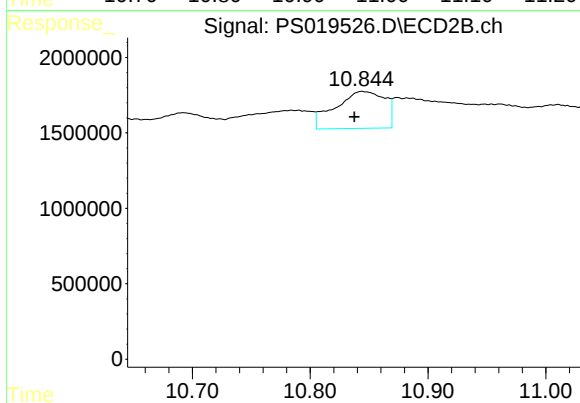

#15 Picloram

R.T.: 10.844 min
Delta R.T.: 0.007 min
Response: 7161766
Conc: 1.11 ng/ml