

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
 Data File : PS019532.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2022 19:03
 Operator : AJ\MA
 Sample : I,BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 00:51:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.198	6.782	1115.2E6	414.0E6	464.841	534.238
Target Compounds							
1) T	Dalapon	3.044	0.000	349090	0	<MDL	N.D. #
6) T	MCPD	0.000	7.052	0	19723	N.D.	<MDL
7) T	MCPA	7.653f	0.000	4696133	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.604	0	1816070	N.D.	2.056
9) T	2,4-D	0.000	7.814f	0	631290	N.D.	<MDL
10) T	Pentachlo...	8.619	8.286	685462	1336365	<MDL	<MDL #
11) T	2,4,5-TP ...	9.129	8.606f	1774900	822448	<MDL	<MDL #
12) T	2,4,5-T	9.469	9.035	13532541	-835787	<MDL	N.D. #
13) T	2,4-DB	10.035	9.545	5628596	383527	1.391	<MDL #
14) T	DINOSEB	11.114f	9.856	18413281	409686	1.190	<MDL #
15) T	Picloram	11.017	10.855	32840668	6409257	1.107	<MDL #
16) T	DCPA	11.429	10.787	-103942	668377	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052622\
Data File : PS019532.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2022 19:03
Operator : AJ\MA
Sample : I,BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 00:51:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

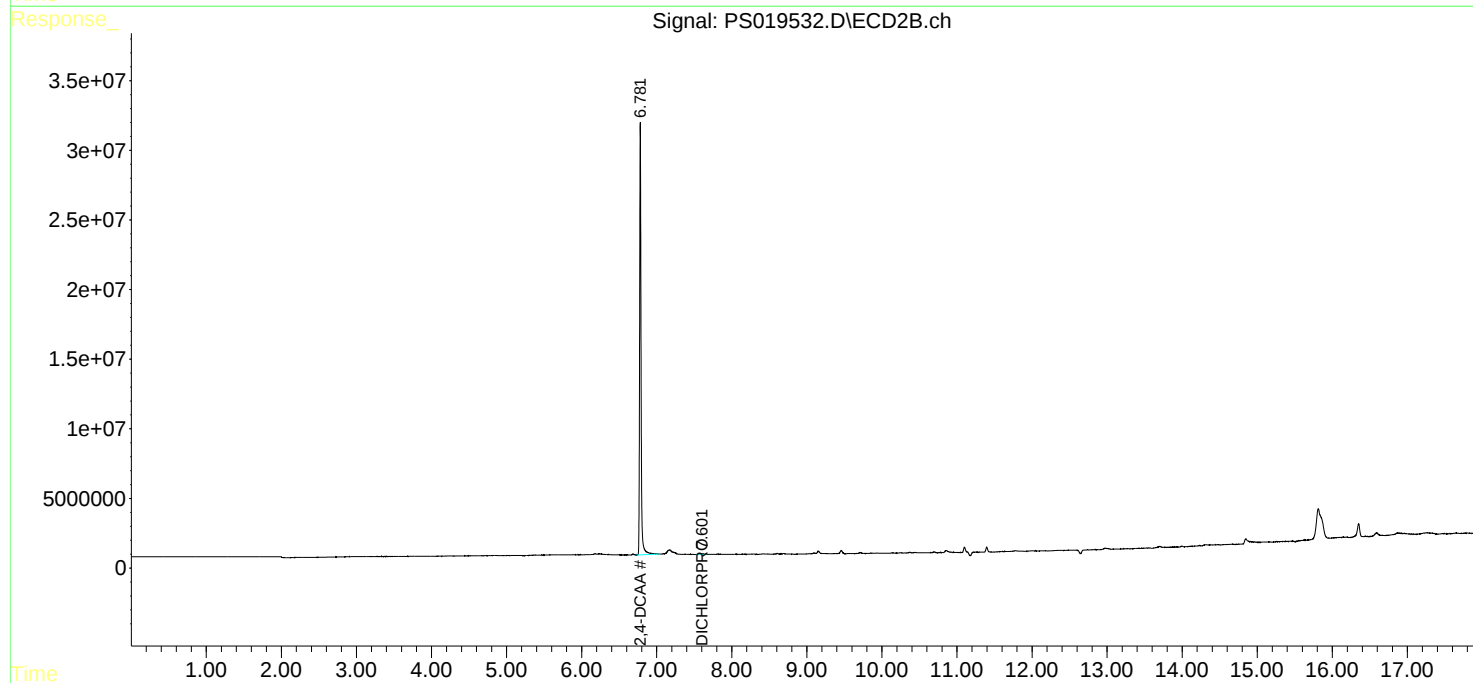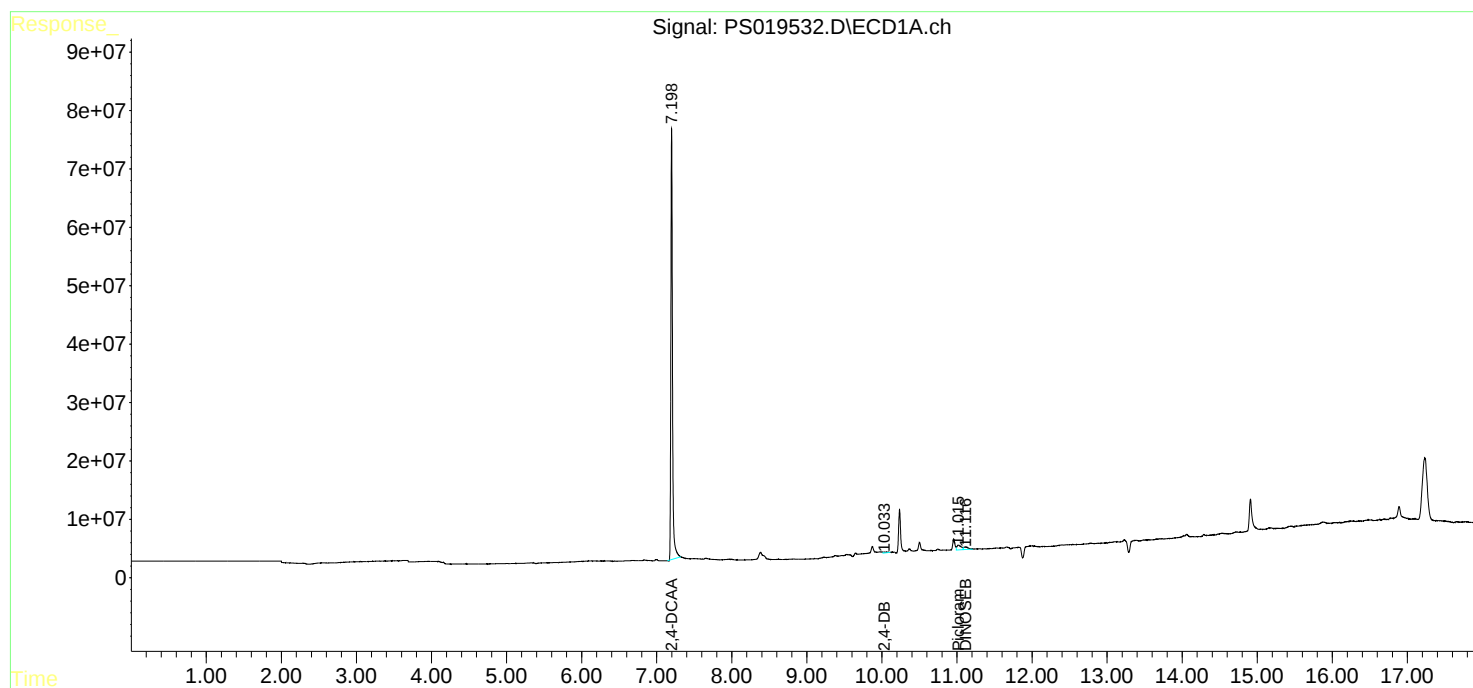


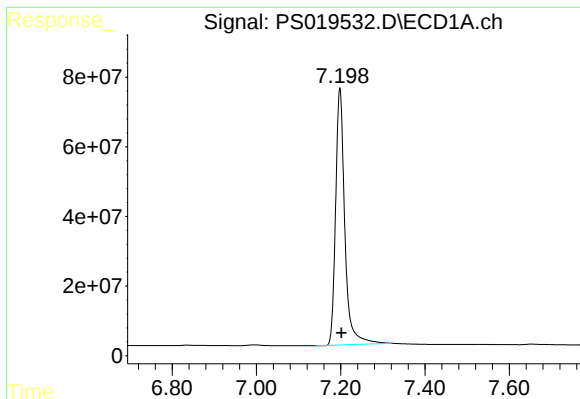

#4 2,4-DCAA


R.T.: 7.198 min
Delta R.T.: -0.004 min
Response: 1115231266
Conc: 464.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

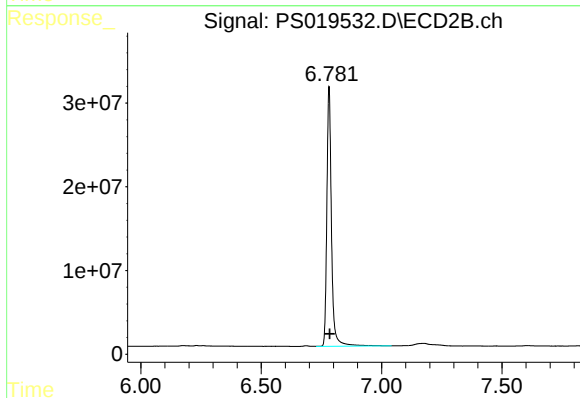


#4 2,4-DCAA

R.T.: 6.782 min
Delta R.T.: -0.003 min
Response: 413965199
Conc: 534.24 ng/ml

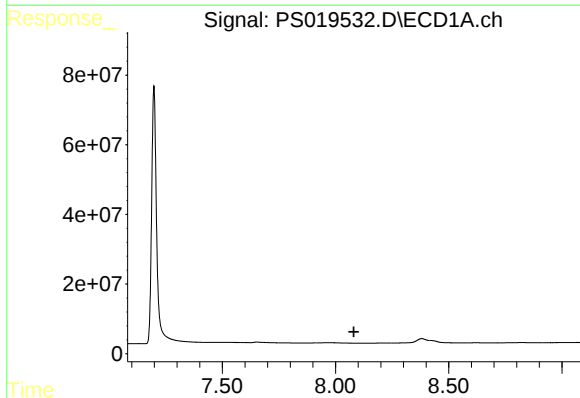


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

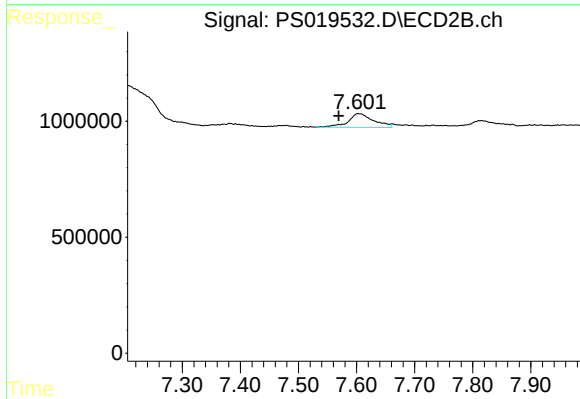

#8 DICHLORPROP


R.T.: 7.604 min
Delta R.T.: 0.035 min
Response: 1816070
Conc: 2.06 ng/ml

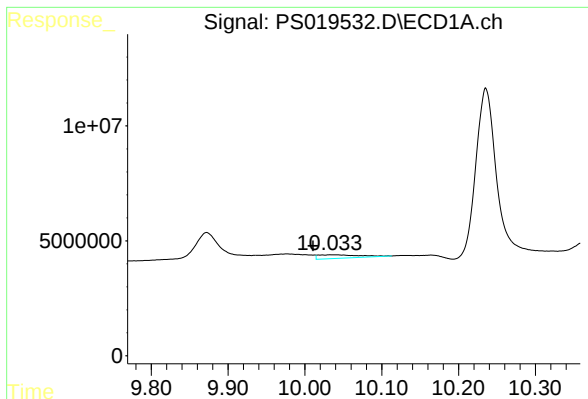

#13 2,4-DB


R.T.: 10.035 min
Delta R.T.: 0.025 min
Response: 5628596
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

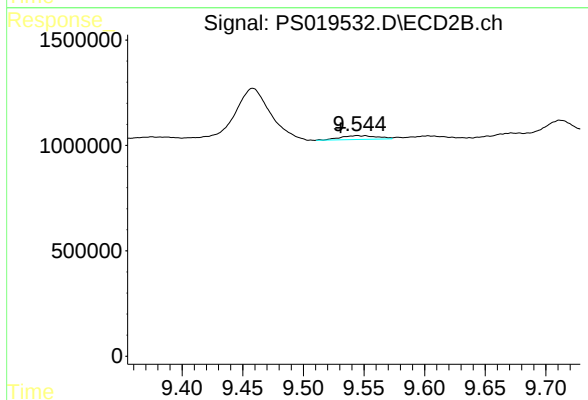


#13 2,4-DB

R.T.: 9.545 min
Delta R.T.: 0.014 min
Response: 383527
Conc: N.D.

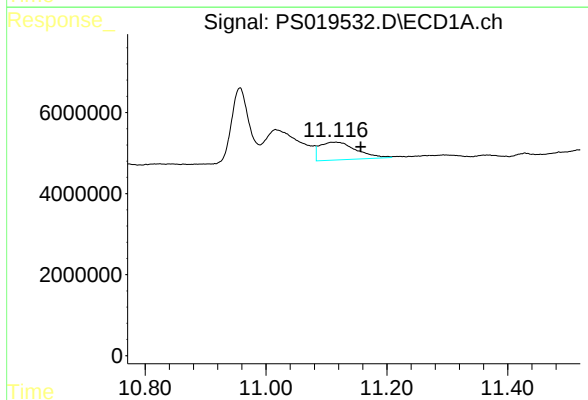


#14 DINOSEB

R.T.: 11.114 min
Delta R.T.: -0.042 min
Response: 18413281
Conc: 1.19 ng/ml

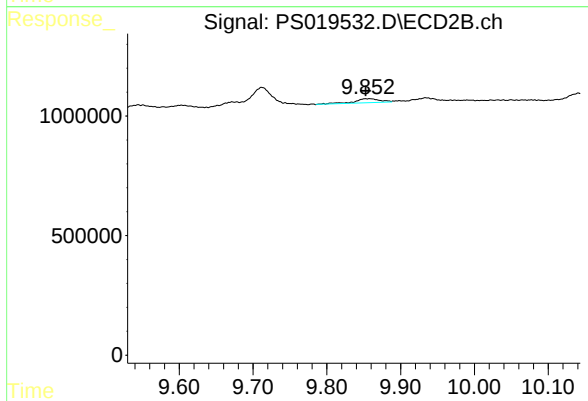

#14 DINOSEB


R.T.: 9.856 min
Delta R.T.: 0.003 min
Response: 409686
Conc: N.D.

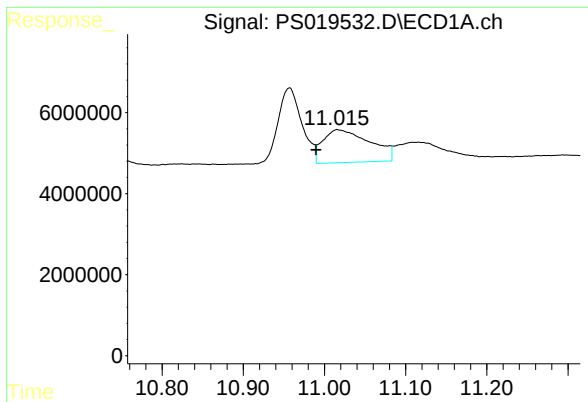

#15 Picloram

R.T.: 11.017 min
Delta R.T.: 0.027 min
Response: 32840668
Conc: 1.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

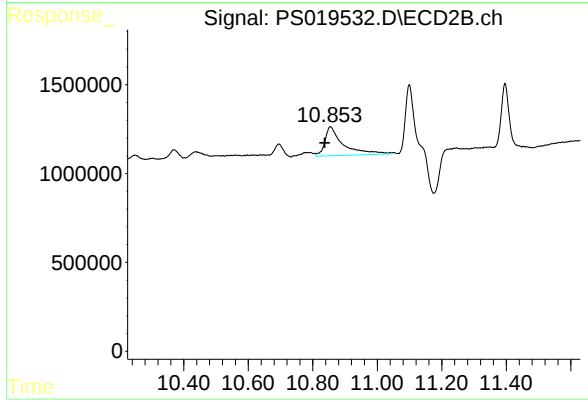

#15 Picloram

R.T.: 10.855 min
Delta R.T.: 0.017 min
Response: 6409257
Conc: N.D.