

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052623\
 Data File : PS023138.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2023 11:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 21:26:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.485	6.857	819.9E6	309.4E6	539.034	551.418
Target Compounds							
1) T	Dalapon	2.574	0.000	1856883	0	1.148	N.D. #
3) T	4-Nitroph...	6.318	0.000	7731653	0	7.344	N.D. #
5) T	DICAMBA	0.000	7.077f	0	2748452	N.D.	1.103
6) T	MCP	6.754	7.077f	151244	2748452	<MDL	1.553 #
8) T	DICHLORPROP	7.234	7.664	1831866	2323742	<MDL	3.755 #
9) T	2,4-D	7.408	0.000	61935133	0	26.762	N.D. #
10) T	Pentachlo...	7.682	0.000	793508	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.217	0.000	3135128	0	<MDL	N.D. #
12) T	2,4,5-T	8.485	9.145f	2250772	1701781	<MDL	<MDL #
13) T	2,4-DB	8.997	0.000	2127399	0	<MDL	N.D. #
14) T	DINOSEB	10.069	0.000	544218	0	<MDL	N.D. #
15) T	Picloram	9.900	10.903	46136736	5880961	2.690	1.381 #
16) T	DCPA	10.340	10.903	2144138	5880961	<MDL	1.574 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052623\
Data File : PS023138.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2023 11:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 21:26:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

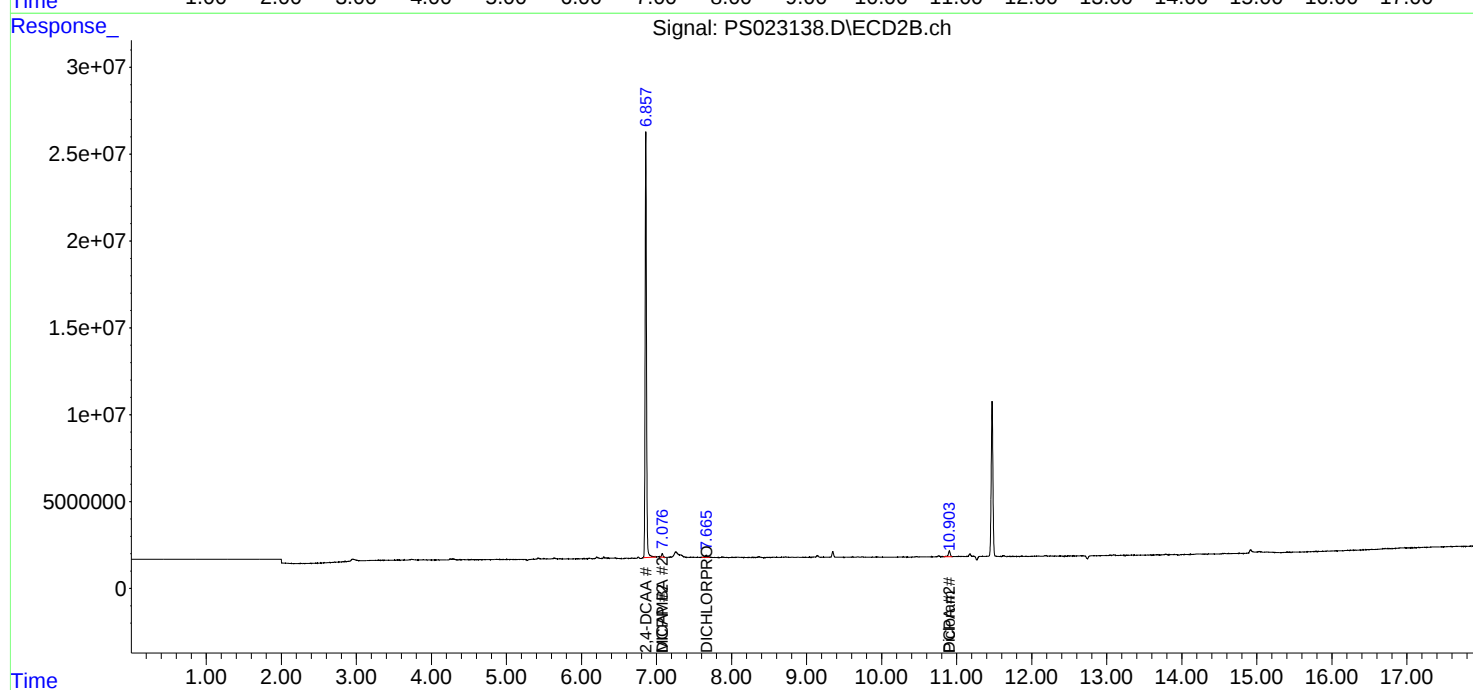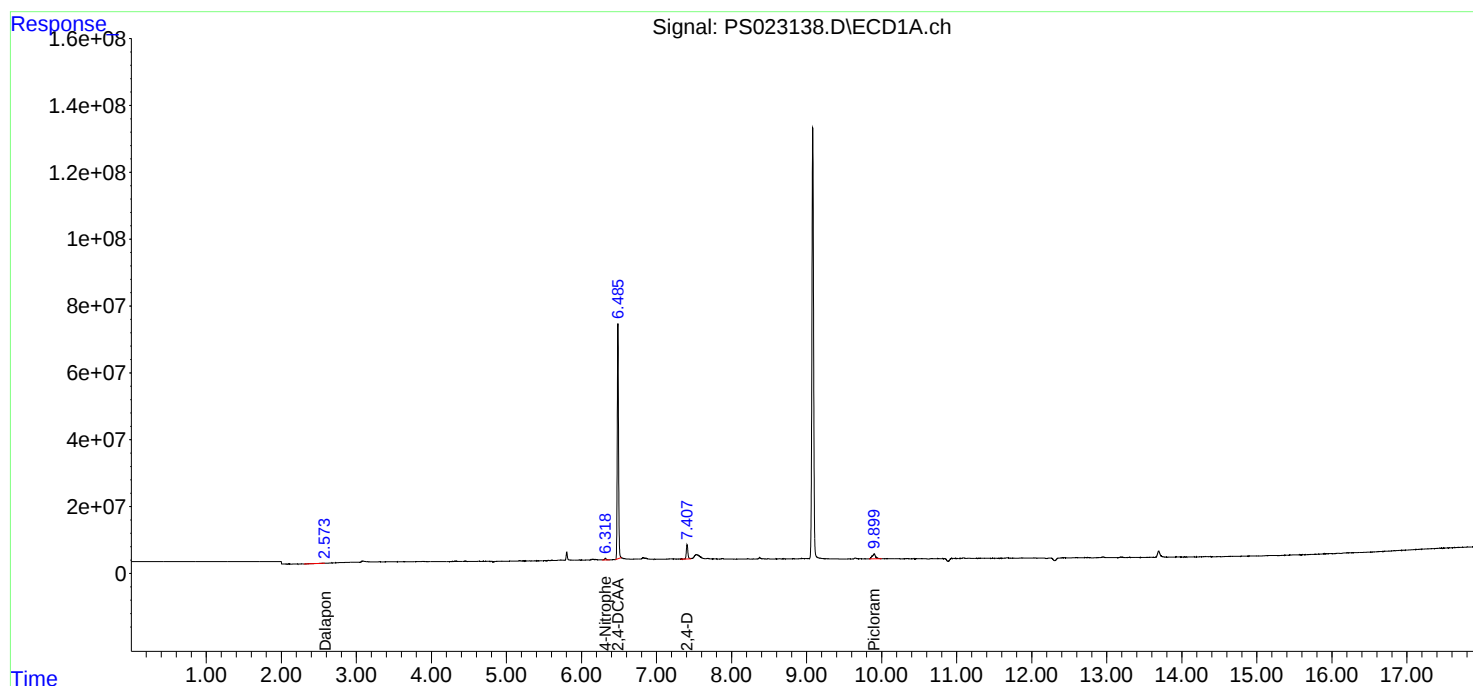


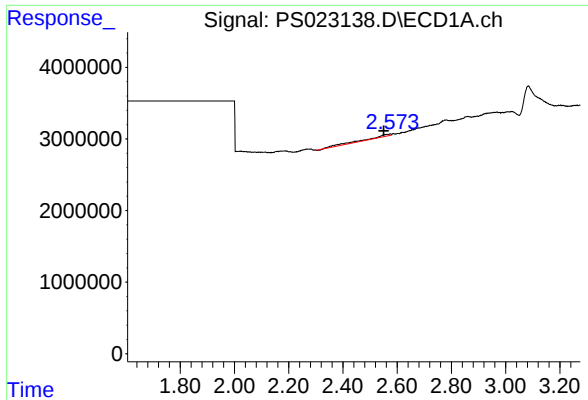

#1 Dalapon


R.T.: 2.574 min
Delta R.T.: 0.023 min
Response: 1856883
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

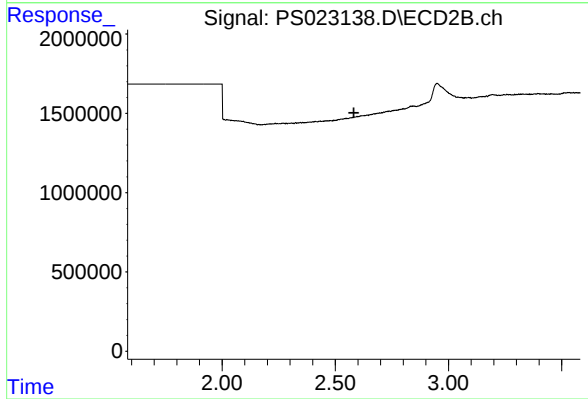


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.582 min
Response: 0
Conc: N.D.

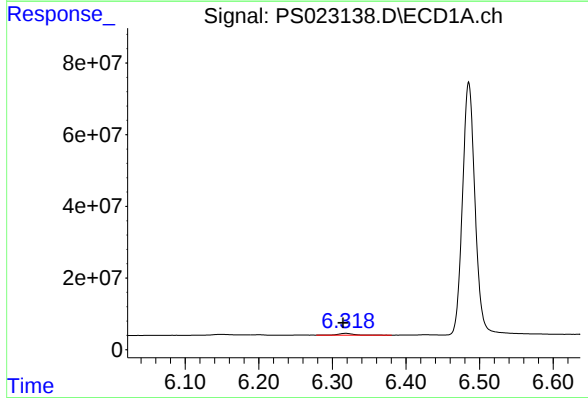


#3 4-Nitrophenol

R.T.: 6.318 min
Delta R.T.: 0.004 min
Response: 7731653
Conc: 7.34 ng/ml

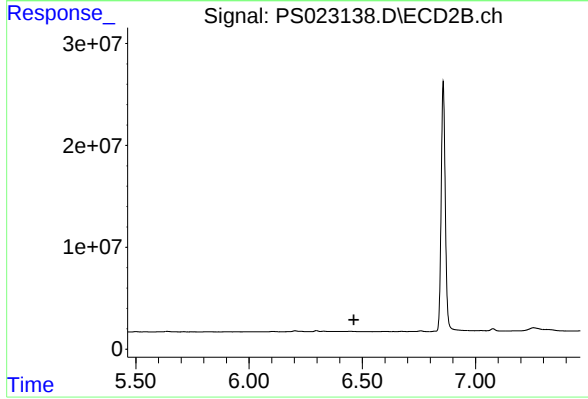

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

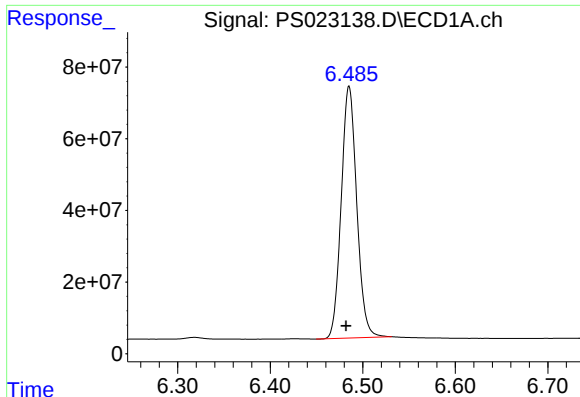

#4 2,4-DCAA


R.T.: 6.485 min
Delta R.T.: 0.003 min
Response: 819867751
Conc: 539.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

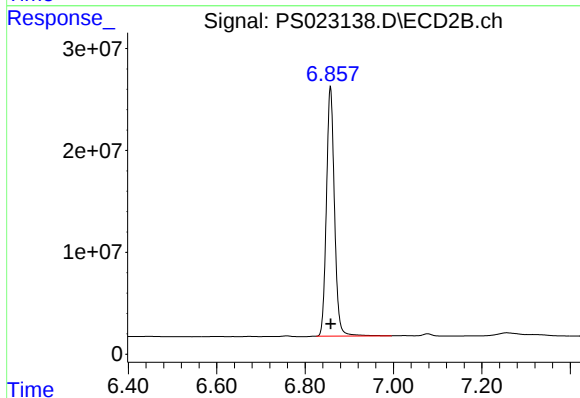


#4 2,4-DCAA

R.T.: 6.857 min
Delta R.T.: 0.000 min
Response: 309409344
Conc: 551.42 ng/ml

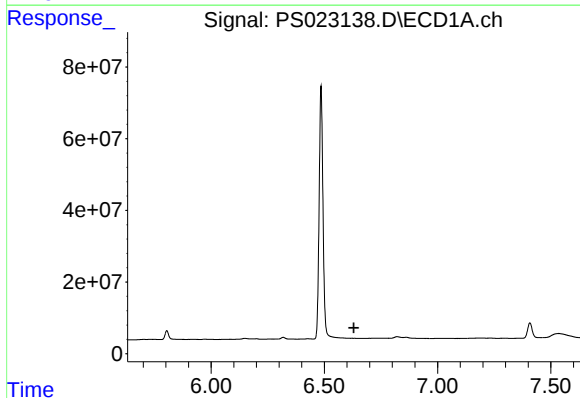


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.631 min
Response: 0
Conc: N.D.

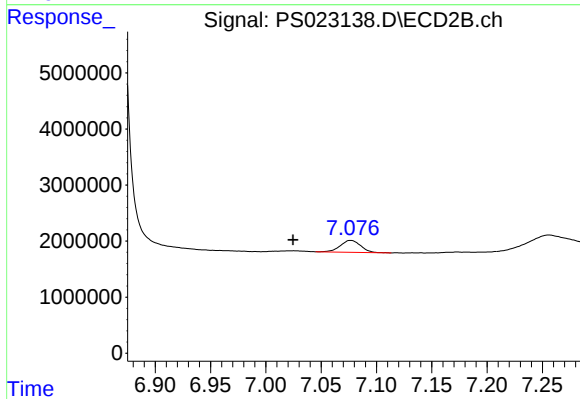

#5 DICAMBA


R.T.: 7.077 min
Delta R.T.: 0.052 min
Response: 2748452
Conc: 1.10 ng/ml

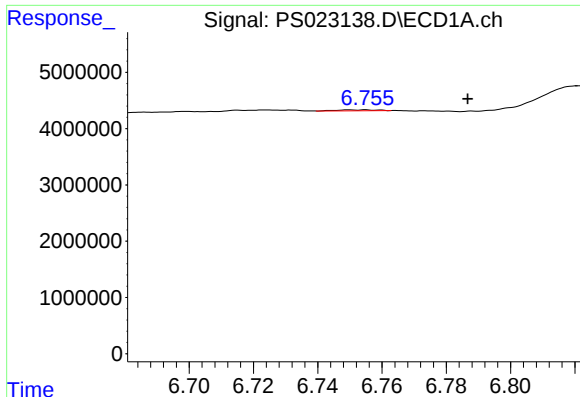

#6 MCPP


R.T.: 6.754 min
Delta R.T.: -0.033 min
Response: 151244
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

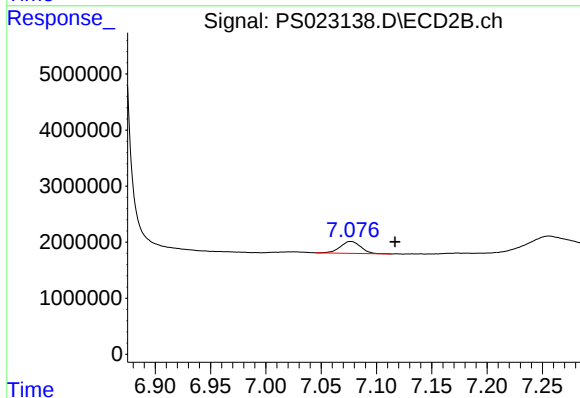


#6 MCPP

R.T.: 7.077 min
Delta R.T.: -0.040 min
Response: 2748452
Conc: 1.55 ug/ml

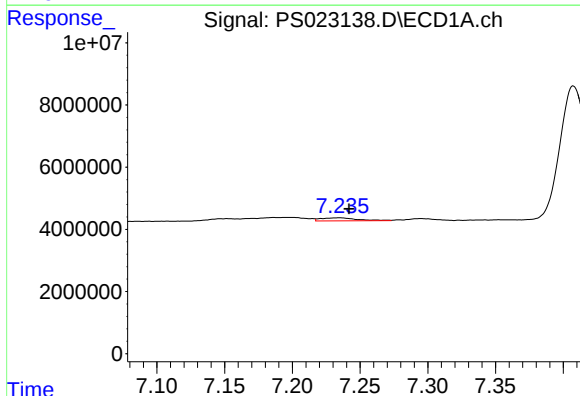


#8 DICHLORPROP

R.T.: 7.234 min
Delta R.T.: -0.008 min
Response: 1831866
Conc: N.D.

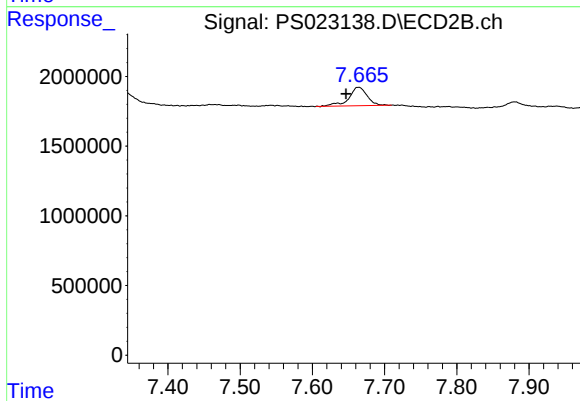

#8 DICHLORPROP


R.T.: 7.664 min
Delta R.T.: 0.017 min
Response: 2323742
Conc: 3.75 ng/ml

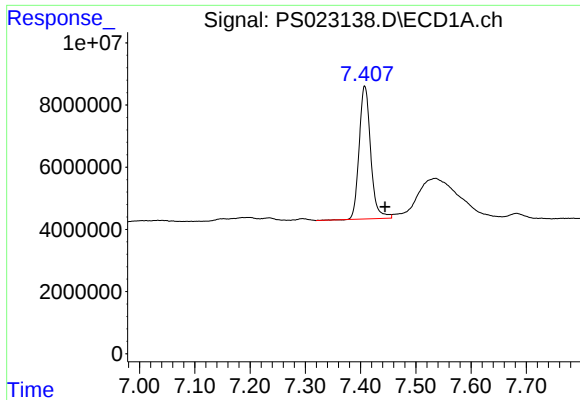

#9 2,4-D


R.T.: 7.408 min
Delta R.T.: -0.036 min
Response: 61935133
Conc: 26.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

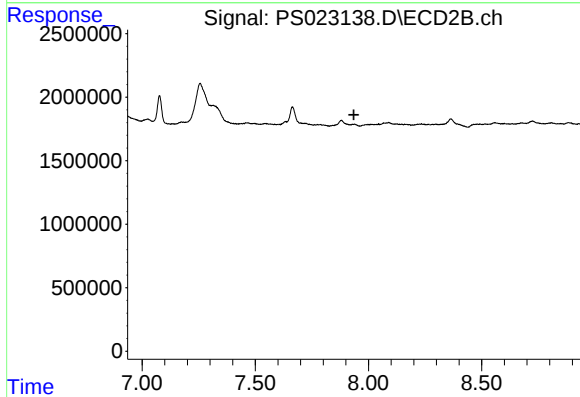


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.935 min
Response: 0
Conc: N.D.

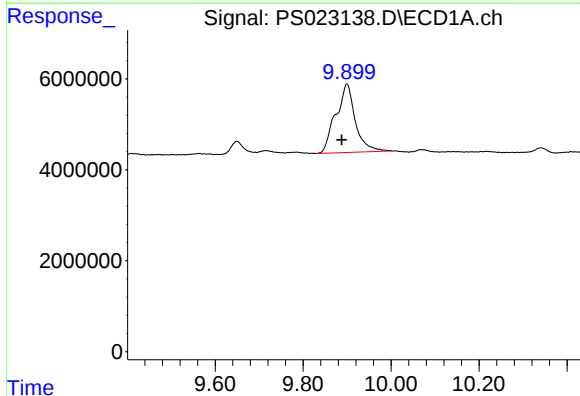


#15 Picloram

R.T.: 9.900 min
Delta R.T.: 0.012 min
Response: 46136736
Conc: 2.69 ng/ml

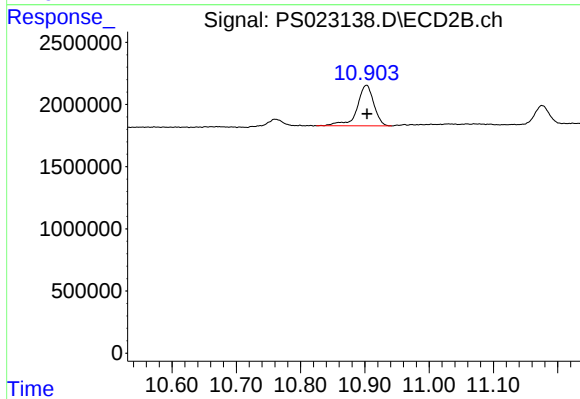

#15 Picloram


R.T.: 10.903 min
Delta R.T.: 0.000 min
Response: 5880961
Conc: 1.38 ng/ml

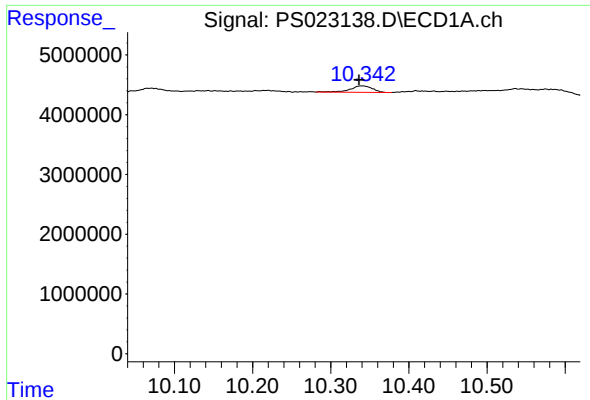

#16 DCPA

R.T.: 10.340 min
Delta R.T.: 0.004 min
Response: 2144138
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

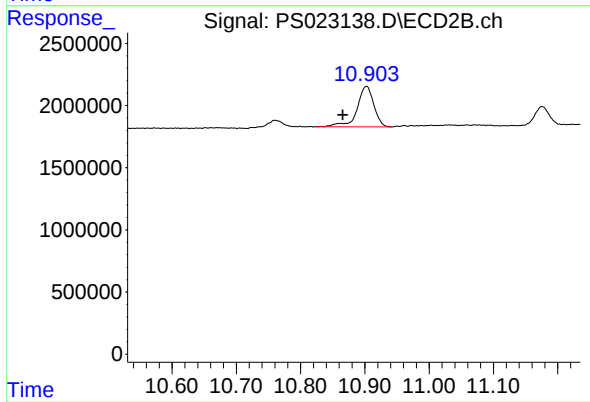

#16 DCPA

R.T.: 10.903 min
Delta R.T.: 0.037 min
Response: 5880961
Conc: 1.57 ng/ml