

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
 Data File : PS010416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 08:36
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 12:04:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.921	333.1E6	284.5E6	473.740	530.532
Target Compounds							
1) T	Dalapon	0.000	2.620	0	81670	N.D.	<MDL
5) T	DICAMBA	0.000	7.082	0	2151877	N.D.	<MDL
6) T	MCPD	0.000	7.211	0	497660	N.D.	<MDL
7) T	MCPA	0.000	7.358	0	3888090	N.D.	1.429
8) T	DICHLORPROP	0.000	7.752	0	536394	N.D.	<MDL
9) T	2,4-D	0.000	7.951	0	1425000	N.D.	2.055
11) T	2,4,5-TP ...	0.000	8.803	0	347006	N.D.	<MDL
12) T	2,4,5-T	0.000	9.194	0	199287	N.D.	<MDL
15) T	Picloram	0.000	11.017	0	5459339	N.D.	1.293
16) T	DCPA	0.000	10.949	0	526995	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
Data File : PS010416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 08:36
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 12:04:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

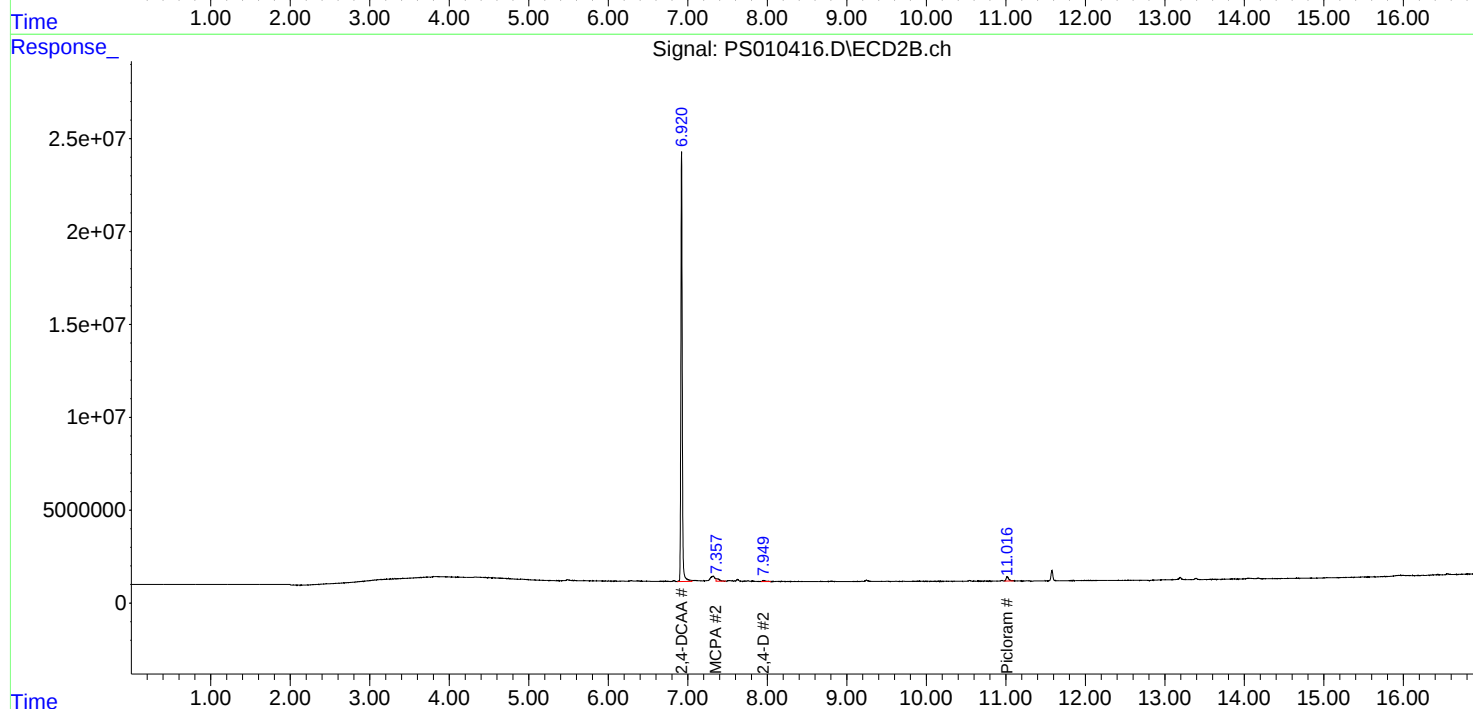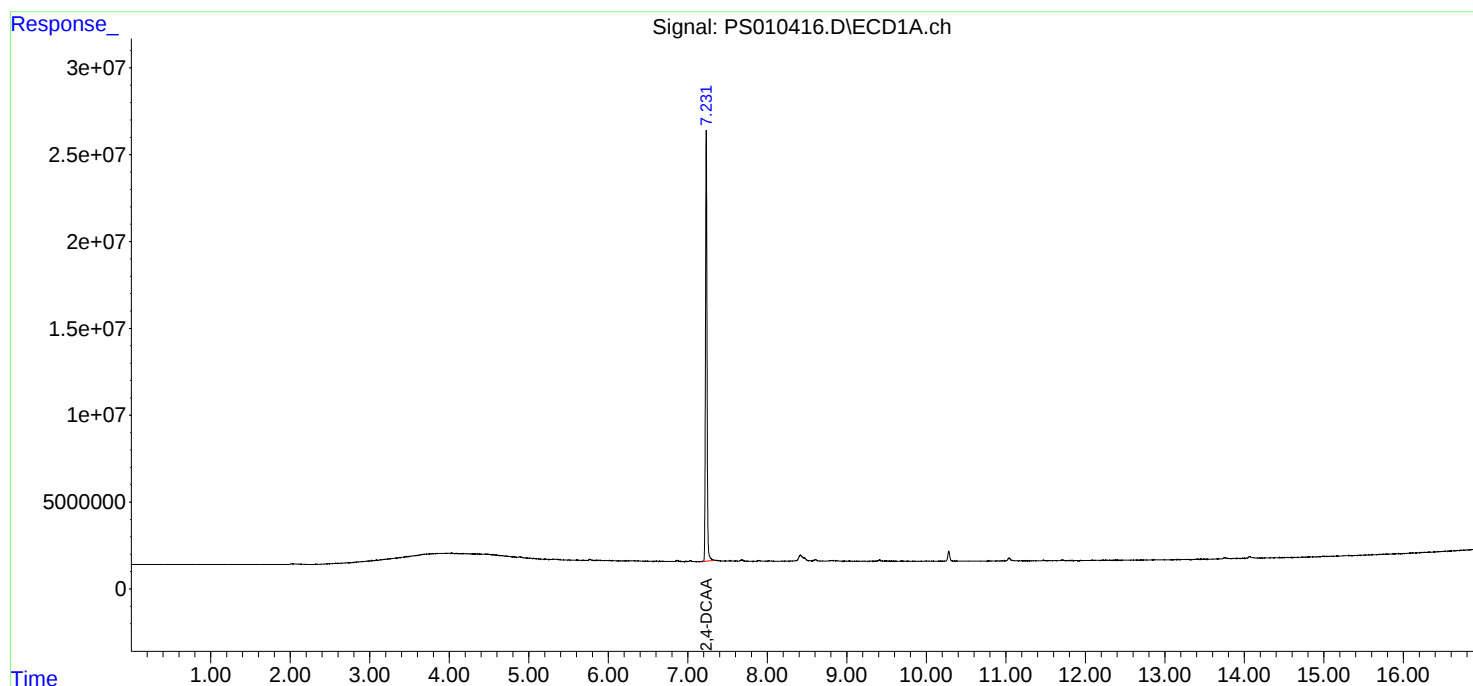


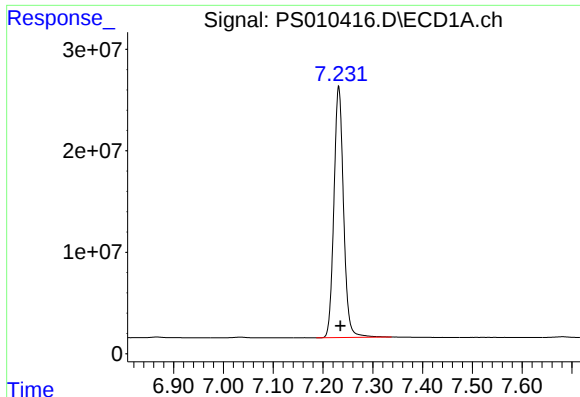

#4 2,4-DCAA


R.T.: 7.232 min
Delta R.T.: -0.003 min
Response: 333083915
Conc: 473.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

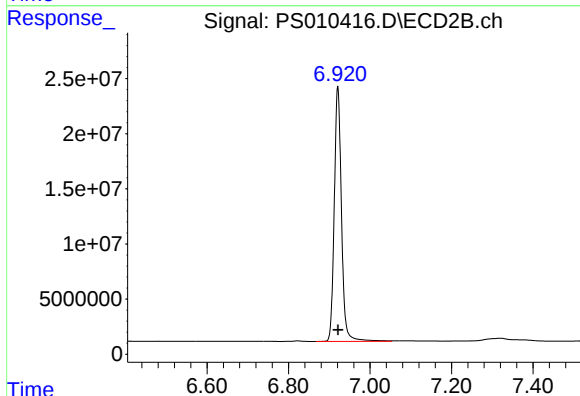


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 284519751
Conc: 530.53 ng/ml

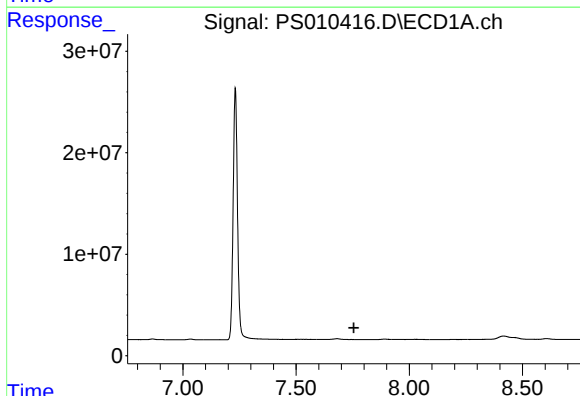


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.756 min
Response: 0
Conc: N.D.

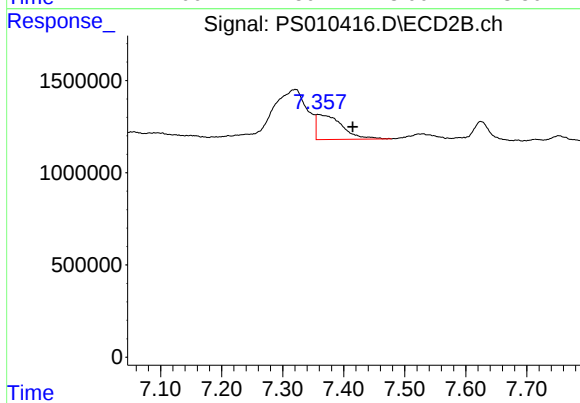

#7 MCPA


R.T.: 7.358 min
Delta R.T.: -0.057 min
Response: 3888090
Conc: 1.43 ug/ml

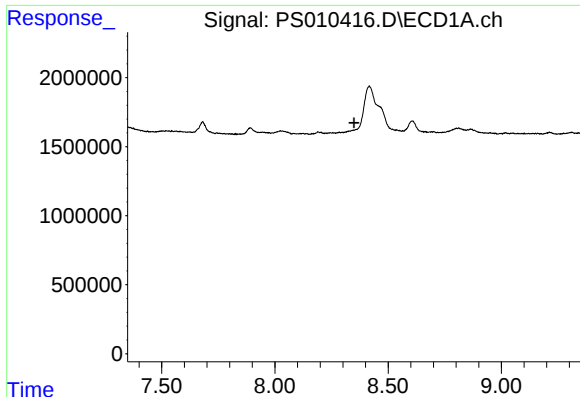

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

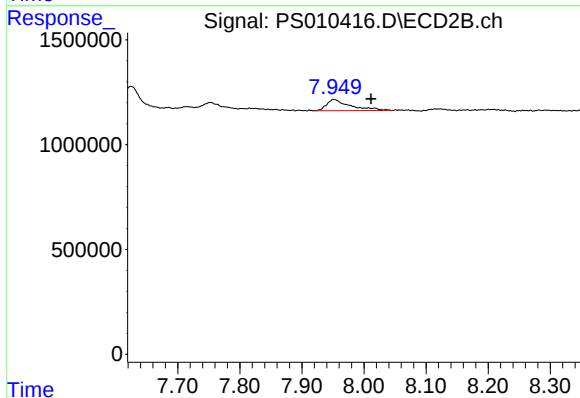


#9 2,4-D

R.T.: 7.951 min
Delta R.T.: -0.060 min
Response: 1425000
Conc: 2.06 ng/ml

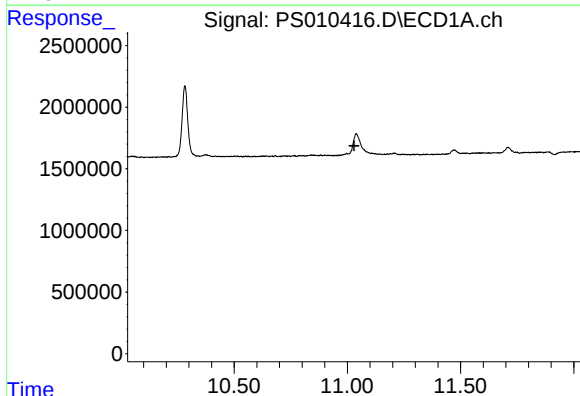

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.029 min
Response: 0
Conc: N.D.

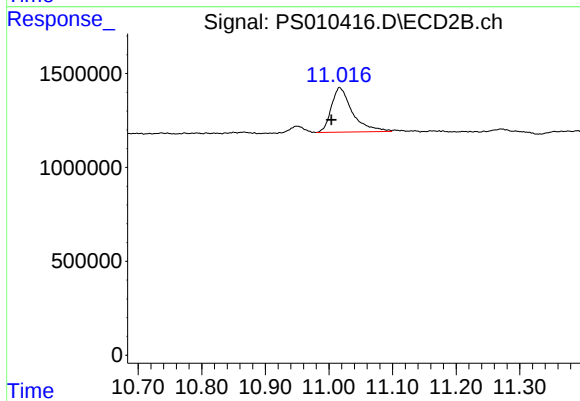

#15 Picloram

R.T.: 11.017 min
Delta R.T.: 0.013 min
Response: 5459339
Conc: 1.29 ng/ml