

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
 Data File : PS010428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2020 14:12
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 15:00:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.921	342.5E6	287.6E6	487.183	536.193
Target Compounds							
5) T	DICAMBA	0.000	7.090	0	1822437	N.D.	<MDL
6) T	MCPD	0.000	7.155	0	1078263	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.746	0	2200300	N.D.	3.897
9) T	2,4-D	8.418	8.012	16355517	149410	23.152	<MDL #
11) T	2,4,5-TP ...	0.000	8.802	0	727931	N.D.	<MDL
12) T	2,4,5-T	0.000	9.184	0	629261	N.D.	<MDL
13) T	2,4-DB	0.000	9.707	0	543547	N.D.	1.364
14) T	DINOSEB	0.000	10.022	0	2273398	N.D.	1.067
15) T	Picloram	0.000	11.008	0	4493871	N.D.	1.064
16) T	DCPA	0.000	10.952	0	1769705	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
Data File : PS010428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2020 14:12
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 15:00:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

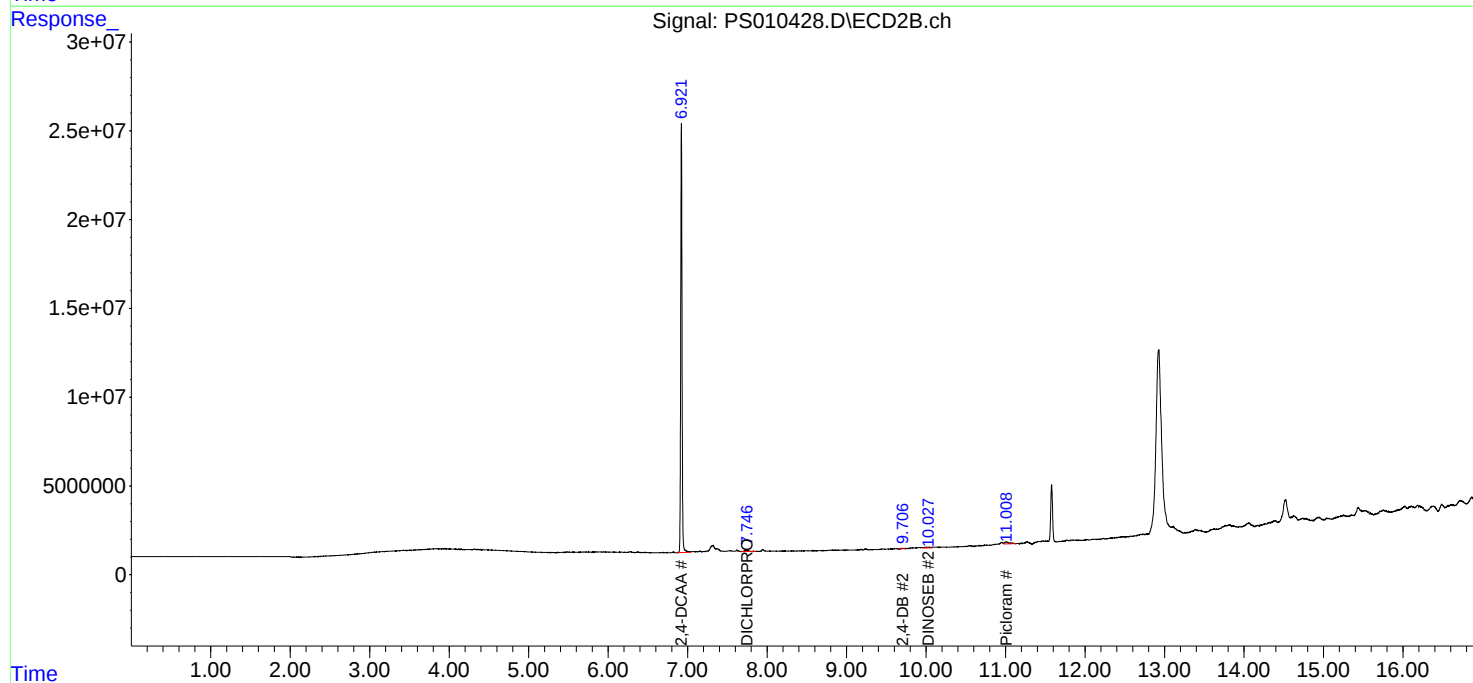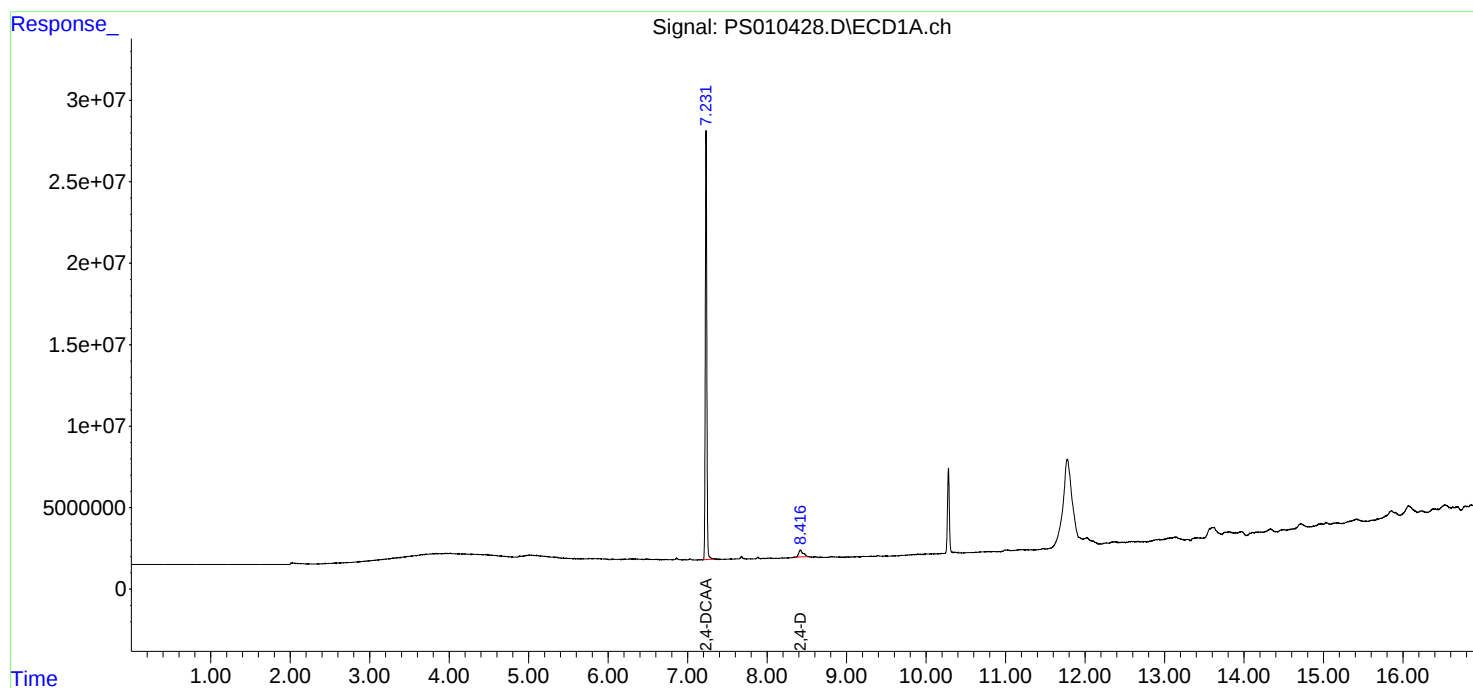


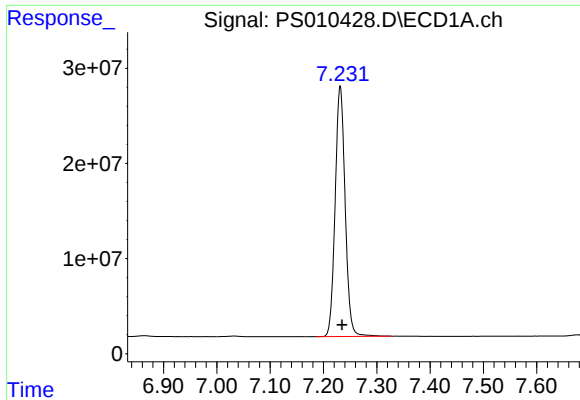

#4 2,4-DCAA


R.T.: 7.231 min
Delta R.T.: -0.003 min
Response: 342535634
Conc: 487.18 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

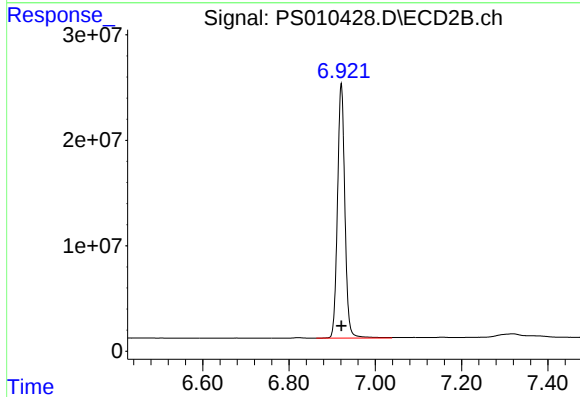


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 287555690
Conc: 536.19 ng/ml

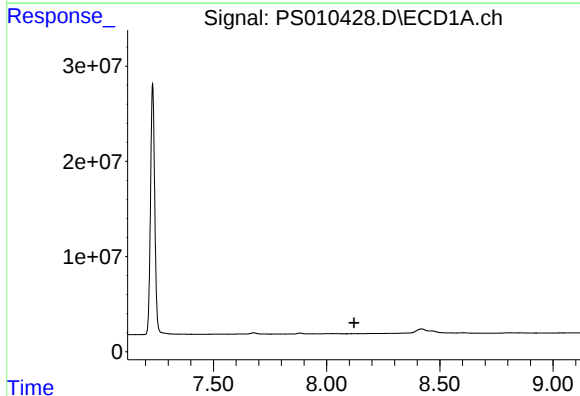


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

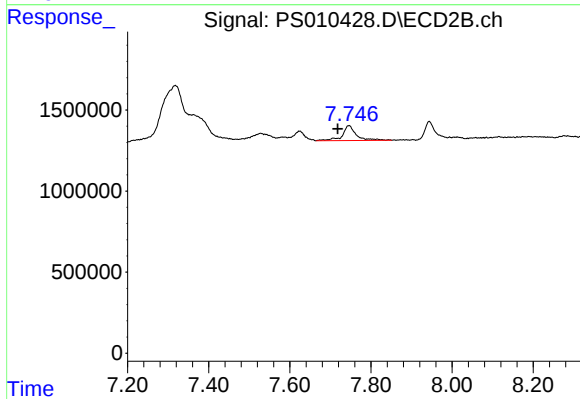

#8 DICHLORPROP


R.T.: 7.746 min
Delta R.T.: 0.027 min
Response: 2200300
Conc: 3.90 ng/ml

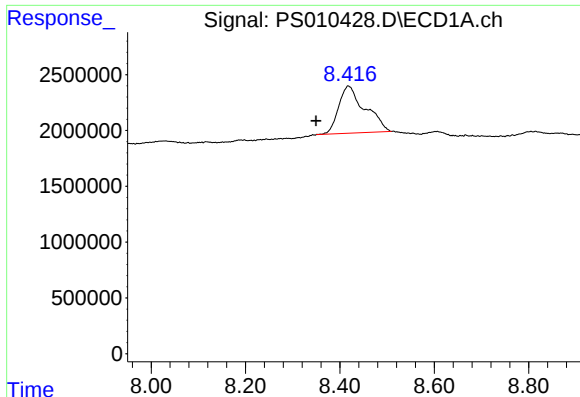

#9 2,4-D


R.T.: 8.418 min
Delta R.T.: 0.068 min
Response: 16355517
Conc: 23.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

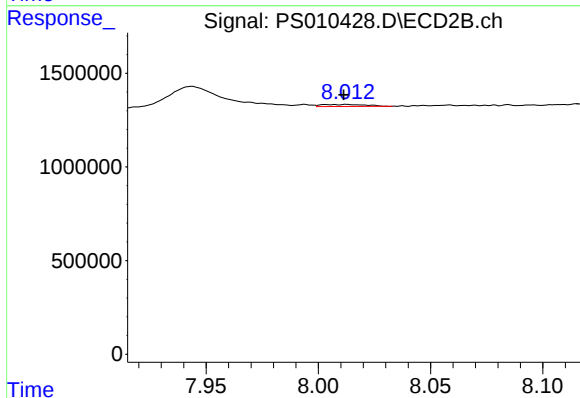


#9 2,4-D

R.T.: 8.012 min
Delta R.T.: 0.000 min
Response: 149410
Conc: N.D.

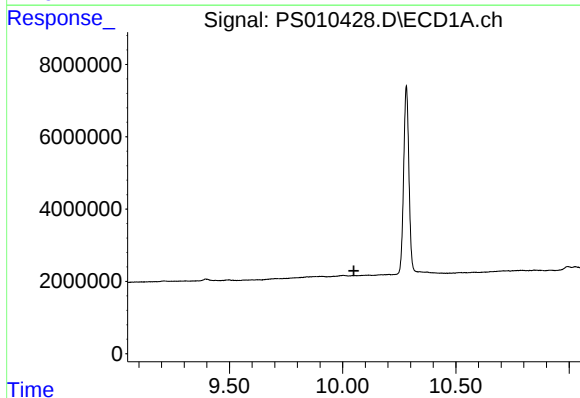


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.050 min
Response: 0
Conc: N.D.

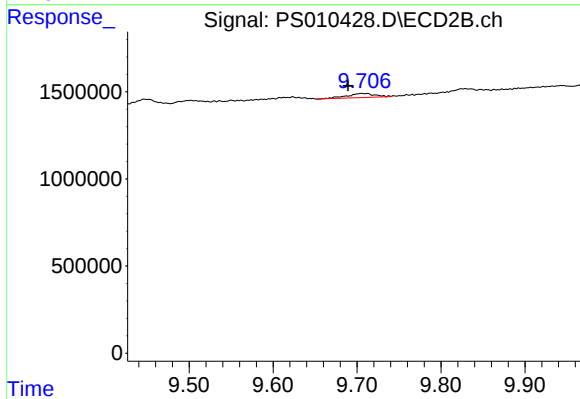

#13 2,4-DB


R.T.: 9.707 min
Delta R.T.: 0.018 min
Response: 543547
Conc: 1.36 ng/ml

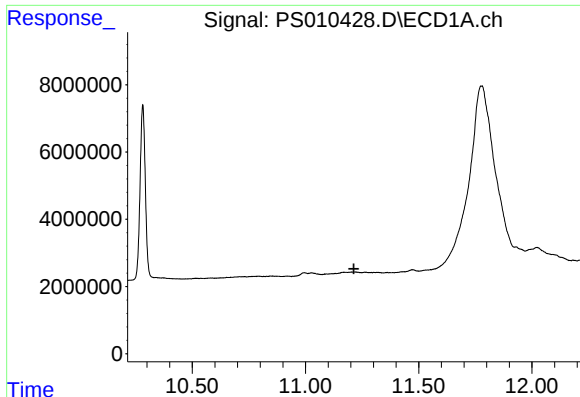

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 11.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

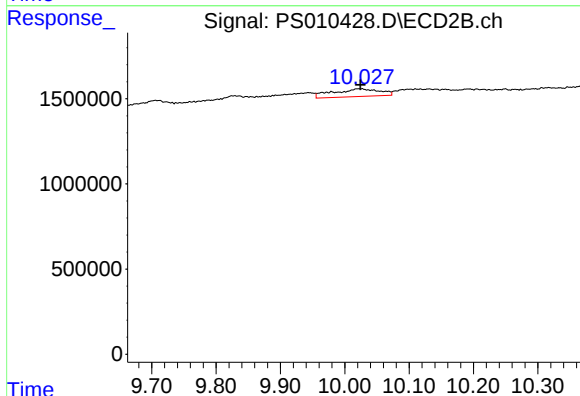


#14 DINOSEB

R.T.: 10.022 min
Delta R.T.: -0.002 min
Response: 2273398
Conc: 1.07 ng/ml

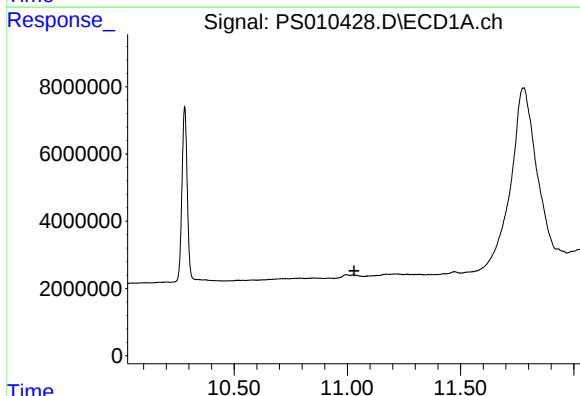

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.029 min
Response: 0
Conc: N.D.

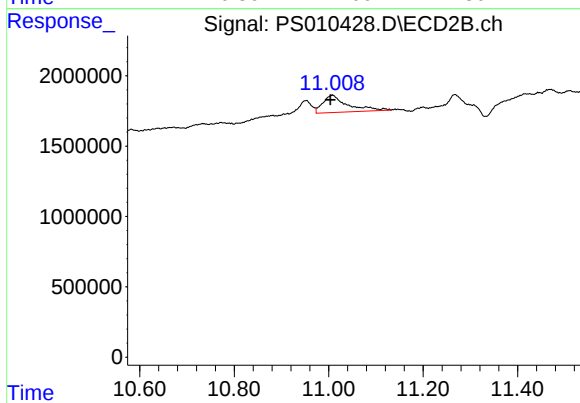

#15 Picloram

R.T.: 11.008 min
Delta R.T.: 0.004 min
Response: 4493871
Conc: 1.06 ng/ml