

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
 Data File : PS010464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 04:05
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 05:33:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.921	355.1E6	291.4E6	505.035	543.398
Target Compounds							
2) T	3,5-DICHL...	6.485	0.000	56703453	0	58.776	N.D. #
5) T	DICAMBA	0.000	7.089	0	2143636	N.D.	<MDL
6) T	MCP	0.000	7.154	0	49412432	N.D.	26.919
8) T	DICHLORPROP	0.000	7.742	0	5116031	N.D.	9.062
9) T	2,4-D	8.414	8.007	72638632	267132	102.822	<MDL #
11) T	2,4,5-TP ...	0.000	8.801	0	1922328	N.D.	<MDL
12) T	2,4,5-T	0.000	9.182	0	1582756	N.D.	<MDL
13) T	2,4-DB	0.000	9.704	0	1230980	N.D.	3.089
14) T	DINOSEB	0.000	10.023	0	1280411	N.D.	<MDL
15) T	Picloram	10.990	11.006	19103981	1903680	4.167	<MDL #
16) T	DCPA	0.000	10.950	0	1669903	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
Data File : PS010464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 04:05
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 05:33:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

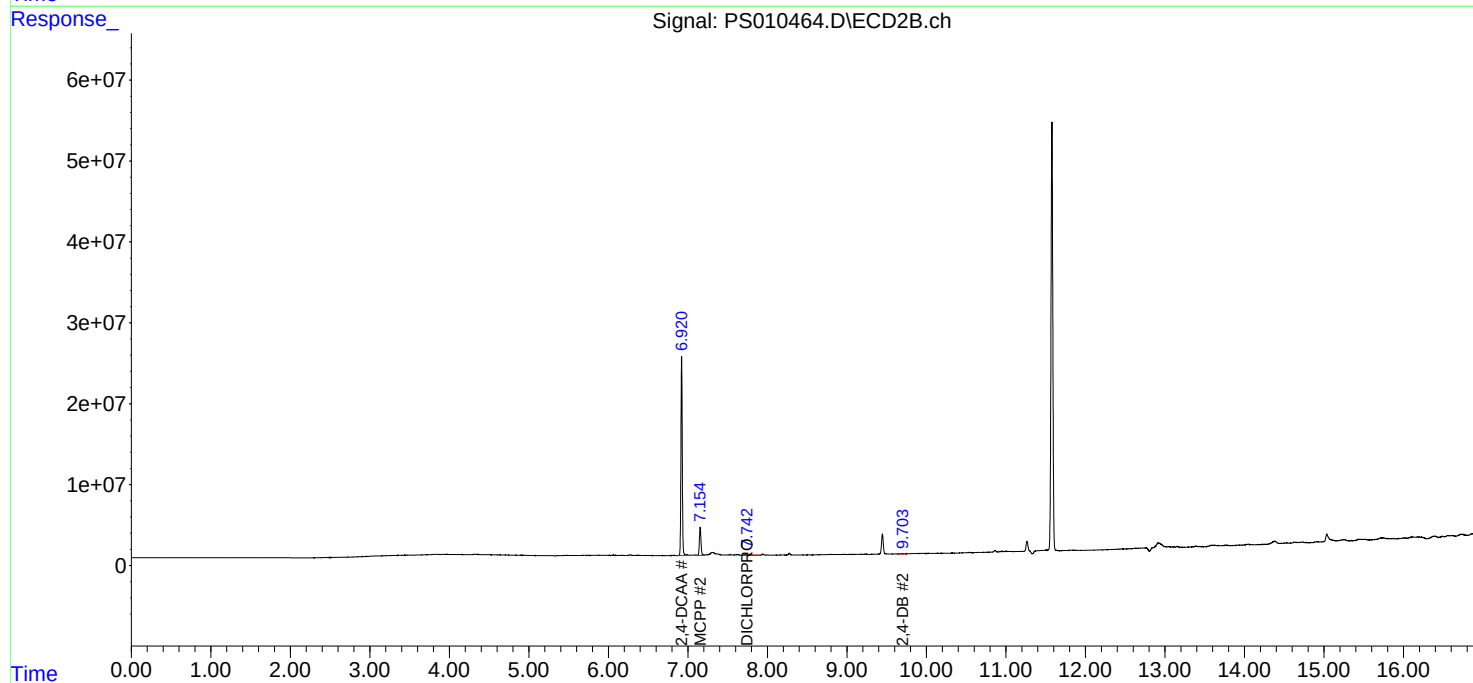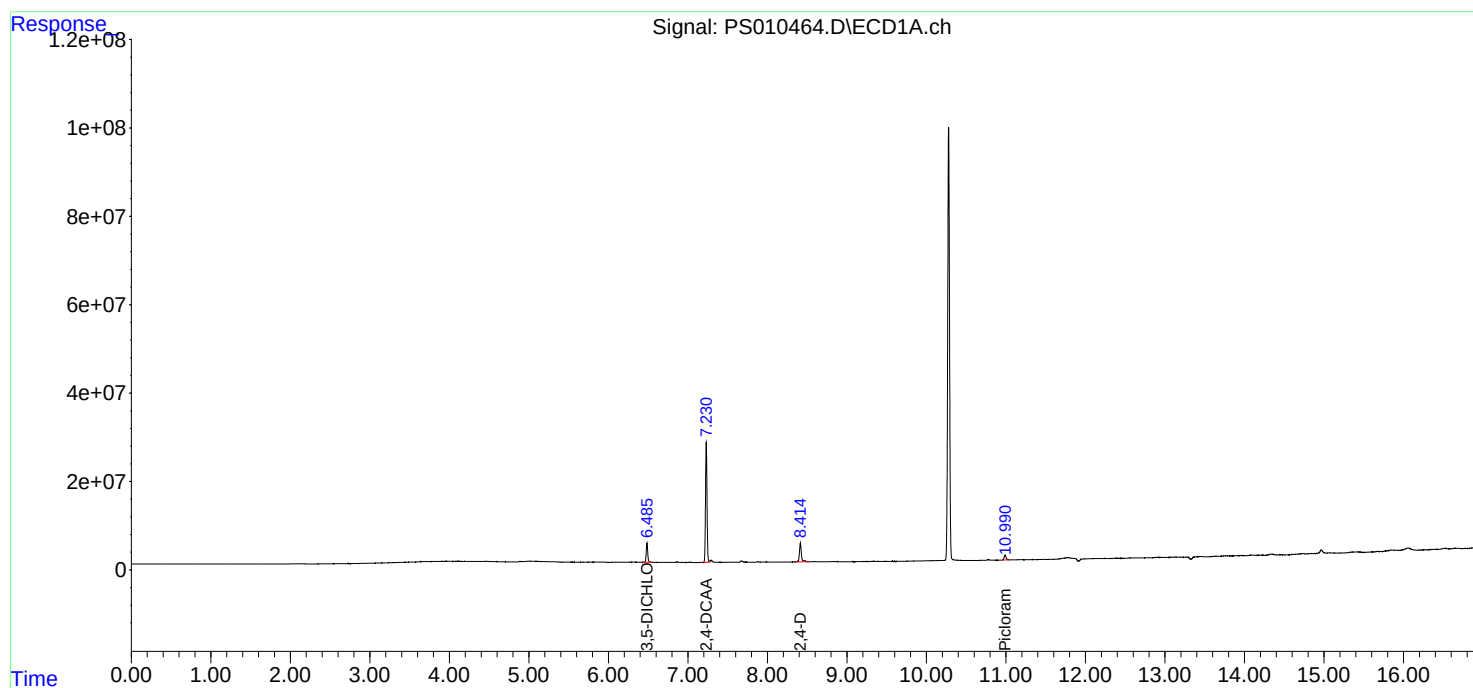


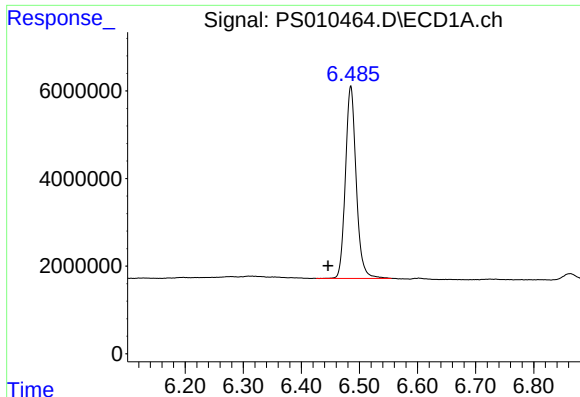

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.485 min
Delta R.T.: 0.039 min
Response: 56703453
Conc: 58.78 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

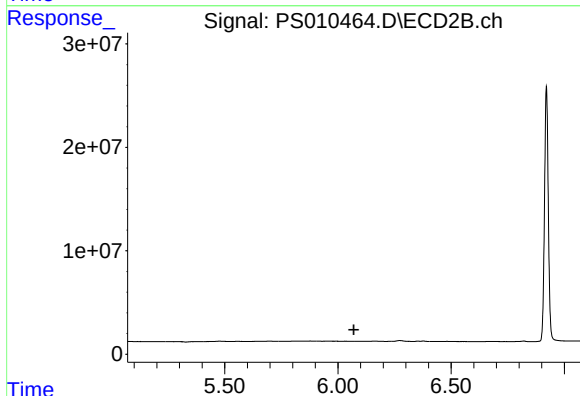


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.071 min
Response: 0
Conc: N.D.

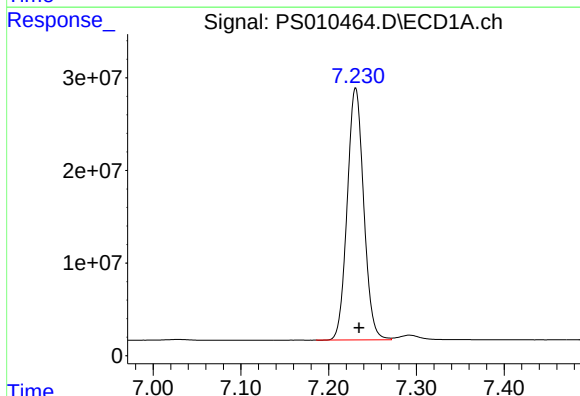


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.004 min
Response: 355087734
Conc: 505.04 ng/ml

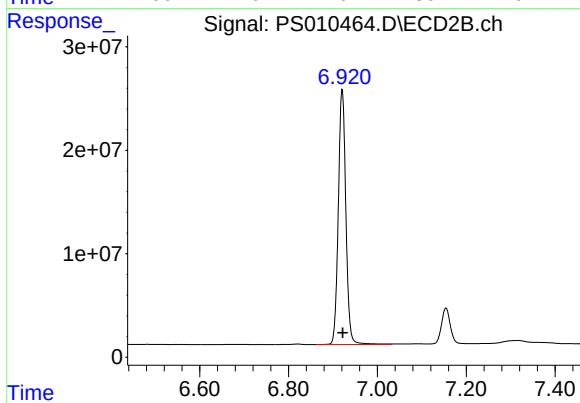

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 291419532
Conc: 543.40 ng/ml

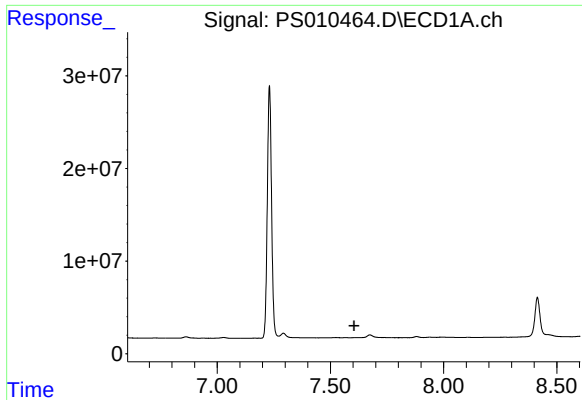

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

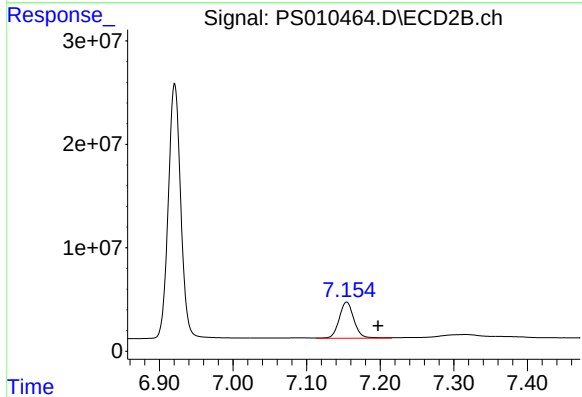


#6 MCP

R.T.: 7.154 min
Delta R.T.: -0.043 min
Response: 49412432
Conc: 26.92 ug/ml

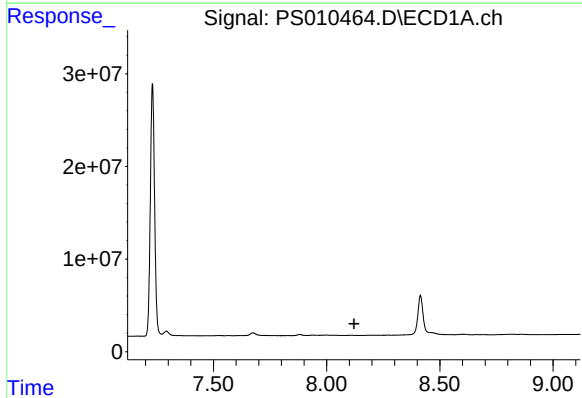


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

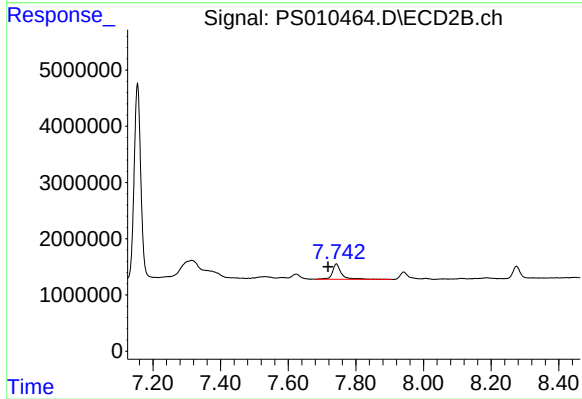

#8 DICHLORPROP


R.T.: 7.742 min
Delta R.T.: 0.024 min
Response: 5116031
Conc: 9.06 ng/ml

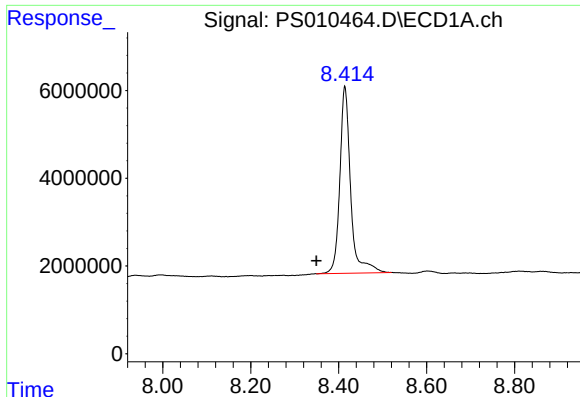

#9 2,4-D


R.T.: 8.414 min
Delta R.T.: 0.065 min
Response: 72638632
Conc: 102.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

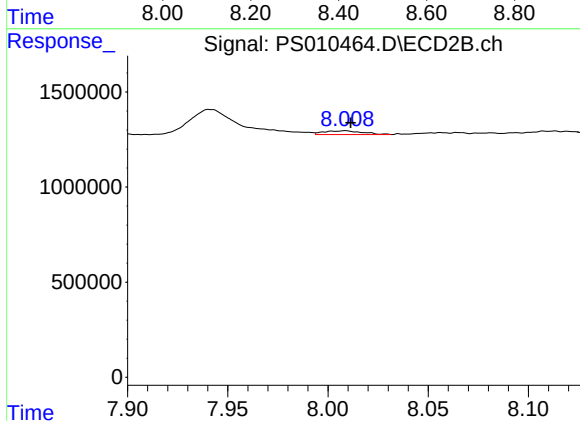


#9 2,4-D

R.T.: 8.007 min
Delta R.T.: -0.004 min
Response: 267132
Conc: N.D.

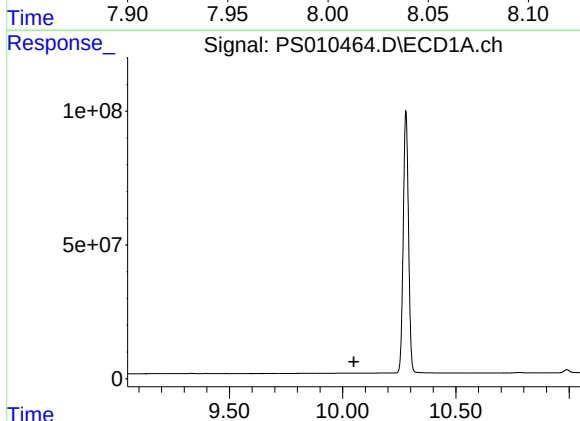


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.050 min
Response: 0
Conc: N.D.

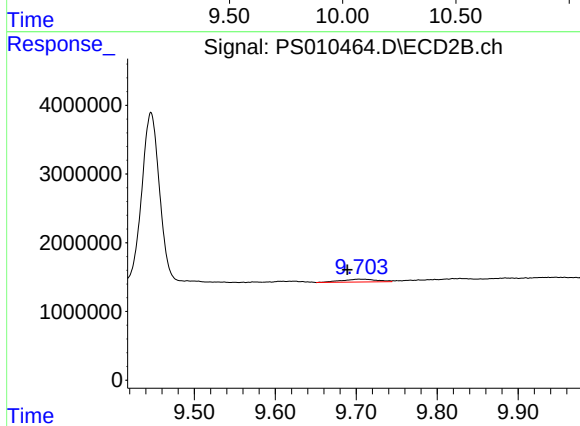

#13 2,4-DB


R.T.: 9.704 min
Delta R.T.: 0.015 min
Response: 1230980
Conc: 3.09 ng/ml

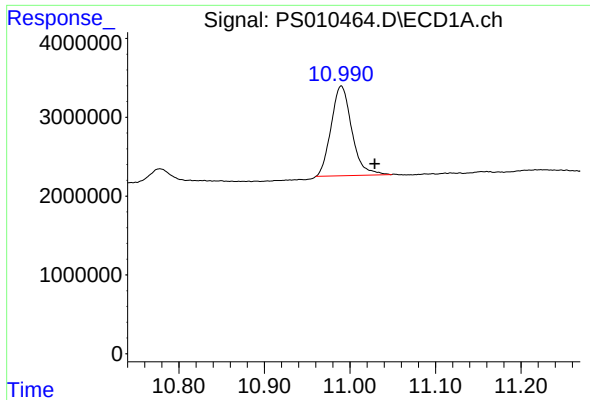

#15 Picloram

R.T.: 10.990 min
Delta R.T.: -0.039 min
Response: 19103981
Conc: 4.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

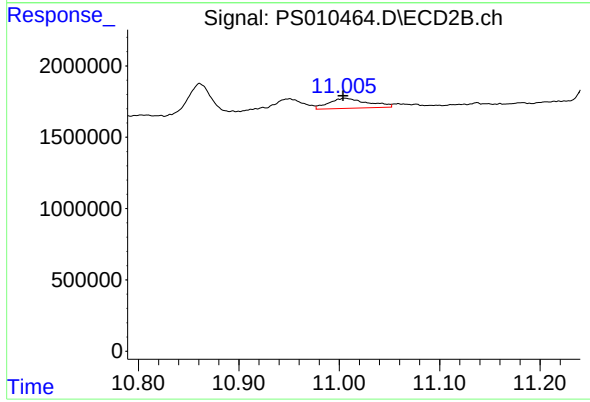

#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.002 min
Response: 1903680
Conc: N.D.