

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
 Data File : PS010476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 08:40
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 10:38:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.920	358.7E6	292.6E6	510.134	545.663
Target Compounds							
1) T	Dalapon	0.000	2.659	0	478559	N.D.	<MDL
2) T	3,5-DICHL...	6.484	0.000	120.1E6	0	124.450	N.D. #
5) T	DICAMBA	0.000	7.089	0	1161353	N.D.	<MDL
6) T	MCP	0.000	7.154	0	99127004	N.D.	54.002
8) T	DICHLORPROP	0.000	7.742	0	3840459	N.D.	6.802
9) T	2,4-D	8.414	8.009	135.2E6	248657	191.312	<MDL #
11) T	2,4,5-TP ...	0.000	8.799	0	1047331	N.D.	<MDL
12) T	2,4,5-T	0.000	9.178	0	444305	N.D.	<MDL
13) T	2,4-DB	0.000	9.705	0	932783	N.D.	2.340
14) T	DINOSEB	0.000	10.023	0	1202457	N.D.	<MDL
15) T	Picloram	10.989	11.006	27512329	1586898	6.001	<MDL #
16) T	DCPA	0.000	10.951	0	1330783	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
Data File : PS010476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 08:40
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 10:38:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

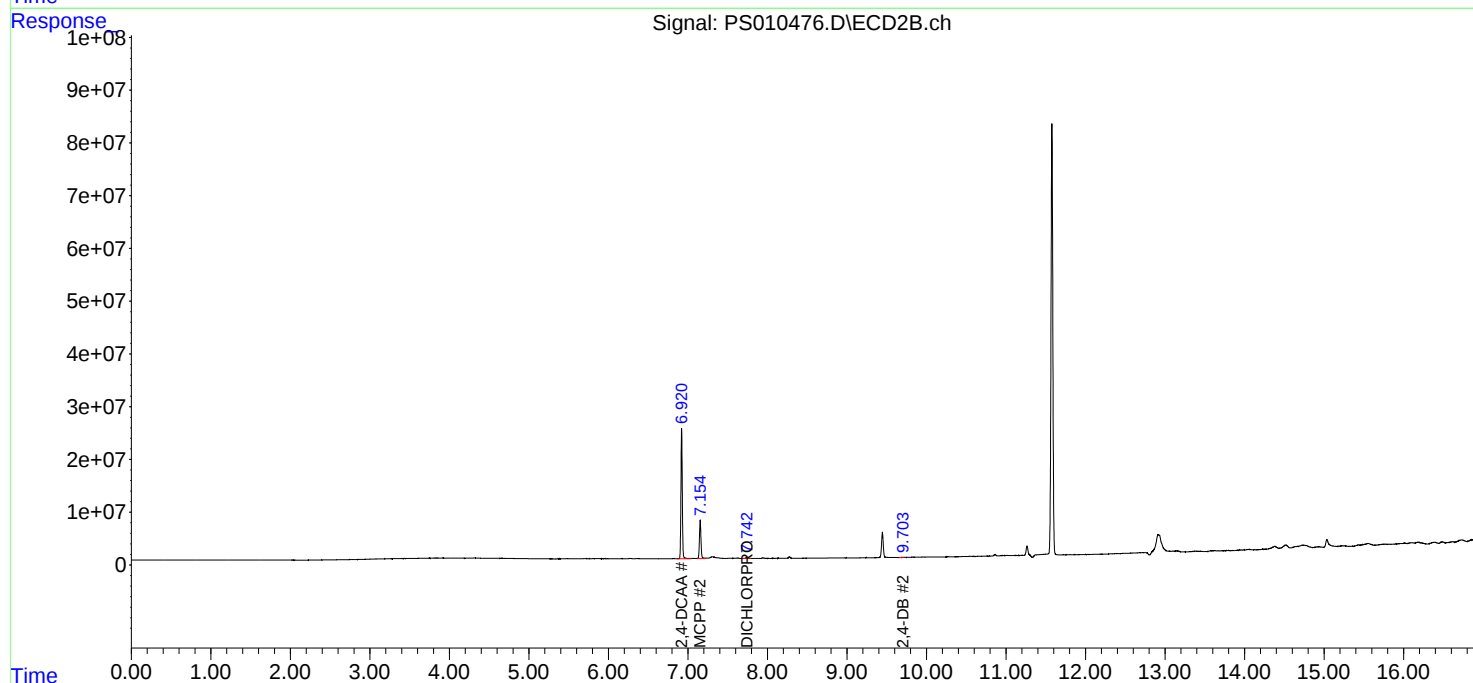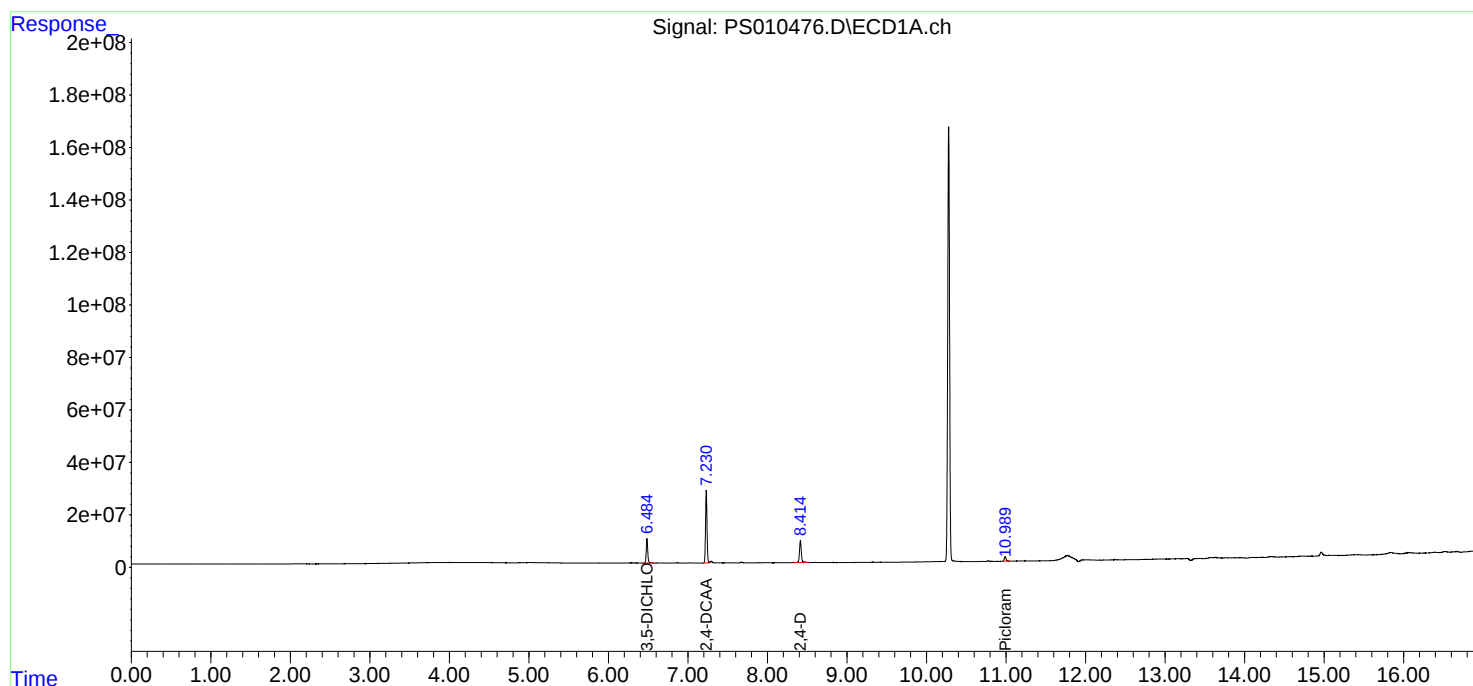


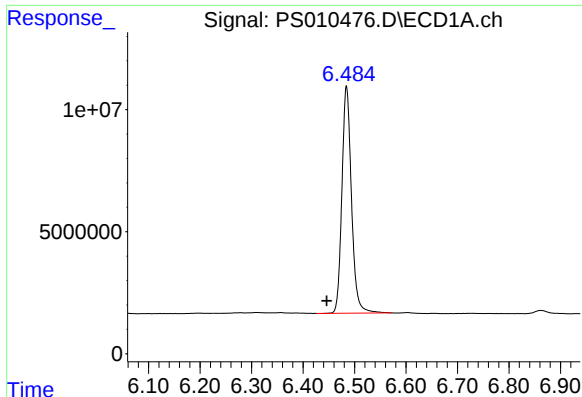

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.484 min
Delta R.T.: 0.038 min
Response: 120062250
Conc: 124.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

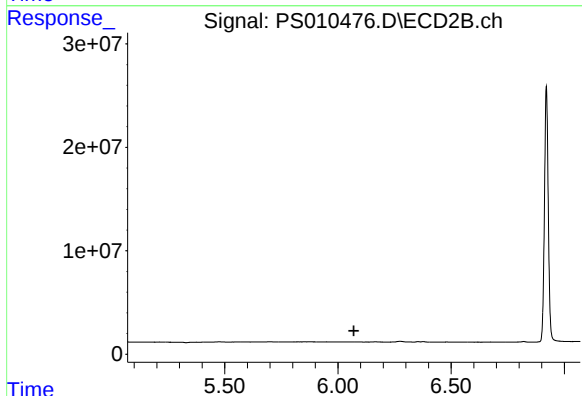


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.071 min
Response: 0
Conc: N.D.

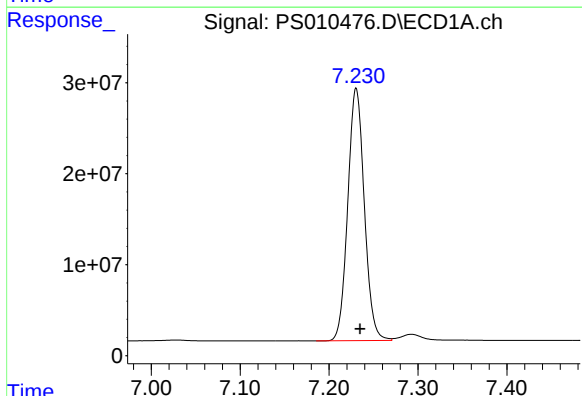


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.004 min
Response: 358672222
Conc: 510.13 ng/ml

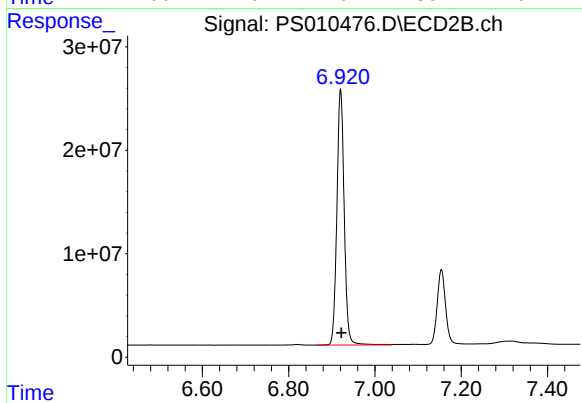

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 292634440
Conc: 545.66 ng/ml

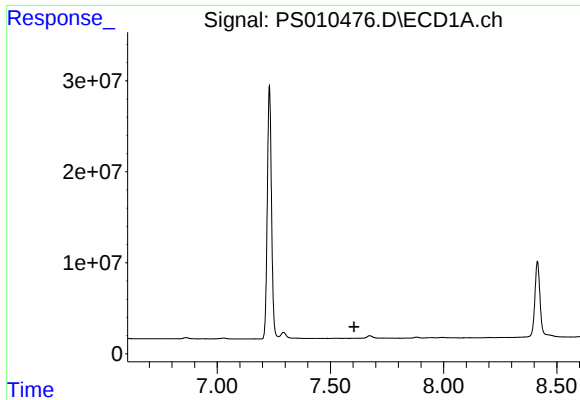

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

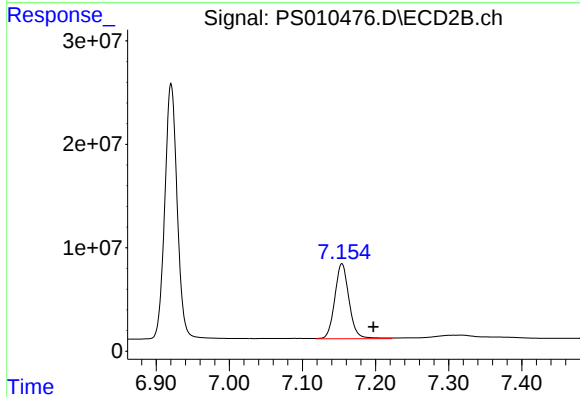


#6 MCP

R.T.: 7.154 min
Delta R.T.: -0.043 min
Response: 99127004
Conc: 54.00 ug/ml

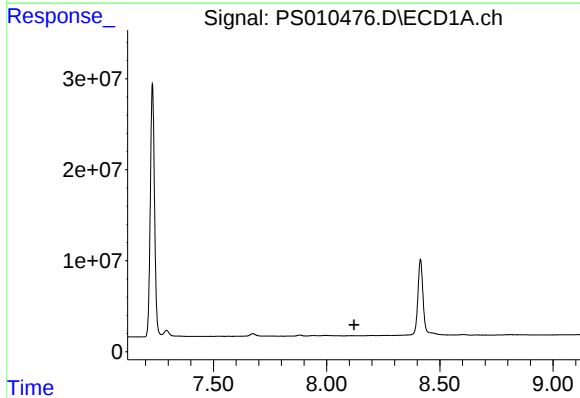


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

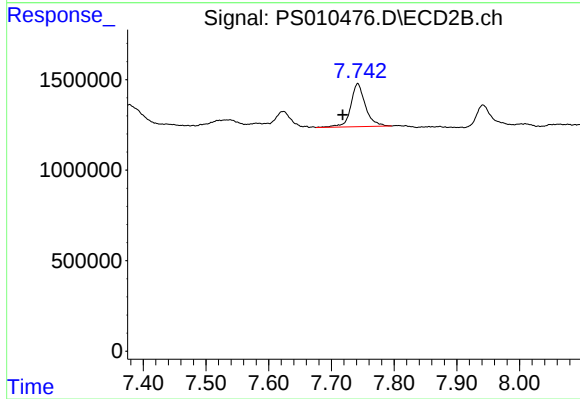

#8 DICHLORPROP


R.T.: 7.742 min
Delta R.T.: 0.024 min
Response: 3840459
Conc: 6.80 ng/ml

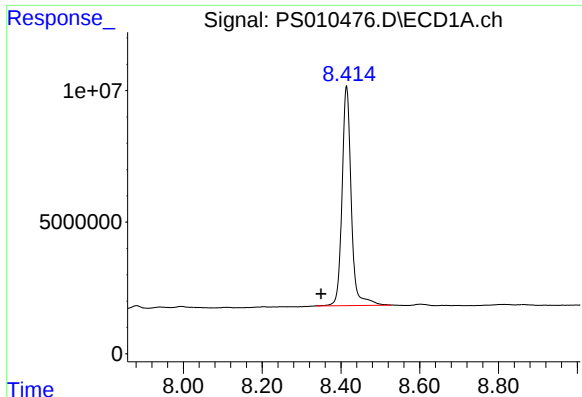

#9 2,4-D


R.T.: 8.414 min
Delta R.T.: 0.065 min
Response: 135153294
Conc: 191.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

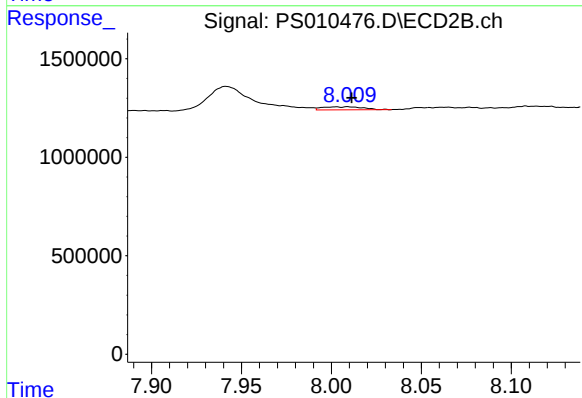


#9 2,4-D

R.T.: 8.009 min
Delta R.T.: -0.002 min
Response: 248657
Conc: N.D.

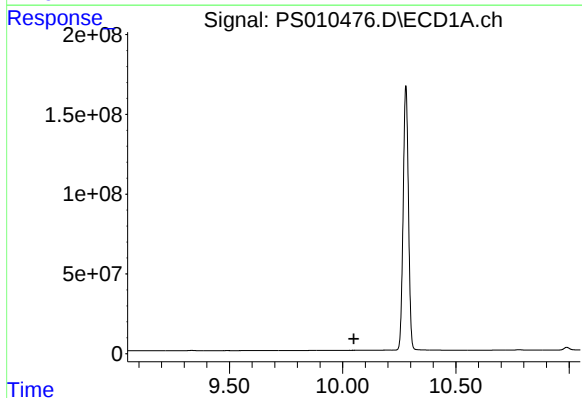


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.050 min
Response: 0
Conc: N.D.

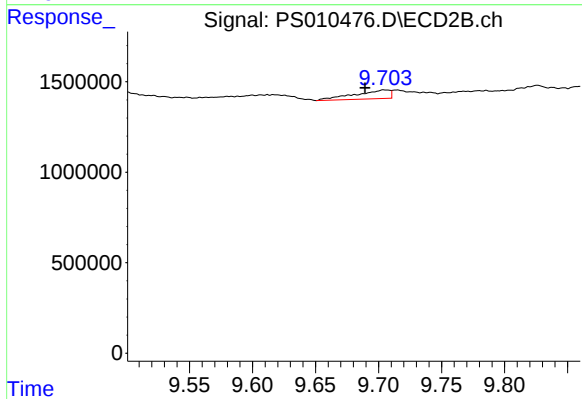

#13 2,4-DB


R.T.: 9.705 min
Delta R.T.: 0.016 min
Response: 932783
Conc: 2.34 ng/ml

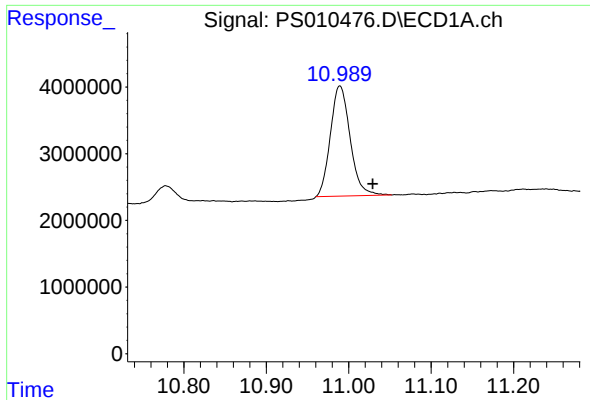

#15 Picloram

R.T.: 10.989 min
Delta R.T.: -0.040 min
Response: 27512329
Conc: 6.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

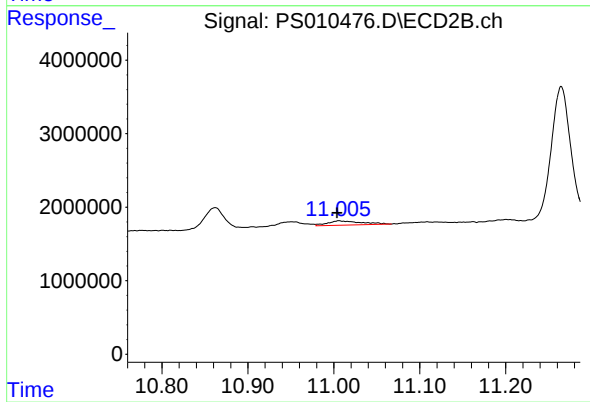

#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.002 min
Response: 1586898
Conc: N.D.