

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
 Data File : PS010486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 12:30
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 13:18:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.921	366.1E6	297.0E6	520.636	553.713
Target Compounds							
2) T	3,5-DICHL...	6.484	6.027	426.1E6	358273	441.633	<MDL #
5) T	DICAMBA	0.000	7.154	0	333.5E6	N.D.	152.324
6) T	MCP	0.000	7.154	0	333.5E6	N.D.	181.698
8) T	DICHLORPROP	0.000	7.742	0	5404436	N.D.	9.573
9) T	2,4-D	8.415	8.055	414.3E6	109790	586.412	<MDL #
10) T	Pentachlo...	0.000	8.444	0	281268	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.801	0	823517	N.D.	<MDL
12) T	2,4,5-T	0.000	9.182	0	742730	N.D.	<MDL
13) T	2,4-DB	0.000	9.707	0	950258	N.D.	2.384
14) T	DINOSEB	0.000	10.022	0	401693	N.D.	<MDL
15) T	Picloram	10.990	11.005	53277489	2141424	11.621	<MDL #
16) T	DCPA	0.000	10.951	0	986015	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052720\
Data File : PS010486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 12:30
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 13:18:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

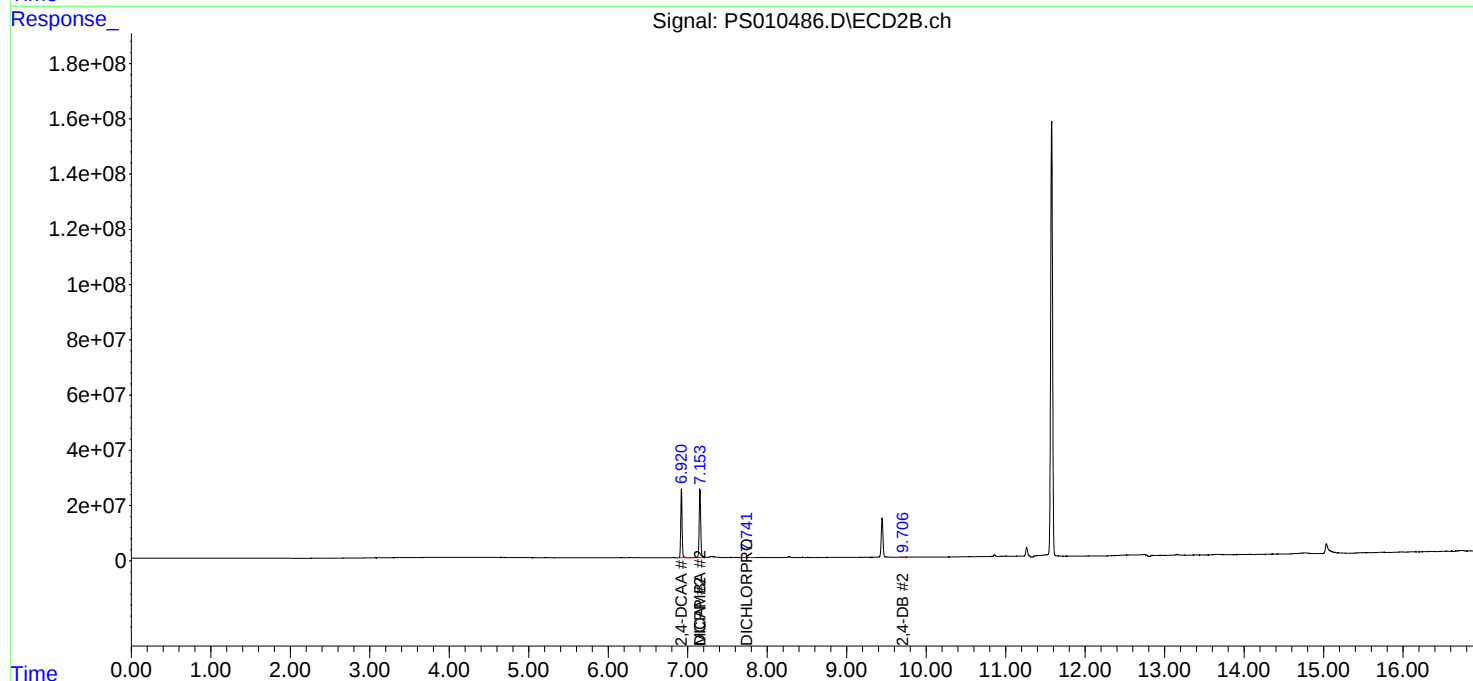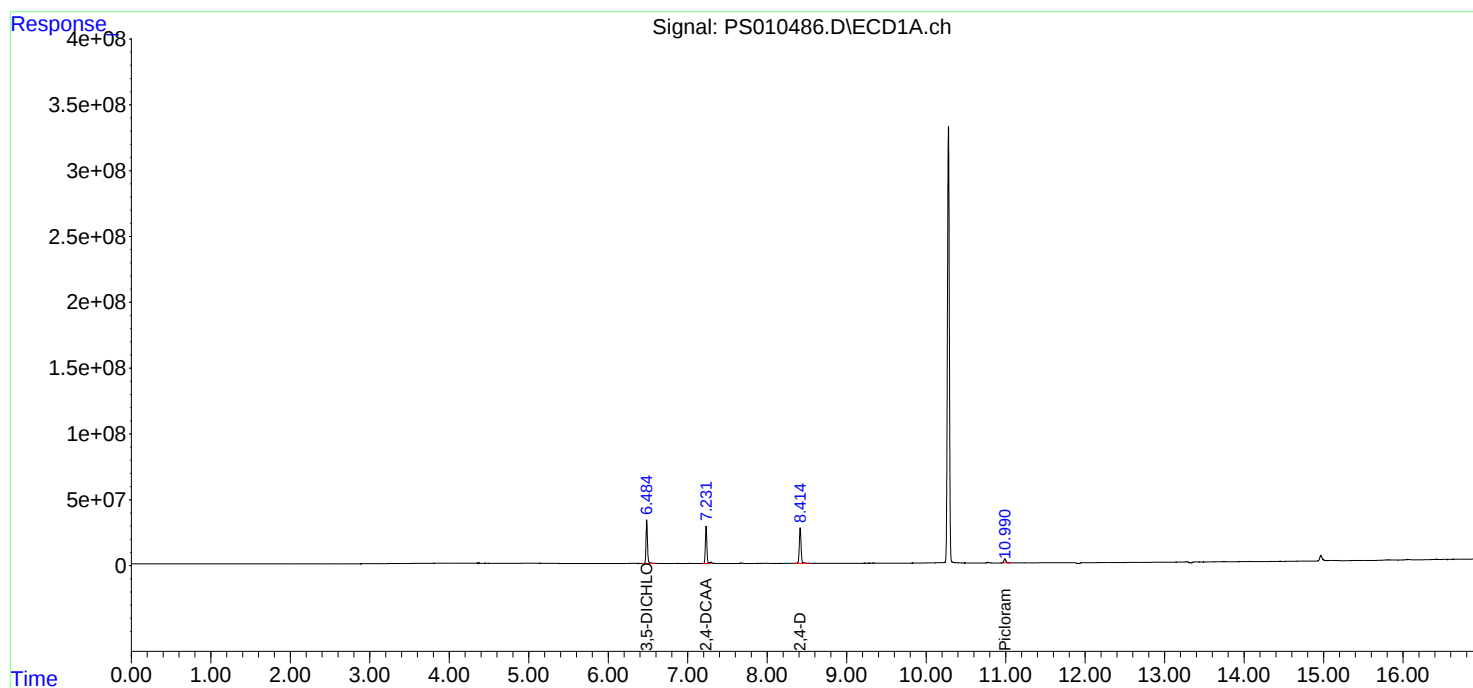


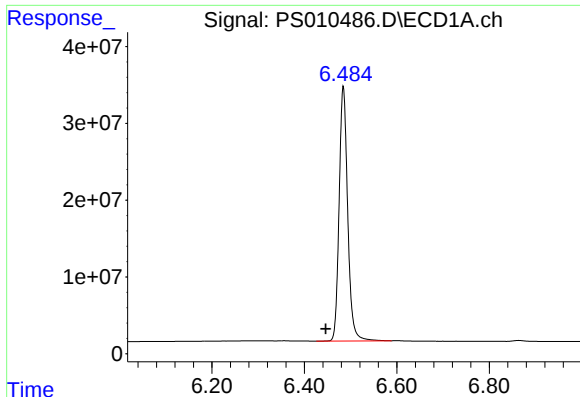

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.484 min
Delta R.T.: 0.038 min
Response: 426062056
Conc: 441.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

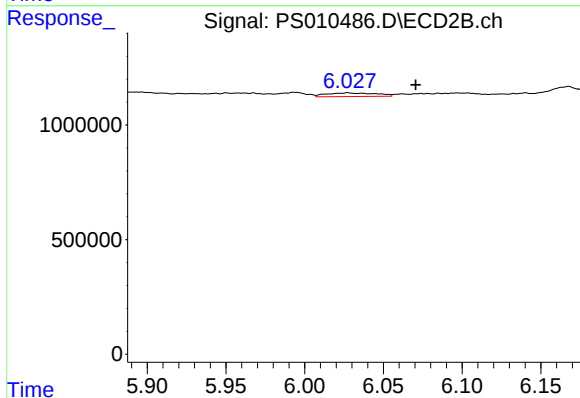


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.027 min
Delta R.T.: -0.043 min
Response: 358273
Conc: N.D.

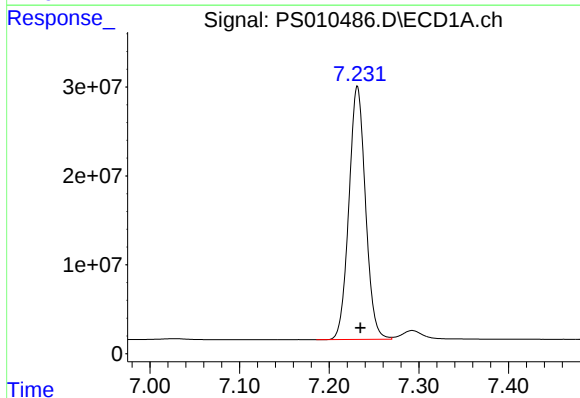


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: -0.003 min
Response: 366056102
Conc: 520.64 ng/ml

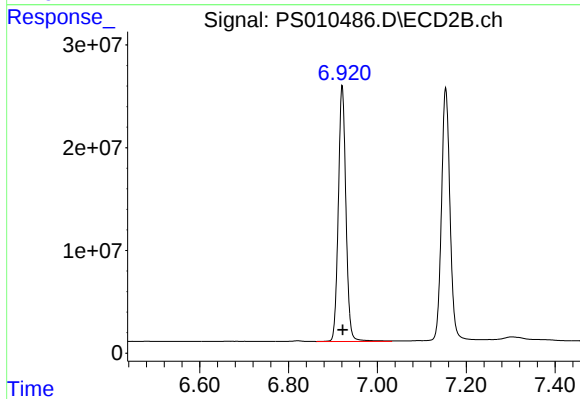

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 296951563
Conc: 553.71 ng/ml

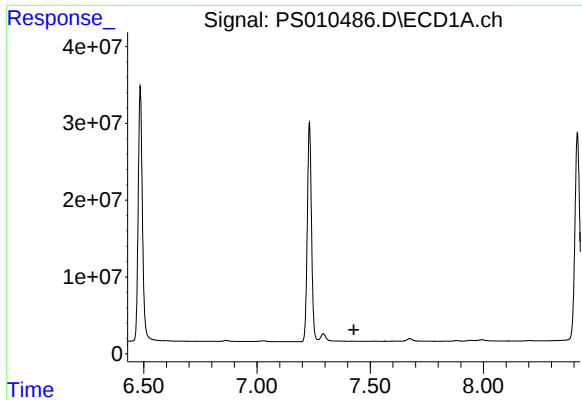

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

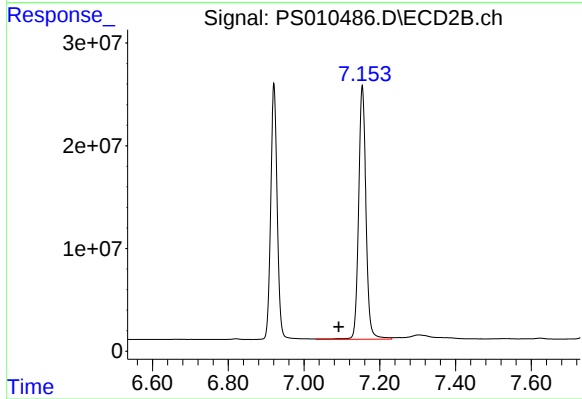


#5 DICAMBA

R.T.: 7.154 min
Delta R.T.: 0.062 min
Response: 333528149
Conc: 152.32 ng/ml

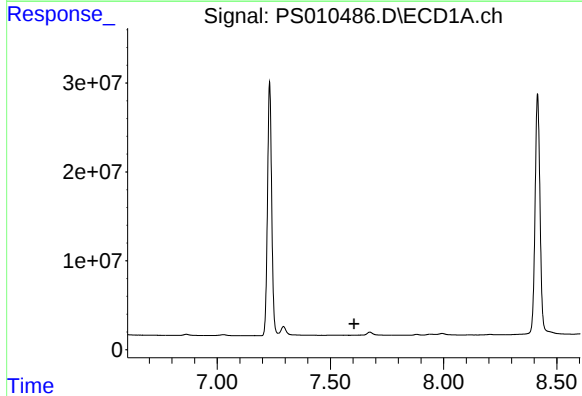


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

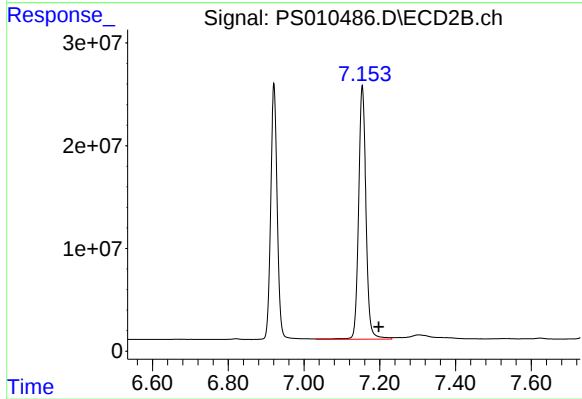

#6 MCP


R.T.: 7.154 min
Delta R.T.: -0.043 min
Response: 333528149
Conc: 181.70 ug/ml

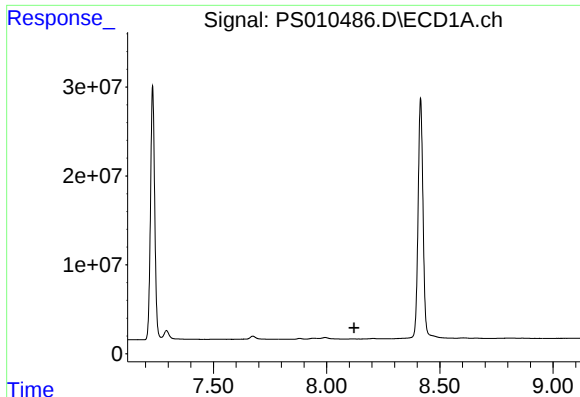

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

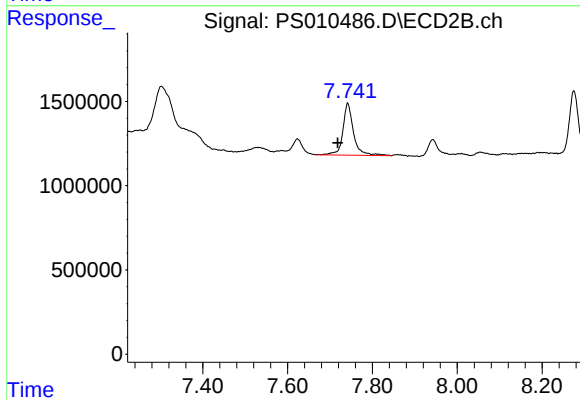


#8 DICHLORPROP

R.T.: 7.742 min
Delta R.T.: 0.024 min
Response: 5404436
Conc: 9.57 ng/ml

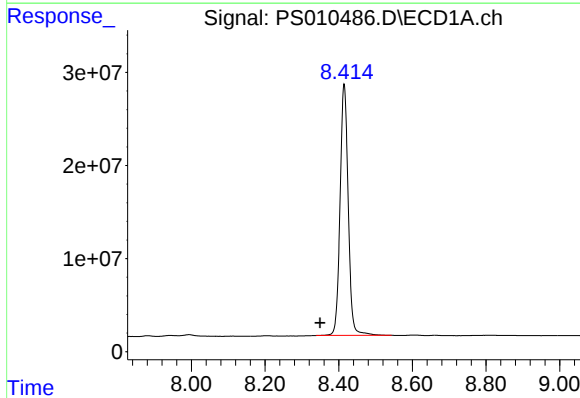


#9 2,4-D

R.T.: 8.415 min
Delta R.T.: 0.066 min
Response: 414272854
Conc: 586.41 ng/ml

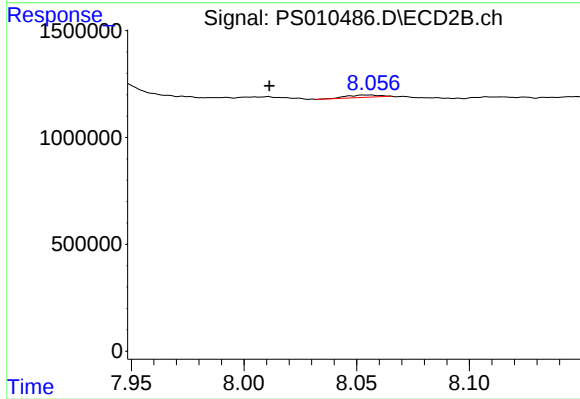

#9 2,4-D


R.T.: 8.055 min
Delta R.T.: 0.044 min
Response: 109790
Conc: N.D.

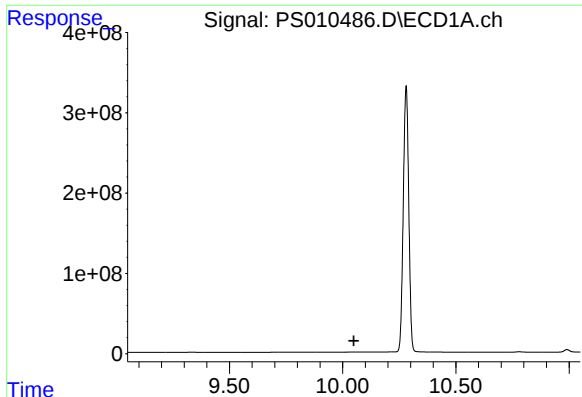

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

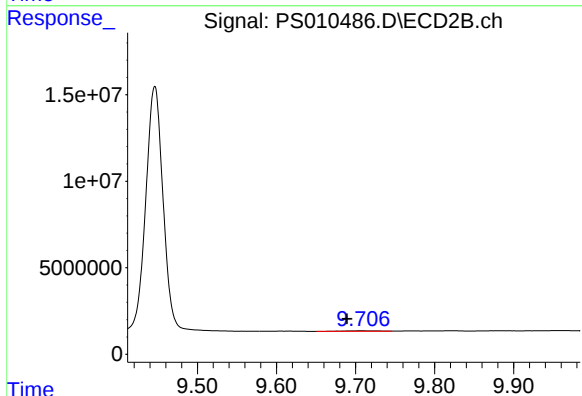


#13 2,4-DB

R.T.: 9.707 min
Delta R.T.: 0.018 min
Response: 950258
Conc: 2.38 ng/ml

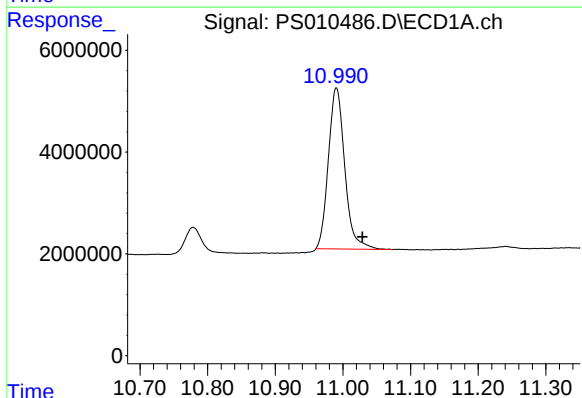

#15 Picloram

R.T.: 10.990 min
Delta R.T.: -0.039 min
Response: 53277489
Conc: 11.62 ng/ml

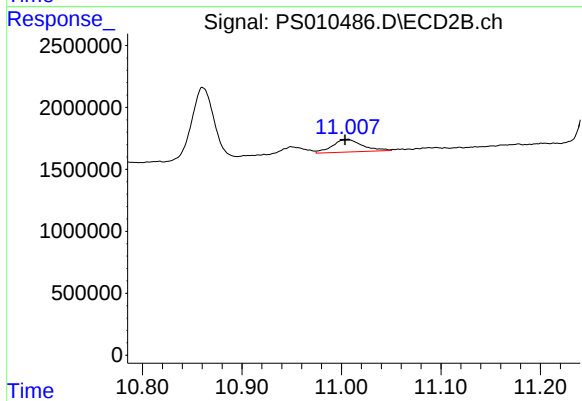

#15 Picloram

R.T.: 11.005 min
Delta R.T.: 0.002 min
Response: 2141424
Conc: N.D.