

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
 Data File : PS015085.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 18:56
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 03:44:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 03:42:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds									
10)	T	Pentachlo...	8.687	0.000	3857915	0	<MDL	N.D.	#
11)	T	2,4,5-TP ...	9.230	0.000	3260841	0	<MDL	N.D.	#
13)	T	2,4-DB	10.036	0.000	7598308	0	3.268	N.D.	#
15)	T	Picloram	11.028	10.856	25249133	5257558	1.540	1.337	
16)	T	DCPA	0.000	10.856f	0	5257558	N.D.	1.377	


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
Data File : PS015085.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 18:56
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 03:44:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
Quant Title : 8080.M
QLast Update : Fri May 28 03:42:14 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

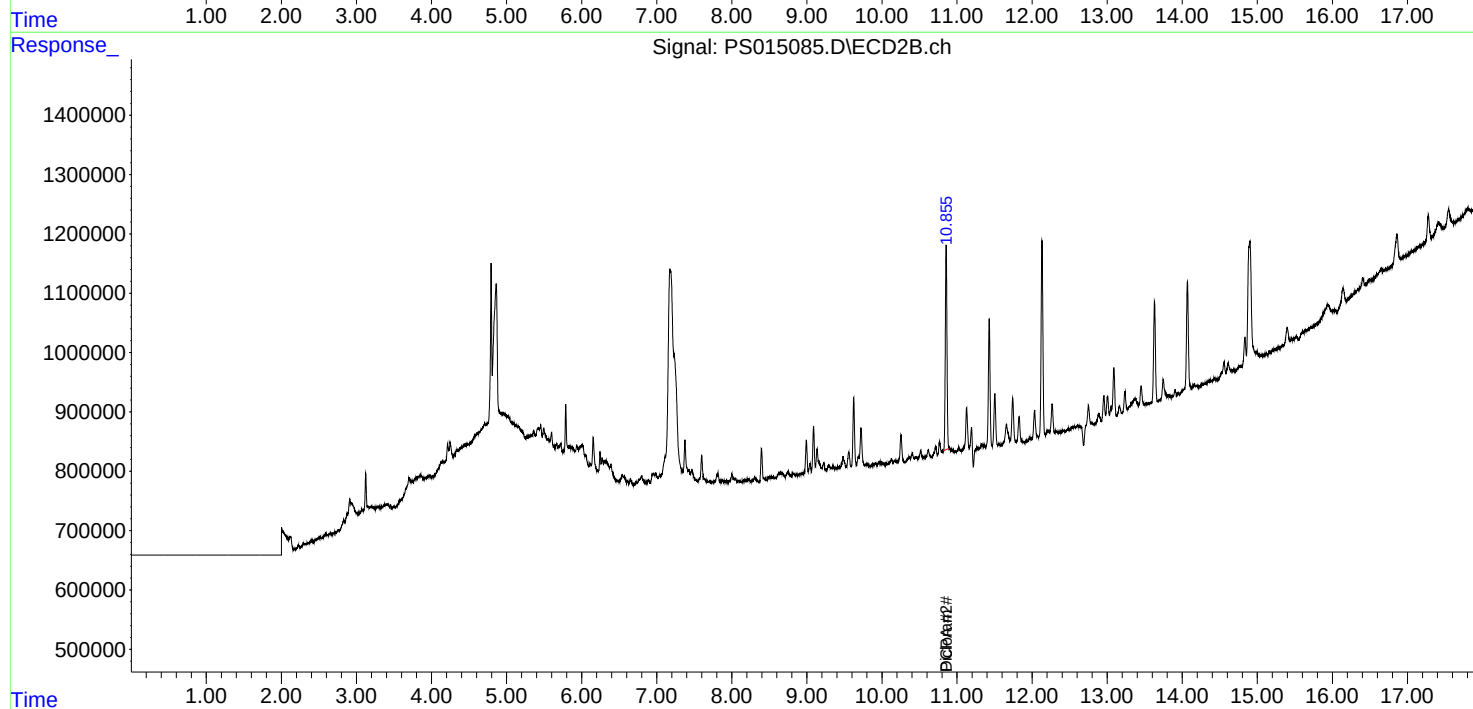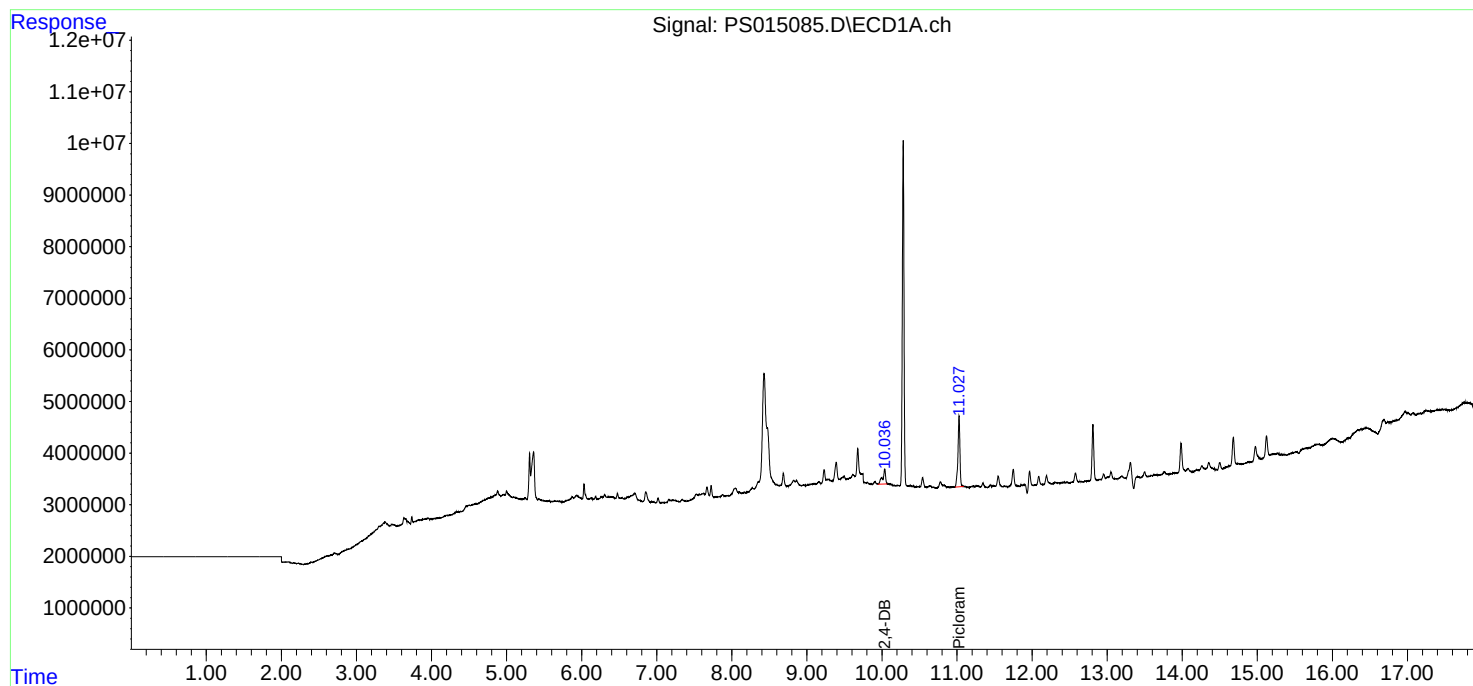

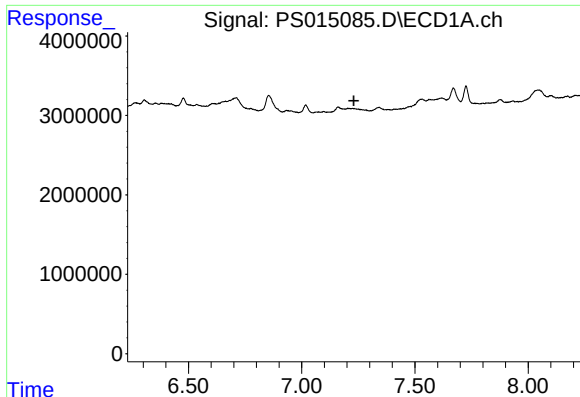


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.231 min
Response: 0
Conc: N.D.

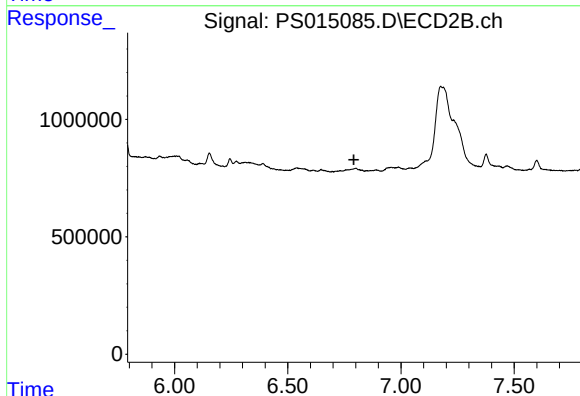


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.792 min
Response: 0
Conc: N.D.

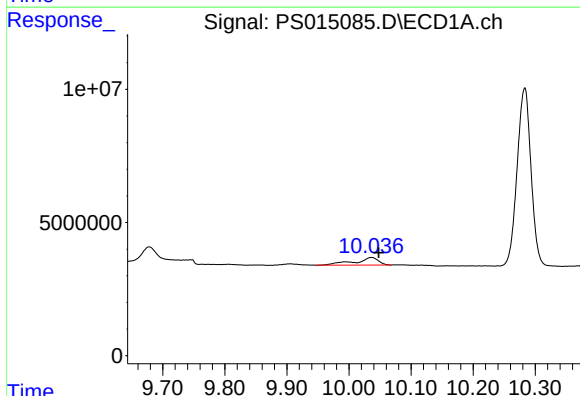


#13 2,4-DB

R.T.: 10.036 min
Delta R.T.: -0.012 min
Response: 7598308
Conc: 3.27 ng/ml

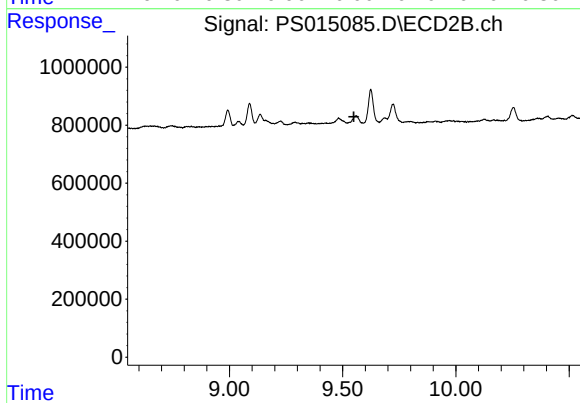


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.549 min
Response: 0
Conc: N.D.

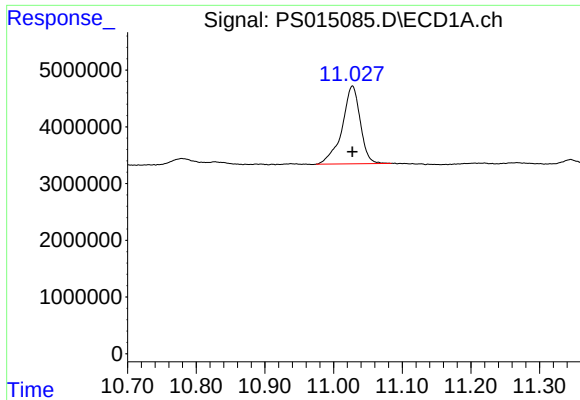


#15 Picloram

R.T.: 11.028 min
Delta R.T.: 0.000 min
Response: 25249133
Conc: 1.54 ng/ml

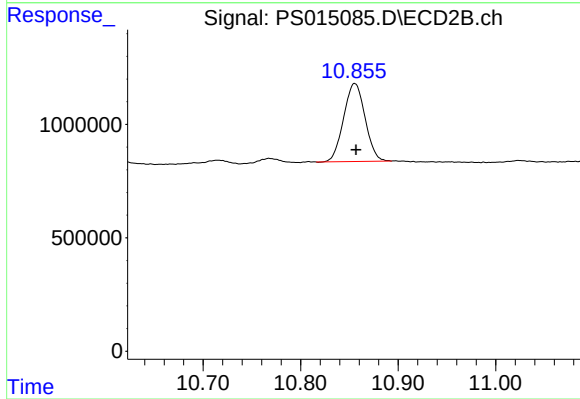


#15 Picloram

R.T.: 10.856 min
Delta R.T.: -0.001 min
Response: 5257558
Conc: 1.34 ng/ml

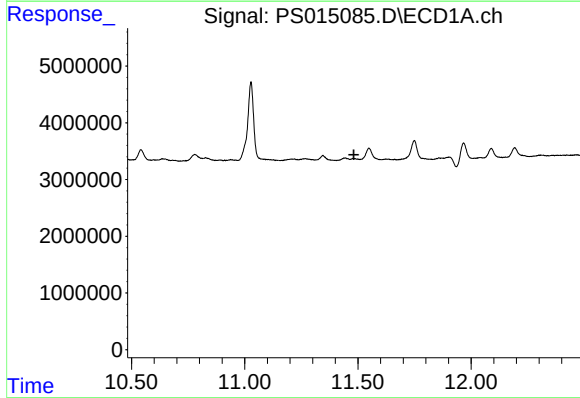

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.482 min
Response: 0
Conc: N.D.

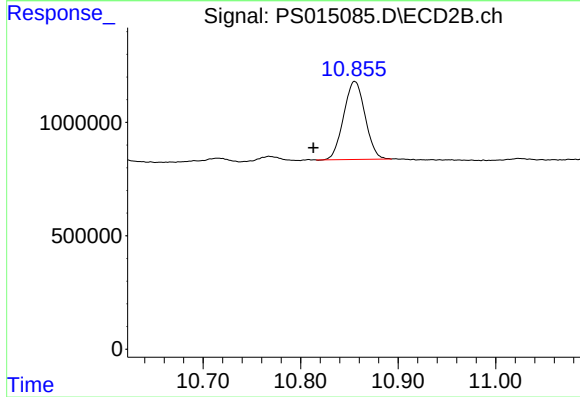

#16 DCPA

R.T.: 10.856 min
Delta R.T.: 0.042 min
Response: 5257558
Conc: 1.38 ng/ml