

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
 Data File : PS015086.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 19:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 03:44:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 03:42:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.792	1147.2E6	239.7E6	542.827	518.712
Target Compounds							
3) T	4-Nitroph...	7.029	0.000	5068803	0	4.237	N.D. #
7) T	MCPA	7.676f	0.000	6755169	0	<MDL	N.D. #
15) T	Picloram	11.027	10.856	19429821	4528654	1.185	1.152
16) T	DCPA	0.000	10.856f	0	4528654	N.D.	1.186


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
Data File : PS015086.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 19:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 03:44:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
Quant Title : 8080.M
QLast Update : Fri May 28 03:42:14 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

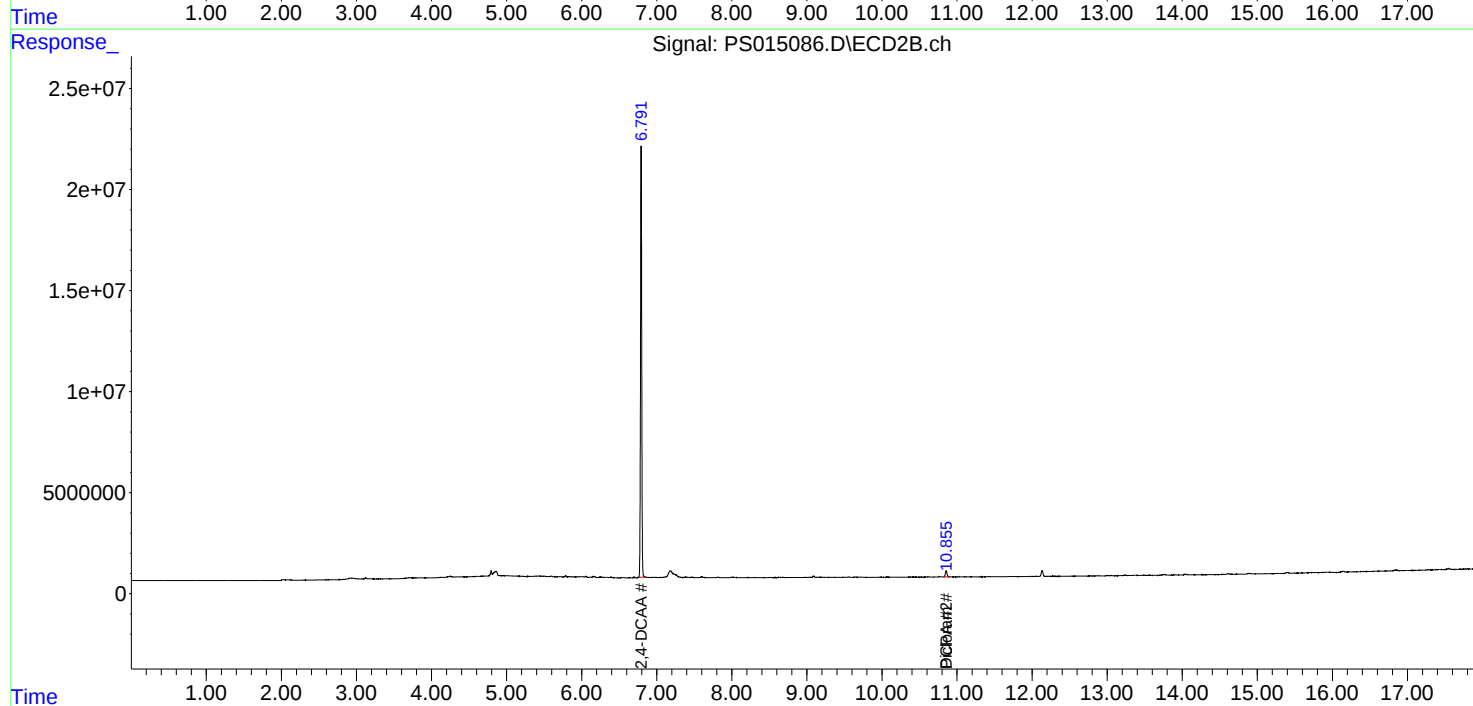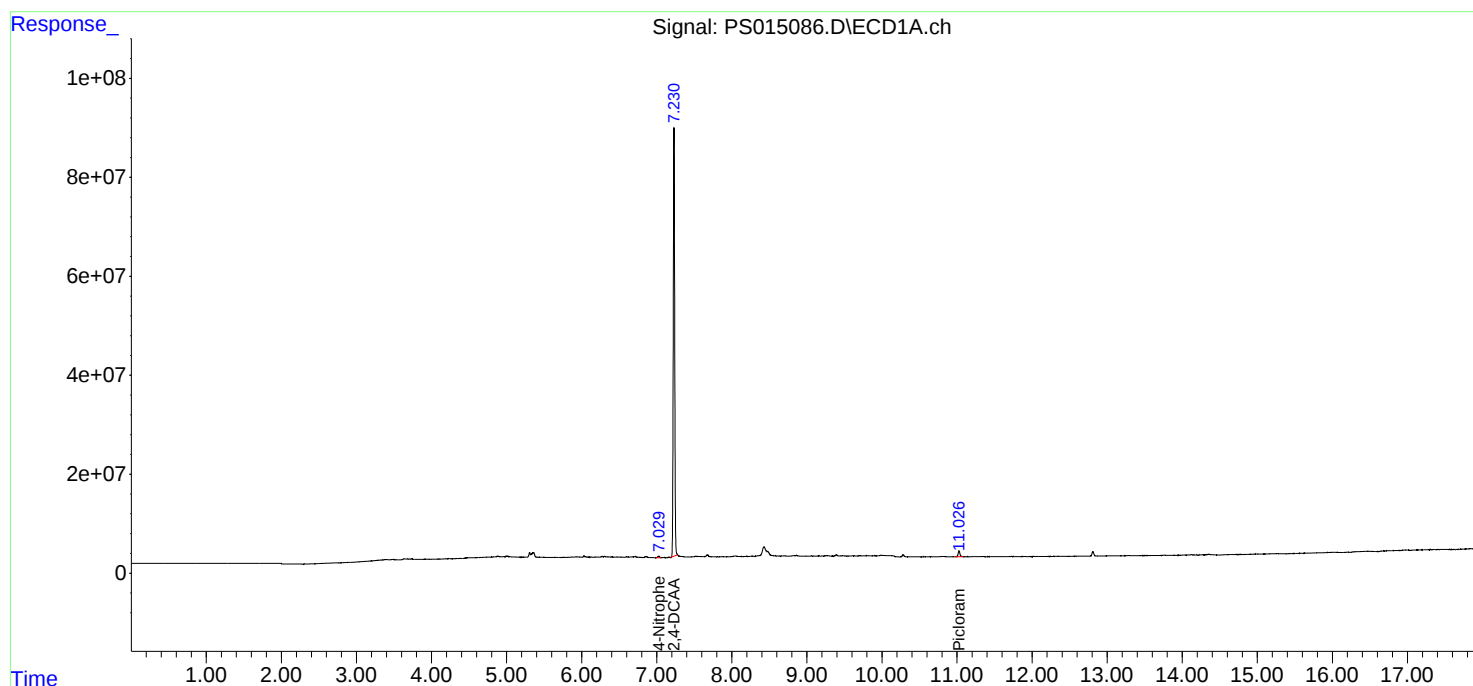

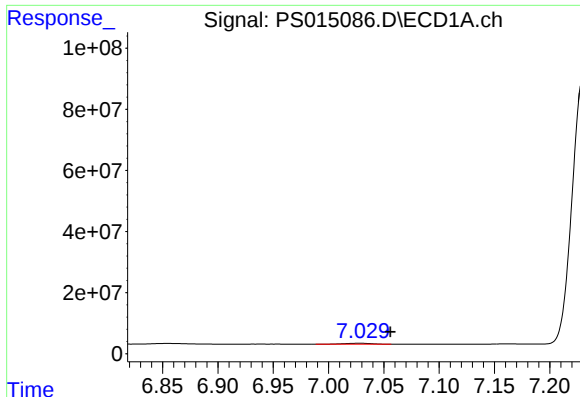


#3 4-Nitrophenol

R.T.: 7.029 min
Delta R.T.: -0.027 min
Response: 5068803
Conc: 4.24 ng/ml

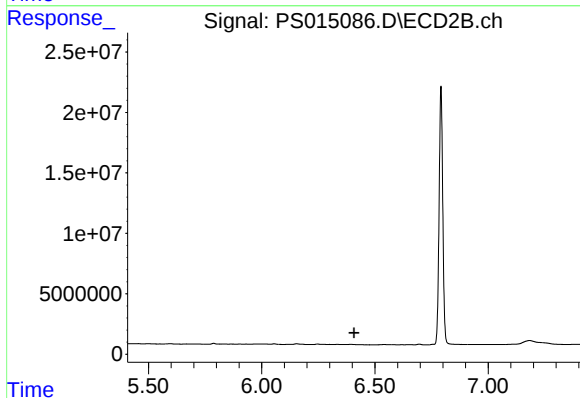


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.407 min
Response: 0
Conc: N.D.

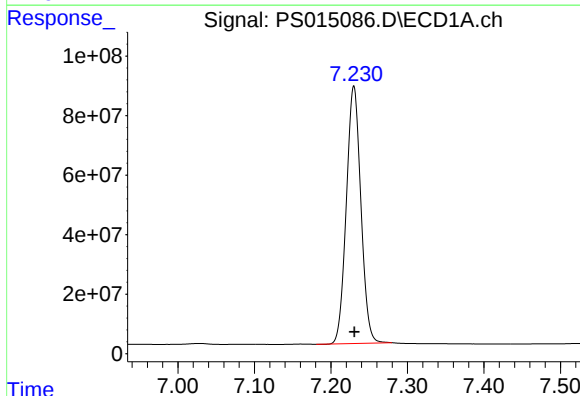


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.000 min
Response: 1147218520
Conc: 542.83 ng/ml

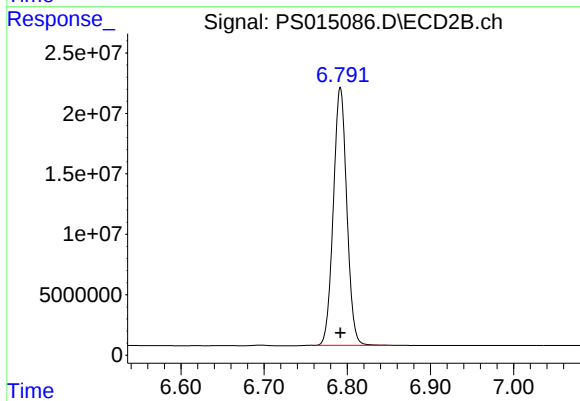


#4 2,4-DCAA

R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 239724477
Conc: 518.71 ng/ml

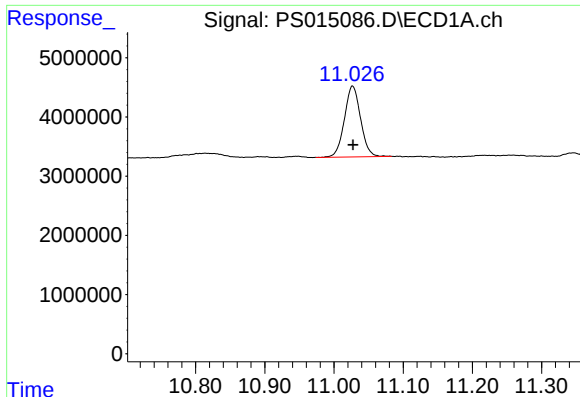


#15 Picloram

R.T.: 11.027 min
Delta R.T.: 0.000 min
Response: 19429821
Conc: 1.19 ng/ml

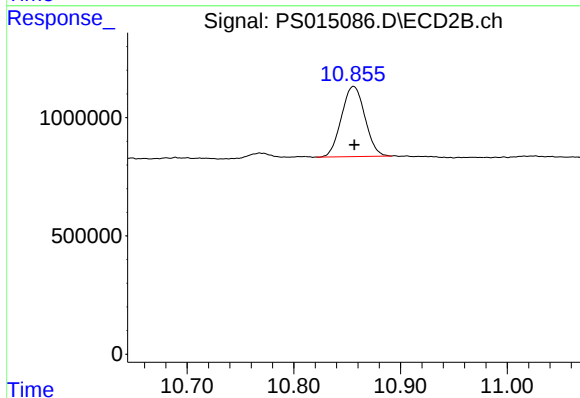


#15 Picloram

R.T.: 10.856 min
Delta R.T.: 0.000 min
Response: 4528654
Conc: 1.15 ng/ml

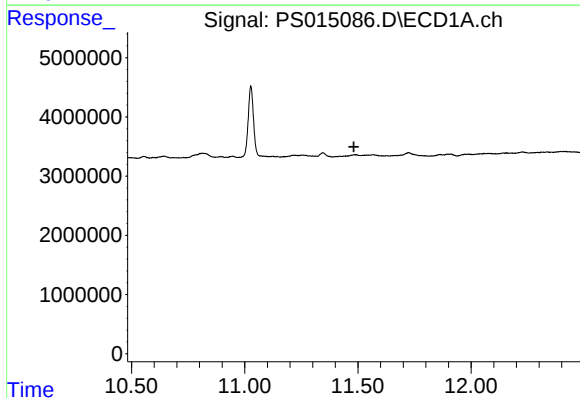

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.482 min
Response: 0
Conc: N.D.

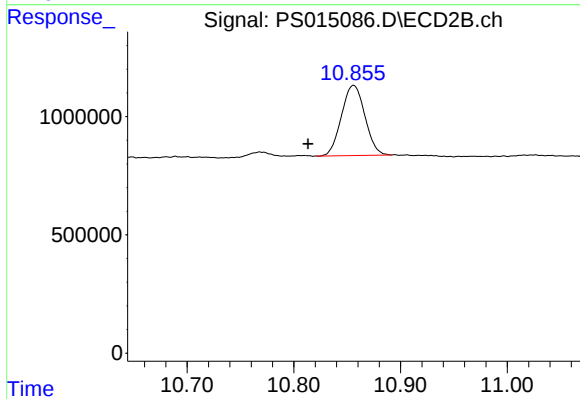

#16 DCPA

R.T.: 10.856 min
Delta R.T.: 0.043 min
Response: 4528654
Conc: 1.19 ng/ml