

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
 Data File : PS015089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 20:32
 Operator : DD\AJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 03:34:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 03:33:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.792	1605.5E6	336.9E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.050	2.535	1628.5E6	409.3E6	682.500	682.500
2) T	3,5-DICHL...	6.441	5.976	1995.4E6	472.2E6	697.500	697.500
3) T	4-Nitroph...	7.056	6.407	831.6E6	188.1E6	682.500	682.500
5) T	DICAMBA	7.424	6.957	5772.4E6	1331.0E6	705.000	705.000
6) T	MCPD	7.595	7.054	454.5E6	105.3E6	70.500	70.500
7) T	MCPA	7.744	7.267	638.2E6	156.3E6	69.750	69.750
8) T	DICHLORPROP	8.119	7.580	1434.9E6	325.2E6	705.000	705.000
9) T	2,4-D	8.347	7.870	1634.4E6	390.8E6	705.000	705.000
10) T	Pentachlo...	8.662	8.303	20798.3E6	4588.3E6	712.500	712.500
11) T	2,4,5-TP ...	9.213	8.664	7945.3E6	1784.5E6	712.500	712.500
12) T	2,4,5-T	9.496	9.041	7638.8E6	1816.4E6	712.500	712.500
13) T	2,4-DB	10.048	9.549	1638.0E6	235.1E6	712.500	712.500
14) T	DINOSEB	11.214	9.879	5690.7E6	1281.3E6	705.000	705.000
15) T	Picloram	11.027	10.857	11621.6E6	2761.6E6	712.500	712.500
16) T	DCPA	11.482	10.813	11448.9E6	2683.3E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
Data File : PS015089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 20:32
Operator : DD\AJ
Sample : HSTDICC750
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 03:34:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
Quant Title : 8080.M
QLast Update : Fri May 28 03:33:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

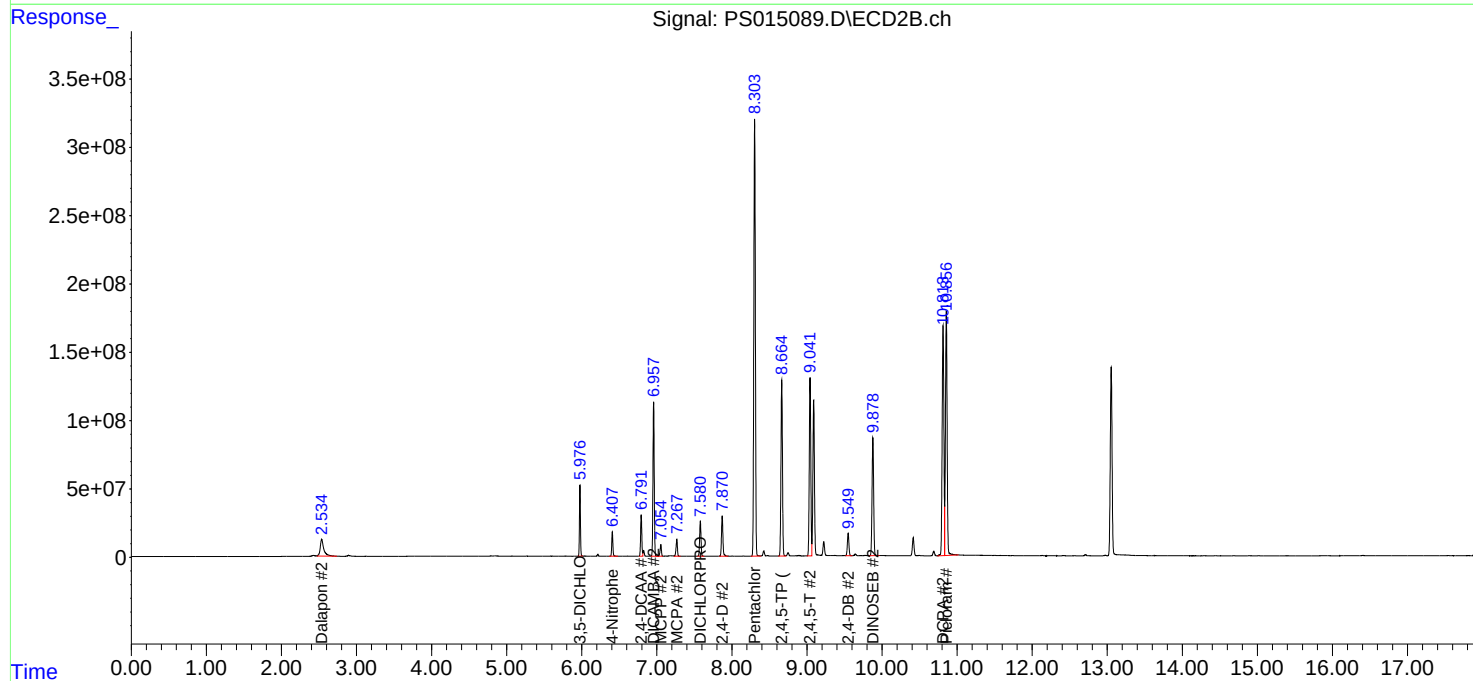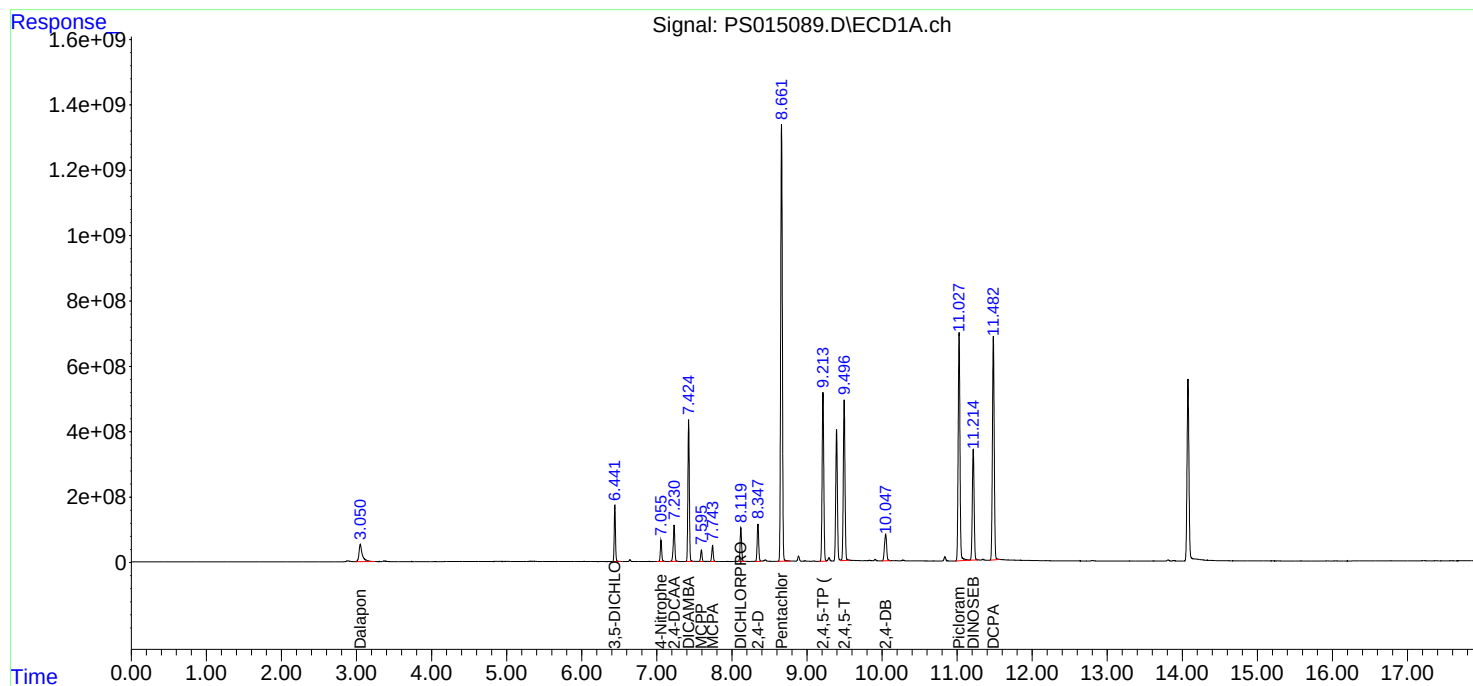


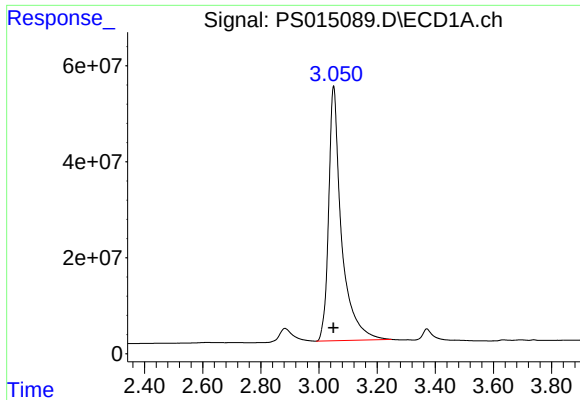

#1 Dalapon


R.T.: 3.050 min
Delta R.T.: 0.000 min
Response: 1628457864
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

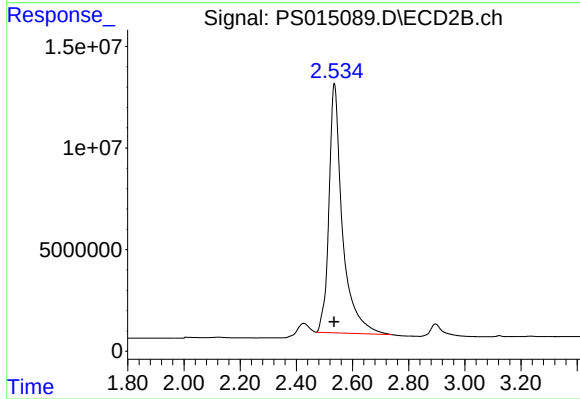


#1 Dalapon

R.T.: 2.535 min
Delta R.T.: 0.000 min
Response: 409286214
Conc: 682.50 ng/ml

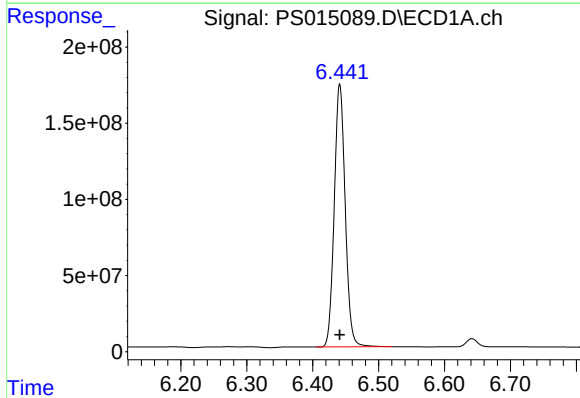


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.441 min
Delta R.T.: 0.000 min
Response: 1995406534
Conc: 697.50 ng/ml

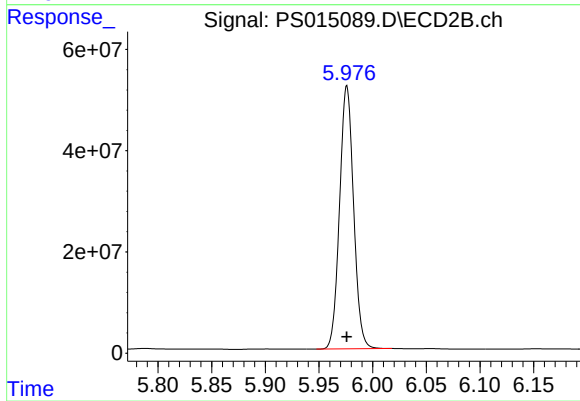

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 472215104
Conc: 697.50 ng/ml

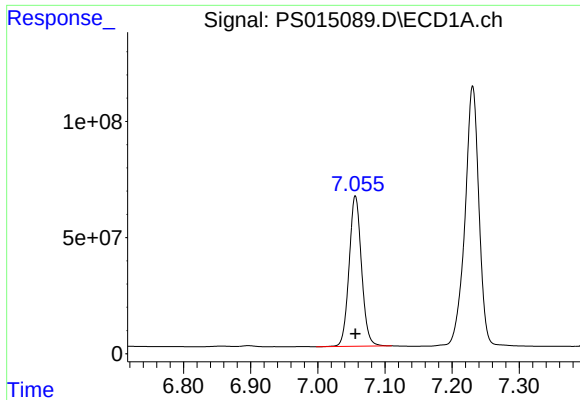

#3 4-Nitrophenol


R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 831553804
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

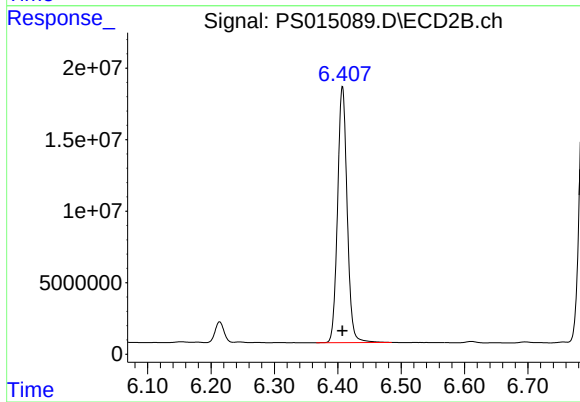


#3 4-Nitrophenol

R.T.: 6.407 min
Delta R.T.: 0.000 min
Response: 188149858
Conc: 682.50 ng/ml

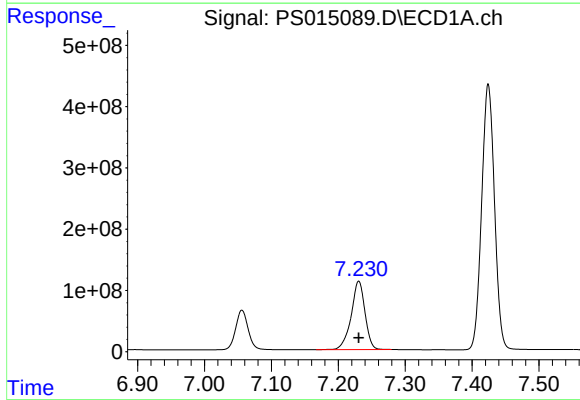


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 1605459946
Conc: 750.00 ng/ml

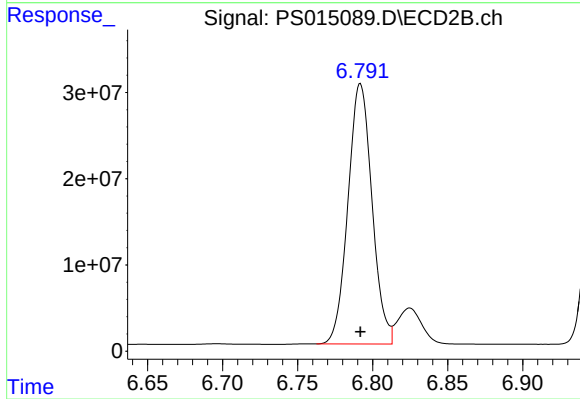

#4 2,4-DCAA


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 336861089
Conc: 750.00 ng/ml

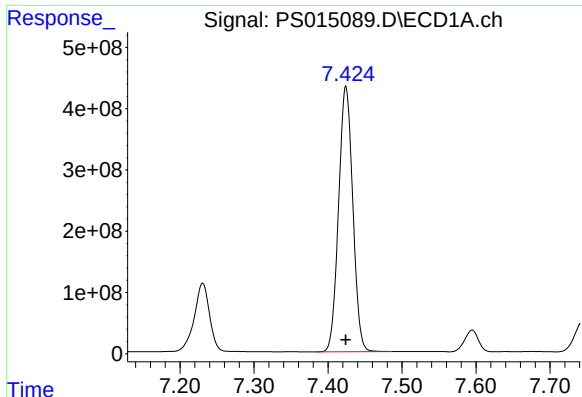

#5 DICAMBA


R.T.: 7.424 min
Delta R.T.: 0.000 min
Response: 5772394614
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

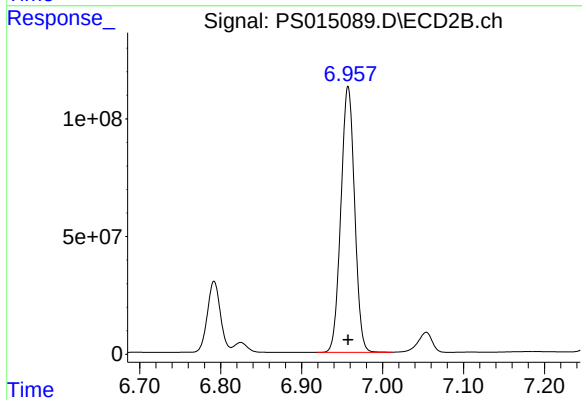


#5 DICAMBA

R.T.: 6.957 min
Delta R.T.: 0.000 min
Response: 1330971720
Conc: 705.00 ng/ml

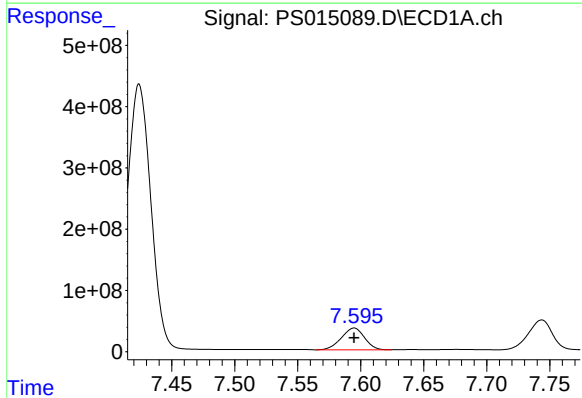


#6 MCP

R.T.: 7.595 min
Delta R.T.: 0.000 min
Response: 454460725
Conc: 70.50 ug/ml

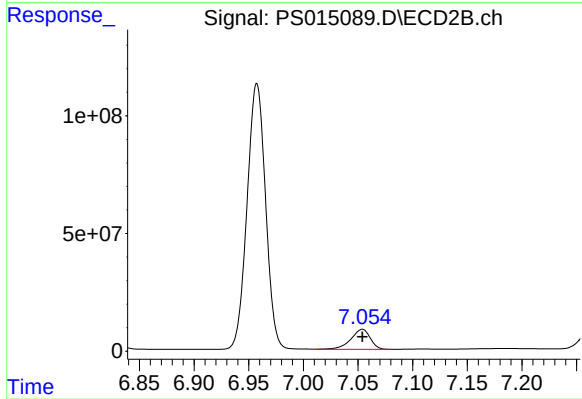

#6 MCP


R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 105286213
Conc: 70.50 ug/ml

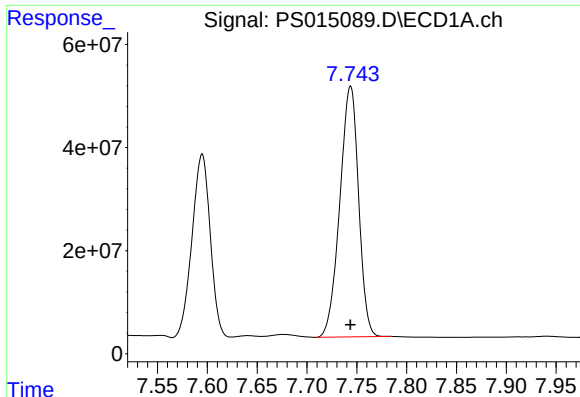

#7 MCPA


R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 638208387
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

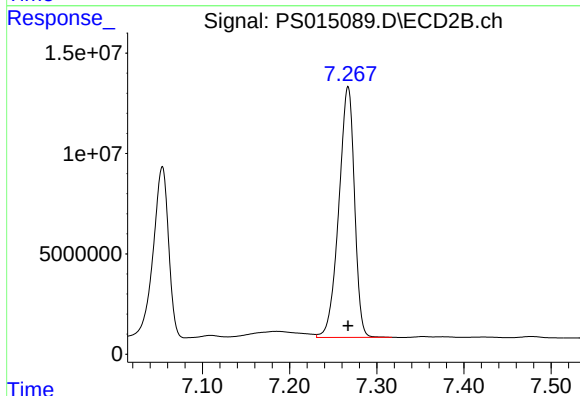


#7 MCPA

R.T.: 7.267 min
Delta R.T.: 0.000 min
Response: 156297928
Conc: 69.75 ug/ml

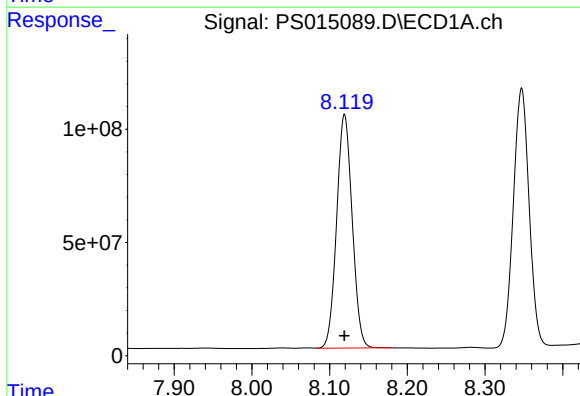


#8 DICHLORPROP

R.T.: 8.119 min
Delta R.T.: 0.000 min
Response: 1434947831
Conc: 705.00 ng/ml

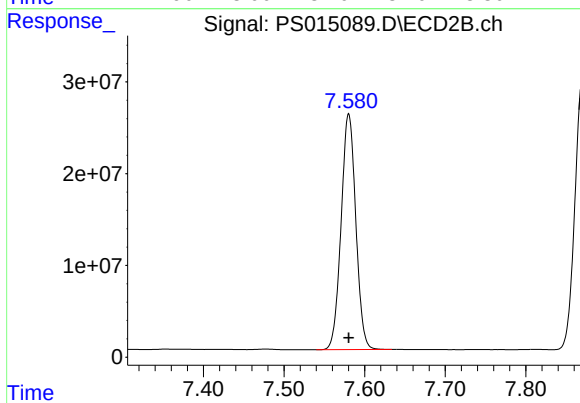

#8 DICHLORPROP


R.T.: 7.580 min
Delta R.T.: 0.000 min
Response: 325242628
Conc: 705.00 ng/ml

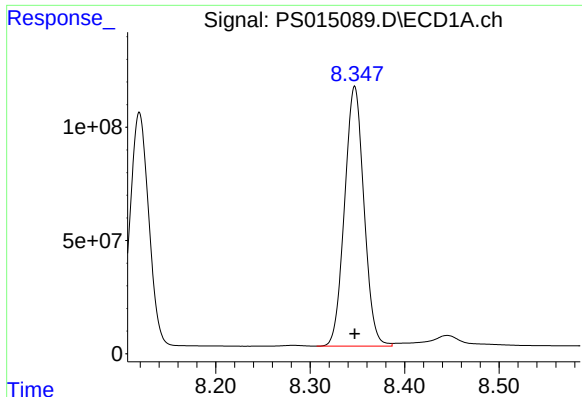

#9 2,4-D


R.T.: 8.347 min
Delta R.T.: 0.000 min
Response: 1634389235
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

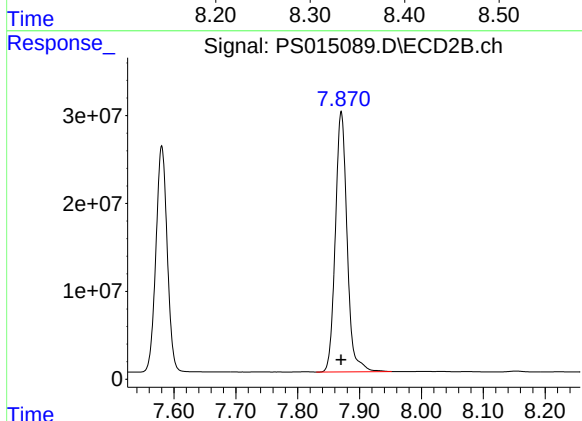


#9 2,4-D

R.T.: 7.870 min
Delta R.T.: 0.000 min
Response: 390824336
Conc: 705.00 ng/ml

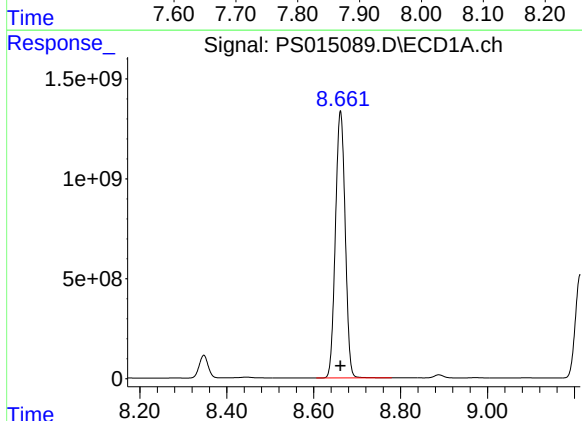


#10 Pentachlorophenol

R.T.: 8.662 min
Delta R.T.: 0.000 min
Response: 20798314850
Conc: 712.50 ng/ml

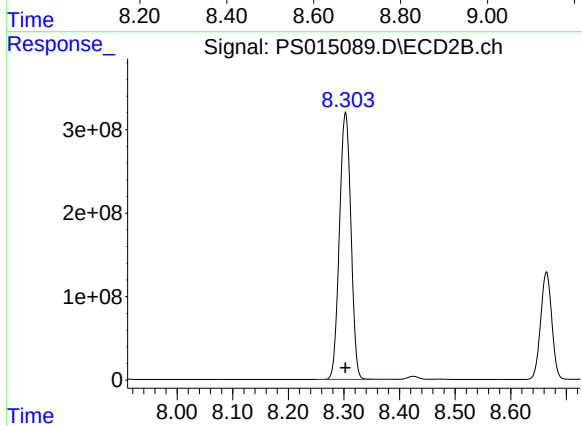

#10 Pentachlorophenol


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 4588311486
Conc: 712.50 ng/ml

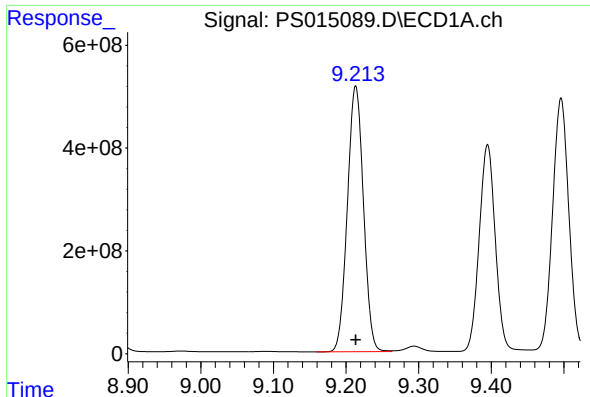

#11 2,4,5-TP (SILVEX)


R.T.: 9.213 min
Delta R.T.: 0.000 min
Response: 7945330116
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

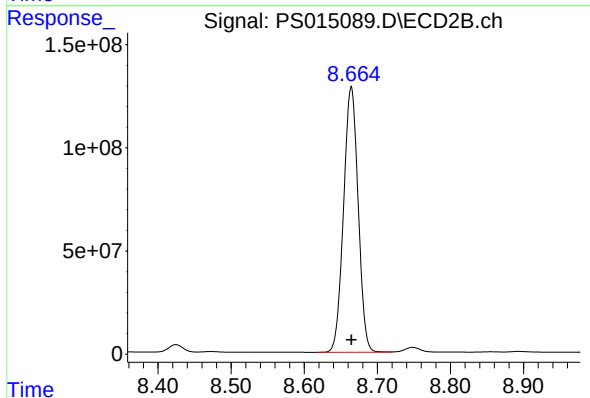


#11 2,4,5-TP (SILVEX)

R.T.: 8.664 min
Delta R.T.: 0.000 min
Response: 1784531494
Conc: 712.50 ng/ml

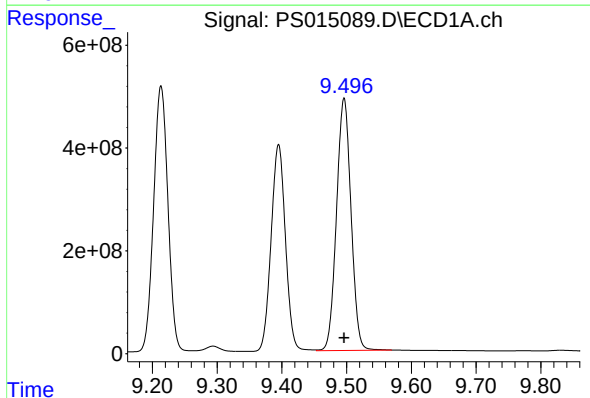


#12 2,4,5-T

R.T.: 9.496 min
Delta R.T.: 0.000 min
Response: 7638779518
Conc: 712.50 ng/ml

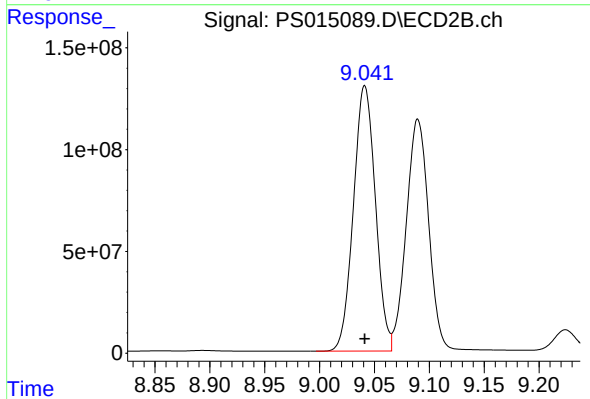

#12 2,4,5-T


R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 1816356479
Conc: 712.50 ng/ml

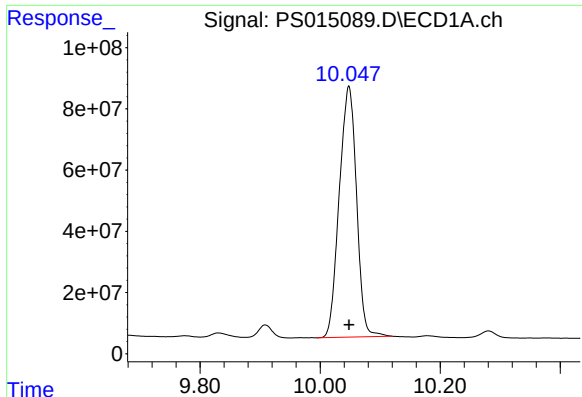

#13 2,4-DB


R.T.: 10.048 min
Delta R.T.: 0.000 min
Response: 1637991405
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

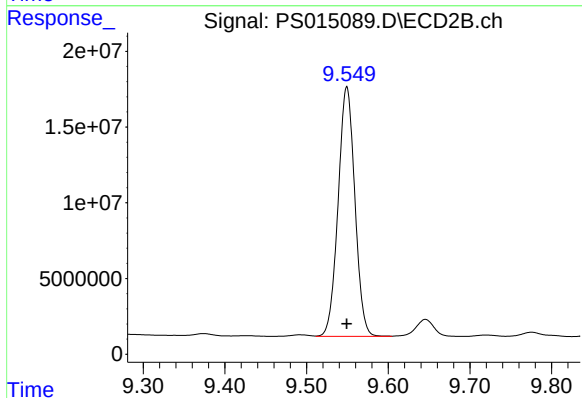


#13 2,4-DB

R.T.: 9.549 min
Delta R.T.: 0.000 min
Response: 235069805
Conc: 712.50 ng/ml

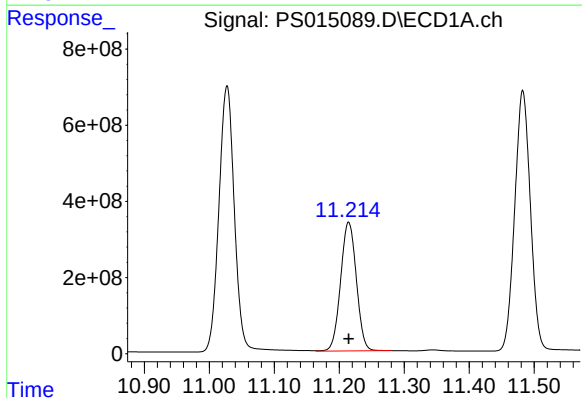


#14 DINOSEB

R.T.: 11.214 min
Delta R.T.: 0.000 min
Response: 5690659445
Conc: 705.00 ng/ml

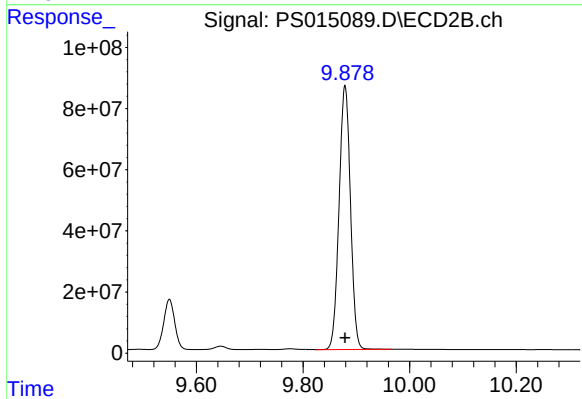

#14 DINOSEB


R.T.: 9.879 min
Delta R.T.: 0.000 min
Response: 1281255498
Conc: 705.00 ng/ml

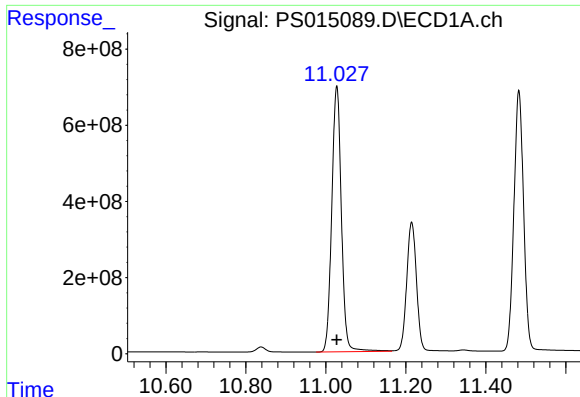

#15 Picloram


R.T.: 11.027 min
Delta R.T.: 0.000 min
Response: 11621596848
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

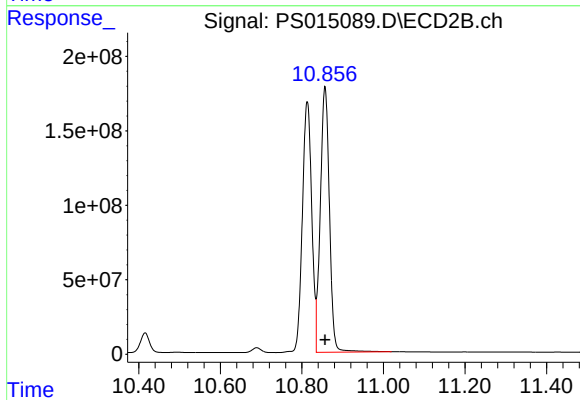


#15 Picloram

R.T.: 10.857 min
Delta R.T.: 0.000 min
Response: 2761621252
Conc: 712.50 ng/ml

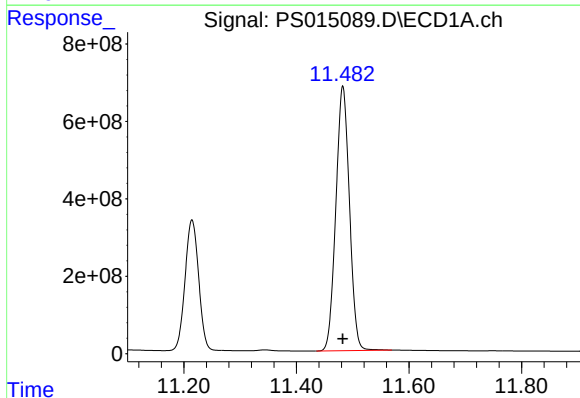

#16 DCPA

R.T.: 11.482 min
Delta R.T.: 0.000 min
Response: 11448891473
Conc: 720.00 ng/ml

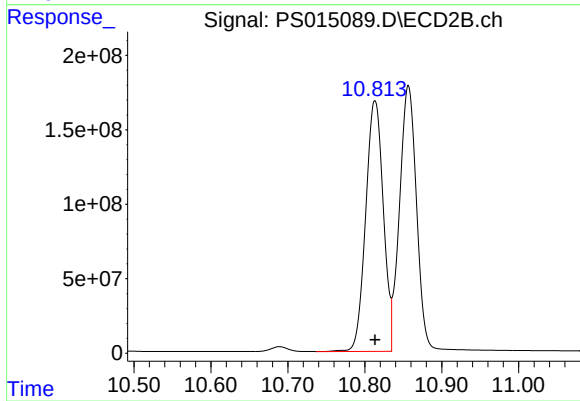

#16 DCPA

R.T.: 10.813 min
Delta R.T.: 0.000 min
Response: 2683265766
Conc: 720.00 ng/ml