

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
 Data File : PS015092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 21:44
 Operator : DD\AJ
 Sample : HSTDICV750
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ICVPS052721

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 03:45:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 03:42:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.792	1581.3E6	343.4E6	748.241	742.972
Target Compounds							
1) T	Dalapon	3.051	2.536	1592.6E6	414.2E6	695.910	673.033
2) T	3,5-DICHL...	6.442	5.976	1968.3E6	481.6E6	703.029	699.512
3) T	4-Nitroph...	7.057	6.408	825.2E6	192.5E6	689.755	680.615
5) T	DICAMBA	7.425	6.958	5719.5E6	1373.8E6	721.488	719.394
6) T	MCPD	7.596	7.054	442.3E6	108.2E6	72.334	70.635
7) T	MCPA	7.745	7.268	614.8E6	157.9E6	70.143	67.891
8) T	DICHLORPROP	8.121	7.580	1450.5E6	343.2E6	735.124	721.080
9) T	2,4-D	8.348	7.871	1718.3E6	430.5E6	765.951	753.863
10) T	Pentachlo...	8.663	8.303	20321.9E6	4637.4E6	722.911	708.526
11) T	2,4,5-TP ...	9.214	8.664	8083.7E6	1854.4E6	736.790	725.896
12) T	2,4,5-T	9.497	9.041	7941.9E6	1852.1E6	730.310	712.679
13) T	2,4-DB	10.048	9.549	1691.2E6	241.5E6	727.400	706.181
14) T	DINOSEB	11.215	9.879	5976.7E6	1319.9E6	729.882	709.535
15) T	Picloram	11.027	10.856	12042.4E6	2806.9E6	734.588	713.885
16) T	DCPA	11.483	10.813	10506.5E6	2387.1E6	648.928	625.380



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
Data File : PS015092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 21:44
Operator : DD\AJ
Sample : HSTDICV750
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 03:45:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
Quant Title : 8080.M
QLast Update : Fri May 28 03:42:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

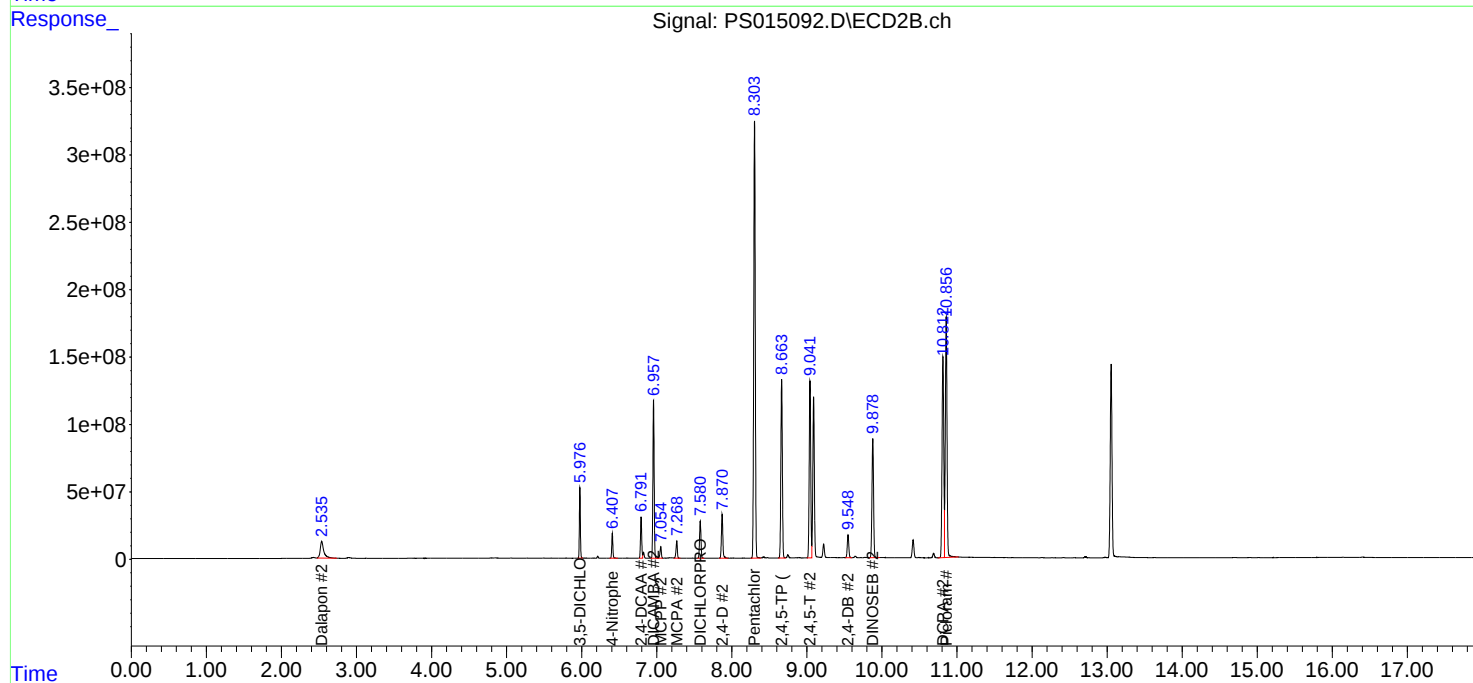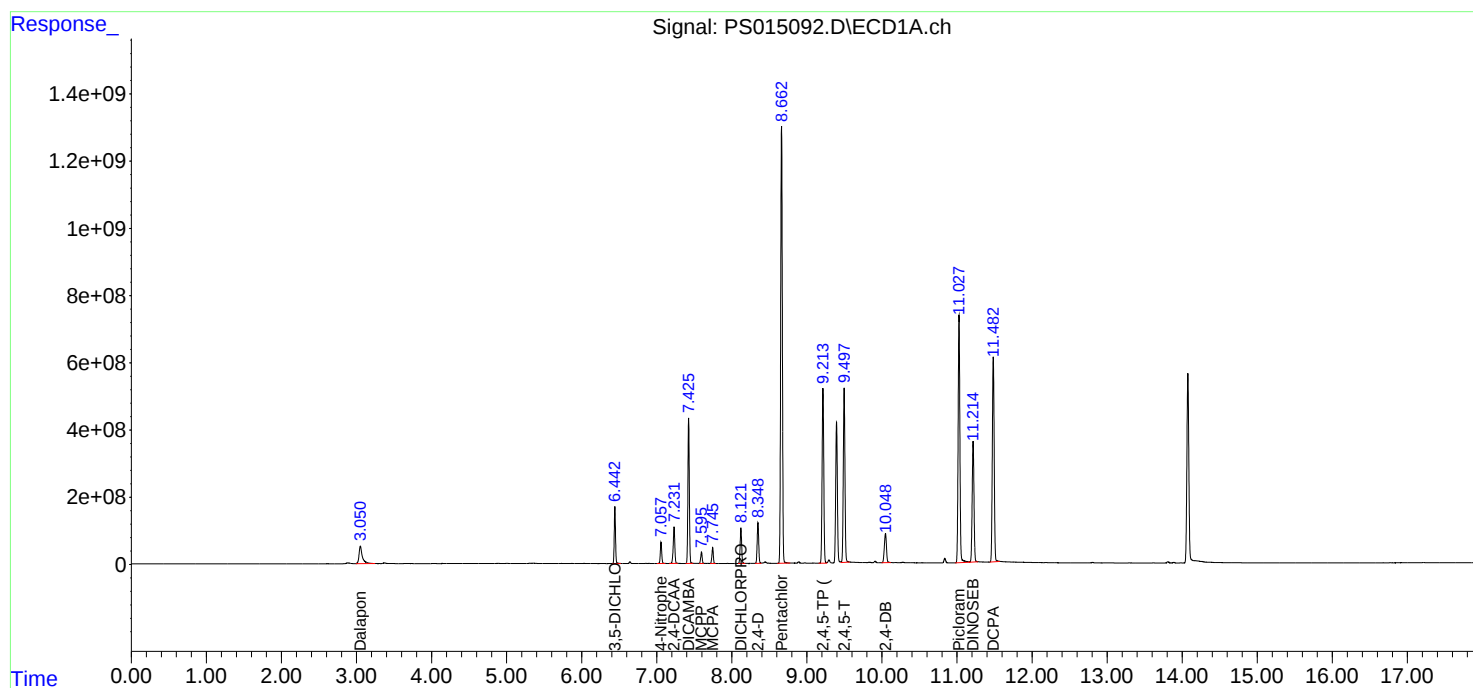


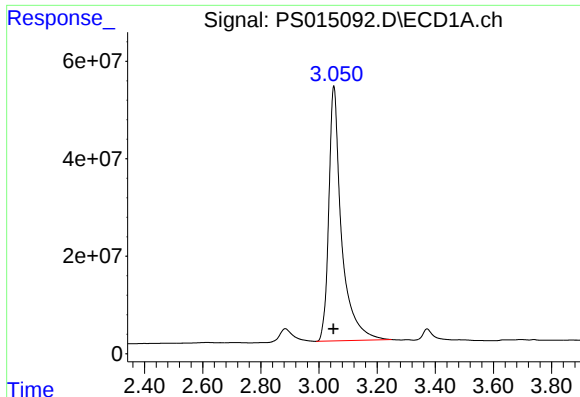

#1 Dalapon


R.T.: 3.051 min
Delta R.T.: 0.000 min
Response: 1592556011
Conc: 695.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

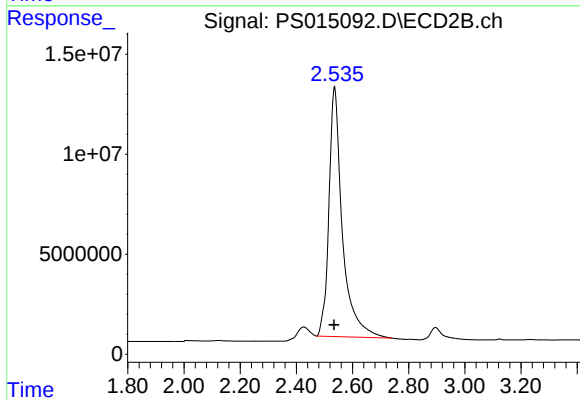


#1 Dalapon

R.T.: 2.536 min
Delta R.T.: 0.000 min
Response: 414181630
Conc: 673.03 ng/ml

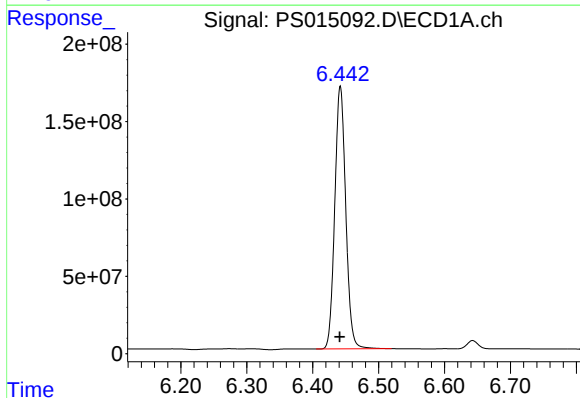


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.442 min
Delta R.T.: 0.000 min
Response: 1968311655
Conc: 703.03 ng/ml

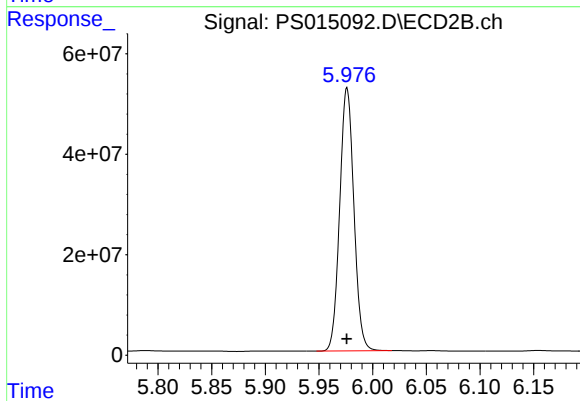

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 481642777
Conc: 699.51 ng/ml

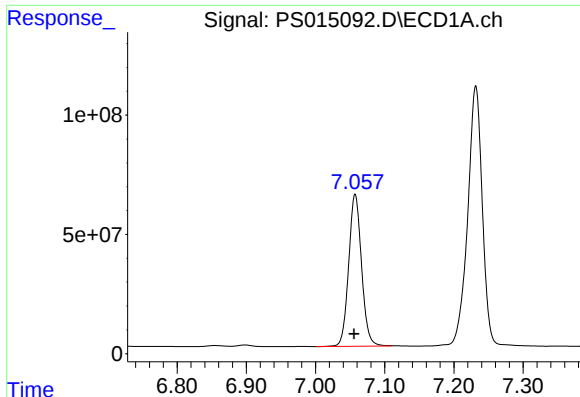

#3 4-Nitrophenol


R.T.: 7.057 min
Delta R.T.: 0.001 min
Response: 825189477
Conc: 689.76 ng/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

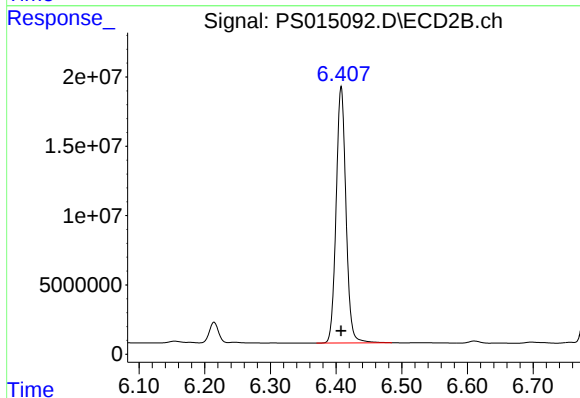


#3 4-Nitrophenol

R.T.: 6.408 min
Delta R.T.: 0.000 min
Response: 192521074
Conc: 680.62 ng/ml

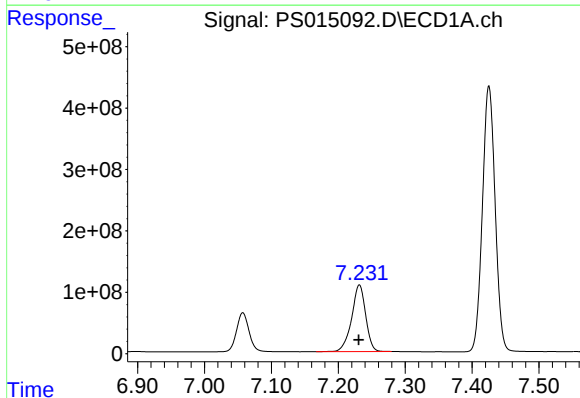


#4 2,4-DCAA

R.T.: 7.232 min
Delta R.T.: 0.000 min
Response: 1581343935
Conc: 748.24 ng/ml

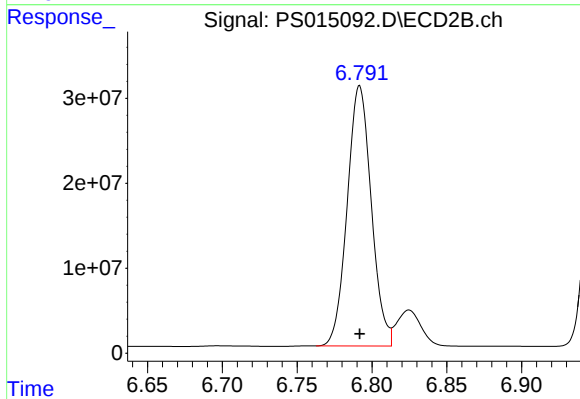

#4 2,4-DCAA


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 343366608
Conc: 742.97 ng/ml

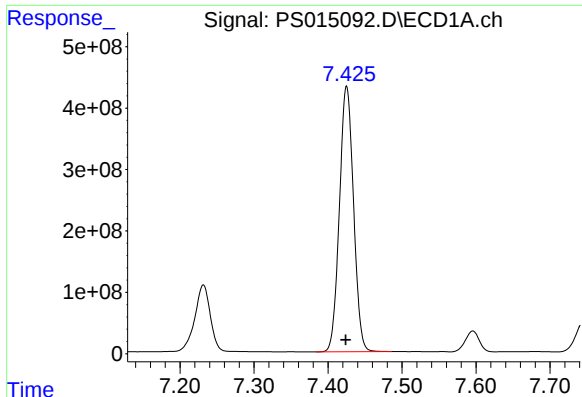

#5 DICAMBA


R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 5719540302
Conc: 721.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

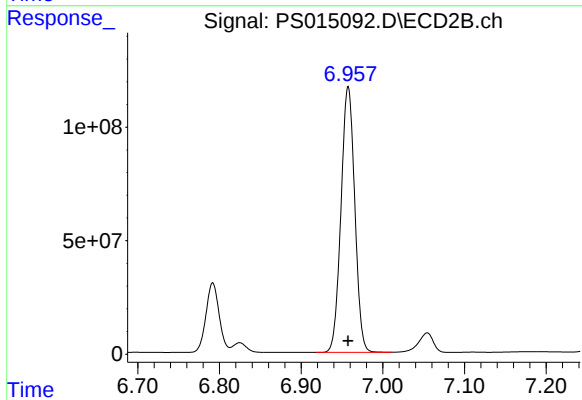


#5 DICAMBA

R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 1373787308
Conc: 719.39 ng/ml

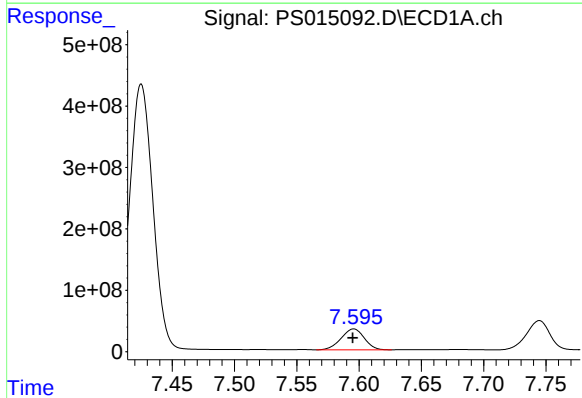


#6 MCP

R.T.: 7.596 min
Delta R.T.: 0.000 min
Response: 442272149
Conc: 72.33 ug/ml

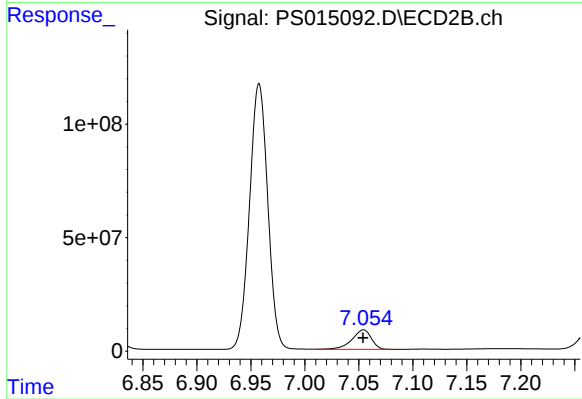

#6 MCP


R.T.: 7.054 min
Delta R.T.: 0.000 min
Response: 108198238
Conc: 70.64 ug/ml

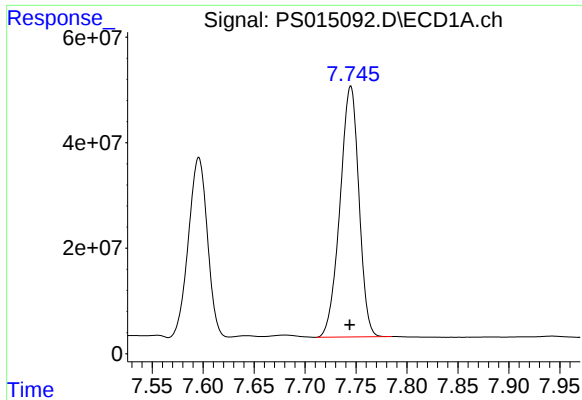

#7 MCPA


R.T.: 7.745 min
Delta R.T.: 0.001 min
Response: 614839069
Conc: 70.14 ug/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

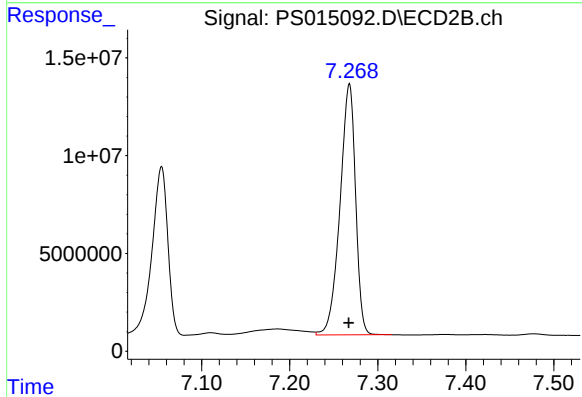


#7 MCPA

R.T.: 7.268 min
Delta R.T.: 0.000 min
Response: 157936947
Conc: 67.89 ug/ml

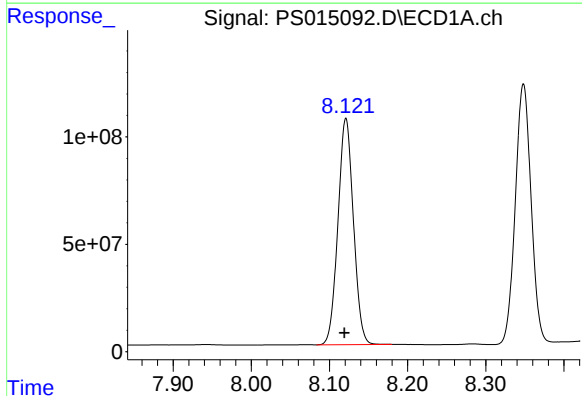


#8 DICHLORPROP

R.T.: 8.121 min
Delta R.T.: 0.002 min
Response: 1450521432
Conc: 735.12 ng/ml

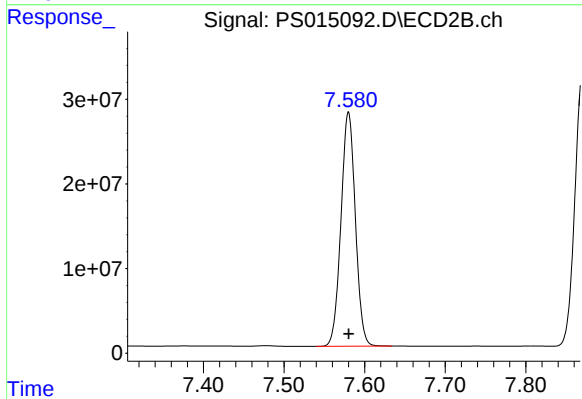

#8 DICHLORPROP


R.T.: 7.580 min
Delta R.T.: 0.000 min
Response: 343169280
Conc: 721.08 ng/ml

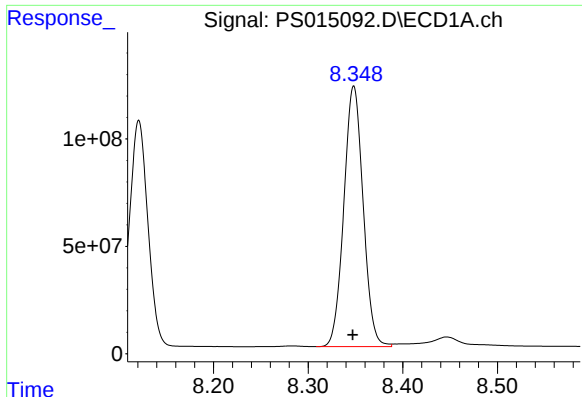

#9 2,4-D


R.T.: 8.348 min
Delta R.T.: 0.001 min
Response: 1718304012
Conc: 765.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

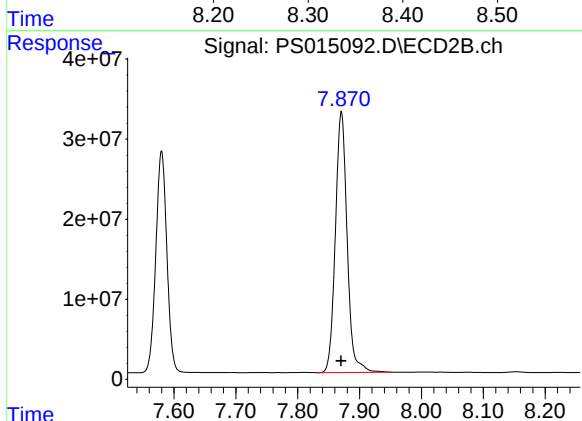


#9 2,4-D

R.T.: 7.871 min
Delta R.T.: 0.000 min
Response: 430451140
Conc: 753.86 ng/ml

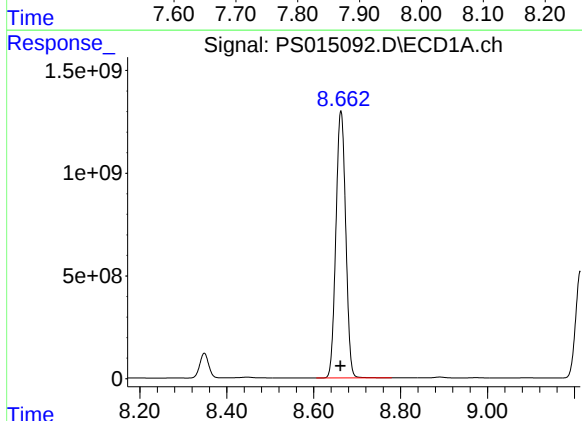


#10 Pentachlorophenol

R.T.: 8.663 min
Delta R.T.: 0.001 min
Response: 20321919651
Conc: 722.91 ng/ml

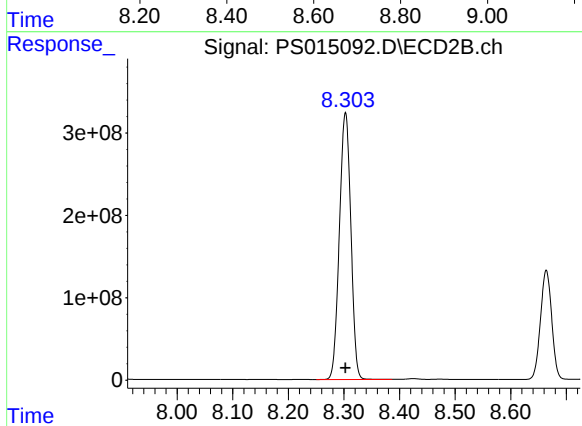

#10 Pentachlorophenol


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 4637379959
Conc: 708.53 ng/ml

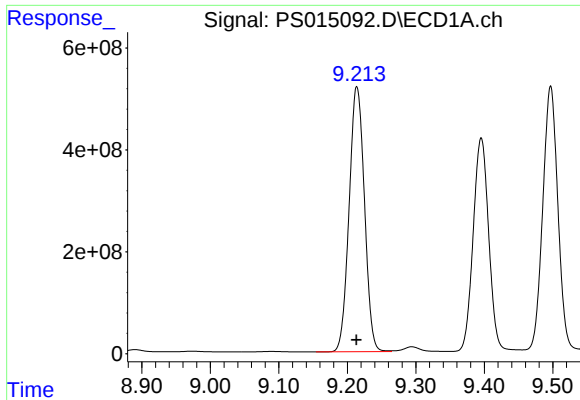

#11 2,4,5-TP (SILVEX)


R.T.: 9.214 min
Delta R.T.: 0.000 min
Response: 8083731085
Conc: 736.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

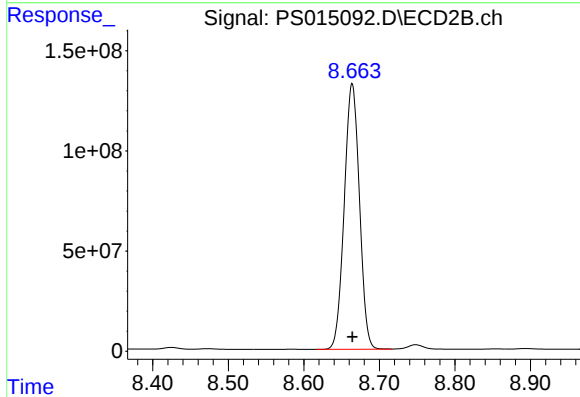


#11 2,4,5-TP (SILVEX)

R.T.: 8.664 min
Delta R.T.: 0.000 min
Response: 1854410705
Conc: 725.90 ng/ml

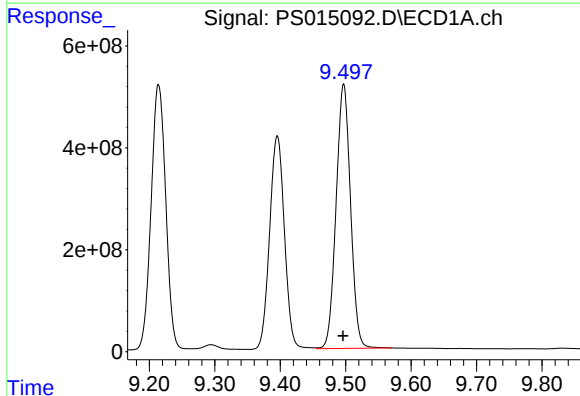


#12 2,4,5-T

R.T.: 9.497 min
Delta R.T.: 0.000 min
Response: 7941874175
Conc: 730.31 ng/ml

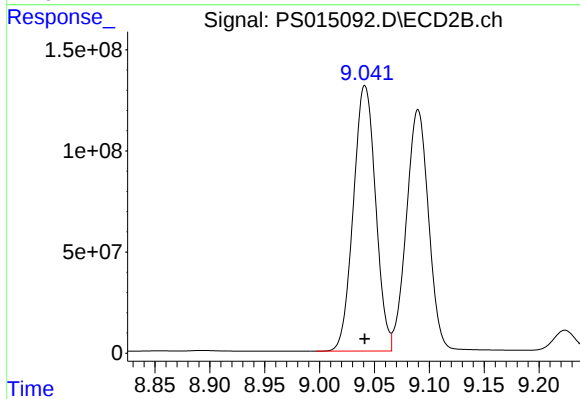

#12 2,4,5-T


R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 1852072317
Conc: 712.68 ng/ml

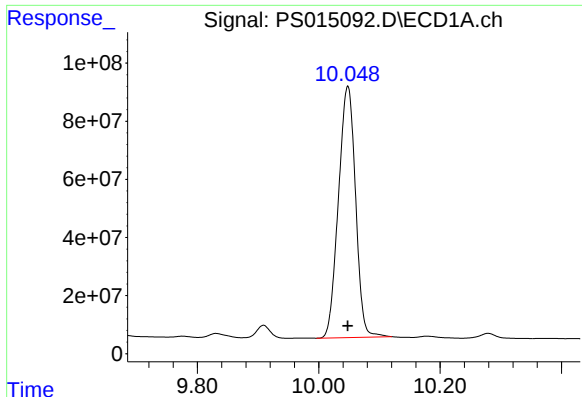

#13 2,4-DB


R.T.: 10.048 min
Delta R.T.: 0.000 min
Response: 1691245156
Conc: 727.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

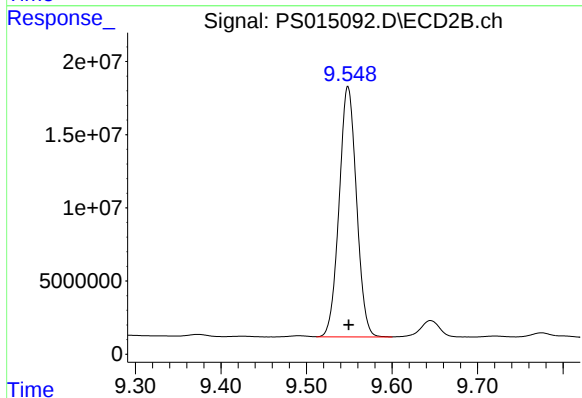


#13 2,4-DB

R.T.: 9.549 min
Delta R.T.: 0.000 min
Response: 241464259
Conc: 706.18 ng/ml

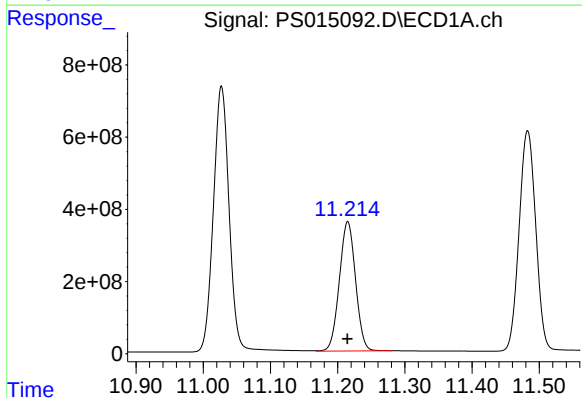


#14 DINOSEB

R.T.: 11.215 min
Delta R.T.: 0.000 min
Response: 5976722650
Conc: 729.88 ng/ml

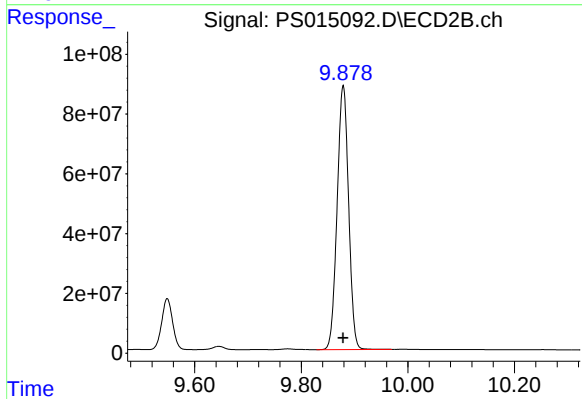

#14 DINOSEB


R.T.: 9.879 min
Delta R.T.: 0.000 min
Response: 1319873884
Conc: 709.54 ng/ml

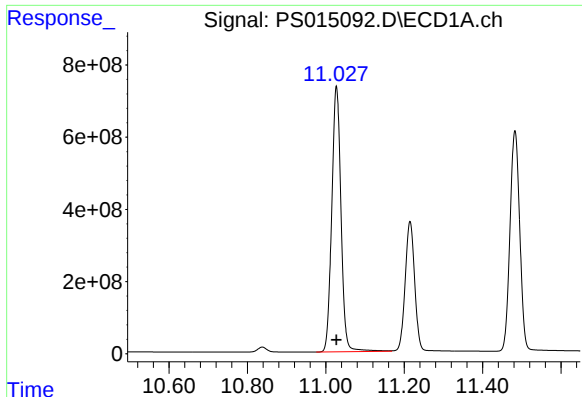

#15 Picloram


R.T.: 11.027 min
Delta R.T.: 0.000 min
Response: 12042421614
Conc: 734.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
ICVPS052721

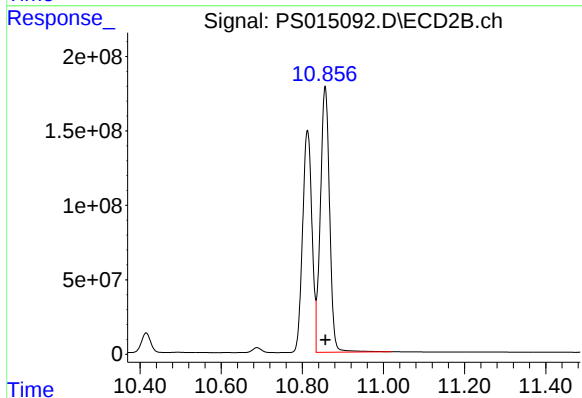


#15 Picloram

R.T.: 10.856 min
Delta R.T.: 0.000 min
Response: 2806899265
Conc: 713.88 ng/ml

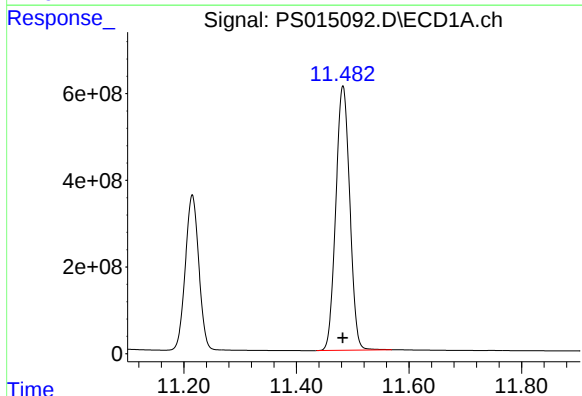

#16 DCPA

R.T.: 11.483 min
Delta R.T.: 0.000 min
Response: 10506460958
Conc: 648.93 ng/ml

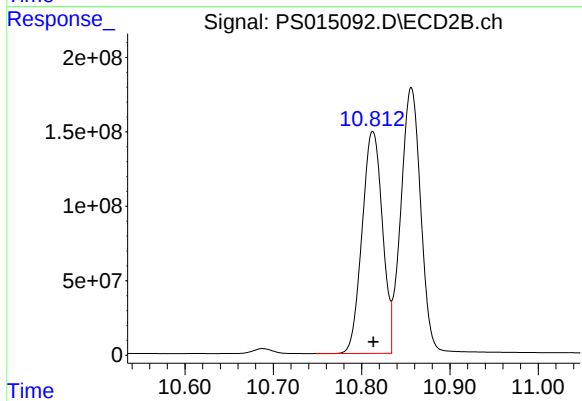

#16 DCPA

R.T.: 10.813 min
Delta R.T.: 0.000 min
Response: 2387084403
Conc: 625.38 ng/ml