

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
 Data File : PS015094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2021 22:57
 Operator : DD\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 03:45:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 03:42:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.792	1745.1E6	354.7E6	825.722	767.496
Target Compounds							
1) T	Dalapon	3.051	2.534	1781.0E6	429.2E6	778.257	697.498
2) T	3,5-DICHL...	6.442	5.976	2142.9E6	493.8E6	765.371	717.237
3) T	4-Nitroph...	7.056	6.408	906.5E6	197.2E6	757.735	697.147
5) T	DICAMBA	7.425	6.958	6274.4E6	1398.6E6	791.484	732.371
6) T	MCPD	7.596	7.055	486.4E6	111.3E6	79.543	72.652
7) T	MCPA	7.744	7.268	678.9E6	164.5E6	77.448	70.696
8) T	DICHLORPROP	8.120	7.580	1501.2E6	343.4E6	760.806	721.543
9) T	2,4-D	8.348	7.871	1710.7E6	414.2E6	762.565	725.465
10) T	Pentachlo...	8.662	8.303	21673.3E6	4798.5E6	770.982	733.145
11) T	2,4,5-TP ...	9.214	8.665	8533.6E6	1898.9E6	777.791	743.309
12) T	2,4,5-T	9.496	9.041	8562.2E6	1938.0E6	787.354	745.753
13) T	2,4-DB	10.048	9.549	1878.0E6	252.5E6	807.733	738.493
14) T	DINOSEB	11.214	9.878	6318.9E6	1371.9E6	771.664	737.482
15) T	Picloram	11.027	10.856	13113.7E6	2982.8E6	799.938	758.617
16) T	DCPA	11.483	10.813	12640.9E6	2873.7E6	780.758	752.871



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052721\
Data File : PS015094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2021 22:57
Operator : DD\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 03:45:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052721.M
Quant Title : 8080.M
QLast Update : Fri May 28 03:42:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

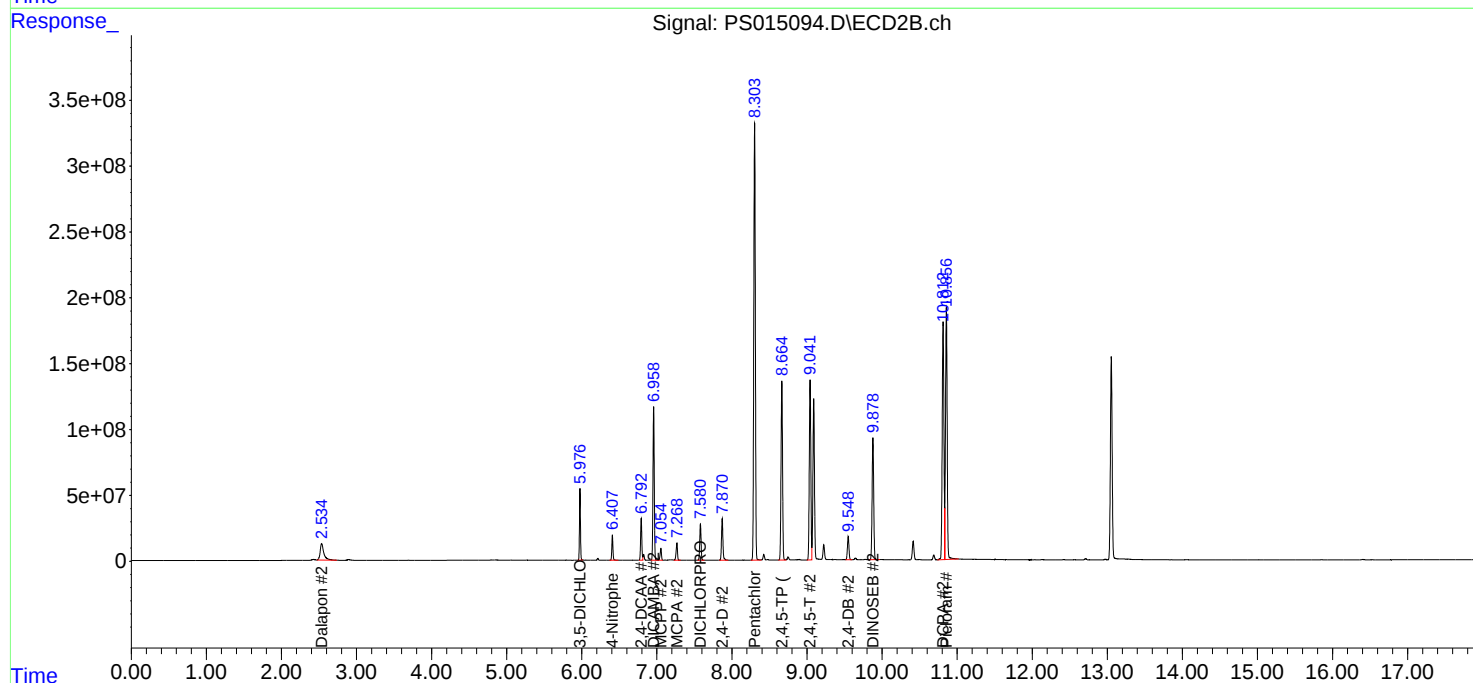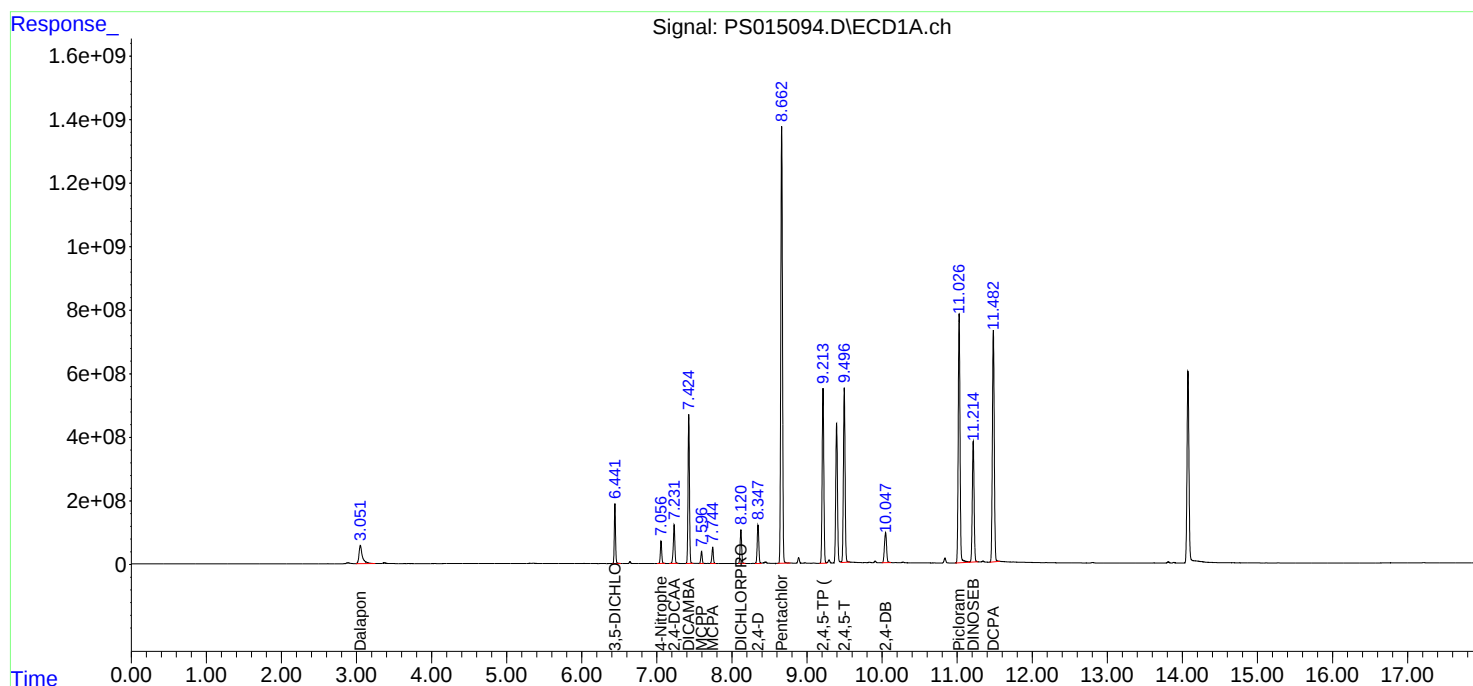


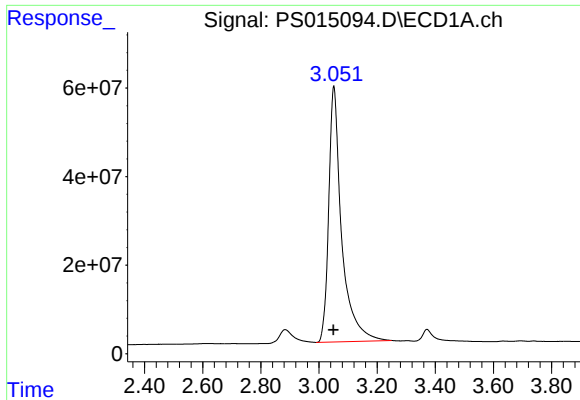

#1 Dalapon


R.T.: 3.051 min
Delta R.T.: 0.000 min
Response: 1781004313
Conc: 778.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

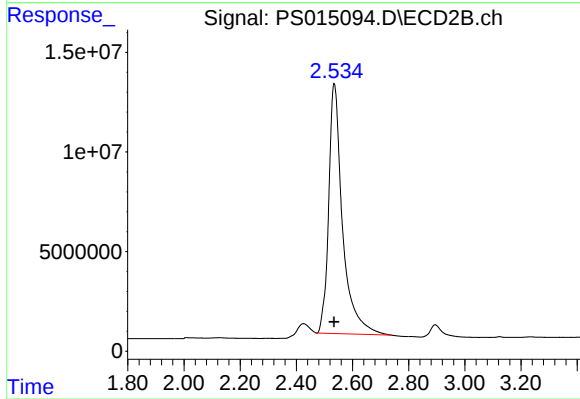


#1 Dalapon

R.T.: 2.534 min
Delta R.T.: 0.000 min
Response: 429236845
Conc: 697.50 ng/ml

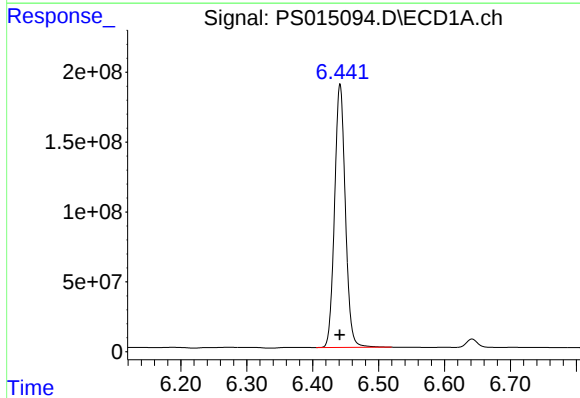


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.442 min
Delta R.T.: 0.000 min
Response: 2142855028
Conc: 765.37 ng/ml

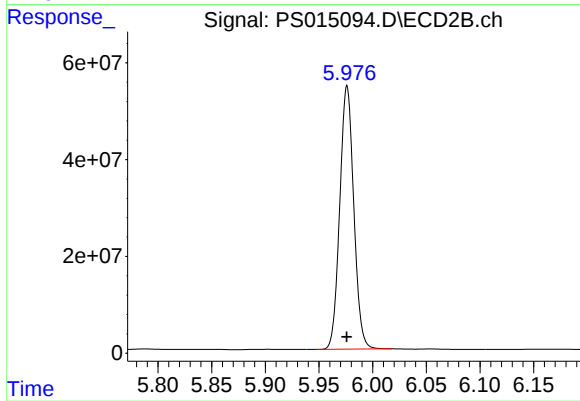

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.976 min
Delta R.T.: 0.000 min
Response: 493847535
Conc: 717.24 ng/ml

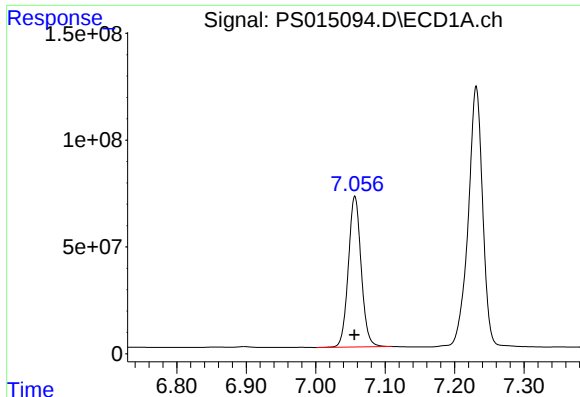

#3 4-Nitrophenol


R.T.: 7.056 min
Delta R.T.: 0.000 min
Response: 906516565
Conc: 757.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

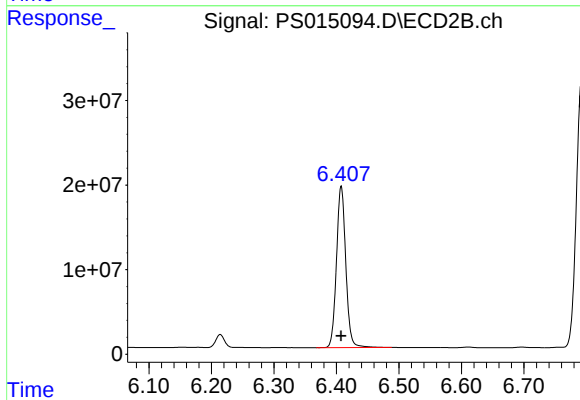


#3 4-Nitrophenol

R.T.: 6.408 min
Delta R.T.: 0.000 min
Response: 197197369
Conc: 697.15 ng/ml

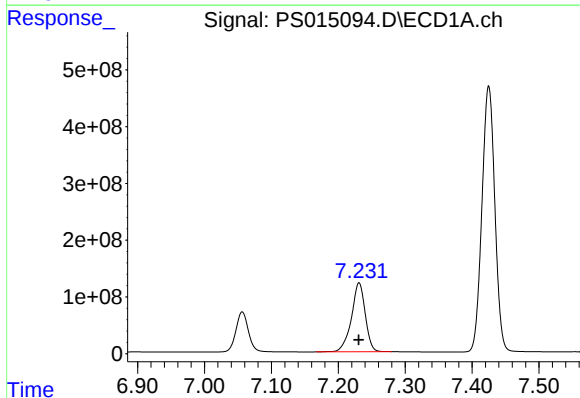


#4 2,4-DCAA

R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 1745093860
Conc: 825.72 ng/ml

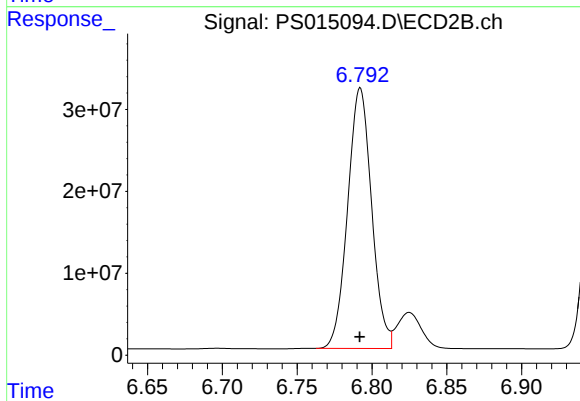

#4 2,4-DCAA


R.T.: 6.792 min
Delta R.T.: 0.000 min
Response: 354700849
Conc: 767.50 ng/ml

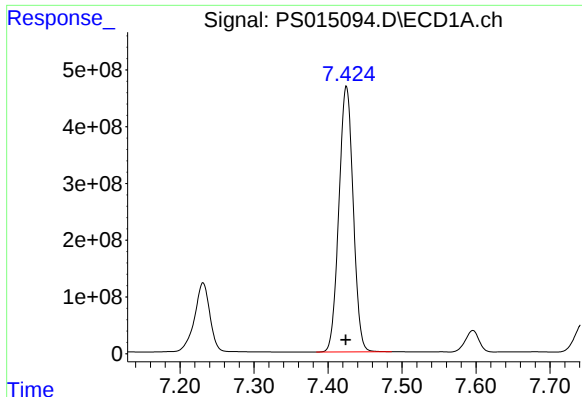

#5 DICAMBA


R.T.: 7.425 min
Delta R.T.: 0.000 min
Response: 6274433882
Conc: 791.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

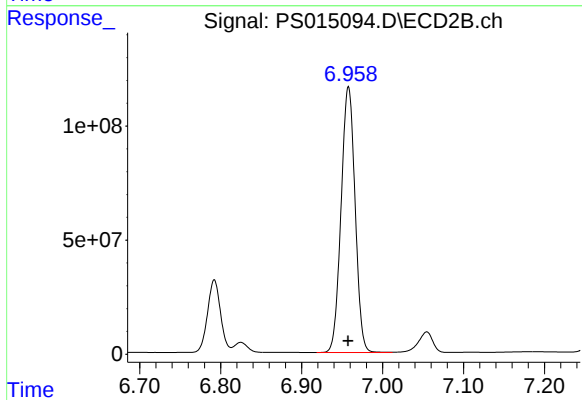


#5 DICAMBA

R.T.: 6.958 min
Delta R.T.: 0.000 min
Response: 1398568744
Conc: 732.37 ng/ml

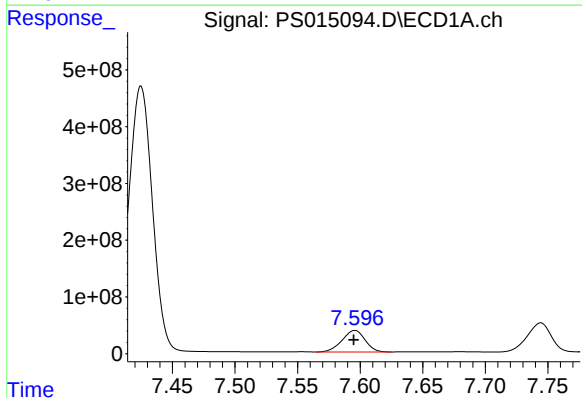


#6 MCP

R.T.: 7.596 min
Delta R.T.: 0.000 min
Response: 486351663
Conc: 79.54 ug/ml

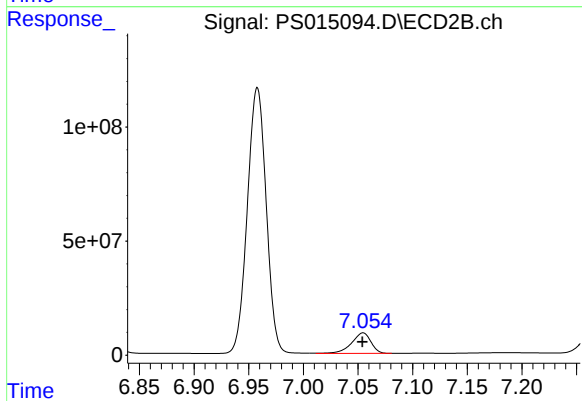

#6 MCP


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 111287296
Conc: 72.65 ug/ml

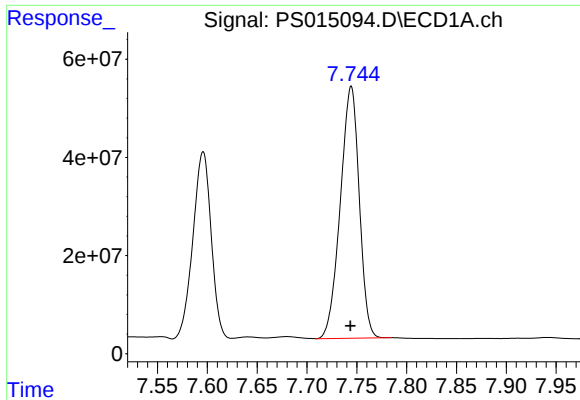

#7 MCPA


R.T.: 7.744 min
Delta R.T.: 0.000 min
Response: 678873808
Conc: 77.45 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

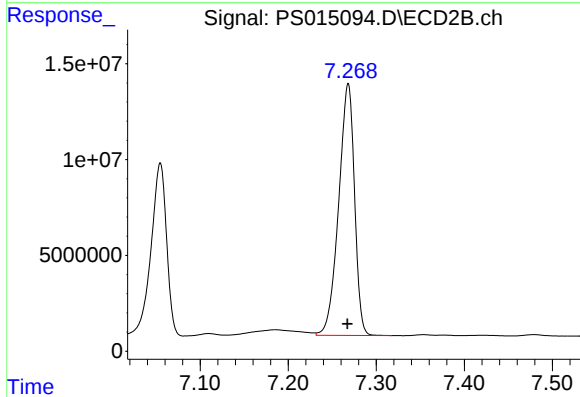


#7 MCPA

R.T.: 7.268 min
Delta R.T.: 0.001 min
Response: 164461822
Conc: 70.70 ug/ml

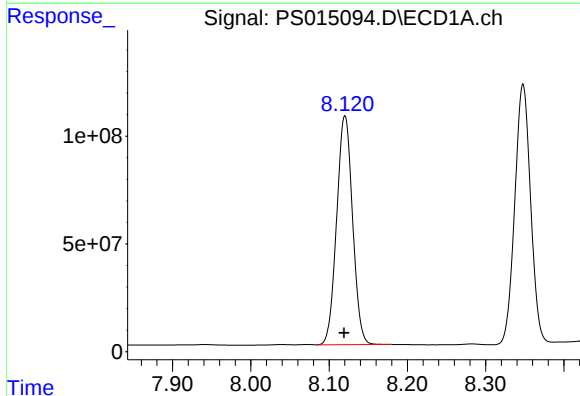


#8 DICHLORPROP

R.T.: 8.120 min
Delta R.T.: 0.001 min
Response: 1501195887
Conc: 760.81 ng/ml

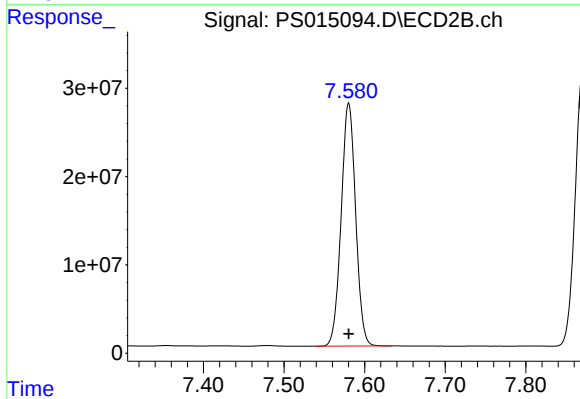

#8 DICHLORPROP


R.T.: 7.580 min
Delta R.T.: 0.000 min
Response: 343389646
Conc: 721.54 ng/ml

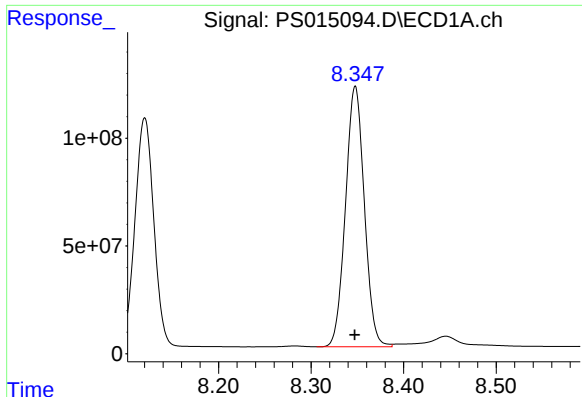

#9 2,4-D


R.T.: 8.348 min
Delta R.T.: 0.000 min
Response: 1710707950
Conc: 762.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

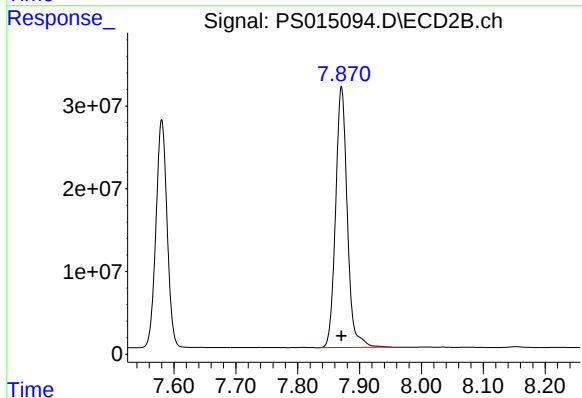


#9 2,4-D

R.T.: 7.871 min
Delta R.T.: 0.000 min
Response: 414235865
Conc: 725.46 ng/ml

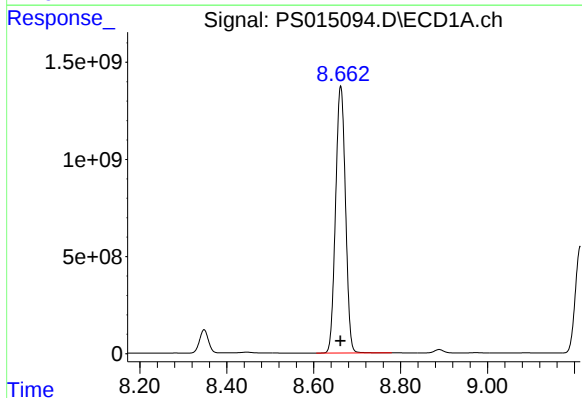


#10 Pentachlorophenol

R.T.: 8.662 min
Delta R.T.: 0.000 min
Response: 21673267854
Conc: 770.98 ng/ml

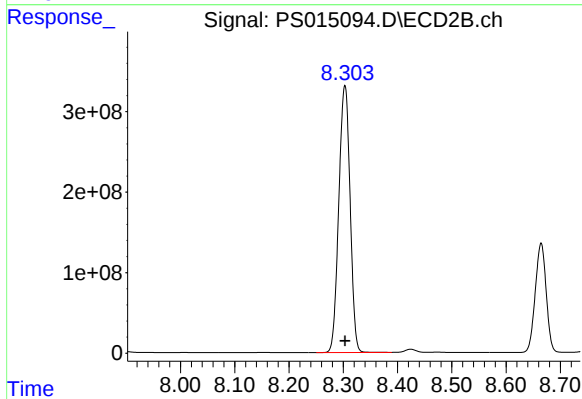

#10 Pentachlorophenol


R.T.: 8.303 min
Delta R.T.: 0.000 min
Response: 4798516980
Conc: 733.15 ng/ml

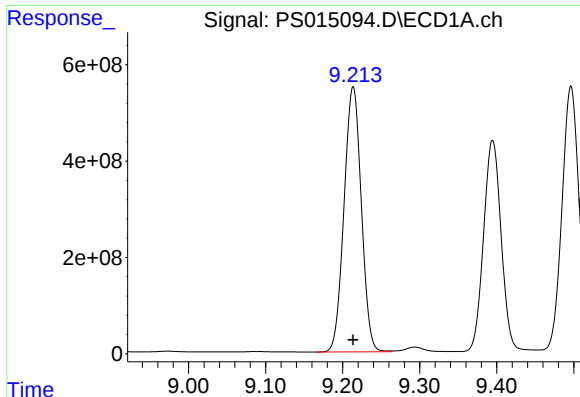

#11 2,4,5-TP (SILVEX)


R.T.: 9.214 min
Delta R.T.: 0.000 min
Response: 8533576606
Conc: 777.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

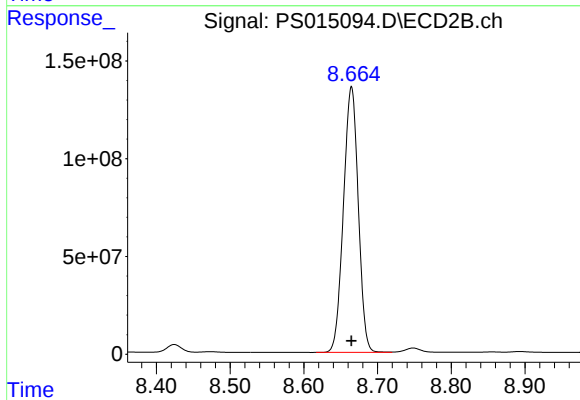


#11 2,4,5-TP (SILVEX)

R.T.: 8.665 min
Delta R.T.: 0.000 min
Response: 1898895094
Conc: 743.31 ng/ml

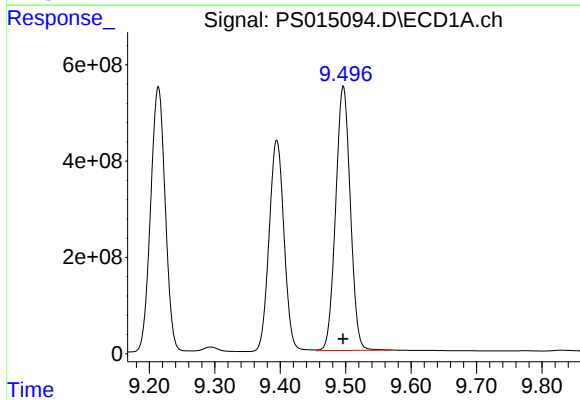


#12 2,4,5-T

R.T.: 9.496 min
Delta R.T.: 0.000 min
Response: 8562206849
Conc: 787.35 ng/ml

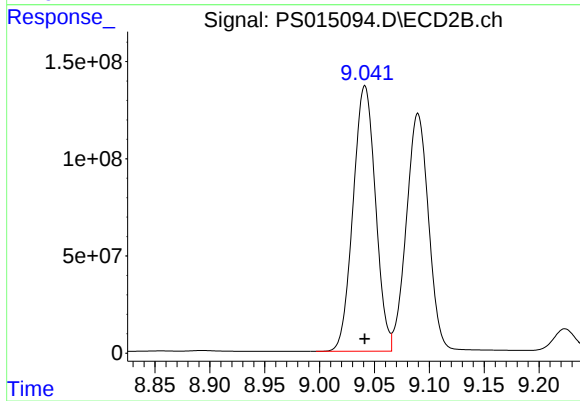

#12 2,4,5-T


R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 1938022290
Conc: 745.75 ng/ml

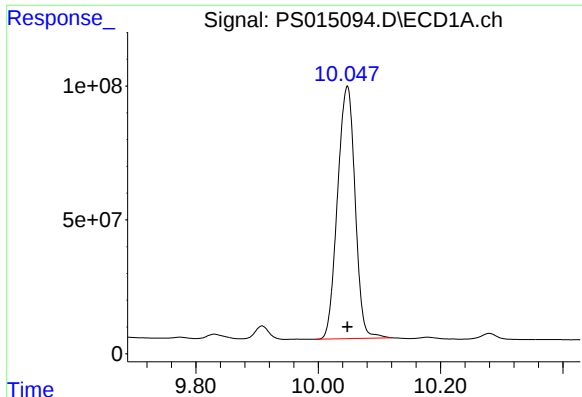

#13 2,4-DB


R.T.: 10.048 min
Delta R.T.: 0.000 min
Response: 1878024174
Conc: 807.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

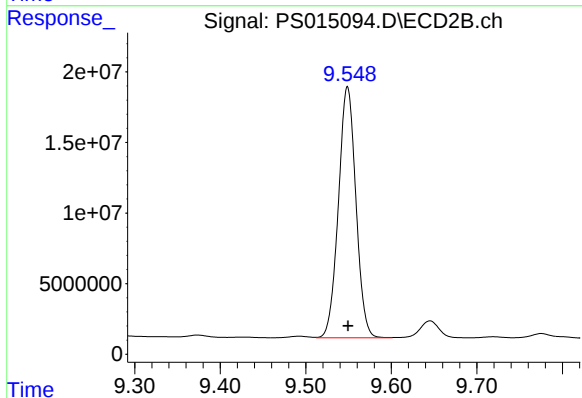


#13 2,4-DB

R.T.: 9.549 min
Delta R.T.: 0.000 min
Response: 252512982
Conc: 738.49 ng/ml

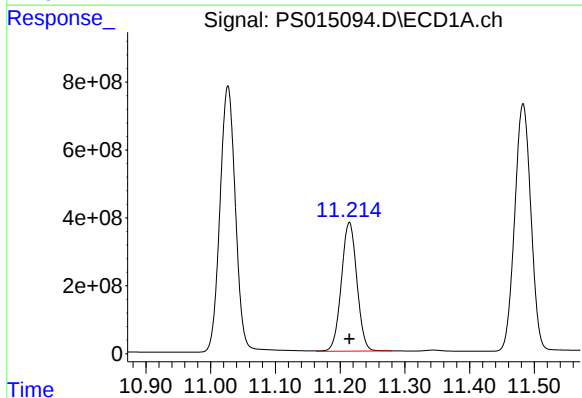


#14 DINOSEB

R.T.: 11.214 min
Delta R.T.: 0.000 min
Response: 6318862155
Conc: 771.66 ng/ml

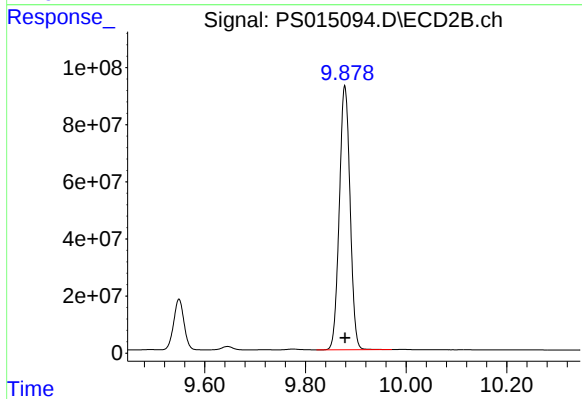

#14 DINOSEB


R.T.: 9.878 min
Delta R.T.: 0.000 min
Response: 1371860268
Conc: 737.48 ng/ml

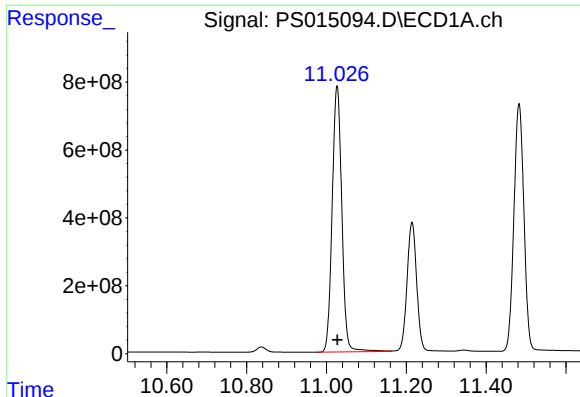

#15 Picloram


R.T.: 11.027 min
Delta R.T.: 0.000 min
Response: 13113726625
Conc: 799.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

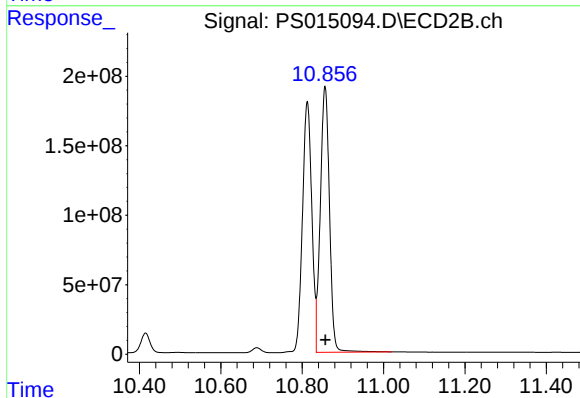


#15 Picloram

R.T.: 10.856 min
Delta R.T.: 0.000 min
Response: 2982778746
Conc: 758.62 ng/ml

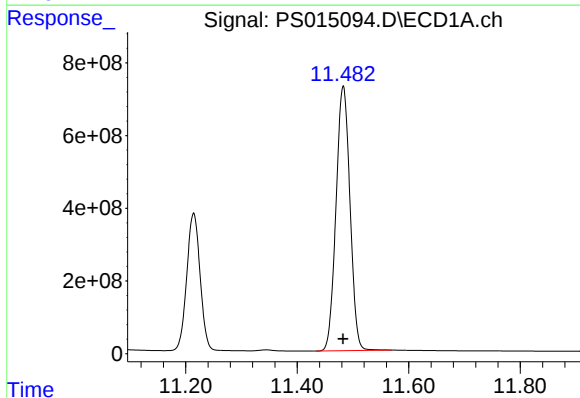

#16 DCPA

R.T.: 11.483 min
Delta R.T.: 0.000 min
Response: 12640857247
Conc: 780.76 ng/ml

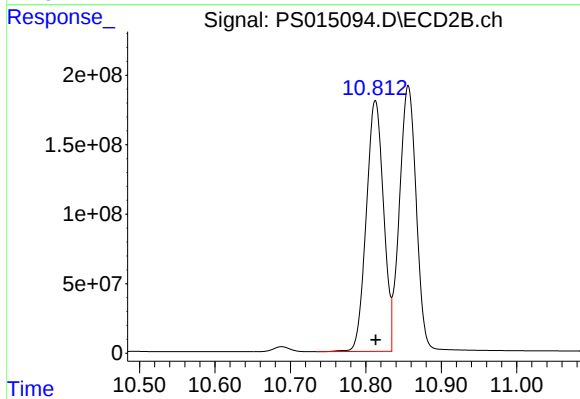

#16 DCPA

R.T.: 10.813 min
Delta R.T.: 0.000 min
Response: 2873722159
Conc: 752.87 ng/ml