

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052722\
 Data File : PS019540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2022 10:11
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 02:55:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.213	0.000	586782	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	3.044	0.000	290860	0	<MDL	N.D. #
5) T	DICAMBA	7.391	6.946	862262	458089	<MDL	<MDL #
6) T	MCPD	0.000	7.005	0	1398223	N.D.	<MDL
7) T	MCPA	7.655f	0.000	5950734	0	<MDL	N.D. #
8) T	DICHLORPROP	8.085	7.594	487820	2758753	<MDL	3.123 #
9) T	2,4-D	8.323	7.860	2806427	500010	<MDL	<MDL #
10) T	Pentachlo...	8.624	8.282	3932651	959518	<MDL	<MDL #
12) T	2,4,5-T	9.468	9.030	3124757	933388	<MDL	<MDL #
13) T	2,4-DB	9.962f	9.542	6064653	1098489	1.499	1.778
14) T	DINOSEB	11.162	9.852	8763594	494845	<MDL	<MDL #
15) T	Picloram	10.958	10.846	296.6E6	11334815	9.994	1.762 #
16) T	DCPA	11.432	10.782	8620481	7346864	<MDL	1.190 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052722\
Data File : PS019540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2022 10:11
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:55:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

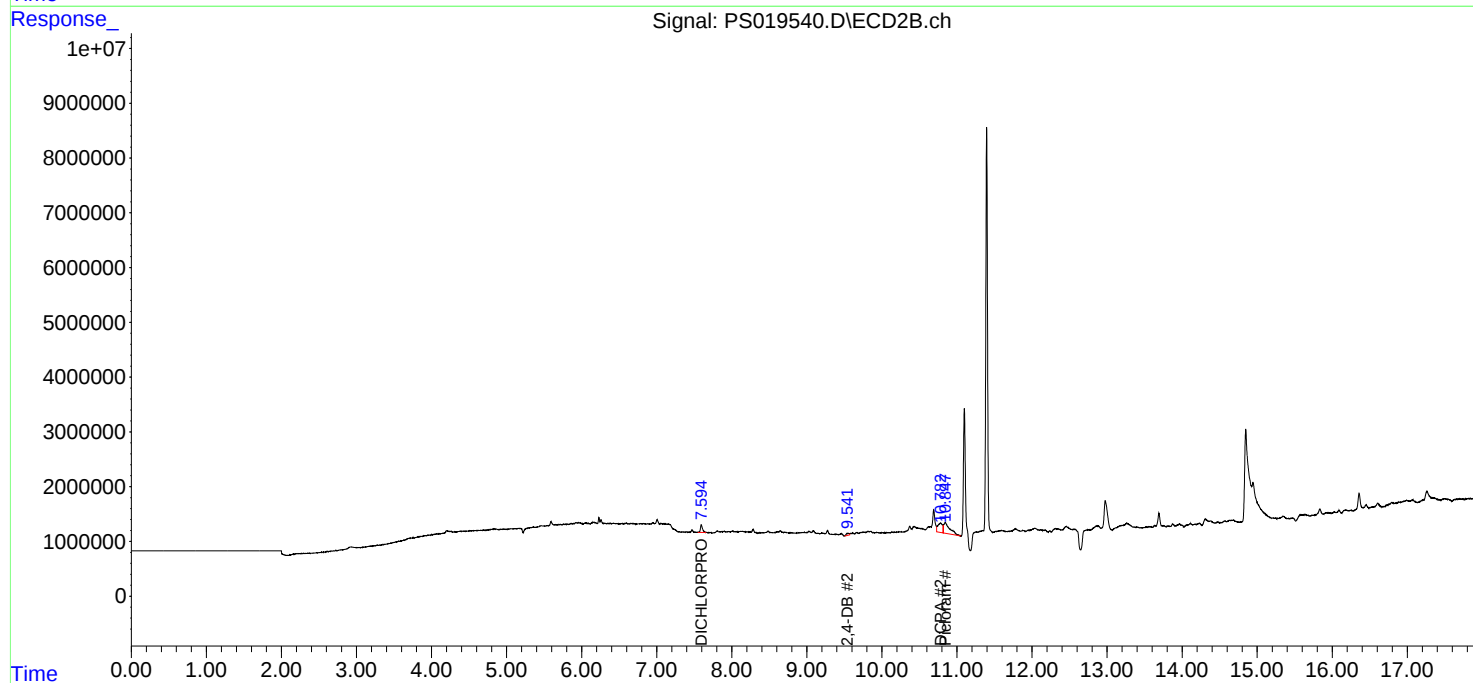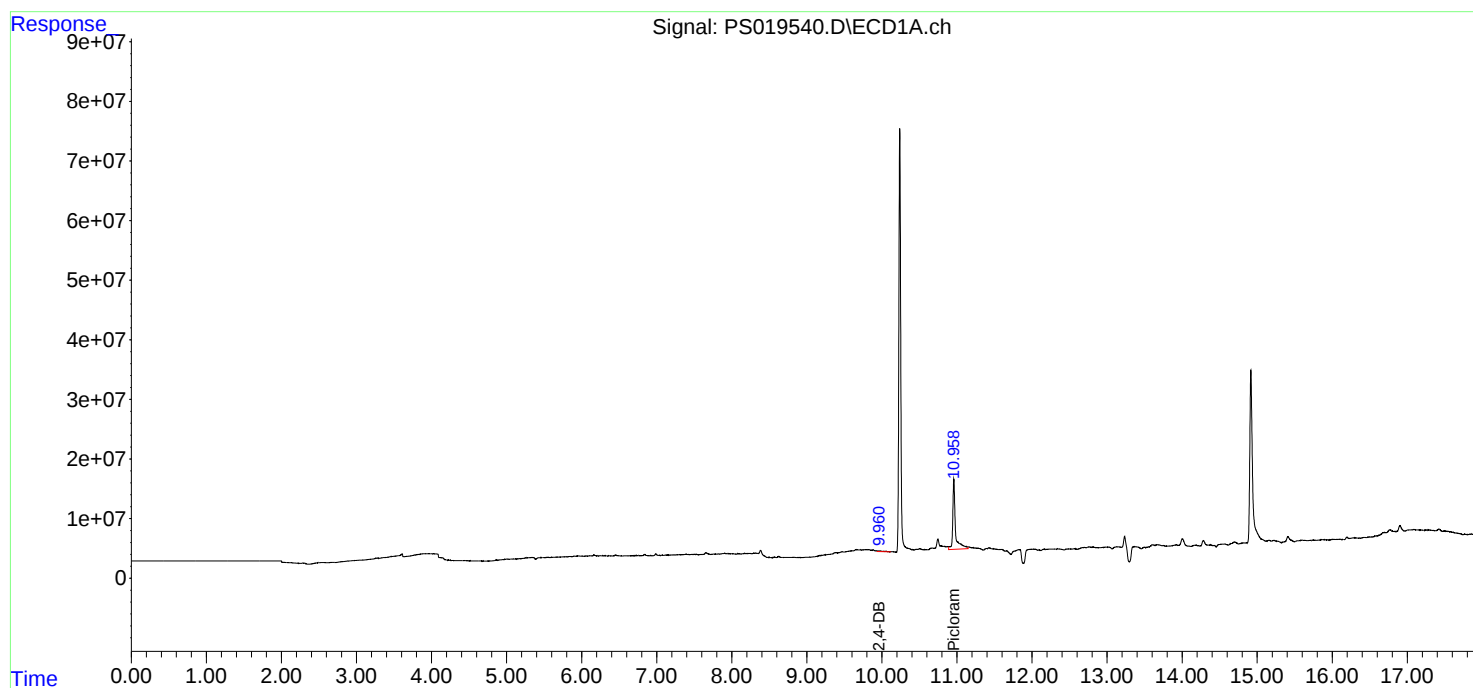


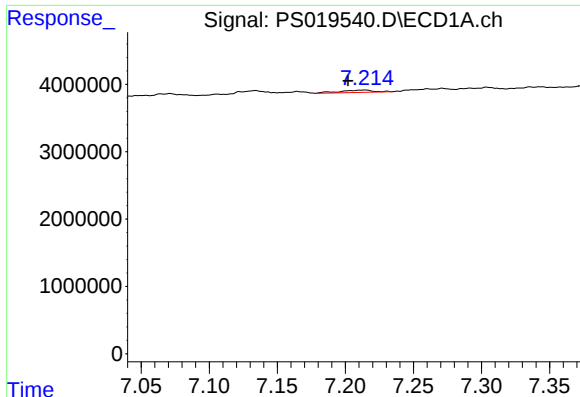

#4 2,4-DCAA


R.T.: 7.213 min
Delta R.T.: 0.011 min
Response: 586782
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

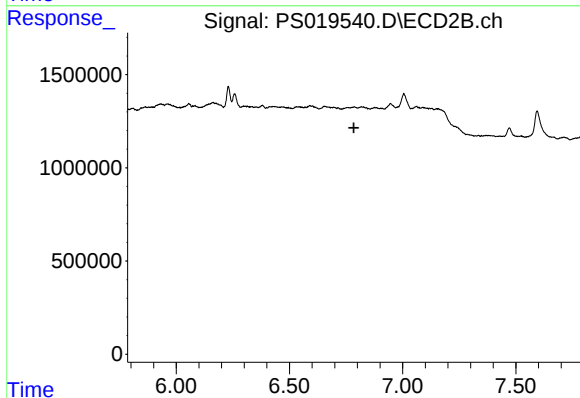


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

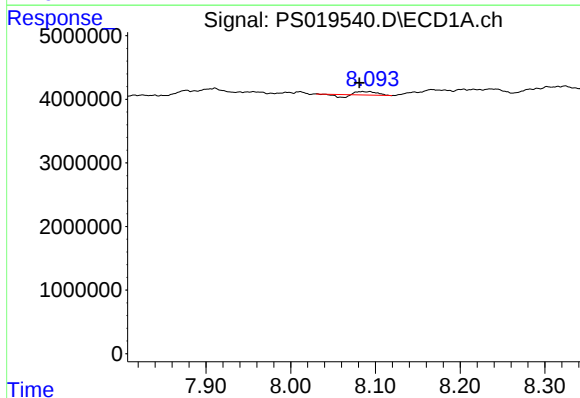


#8 DICHLORPROP

R.T.: 8.085 min
Delta R.T.: 0.004 min
Response: 487820
Conc: N.D.

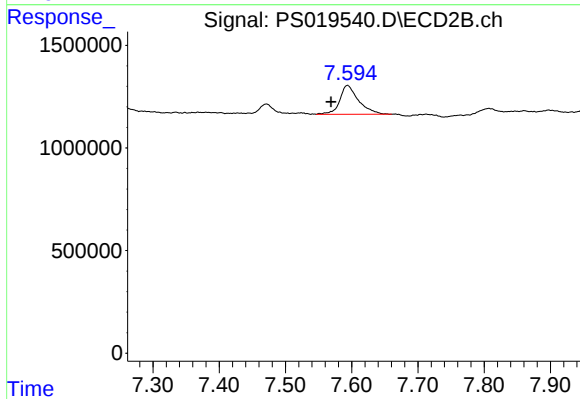

#8 DICHLORPROP


R.T.: 7.594 min
Delta R.T.: 0.025 min
Response: 2758753
Conc: 3.12 ng/ml

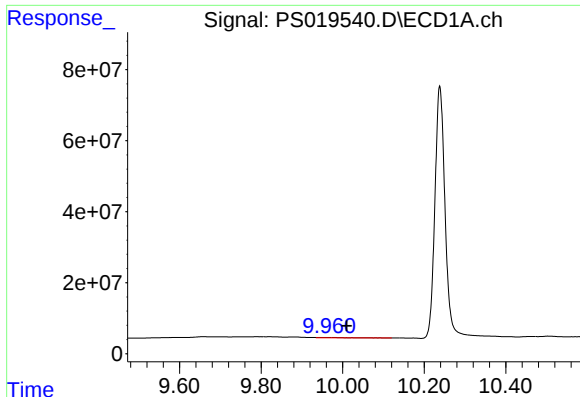

#13 2,4-DB


R.T.: 9.962 min
Delta R.T.: -0.049 min
Response: 6064653
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

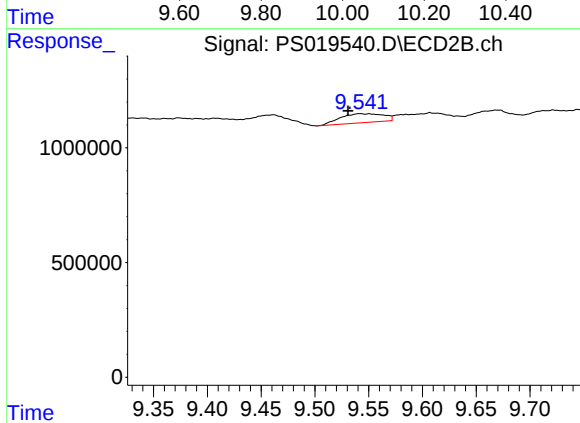


#13 2,4-DB

R.T.: 9.542 min
Delta R.T.: 0.011 min
Response: 1098489
Conc: 1.78 ng/ml

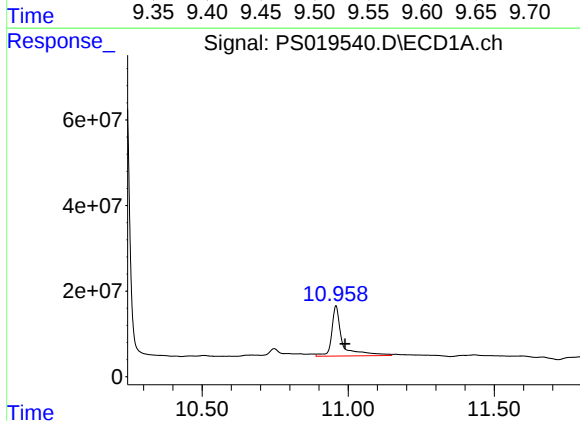


#15 Picloram

R.T.: 10.958 min
Delta R.T.: -0.032 min
Response: 296603199
Conc: 9.99 ng/ml

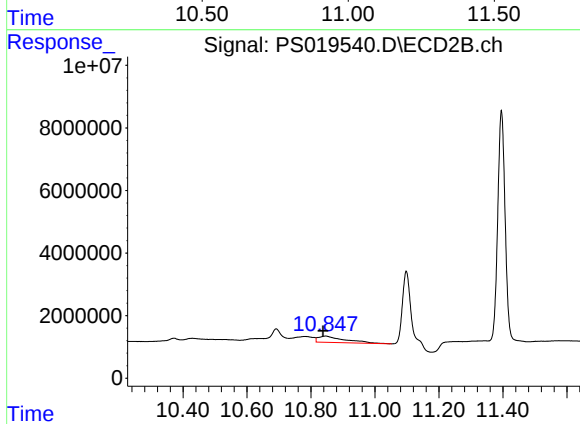

#15 Picloram


R.T.: 10.846 min
Delta R.T.: 0.009 min
Response: 11334815
Conc: 1.76 ng/ml

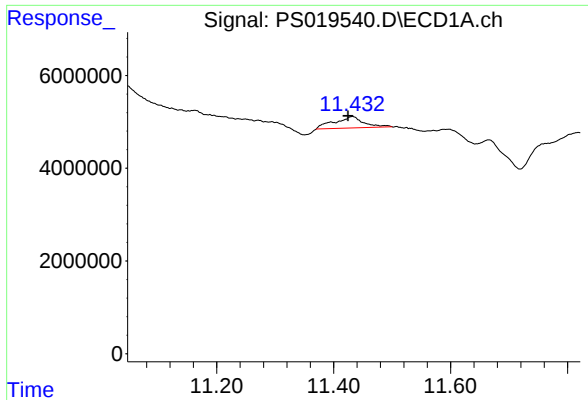

#16 DCPA

R.T.: 11.432 min
Delta R.T.: 0.008 min
Response: 8620481
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

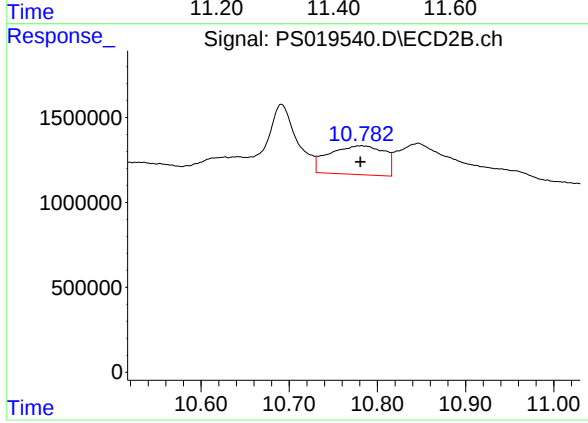

#16 DCPA

R.T.: 10.782 min
Delta R.T.: 0.001 min
Response: 7346864
Conc: 1.19 ng/ml