

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052722\
 Data File : PS0CCC-09.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2022 00:22
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 03:00:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.196	6.782	2086.3E6	669.2E6	869.593	863.597
Target Compounds							
1) T	Dalapon	3.019	2.532	3728.0E6	748.5E6	735.494	745.895
2) T	3,5-DICHL...	6.411	5.962	2543.6E6	967.4E6	804.765	807.037
3) T	4-Nitroph...	7.026	6.398	870.0E6	331.1E6	886.595	773.597
5) T	DICAMBA	7.387	6.947	7601.0E6	2748.1E6	800.299	803.891
6) T	MCPD	7.557	7.046	631.5E6	222.1E6	84.143	82.039
7) T	MCPA	7.707	7.258	885.1E6	305.8E6	81.922	79.583
8) T	DICHLORPROP	8.077	7.567	2034.7E6	739.8E6	794.600	837.468
9) T	2,4-D	8.306	7.857	2361.1E6	840.3E6	825.709	787.778
10) T	Pentachlo...	8.614	8.284	28878.2E6	9597.4E6	834.900	823.366
11) T	2,4,5-TP ...	9.164	8.644	12788.6E6	4099.9E6	814.513	815.540
12) T	2,4,5-T	9.448	9.020	14648.3E6	3837.0E6	778.349	815.835
13) T	2,4-DB	9.999	9.525	3321.2E6	524.1E6	820.859	848.077
14) T	DINOSEB	11.156	9.851	11660.8E6	2801.5E6	753.910	788.562
15) T	Picloram	10.977	10.831	20166.9E6	4293.8E6	679.540	667.548
16) T	DCPA	11.424	10.781	18132.5E6	5038.1E6	752.261	816.225



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052722\
Data File : PS0CCC-09.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2022 00:22
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 03:00:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

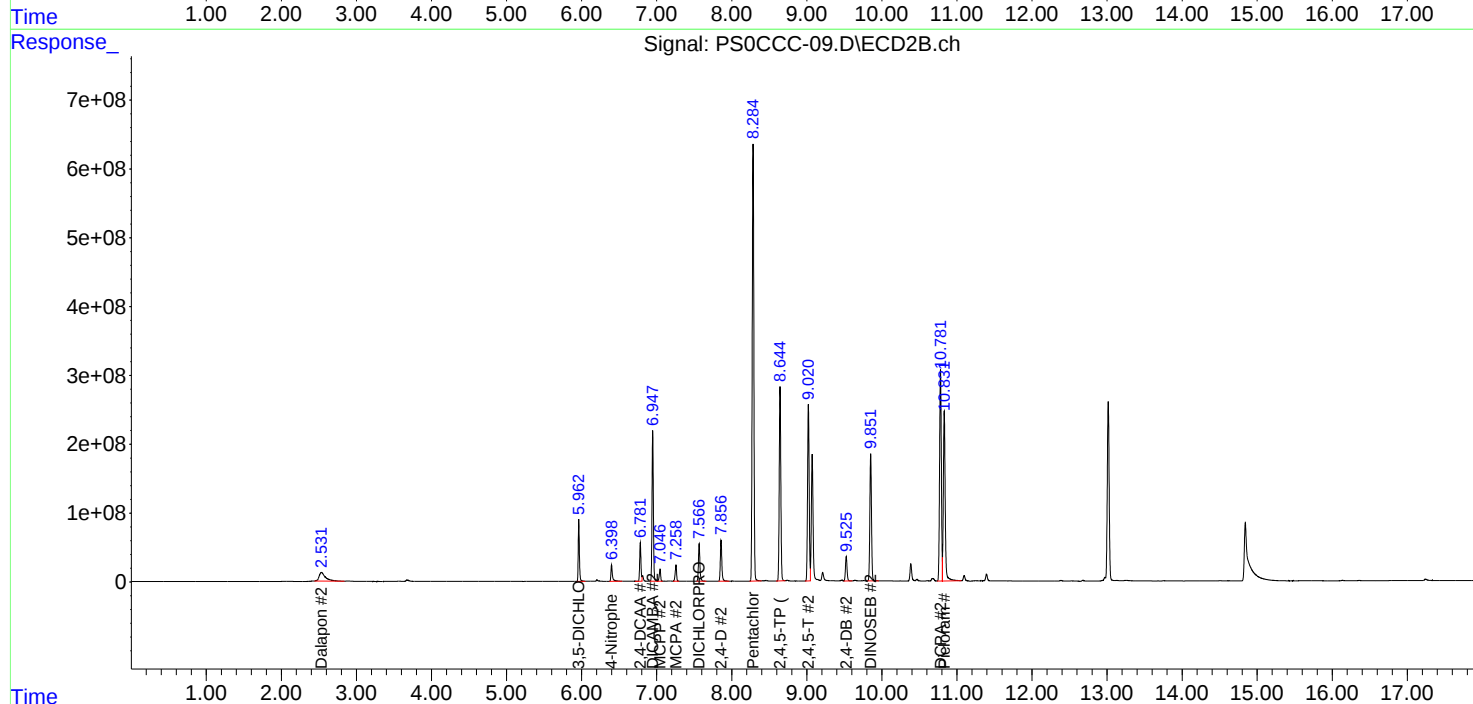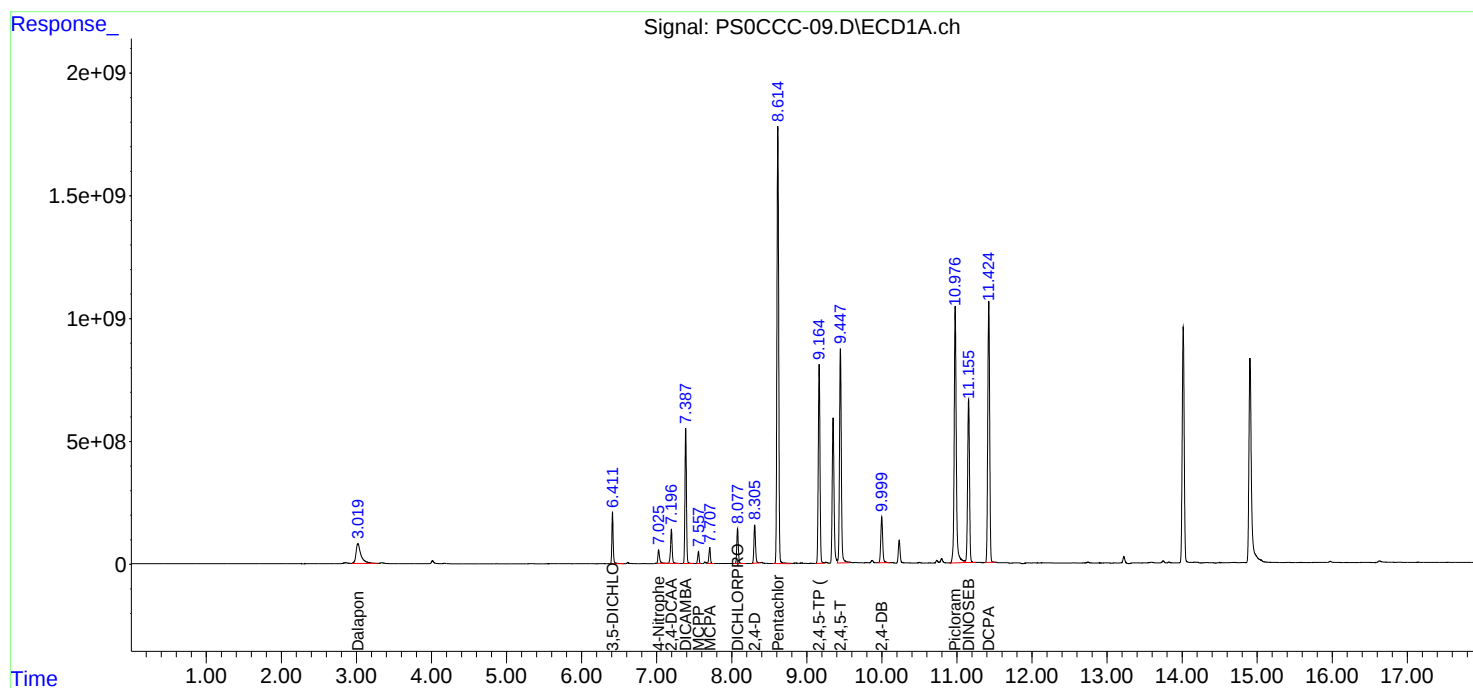


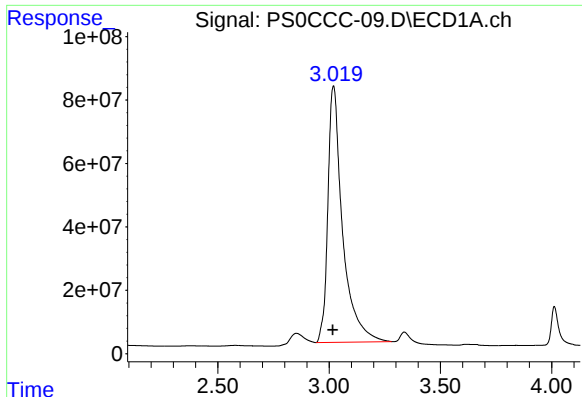

#1 Dalapon


R.T.: 3.019 min
Delta R.T.: 0.003 min
Response: 3728045299
Conc: 735.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

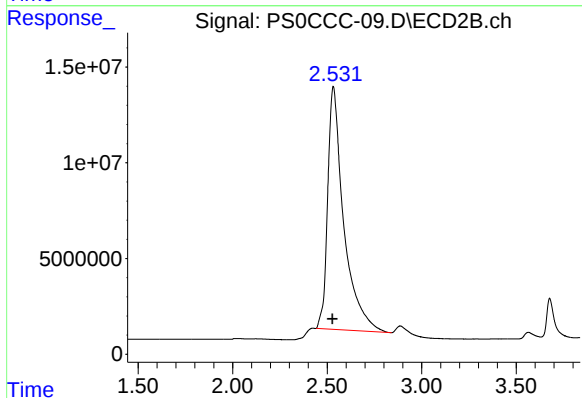


#1 Dalapon

R.T.: 2.532 min
Delta R.T.: 0.004 min
Response: 748462332
Conc: 745.90 ng/ml

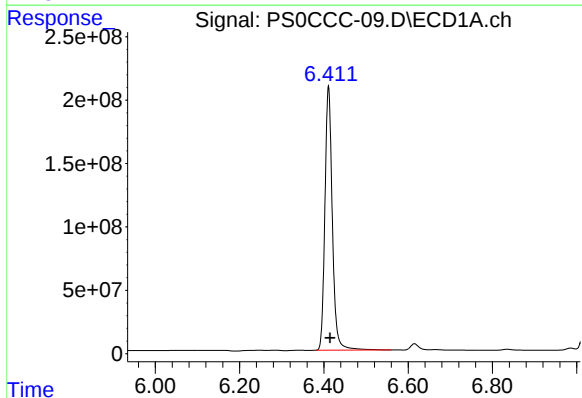


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.411 min
Delta R.T.: -0.004 min
Response: 2543569828
Conc: 804.77 ng/ml

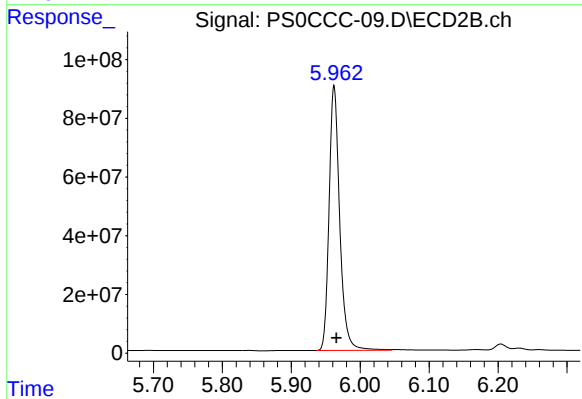

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.962 min
Delta R.T.: -0.003 min
Response: 967373522
Conc: 807.04 ng/ml

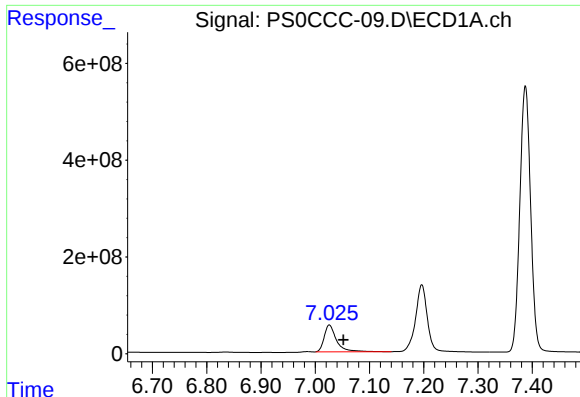

#3 4-Nitrophenol


R.T.: 7.026 min
Delta R.T.: -0.026 min
Response: 870031697
Conc: 886.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

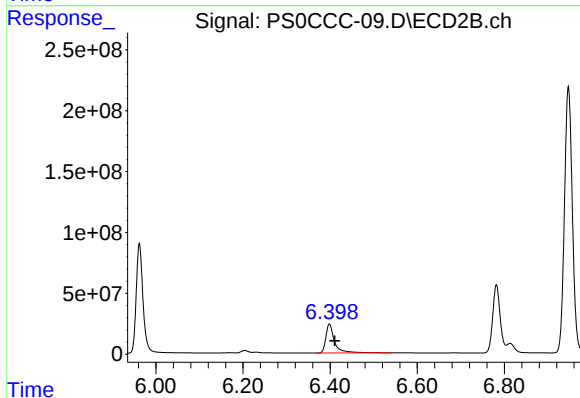


#3 4-Nitrophenol

R.T.: 6.398 min
Delta R.T.: -0.012 min
Response: 331127485
Conc: 773.60 ng/ml

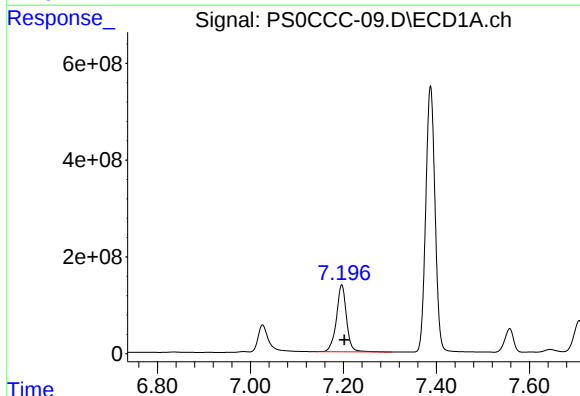


#4 2,4-DCAA

R.T.: 7.196 min
Delta R.T.: -0.006 min
Response: 2086298848
Conc: 869.59 ng/ml

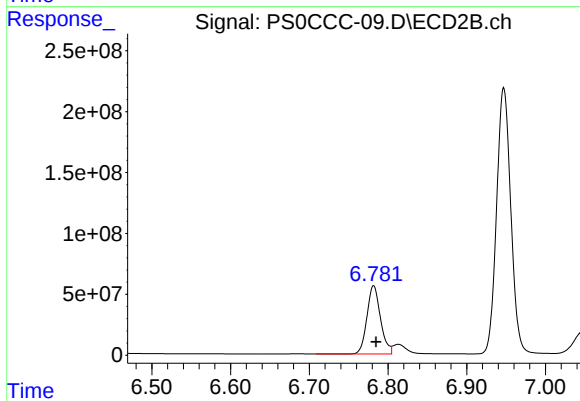

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.003 min
Response: 669175421
Conc: 863.60 ng/ml

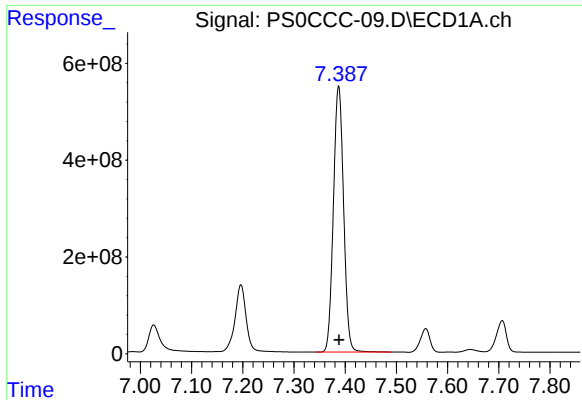

#5 DICAMBA


R.T.: 7.387 min
Delta R.T.: -0.001 min
Response: 7601042522
Conc: 800.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

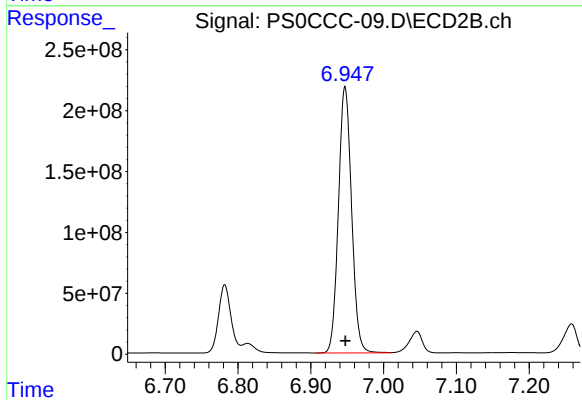


#5 DICAMBA

R.T.: 6.947 min
Delta R.T.: 0.000 min
Response: 2748055571
Conc: 803.89 ng/ml

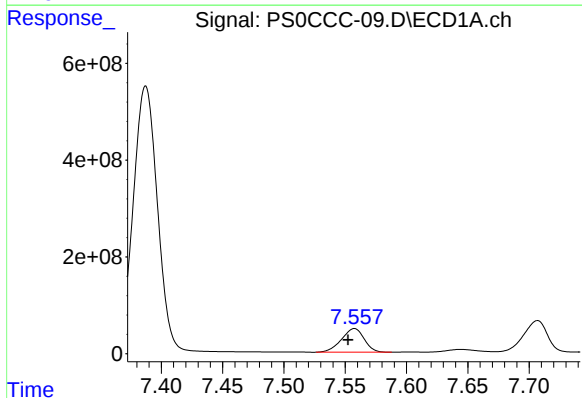


#6 MCP

R.T.: 7.557 min
Delta R.T.: 0.005 min
Response: 631539039
Conc: 84.14 ug/ml

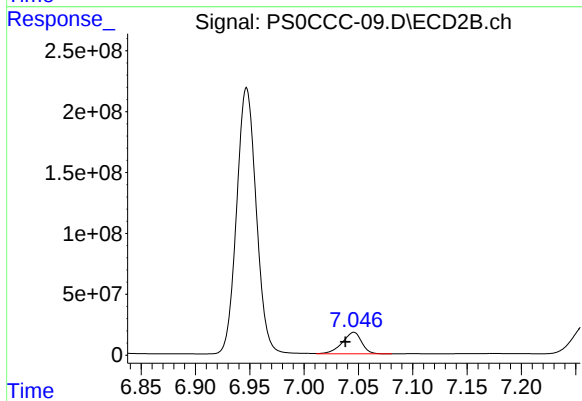

#6 MCP


R.T.: 7.046 min
Delta R.T.: 0.008 min
Response: 222081693
Conc: 82.04 ug/ml

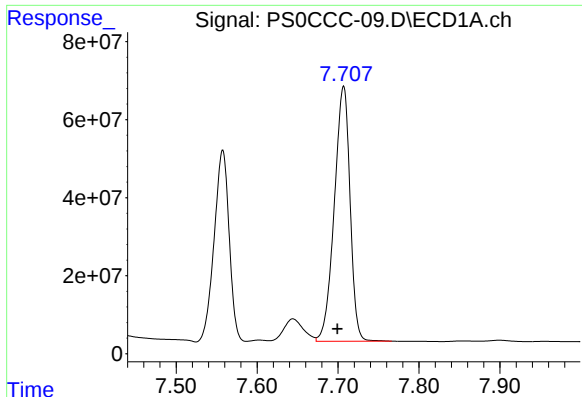

#7 MCPA


R.T.: 7.707 min
Delta R.T.: 0.007 min
Response: 885083876
Conc: 81.92 ug/ml

Instrument :
ECD_S
ClientSampleId :

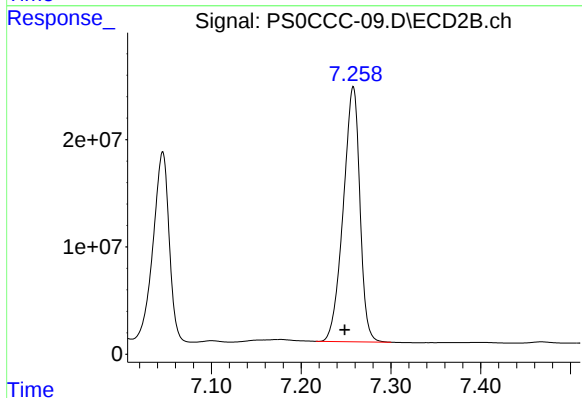


#7 MCPA

R.T.: 7.258 min
Delta R.T.: 0.010 min
Response: 305800177
Conc: 79.58 ug/ml

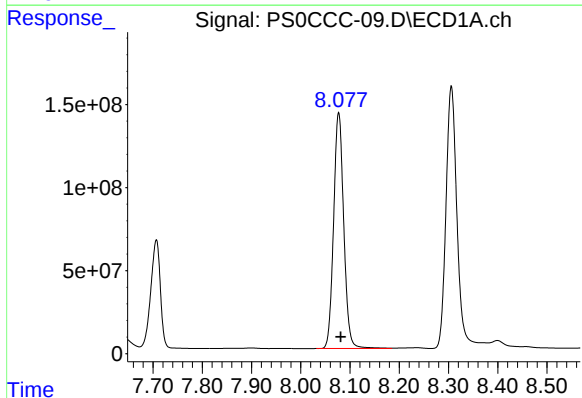


#8 DICHLORPROP

R.T.: 8.077 min
Delta R.T.: -0.004 min
Response: 2034660865
Conc: 794.60 ng/ml

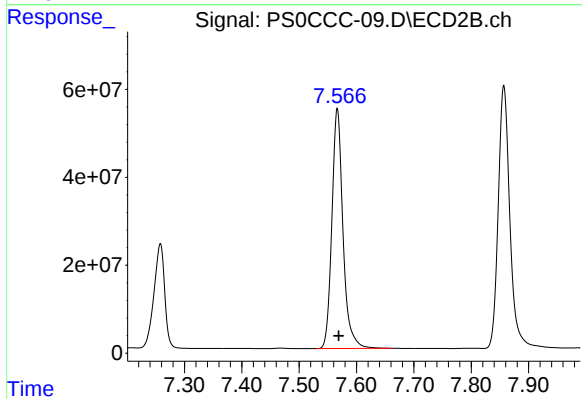

#8 DICHLORPROP


R.T.: 7.567 min
Delta R.T.: -0.003 min
Response: 739795607
Conc: 837.47 ng/ml

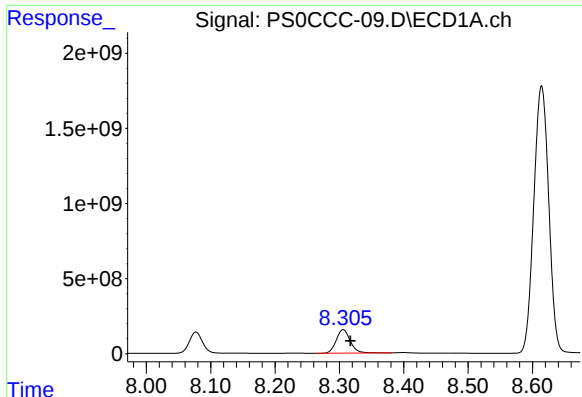

#9 2,4-D


R.T.: 8.306 min
Delta R.T.: -0.011 min
Response: 2361105619
Conc: 825.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

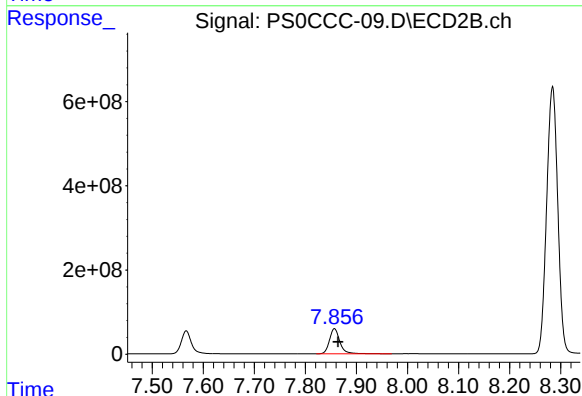


#9 2,4-D

R.T.: 7.857 min
Delta R.T.: -0.007 min
Response: 840265496
Conc: 787.78 ng/ml

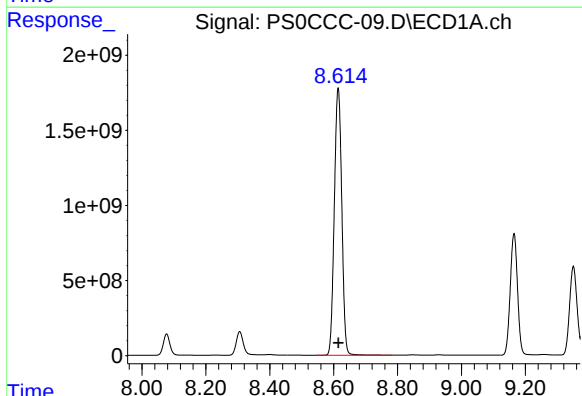


#10 Pentachlorophenol

R.T.: 8.614 min
Delta R.T.: 0.000 min
Response: 28878237741
Conc: 834.90 ng/ml

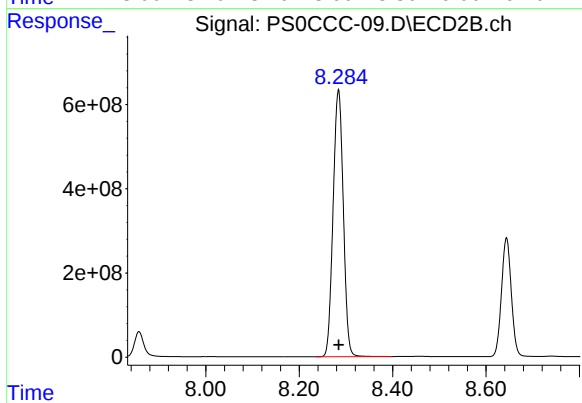

#10 Pentachlorophenol


R.T.: 8.284 min
Delta R.T.: 0.000 min
Response: 9597354890
Conc: 823.37 ng/ml

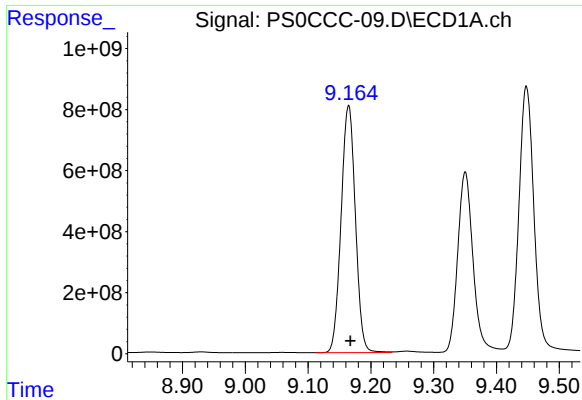

#11 2,4,5-TP (SILVEX)


R.T.: 9.164 min
Delta R.T.: -0.003 min
Response: 12788622603
Conc: 814.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

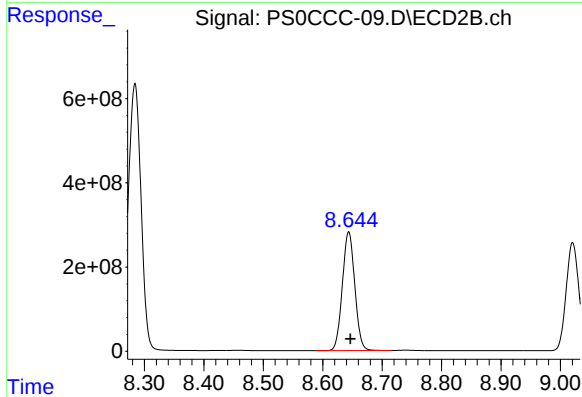


#11 2,4,5-TP (SILVEX)

R.T.: 8.644 min
Delta R.T.: -0.003 min
Response: 4099853652
Conc: 815.54 ng/ml

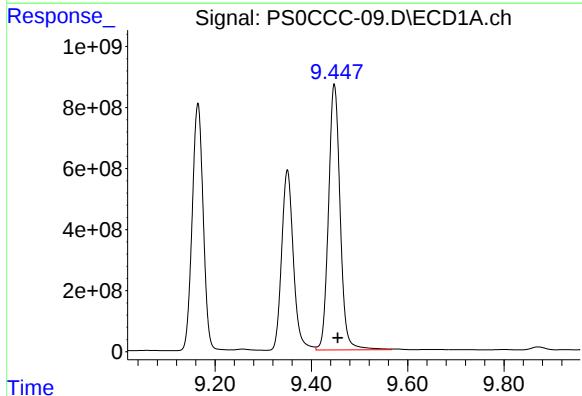


#12 2,4,5-T

R.T.: 9.448 min
Delta R.T.: -0.007 min
Response: 14648262123
Conc: 778.35 ng/ml

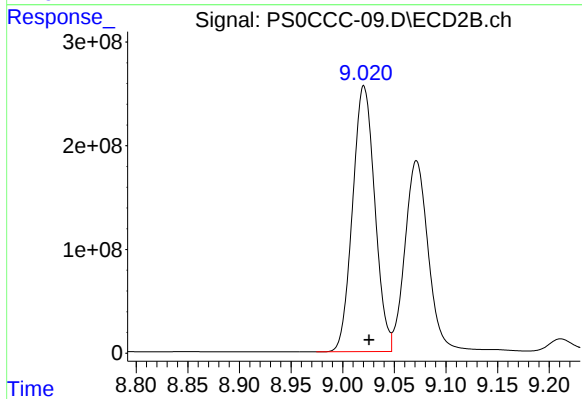

#12 2,4,5-T


R.T.: 9.020 min
Delta R.T.: -0.005 min
Response: 3837039907
Conc: 815.83 ng/ml

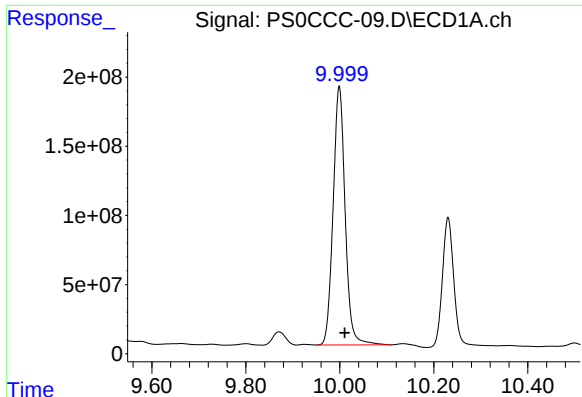

#13 2,4-DB


R.T.: 9.999 min
Delta R.T.: -0.012 min
Response: 3321210271
Conc: 820.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

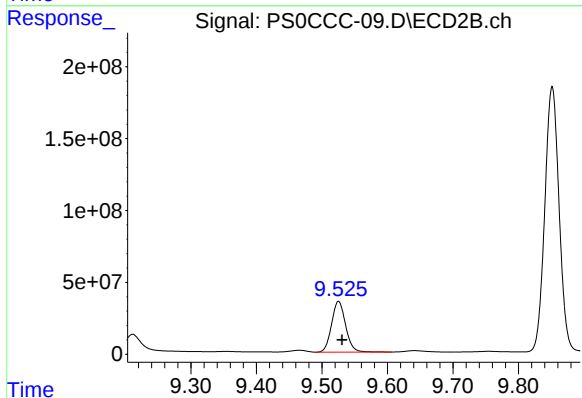


#13 2,4-DB

R.T.: 9.525 min
Delta R.T.: -0.005 min
Response: 524081854
Conc: 848.08 ng/ml

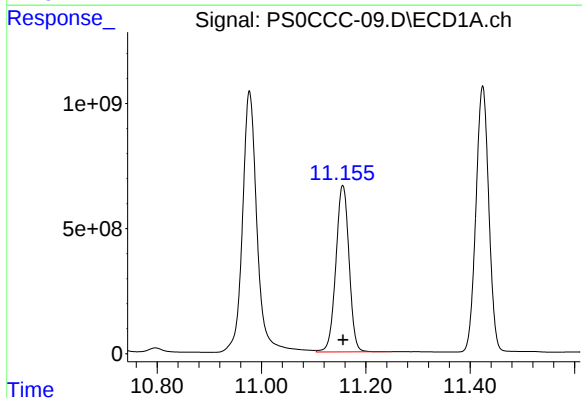


#14 DINOSEB

R.T.: 11.156 min
Delta R.T.: 0.000 min
Response: 11660844697
Conc: 753.91 ng/ml

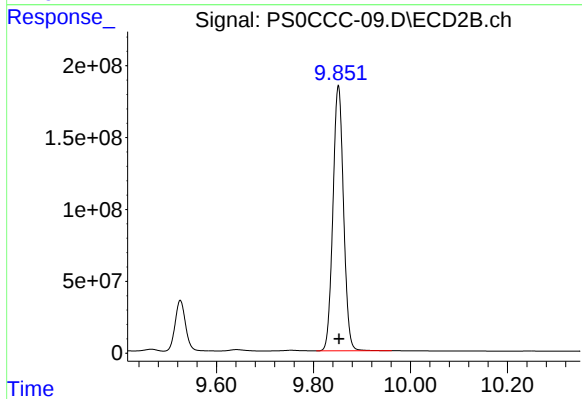

#14 DINOSEB


R.T.: 9.851 min
Delta R.T.: -0.001 min
Response: 2801461239
Conc: 788.56 ng/ml

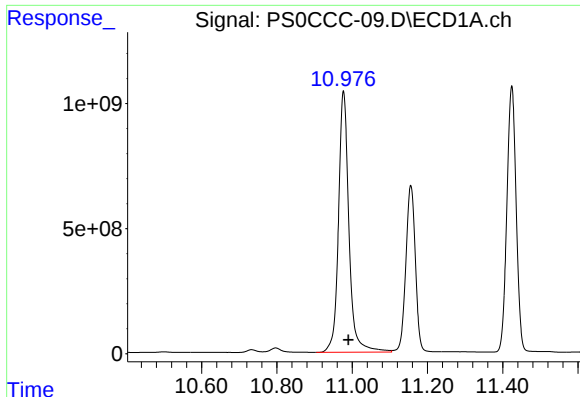

#15 Picloram


R.T.: 10.977 min
Delta R.T.: -0.013 min
Response: 20166887775
Conc: 679.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

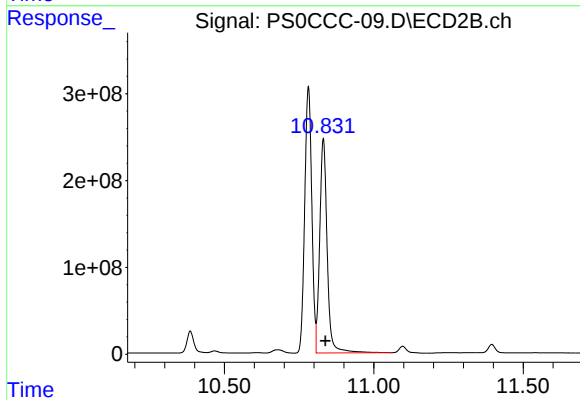


#15 Picloram

R.T.: 10.831 min
Delta R.T.: -0.006 min
Response: 4293839242
Conc: 667.55 ng/ml

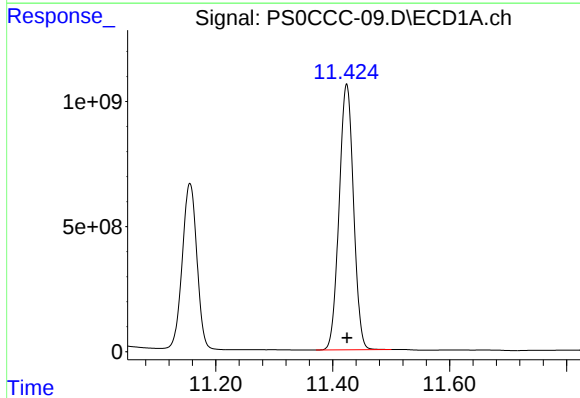

#16 DCPA

R.T.: 11.424 min
Delta R.T.: 0.000 min
Response: 18132503335
Conc: 752.26 ng/ml

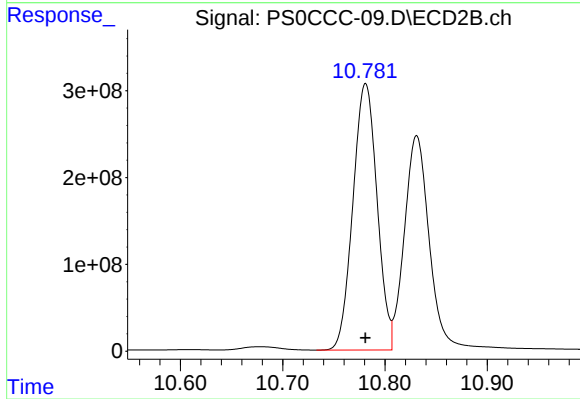

#16 DCPA

R.T.: 10.781 min
Delta R.T.: 0.000 min
Response: 5038138045
Conc: 816.23 ng/ml