

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052725\
 Data File : PS030411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 May 2025 09:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 09:16:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051225.M
 Quant Title : 8080.M
 QLast Update : Mon May 12 14:29:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.924	7.439	1321.0E6	349.5E6	463.875	436.701
Target Compounds							
1) T	Dalapon	2.489f	2.560f	181.3E6	10363271	36.893	5.102 #
2) T	3,5-DICHL...	6.140	0.000	2251643	0	<MDL	N.D. #
3) T	4-Nitroph...	6.726	0.000	7455223	0	3.609	N.D. #
5) T	DICAMBA	7.149f	7.609f	-335959	3261566	N.D.	<MDL
6) T	MCPD	7.332f	0.000	5468969	0	<MDL	N.D. #
7) T	MCPA	7.432	0.000	189131	0	<MDL	N.D. #
8) T	DICHLORPROP	7.784	0.000	3120512	0	1.068	N.D. #
10) T	Pentachlo...	8.272	0.000	9894964	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.840	0.000	2008722	0	<MDL	N.D. #
13) T	2,4-DB	9.650f	0.000	2055725	0	<MDL	N.D. #
14) T	DINOSEB	10.877f	0.000	440063	0	<MDL	N.D. #
15) T	Picloram	10.653	11.882	100.7E6	16219680	4.708	1.153 #
16) T	DCPA	11.123f	11.882	4645104	16219680	<MDL	1.201 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052725\
Data File : PS030411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 May 2025 09:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 09:16:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051225.M
Quant Title : 8080.M
QLast Update : Mon May 12 14:29:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

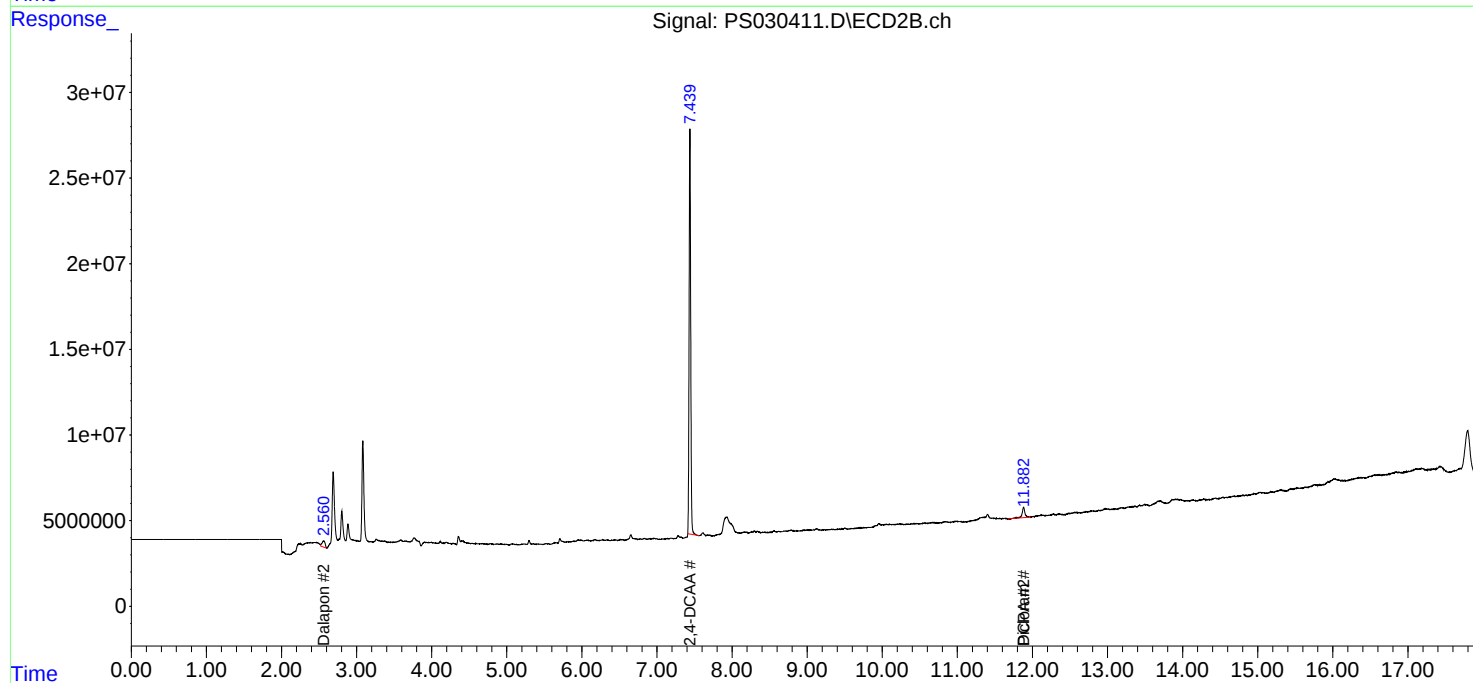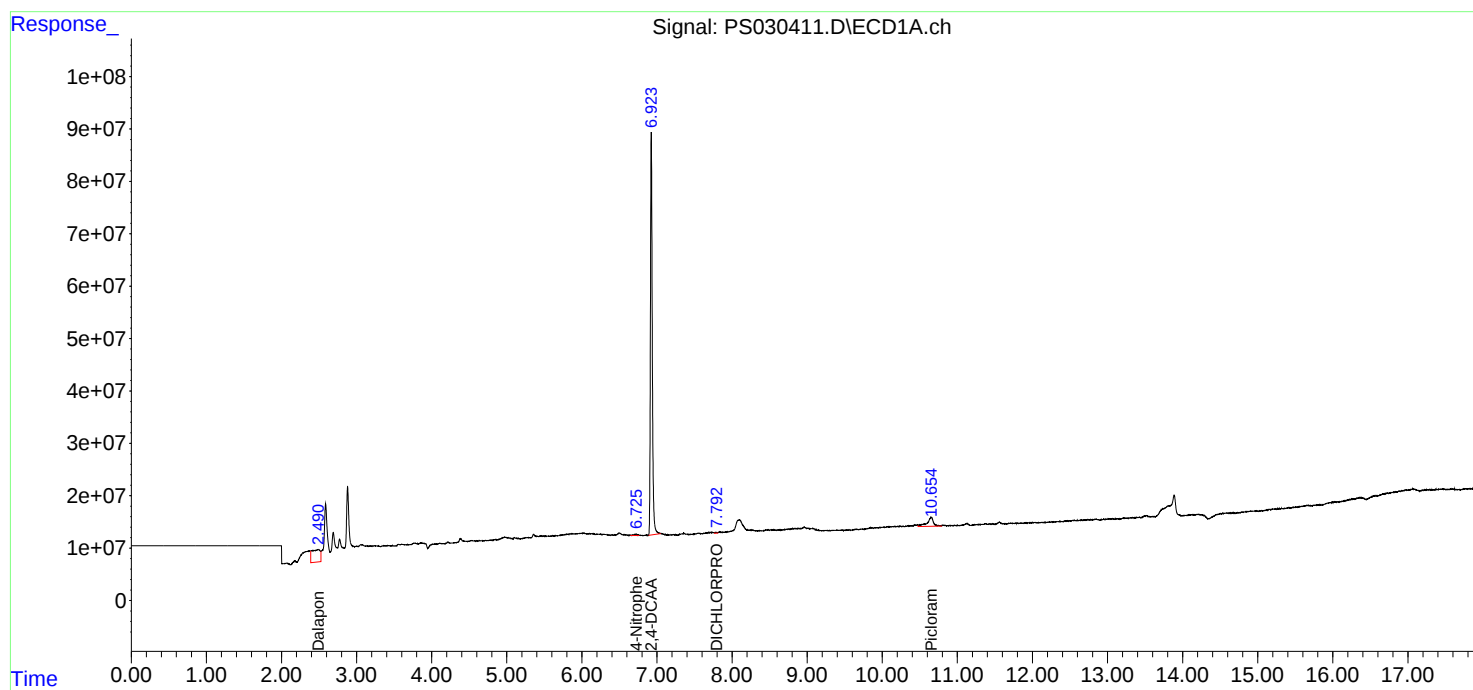


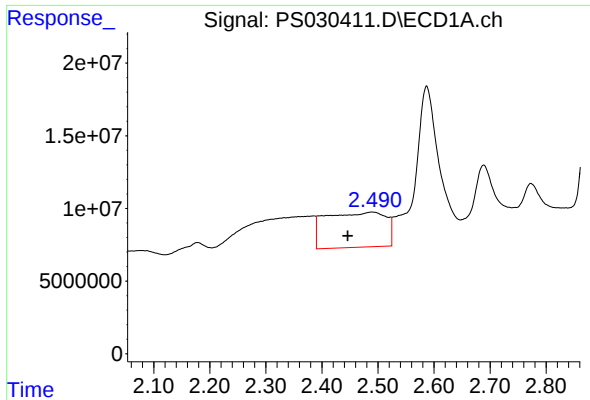

#1 Dalapon


R.T.: 2.489 min
Delta R.T.: 0.043 min
Response: 181340438
Conc: 36.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

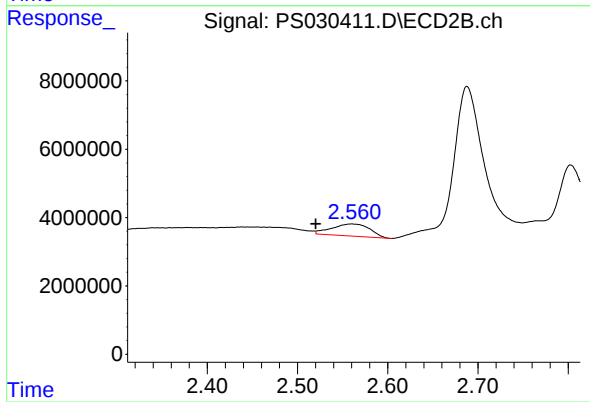


#1 Dalapon

R.T.: 2.560 min
Delta R.T.: 0.040 min
Response: 10363271
Conc: 5.10 ng/ml

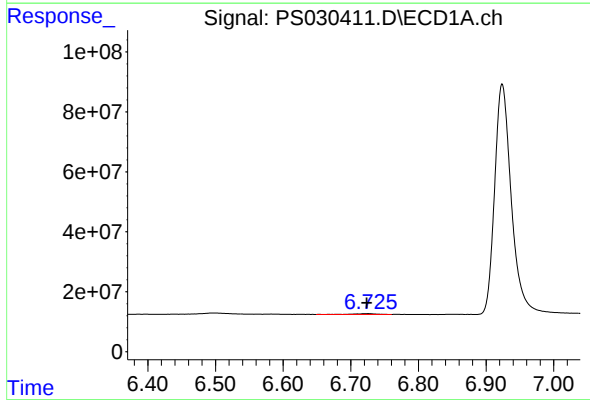


#3 4-Nitrophenol

R.T.: 6.726 min
Delta R.T.: 0.002 min
Response: 7455223
Conc: 3.61 ng/ml

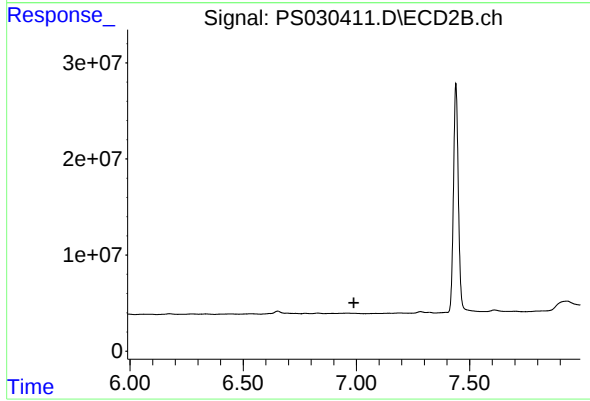

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.988 min
Response: 0
Conc: N.D.

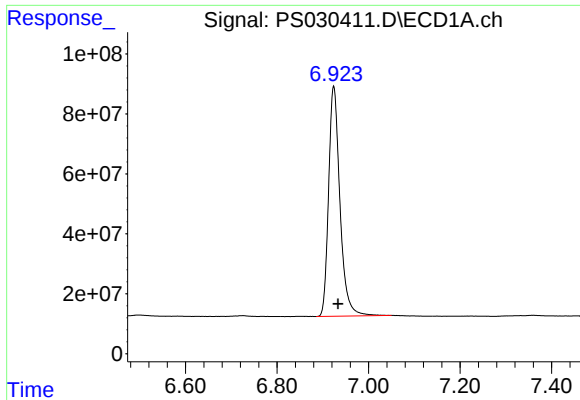

#4 2,4-DCAA


R.T.: 6.924 min
Delta R.T.: -0.010 min
Response: 1321026054
Conc: 463.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

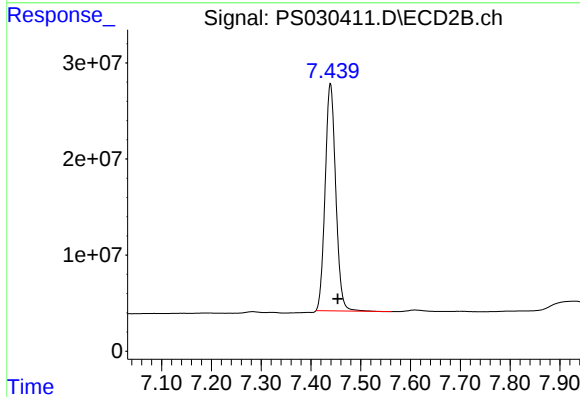


#4 2,4-DCAA

R.T.: 7.439 min
Delta R.T.: -0.015 min
Response: 349450041
Conc: 436.70 ng/ml

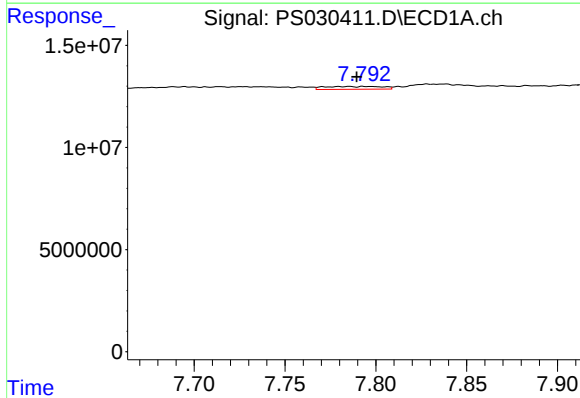


#8 DICHLORPROP

R.T.: 7.784 min
Delta R.T.: -0.006 min
Response: 3120512
Conc: 1.07 ng/ml

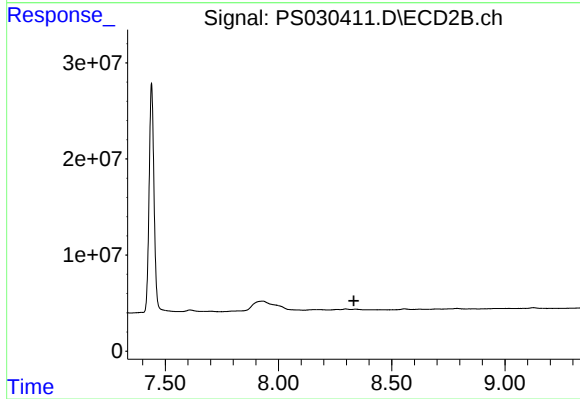

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 8.333 min
Response: 0
Conc: N.D.

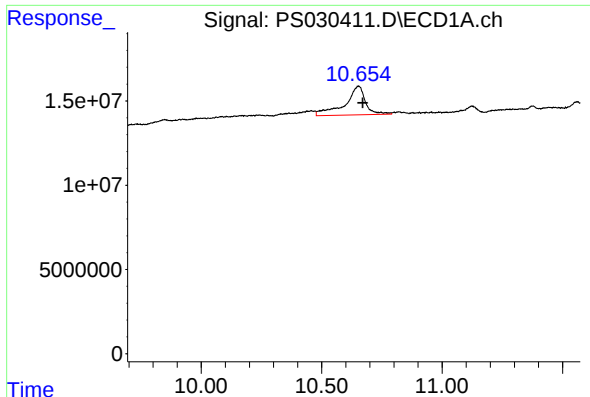

#15 Picloram


R.T.: 10.653 min
Delta R.T.: -0.017 min
Response: 100690507
Conc: 4.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

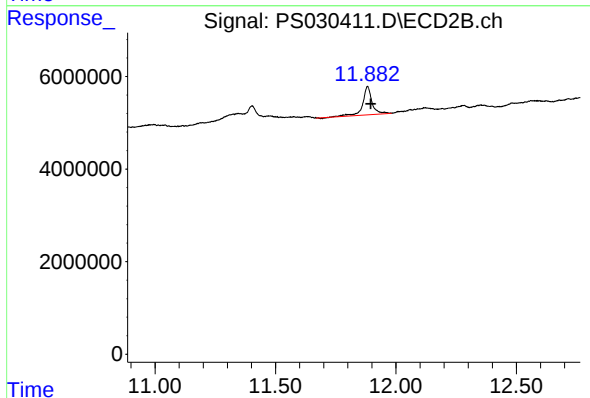


#15 Picloram

R.T.: 11.882 min
Delta R.T.: -0.013 min
Response: 16219680
Conc: 1.15 ng/ml

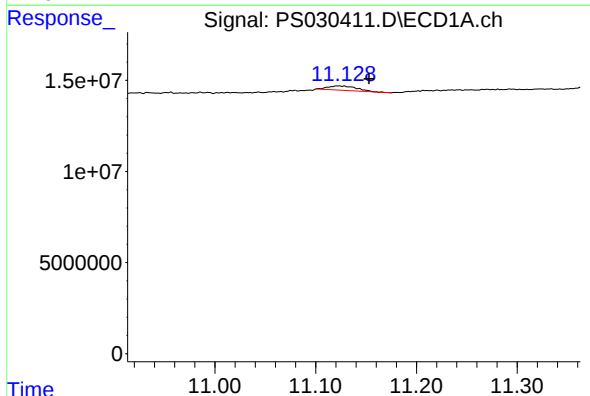

#16 DCPA

R.T.: 11.123 min
Delta R.T.: -0.029 min
Response: 4645104
Conc: N.D.

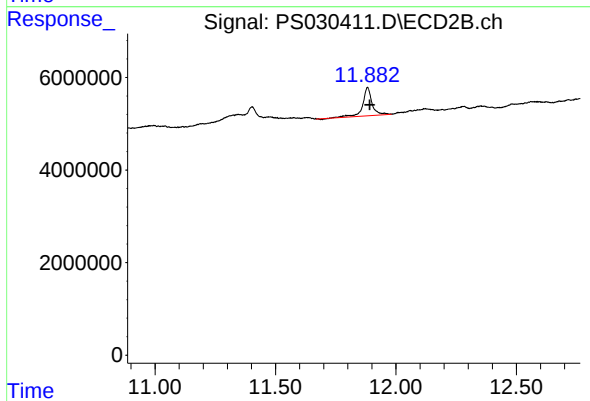

#16 DCPA

R.T.: 11.882 min
Delta R.T.: -0.010 min
Response: 16219680
Conc: 1.20 ng/ml