

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052820\
 Data File : PS010501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2020 21:24
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 06:43:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	350.8E6	279.5E6	498.994	521.204
Target Compounds							
1) T	Dalapon	0.000	2.600	0	148334	N.D.	<MDL
5) T	DICAMBA	0.000	7.091	0	714588	N.D.	<MDL
6) T	MCP	0.000	7.154	0	745813	N.D.	<MDL
7) T	MCPA	0.000	7.360	0	4588586	N.D.	1.687
8) T	DICHLORPROP	0.000	7.743	0	3211223	N.D.	5.688
9) T	2,4-D	8.415	7.964	17643891	169867	24.975	<MDL #
11) T	2,4,5-TP ...	0.000	8.771	0	1338904	N.D.	<MDL
12) T	2,4,5-T	0.000	9.173	0	87270	N.D.	<MDL
13) T	2,4-DB	0.000	9.680	0	165901	N.D.	<MDL
14) T	DINOSEB	0.000	10.037	0	928503	N.D.	<MDL
15) T	Picloram	0.000	11.007	0	1941473	N.D.	<MDL
16) T	DCPA	0.000	10.938	0	216501	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052820\
Data File : PS010501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2020 21:24
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 06:43:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

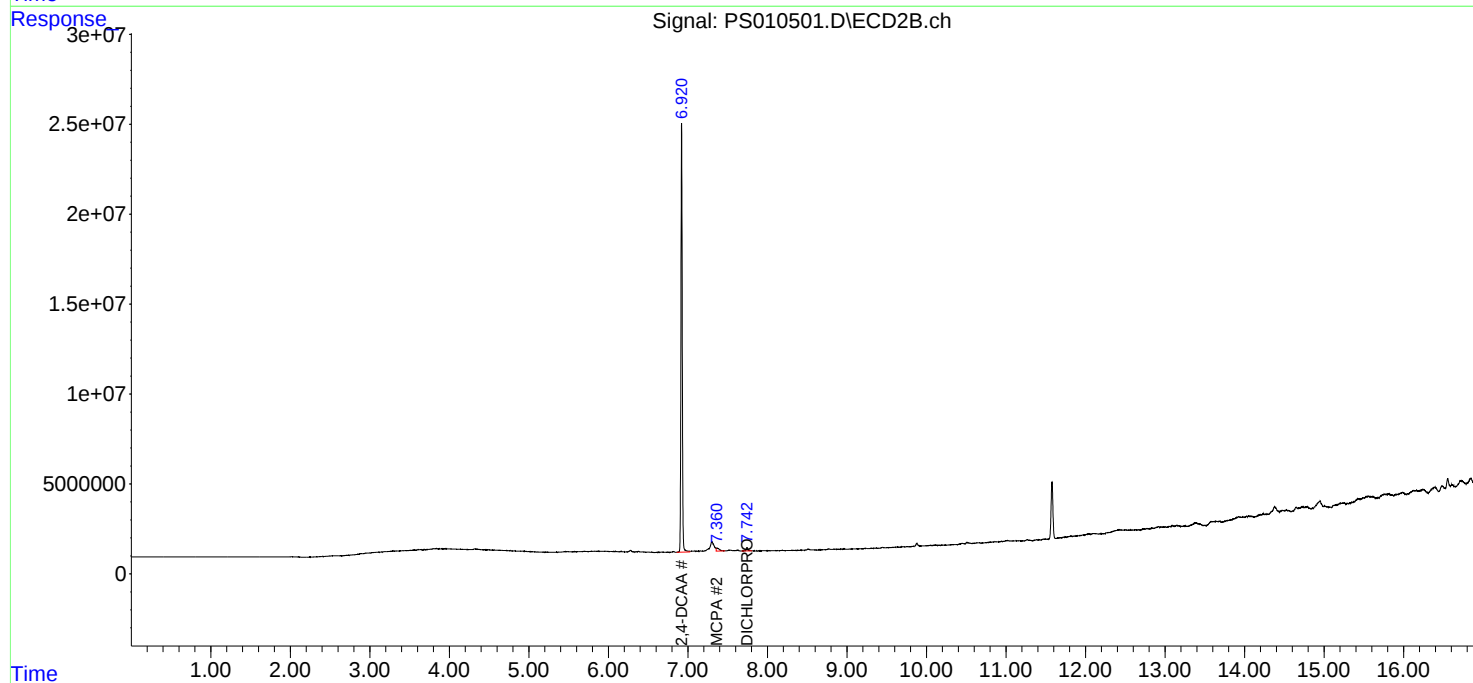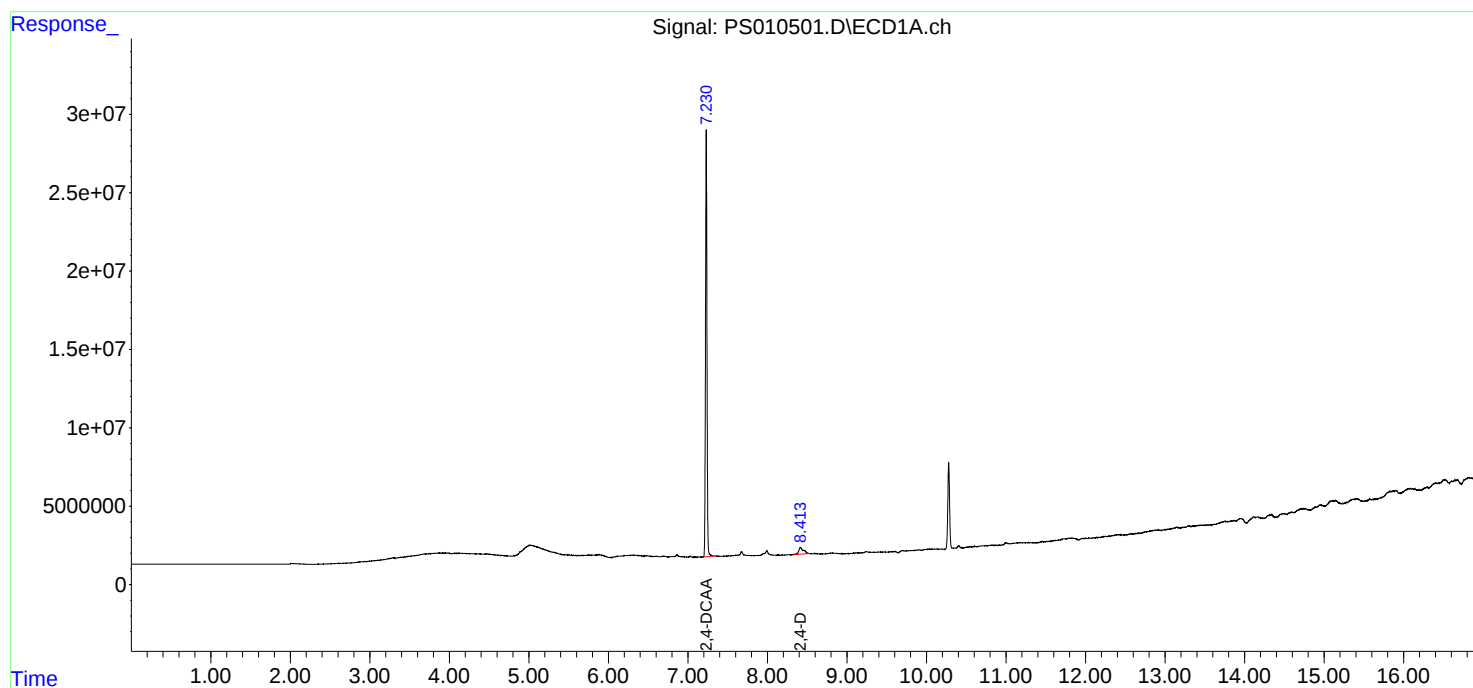


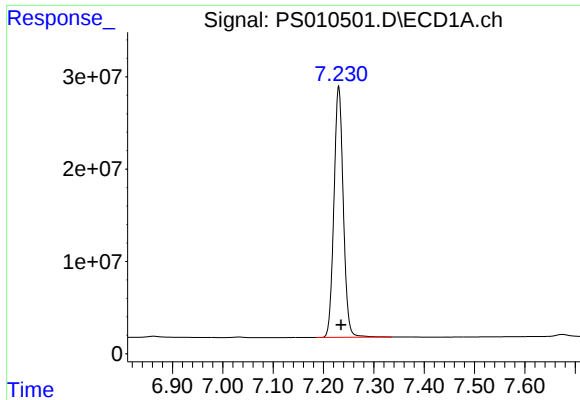

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: -0.005 min
Response: 350840270
Conc: 498.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

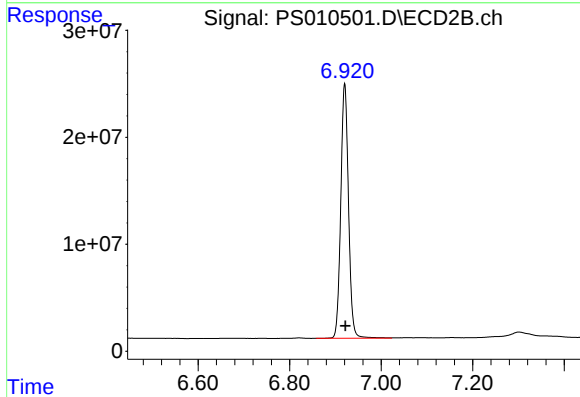


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 279517310
Conc: 521.20 ng/ml

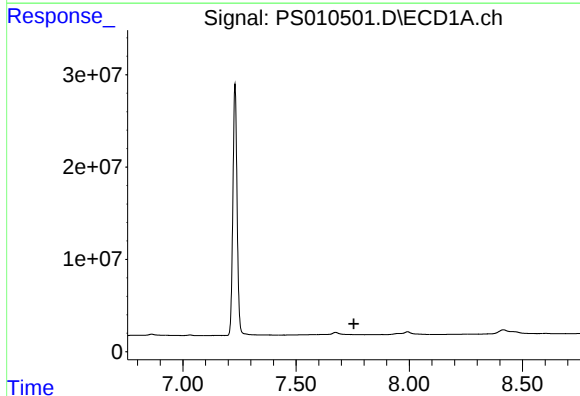


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.756 min
Response: 0
Conc: N.D.

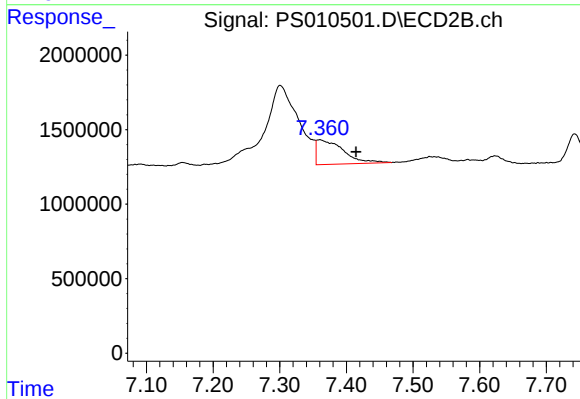

#7 MCPA


R.T.: 7.360 min
Delta R.T.: -0.054 min
Response: 4588586
Conc: 1.69 ug/ml

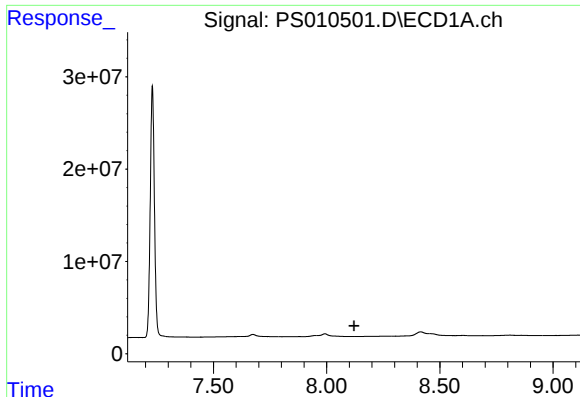

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

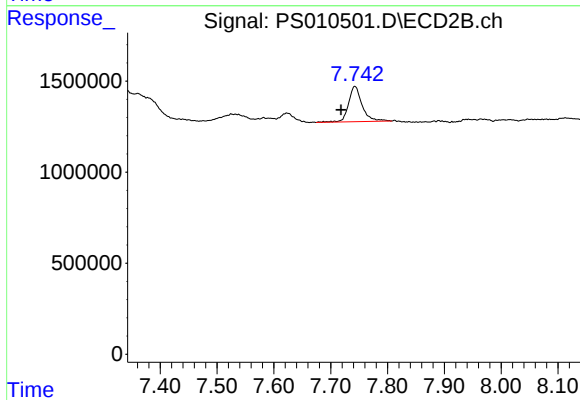


#8 DICHLORPROP

R.T.: 7.743 min
Delta R.T.: 0.024 min
Response: 3211223
Conc: 5.69 ng/ml

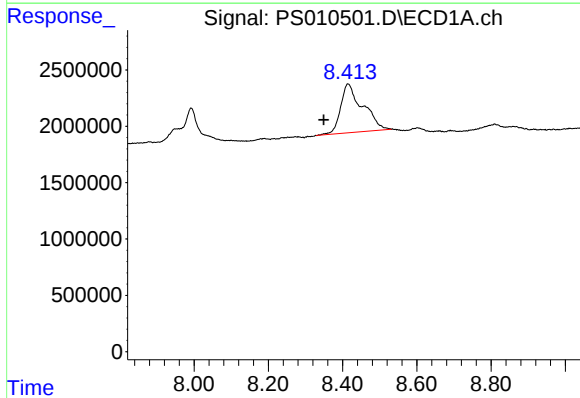

#9 2,4-D

R.T.: 8.415 min
Delta R.T.: 0.066 min
Response: 17643891
Conc: 24.98 ng/ml

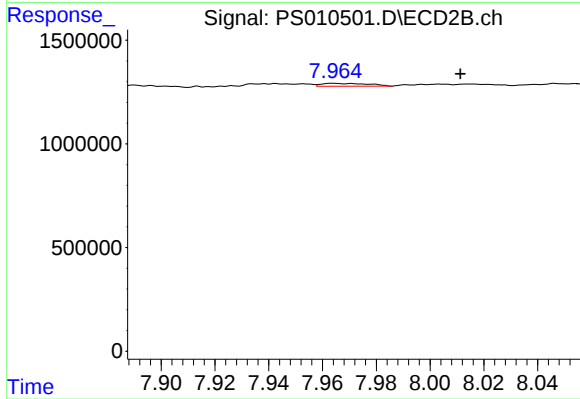

#9 2,4-D

R.T.: 7.964 min
Delta R.T.: -0.047 min
Response: 169867
Conc: N.D.