

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052820\
 Data File : PS010516.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 04:41
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 06:47:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	354.6E6	285.4E6	504.362	532.120
Target Compounds							
1) T	Dalapon	0.000	2.631	0	11505	N.D.	<MDL
5) T	DICAMBA	0.000	7.090	0	1414424	N.D.	<MDL
6) T	MCP	0.000	7.155	0	1278732	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.743	0	1872710	N.D.	3.317
9) T	2,4-D	8.415	7.943	6403198	1351619	9.064	1.949 #
10) T	Pentachlo...	0.000	8.440	0	656370	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.800	0	541677	N.D.	<MDL
12) T	2,4,5-T	0.000	9.183	0	1192303	N.D.	<MDL
13) T	2,4-DB	0.000	9.705	0	396935	N.D.	<MDL
14) T	DINOSEB	0.000	10.024	0	532093	N.D.	<MDL
15) T	Picloram	0.000	11.007	0	6755690	N.D.	1.600
16) T	DCPA	0.000	10.951	0	576255	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052820\
Data File : PS010516.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 04:41
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 06:47:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

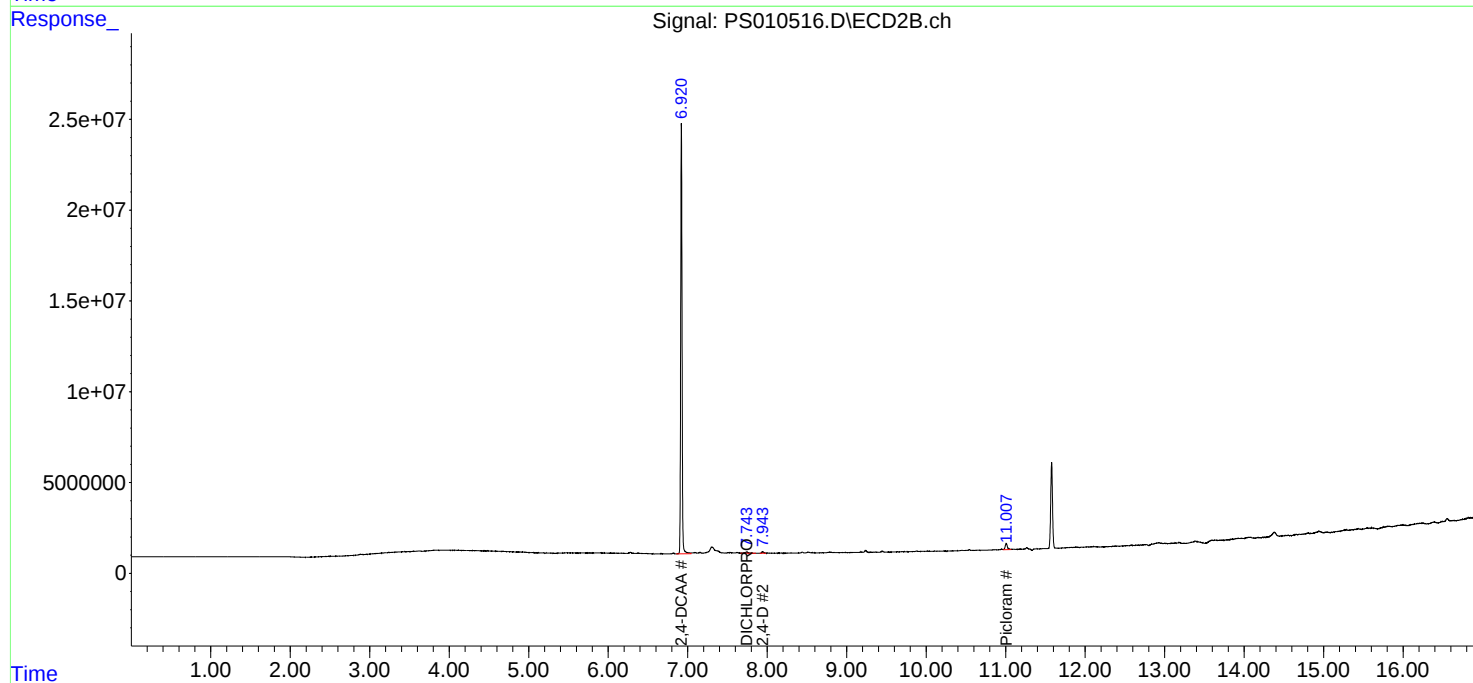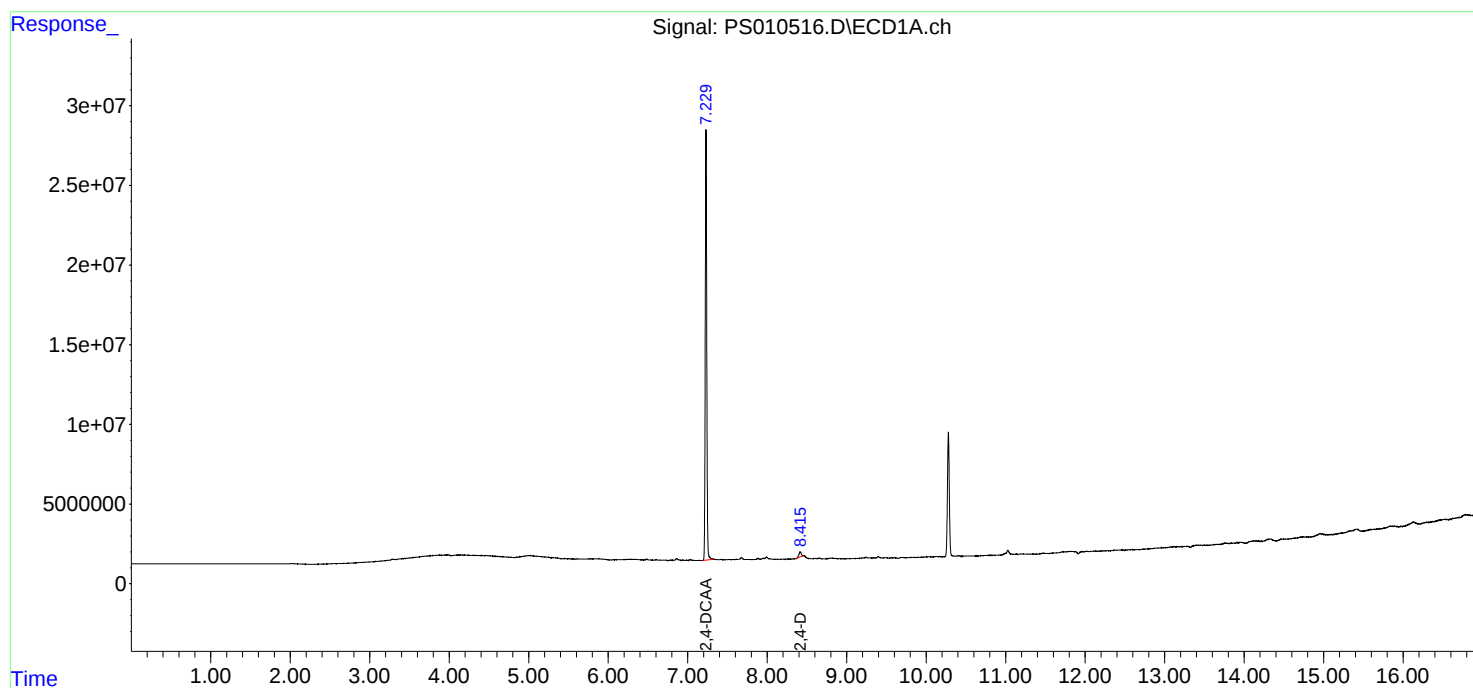


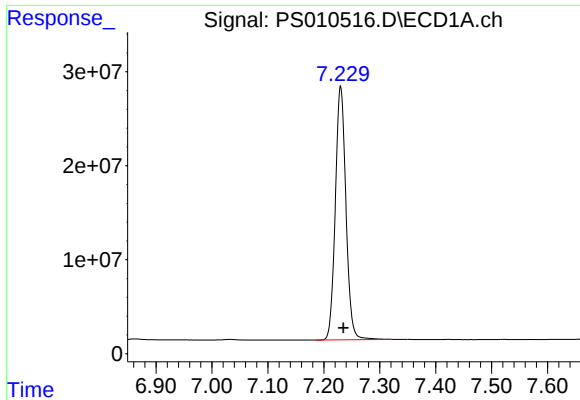

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: -0.005 min
Response: 354613893
Conc: 504.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

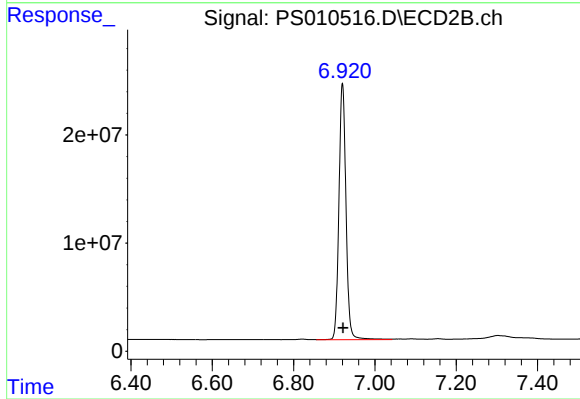


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 285371368
Conc: 532.12 ng/ml

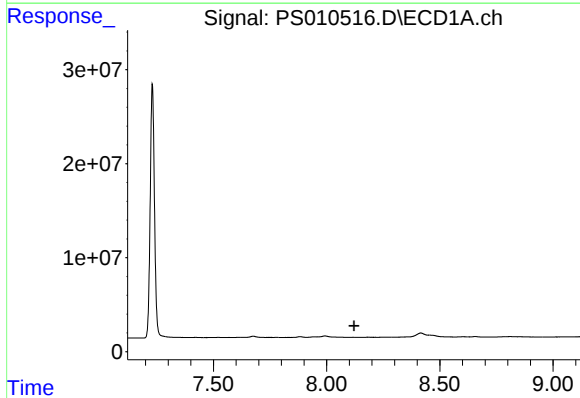


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

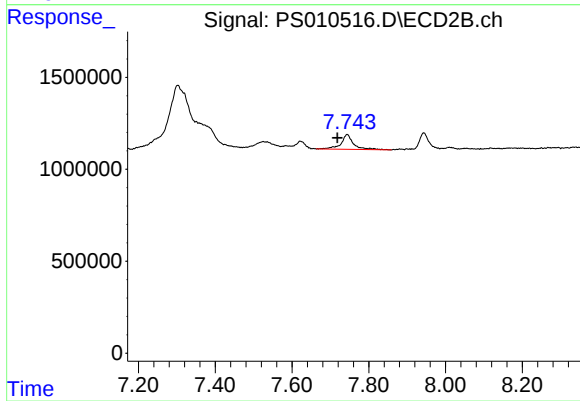

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.025 min
Response: 1872710
Conc: 3.32 ng/ml

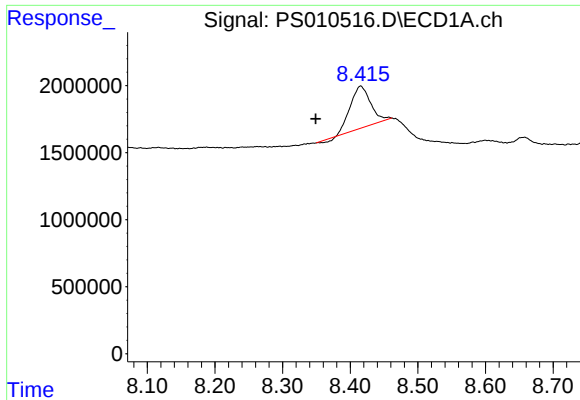

#9 2,4-D


R.T.: 8.415 min
Delta R.T.: 0.066 min
Response: 6403198
Conc: 9.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

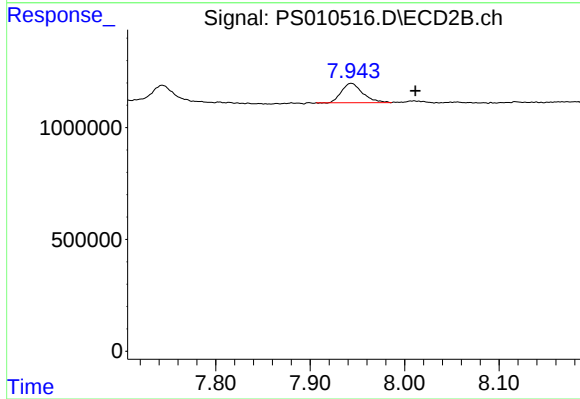


#9 2,4-D

R.T.: 7.943 min
Delta R.T.: -0.068 min
Response: 1351619
Conc: 1.95 ng/ml

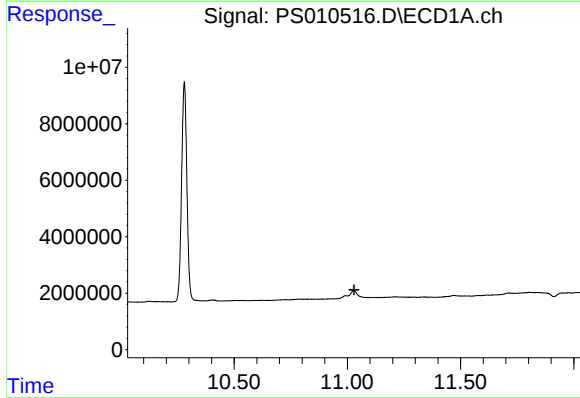

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.029 min
Response: 0
Conc: N.D.

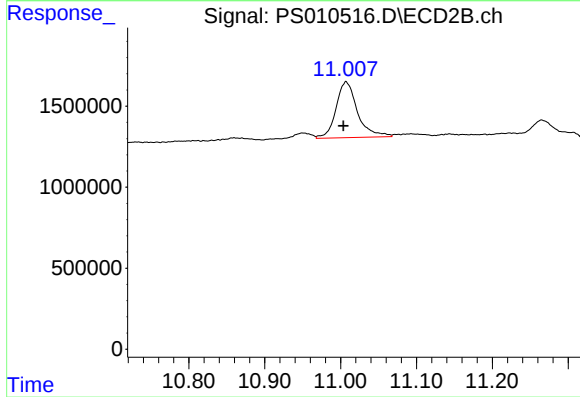

#15 Picloram

R.T.: 11.007 min
Delta R.T.: 0.004 min
Response: 6755690
Conc: 1.60 ng/ml