

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS052821\  
 Data File : PS015105.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 28 May 2021 11:19  
 Operator : DD\AJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 28 14:35:00 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052821.M  
 Quant Title : 8080.M  
 QLast Update : Fri May 28 14:34:22 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |              |        |         |          |          |              |
|------------------|--------------|--------|---------|----------|----------|--------------|
| 7) T             | MCPA         | 0.000  | 7.193f  | 0        | 10112983 | N.D. 3.891   |
| 10) T            | Pentachlo... | 8.658  | 0.000   | 3493313  | 0        | <MDL N.D. #  |
| 13) T            | 2,4-DB       | 10.023 | 0.000   | 15168527 | 0        | 5.957 N.D. # |
| 15) T            | Picloram     | 11.021 | 10.850  | 50576270 | 12118690 | 3.053 2.918  |
| 16) T            | DCPA         | 0.000  | 10.850f | 0        | 12118690 | N.D. 2.811   |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS052821\  
Data File : PS015105.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 28 May 2021 11:19  
Operator : DD\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 28 14:35:00 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS052821.M  
Quant Title : 8080.M  
QLast Update : Fri May 28 14:34:22 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

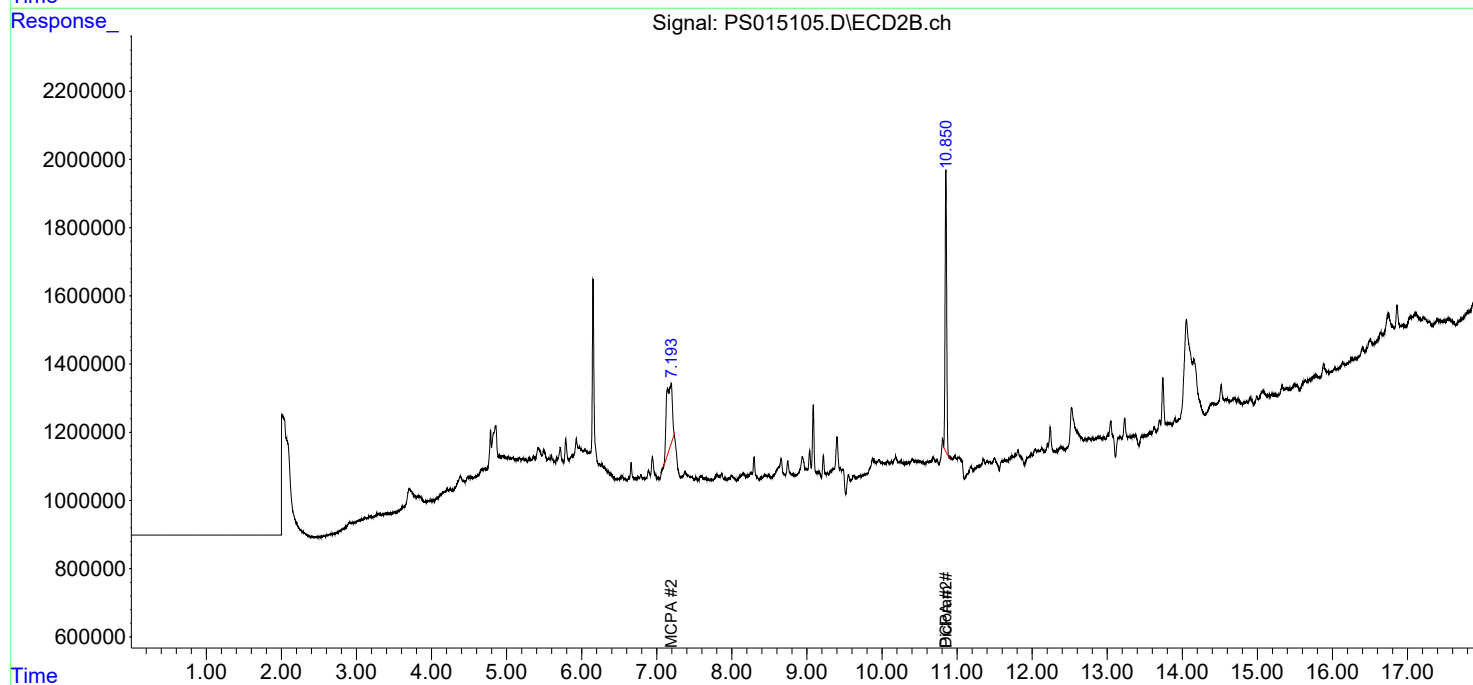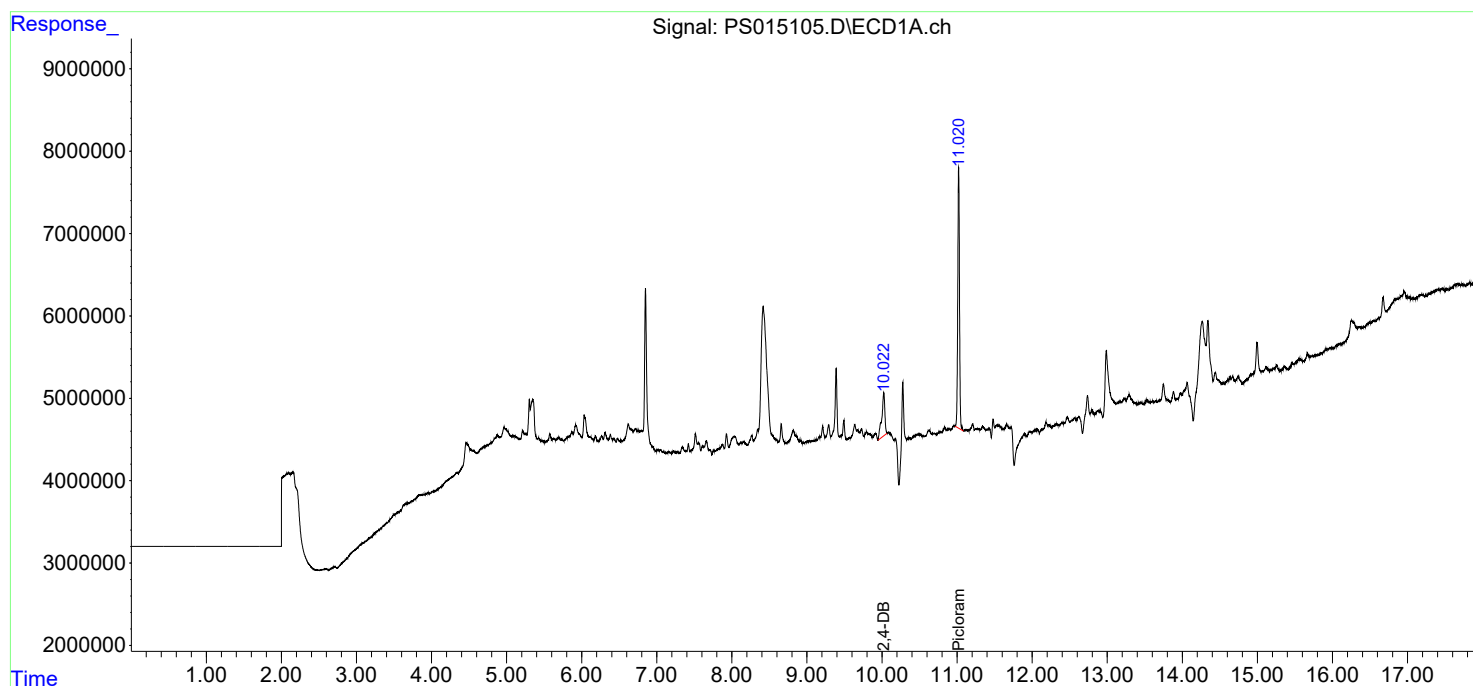


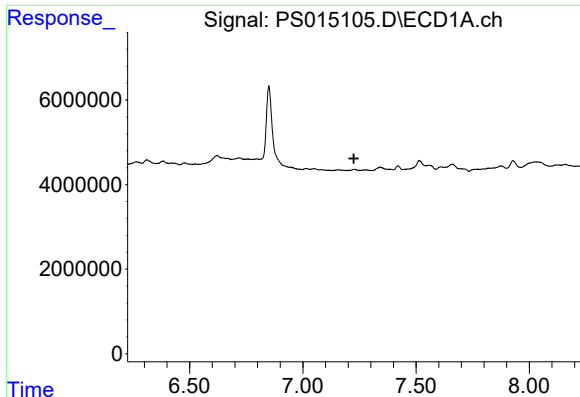

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T. : 7.225 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

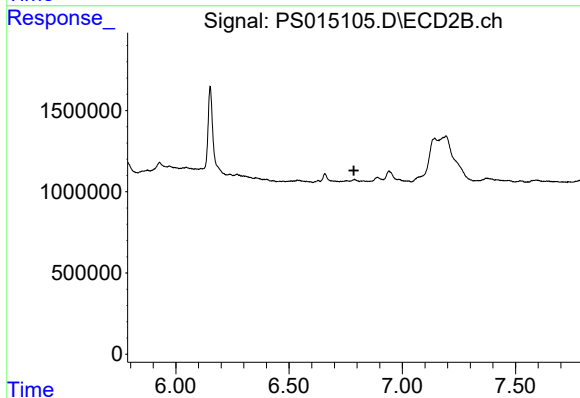


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 6.786 min  
Response: 0  
Conc: N.D.

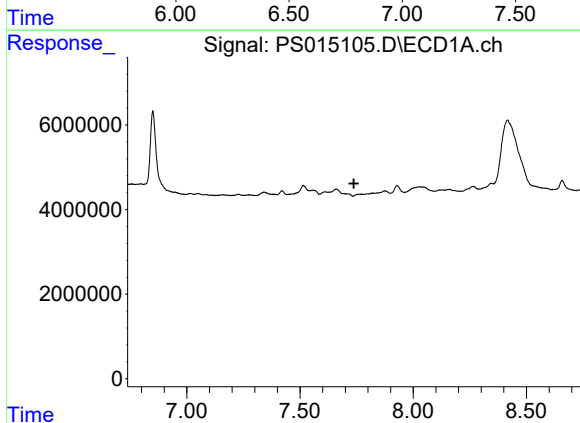


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 7.738 min  
Response: 0  
Conc: N.D.

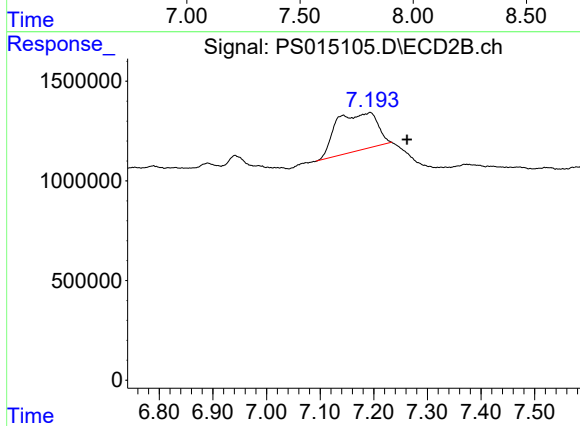

#7 MCPA


R.T.: 7.193 min  
Delta R.T.: -0.069 min  
Response: 10112983  
Conc: 3.89 ug/ml

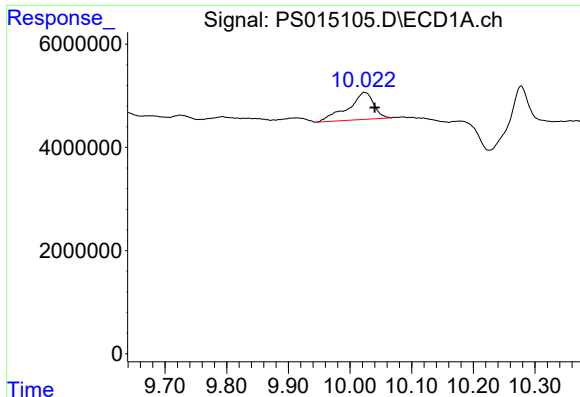

#13 2,4-DB


R.T.: 10.023 min  
Delta R.T.: -0.017 min  
Response: 15168527  
Conc: 5.96 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :

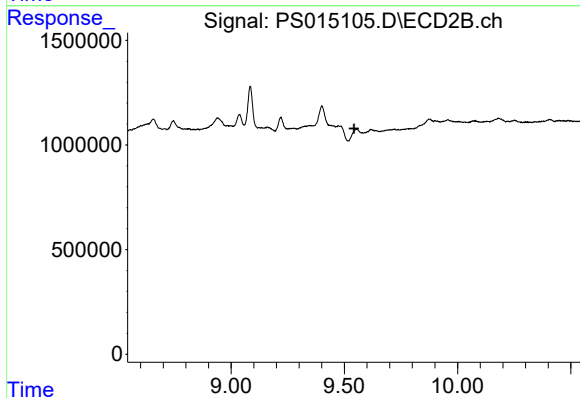


#13 2,4-DB

R.T.: 0.000 min  
Exp R.T. : 9.542 min  
Response: 0  
Conc: N.D.

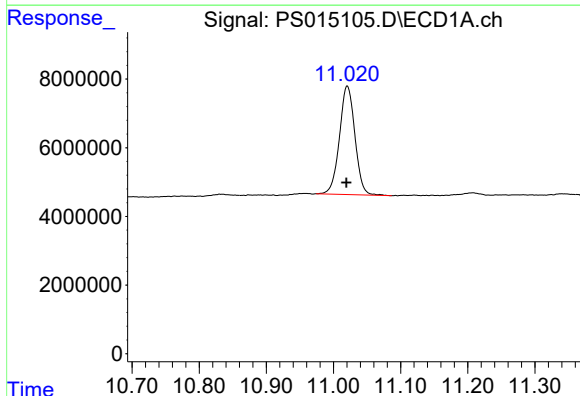


#15 Picloram

R.T.: 11.021 min  
Delta R.T.: 0.001 min  
Response: 50576270  
Conc: 3.05 ng/ml

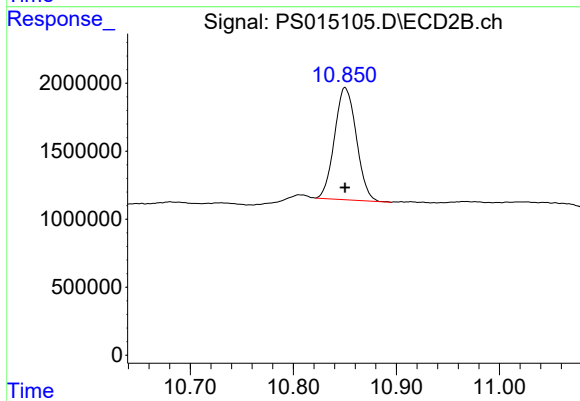

#15 Picloram


R.T.: 10.850 min  
Delta R.T.: 0.000 min  
Response: 12118690  
Conc: 2.92 ng/ml

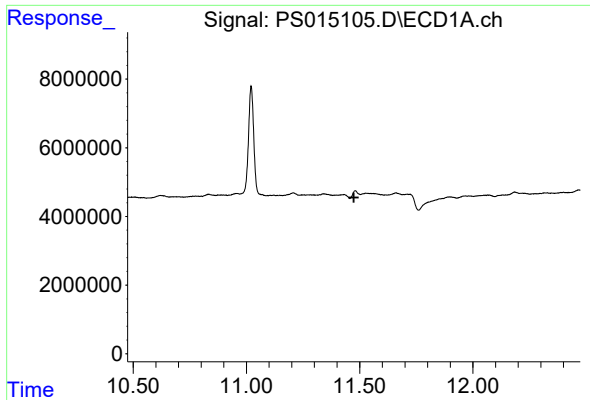

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 11.475 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :

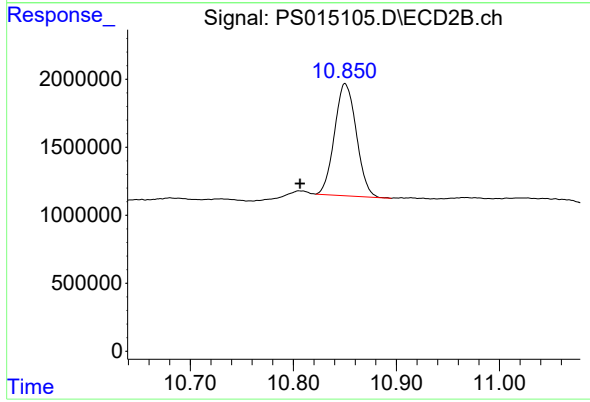

#16 DCPA

R.T.: 10.850 min  
Delta R.T.: 0.044 min  
Response: 12118690  
Conc: 2.81 ng/ml