

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052821\
 Data File : PS015106.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2021 11:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 14:35:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.786	1062.7E6	253.8E6	421.644	473.680
Target Compounds							
13) T	2,4-DB	10.022	0.000	6885942	0	2.704	N.D. #
15) T	Picloram	11.018	10.850	28531017	6879962	1.722	1.657
16) T	DCPA	0.000	10.850f	0	6879962	N.D.	1.596



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052821\
Data File : PS015106.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2021 11:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 14:35:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

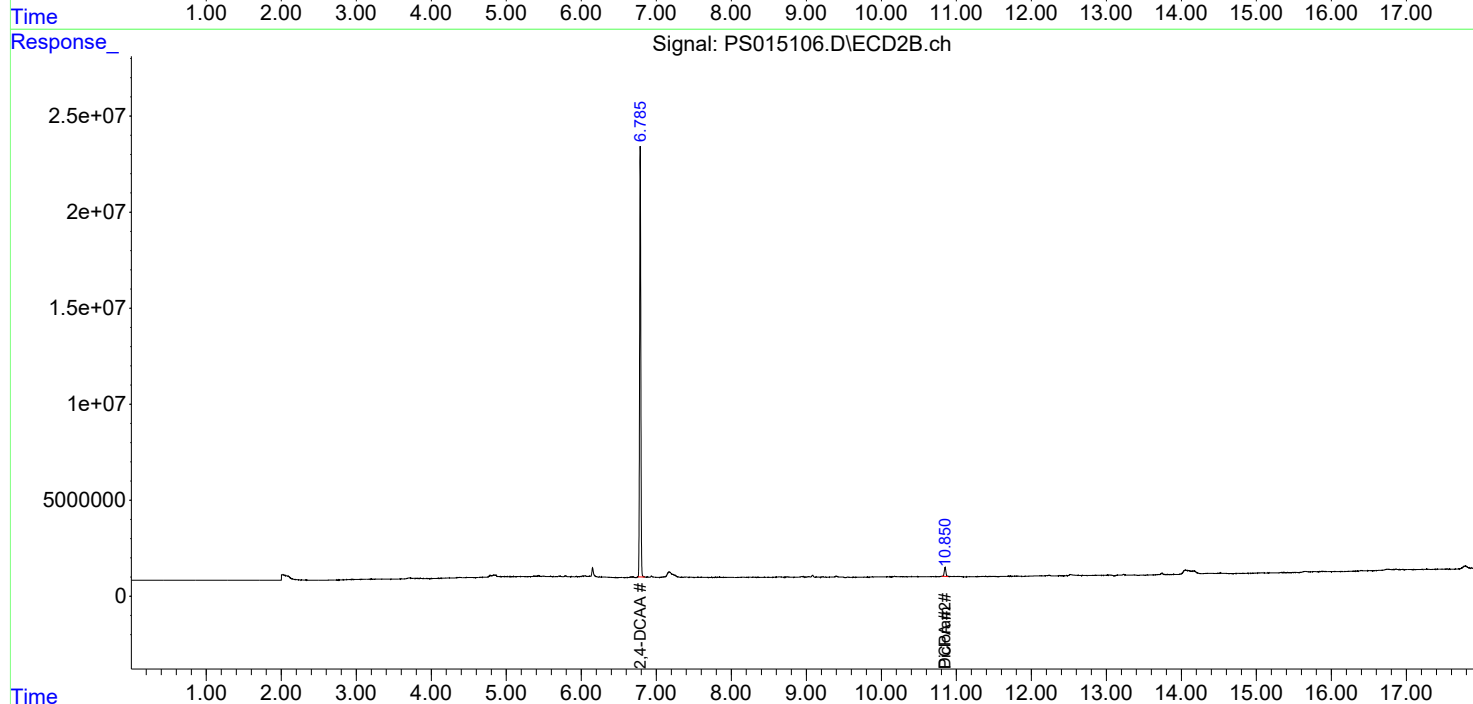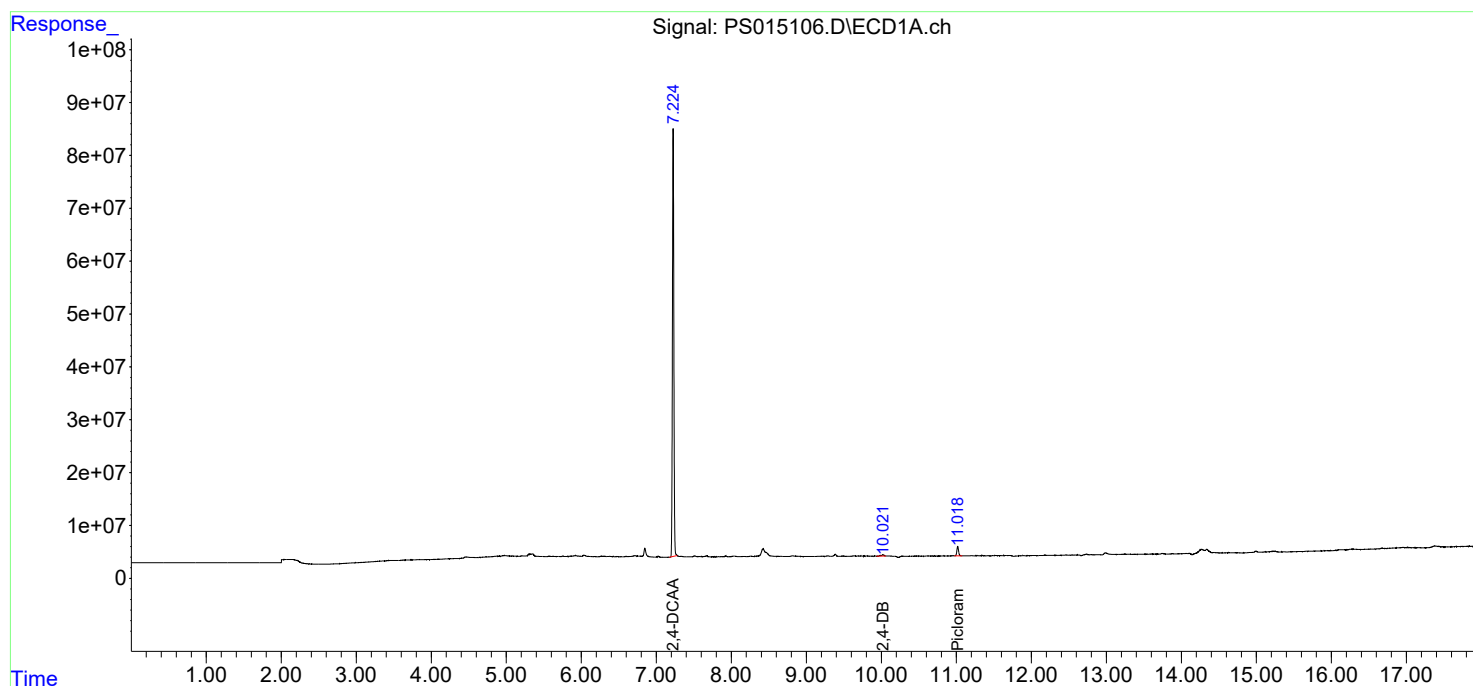


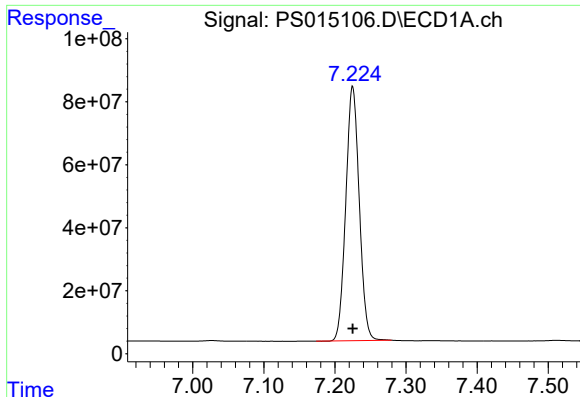

#4 2,4-DCAA


R.T.: 7.225 min
Delta R.T.: 0.000 min
Response: 1062700128
Conc: 421.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

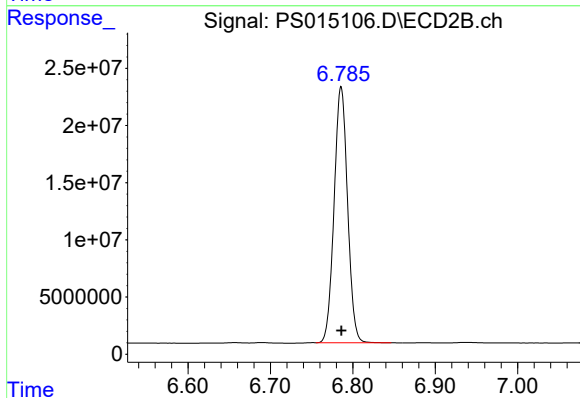


#4 2,4-DCAA

R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 253784210
Conc: 473.68 ng/ml

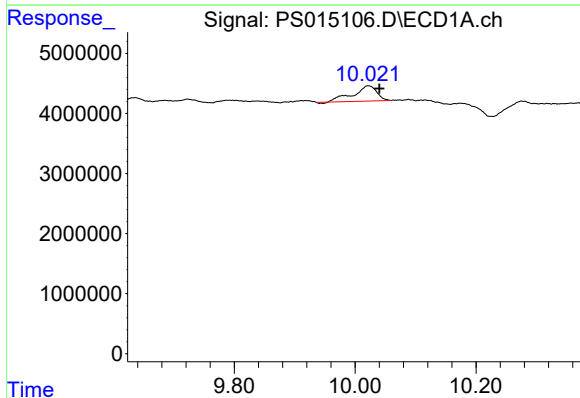


#13 2,4-DB

R.T.: 10.022 min
Delta R.T.: -0.019 min
Response: 6885942
Conc: 2.70 ng/ml

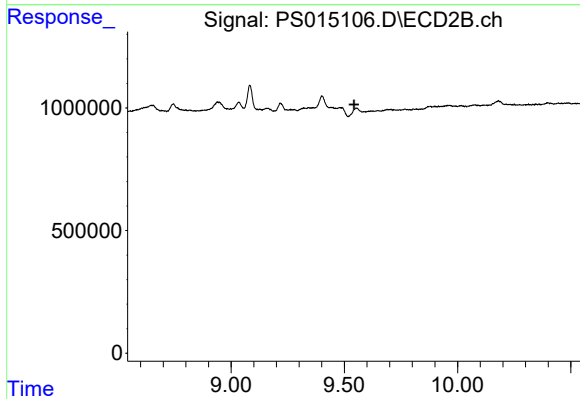

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.542 min
Response: 0
Conc: N.D.

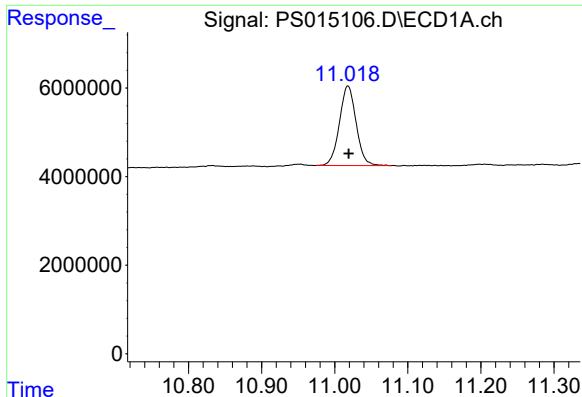

#15 Picloram


R.T.: 11.018 min
Delta R.T.: -0.001 min
Response: 28531017
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

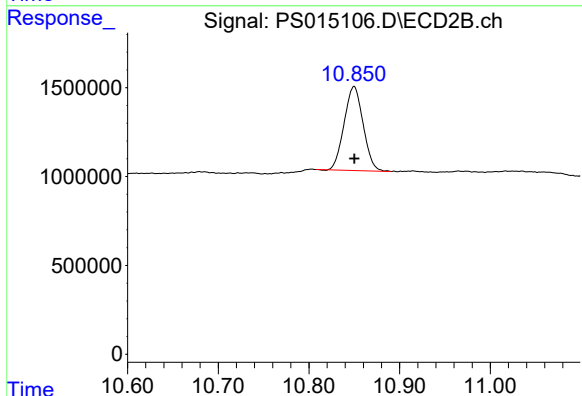


#15 Picloram

R.T.: 10.850 min
Delta R.T.: 0.000 min
Response: 6879962
Conc: 1.66 ng/ml

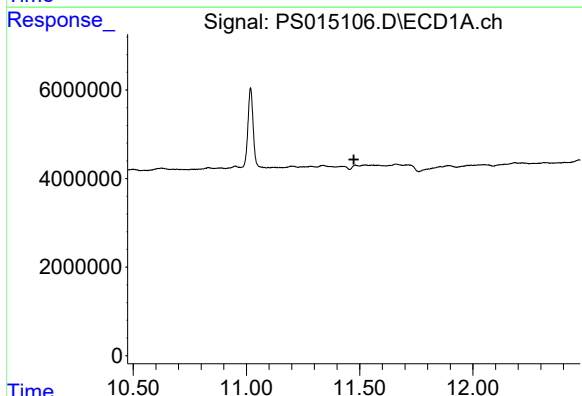

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

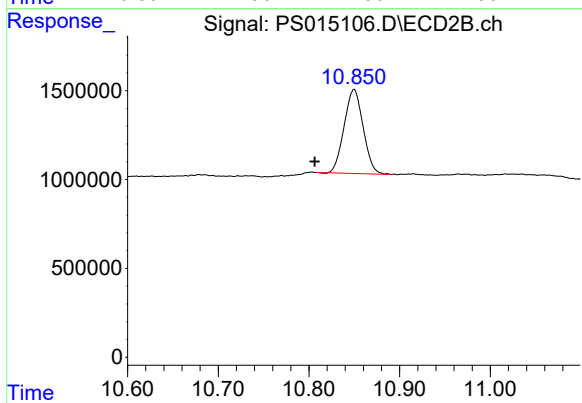

#16 DCPA

R.T.: 10.850 min
Delta R.T.: 0.043 min
Response: 6879962
Conc: 1.60 ng/ml