

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052821\
 Data File : PS015113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2021 14:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 01:51:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
 Quant Title : 8080.M
 QLast Update : Fri May 28 14:34:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.787	1075.3E6	255.4E6	426.629	476.605
Target Compounds							
3) T	4-Nitroph...	7.028	0.000	3239175	0	2.298	N.D. #
7) T	MCPA	7.675f	0.000	3940065	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	9.084f	0	3161853	N.D.	1.092
13) T	2,4-DB	10.031	0.000	7350736	0	2.887	N.D. #
15) T	Picloram	11.020	10.852	62203865	15186141	3.755	3.657
16) T	DCPA	0.000	10.852f	0	15186141	N.D.	3.523



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052821\
Data File : PS015113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2021 14:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 01:51:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052821.M
Quant Title : 8080.M
QLast Update : Fri May 28 14:34:22 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

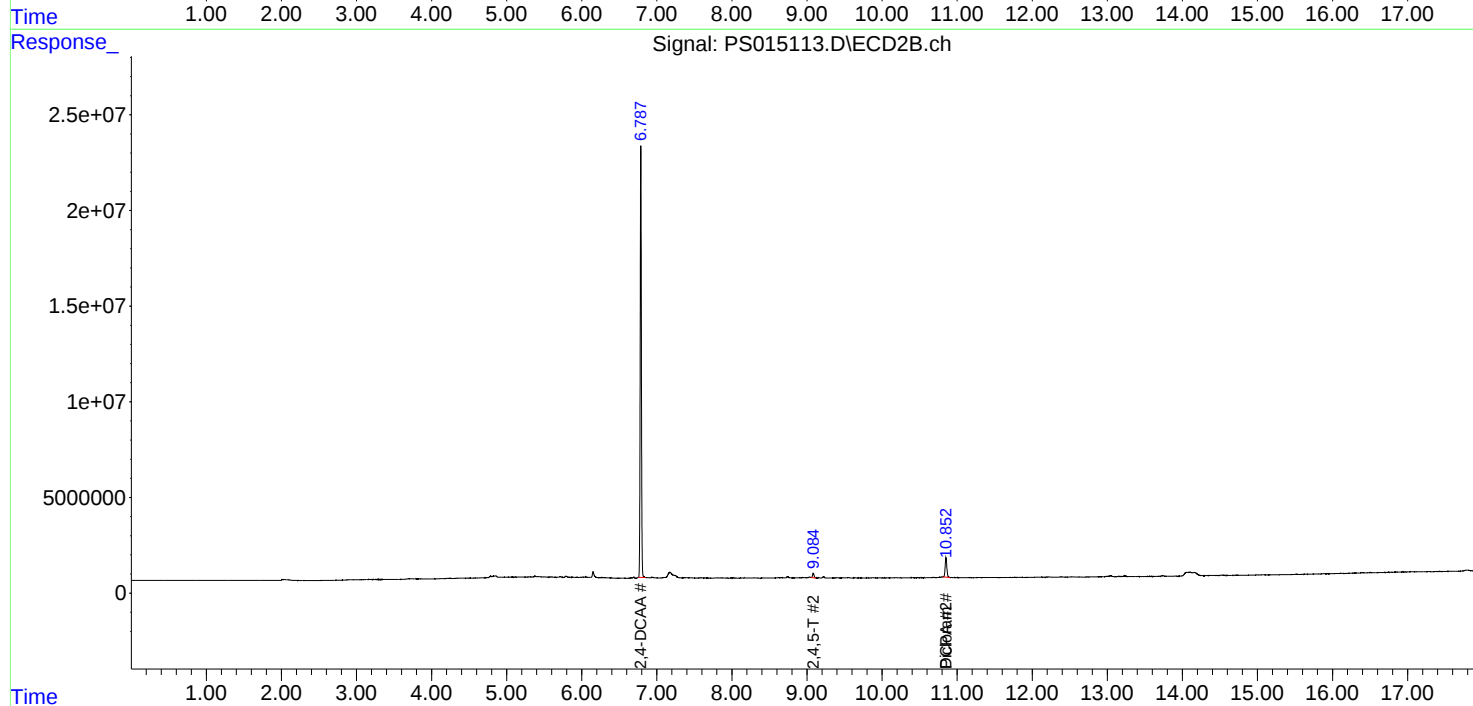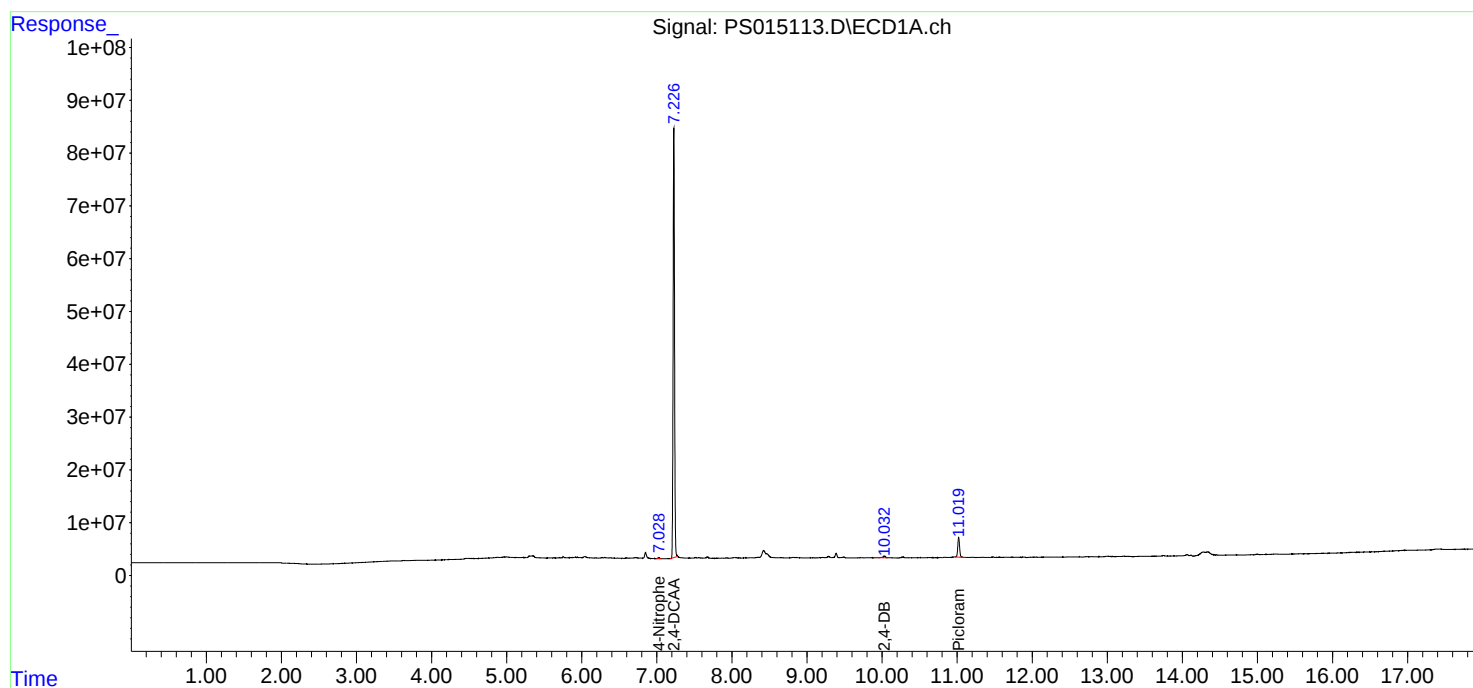


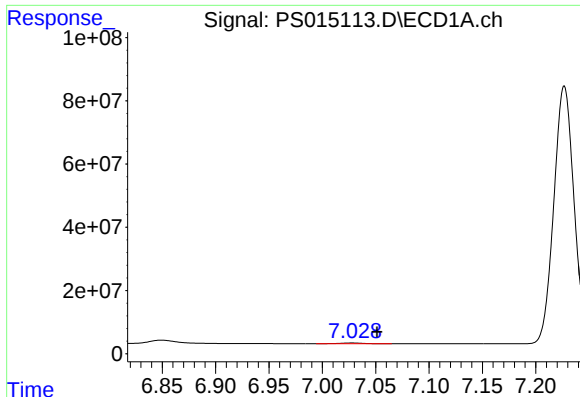

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.023 min
Response: 3239175
Conc: 2.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

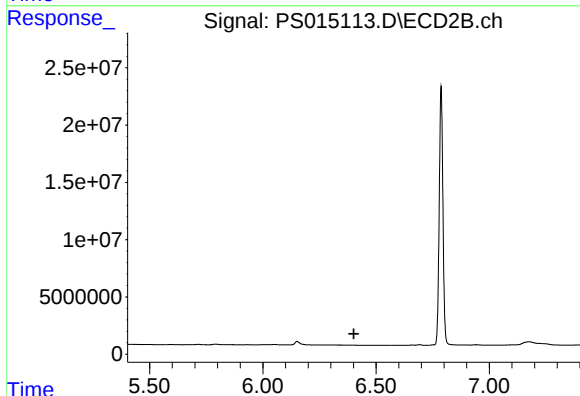


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.402 min
Response: 0
Conc: N.D.

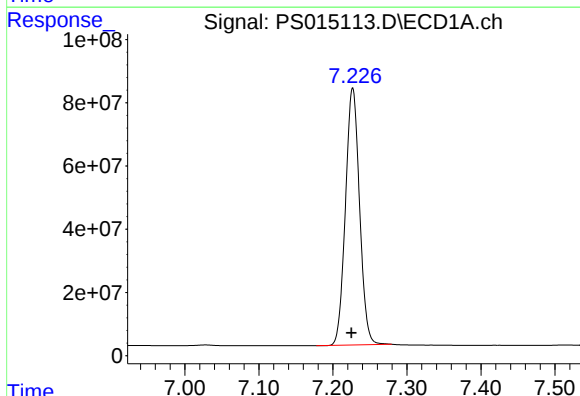


#4 2,4-DCAA

R.T.: 7.227 min
Delta R.T.: 0.002 min
Response: 1075266133
Conc: 426.63 ng/ml

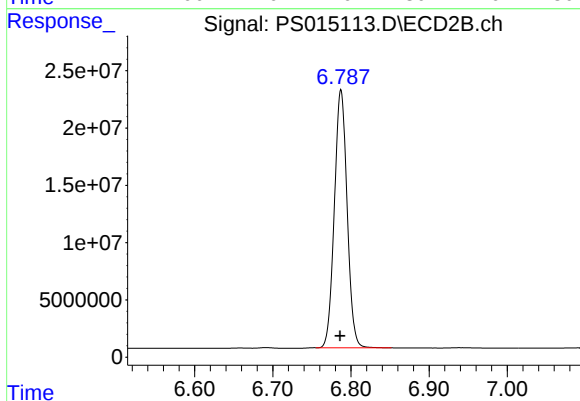

#4 2,4-DCAA


R.T.: 6.787 min
Delta R.T.: 0.001 min
Response: 255351103
Conc: 476.60 ng/ml

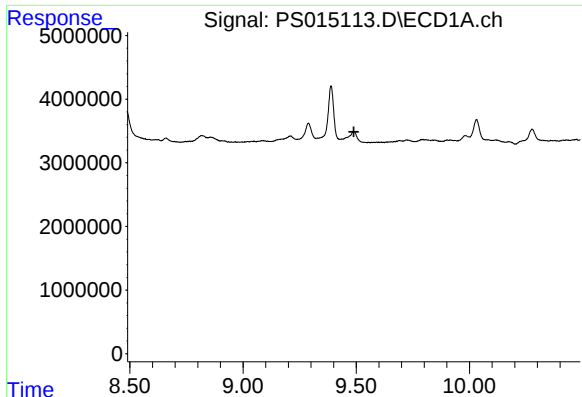

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

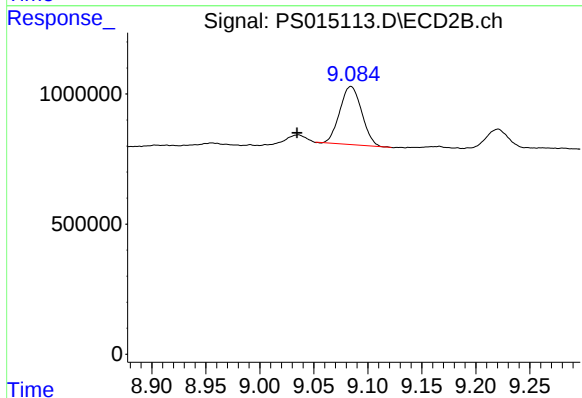


#12 2,4,5-T

R.T.: 9.084 min
Delta R.T.: 0.050 min
Response: 3161853
Conc: 1.09 ng/ml

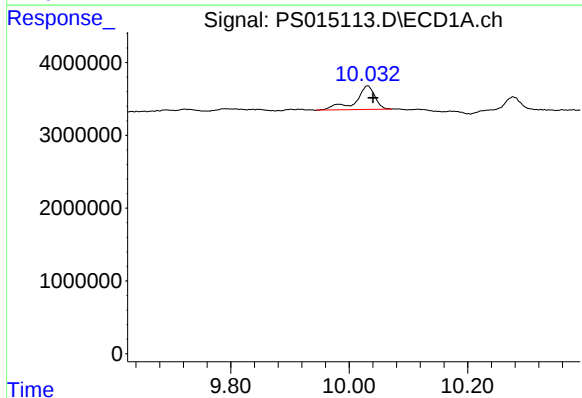


#13 2,4-DB

R.T.: 10.031 min
Delta R.T.: -0.009 min
Response: 7350736
Conc: 2.89 ng/ml

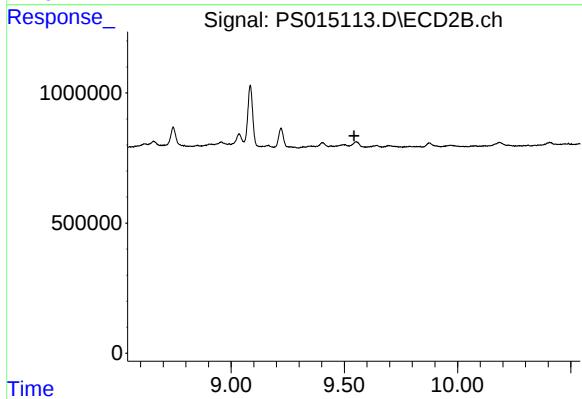

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.542 min
Response: 0
Conc: N.D.

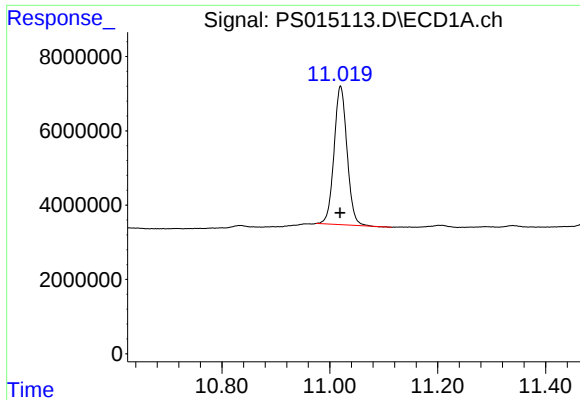

#15 Picloram


R.T.: 11.020 min
Delta R.T.: 0.000 min
Response: 62203865
Conc: 3.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

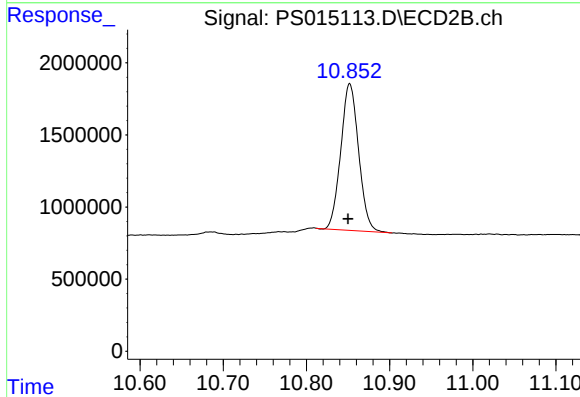


#15 Picloram

R.T.: 10.852 min
Delta R.T.: 0.002 min
Response: 15186141
Conc: 3.66 ng/ml

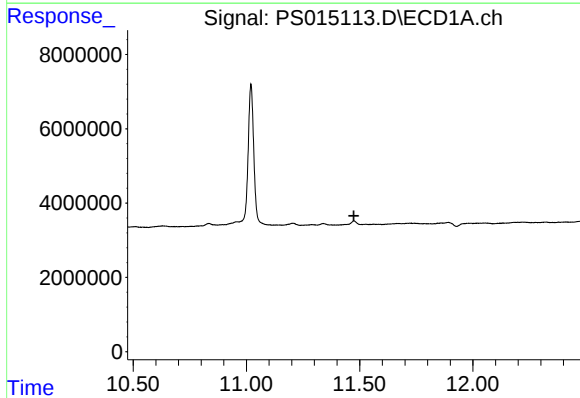

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.475 min
Response: 0
Conc: N.D.

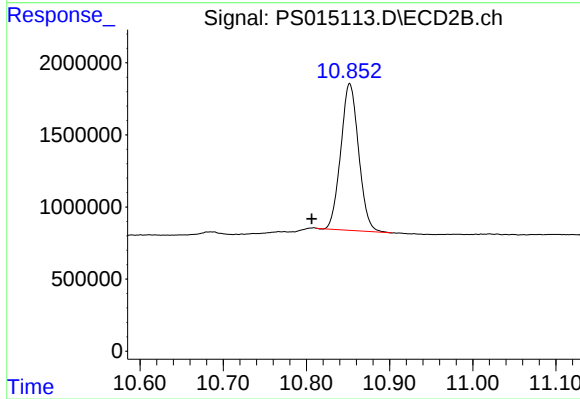

#16 DCPA

R.T.: 10.852 min
Delta R.T.: 0.046 min
Response: 15186141
Conc: 3.52 ng/ml