

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052920\
 Data File : PS010518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 12:26
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 15:44:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
9) T	2,4-D	0.000	7.947	0	7393052	N.D. 9.750
12) T	2,4,5-T	0.000	9.242	0	13954904	N.D. 4.650
15) T	Picloram	11.035	11.012	40720716	47643779	7.976 11.547 #
16) T	DCPA	0.000	11.012	0	47643779	N.D. 12.848



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052920\
Data File : PS010518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 12:26
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 15:44:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

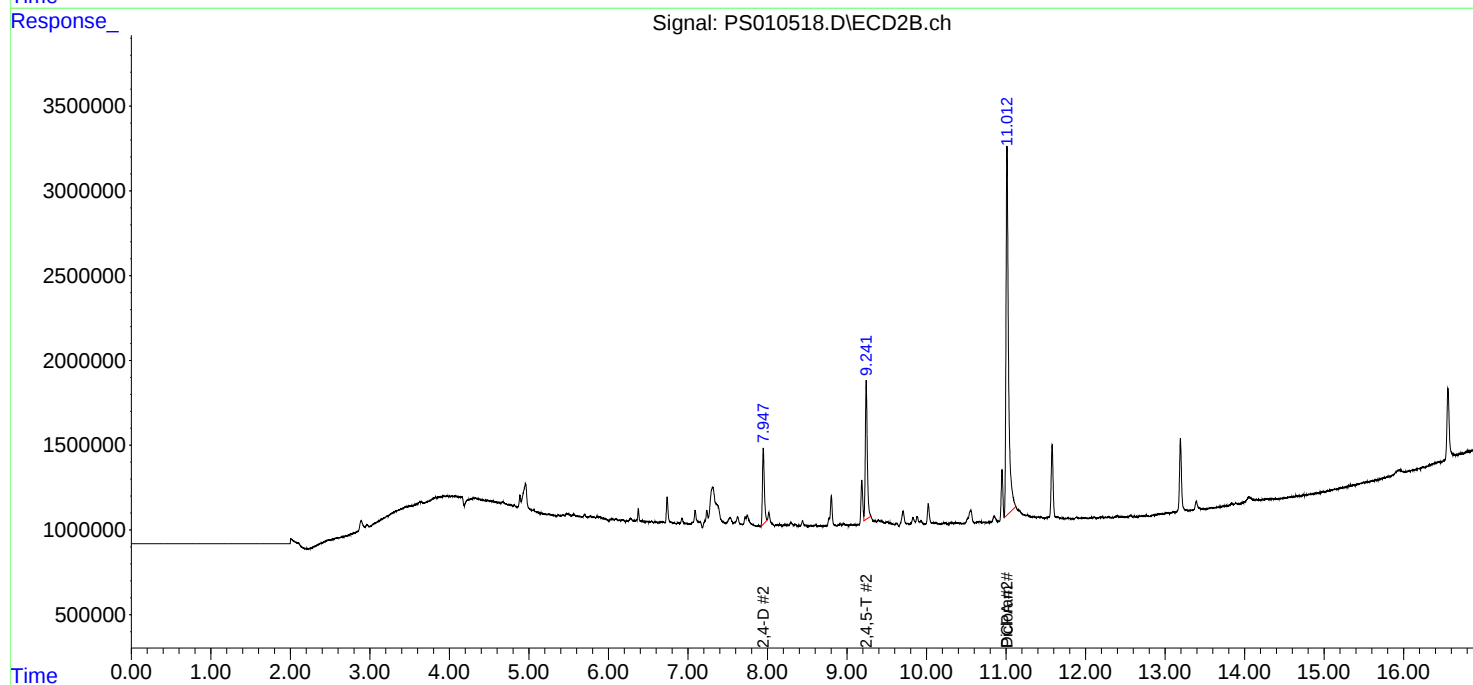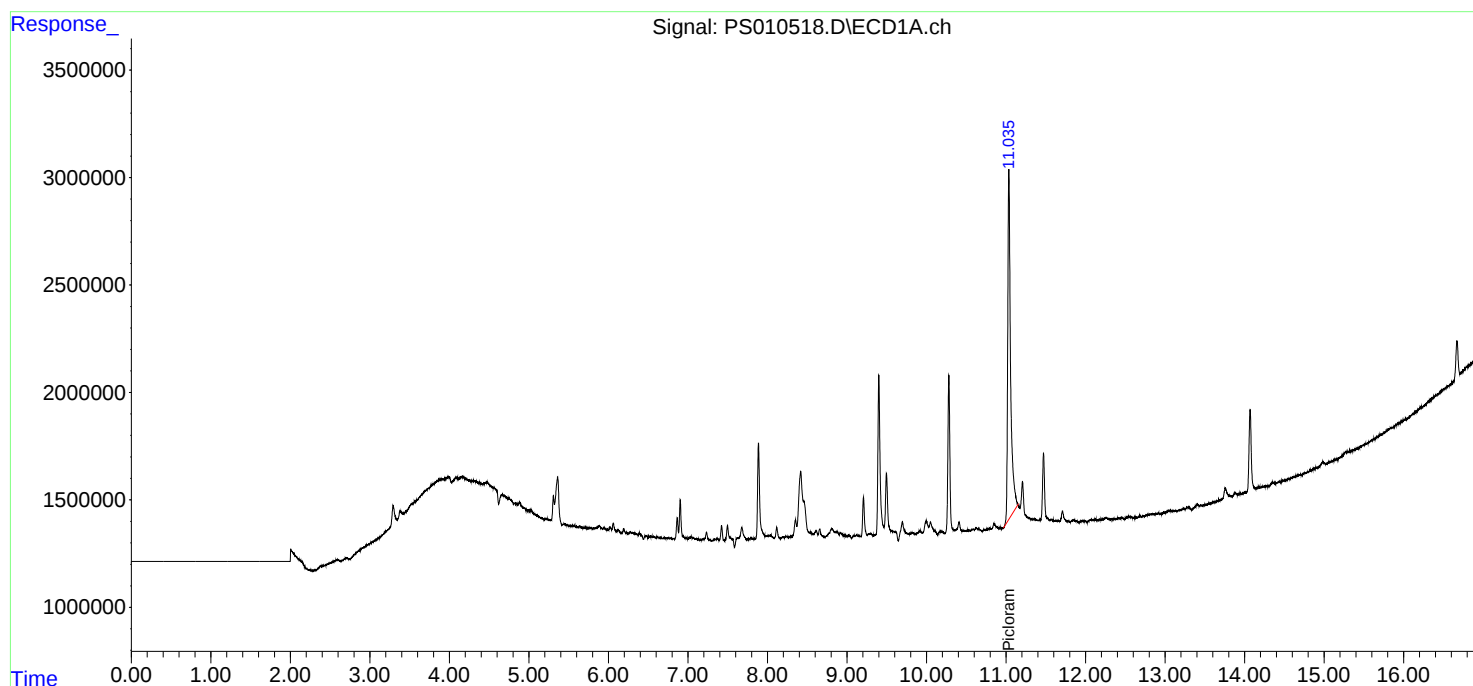


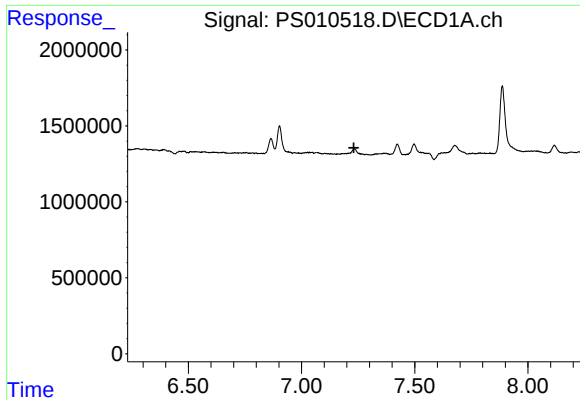

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

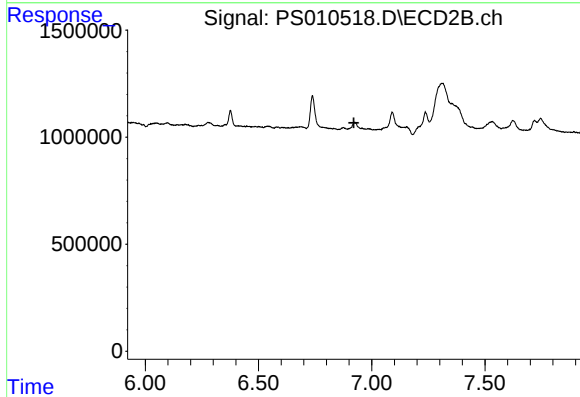


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

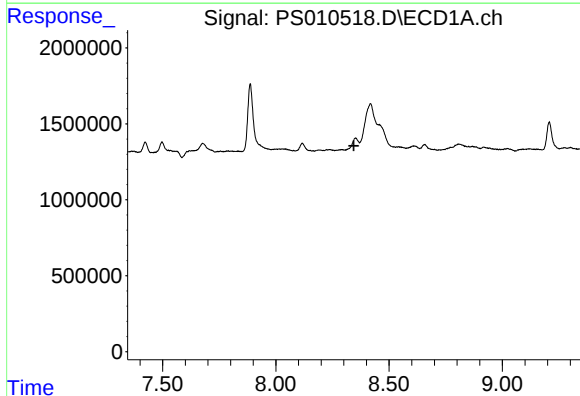


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

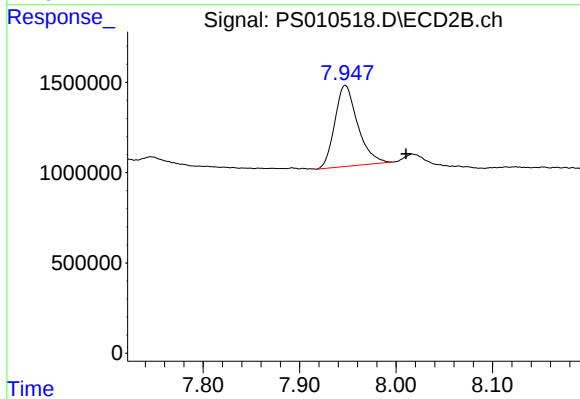

#9 2,4-D


R.T.: 7.947 min
Delta R.T.: -0.063 min
Response: 7393052
Conc: 9.75 ng/ml

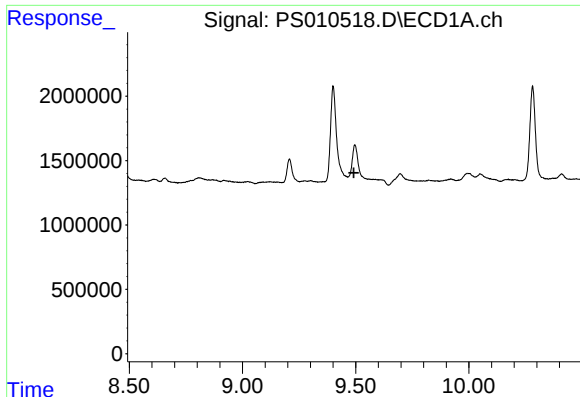

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

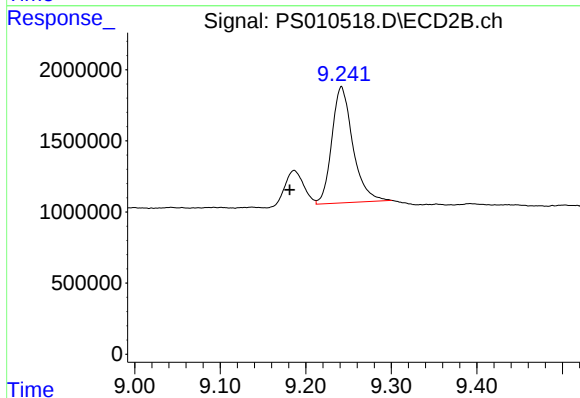


#12 2,4,5-T

R.T.: 9.242 min
Delta R.T.: 0.060 min
Response: 13954904
Conc: 4.65 ng/ml

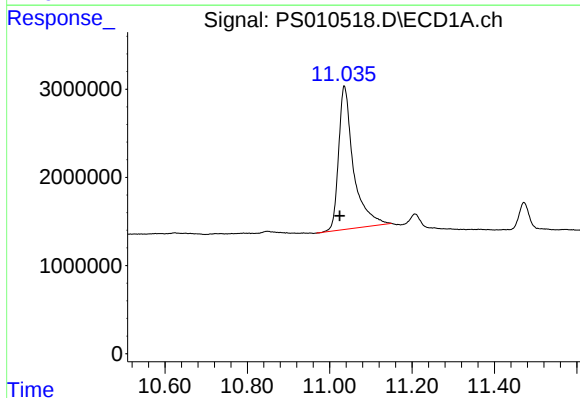


#15 Picloram

R.T.: 11.035 min
Delta R.T.: 0.011 min
Response: 40720716
Conc: 7.98 ng/ml

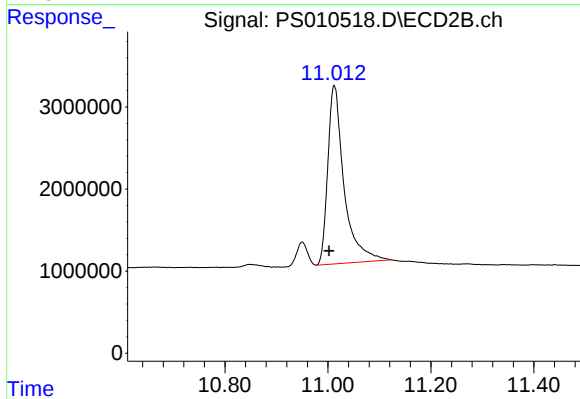

#15 Picloram


R.T.: 11.012 min
Delta R.T.: 0.010 min
Response: 47643779
Conc: 11.55 ng/ml

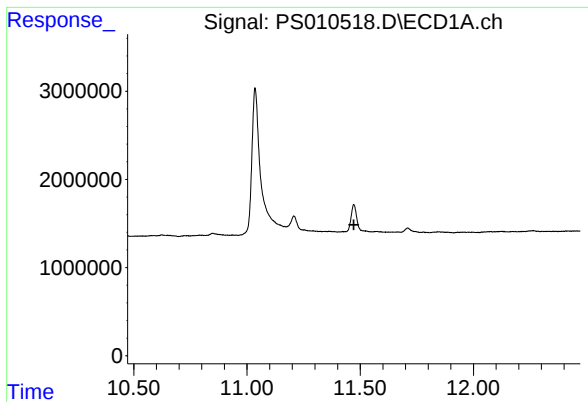

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

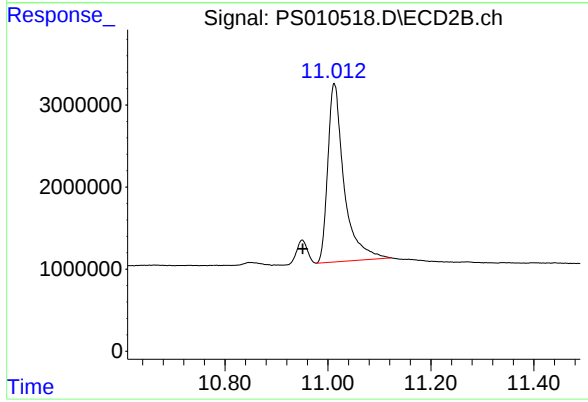

#16 DCPA

R.T.: 11.012 min
Delta R.T.: 0.061 min
Response: 47643779
Conc: 12.85 ng/ml