

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052920\
 Data File : PS010519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 12:49
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 15:44:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.921	328.5E6	263.6E6	415.412	483.250
Target Compounds							
12) T	2,4,5-T	0.000	9.244	0	12346472	N.D.	4.114
15) T	Picloram	11.039	11.015	32390586	37858073	6.345	9.176 #
16) T	DCPA	0.000	11.015	0	37858073	N.D.	10.209



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052920\
Data File : PS010519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 12:49
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 15:44:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

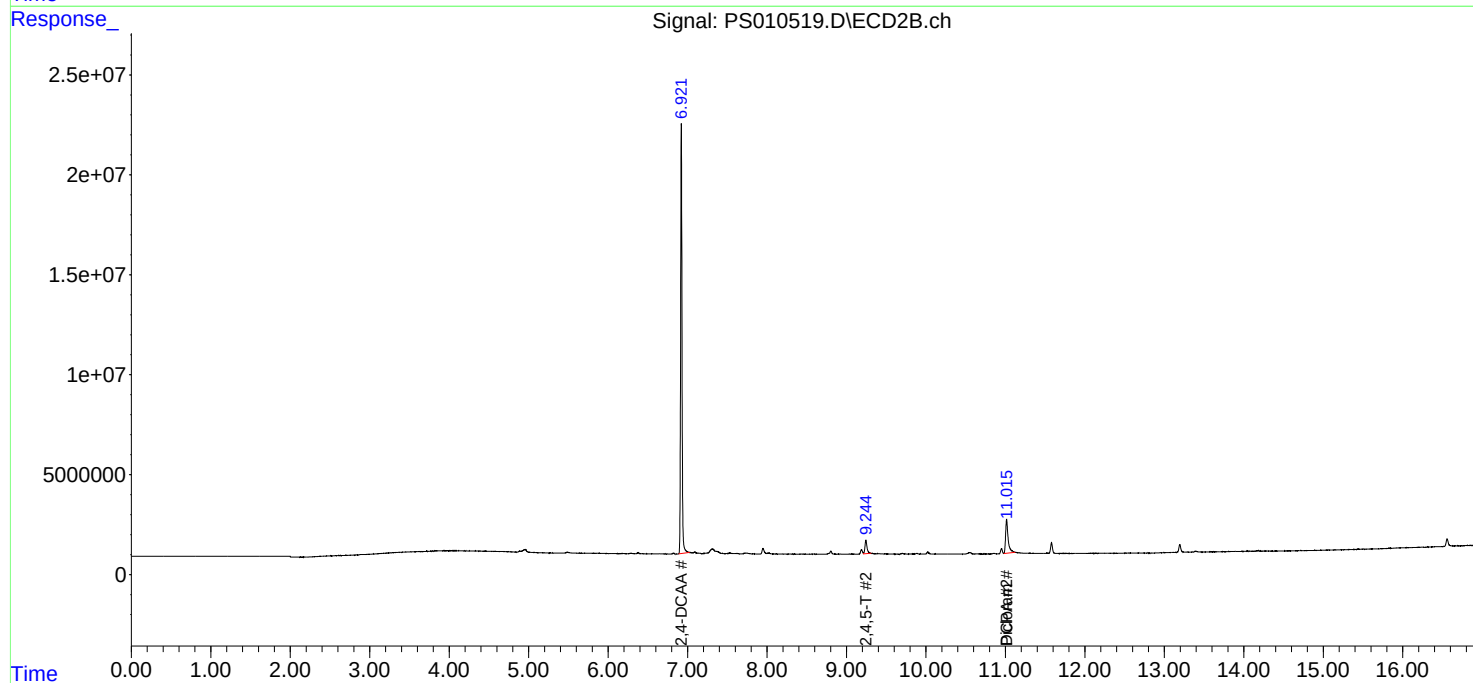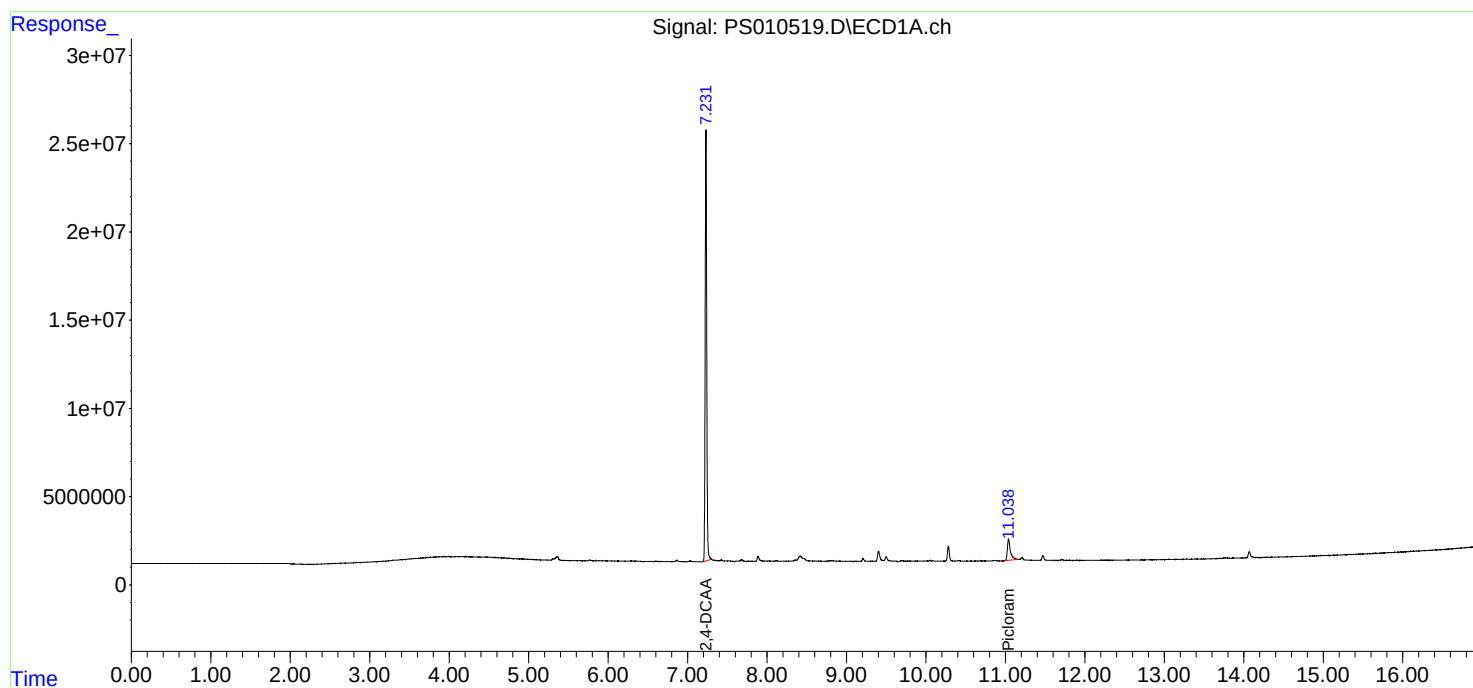


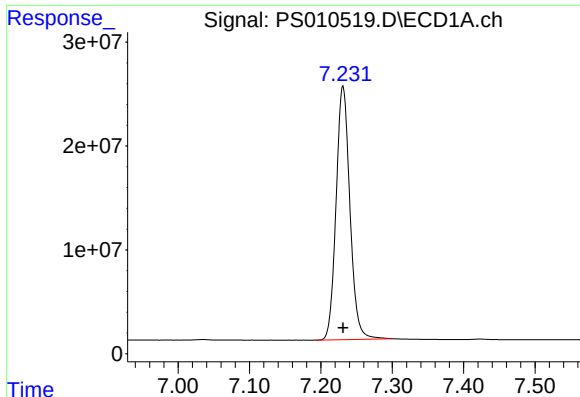

#4 2,4-DCAA


R.T.: 7.231 min
Delta R.T.: 0.000 min
Response: 328533850
Conc: 415.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

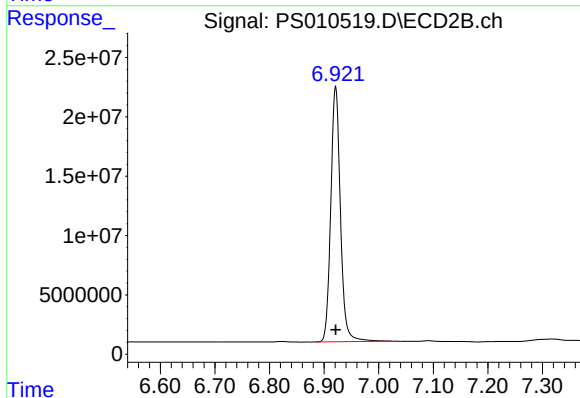


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 263572192
Conc: 483.25 ng/ml

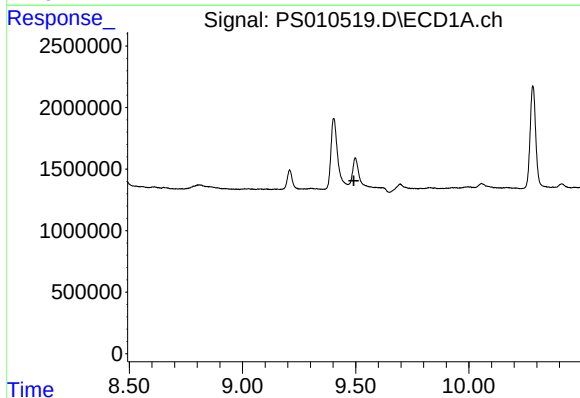


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.492 min
Response: 0
Conc: N.D.

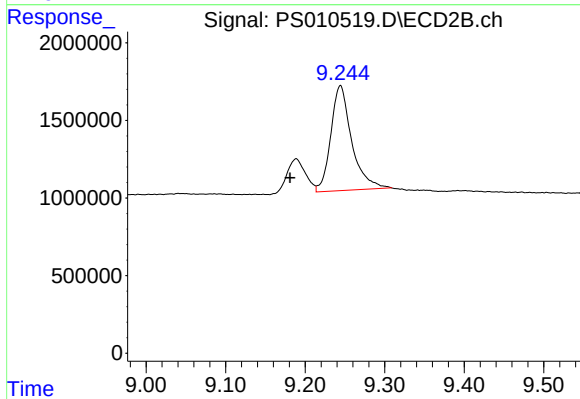

#12 2,4,5-T


R.T.: 9.244 min
Delta R.T.: 0.063 min
Response: 12346472
Conc: 4.11 ng/ml

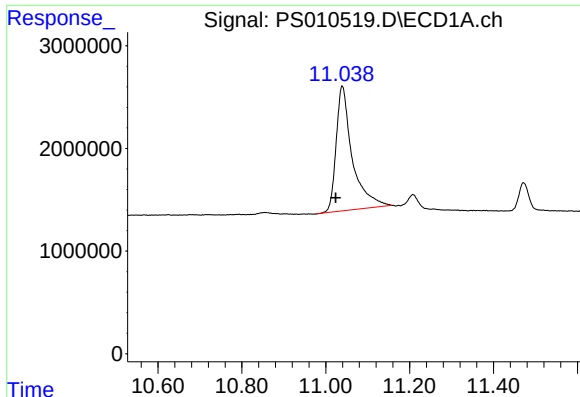

#15 Picloram


R.T.: 11.039 min
Delta R.T.: 0.015 min
Response: 32390586
Conc: 6.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

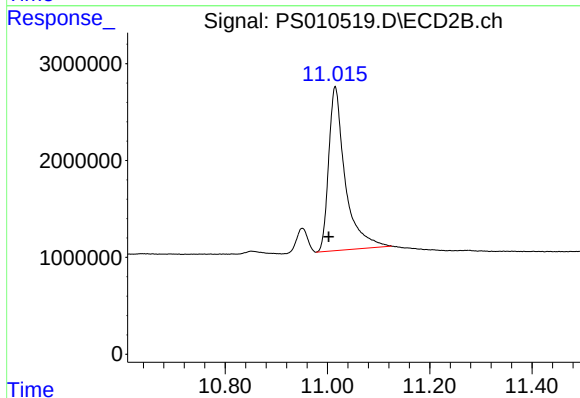


#15 Picloram

R.T.: 11.015 min
Delta R.T.: 0.013 min
Response: 37858073
Conc: 9.18 ng/ml

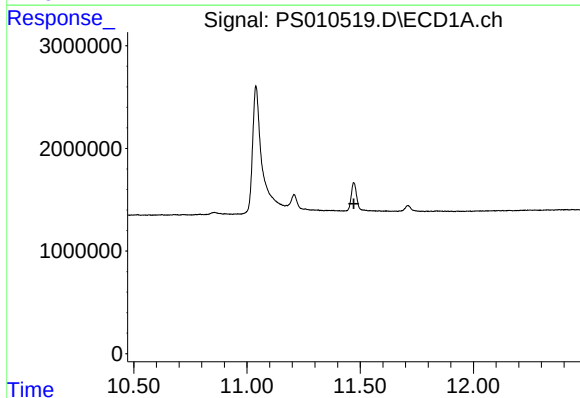

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.472 min
Response: 0
Conc: N.D.

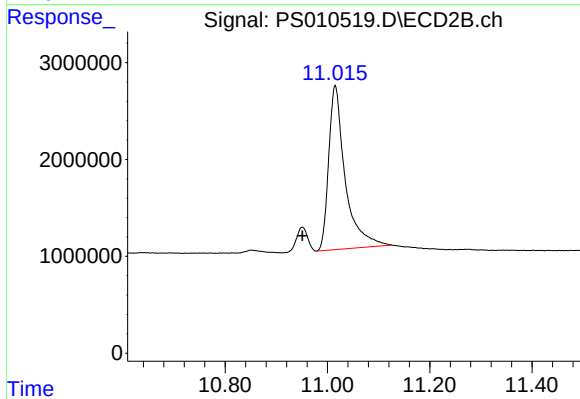

#16 DCPA

R.T.: 11.015 min
Delta R.T.: 0.064 min
Response: 37858073
Conc: 10.21 ng/ml