

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052920\
 Data File : PS010536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 May 2020 19:19
 Operator : DD\AJ
 Sample : L2790-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 23:13:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.921	257.7E6	207.4E6	325.877	380.280
Target Compounds							
1) T	Dalapon	2.999	2.584	40087740	198.3E6	40.773	270.798 #
2) T	3,5-DICHL...	0.000	6.101	0	75950381	N.D.	92.663
5) T	DICAMBA	7.411	7.054	5649356	12333308	1.797	5.479 #
7) T	MCPA	7.683	7.451	150.8E6	166.3E6	43.125	61.177 #
8) T	DICHLORPROP	0.000	7.739	0	8825799	N.D.	15.306
10) T	Pentachlo...	8.713	0.000	9771763	0	<MDL	N.D. #
12) T	2,4,5-T	9.432	0.000	29786081	0	7.324	N.D. #
13) T	2,4-DB	10.005	0.000	4808358	0	8.696	N.D. #
14) T	DINOSEB	0.000	10.067	0	23731015	N.D.	11.030
15) T	Picloram	10.998	0.000	21365519	0	4.185	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052920\
Data File : PS010536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 May 2020 19:19
Operator : DD\AJ
Sample : L2790-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 23:13:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

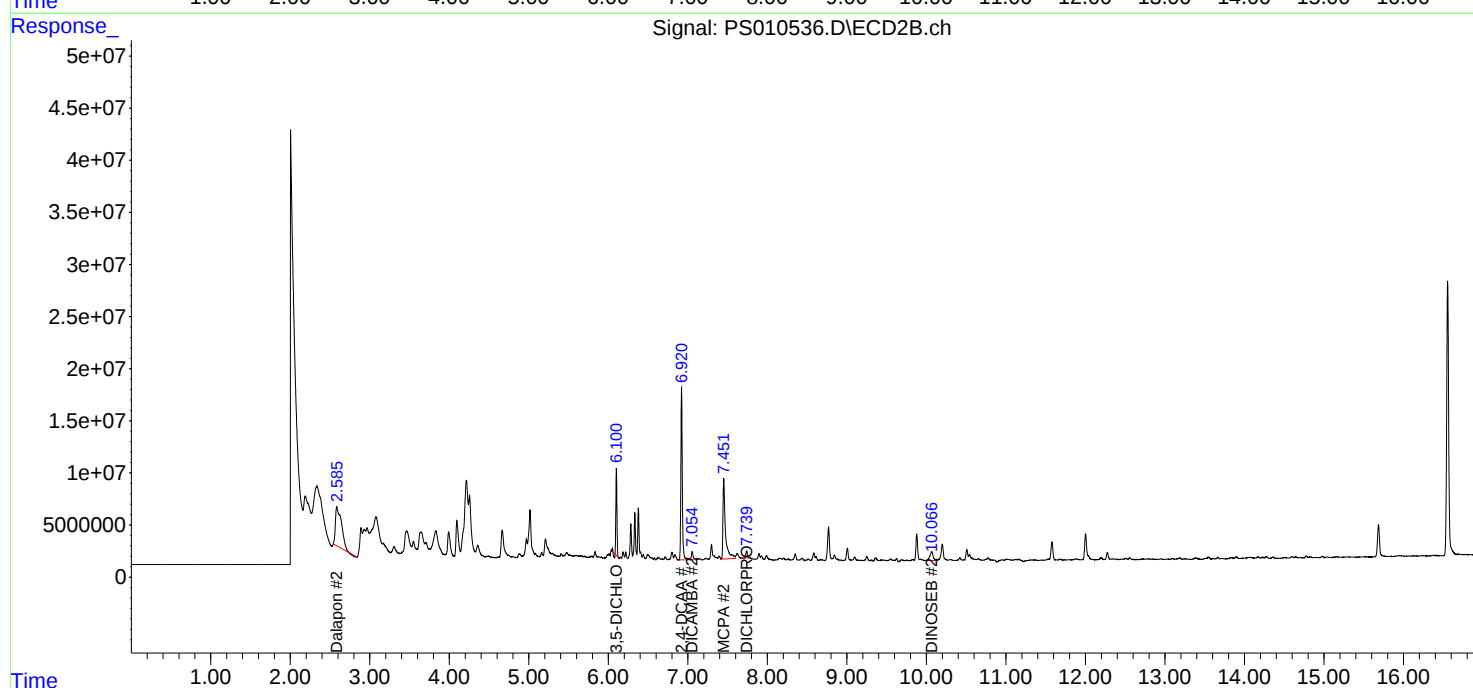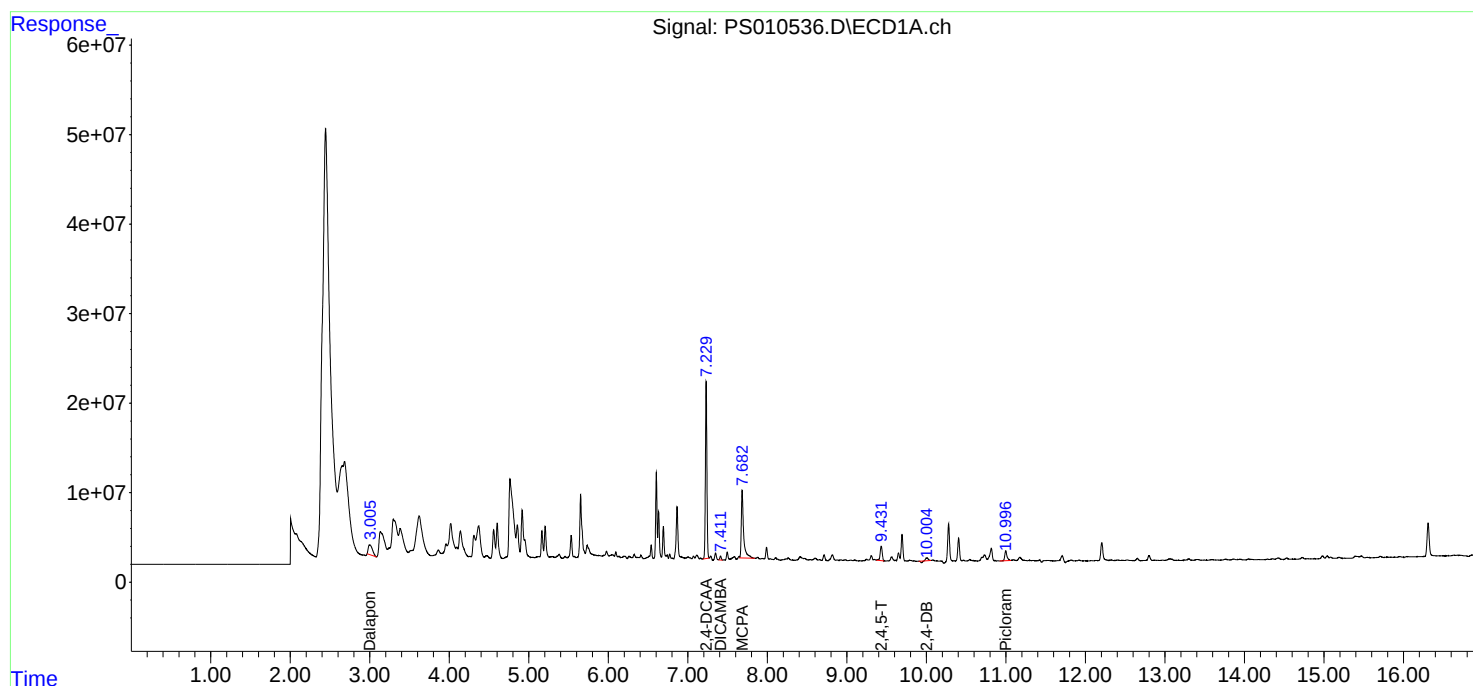


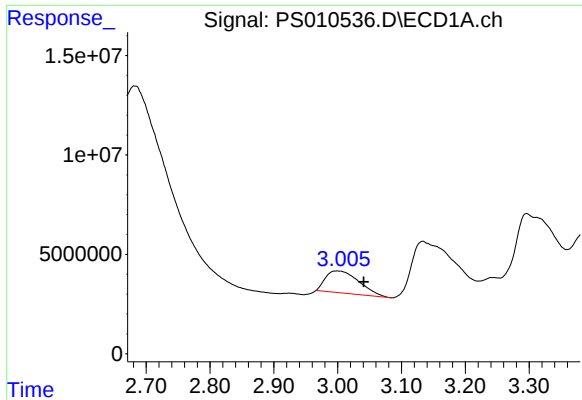

#1 Dalapon


R.T.: 2.999 min
Delta R.T.: -0.042 min
Response: 40087740
Conc: 40.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

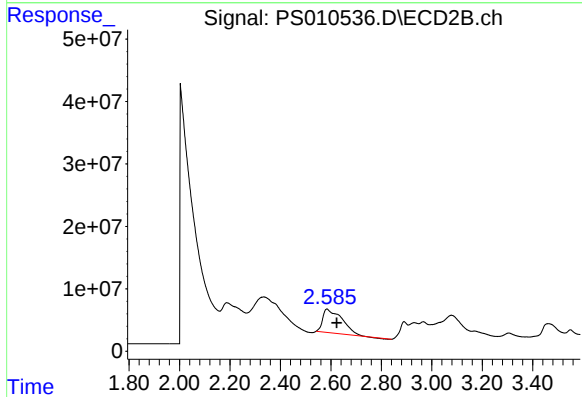


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.039 min
Response: 198263409
Conc: 270.80 ng/ml

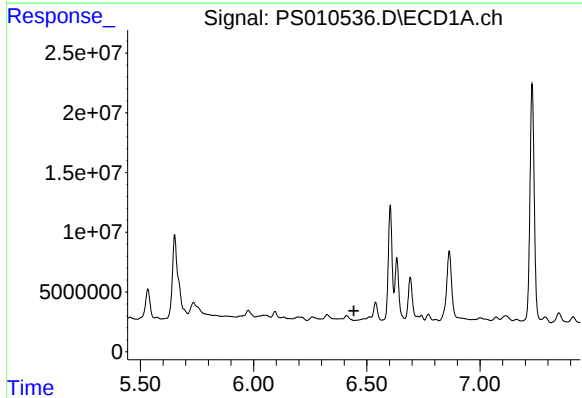


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

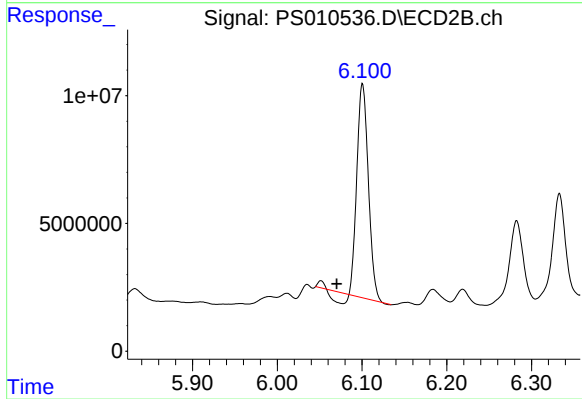

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.101 min
Delta R.T.: 0.030 min
Response: 75950381
Conc: 92.66 ng/ml

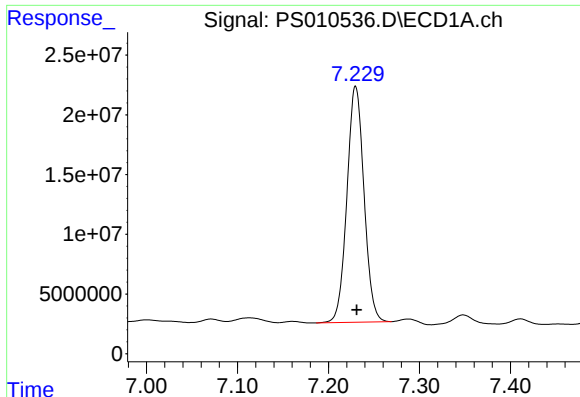

#4 2,4-DCAA


R.T.: 7.230 min
Delta R.T.: -0.001 min
Response: 257723976
Conc: 325.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

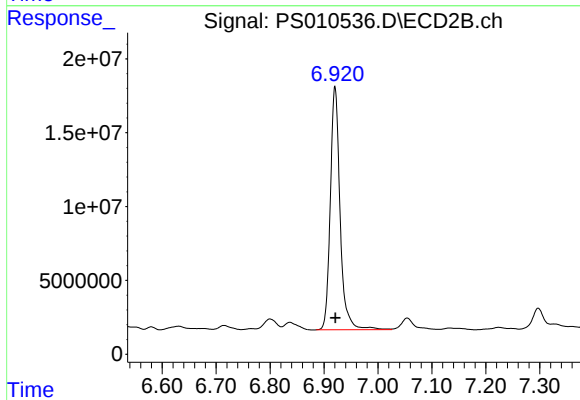


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 207410601
Conc: 380.28 ng/ml

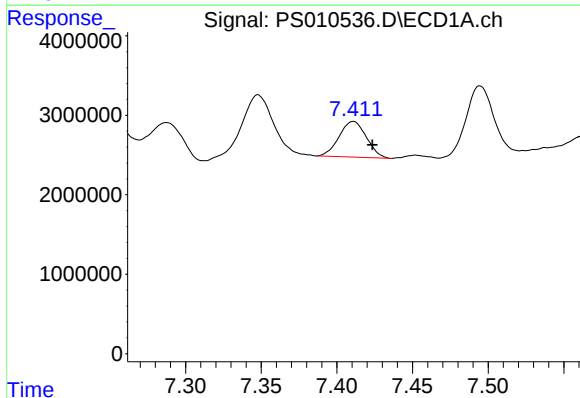


#5 DICAMBA

R.T.: 7.411 min
Delta R.T.: -0.013 min
Response: 5649356
Conc: 1.80 ng/ml

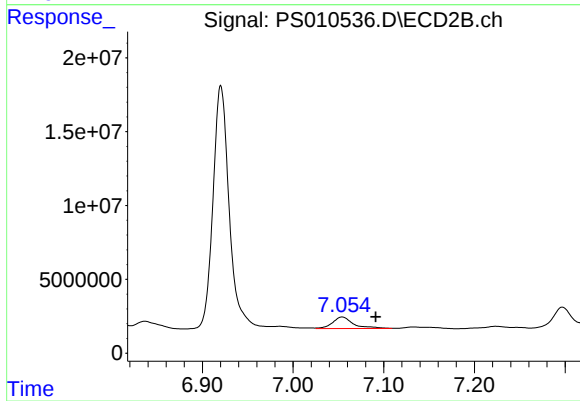

#5 DICAMBA


R.T.: 7.054 min
Delta R.T.: -0.037 min
Response: 12333308
Conc: 5.48 ng/ml

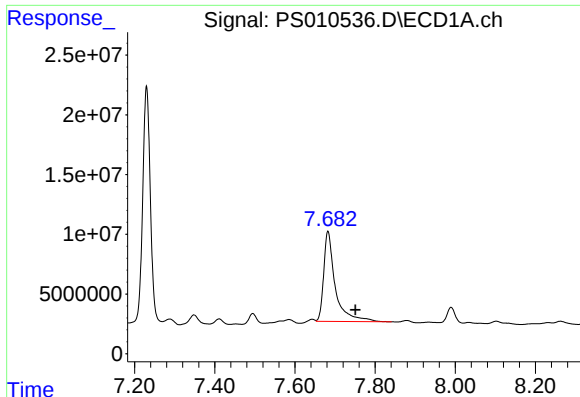

#7 MCPA


R.T.: 7.683 min
Delta R.T.: -0.068 min
Response: 150762809
Conc: 43.12 ug/ml

Instrument :
ECD_S
ClientSampleId :

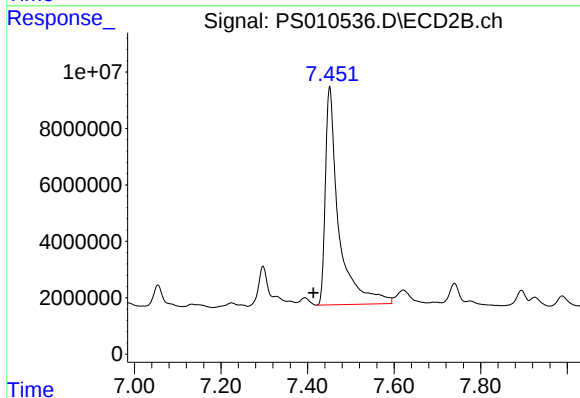


#7 MCPA

R.T.: 7.451 min
Delta R.T.: 0.038 min
Response: 166263721
Conc: 61.18 ug/ml

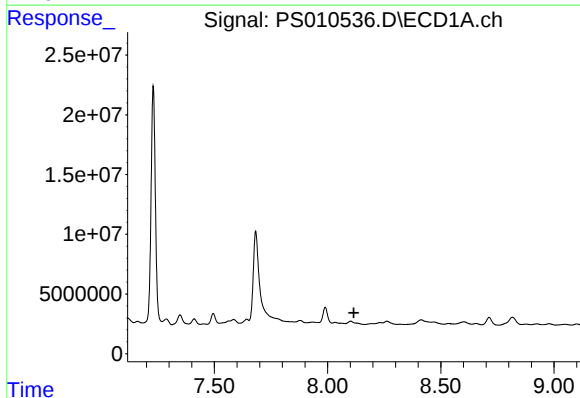


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

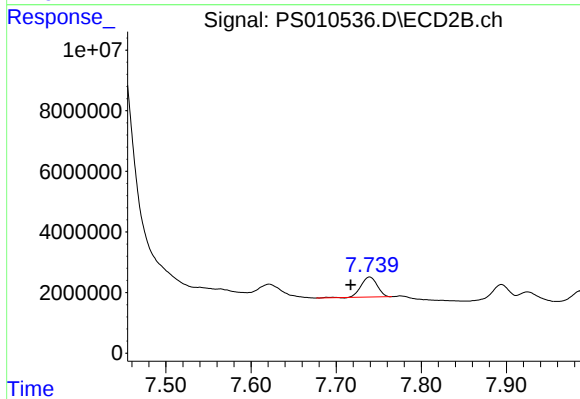

#8 DICHLORPROP


R.T.: 7.739 min
Delta R.T.: 0.022 min
Response: 8825799
Conc: 15.31 ng/ml

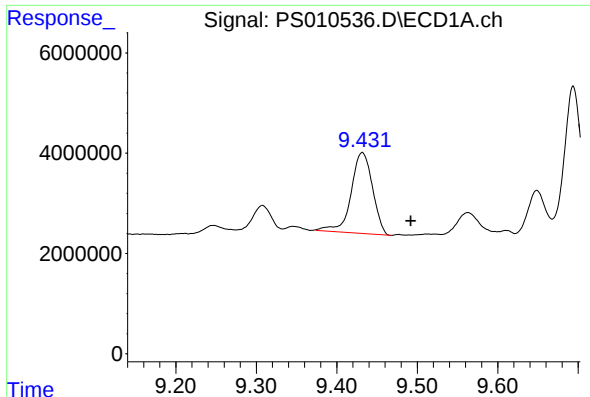

#12 2,4,5-T


R.T.: 9.432 min
Delta R.T.: -0.060 min
Response: 29786081
Conc: 7.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

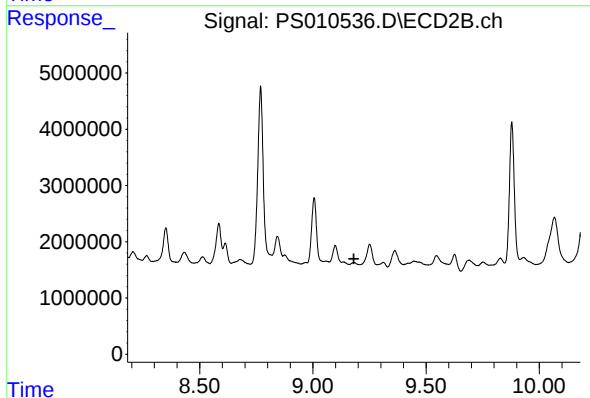


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.181 min
Response: 0
Conc: N.D.

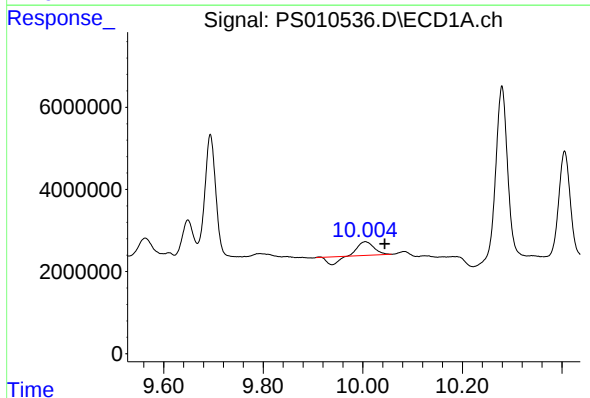


#13 2,4-DB

R.T.: 10.005 min
Delta R.T.: -0.039 min
Response: 4808358
Conc: 8.70 ng/ml

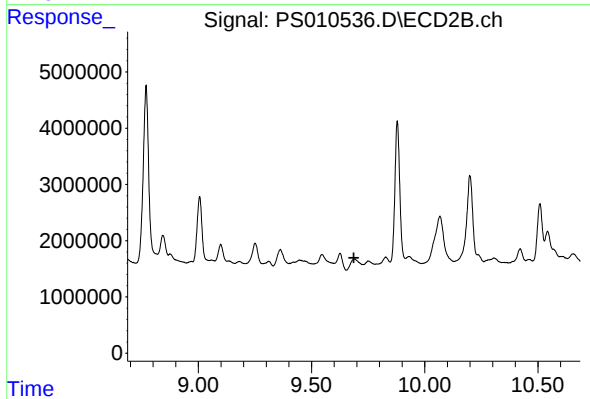

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.687 min
Response: 0
Conc: N.D.

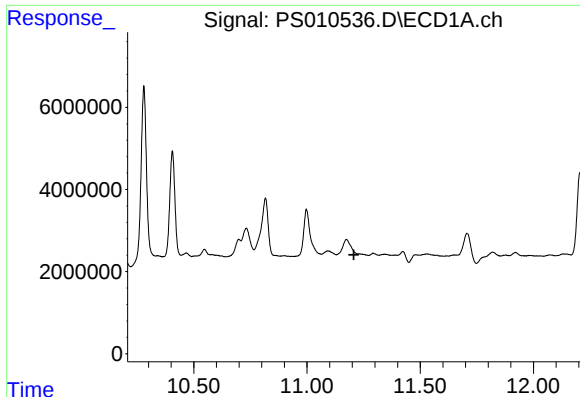

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

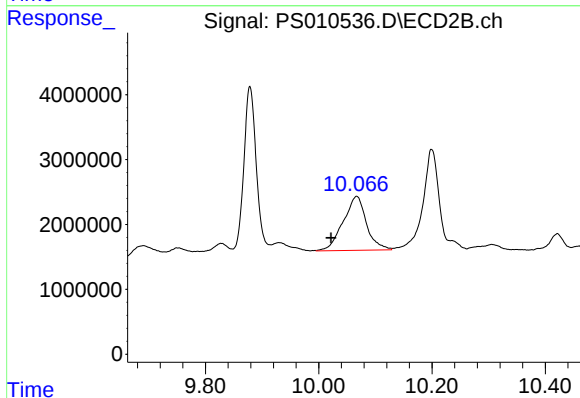


#14 DINOSEB

R.T.: 10.067 min
Delta R.T.: 0.045 min
Response: 23731015
Conc: 11.03 ng/ml

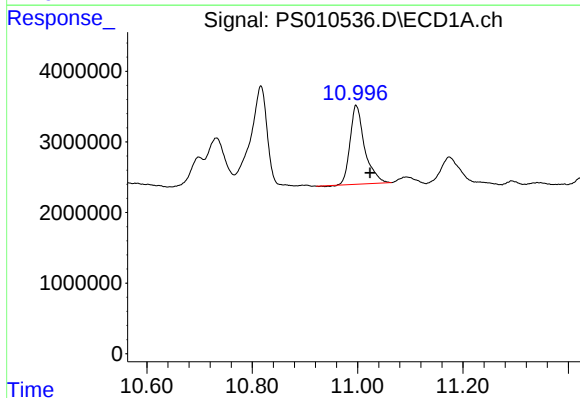

#15 Picloram

R.T.: 10.998 min
Delta R.T.: -0.026 min
Response: 21365519
Conc: 4.19 ng/ml

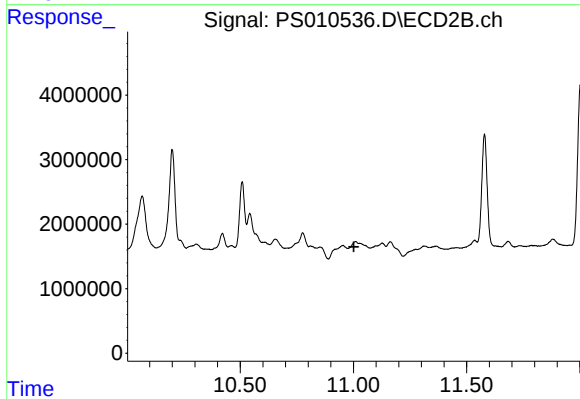

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.002 min
Response: 0
Conc: N.D.