

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053122\
 Data File : PS019562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 13:02
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 16:39:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.205	6.784	949.3E6	369.3E6	395.685	476.598
Target Compounds							
1) T	Dalapon	3.051	0.000	206363	0	<MDL	N.D. #
2) T	3,5-DICHL...	0.000	5.915f	0	514406	N.D.	<MDL
5) T	DICAMBA	0.000	6.972	0	6919456	N.D.	2.024
6) T	MCP	0.000	7.022	0	1544045	N.D.	<MDL
7) T	MCPA	7.666	0.000	1122093	0	<MDL	N.D. #
9) T	2,4-D	8.312	0.000	7566552	0	2.646	N.D. #
10) T	Pentachlo...	8.624	8.286	1082359	1115670	<MDL	<MDL #
11) T	2,4,5-TP ...	9.186	8.653	1440709	373535	<MDL	<MDL #
12) T	2,4,5-T	9.430	9.059	11556256	668406	<MDL	<MDL #
13) T	2,4-DB	9.989	9.474f	1284748	886144	<MDL	1.434 #
14) T	DINOSEB	0.000	9.855	0	984106	N.D.	<MDL
15) T	Picloram	10.983	10.892f	1034437	12563367	<MDL	1.953 #
16) T	DCPA	11.426	10.780	6542970	1607270	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053122\
Data File : PS019562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 13:02
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 16:39:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

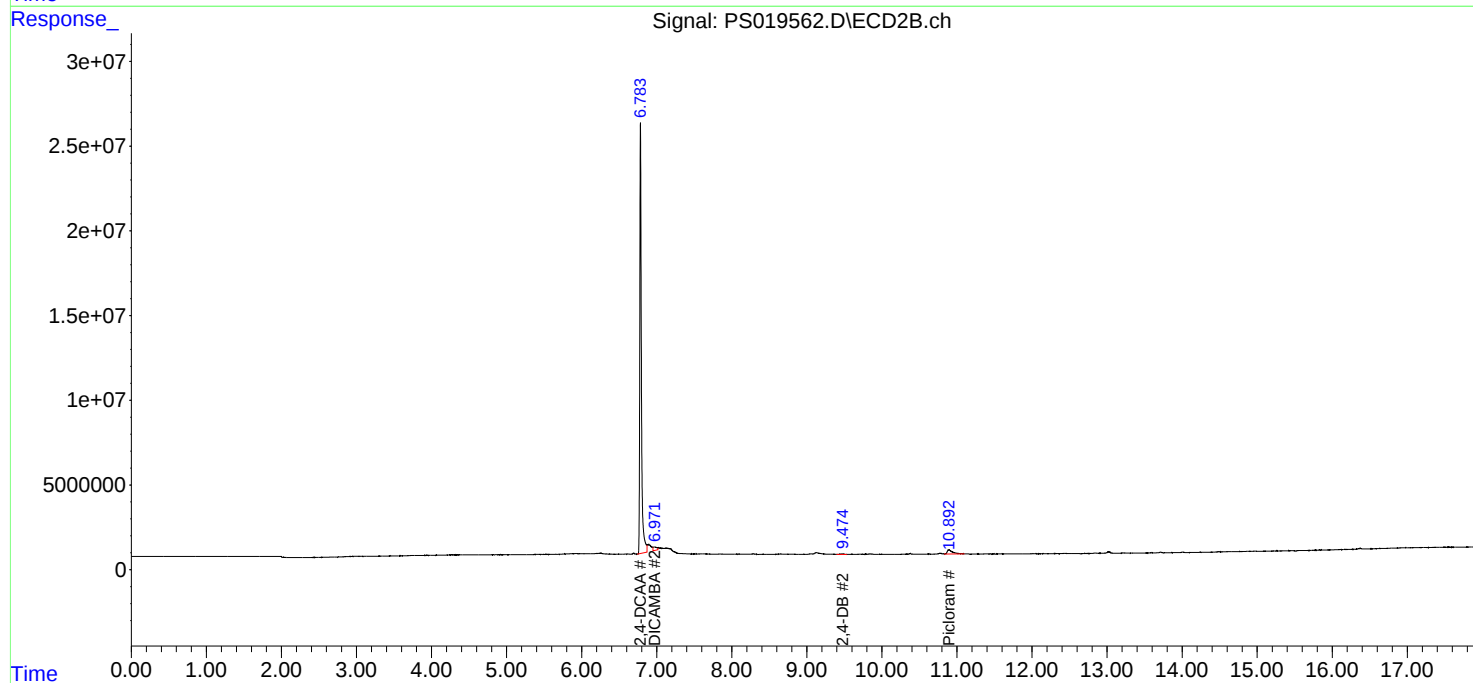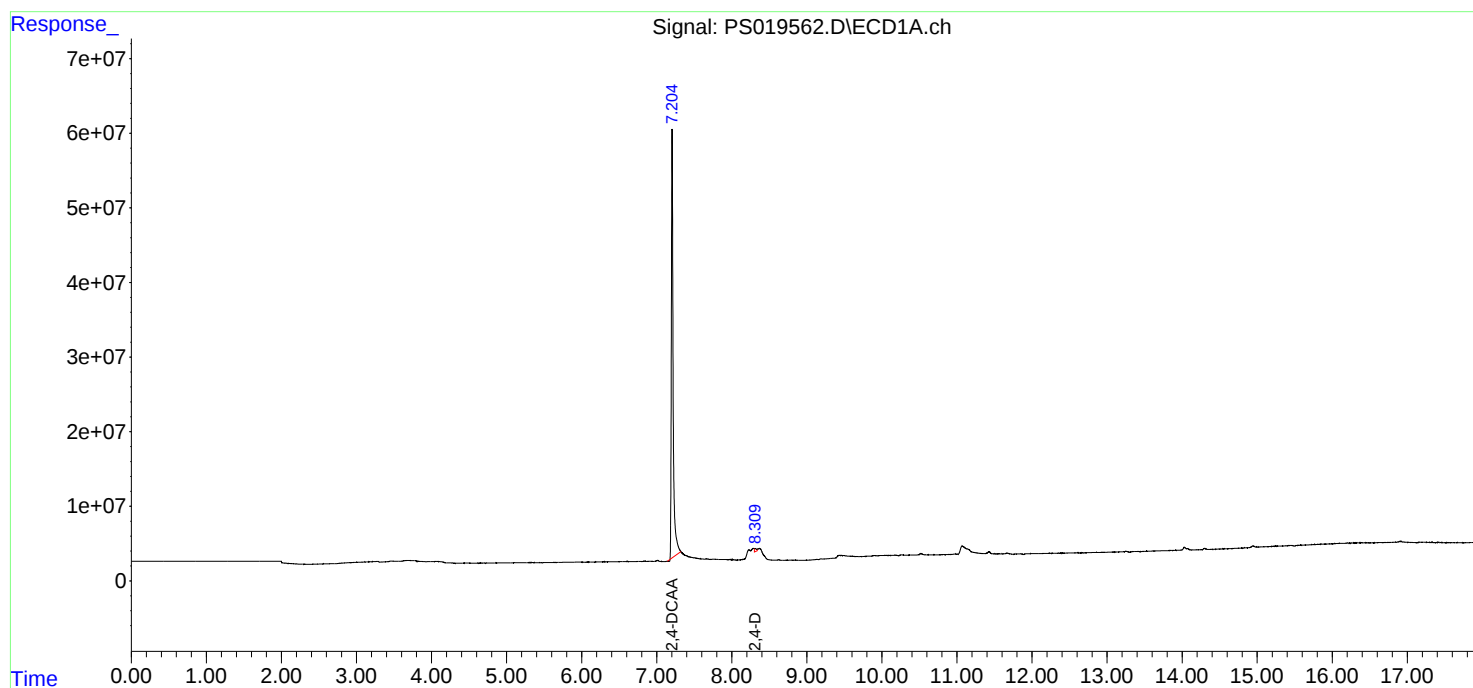


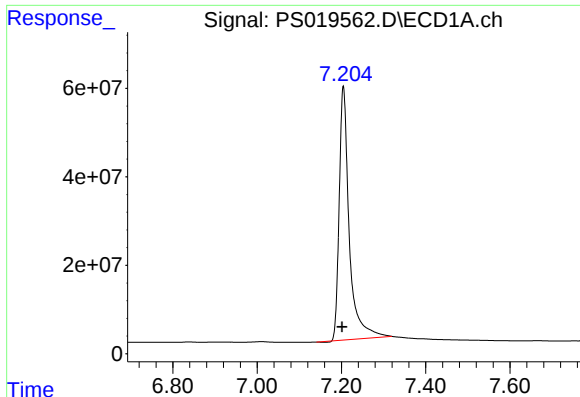

#4 2,4-DCAA


R.T.: 7.205 min
Delta R.T.: 0.003 min
Response: 949314141
Conc: 395.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

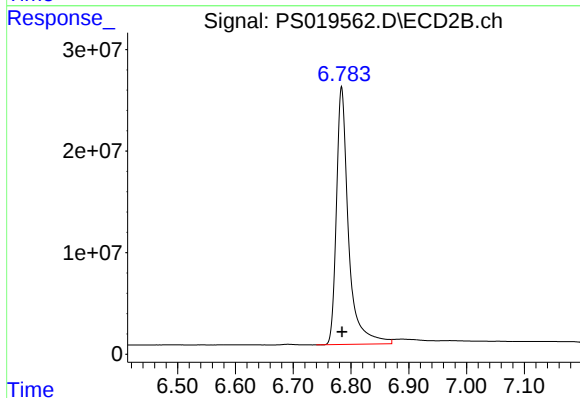


#4 2,4-DCAA

R.T.: 6.784 min
Delta R.T.: 0.000 min
Response: 369301813
Conc: 476.60 ng/ml

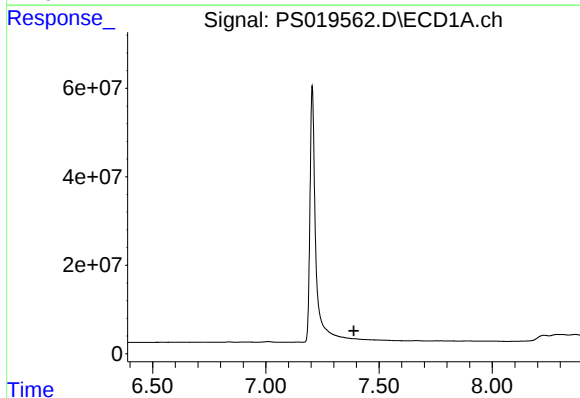


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.388 min
Response: 0
Conc: N.D.

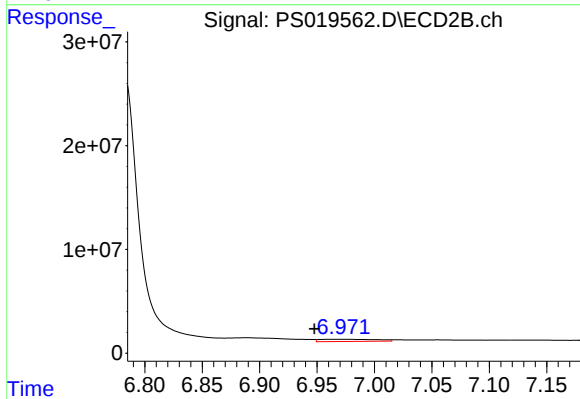

#5 DICAMBA


R.T.: 6.972 min
Delta R.T.: 0.024 min
Response: 6919456
Conc: 2.02 ng/ml

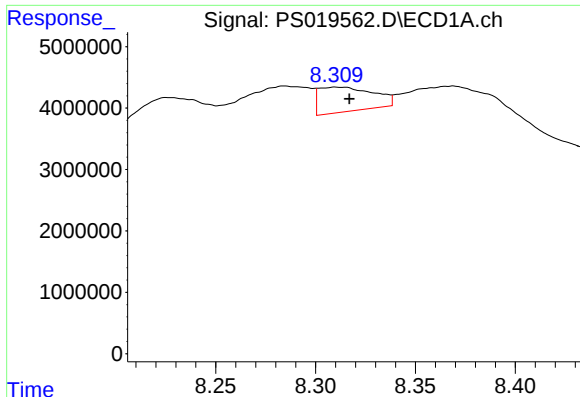

#9 2,4-D


R.T.: 8.312 min
Delta R.T.: -0.005 min
Response: 7566552
Conc: 2.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

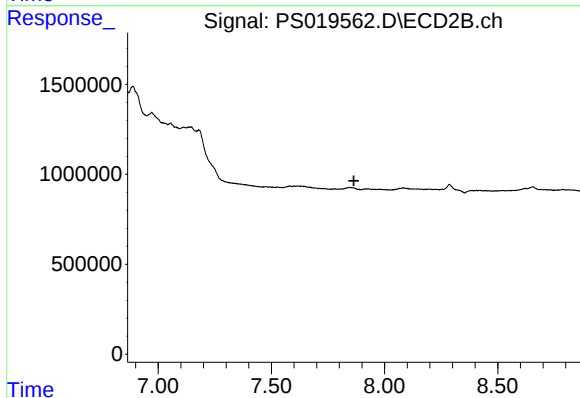


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.864 min
Response: 0
Conc: N.D.

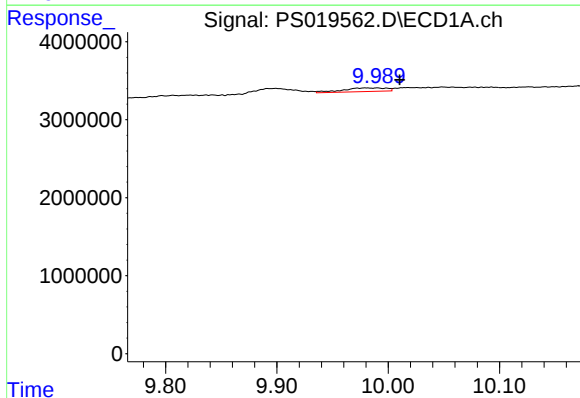


#13 2,4-DB

R.T.: 9.989 min
Delta R.T.: -0.022 min
Response: 1284748
Conc: N.D.

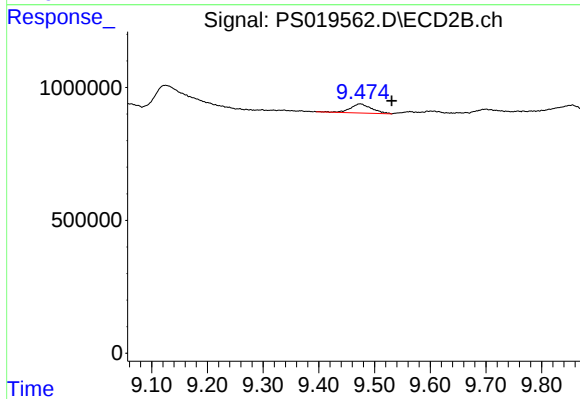

#13 2,4-DB


R.T.: 9.474 min
Delta R.T.: -0.057 min
Response: 886144
Conc: 1.43 ng/ml

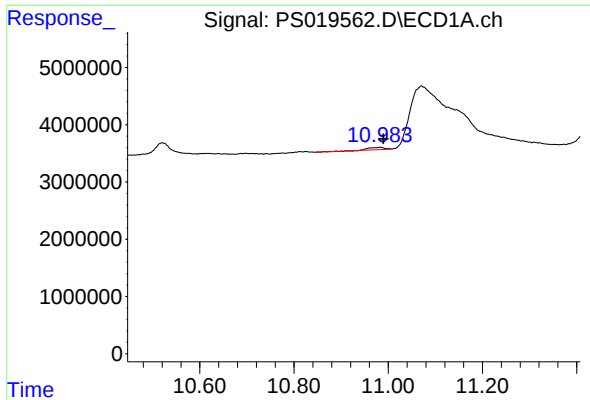

#15 Picloram

R.T.: 10.983 min
Delta R.T.: -0.007 min
Response: 1034437
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

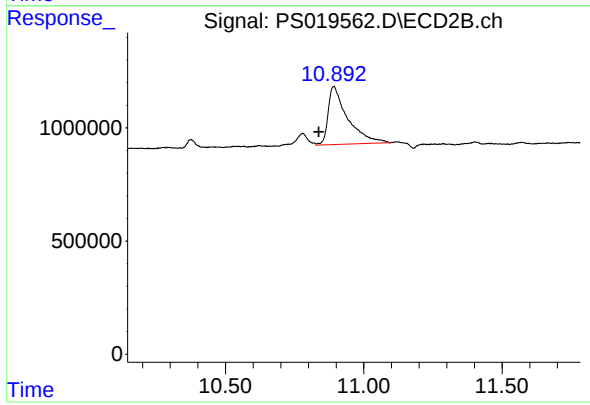

#15 Picloram

R.T.: 10.892 min
Delta R.T.: 0.054 min
Response: 12563367
Conc: 1.95 ng/ml