

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053122\
 Data File : PS019569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 15:52
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 17:13:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.199	6.783	1029.0E6	391.9E6	428.897	505.824
Target Compounds							
1) T	Dalapon	2.991	0.000	688121	0	<MDL	N.D. #
6) T	MCP	7.508f	0.000	147365	0	<MDL	N.D. #
7) T	MCPA	7.689	0.000	802498	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.616f	0	755641	N.D.	<MDL
9) T	2,4-D	0.000	7.834	0	262592	N.D.	<MDL
10) T	Pentachlo...	8.617	8.285	391385	1924246	<MDL	<MDL #
11) T	2,4,5-TP ...	9.134	8.645	1256858	254405	<MDL	<MDL #
12) T	2,4,5-T	9.477	9.040	3474783	1474485	<MDL	<MDL #
13) T	2,4-DB	9.994	9.466f	2338200	1749826	<MDL	2.832 #
14) T	DINOSEB	11.162	9.857	3775147	2265	<MDL	<MDL #
15) T	Picloram	10.975	10.863	2286440	6607751	<MDL	1.027 #
16) T	DCPA	11.432	10.782	3117403	637399	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053122\
Data File : PS019569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 15:52
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 17:13:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

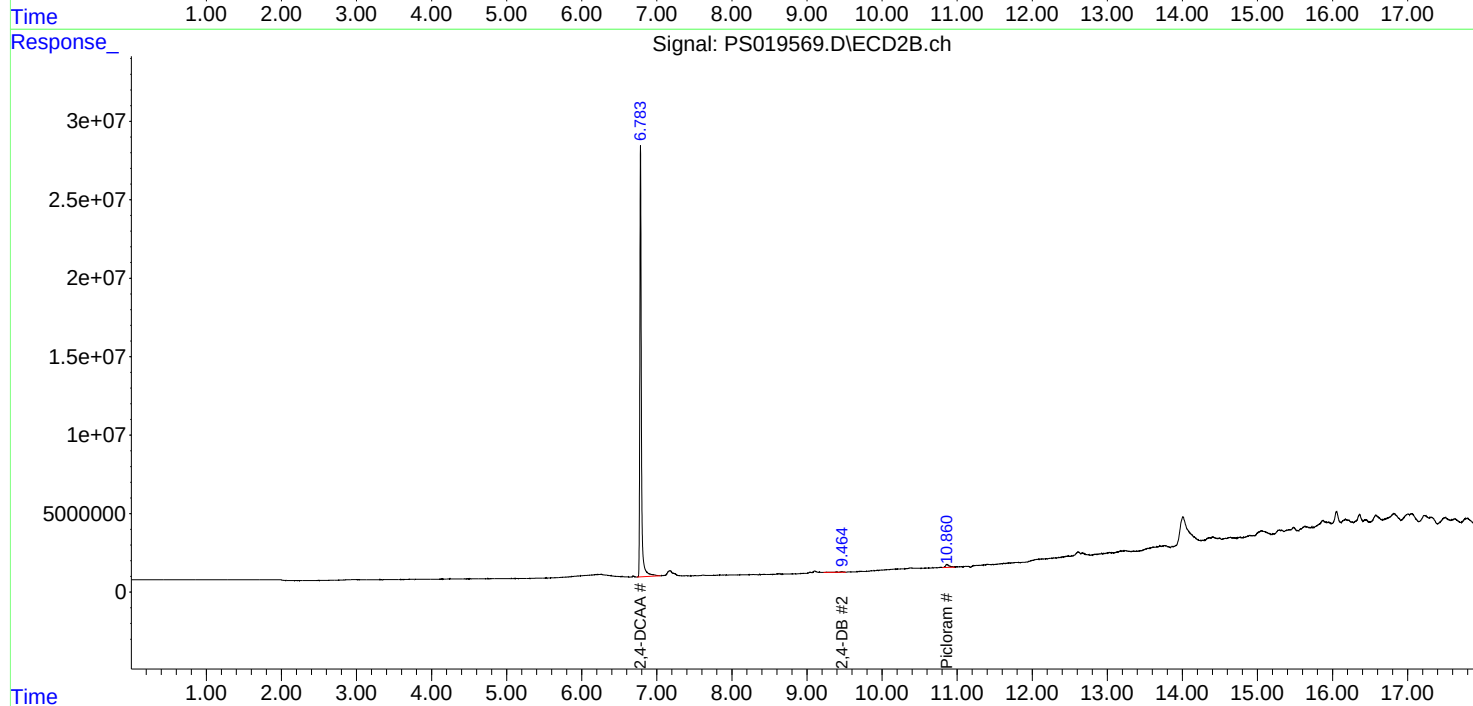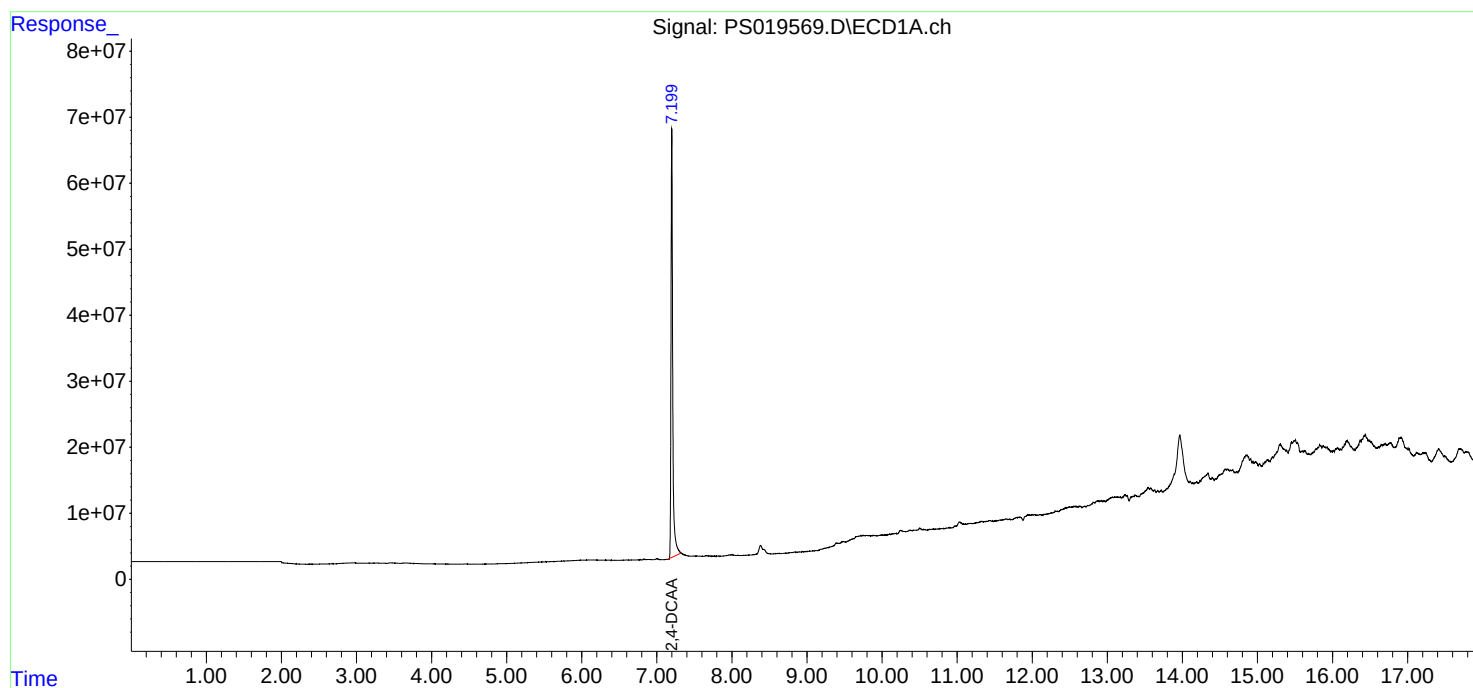


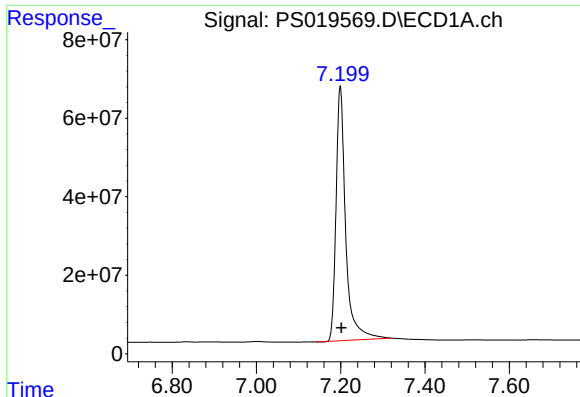

#4 2,4-DCAA


R.T.: 7.199 min
Delta R.T.: -0.003 min
Response: 1028994598
Conc: 428.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

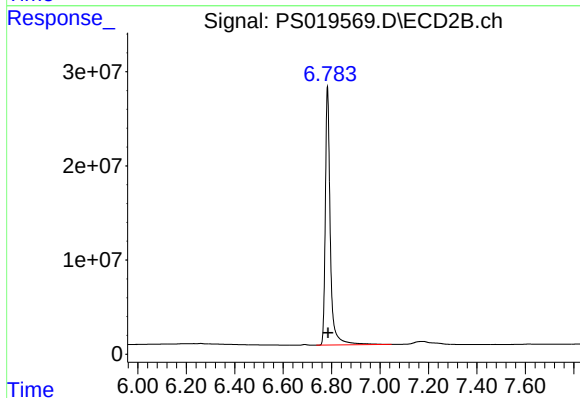


#4 2,4-DCAA

R.T.: 6.783 min
Delta R.T.: -0.002 min
Response: 391947714
Conc: 505.82 ng/ml

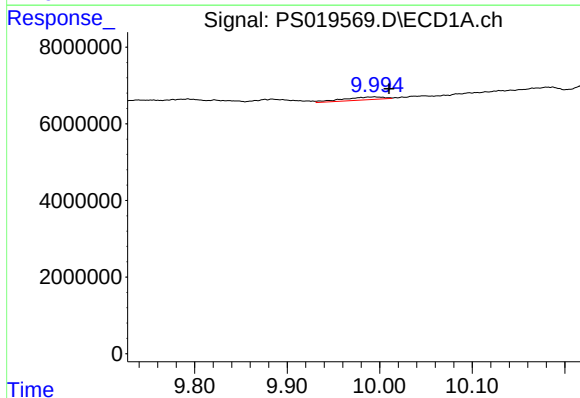


#13 2,4-DB

R.T.: 9.994 min
Delta R.T.: -0.016 min
Response: 2338200
Conc: N.D.

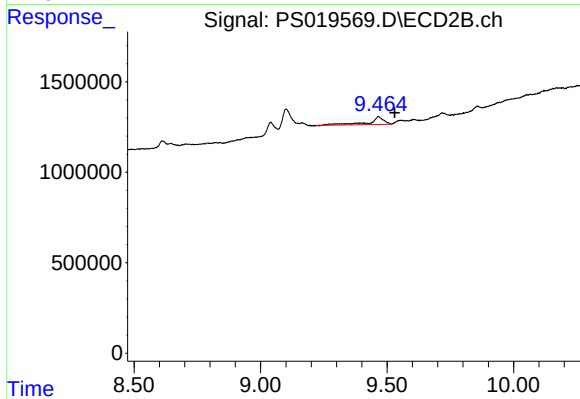

#13 2,4-DB


R.T.: 9.466 min
Delta R.T.: -0.065 min
Response: 1749826
Conc: 2.83 ng/ml

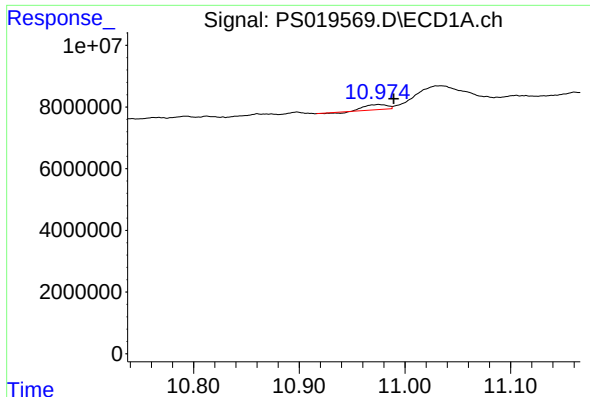

#15 Picloram

R.T.: 10.975 min
Delta R.T.: -0.015 min
Response: 2286440
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

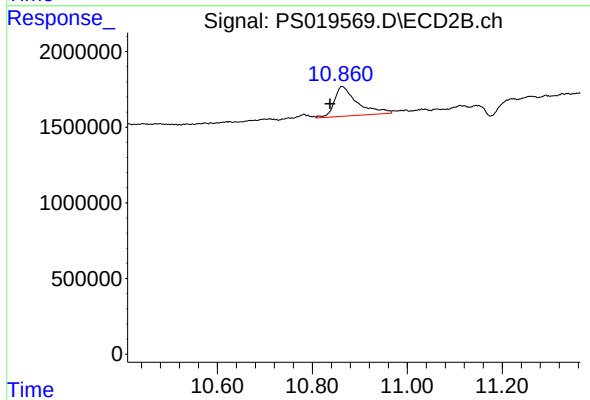

#15 Picloram

R.T.: 10.863 min
Delta R.T.: 0.025 min
Response: 6607751
Conc: 1.03 ng/ml