

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053122\
 Data File : PS019576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 May 2022 19:29
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 01:14:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.200	6.784	1008.5E6	396.6E6	420.349	511.792
Target Compounds							
1) T	Dalapon	3.046	0.000	194868	0	<MDL	N.D. #
7) T	MCPA	7.659f	7.182f	728444	7725746	<MDL	2.011 #
8) T	DICHLORPROP	0.000	7.630f	0	261691	N.D.	<MDL
10) T	Pentachlo...	8.619	8.285	650270	923114	<MDL	<MDL #
11) T	2,4,5-TP ...	9.130	8.650	1035000	217540	<MDL	<MDL #
12) T	2,4,5-T	9.430	9.054	5461000	228293	<MDL	<MDL #
13) T	2,4-DB	10.028	9.471f	2671253	676845	<MDL	1.095 #
14) T	DINOSEB	11.151	0.000	5552003	0	<MDL	N.D. #
15) T	Picloram	10.980	10.882f	6321667	4391264	<MDL	<MDL #
16) T	DCPA	11.427	10.784	1578661	441489	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS053122\
Data File : PS019576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 May 2022 19:29
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 01:14:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

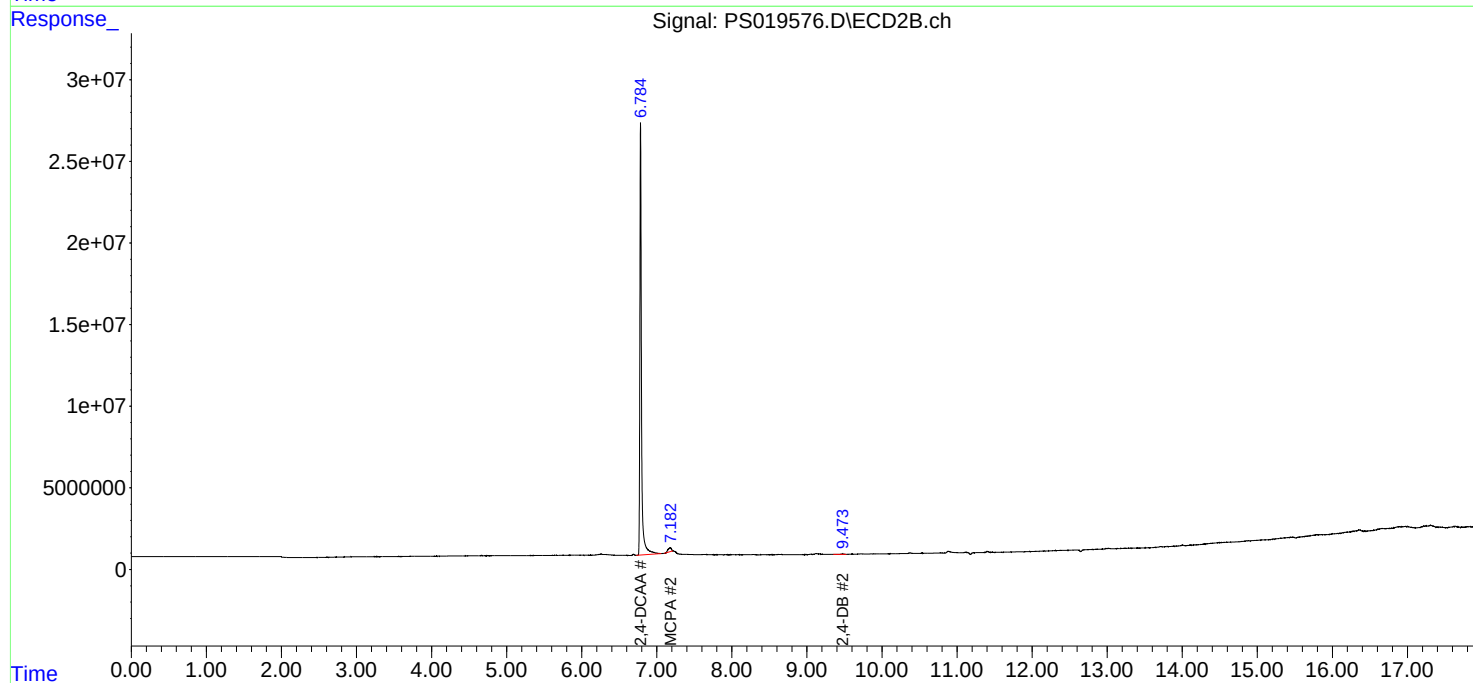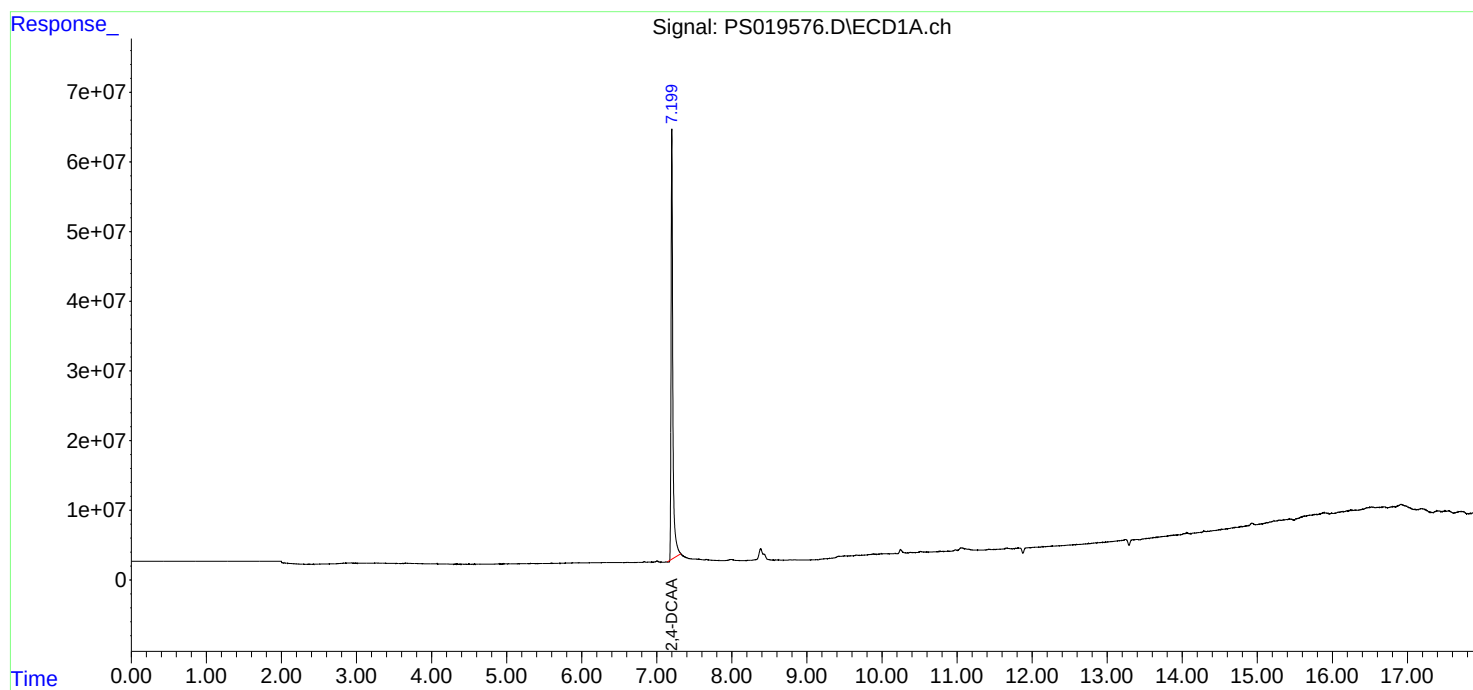


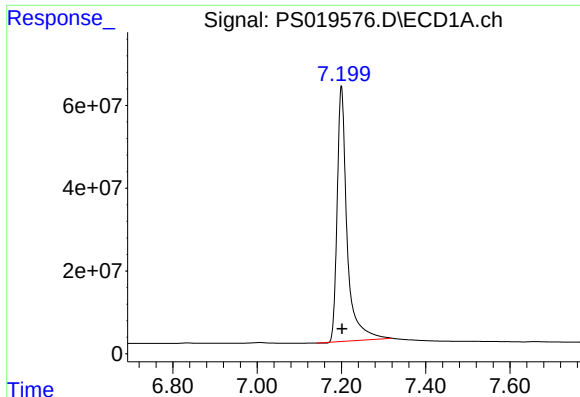

#4 2,4-DCAA


R.T.: 7.200 min
Delta R.T.: -0.002 min
Response: 1008488510
Conc: 420.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

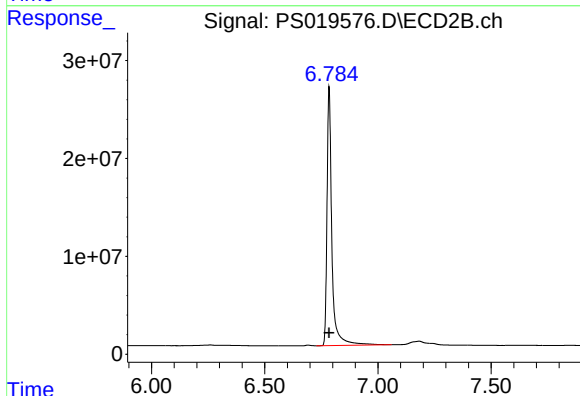


#4 2,4-DCAA

R.T.: 6.784 min
Delta R.T.: 0.000 min
Response: 396572675
Conc: 511.79 ng/ml

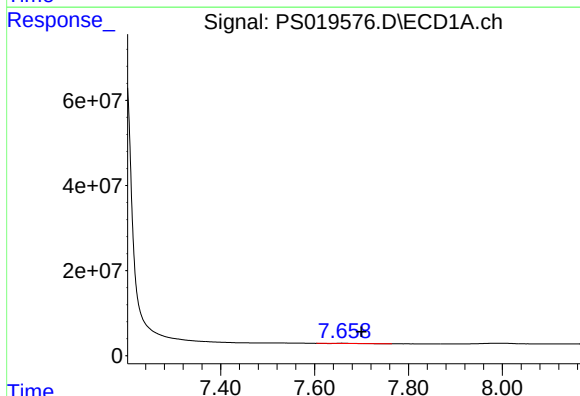


#7 MCPA

R.T.: 7.659 min
Delta R.T.: -0.040 min
Response: 728444
Conc: N.D.

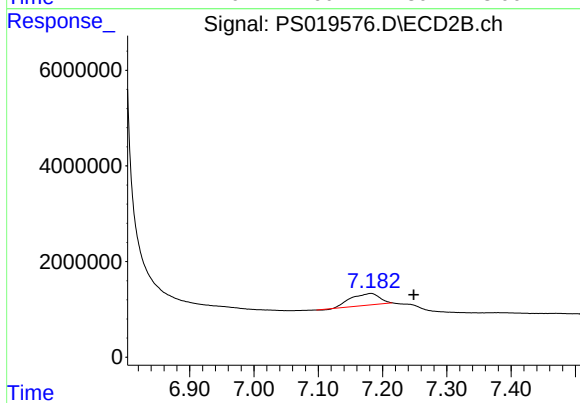

#7 MCPA


R.T.: 7.182 min
Delta R.T.: -0.067 min
Response: 7725746
Conc: 2.01 ug/ml

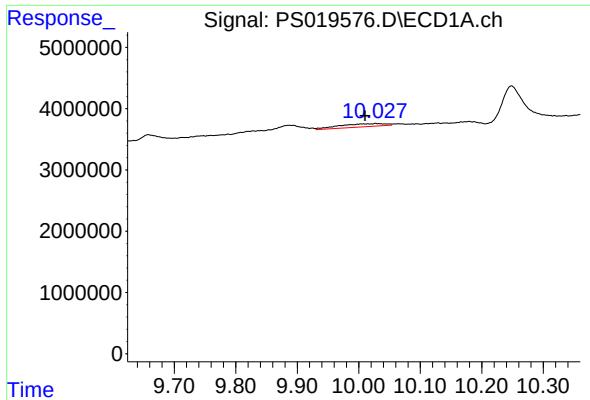

#13 2,4-DB

R.T.: 10.028 min
Delta R.T.: 0.018 min
Response: 2671253
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

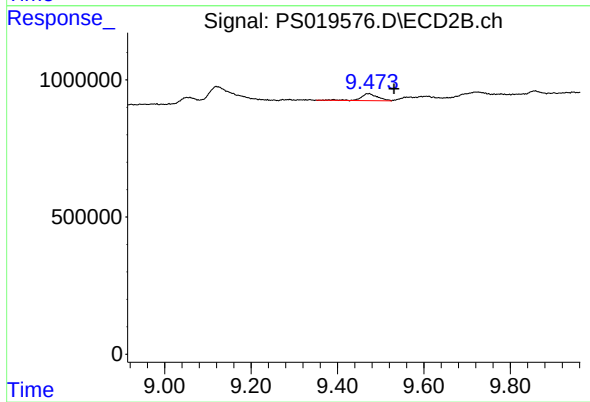

#13 2,4-DB

R.T.: 9.471 min
Delta R.T.: -0.060 min
Response: 676845
Conc: 1.10 ng/ml