

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
 Data File : PS010545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2020 10:27
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 12:30:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds							
2) T	3,5-DICHL...	6.485	0.000	17975088	0	16.442	N.D. #
5) T	DICAMBA	0.000	7.155	0	10589188	N.D.	4.705
6) T	MCP	0.000	7.155	0	10589188	N.D.	5.682
9) T	2,4-D	0.000	7.941	0	1319.2E6	N.D.	1739.840
12) T	2,4,5-T	0.000	9.244	0	7577478	N.D.	2.525
15) T	Picloram	11.036	11.013	19346793	22836203	3.790	5.535 #
16) T	DCPA	0.000	11.013	0	22836203	N.D.	6.158


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
Data File : PS010545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2020 10:27
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 12:30:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

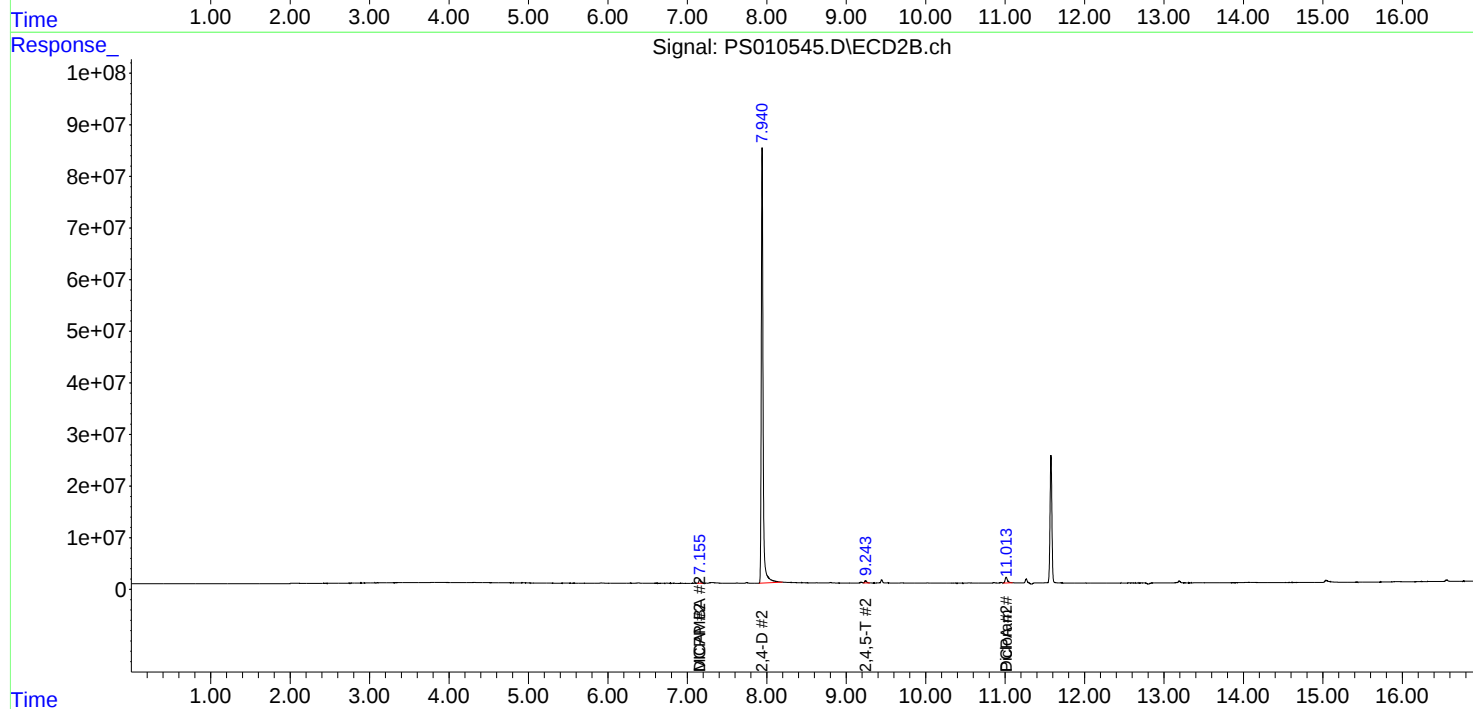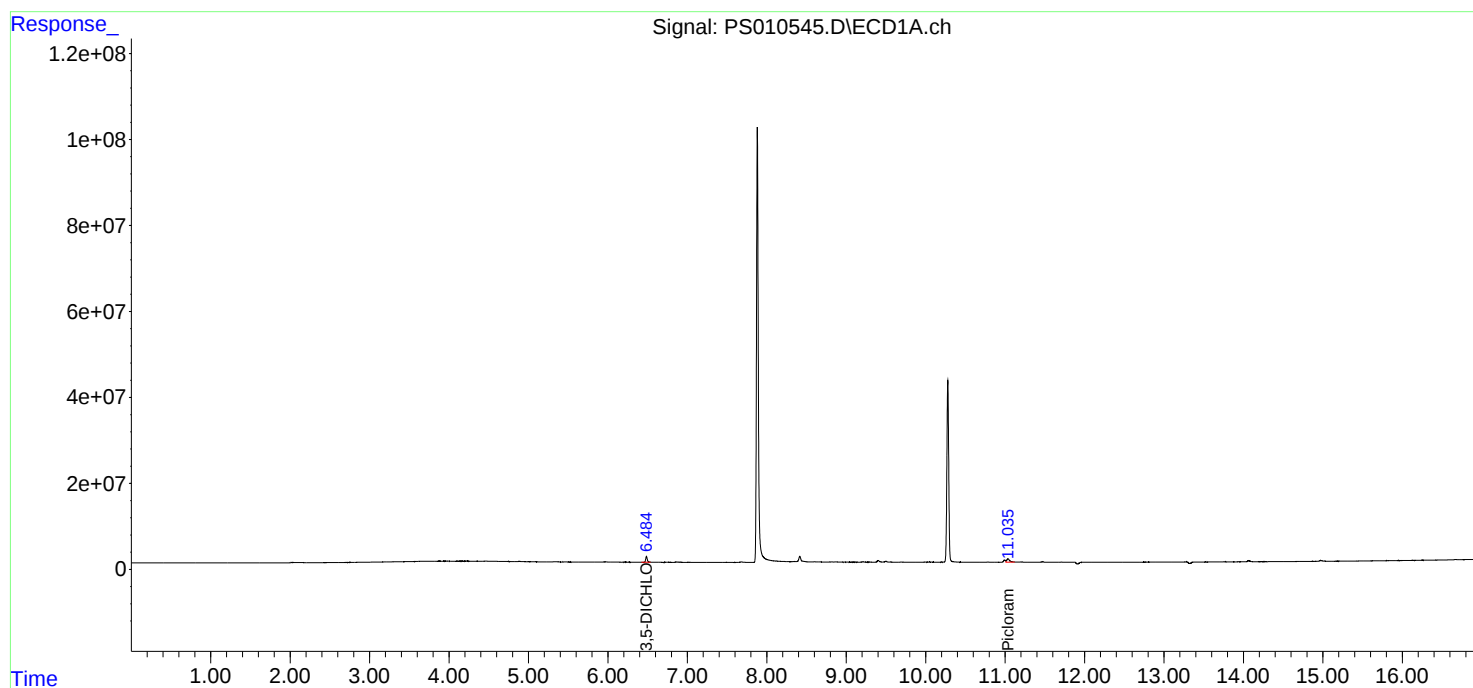

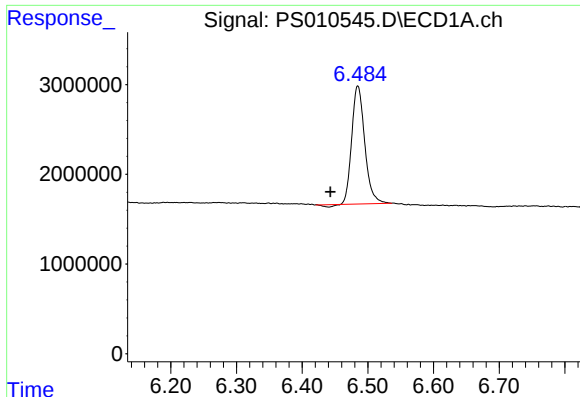


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.485 min
Delta R.T.: 0.042 min
Response: 17975088
Conc: 16.44 ng/ml

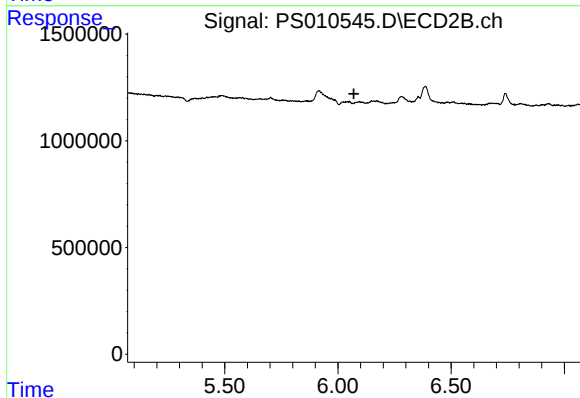


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.070 min
Response: 0
Conc: N.D.

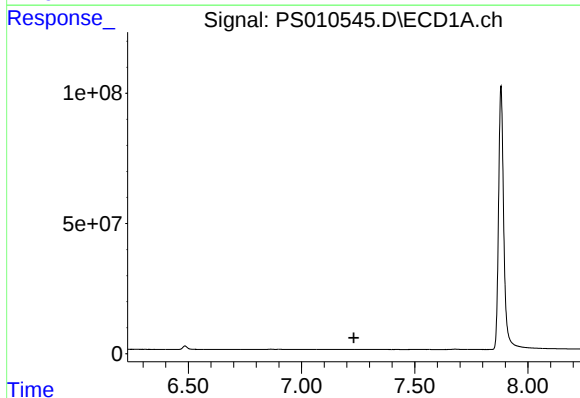


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.231 min
Response: 0
Conc: N.D.

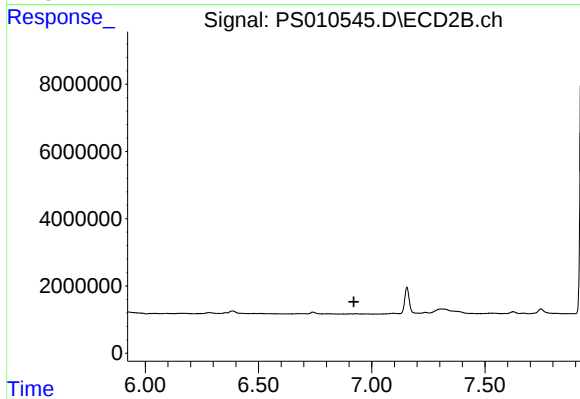


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.921 min
Response: 0
Conc: N.D.

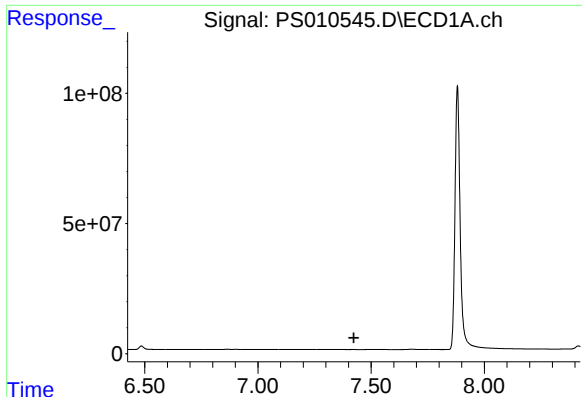


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.423 min
Response: 0
Conc: N.D.

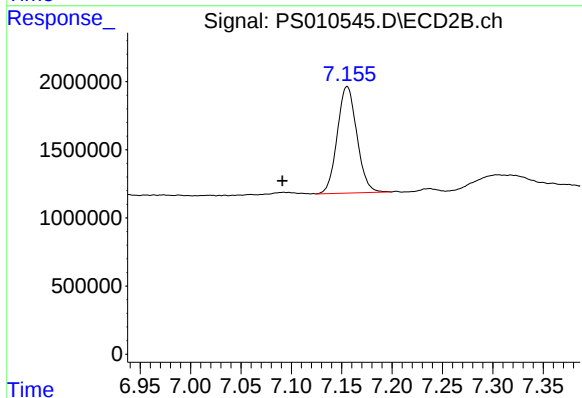


#5 DICAMBA

R.T.: 7.155 min
Delta R.T.: 0.064 min
Response: 10589188
Conc: 4.70 ng/ml

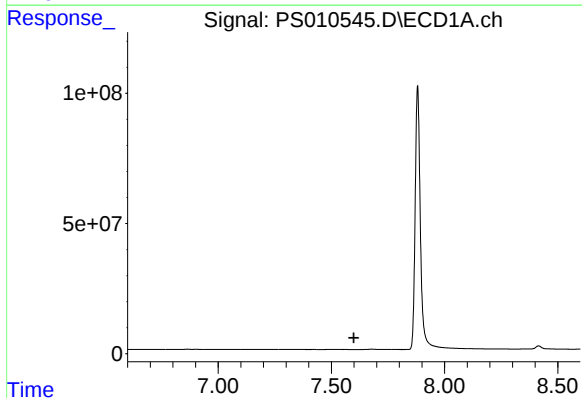


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.600 min
Response: 0
Conc: N.D.

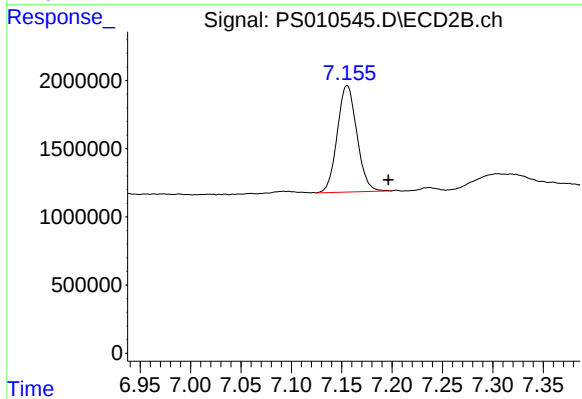


#6 MCP

R.T.: 7.155 min
Delta R.T.: -0.041 min
Response: 10589188
Conc: 5.68 ug/ml

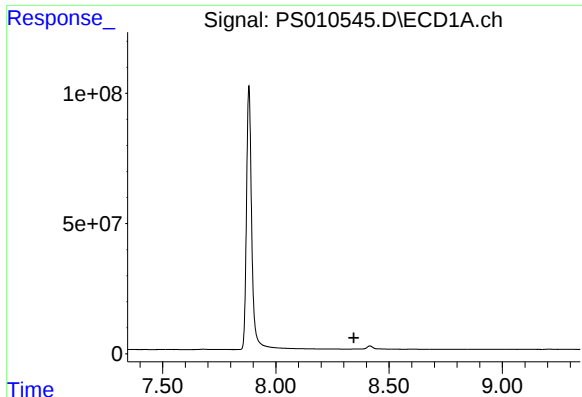


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.345 min
Response: 0
Conc: N.D.

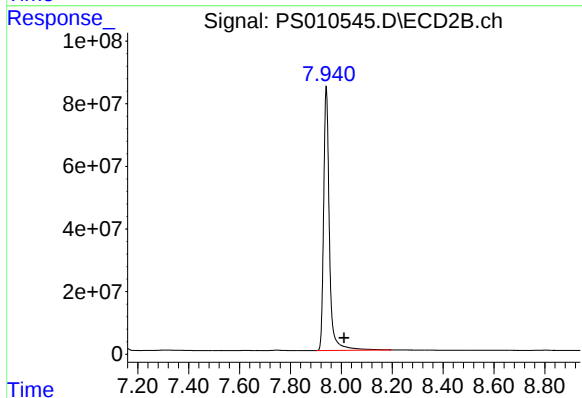


#9 2,4-D

R.T.: 7.941 min
Delta R.T.: -0.070 min
Response: 1319243467
Conc: 1739.84 ng/ml

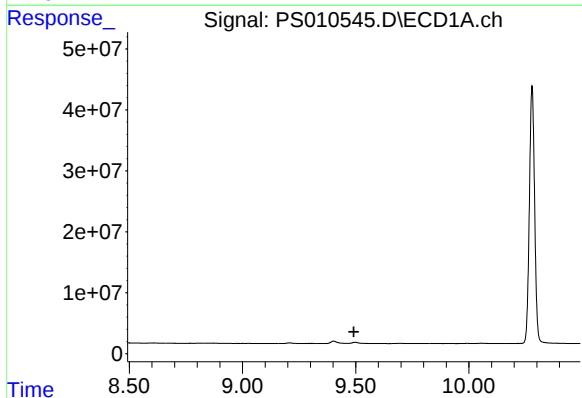


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.492 min
Response: 0
Conc: N.D.

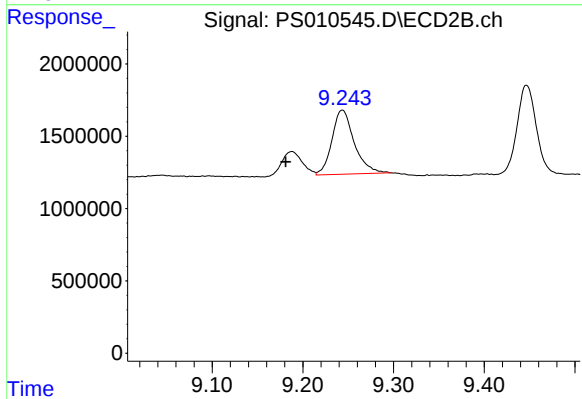


#12 2,4,5-T

R.T.: 9.244 min
Delta R.T.: 0.062 min
Response: 7577478
Conc: 2.53 ng/ml

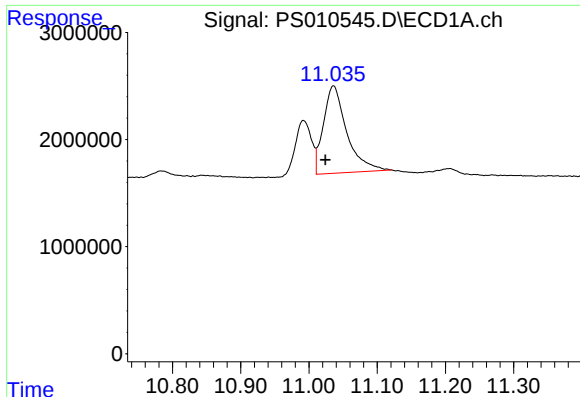


#15 Picloram

R.T.: 11.036 min
Delta R.T.: 0.012 min
Response: 19346793
Conc: 3.79 ng/ml

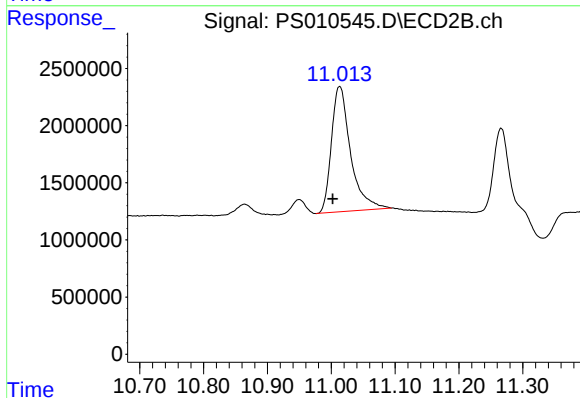


#15 Picloram

R.T.: 11.013 min
Delta R.T.: 0.011 min
Response: 22836203
Conc: 5.53 ng/ml

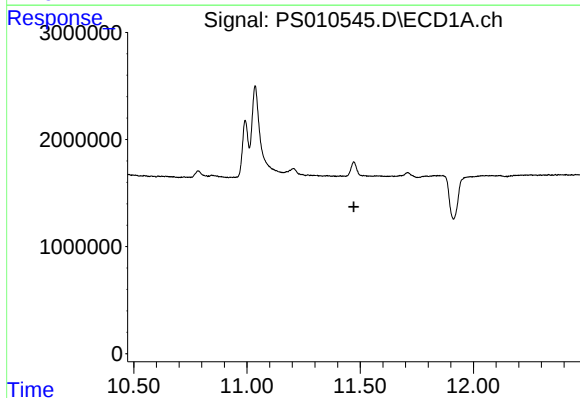

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.472 min
Response: 0
Conc: N.D.

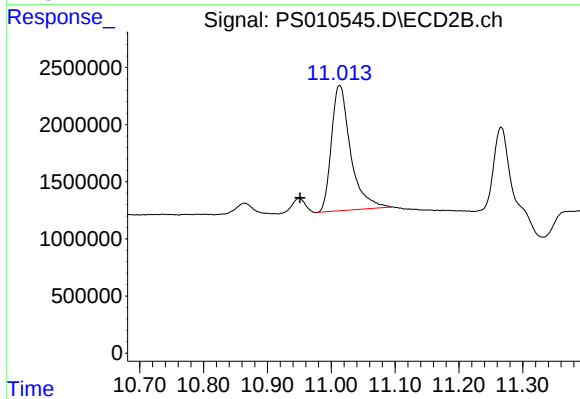

#16 DCPA

R.T.: 11.013 min
Delta R.T.: 0.062 min
Response: 22836203
Conc: 6.16 ng/ml