

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
 Data File : PS010581.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2020 00:12
 Operator : DD\AJ
 Sample : L2814-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 06:47:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
 Quant Title : 8080.M
 QLast Update : Fri May 29 15:43:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.230	6.920	296.3E6	233.0E6	374.602	427.250
Target Compounds							
1) T	Dalapon	2.998	2.586	38555683	116.4E6	39.215	158.966 #
2) T	3,5-DICHL...	0.000	6.100	0	59272700	N.D.	72.315
3) T	4-Nitroph...	7.118	0.000	5928756	0	15.992	N.D. #
5) T	DICAMBA	0.000	7.053	0	15125377	N.D.	6.720
6) T	MCPD	7.637	0.000	2140373	0	<MDL	N.D. #
7) T	MCPA	0.000	7.402	0	6194062	N.D.	2.279
8) T	DICHLORPROP	0.000	7.738	0	12204368	N.D.	21.165
10) T	Pentachlo...	8.713	8.437	7215770	8243962	<MDL	1.160 #
12) T	2,4,5-T	9.432	0.000	39417592	0	9.692	N.D. #
13) T	2,4-DB	10.009	0.000	12984754	0	23.484	N.D. #
14) T	DINOSEB	0.000	10.065	0	93505388	N.D.	43.462
15) T	Picloram	10.998	0.000	44464676	0	8.710	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS060120\
Data File : PS010581.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2020 00:12
Operator : DD\AJ
Sample : L2814-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 06:47:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052920.M
Quant Title : 8080.M
QLast Update : Fri May 29 15:43:50 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

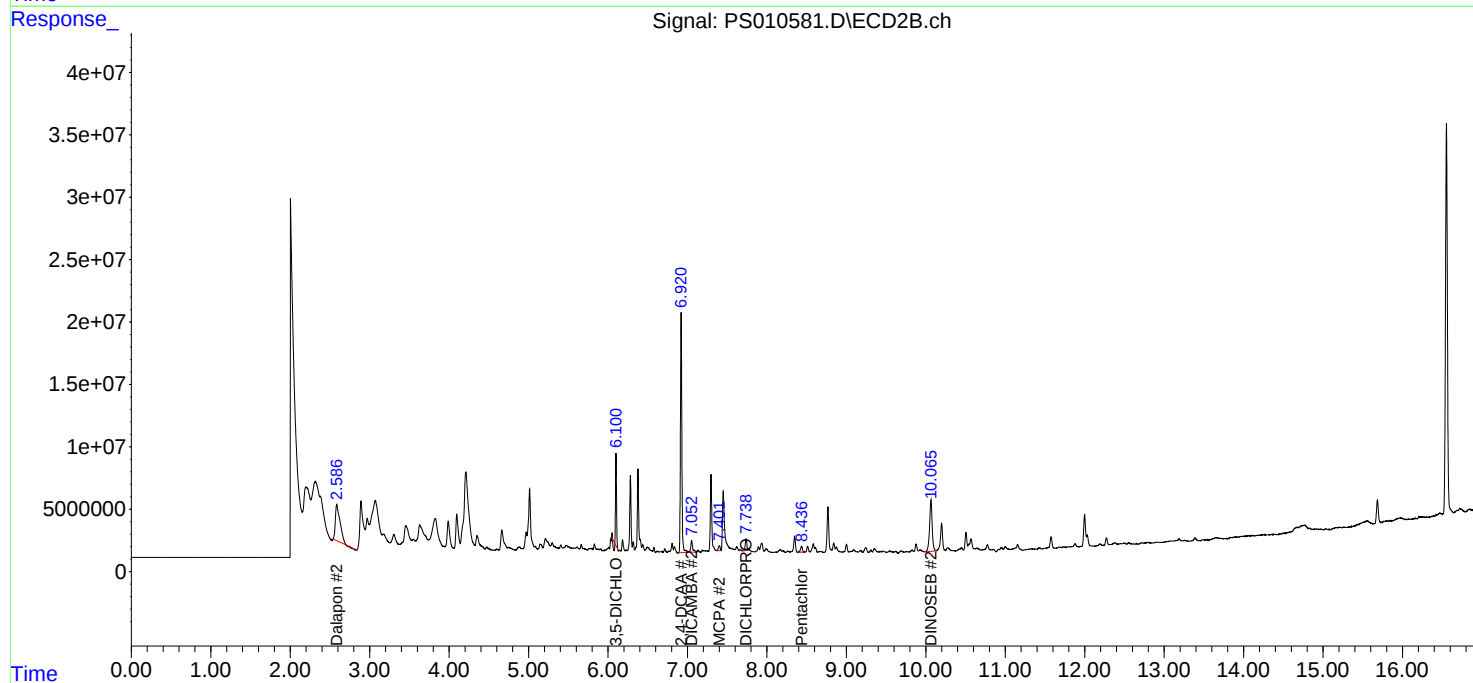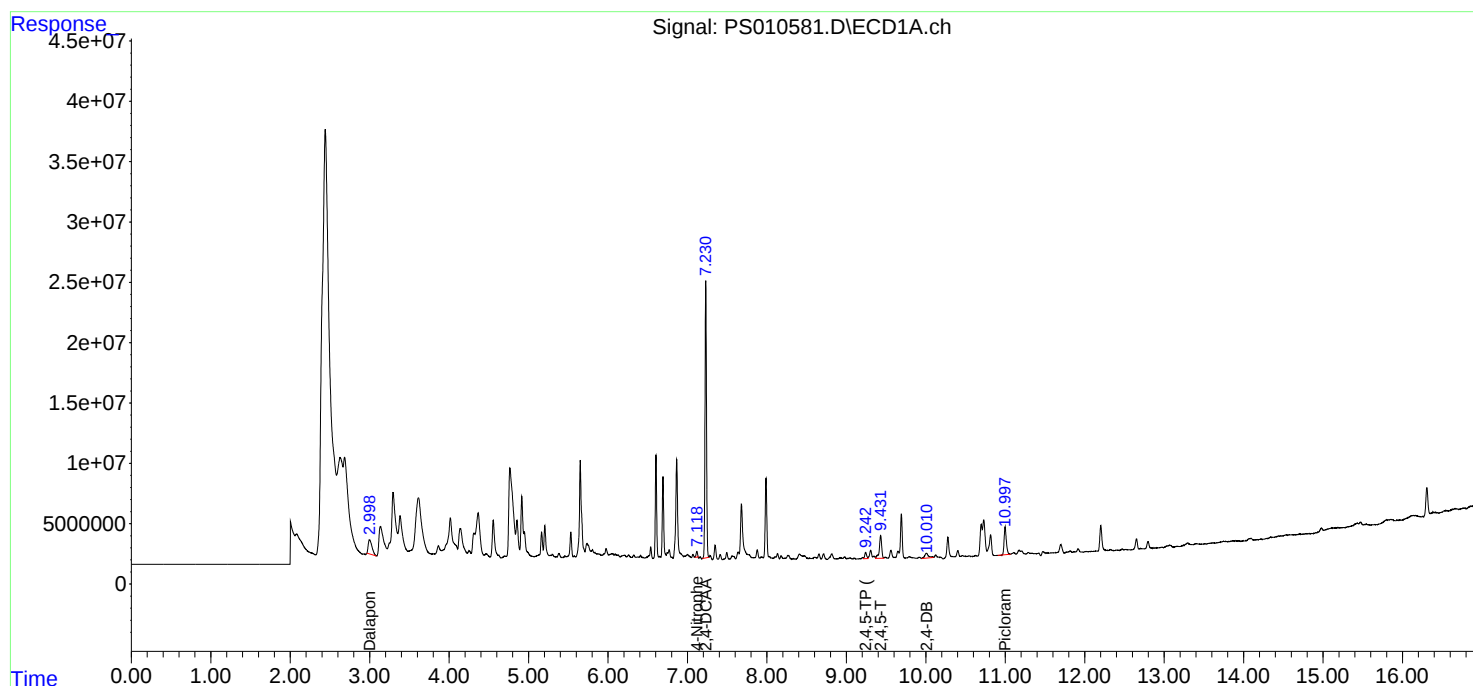

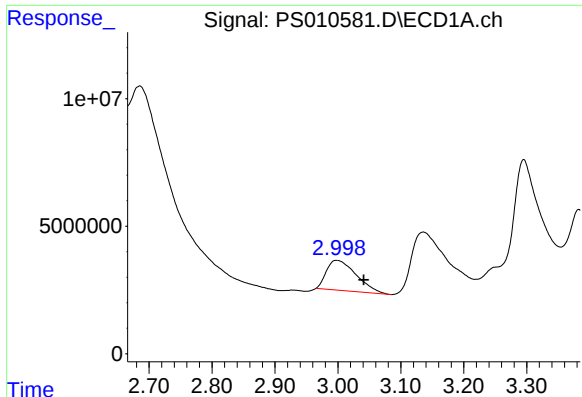


#1 Dalapon

R.T.: 2.998 min
Delta R.T.: -0.043 min
Response: 38555683
Conc: 39.21 ng/ml

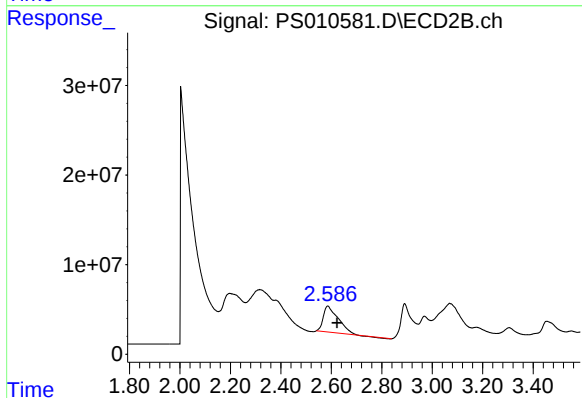


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.037 min
Response: 116385911
Conc: 158.97 ng/ml

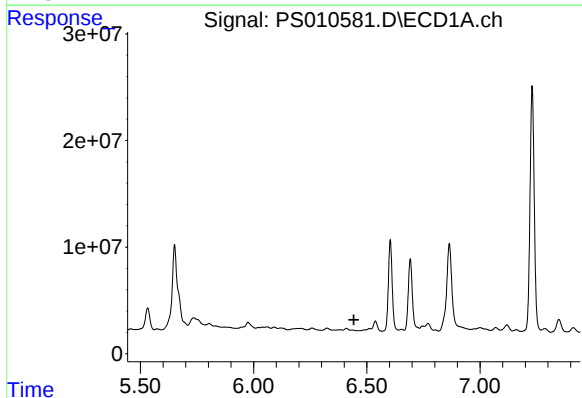


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

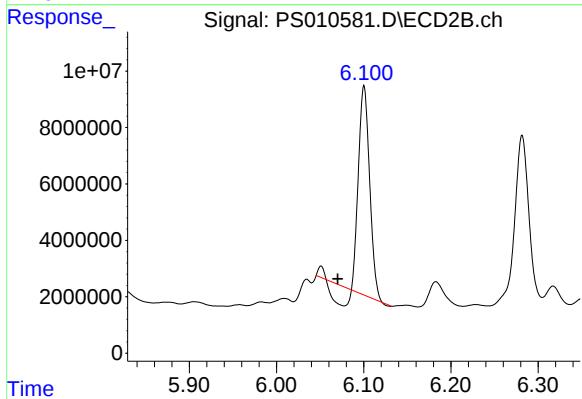


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 59272700
Conc: 72.32 ng/ml

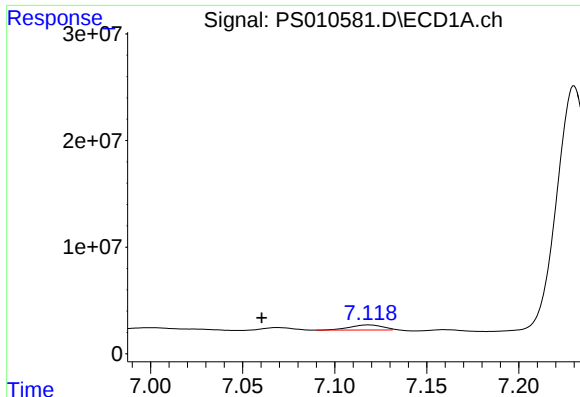


#3 4-Nitrophenol

R.T.: 7.118 min
Delta R.T.: 0.058 min
Response: 5928756
Conc: 15.99 ng/ml

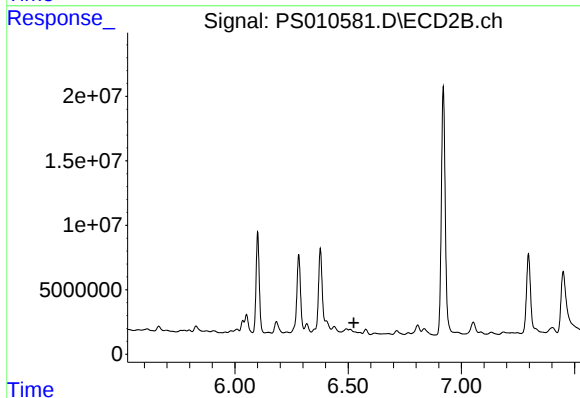


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.525 min
Response: 0
Conc: N.D.

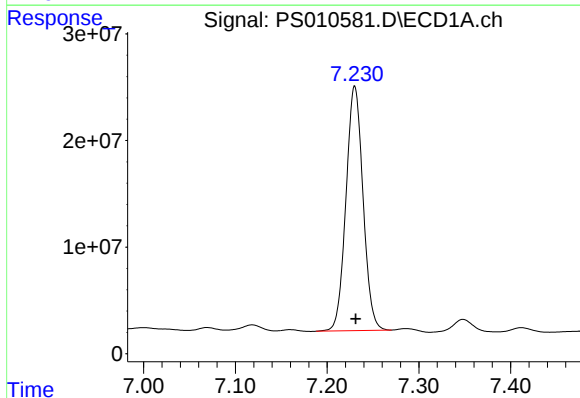


#4 2,4-DCAA

R.T.: 7.230 min
Delta R.T.: 0.000 min
Response: 296258335
Conc: 374.60 ng/ml

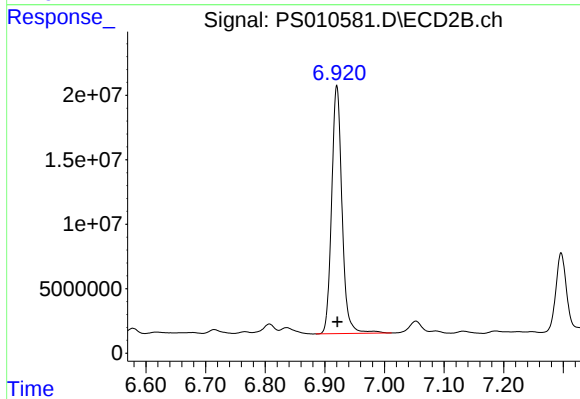


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 233029072
Conc: 427.25 ng/ml

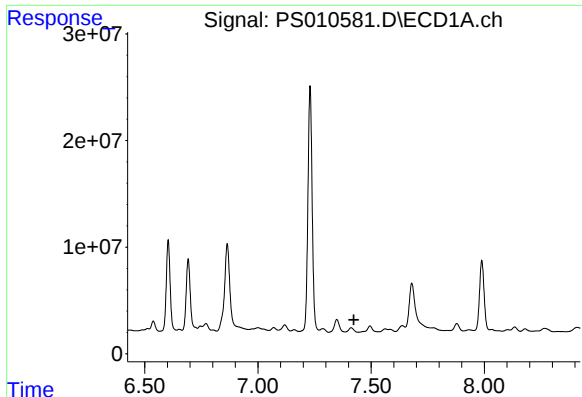


#5 DICAMBA

R.T.: 0.000 min
Exp R.T.: 7.423 min
Response: 0
Conc: N.D.

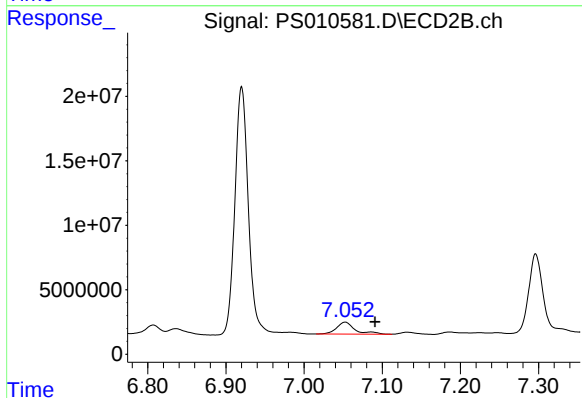


#5 DICAMBA

R.T.: 7.053 min
Delta R.T.: -0.039 min
Response: 15125377
Conc: 6.72 ng/ml

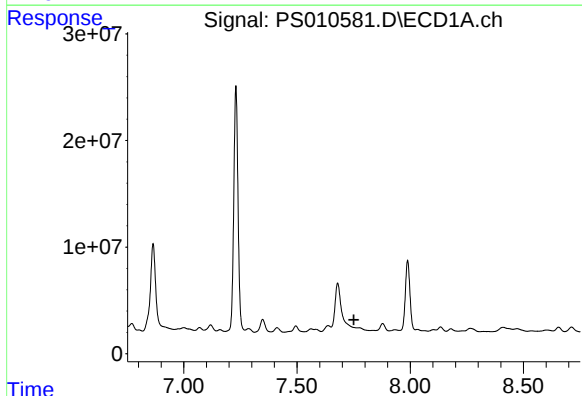


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.751 min
Response: 0
Conc: N.D.

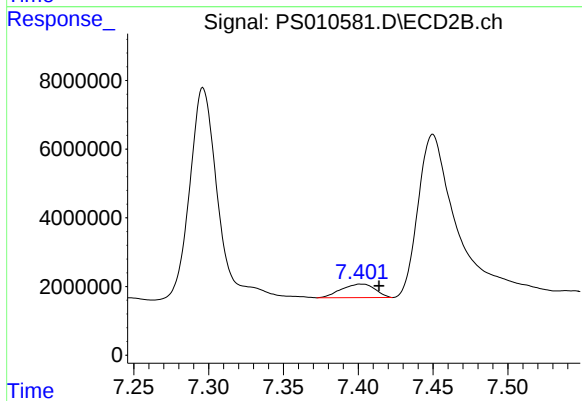


#7 MCPA

R.T.: 7.402 min
Delta R.T.: -0.012 min
Response: 6194062
Conc: 2.28 ug/ml

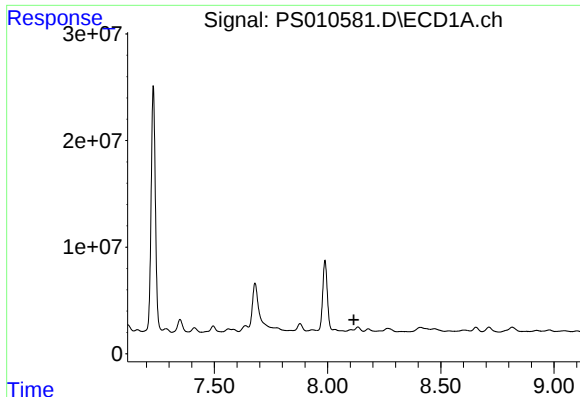


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.116 min
Response: 0
Conc: N.D.

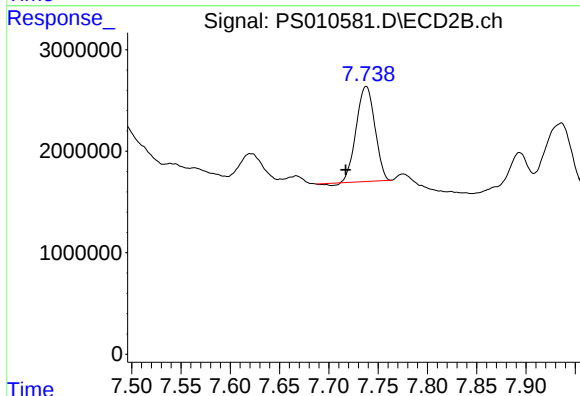


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.021 min
Response: 12204368
Conc: 21.17 ng/ml

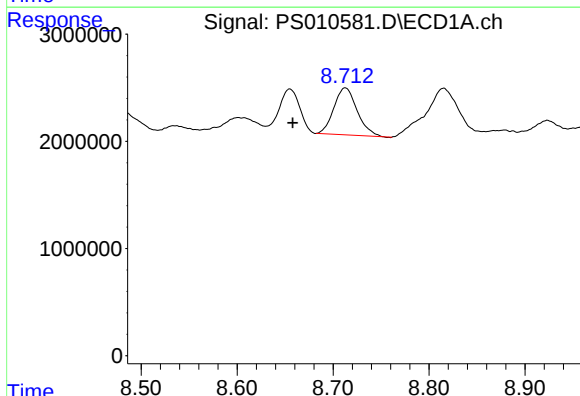


#10 Pentachlorophenol

R.T.: 8.713 min
Delta R.T.: 0.055 min
Response: 7215770
Conc: N.D.

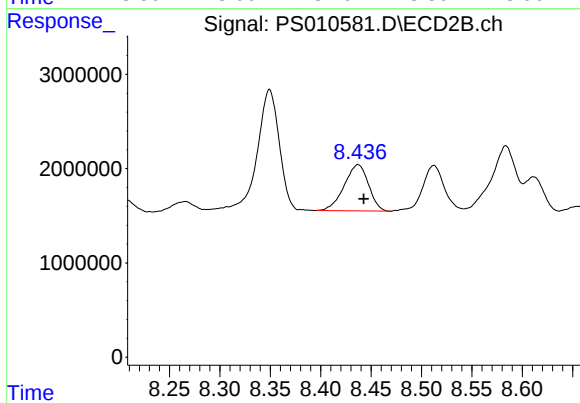


#10 Pentachlorophenol

R.T.: 8.437 min
Delta R.T.: -0.006 min
Response: 8243962
Conc: 1.16 ng/ml

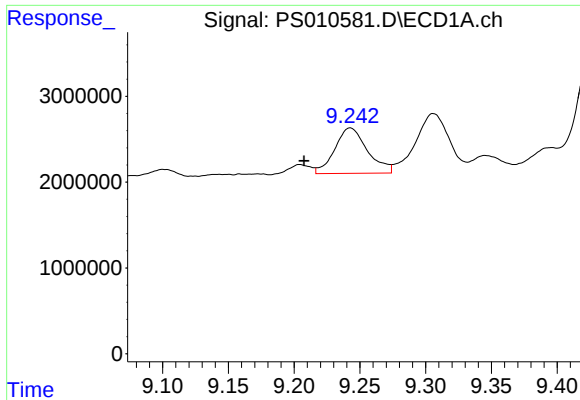


#11 2,4,5-TP (SILVEX)

R.T.: 9.243 min
Delta R.T.: 0.035 min
Response: 9154963
Conc: 2.14 ng/ml

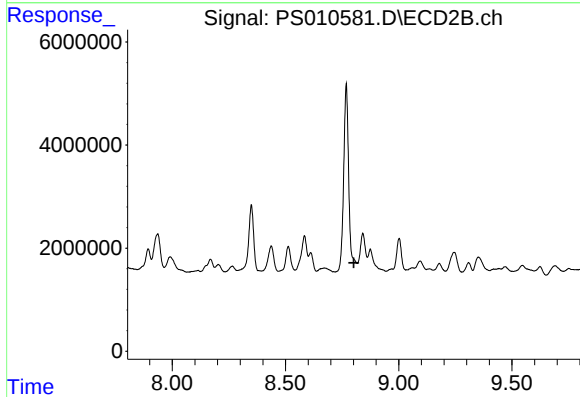


#11 2,4,5-TP (SILVEX)

R.T.: 8.842 min
Delta R.T.: 0.040 min
Response: -27170219
Conc: N.D.

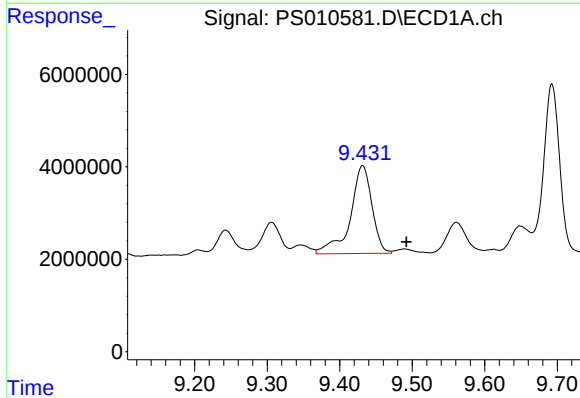


#12 2,4,5-T

R.T.: 9.432 min
Delta R.T.: -0.060 min
Response: 39417592
Conc: 9.69 ng/ml

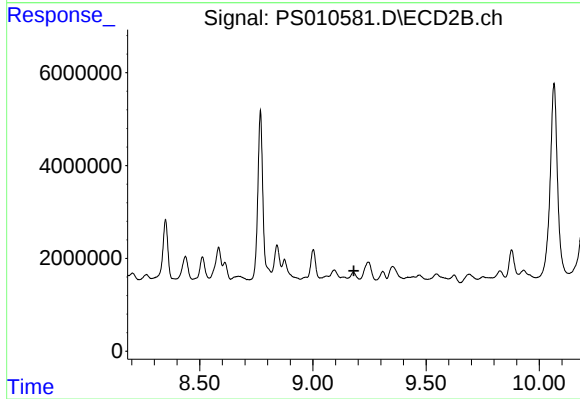


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.181 min
Response: 0
Conc: N.D.

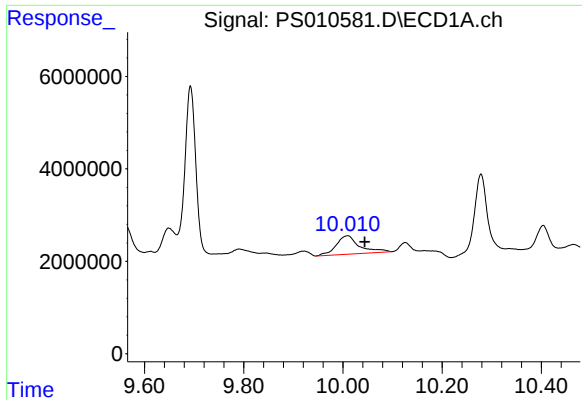


#13 2,4-DB

R.T.: 10.009 min
Delta R.T.: -0.035 min
Response: 12984754
Conc: 23.48 ng/ml

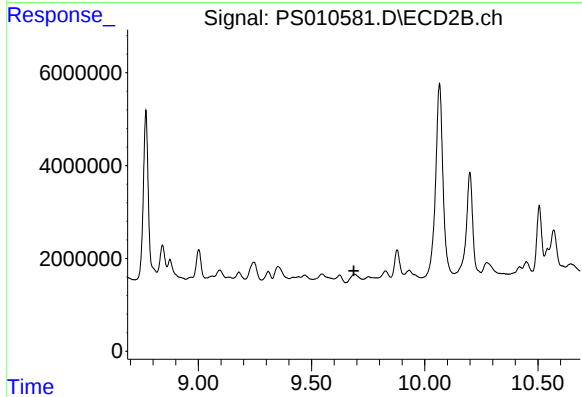


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.687 min
Response: 0
Conc: N.D.

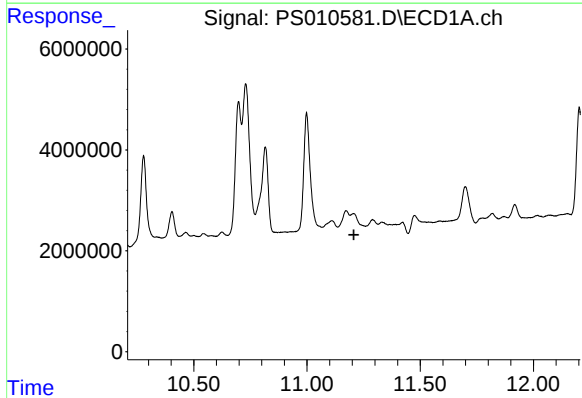


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.207 min
Response: 0
Conc: N.D.

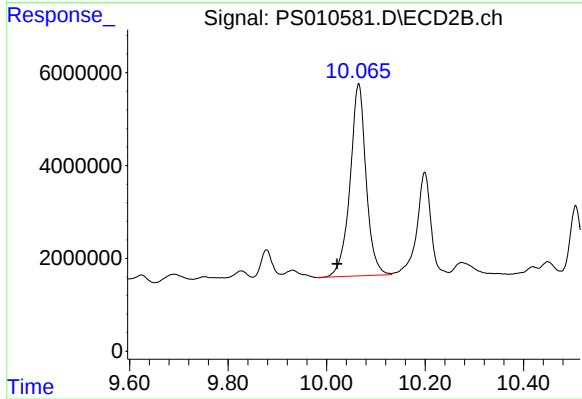


#14 DINOSEB

R.T.: 10.065 min
Delta R.T.: 0.043 min
Response: 93505388
Conc: 43.46 ng/ml

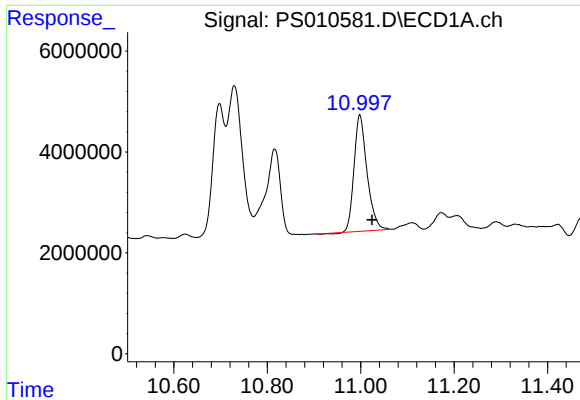

#15 Picloram

R.T.: 10.998 min
Delta R.T.: -0.026 min
Response: 44464676
Conc: 8.71 ng/ml

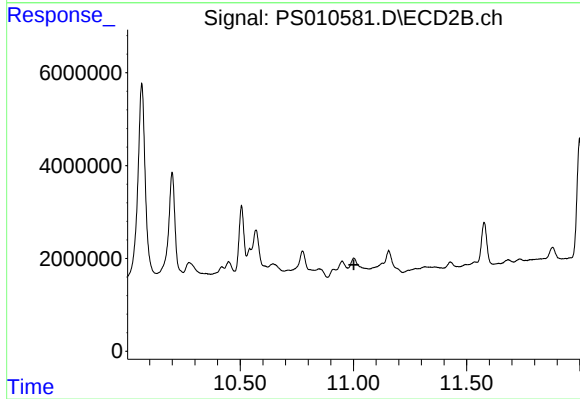

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.002 min
Response: 0
Conc: N.D.